

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
 Data File : PS010593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 04:47
 Operator : DD\AJ
 Sample : PB129174BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 06:51:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.920	541.9E6	405.0E6	685.245	742.576
Target Compounds							
1) T	Dalapon	2.995	2.585	32080713	102.7E6	32.629	140.251 #
2) T	3,5-DICHL...	0.000	6.100	0	34839158	N.D.	42.505
5) T	DICAMBA	0.000	7.052	0	7749424	N.D.	3.443
7) T	MCPA	7.780	7.385	41943216	34151367	11.998	12.566
8) T	DICHLORPROP	0.000	7.738	0	6091153	N.D.	10.563
10) T	Pentachlo...	8.711	8.513	9325243	6482541	<MDL	<MDL #
12) T	2,4,5-T	9.434	0.000	24179181	0	5.945	N.D. #
13) T	2,4-DB	10.076	0.000	17226362	0	31.155	N.D. #
14) T	DINOSEB	0.000	10.040	0	30040180	N.D.	13.963
15) T	Picloram	10.997	0.000	22396939	0	4.387	N.D. #
16) T	DCPA	11.535	0.000	48823776	0	9.112	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
Data File : PS010593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 04:47
Operator : DD\AJ
Sample : PB129174BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 06:51:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

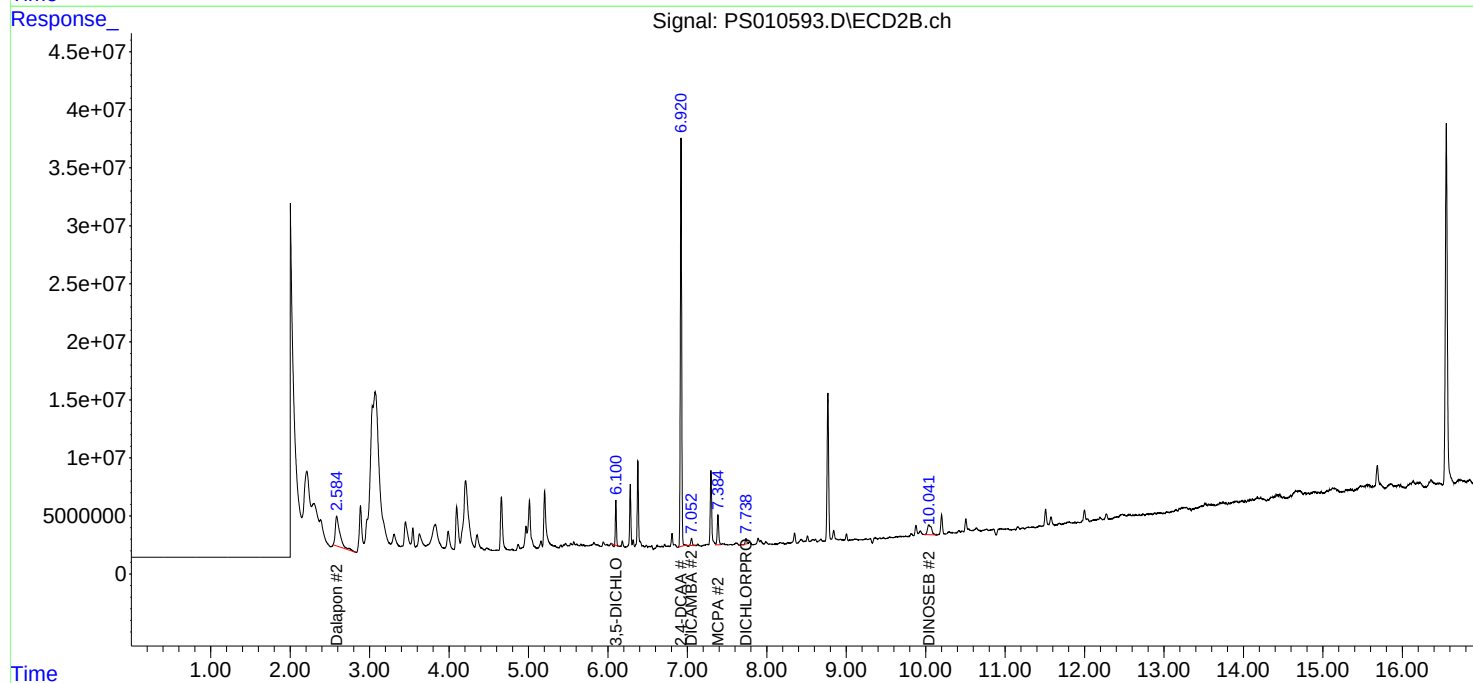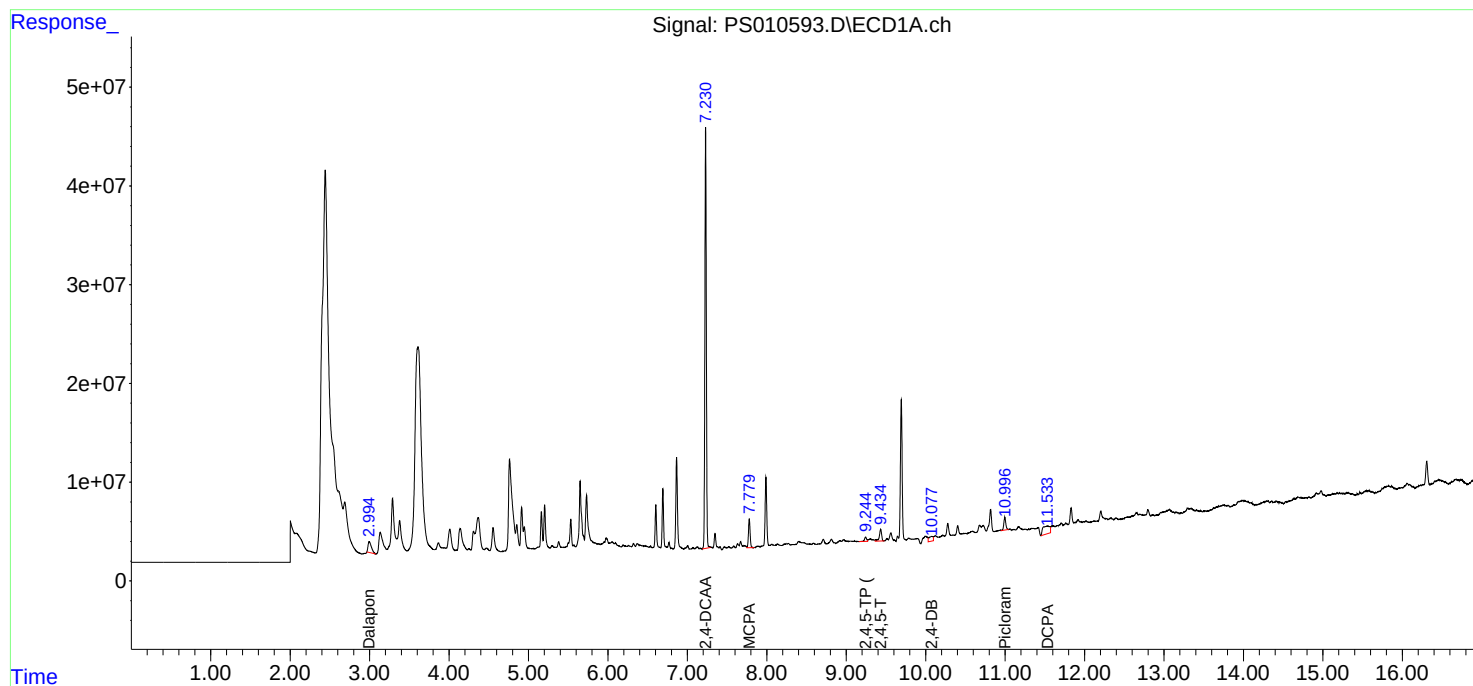

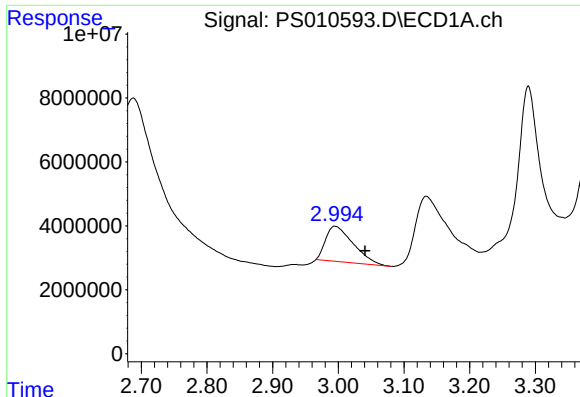


#1 Dalapon

R.T.: 2.995 min
Delta R.T.: -0.046 min
Response: 32080713
Conc: 32.63 ng/ml

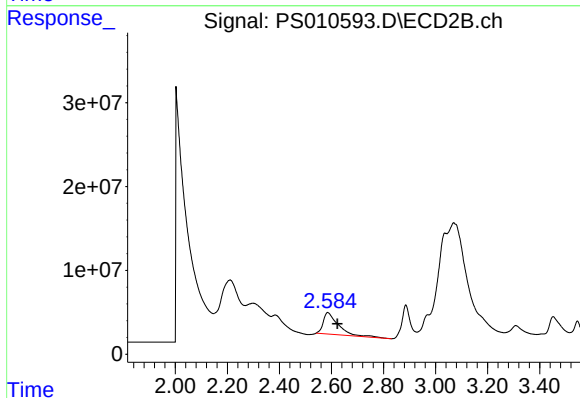


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.038 min
Response: 102684085
Conc: 140.25 ng/ml

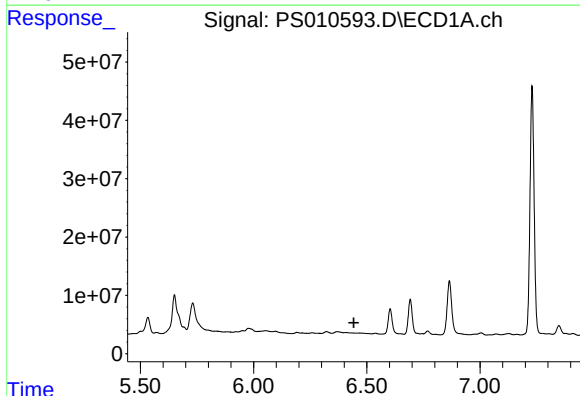


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

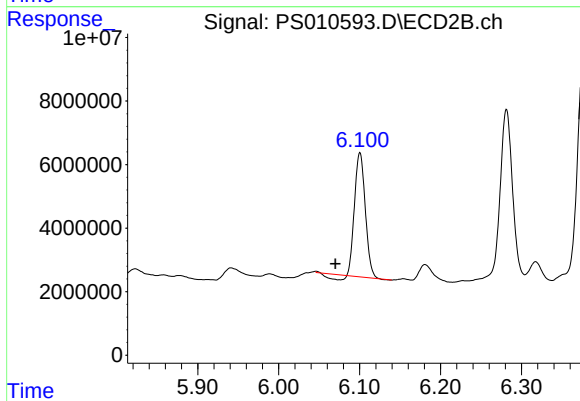


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 34839158
Conc: 42.51 ng/ml

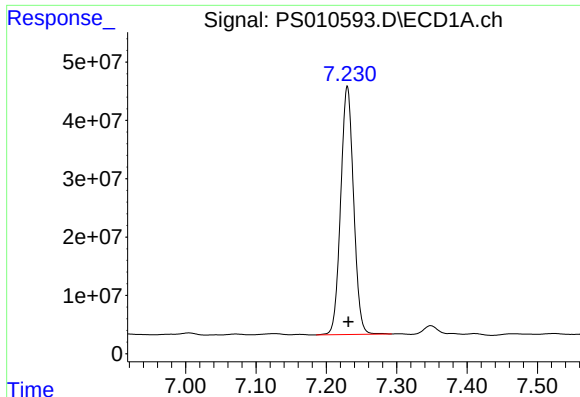


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: -0.001 min
Response: 541934237
Conc: 685.25 ng/ml

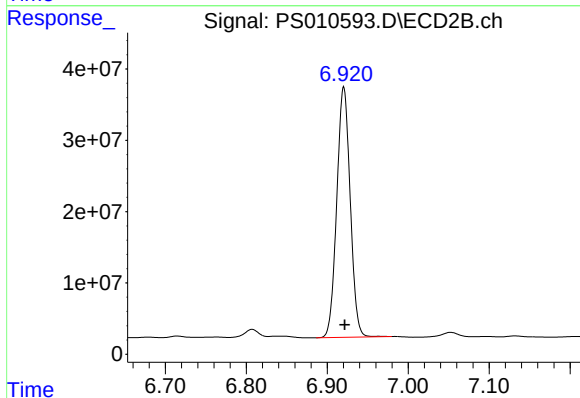


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 405012878
Conc: 742.58 ng/ml

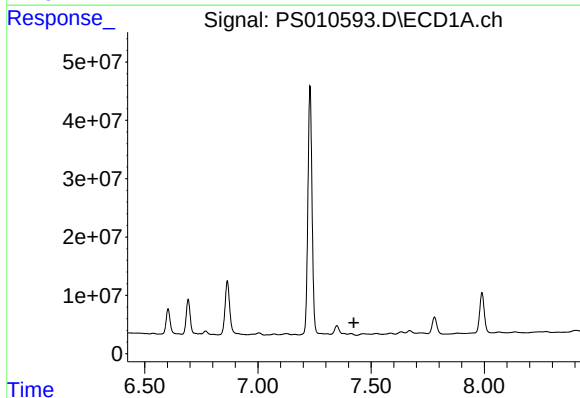


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.423 min
Response: 0
Conc: N.D.

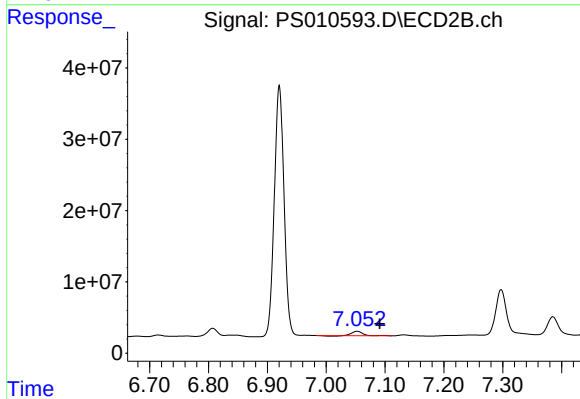


#5 DICAMBA

R.T.: 7.052 min
Delta R.T.: -0.039 min
Response: 7749424
Conc: 3.44 ng/ml

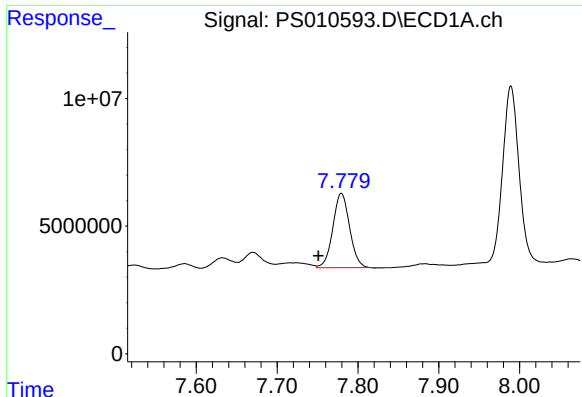


#7 MCPA

R.T.: 7.780 min
Delta R.T.: 0.029 min
Response: 41943216
Conc: 12.00 ug/ml

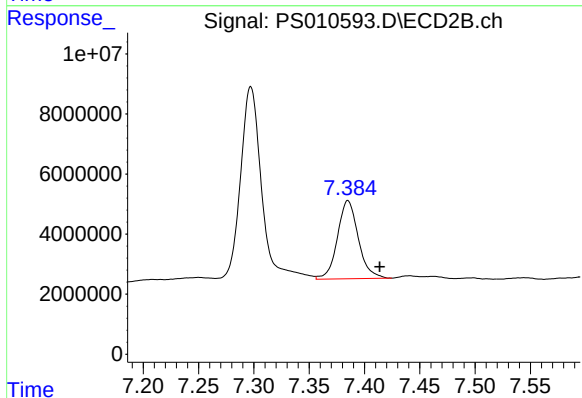


#7 MCPA

R.T.: 7.385 min
Delta R.T.: -0.029 min
Response: 34151367
Conc: 12.57 ug/ml

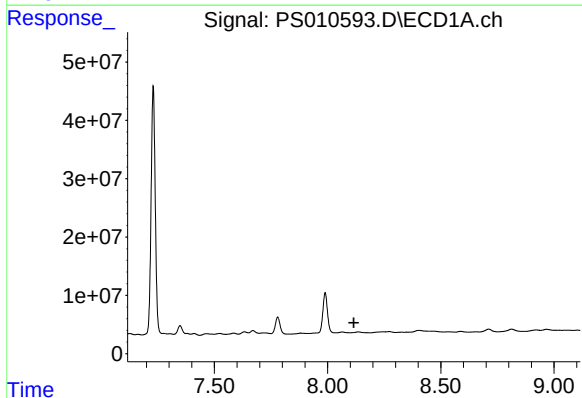


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

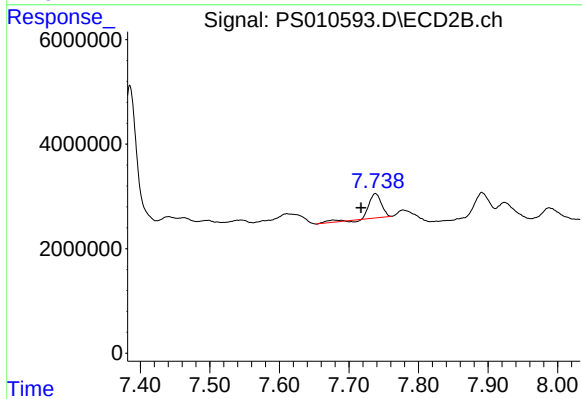

#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.021 min
Response: 6091153
Conc: 10.56 ng/ml

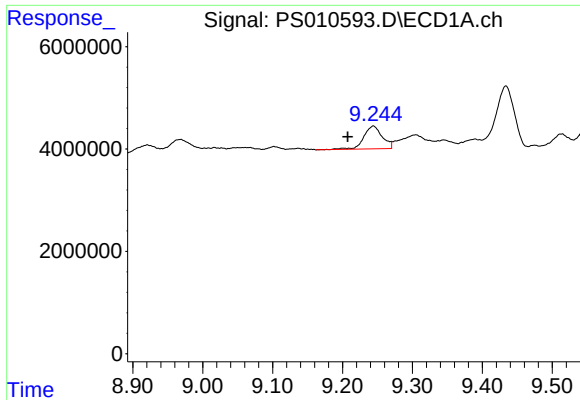


#11 2,4,5-TP (SILVEX)

R.T.: 9.244 min

Delta R.T.: 0.036 min

Response: 8122341

Conc: 1.90 ng/ml

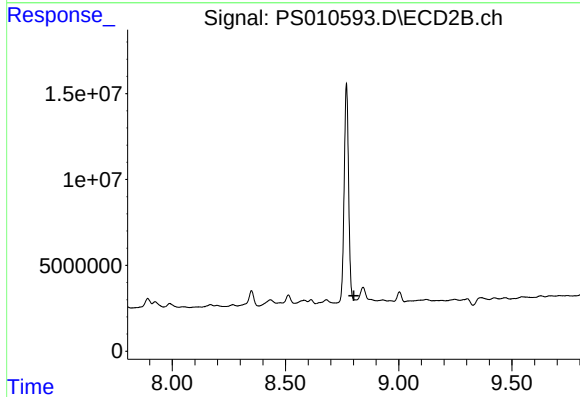


#11 2,4,5-TP (SILVEX)

R.T.: 8.842 min

Delta R.T.: 0.040 min

Response: -59347386

Conc: N.D.

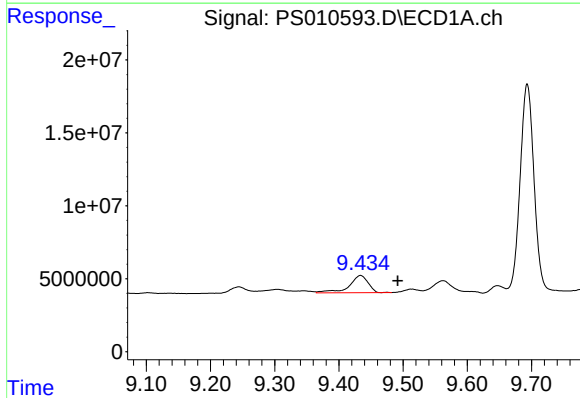


#12 2,4,5-T

R.T.: 9.434 min

Delta R.T.: -0.058 min

Response: 24179181

Conc: 5.95 ng/ml

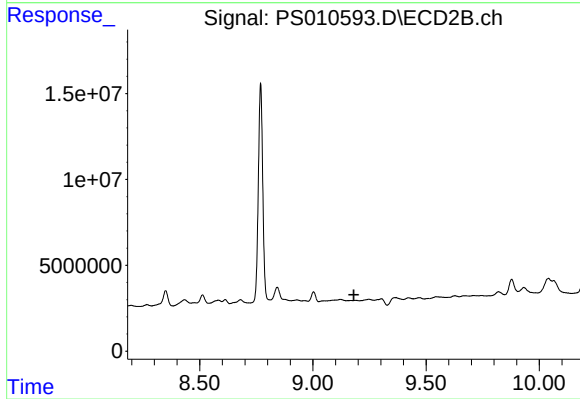


#12 2,4,5-T

R.T.: 0.000 min

Exp R.T.: 9.181 min


Response: 0

Conc: N.D.

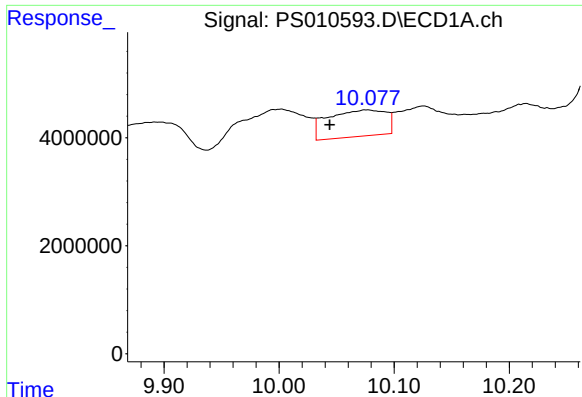


#13 2,4-DB

R.T.: 10.076 min
Delta R.T.: 0.032 min
Response: 17226362
Conc: 31.15 ng/ml

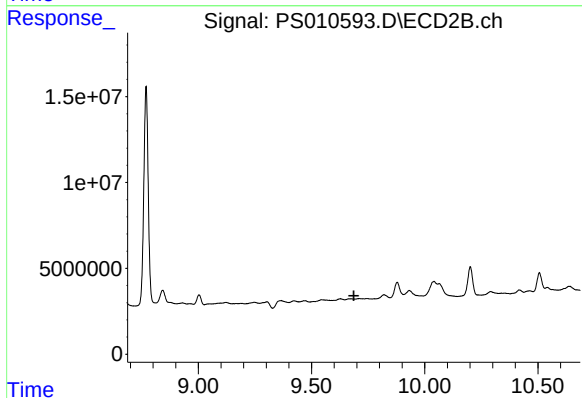


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.687 min
Response: 0
Conc: N.D.

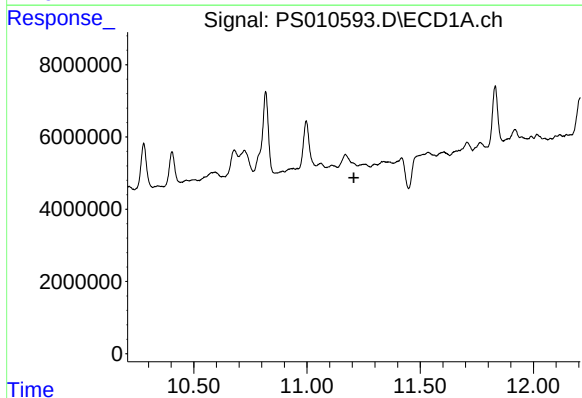


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.207 min
Response: 0
Conc: N.D.

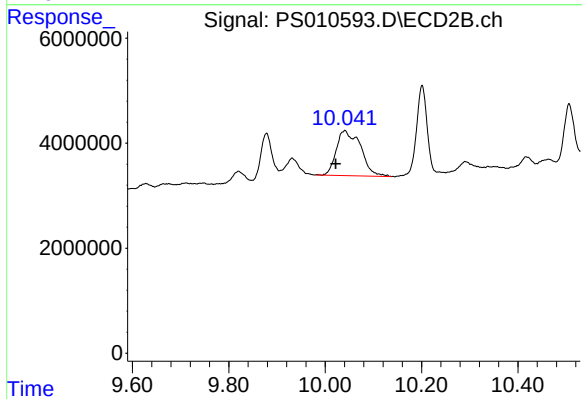


#14 DINOSEB

R.T.: 10.040 min
Delta R.T.: 0.019 min
Response: 30040180
Conc: 13.96 ng/ml

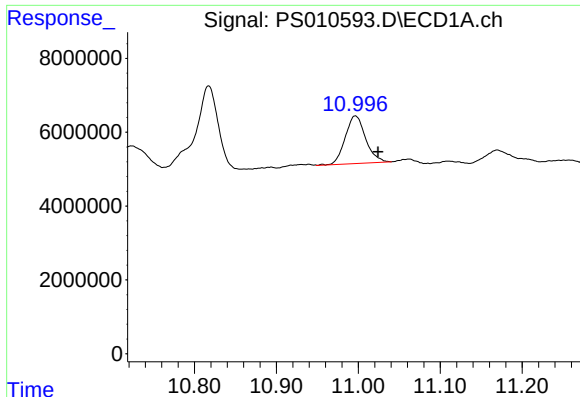


#15 Picloram

R.T.: 10.997 min
Delta R.T.: -0.027 min
Response: 22396939
Conc: 4.39 ng/ml

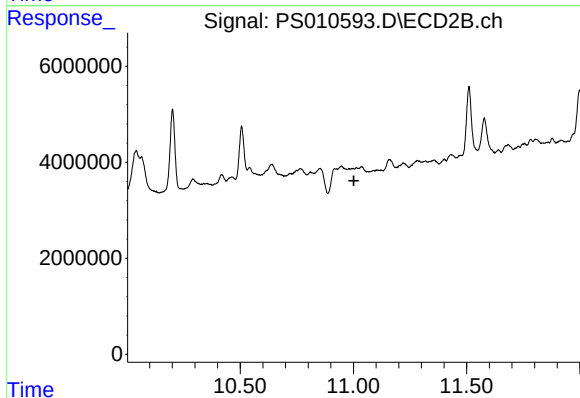


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.002 min
Response: 0
Conc: N.D.

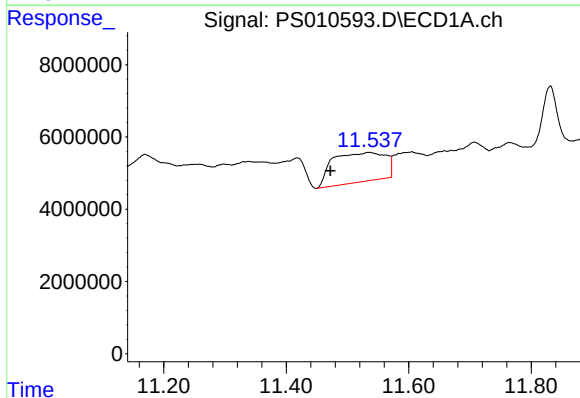

#16 DCPA

R.T.: 11.535 min
Delta R.T.: 0.063 min
Response: 48823776
Conc: 9.11 ng/ml

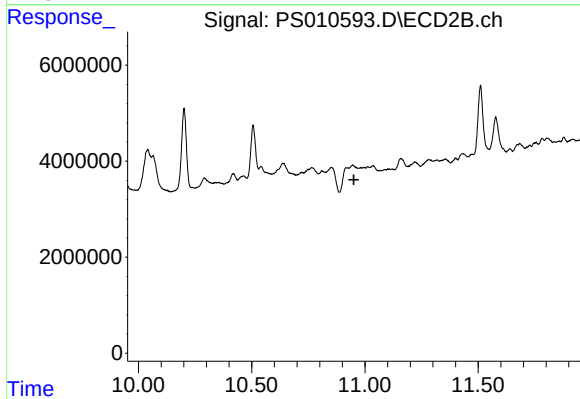

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.951 min
Response: 0
Conc: N.D.