

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
 Data File : PS010608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 10:31
 Operator : DD\AJ
 Sample : L2797-01
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 11:16:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.920	321.2E6	192.9E6	406.182	353.681
Target Compounds							
2) T	3,5-DICHL...	6.511	6.100	7560643	41623665	6.916	50.783 #
3) T	4-Nitroph...	7.053	0.000	11631688	0	31.375	N.D. #
5) T	DICAMBA	7.355	7.089	43985924	4565182	13.988	2.028 #
6) T	MCP	7.626	0.000	14841490	0	6.008	N.D. #
7) T	MCPA	7.779	7.409	37353766	27337292	10.685	10.059
8) T	DICHLORPROP	0.000	7.737	0	18561315	N.D.	32.189
9) T	2,4-D	8.352	8.046	35894216	6301029	45.535	8.310 #
10) T	Pentachlo...	8.645	8.439	40474459	-19826480	3.795	N.D. #
12) T	2,4,5-T	9.492	9.179	23360719	21159973	5.744	7.051
13) T	2,4-DB	10.045	9.694	56125418	37452261	101.506	92.196
14) T	DINOSEB	0.000	10.036	0	70347903	N.D.	32.698
15) T	Picloram	11.023	11.001	257.4E6	153.0E6	50.423	37.080 #
16) T	DCPA	11.483	10.930	43232011	35743691	8.069	9.639


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
Data File : PS010608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 10:31
Operator : DD\AJ
Sample : L2797-01
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 11:16:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

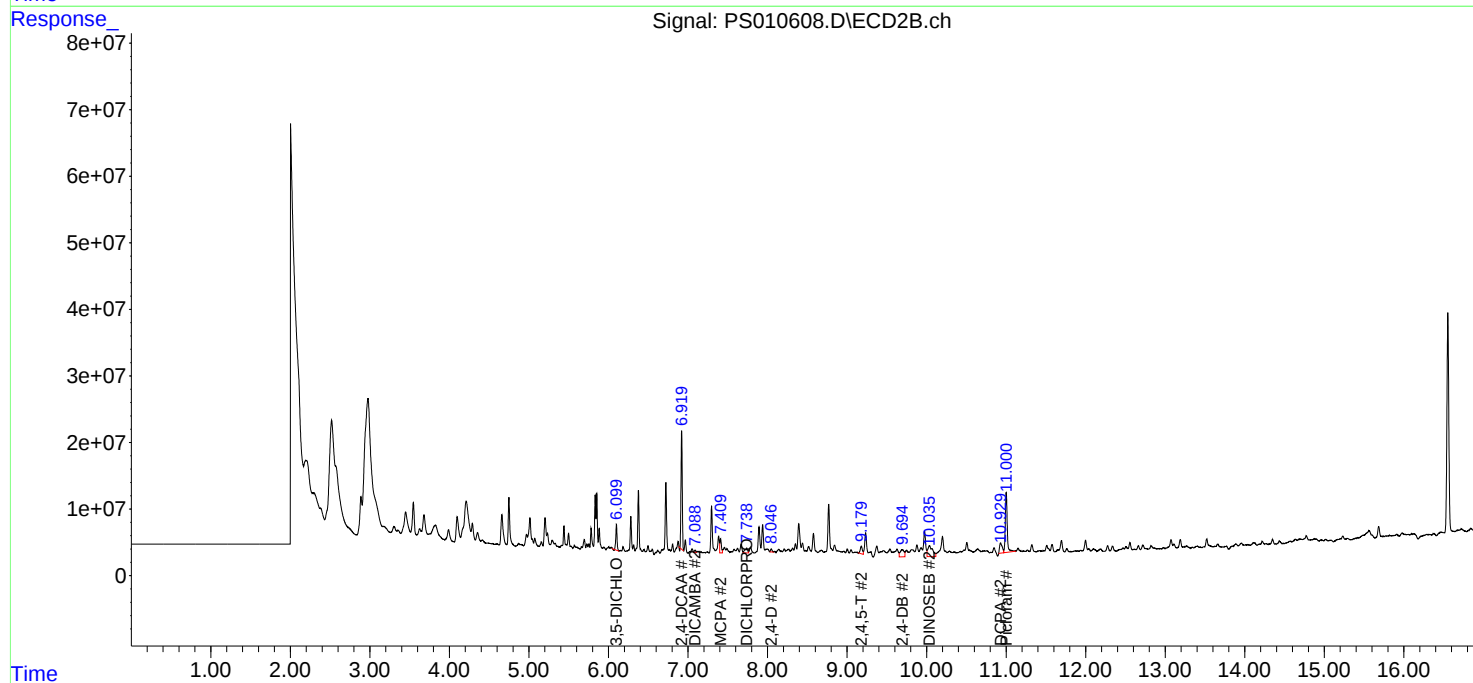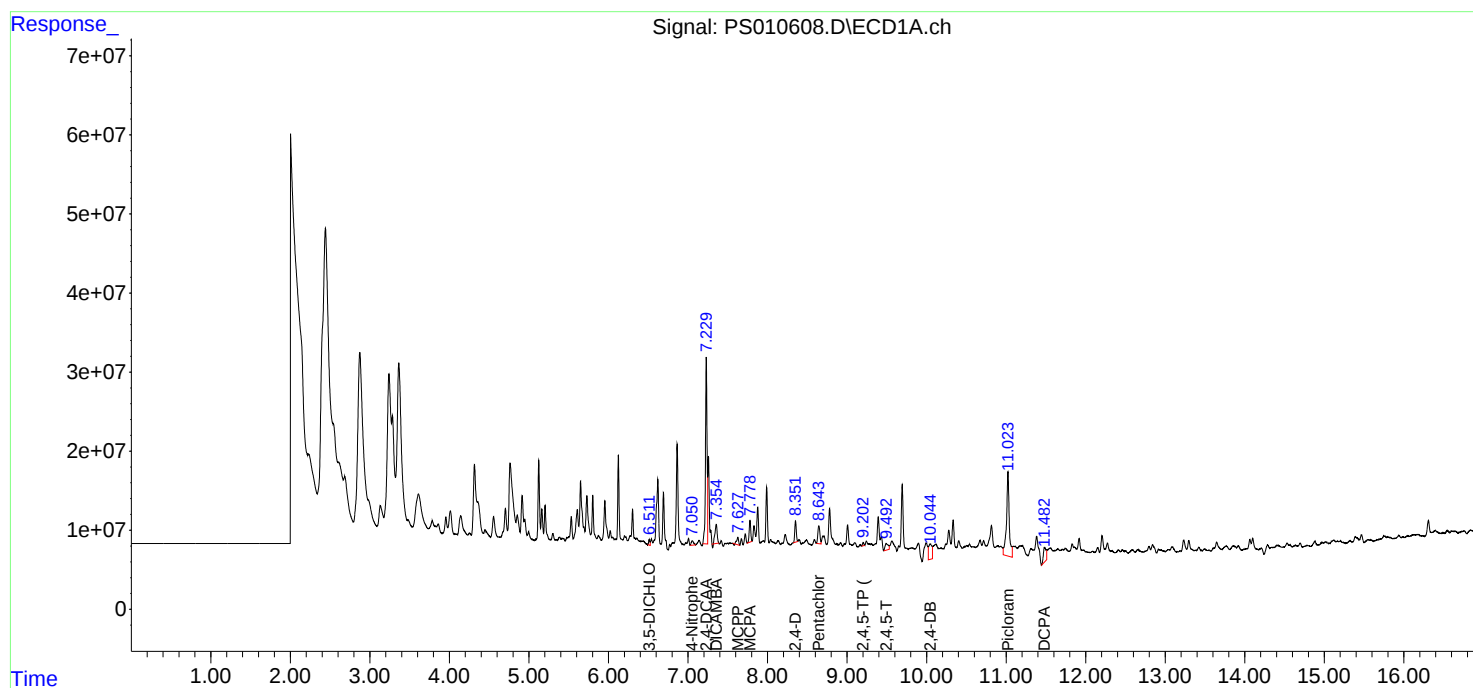

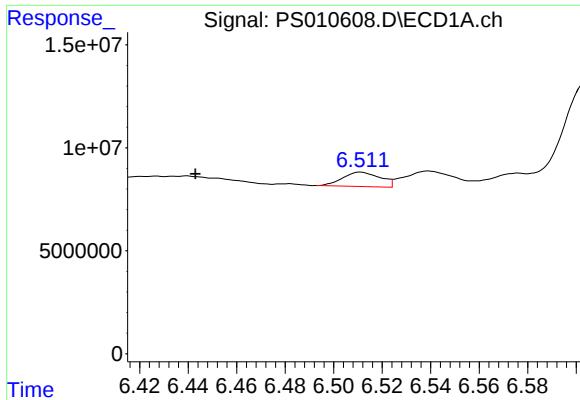


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.511 min
Delta R.T.: 0.068 min
Response: 7560643
Conc: 6.92 ng/ml

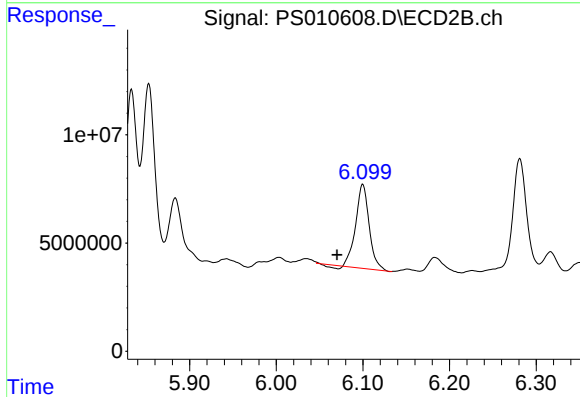


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 41623665
Conc: 50.78 ng/ml

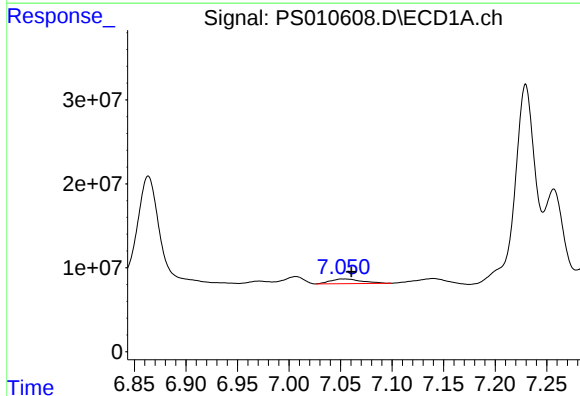


#3 4-Nitrophenol

R.T.: 7.053 min
Delta R.T.: -0.007 min
Response: 11631688
Conc: 31.38 ng/ml

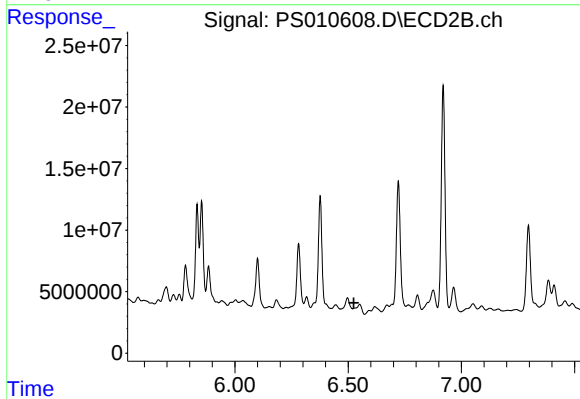


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

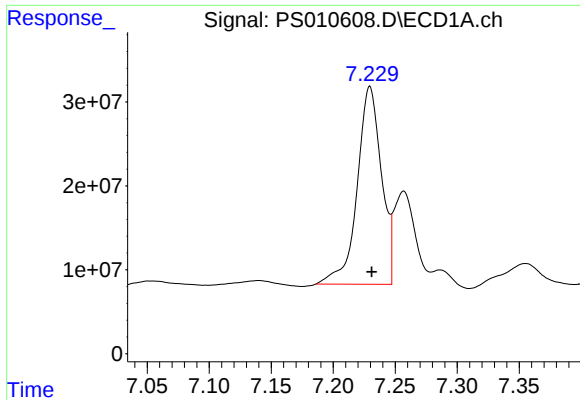


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: -0.002 min
Response: 321234119
Conc: 406.18 ng/ml

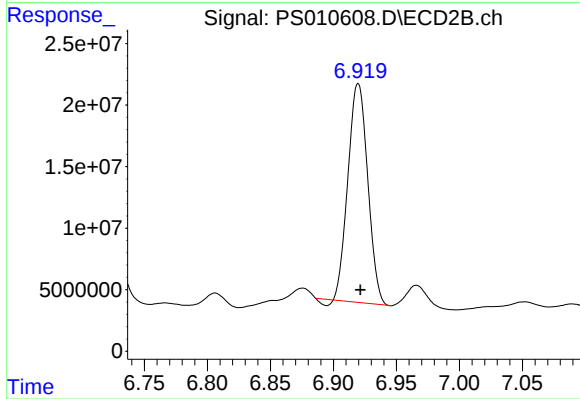


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 192903364
Conc: 353.68 ng/ml

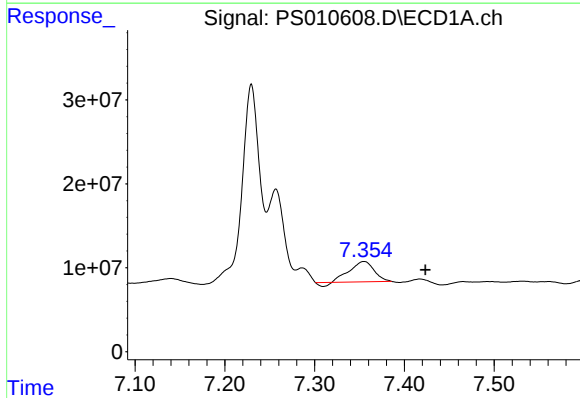


#5 DICAMBA

R.T.: 7.355 min
Delta R.T.: -0.009 min
Response: 43985924
Conc: 13.99 ng/ml

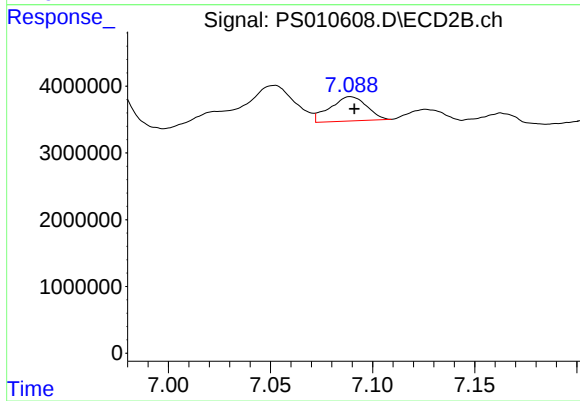


#5 DICAMBA

R.T.: 7.089 min
Delta R.T.: -0.002 min
Response: 4565182
Conc: 2.03 ng/ml

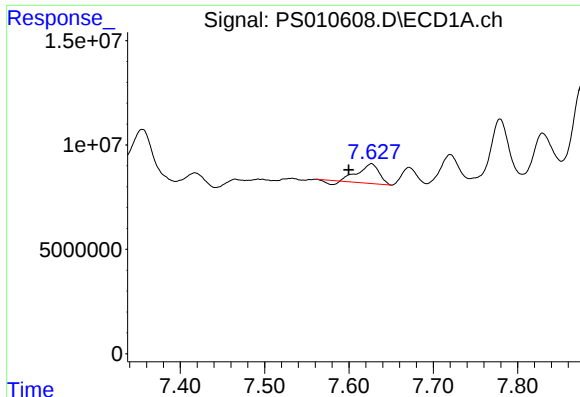


#6 MCP

R.T.: 7.626 min
Delta R.T.: 0.027 min
Response: 14841490
Conc: 6.01 ug/ml

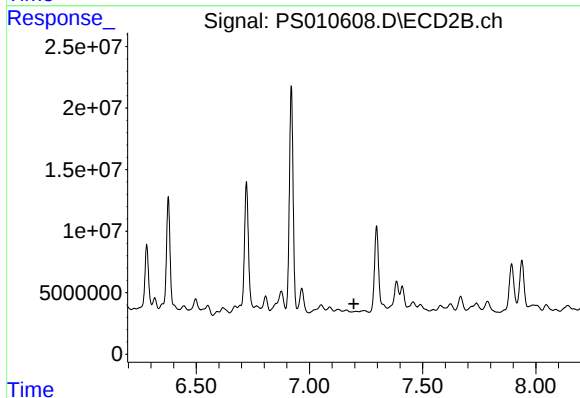


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.196 min
Response: 0
Conc: N.D.

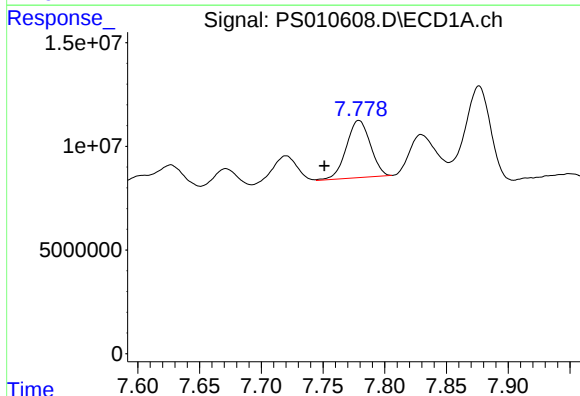


#7 MCP

R.T.: 7.779 min
Delta R.T.: 0.028 min
Response: 37353766
Conc: 10.68 ug/ml

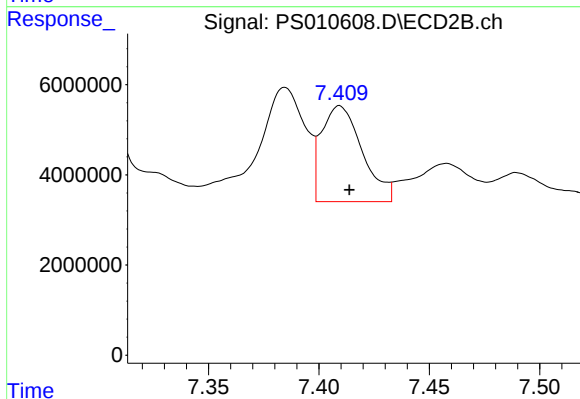


#7 MCP

R.T.: 7.409 min
Delta R.T.: -0.004 min
Response: 27337292
Conc: 10.06 ug/ml

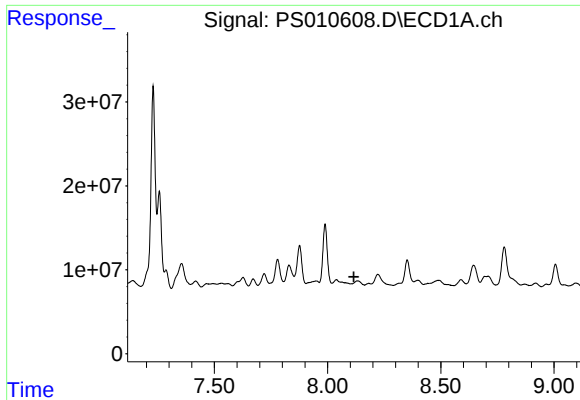


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

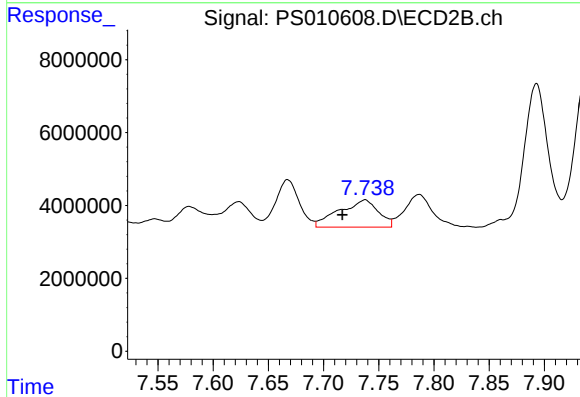


#8 DICHLORPROP

R.T.: 7.737 min
Delta R.T.: 0.020 min
Response: 18561315
Conc: 32.19 ng/ml

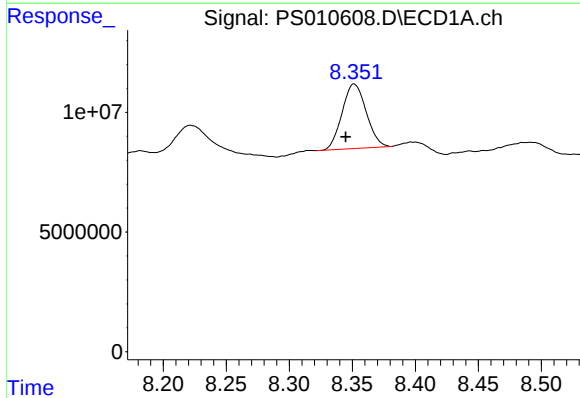


#9 2,4-D

R.T.: 8.352 min
Delta R.T.: 0.007 min
Response: 35894216
Conc: 45.54 ng/ml

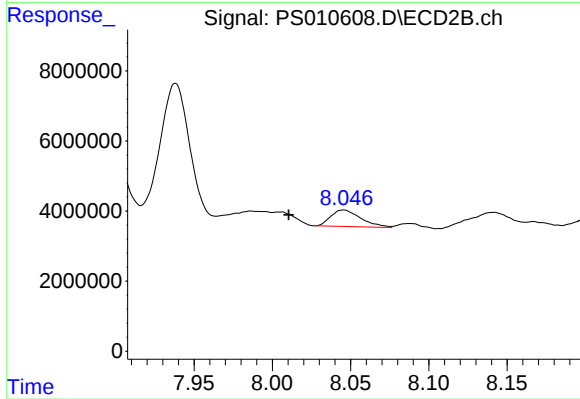


#9 2,4-D

R.T.: 8.046 min
Delta R.T.: 0.035 min
Response: 6301029
Conc: 8.31 ng/ml

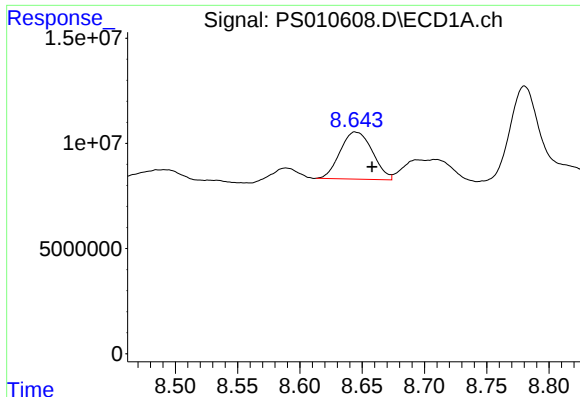


#10 Pentachlorophenol

R.T.: 8.645 min
Delta R.T.: -0.013 min
Response: 40474459
Conc: 3.79 ng/ml

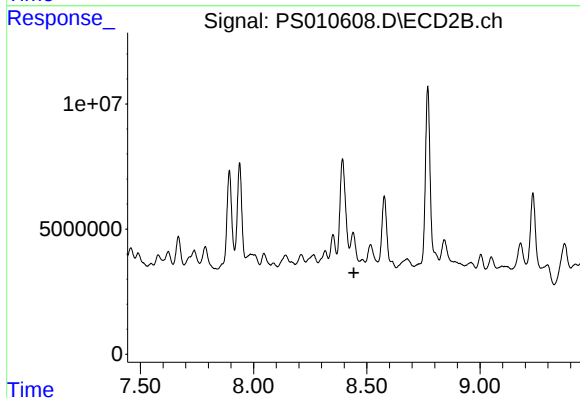


#10 Pentachlorophenol

R.T.: 8.439 min
Delta R.T.: -0.003 min
Response: -19826480
Conc: N.D.

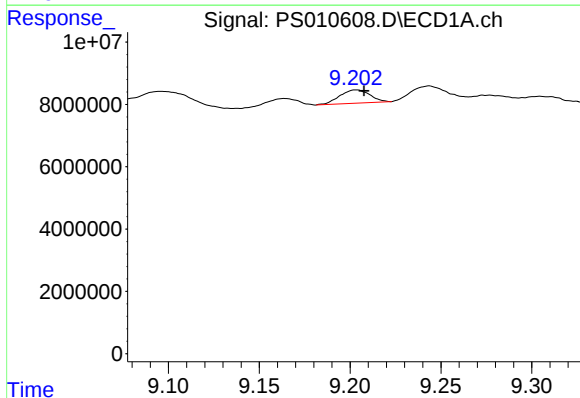


#11 2,4,5-TP (SILVEX)

R.T.: 9.203 min
Delta R.T.: -0.004 min
Response: 4920678
Conc: 1.15 ng/ml

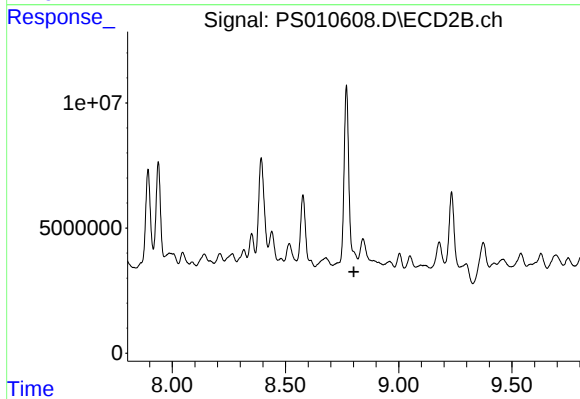


#11 2,4,5-TP (SILVEX)

R.T.: 8.842 min
Delta R.T.: 0.040 min
Response: -103252607
Conc: N.D.

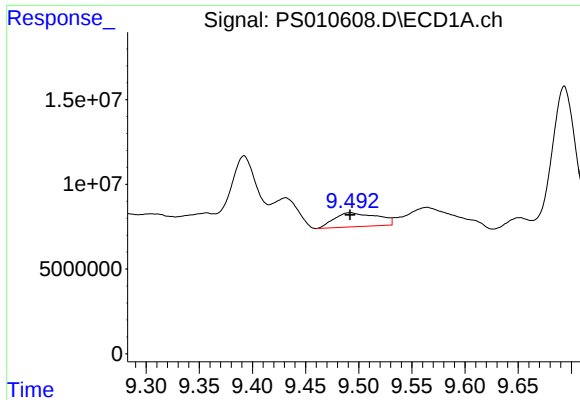


#12 2,4,5-T

R.T.: 9.492 min
Delta R.T.: 0.000 min
Response: 23360719
Conc: 5.74 ng/ml

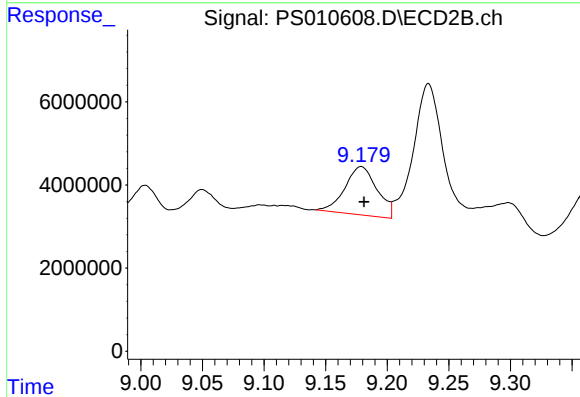


#12 2,4,5-T

R.T.: 9.179 min
Delta R.T.: -0.002 min
Response: 21159973
Conc: 7.05 ng/ml

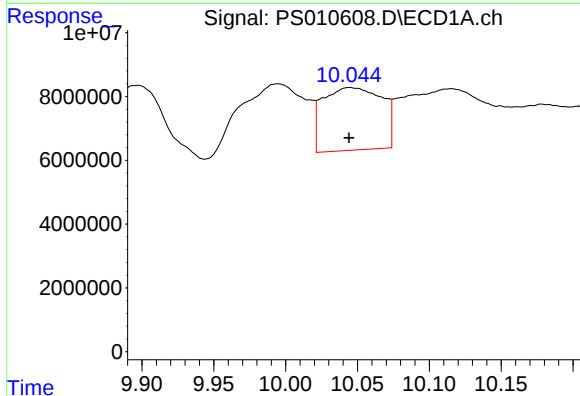


#13 2,4-DB

R.T.: 10.045 min
Delta R.T.: 0.001 min
Response: 56125418
Conc: 101.51 ng/ml

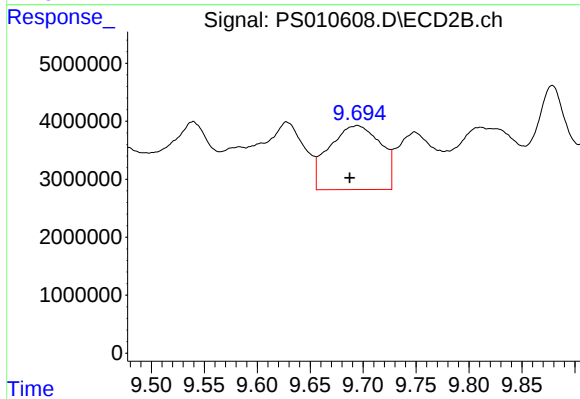


#13 2,4-DB

R.T.: 9.694 min
Delta R.T.: 0.007 min
Response: 37452261
Conc: 92.20 ng/ml

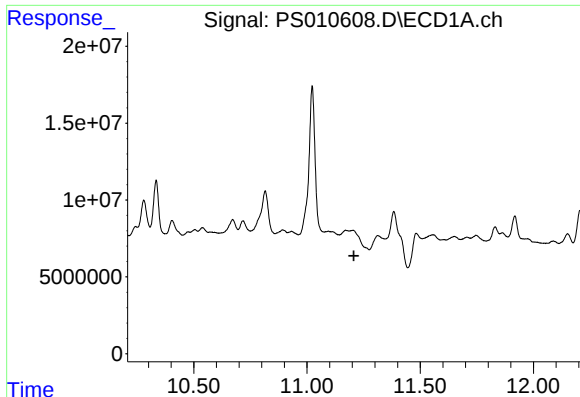


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.207 min
Response: 0
Conc: N.D.

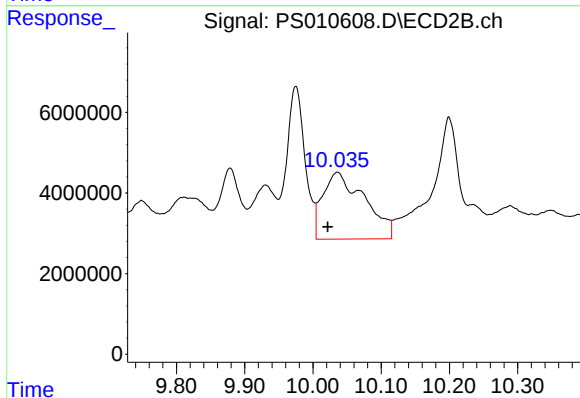


#14 DINOSEB

R.T.: 10.036 min
Delta R.T.: 0.014 min
Response: 70347903
Conc: 32.70 ng/ml

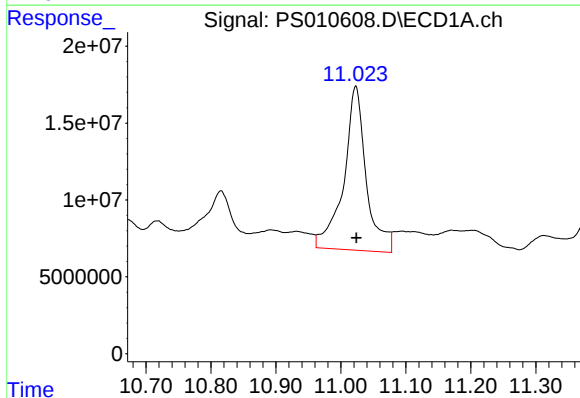


#15 Picloram

R.T.: 11.023 min
Delta R.T.: -0.001 min
Response: 257415684
Conc: 50.42 ng/ml

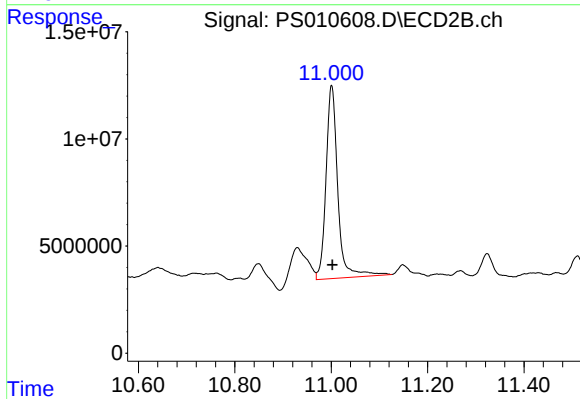


#15 Picloram

R.T.: 11.001 min
Delta R.T.: -0.001 min
Response: 152992486
Conc: 37.08 ng/ml

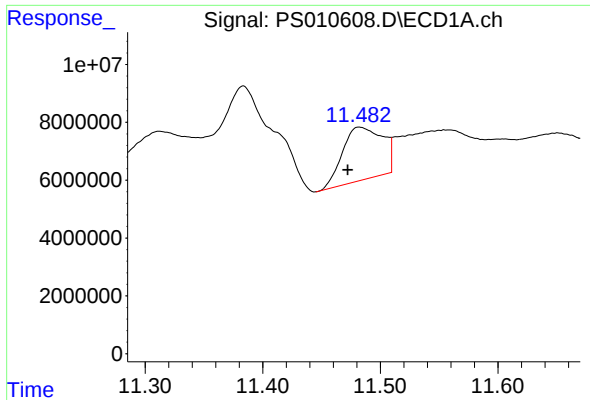

#16 DCPA

R.T.: 11.483 min
Delta R.T.: 0.010 min
Response: 43232011
Conc: 8.07 ng/ml

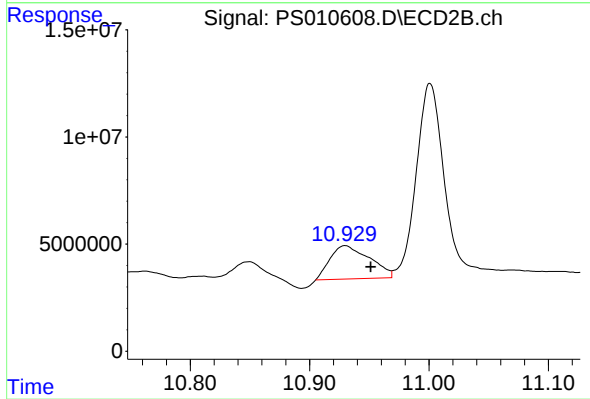

#16 DCPA

R.T.: 10.930 min
Delta R.T.: -0.021 min
Response: 35743691
Conc: 9.64 ng/ml