

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
 Data File : PS010609.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 10:54
 Operator : DD\AJ
 Sample : L2797-06
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 11:16:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.920	505.2E6	343.1E6	638.825	629.139
Target Compounds							
1) T	Dalapon	2.997	2.587	33848123	129.1E6	34.427	176.275 #
2) T	3,5-DICHL...	6.512	6.100	10773260	53663556	9.855	65.472 #
3) T	4-Nitroph...	7.044	0.000	10182551	0	27.466	N.D. #
5) T	DICAMBA	0.000	7.056	0	16108551	N.D.	7.157
6) T	MCPD	7.627	0.000	10744231	0	4.349	N.D. #
7) T	MCPA	7.779	7.384	20879935	29749255	5.973	10.946 #
8) T	DICHLORPROP	0.000	7.739	0	11406287	N.D.	19.781
10) T	Pentachlo...	8.708	0.000	16926703	0	1.587	N.D. #
12) T	2,4,5-T	9.517	0.000	18043787	0	4.437	N.D. #
13) T	2,4-DB	10.058	0.000	81924917	0	148.166	N.D. #
14) T	DINOSEB	0.000	10.037	0	28634755	N.D.	13.310
15) T	Picloram	10.996	11.001	118.2E6	10436601	23.147	2.529 #
16) T	DCPA	11.540	10.933	173.3E6	8854295	32.342	2.388 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
Data File : PS010609.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 10:54
Operator : DD\AJ
Sample : L2797-06
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 11:16:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

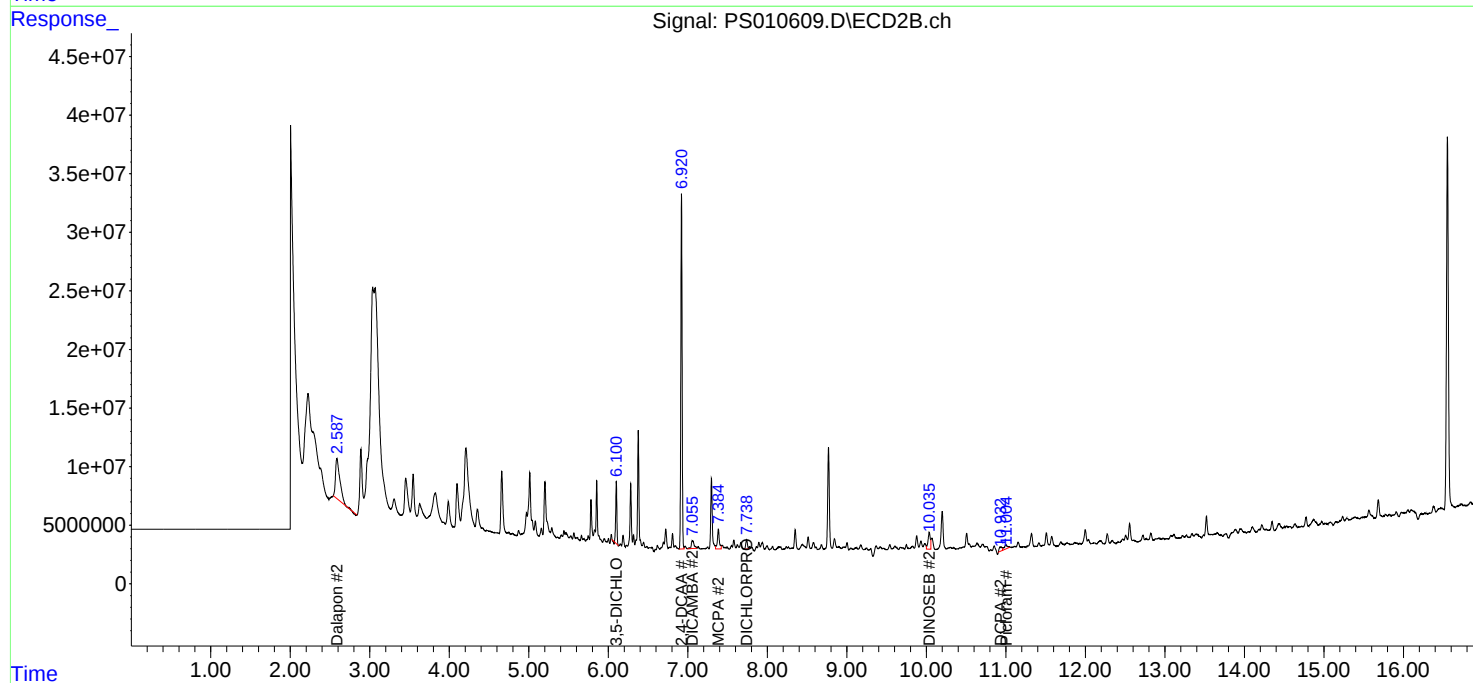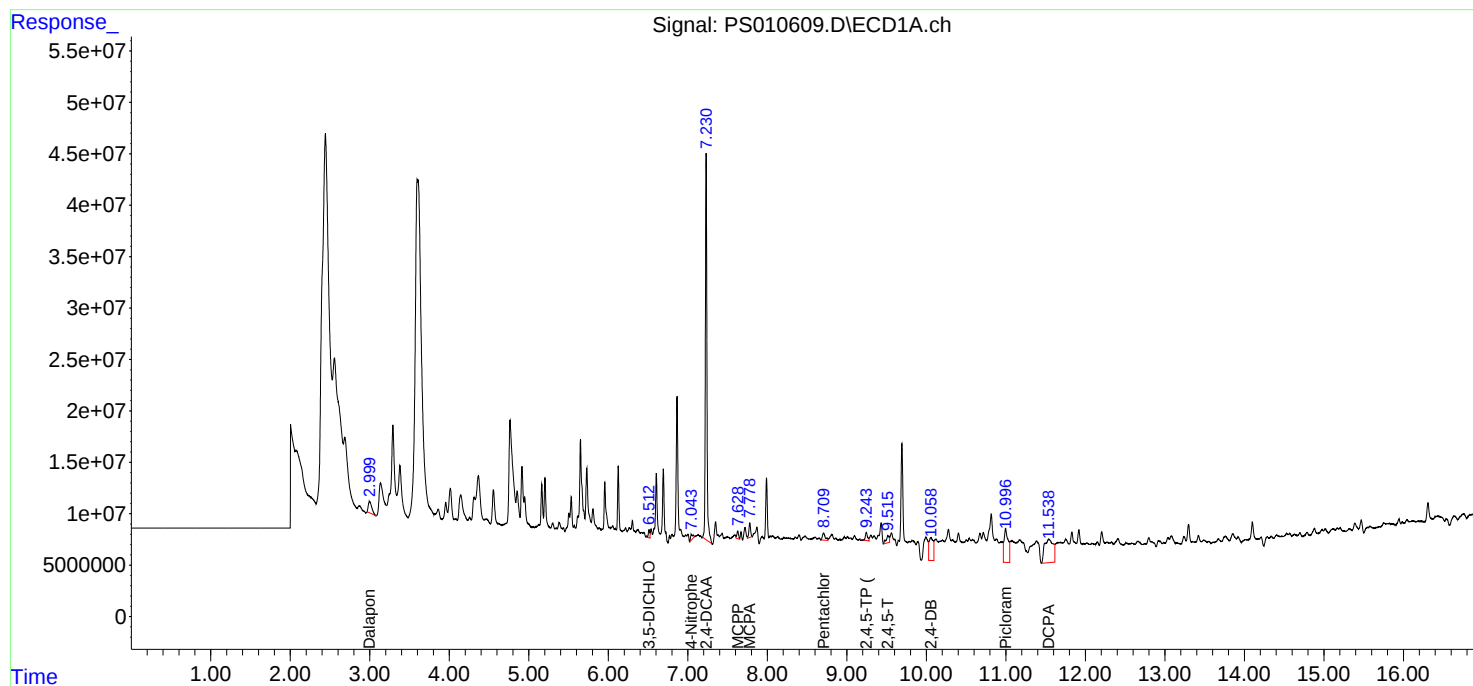

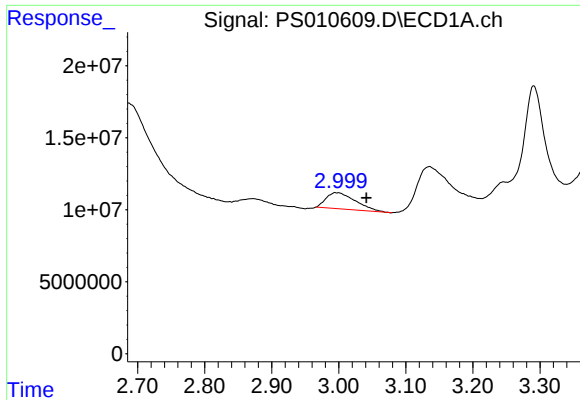


#1 Dalapon

R.T.: 2.997 min
Delta R.T.: -0.044 min
Response: 33848123
Conc: 34.43 ng/ml

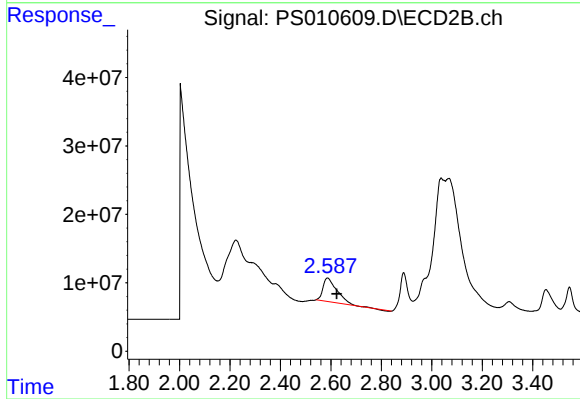


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.037 min
Response: 129058778
Conc: 176.28 ng/ml

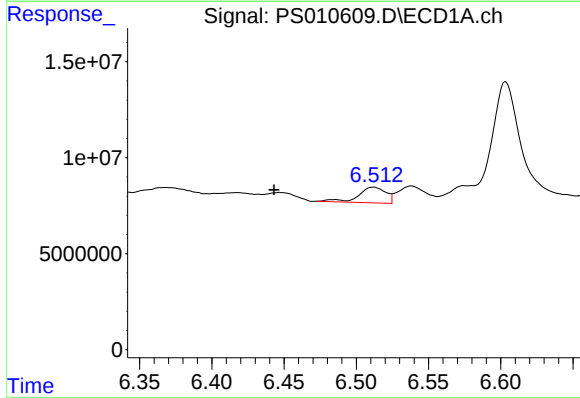


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.512 min
Delta R.T.: 0.069 min
Response: 10773260
Conc: 9.85 ng/ml

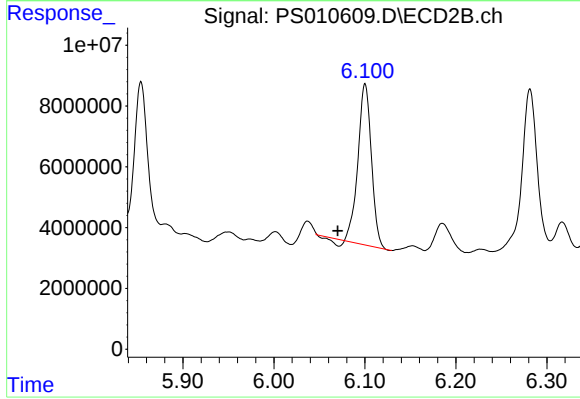


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 53663556
Conc: 65.47 ng/ml

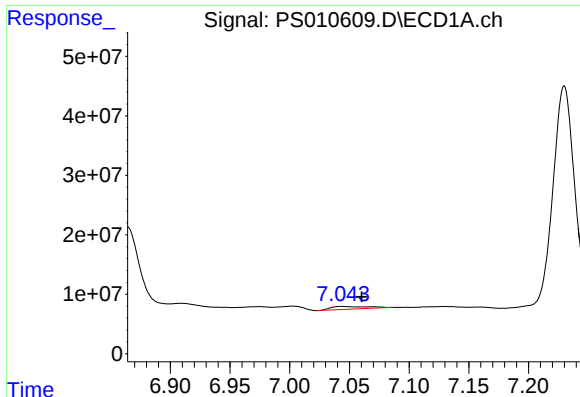


#3 4-Nitrophenol

R.T.: 7.044 min
Delta R.T.: -0.016 min
Response: 10182551
Conc: 27.47 ng/ml

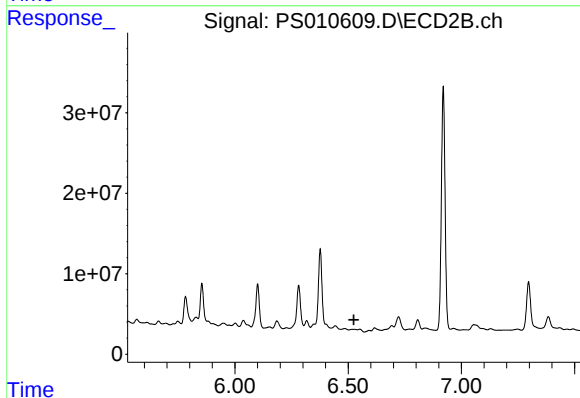


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

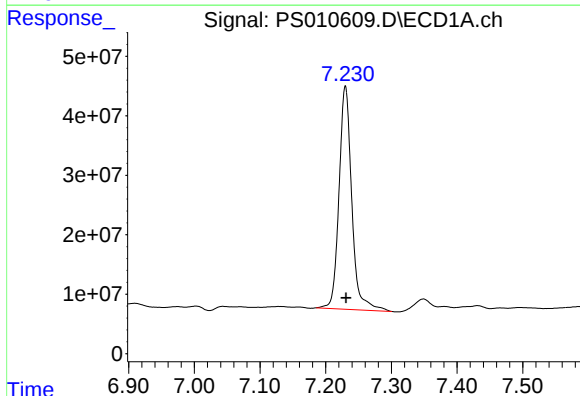


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: -0.001 min
Response: 505222375
Conc: 638.83 ng/ml

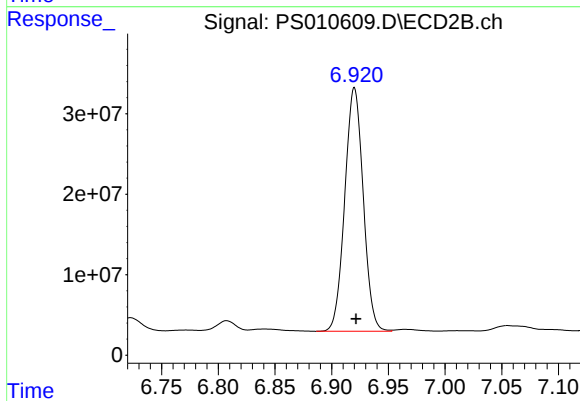


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 343142570
Conc: 629.14 ng/ml

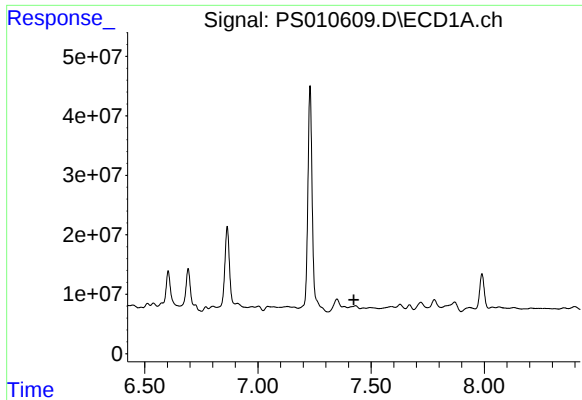


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.423 min
Response: 0
Conc: N.D.

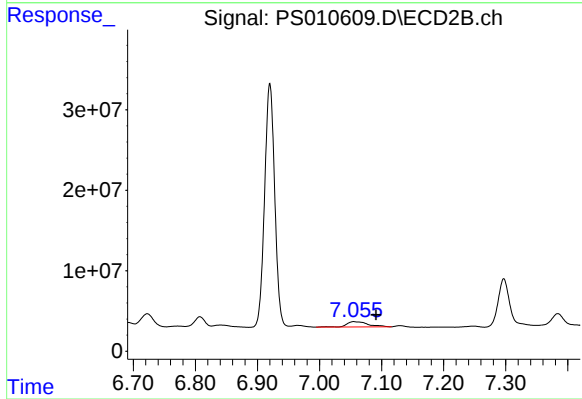


#5 DICAMBA

R.T.: 7.056 min
Delta R.T.: -0.035 min
Response: 16108551
Conc: 7.16 ng/ml

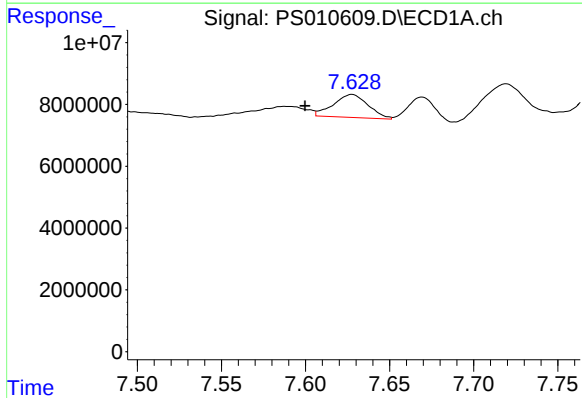


#6 MCP

R.T.: 7.627 min
Delta R.T.: 0.028 min
Response: 10744231
Conc: 4.35 ug/ml

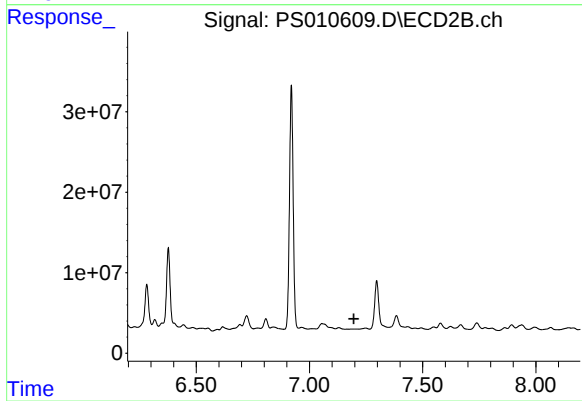


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.196 min
Response: 0
Conc: N.D.

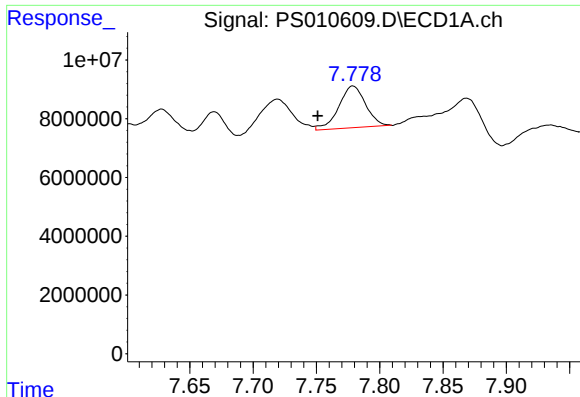


#7 MCPA

R.T.: 7.779 min
Delta R.T.: 0.028 min
Response: 20879935
Conc: 5.97 ug/ml

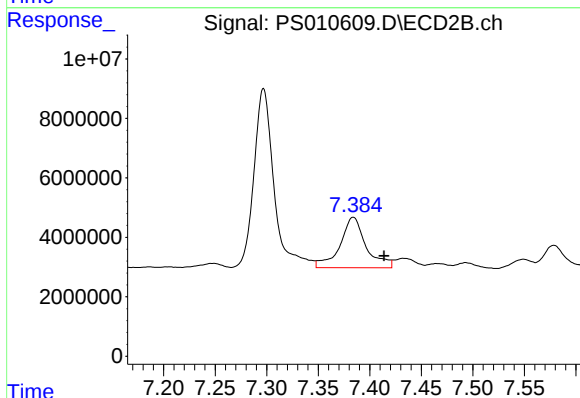


#7 MCPA

R.T.: 7.384 min
Delta R.T.: -0.030 min
Response: 29749255
Conc: 10.95 ug/ml

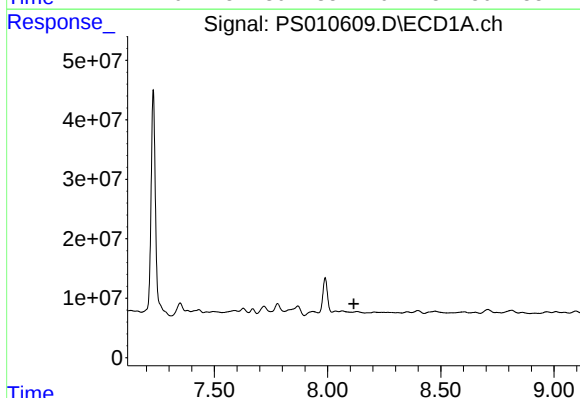


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

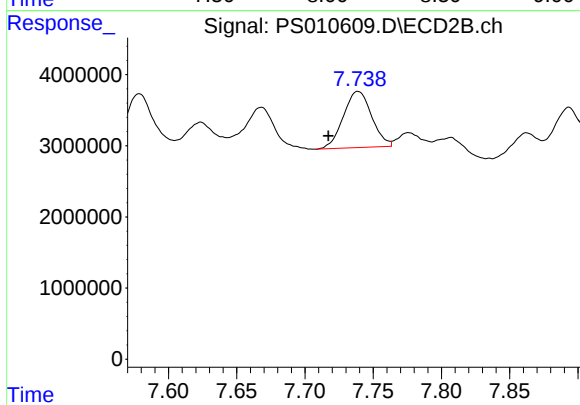


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.022 min
Response: 11406287
Conc: 19.78 ng/ml

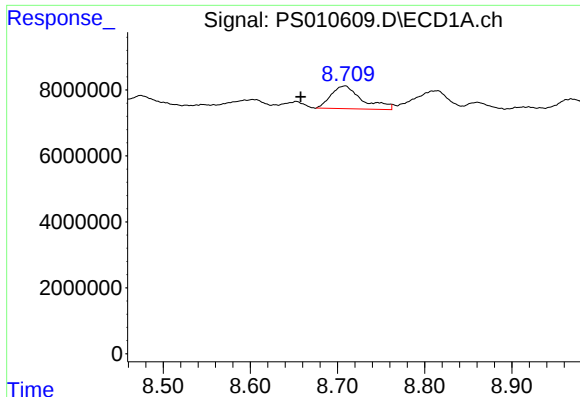


#10 Pentachlorophenol

R.T.: 8.708 min
Delta R.T.: 0.050 min
Response: 16926703
Conc: 1.59 ng/ml

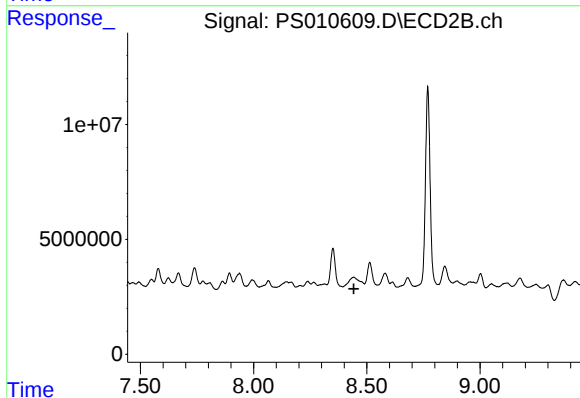


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 8.443 min
Response: 0
Conc: N.D.

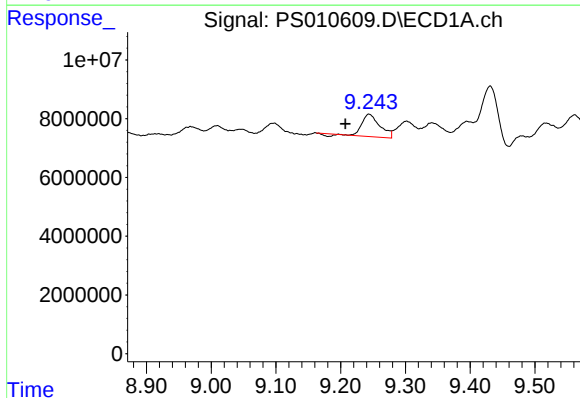


#11 2,4,5-TP (SILVEX)

R.T.: 9.244 min
Delta R.T.: 0.036 min
Response: 13816593
Conc: 3.23 ng/ml

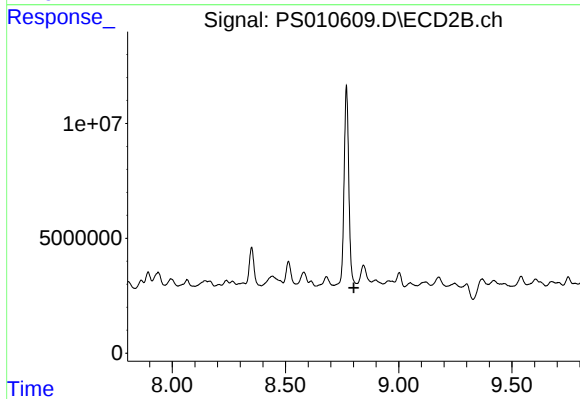


#11 2,4,5-TP (SILVEX)

R.T.: 8.844 min
Delta R.T.: 0.042 min
Response: -46427332
Conc: N.D.

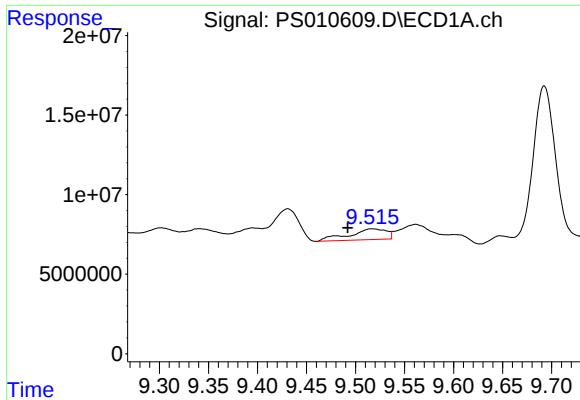


#12 2,4,5-T

R.T.: 9.517 min
Delta R.T.: 0.025 min
Response: 18043787
Conc: 4.44 ng/ml

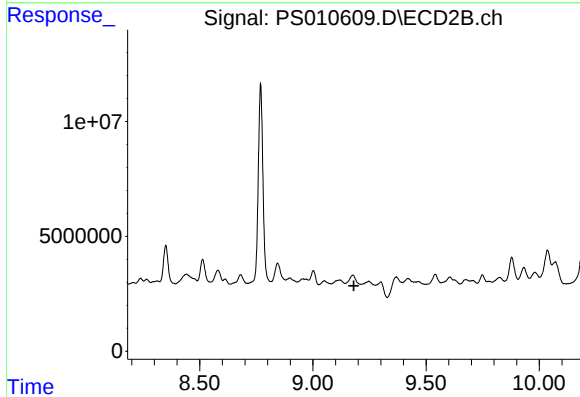


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

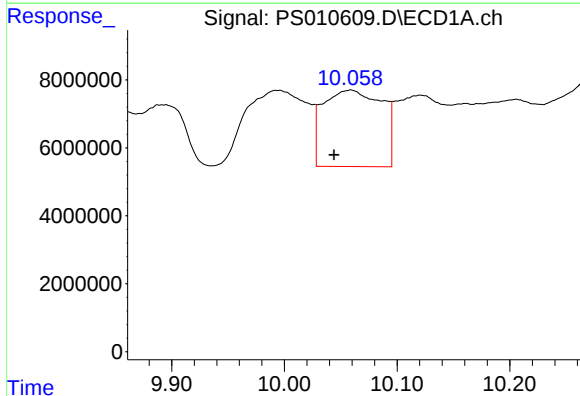


#13 2,4-DB

R.T.: 10.058 min
Delta R.T.: 0.014 min
Response: 81924917
Conc: 148.17 ng/ml

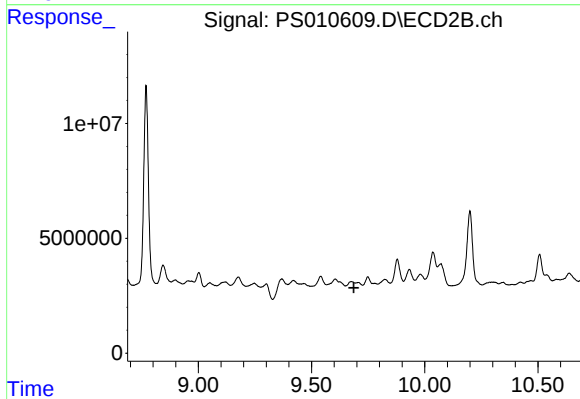


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.687 min
Response: 0
Conc: N.D.

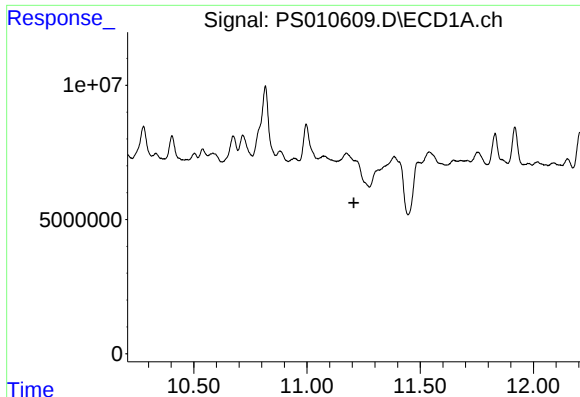


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.207 min
Response: 0
Conc: N.D.

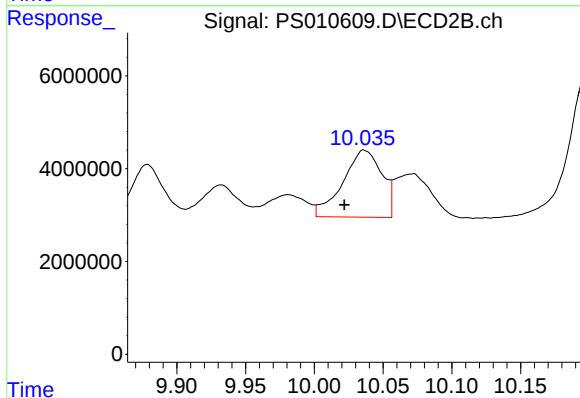


#14 DINOSEB

R.T.: 10.037 min
Delta R.T.: 0.015 min
Response: 28634755
Conc: 13.31 ng/ml

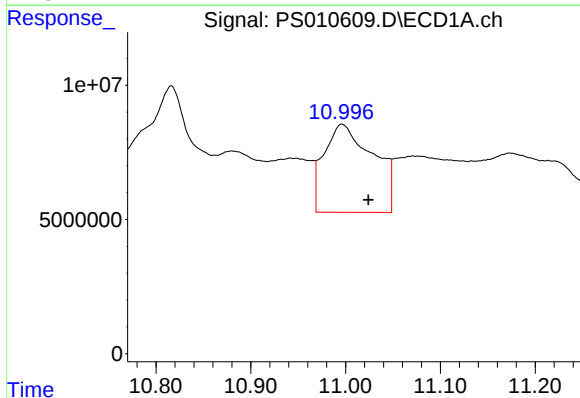


#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.028 min
Response: 118166313
Conc: 23.15 ng/ml

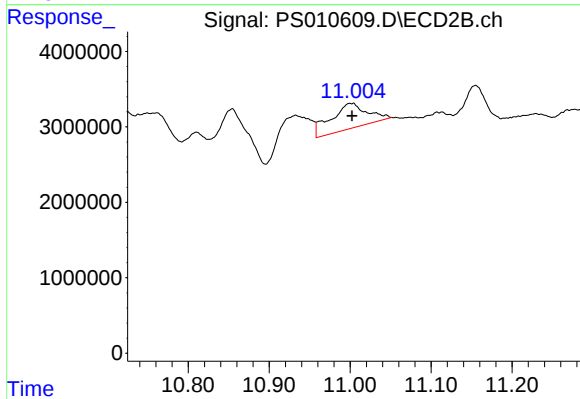


#15 Picloram

R.T.: 11.001 min
Delta R.T.: -0.001 min
Response: 10436601
Conc: 2.53 ng/ml

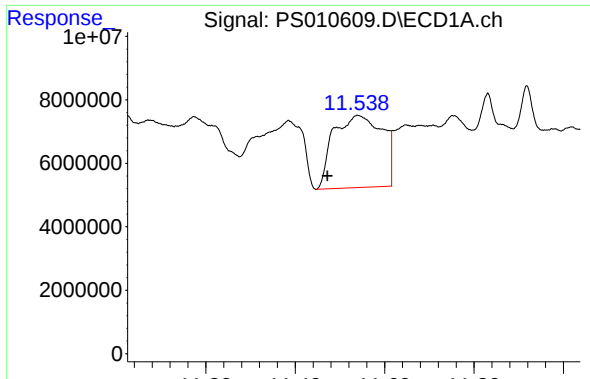

#16 DCPA

R.T.: 11.540 min
Delta R.T.: 0.067 min
Response: 173287546
Conc: 32.34 ng/ml

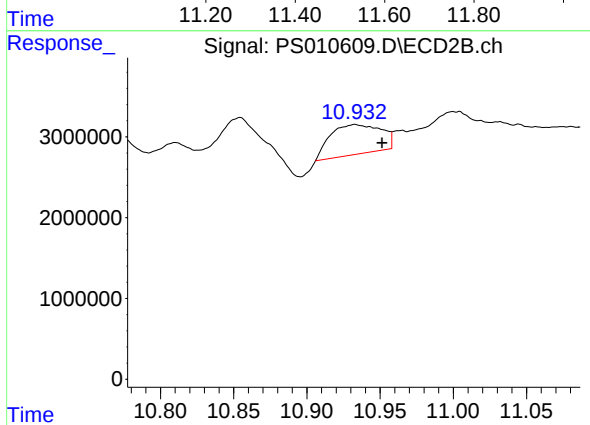

#16 DCPA

R.T.: 10.933 min
Delta R.T.: -0.018 min
Response: 8854295
Conc: 2.39 ng/ml