

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
 Data File : PS015145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2021 11:01
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:30:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.787	2003.9E6	396.4E6	795.091	739.900
Target Compounds							
1) T	Dalapon	3.040	2.522	1818.5E6	443.7E6	691.855	678.032
2) T	3,5-DICHL...	6.437	5.973	2581.6E6	560.6E6	748.645	693.986
3) T	4-Nitroph...	7.051	6.404	1027.0E6	213.5E6	728.549	670.948
5) T	DICAMBA	7.419	6.953	7086.8E6	1544.9E6	743.496	698.124
6) T	MCPD	7.590	7.050	536.6E6	119.7E6	74.566	67.722
7) T	MCPA	7.738	7.264	732.6E6	175.4E6	72.990	67.485
8) T	DICHLORPROP	8.113	7.575	1709.8E6	377.2E6	742.411	694.330
9) T	2,4-D	8.340	7.865	1905.9E6	448.1E6	747.949	695.801
10) T	Pentachlo...	8.655	8.297	24243.6E6	5188.7E6	748.935	704.871
11) T	2,4,5-TP ...	9.205	8.659	9294.9E6	2061.1E6	748.925	710.237
12) T	2,4,5-T	9.487	9.036	9083.6E6	2077.0E6	756.282	717.442
13) T	2,4-DB	10.037	9.543	1941.1E6	267.3E6	762.263	692.827
14) T	DINOSEB	11.202	9.872	6047.1E6	1349.2E6	756.877	738.850
15) T	Picloram	11.015	10.850	12366.0E6	2993.8E6	746.436	720.900
16) T	DCPA	11.471	10.806	12813.7E6	3120.3E6	759.914	723.795



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
Data File : PS015145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2021 11:01
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:30:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

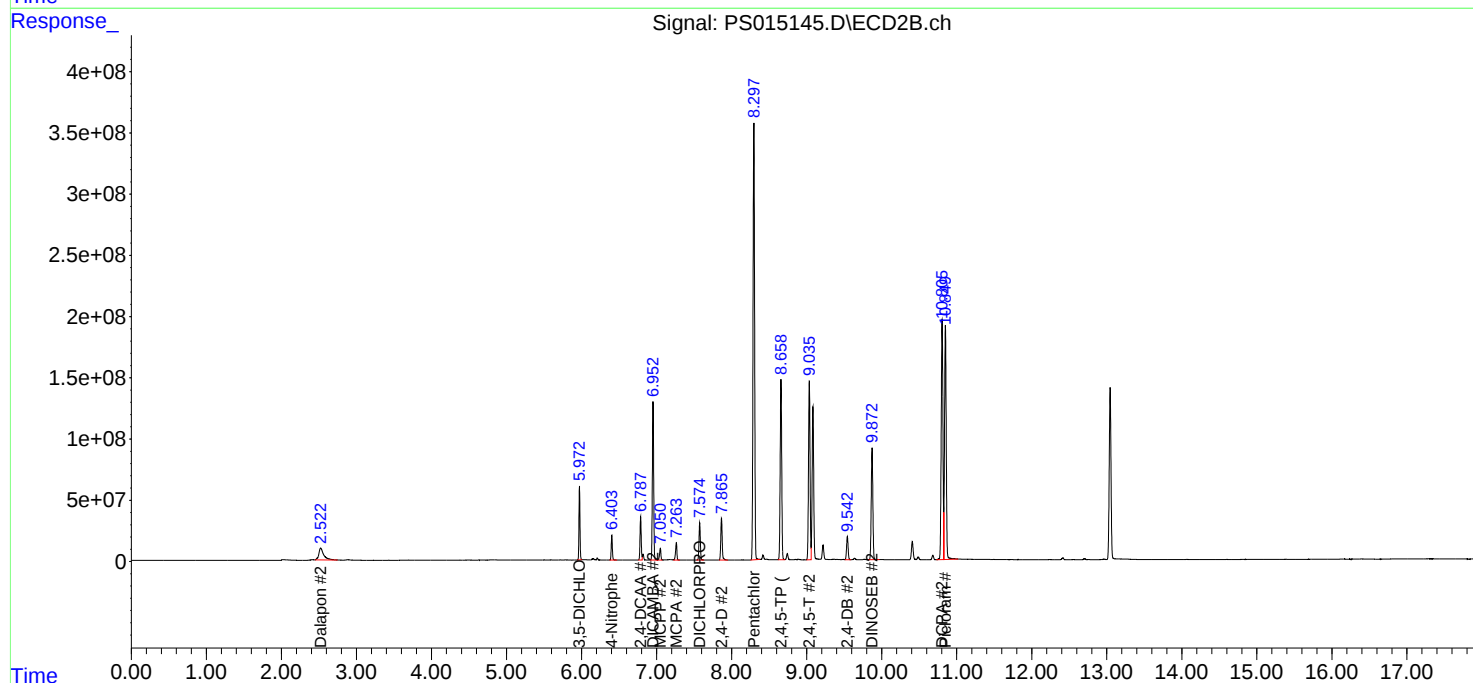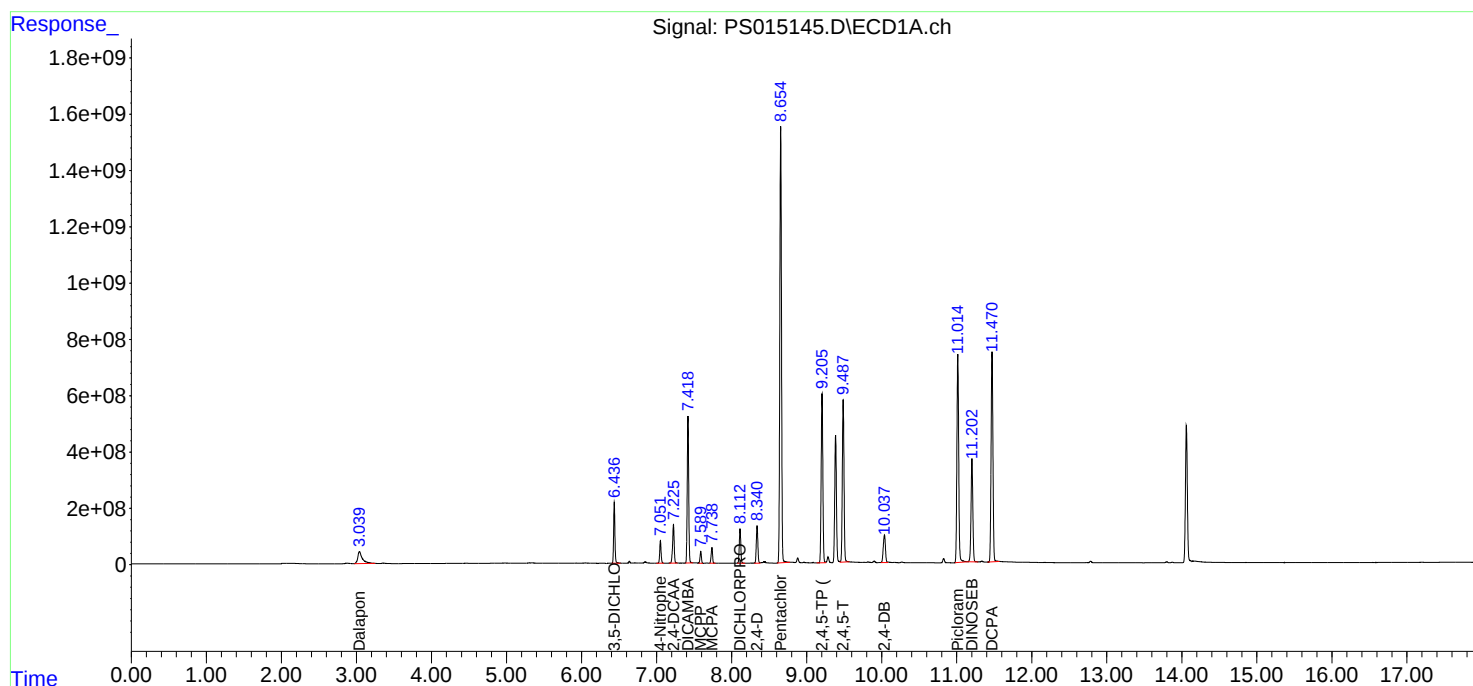


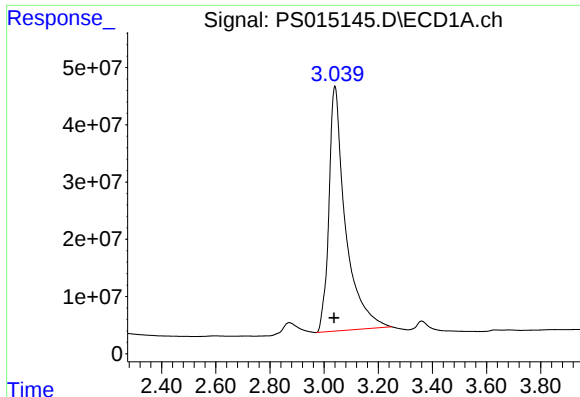

#1 Dalapon


R.T.: 3.040 min
Delta R.T.: 0.003 min
Response: 1818456383
Conc: 691.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

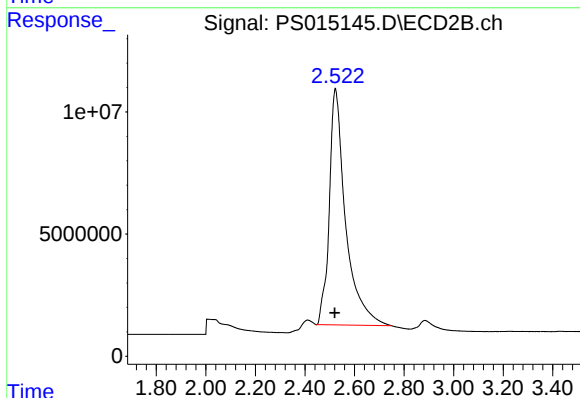


#1 Dalapon

R.T.: 2.522 min
Delta R.T.: 0.002 min
Response: 443739692
Conc: 678.03 ng/ml

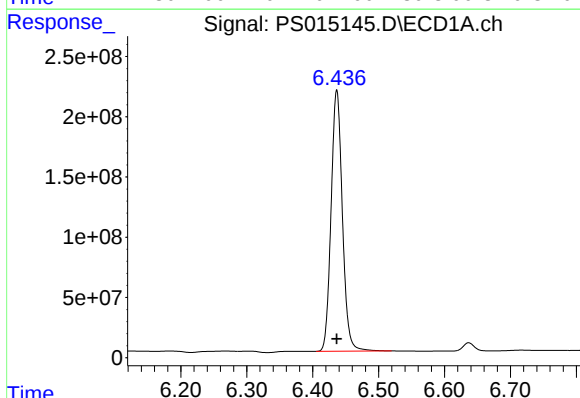


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.437 min
Delta R.T.: 0.000 min
Response: 2581636172
Conc: 748.64 ng/ml

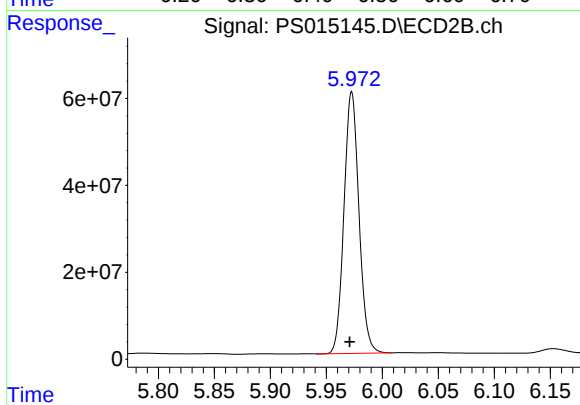

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.973 min
Delta R.T.: 0.002 min
Response: 560632515
Conc: 693.99 ng/ml

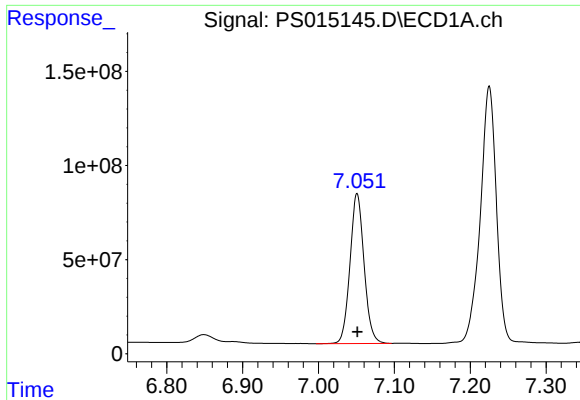

#3 4-Nitrophenol


R.T.: 7.051 min
Delta R.T.: 0.000 min
Response: 1027034056
Conc: 728.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

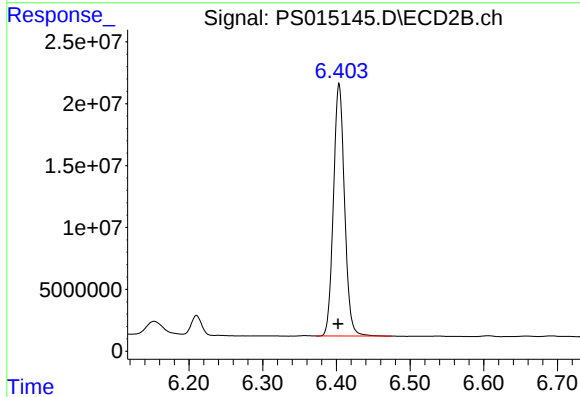


#3 4-Nitrophenol

R.T.: 6.404 min
Delta R.T.: 0.002 min
Response: 213478291
Conc: 670.95 ng/ml

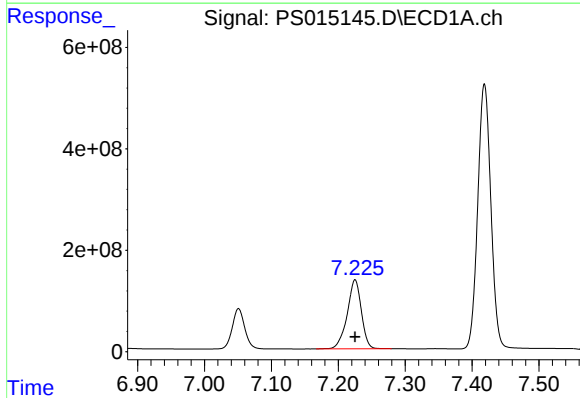


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 2003927864
Conc: 795.09 ng/ml

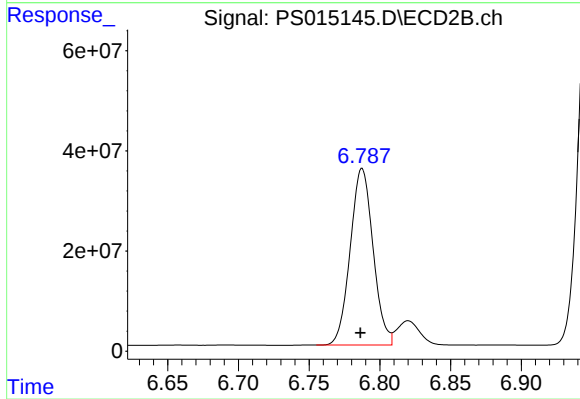

#4 2,4-DCAA


R.T.: 6.787 min
Delta R.T.: 0.001 min
Response: 396416862
Conc: 739.90 ng/ml

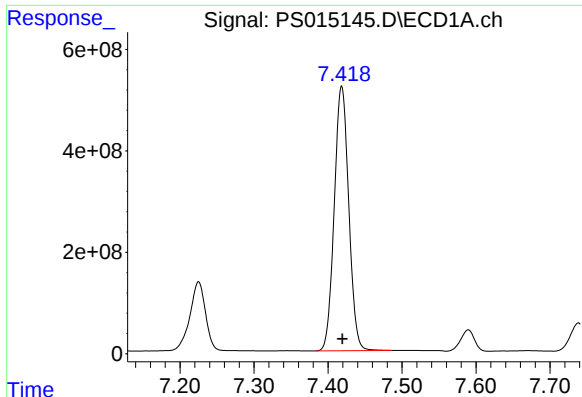

#5 DICAMBA


R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 7086817340
Conc: 743.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

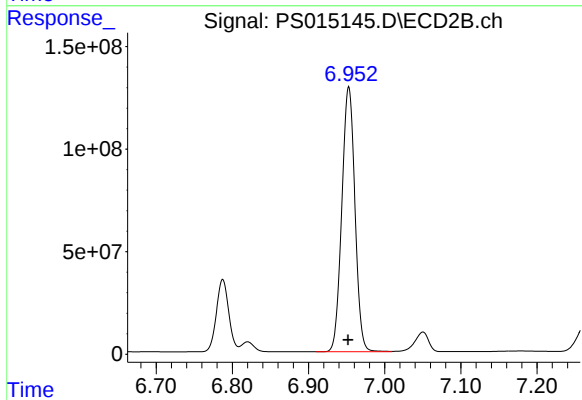


#5 DICAMBA

R.T.: 6.953 min
Delta R.T.: 0.001 min
Response: 1544904130
Conc: 698.12 ng/ml

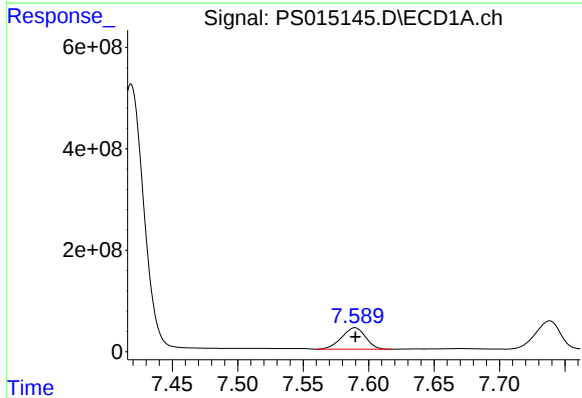


#6 MCP

R.T.: 7.590 min
Delta R.T.: 0.000 min
Response: 536600147
Conc: 74.57 ug/ml

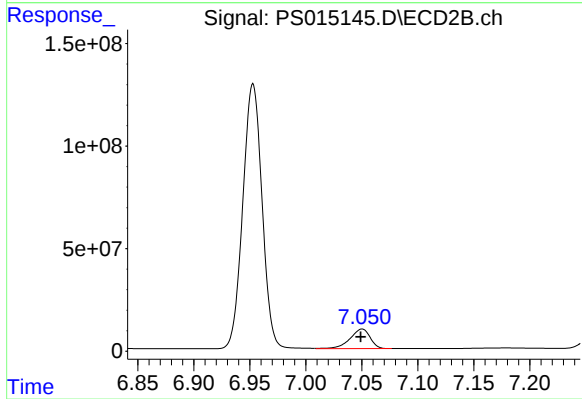

#6 MCP


R.T.: 7.050 min
Delta R.T.: 0.001 min
Response: 119672069
Conc: 67.72 ug/ml

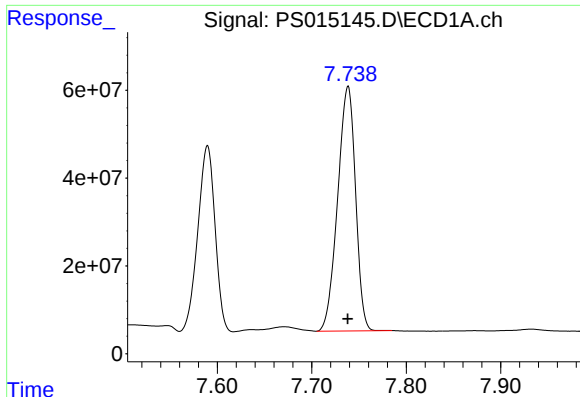

#7 MCPA


R.T.: 7.738 min
Delta R.T.: 0.000 min
Response: 732563670
Conc: 72.99 ug/ml

Instrument :
ECD_S
ClientSampleId :

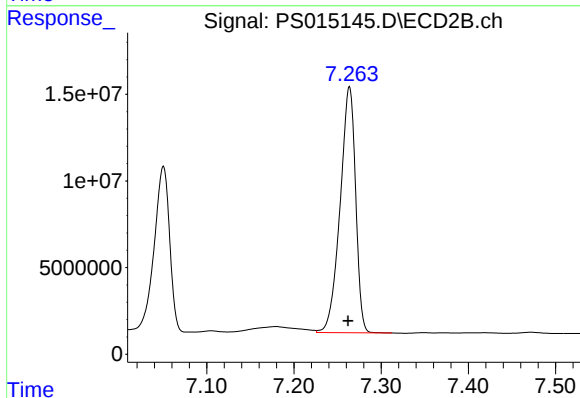


#7 MCPA

R.T.: 7.264 min
Delta R.T.: 0.001 min
Response: 175378718
Conc: 67.49 ug/ml

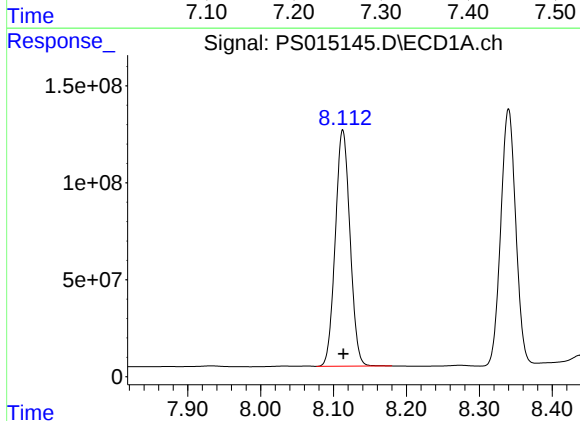


#8 DICHLORPROP

R.T.: 8.113 min
Delta R.T.: 0.000 min
Response: 1709849282
Conc: 742.41 ng/ml

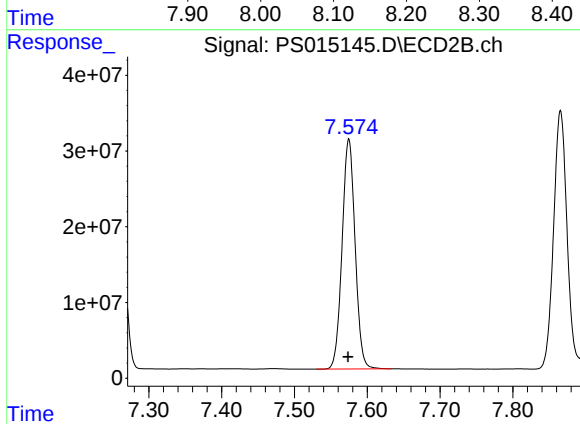

#8 DICHLORPROP


R.T.: 7.575 min
Delta R.T.: 0.001 min
Response: 377204507
Conc: 694.33 ng/ml

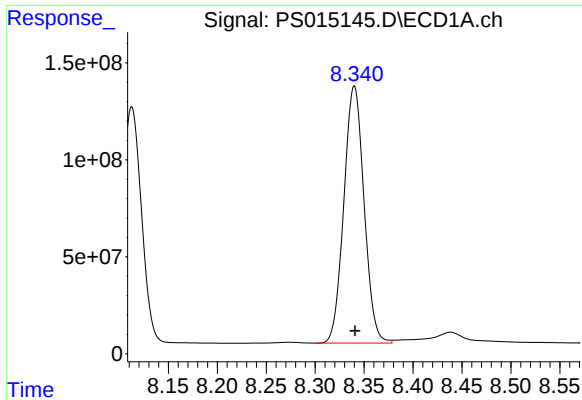

#9 2,4-D


R.T.: 8.340 min
Delta R.T.: 0.000 min
Response: 1905861661
Conc: 747.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

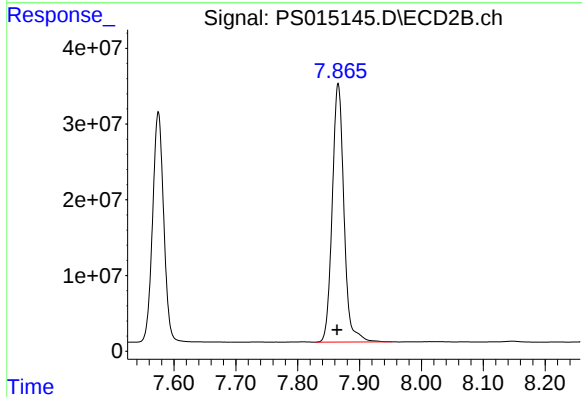


#9 2,4-D

R.T.: 7.865 min
Delta R.T.: 0.002 min
Response: 448113369
Conc: 695.80 ng/ml

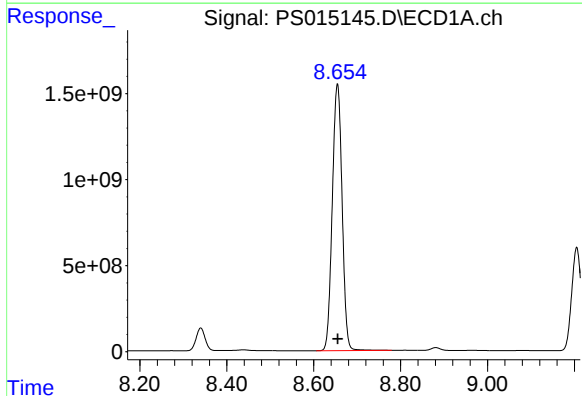


#10 Pentachlorophenol

R.T.: 8.655 min
Delta R.T.: 0.000 min
Response: 24243624259
Conc: 748.94 ng/ml

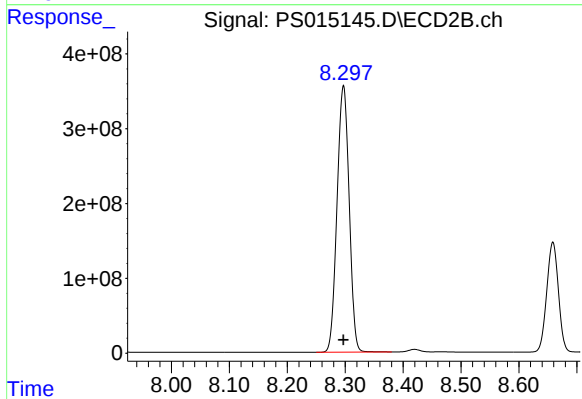

#10 Pentachlorophenol


R.T.: 8.297 min
Delta R.T.: 0.000 min
Response: 5188694041
Conc: 704.87 ng/ml

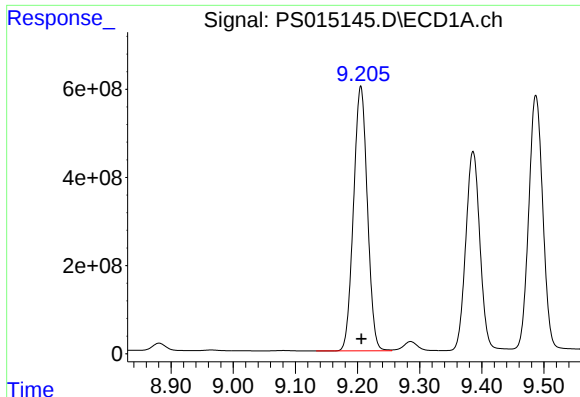

#11 2,4,5-TP (SILVEX)


R.T.: 9.205 min
Delta R.T.: -0.001 min
Response: 9294912990
Conc: 748.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

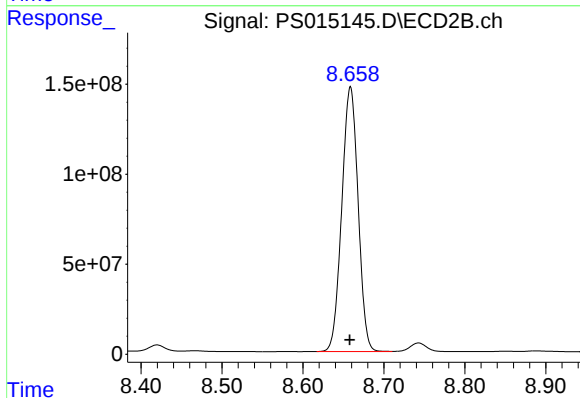


#11 2,4,5-TP (SILVEX)

R.T.: 8.659 min
Delta R.T.: 0.000 min
Response: 2061064684
Conc: 710.24 ng/ml

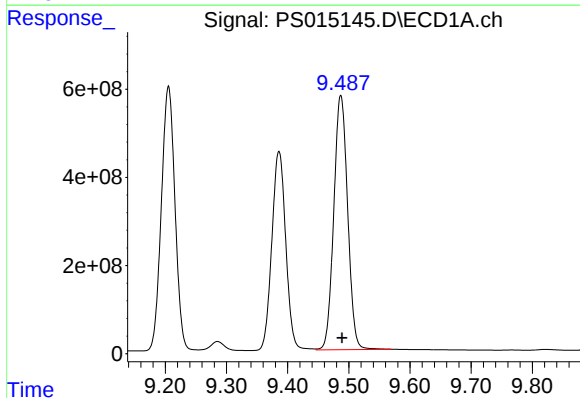


#12 2,4,5-T

R.T.: 9.487 min
Delta R.T.: -0.002 min
Response: 9083625219
Conc: 756.28 ng/ml

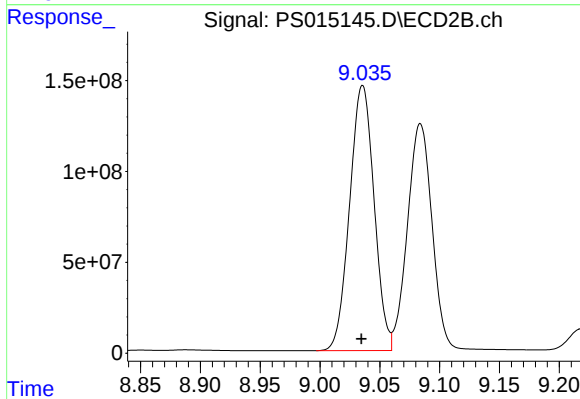

#12 2,4,5-T


R.T.: 9.036 min
Delta R.T.: 0.000 min
Response: 2076995578
Conc: 717.44 ng/ml

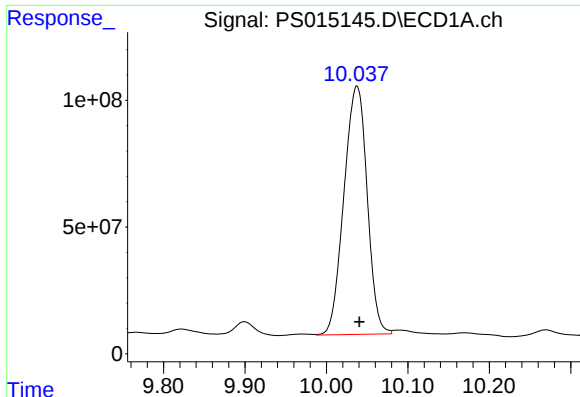

#13 2,4-DB


R.T.: 10.037 min
Delta R.T.: -0.003 min
Response: 1941122219
Conc: 762.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

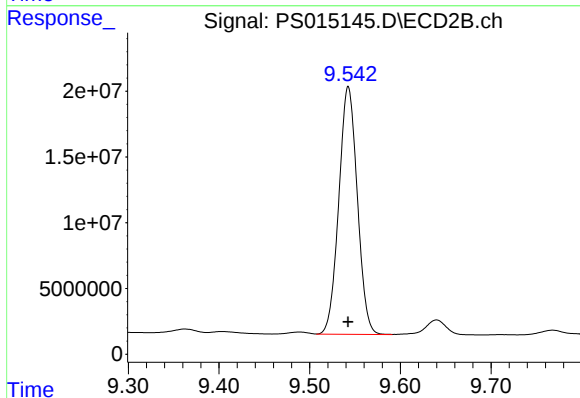


#13 2,4-DB

R.T.: 9.543 min
Delta R.T.: 0.000 min
Response: 267257513
Conc: 692.83 ng/ml

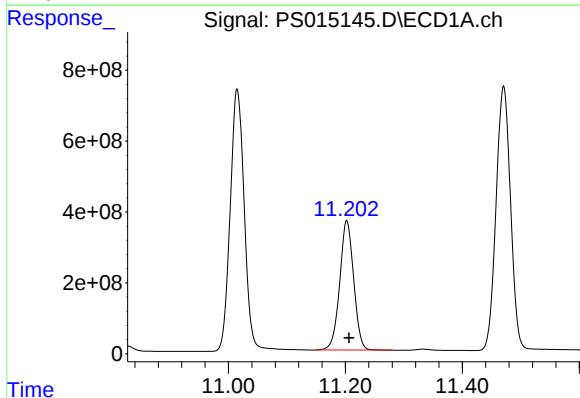


#14 DINOSEB

R.T.: 11.202 min
Delta R.T.: -0.004 min
Response: 6047126224
Conc: 756.88 ng/ml

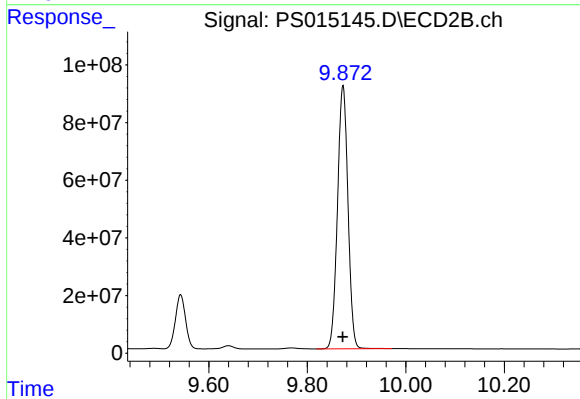

#14 DINOSEB


R.T.: 9.872 min
Delta R.T.: 0.000 min
Response: 1349244651
Conc: 738.85 ng/ml

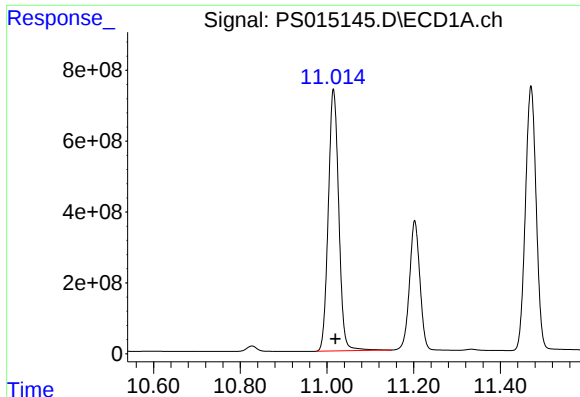

#15 Picloram


R.T.: 11.015 min
Delta R.T.: -0.004 min
Response: 12366033716
Conc: 746.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

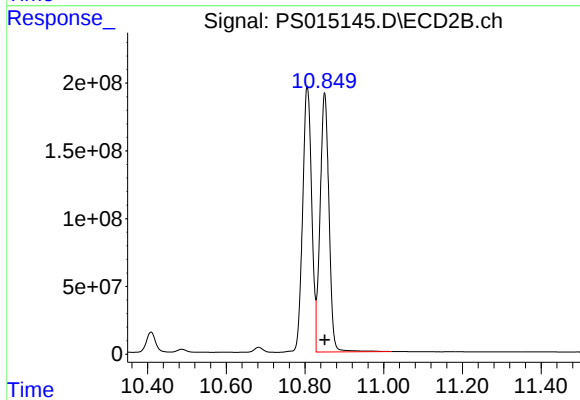


#15 Picloram

R.T.: 10.850 min
Delta R.T.: 0.000 min
Response: 2993821147
Conc: 720.90 ng/ml

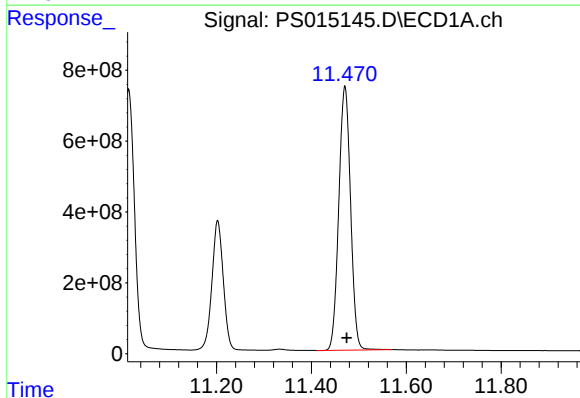

#16 DCPA

R.T.: 11.471 min
Delta R.T.: -0.004 min
Response: 12813727186
Conc: 759.91 ng/ml

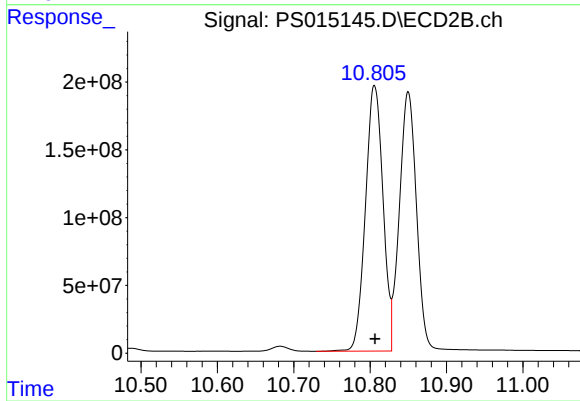

#16 DCPA

R.T.: 10.806 min
Delta R.T.: 0.000 min
Response: 3120277892
Conc: 723.80 ng/ml