

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
 Data File : PS015148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2021 15:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:31:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.783	1171.0E6	255.5E6	464.606	476.970
Target Compounds							
3) T	4-Nitroph...	7.020	0.000	6067166	0	4.304	N.D. #
9) T	2,4-D	8.341	0.000	6139364	0	2.409	N.D. #
12) T	2,4,5-T	9.486	0.000	10858740	0	<MDL	N.D. #
13) T	2,4-DB	10.012	0.000	3331436	0	1.308	N.D. #
15) T	Picloram	11.016	10.848	99425723	22863017	6.002	5.505
16) T	DCPA	0.000	10.848f	0	22863017	N.D.	5.303



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
Data File : PS015148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2021 15:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:31:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

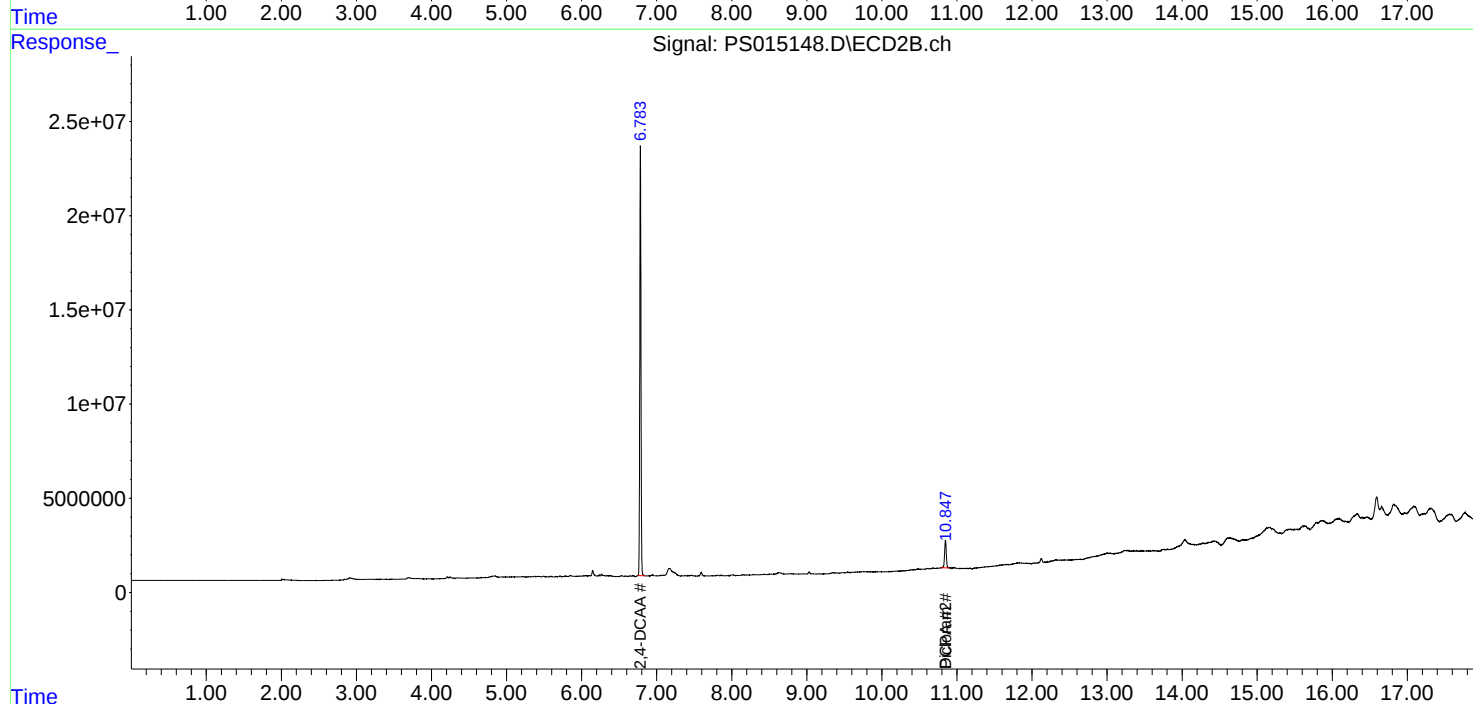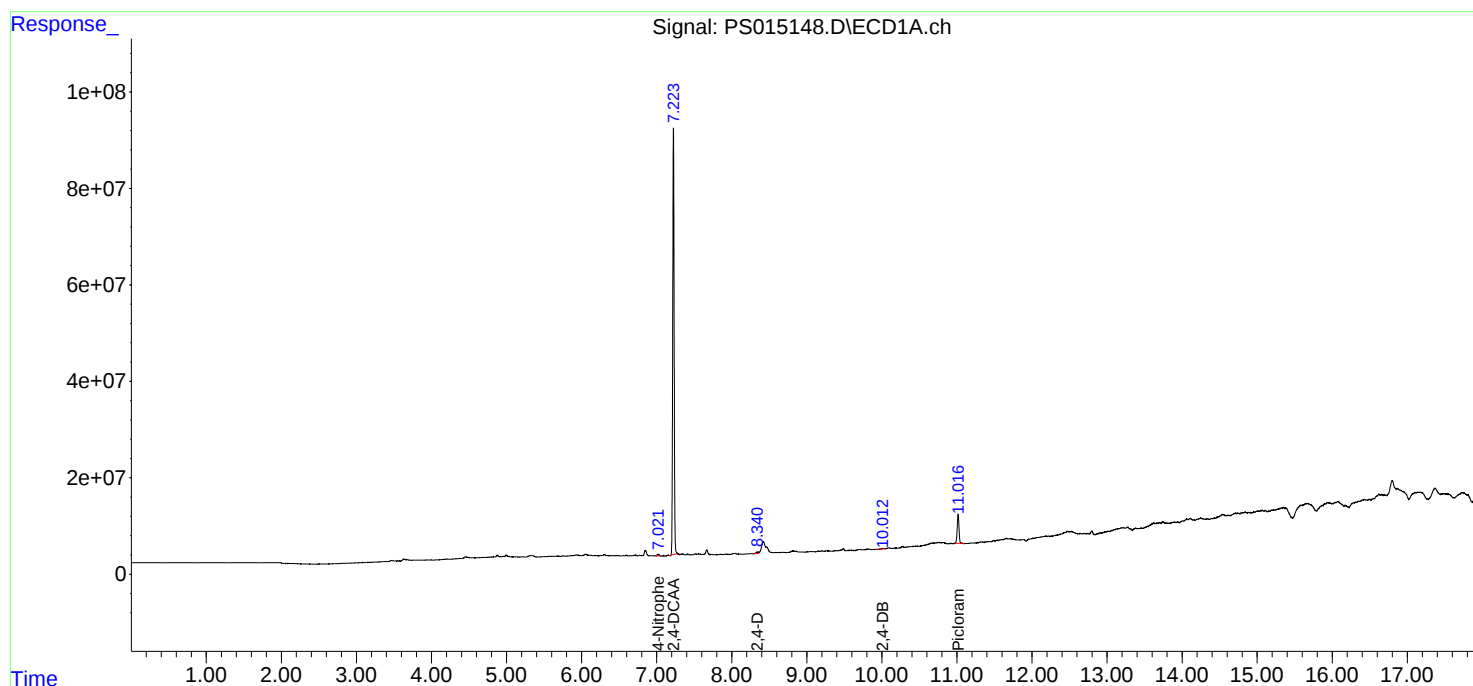


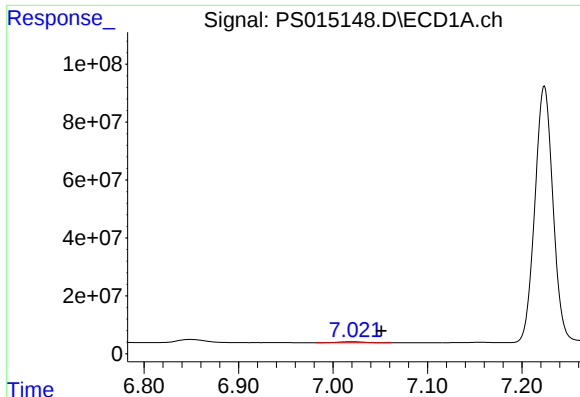

#3 4-Nitrophenol


R.T.: 7.020 min
Delta R.T.: -0.031 min
Response: 6067166
Conc: 4.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

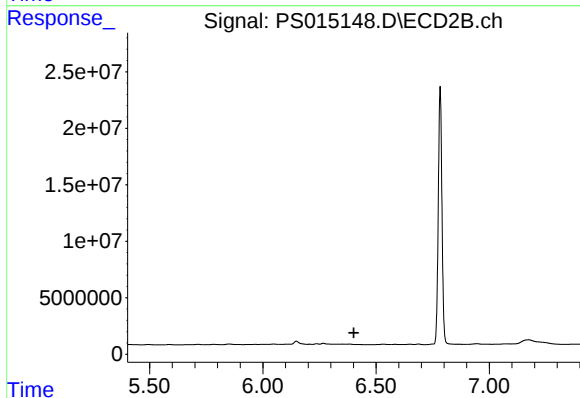


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

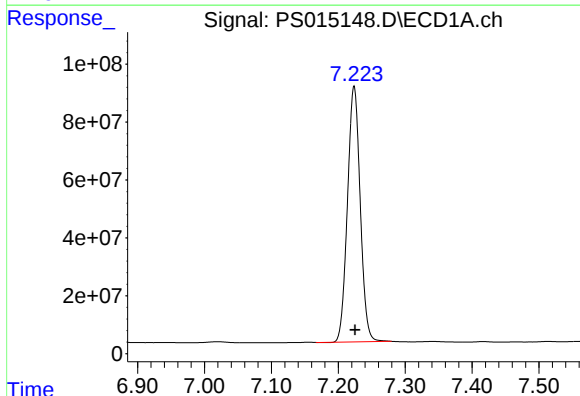


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: -0.001 min
Response: 1170981467
Conc: 464.61 ng/ml

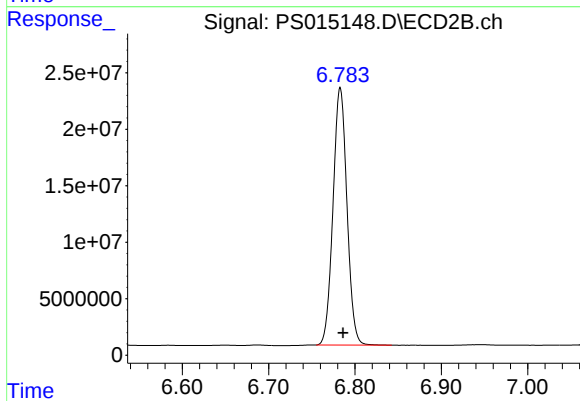

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: -0.003 min
Response: 255546983
Conc: 476.97 ng/ml

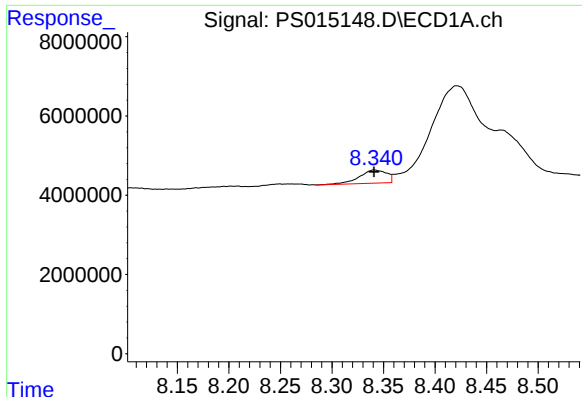

#9 2,4-D


R.T.: 8.341 min
Delta R.T.: 0.000 min
Response: 6139364
Conc: 2.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

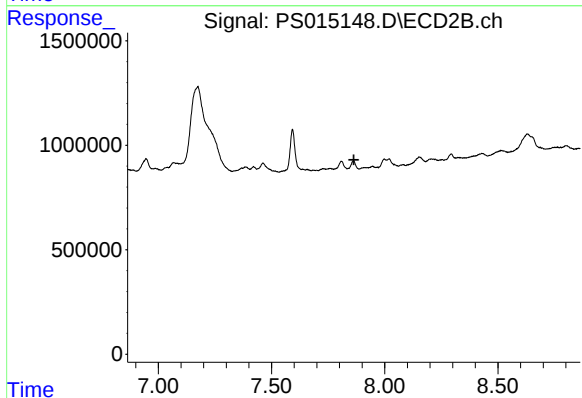


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

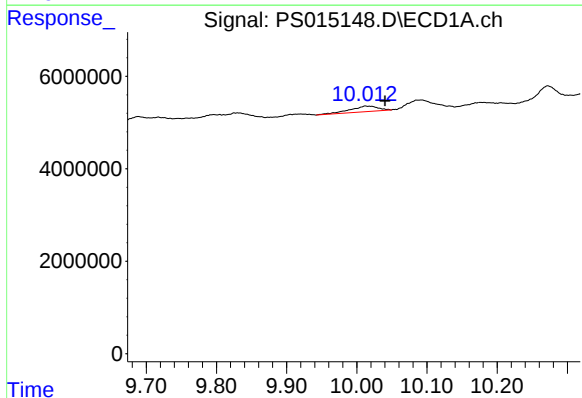


#13 2,4-DB

R.T.: 10.012 min
Delta R.T.: -0.028 min
Response: 3331436
Conc: 1.31 ng/ml

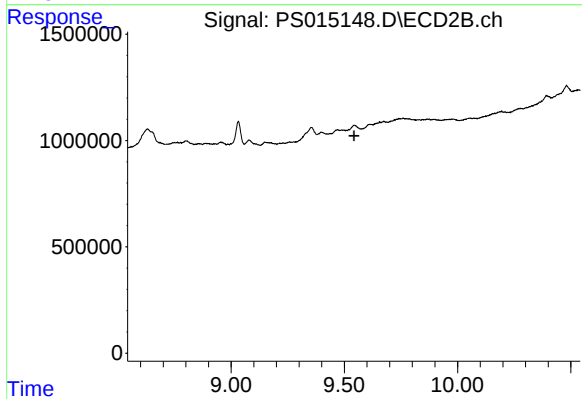

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.542 min
Response: 0
Conc: N.D.

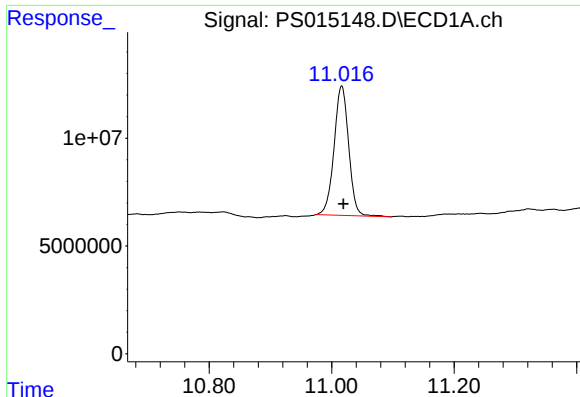

#15 Picloram


R.T.: 11.016 min
Delta R.T.: -0.003 min
Response: 99425723
Conc: 6.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

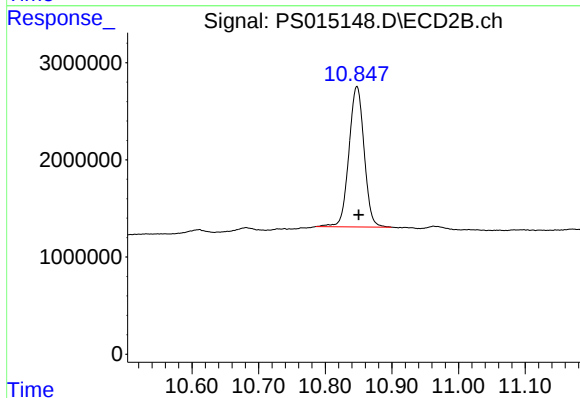


#15 Picloram

R.T.: 10.848 min
Delta R.T.: -0.003 min
Response: 22863017
Conc: 5.51 ng/ml

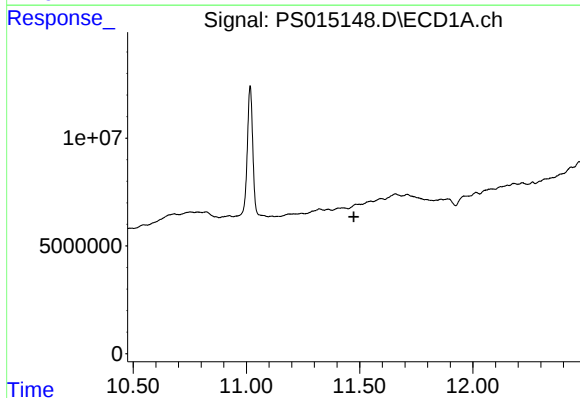

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.475 min
Response: 0
Conc: N.D.

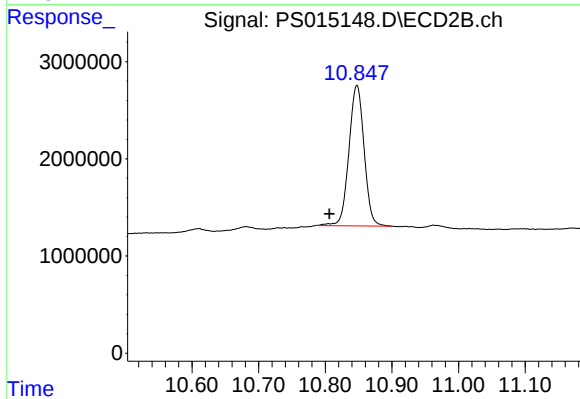

#16 DCPA

R.T.: 10.848 min
Delta R.T.: 0.041 min
Response: 22863017
Conc: 5.30 ng/ml