

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
 Data File : PS015157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2021 19:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:34:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.783	1133.7E6	258.4E6	449.827	482.332
Target Compounds							
3) T	4-Nitroph...	7.023	0.000	5534844	0	3.926	N.D. #
5) T	DICAMBA	7.417	0.000	6790438	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.591	0	3904238	N.D.	7.187
9) T	2,4-D	8.342	0.000	9475421	0	3.719	N.D. #
10) T	Pentachlo...	8.653	8.293	16156439	3614103	<MDL	<MDL #
11) T	2,4,5-TP ...	9.204	0.000	9400704	0	<MDL	N.D. #
12) T	2,4,5-T	9.487	0.000	10651868	0	<MDL	N.D. #
13) T	2,4-DB	10.016	0.000	6124713	0	2.405	N.D. #
15) T	Picloram	11.016	10.845	21695760	5224429	1.310	1.258
16) T	DCPA	11.471	10.845	12520563	5224429	<MDL	1.212 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
Data File : PS015157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2021 19:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:34:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

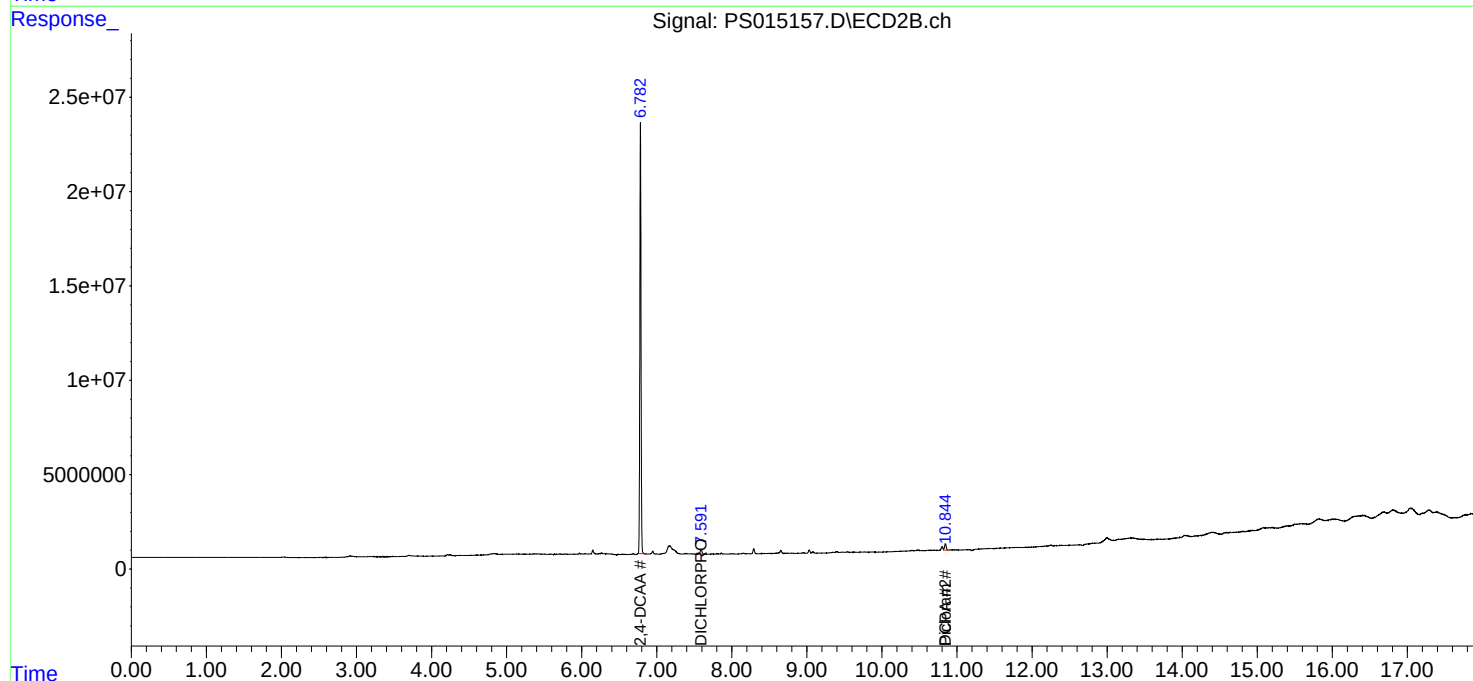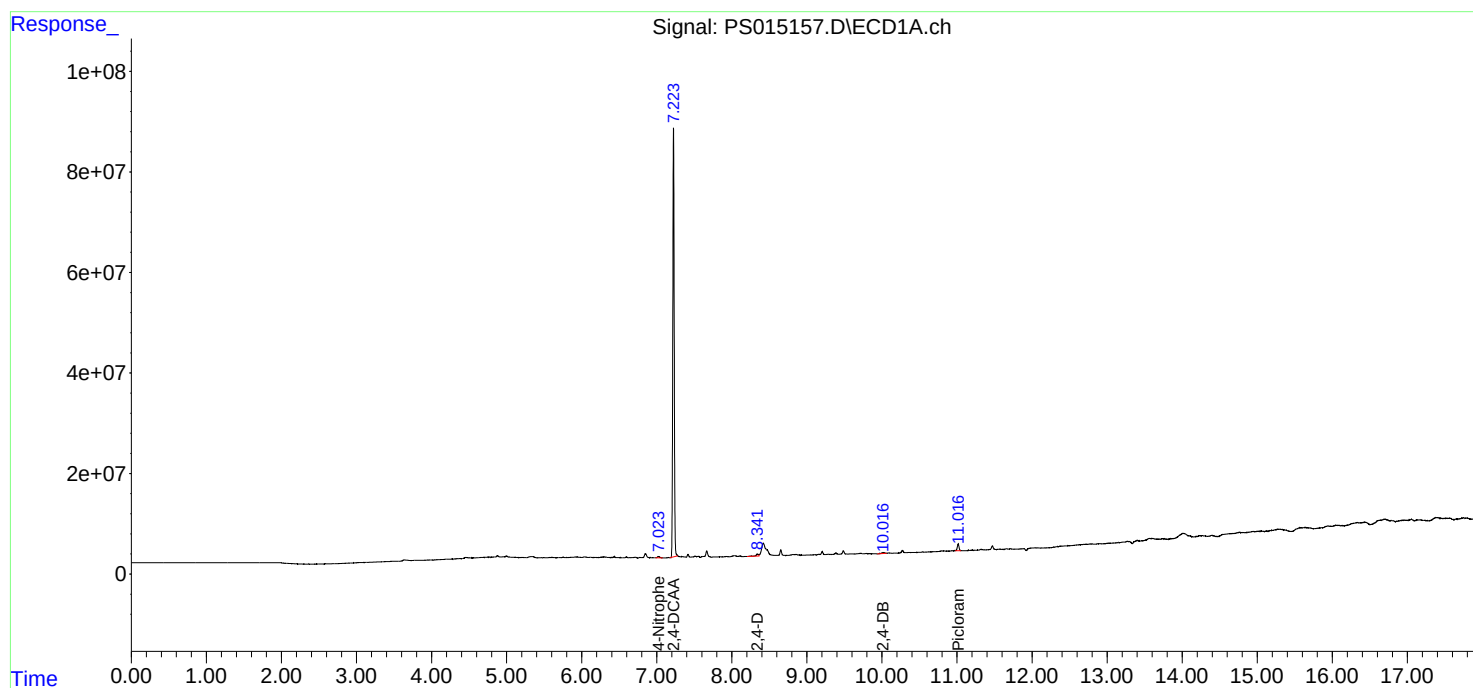


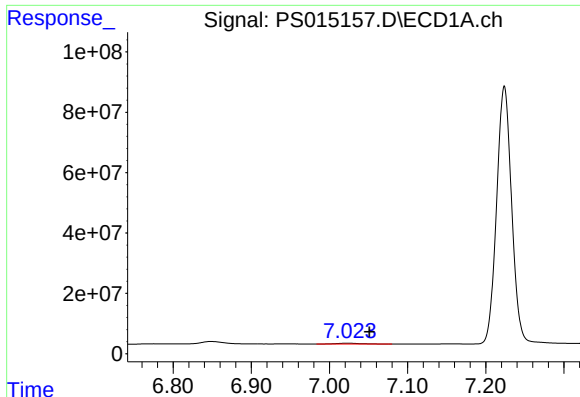

#3 4-Nitrophenol


R.T.: 7.023 min
Delta R.T.: -0.028 min
Response: 5534844
Conc: 3.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

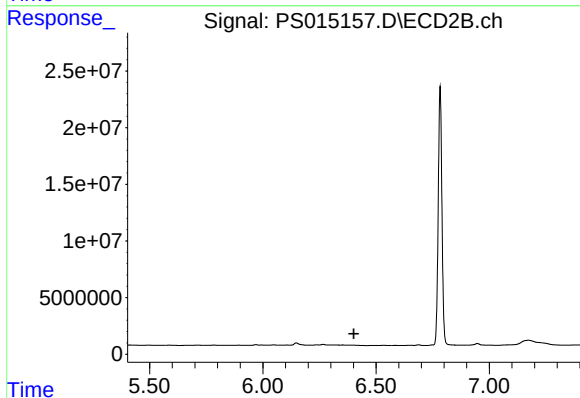


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

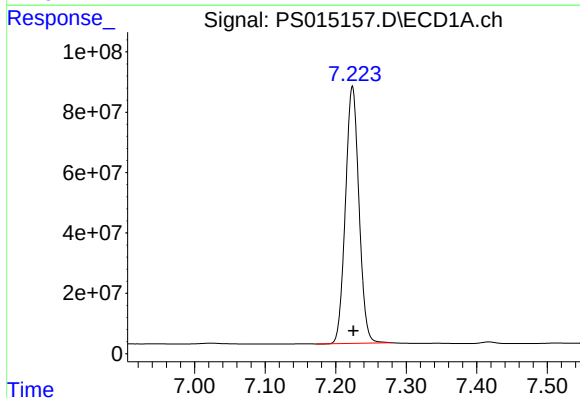


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: -0.001 min
Response: 1133733230
Conc: 449.83 ng/ml

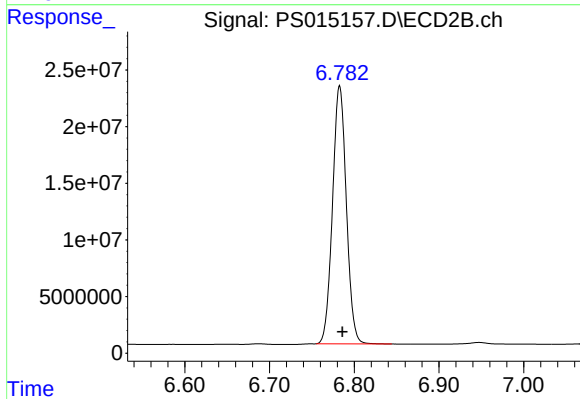

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: -0.003 min
Response: 258419353
Conc: 482.33 ng/ml

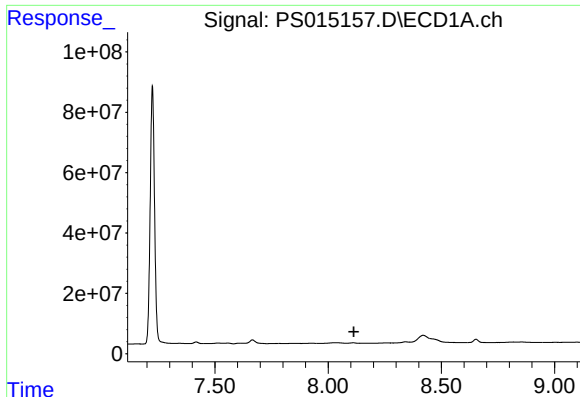

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

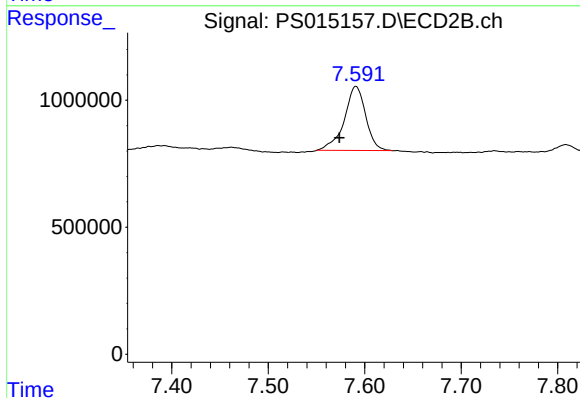


#8 DICHLORPROP

R.T.: 7.591 min
Delta R.T.: 0.017 min
Response: 3904238
Conc: 7.19 ng/ml

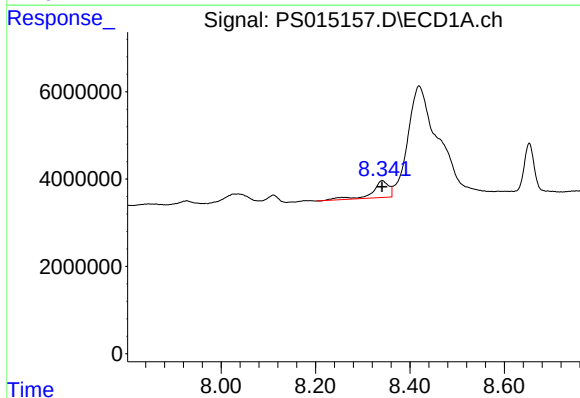


#9 2,4-D

R.T.: 8.342 min
Delta R.T.: 0.000 min
Response: 9475421
Conc: 3.72 ng/ml

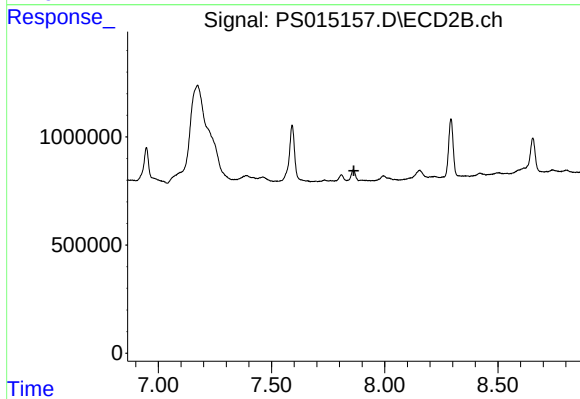

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.864 min
Response: 0
Conc: N.D.

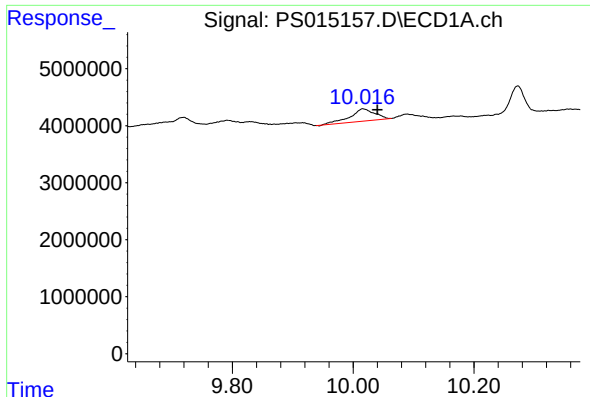

#13 2,4-DB


R.T.: 10.016 min
Delta R.T.: -0.024 min
Response: 6124713
Conc: 2.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

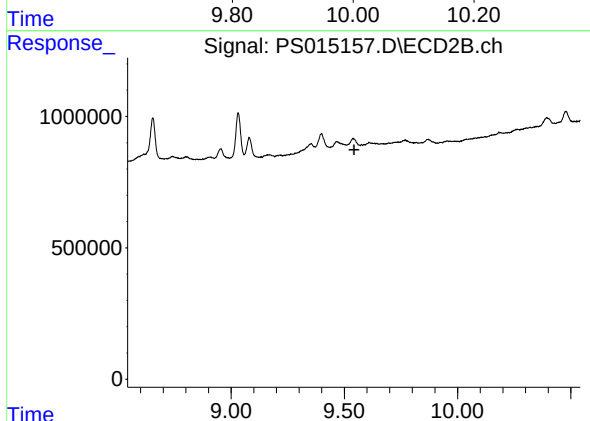


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.542 min
Response: 0
Conc: N.D.

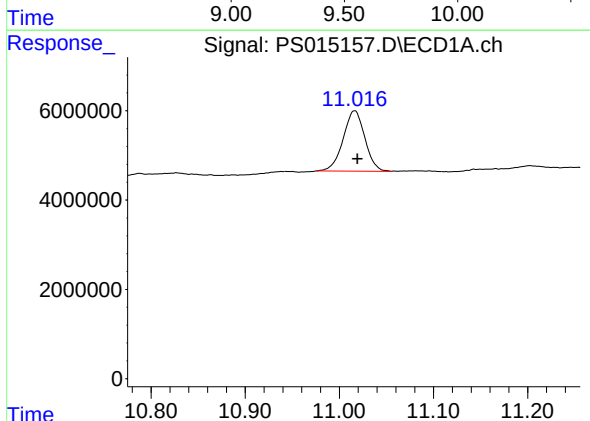


#15 Picloram

R.T.: 11.016 min
Delta R.T.: -0.003 min
Response: 21695760
Conc: 1.31 ng/ml

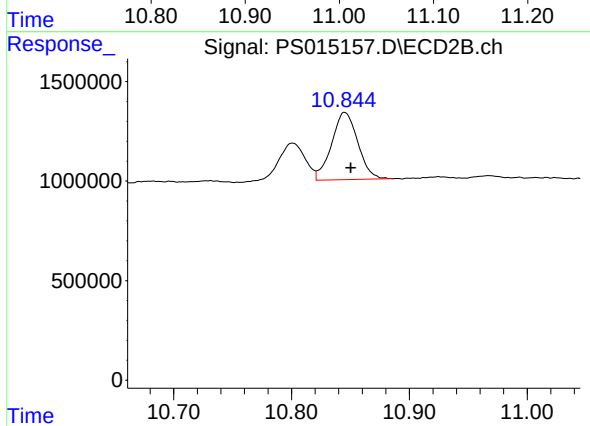

#15 Picloram


R.T.: 10.845 min
Delta R.T.: -0.005 min
Response: 5224429
Conc: 1.26 ng/ml

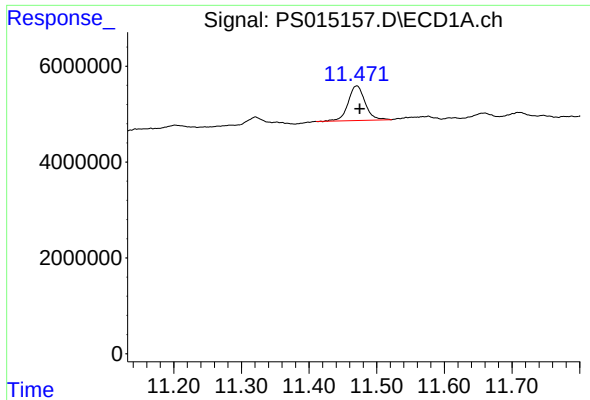

#16 DCPA

R.T.: 11.471 min
Delta R.T.: -0.004 min
Response: 12520563
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

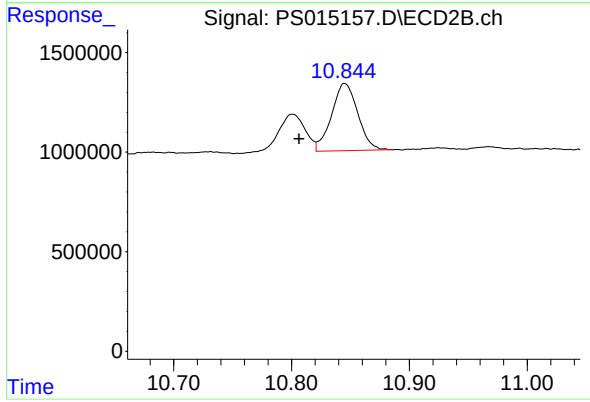

#16 DCPA

R.T.: 10.845 min
Delta R.T.: 0.038 min
Response: 5224429
Conc: 1.21 ng/ml