

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
 Data File : PS015151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2021 16:44
 Operator : DD\AJ
 Sample : M2547-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMPOSITE-SAMPLE-LOAMY-TOP

Manual Integrations
 APPROVED

Ankita
 6/2/2021 11:43:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:32:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.223	6.783	969.3E6	220.9E6	384.596m	412.381

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
Data File : PS015151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2021 16:44
Operator : DD\AJ
Sample : M2547-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
COMPOSITE-SAMPLE-LOAMY-TOP


Manual Integrations
APPROVED

Ankita
6/2/2021 11:43:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:32:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

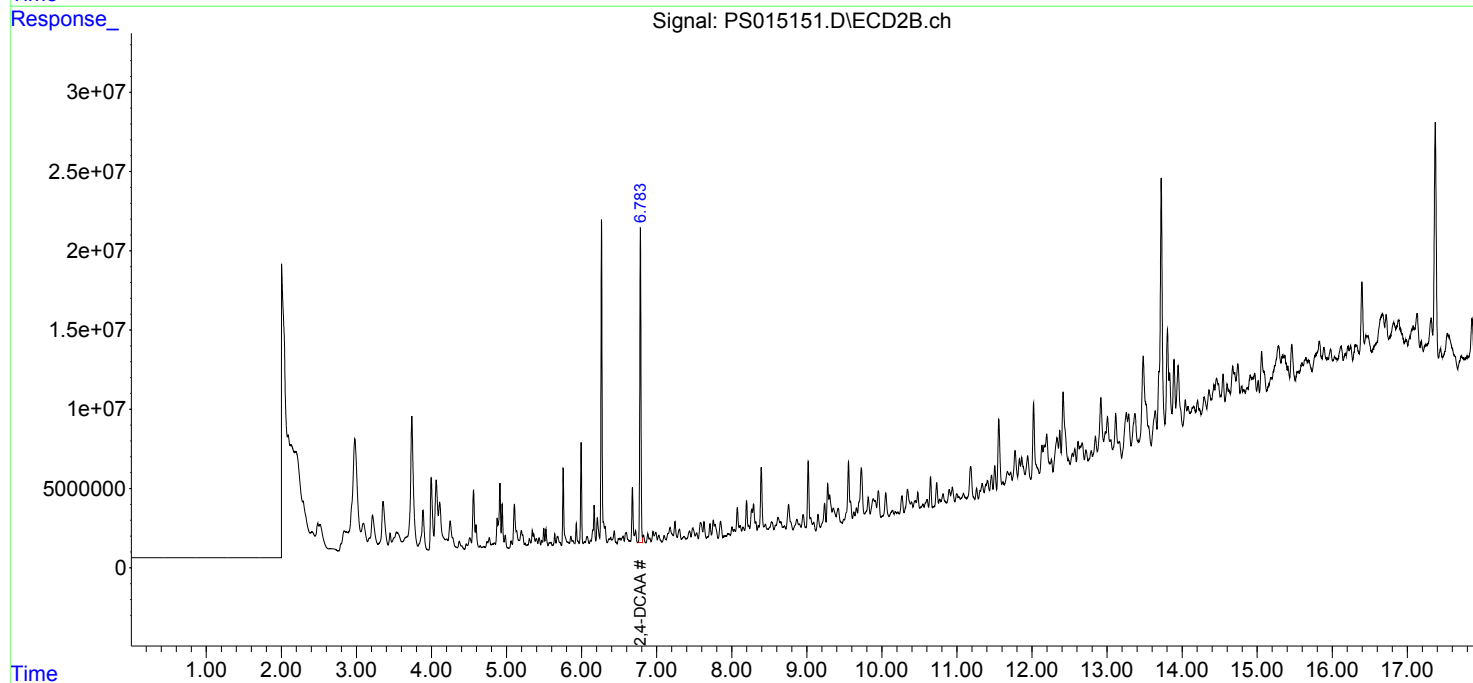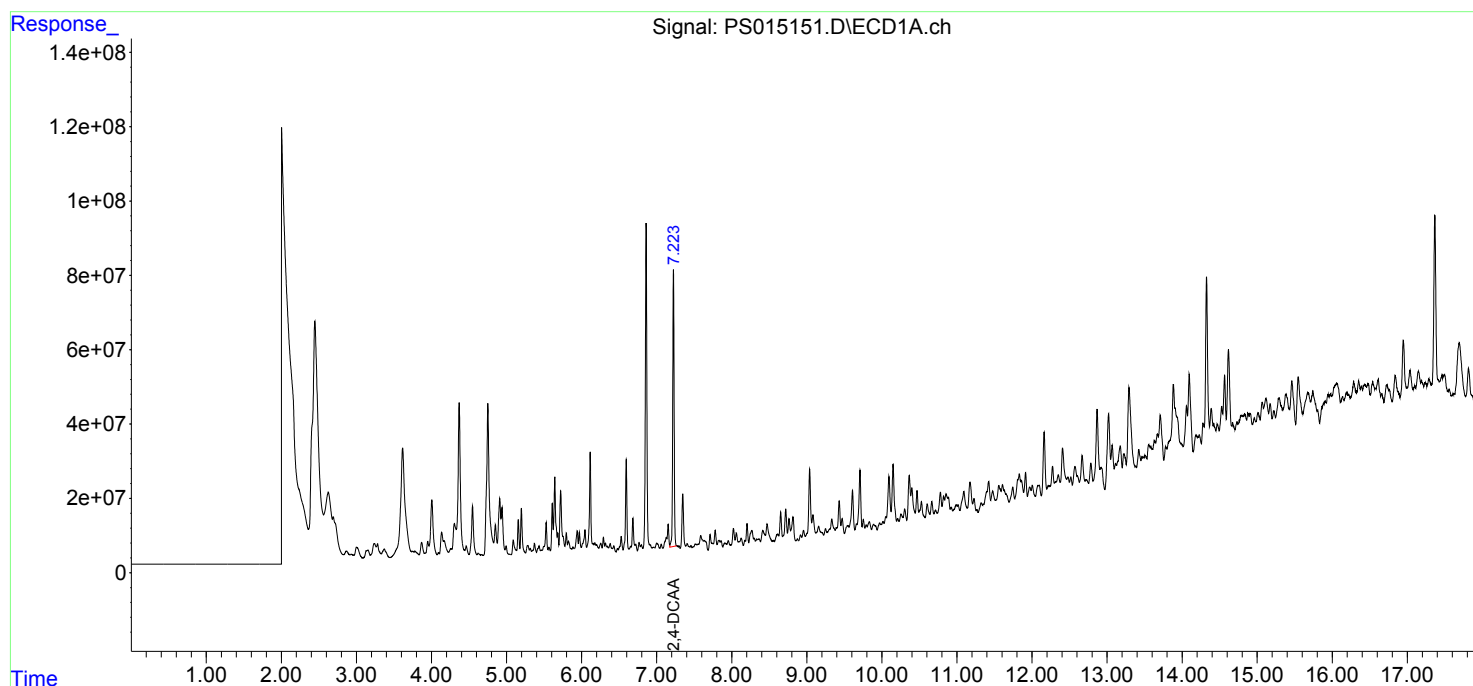

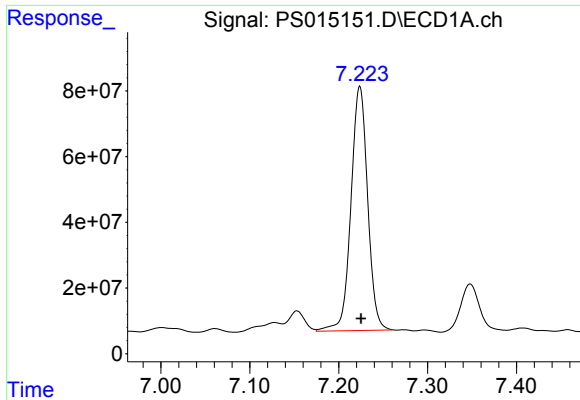


#4 2,4-DCAA

R.T.: 7.223 min
Delta R.T.: -0.002 min
Response: 969325357
Conc: 384.60 ng/ml m

Instrument :
ECD_S
ClientSampleId :
COMPOSITE-SAMPLE-LOAMY-TOP

Manual Integrations
APPROVED

Ankita
6/2/2021 11:43:34 AM

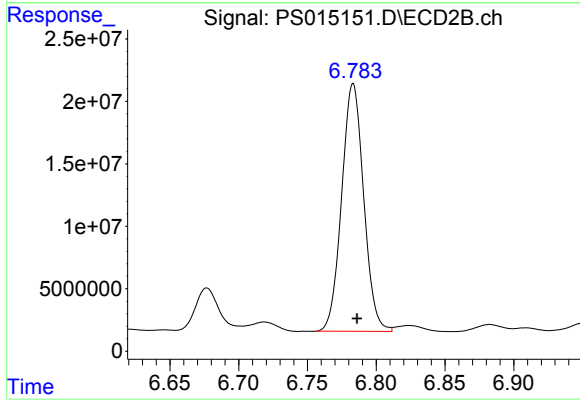

#4 2,4-DCAA

R.T.: 6.783 min
Delta R.T.: -0.003 min
Response: 220941994
Conc: 412.38 ng/ml