

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
 Data File : PS015158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2021 19:32
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:34:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.783	1827.4E6	398.7E6	725.064	744.151
Target Compounds							
1) T	Dalapon	3.037	2.520	1820.0E6	448.0E6	692.450	684.589
2) T	3,5-DICHL...	6.435	5.968	2310.0E6	560.5E6	669.871	693.881
3) T	4-Nitroph...	7.050	6.399	936.1E6	217.2E6	664.076	682.552
5) T	DICAMBA	7.418	6.948	6627.5E6	1581.0E6	695.308	714.417
6) T	MCPD	7.589	7.046	520.7E6	127.6E6	72.357	72.226
7) T	MCPA	7.737	7.259	713.7E6	184.0E6	71.108	70.814
8) T	DICHLORPROP	8.112	7.570	1584.8E6	382.6E6	688.136	704.199
9) T	2,4-D	8.340	7.861	1760.1E6	454.2E6	690.756	705.228
10) T	Pentachlo...	8.654	8.292	22443.3E6	5248.9E6	693.318	713.051
11) T	2,4,5-TP ...	9.204	8.655	8678.3E6	2097.1E6	699.240	722.643
12) T	2,4,5-T	9.487	9.031	8501.8E6	2113.5E6	707.842	730.063
13) T	2,4-DB	10.037	9.539	1844.0E6	276.6E6	724.109	717.012
14) T	DINOSEB	11.202	9.868	6058.1E6	1483.9E6	758.250	812.580
15) T	Picloram	11.016	10.846	11560.9E6	2979.4E6	697.836	717.435
16) T	DCPA	11.471	10.801	12231.6E6	3170.4E6	725.391	735.431



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060121\
Data File : PS015158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2021 19:32
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:34:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

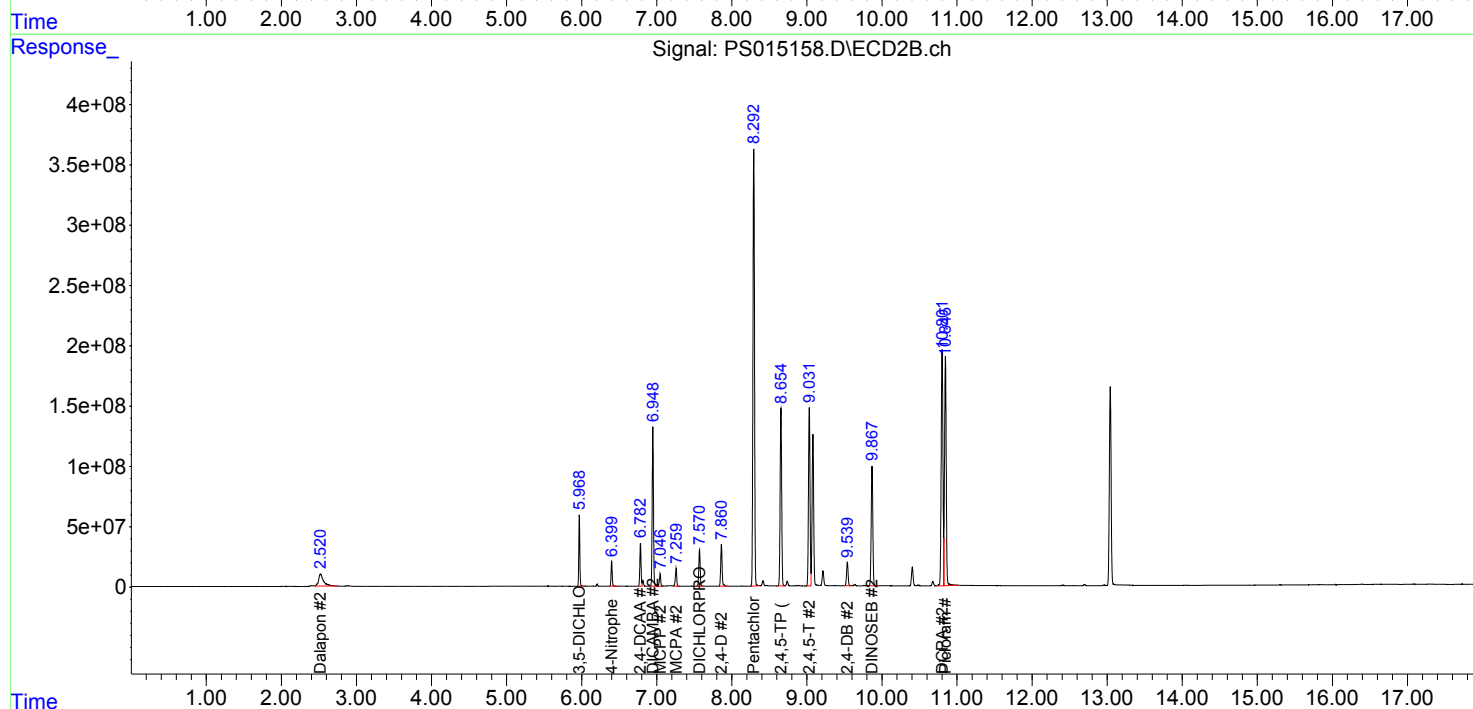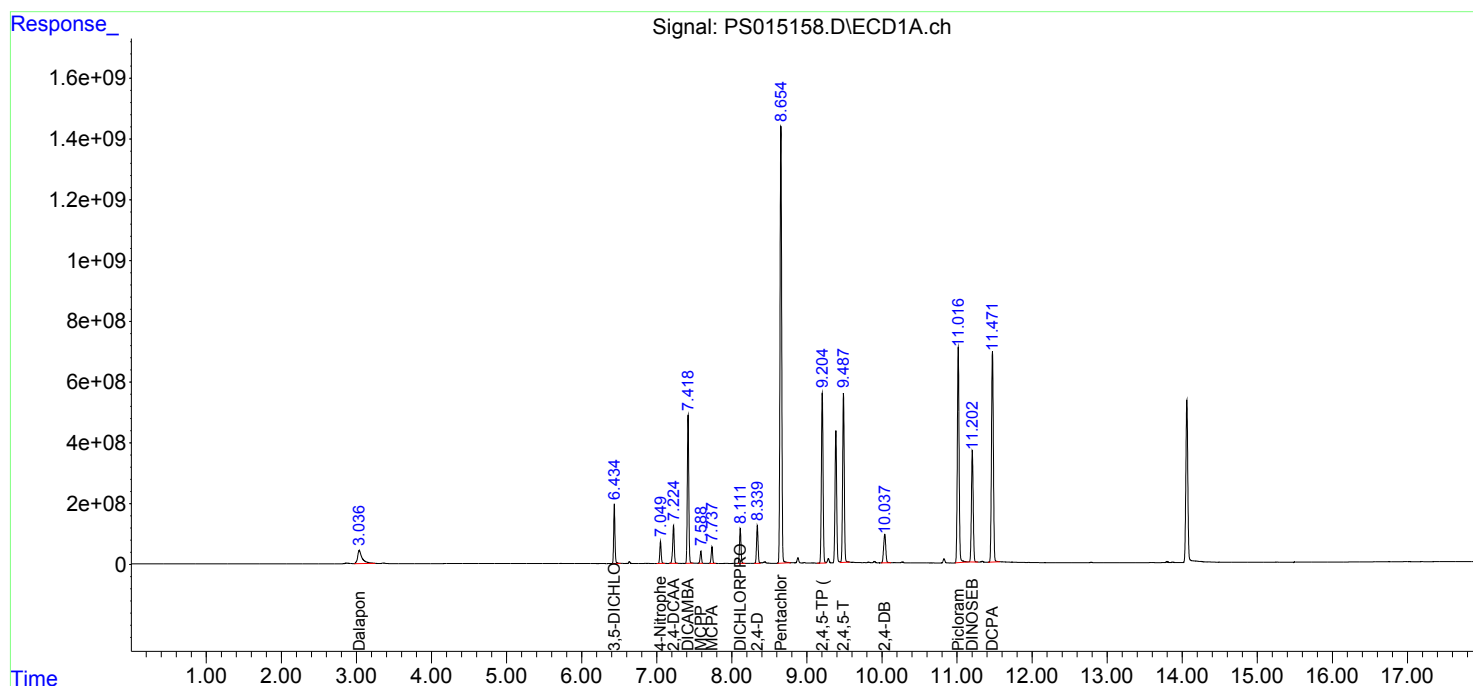


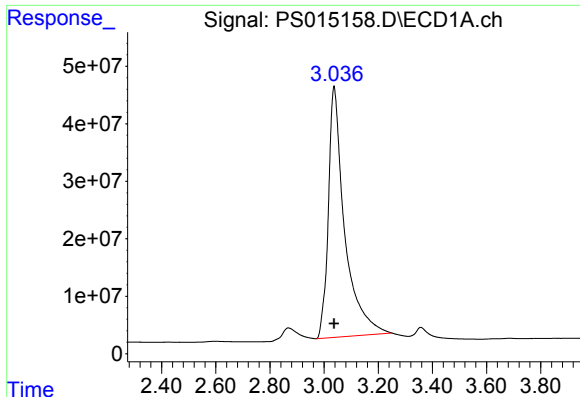

#1 Dalapon


R.T.: 3.037 min
Delta R.T.: 0.000 min
Response: 1820018969
Conc: 692.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

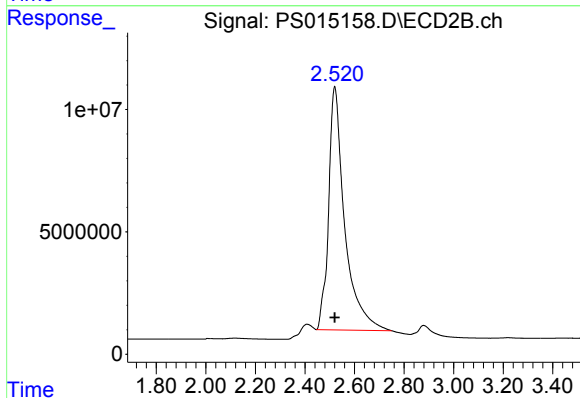


#1 Dalapon

R.T.: 2.520 min
Delta R.T.: 0.000 min
Response: 448031362
Conc: 684.59 ng/ml

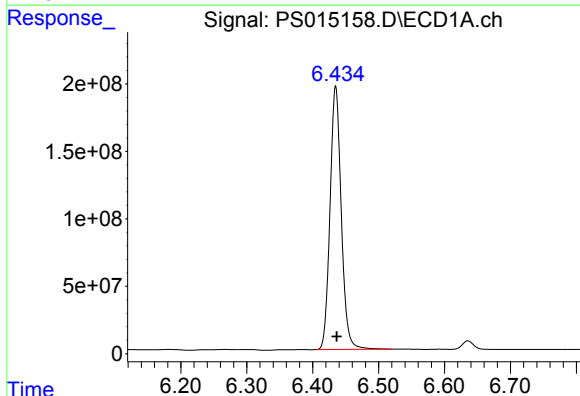


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.435 min
Delta R.T.: -0.002 min
Response: 2309992220
Conc: 669.87 ng/ml

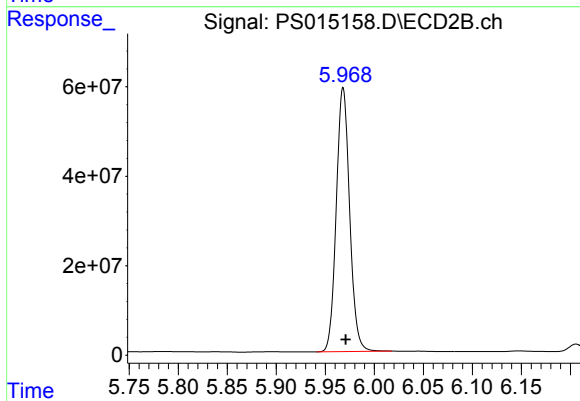

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.968 min
Delta R.T.: -0.003 min
Response: 560548253
Conc: 693.88 ng/ml

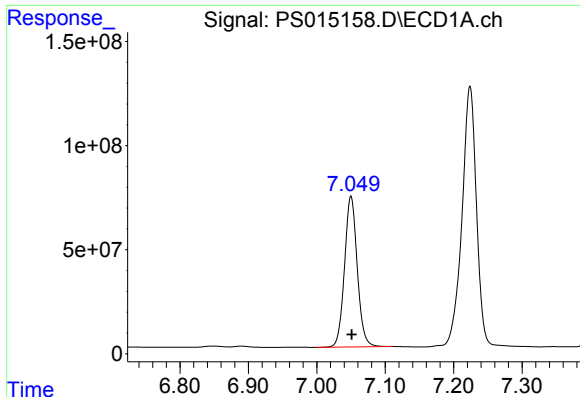

#3 4-Nitrophenol


R.T.: 7.050 min
Delta R.T.: -0.001 min
Response: 936145803
Conc: 664.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

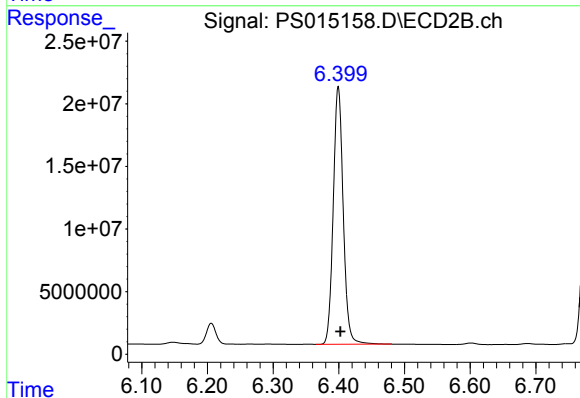


#3 4-Nitrophenol

R.T.: 6.399 min
Delta R.T.: -0.003 min
Response: 217170494
Conc: 682.55 ng/ml

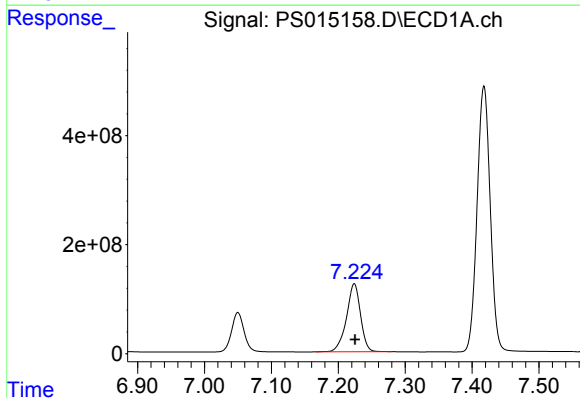


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: -0.001 min
Response: 1827433210
Conc: 725.06 ng/ml

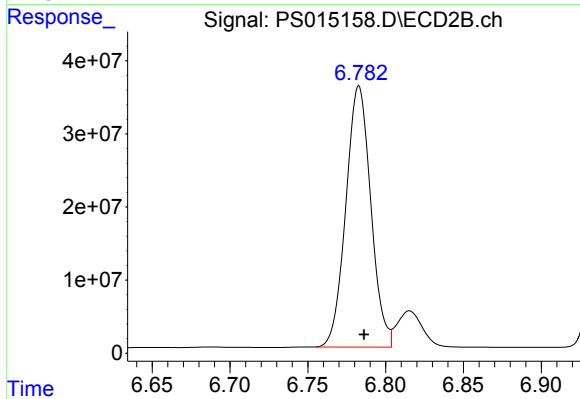

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: -0.003 min
Response: 398694403
Conc: 744.15 ng/ml

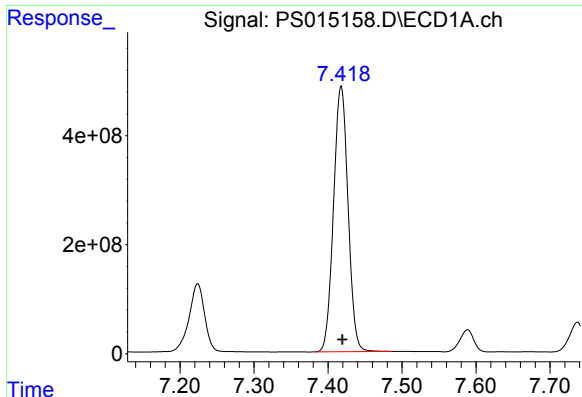

#5 DICAMBA


R.T.: 7.418 min
Delta R.T.: -0.002 min
Response: 6627499403
Conc: 695.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

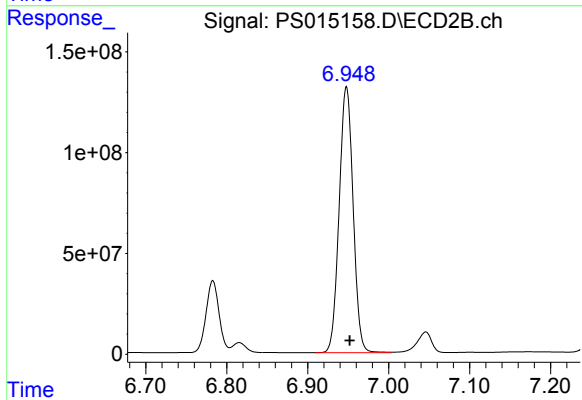


#5 DICAMBA

R.T.: 6.948 min
Delta R.T.: -0.004 min
Response: 1580958608
Conc: 714.42 ng/ml

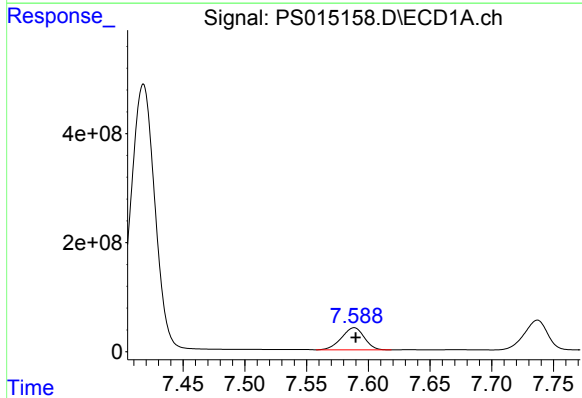


#6 MCP

R.T.: 7.589 min
Delta R.T.: -0.001 min
Response: 520706339
Conc: 72.36 ug/ml

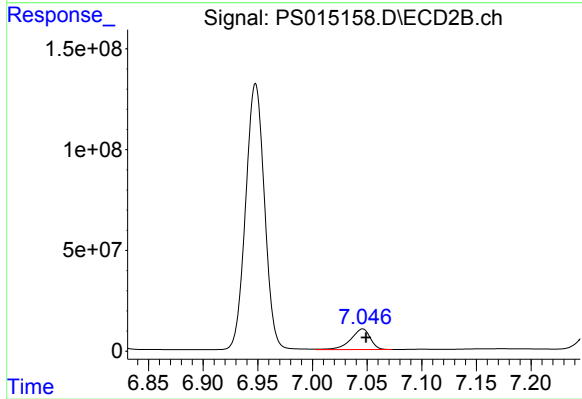

#6 MCP


R.T.: 7.046 min
Delta R.T.: -0.003 min
Response: 127630453
Conc: 72.23 ug/ml

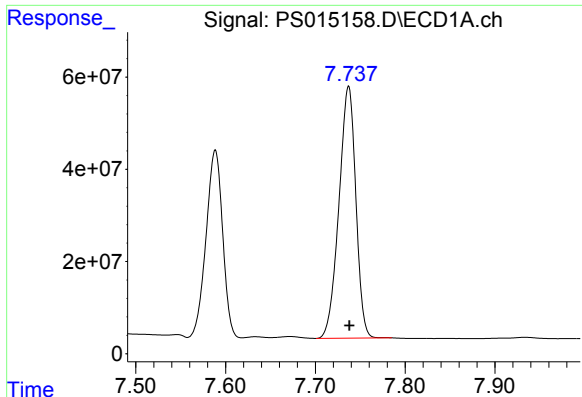

#7 MCPA


R.T.: 7.737 min
Delta R.T.: -0.001 min
Response: 713665562
Conc: 71.11 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

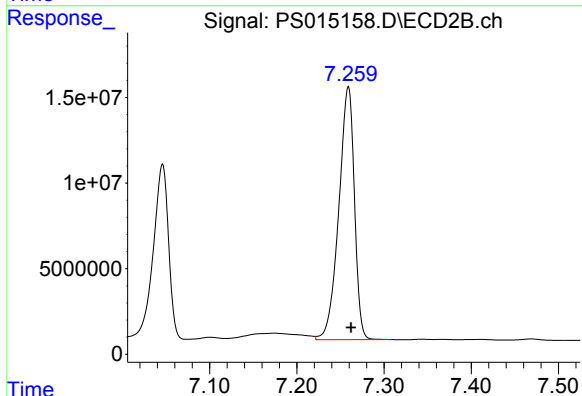


#7 MCPA

R.T.: 7.259 min
Delta R.T.: -0.003 min
Response: 184029248
Conc: 70.81 ug/ml

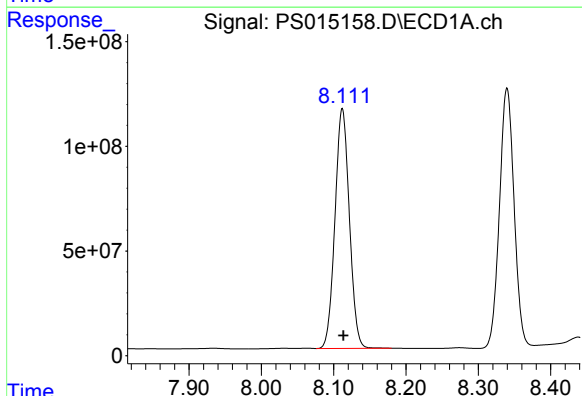


#8 DICHLORPROP

R.T.: 8.112 min
Delta R.T.: -0.001 min
Response: 1584847900
Conc: 688.14 ng/ml

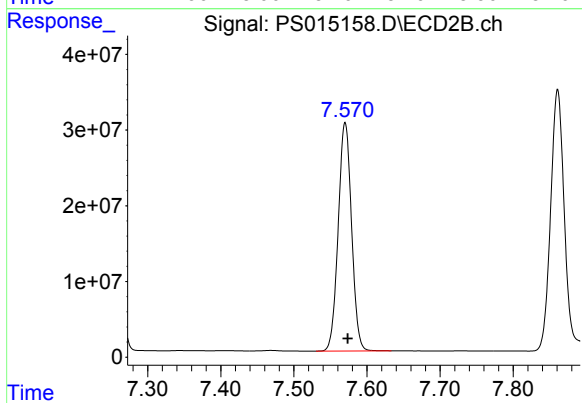

#8 DICHLORPROP


R.T.: 7.570 min
Delta R.T.: -0.004 min
Response: 382566073
Conc: 704.20 ng/ml

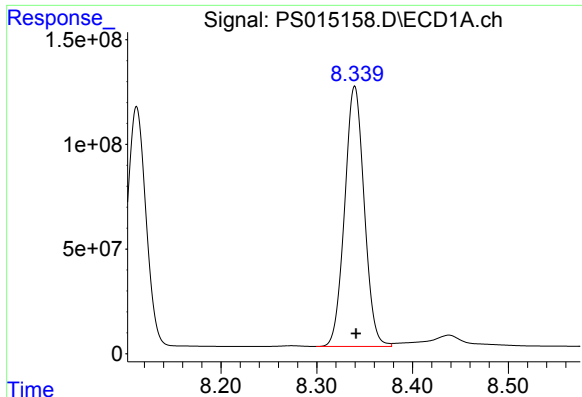

#9 2,4-D


R.T.: 8.340 min
Delta R.T.: -0.001 min
Response: 1760127067
Conc: 690.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

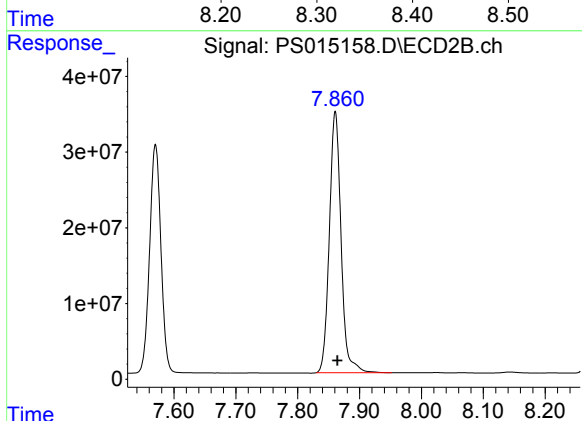


#9 2,4-D

R.T.: 7.861 min
Delta R.T.: -0.003 min
Response: 454184764
Conc: 705.23 ng/ml

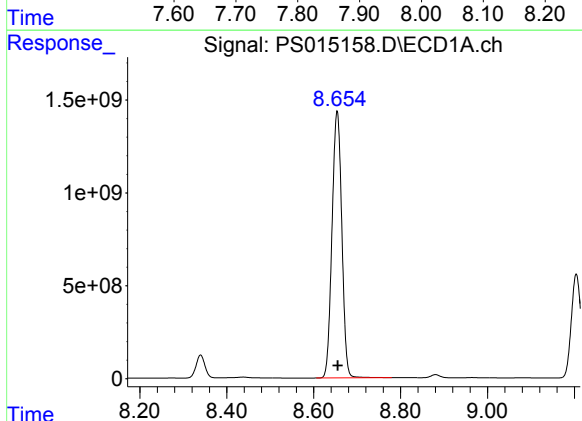


#10 Pentachlorophenol

R.T.: 8.654 min
Delta R.T.: -0.001 min
Response: 22443258535
Conc: 693.32 ng/ml

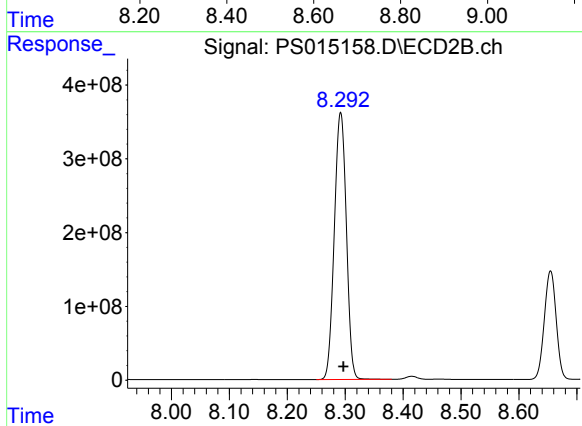

#10 Pentachlorophenol


R.T.: 8.292 min
Delta R.T.: -0.005 min
Response: 5248907057
Conc: 713.05 ng/ml

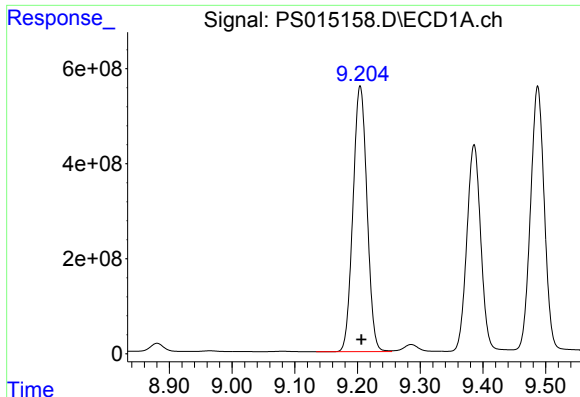

#11 2,4,5-TP (SILVEX)


R.T.: 9.204 min
Delta R.T.: -0.002 min
Response: 8678268561
Conc: 699.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

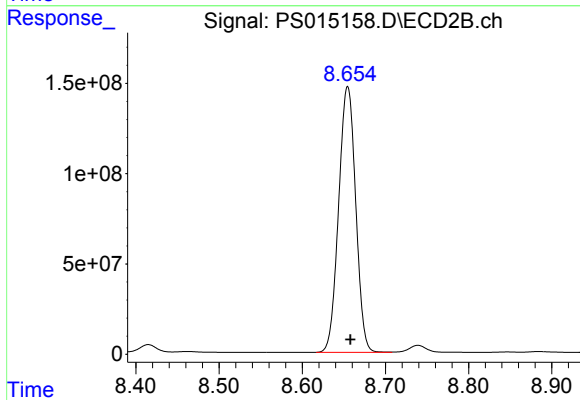


#11 2,4,5-TP (SILVEX)

R.T.: 8.655 min
Delta R.T.: -0.003 min
Response: 2097065324
Conc: 722.64 ng/ml

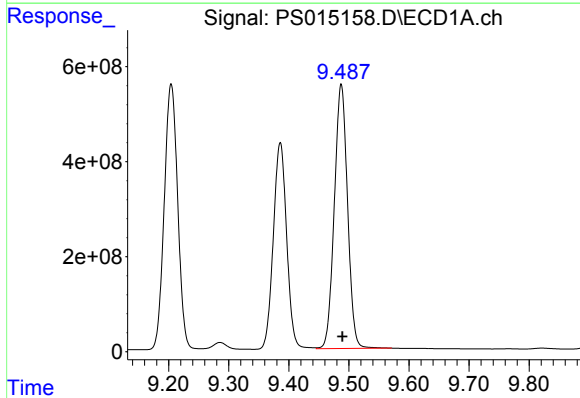


#12 2,4,5-T

R.T.: 9.487 min
Delta R.T.: -0.002 min
Response: 8501826755
Conc: 707.84 ng/ml

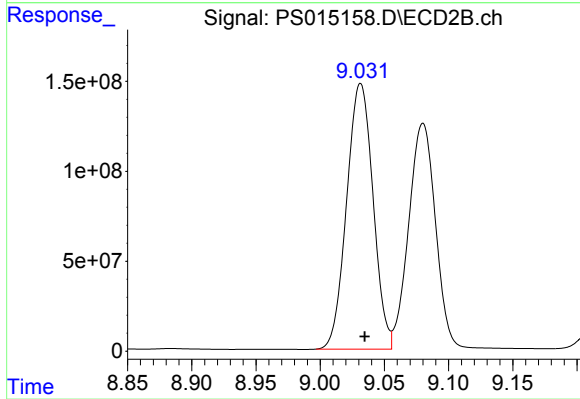

#12 2,4,5-T


R.T.: 9.031 min
Delta R.T.: -0.003 min
Response: 2113532505
Conc: 730.06 ng/ml

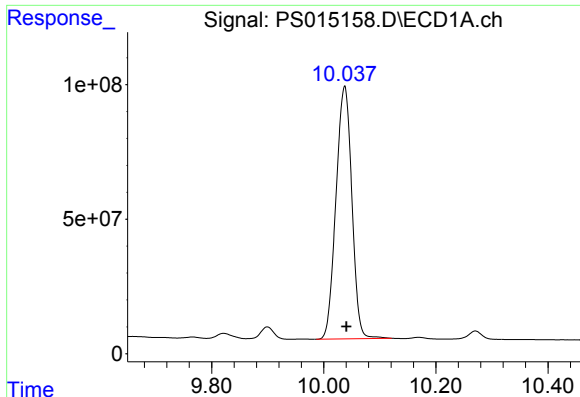

#13 2,4-DB


R.T.: 10.037 min
Delta R.T.: -0.003 min
Response: 1843963705
Conc: 724.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

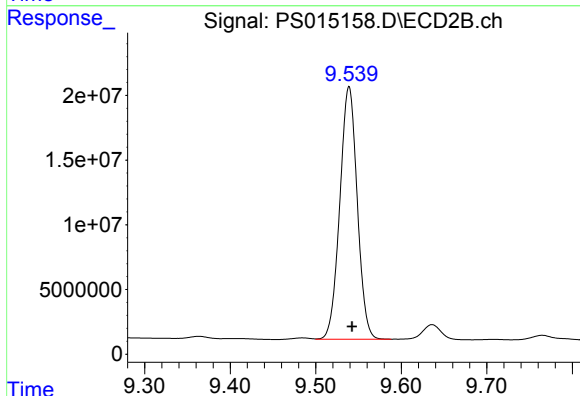


#13 2,4-DB

R.T.: 9.539 min
Delta R.T.: -0.003 min
Response: 276586871
Conc: 717.01 ng/ml

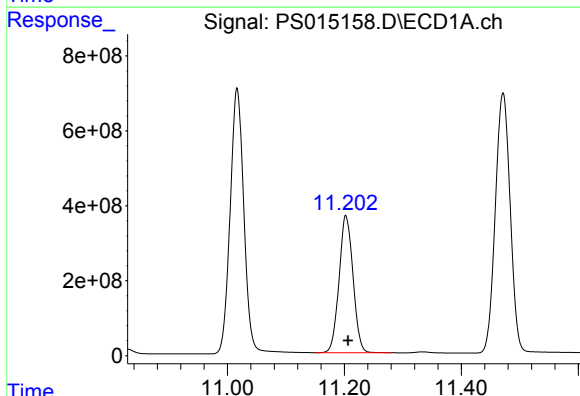


#14 DINOSEB

R.T.: 11.202 min
Delta R.T.: -0.004 min
Response: 6058090950
Conc: 758.25 ng/ml

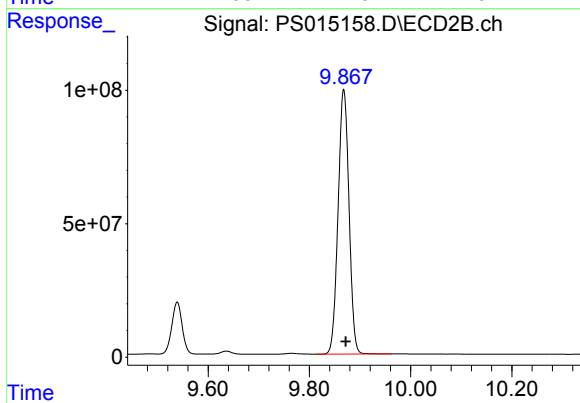

#14 DINOSEB


R.T.: 9.868 min
Delta R.T.: -0.004 min
Response: 1483886868
Conc: 812.58 ng/ml

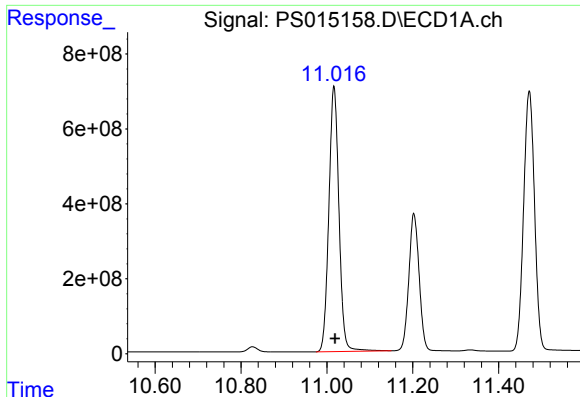

#15 Picloram


R.T.: 11.016 min
Delta R.T.: -0.003 min
Response: 11560891670
Conc: 697.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

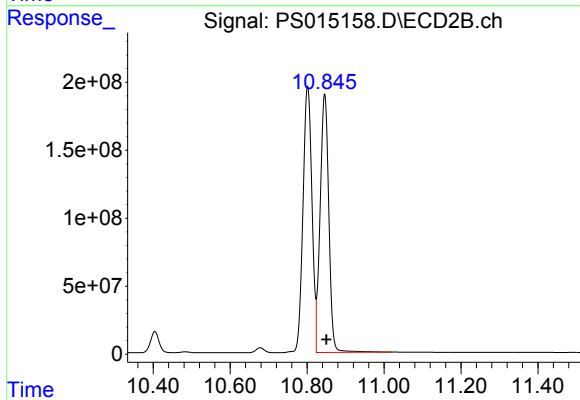


#15 Picloram

R.T.: 10.846 min
Delta R.T.: -0.004 min
Response: 2979431014
Conc: 717.44 ng/ml

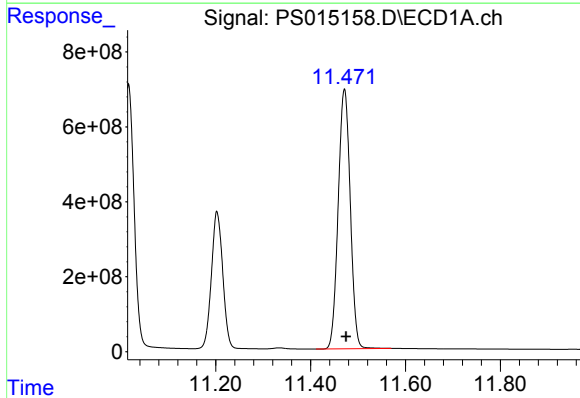

#16 DCPA

R.T.: 11.471 min
Delta R.T.: -0.003 min
Response: 12231601777
Conc: 725.39 ng/ml

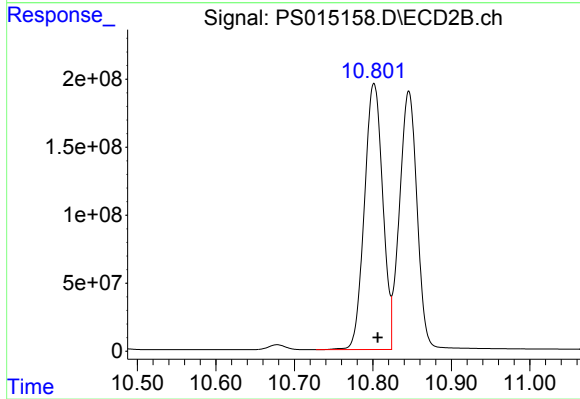

#16 DCPA

R.T.: 10.801 min
Delta R.T.: -0.005 min
Response: 3170439245
Conc: 735.43 ng/ml