

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060122\
 Data File : PS019581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 09:31
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 03:54:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1)	T	Dalapon	2.976	0.000	524560	0	<MDL N.D. #
2)	T	3,5-DICHL...	6.345f	0.000	456104	0	<MDL N.D. #
9)	T	2,4-D	0.000	7.850	0	369447	N.D. <MDL
10)	T	Pentachlo...	8.617	0.000	220377	0	<MDL N.D. #
11)	T	2,4,5-TP ...	0.000	8.654	0	394441	N.D. <MDL
13)	T	2,4-DB	9.979	9.471f	1040326	555585	<MDL <MDL #
15)	T	Picloram	10.982	10.887f	2638451	8174832	<MDL 1.271 #
16)	T	DCPA	11.426	10.783	1808859	644063	<MDL <MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060122\
Data File : PS019581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2022 09:31
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 03:54:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

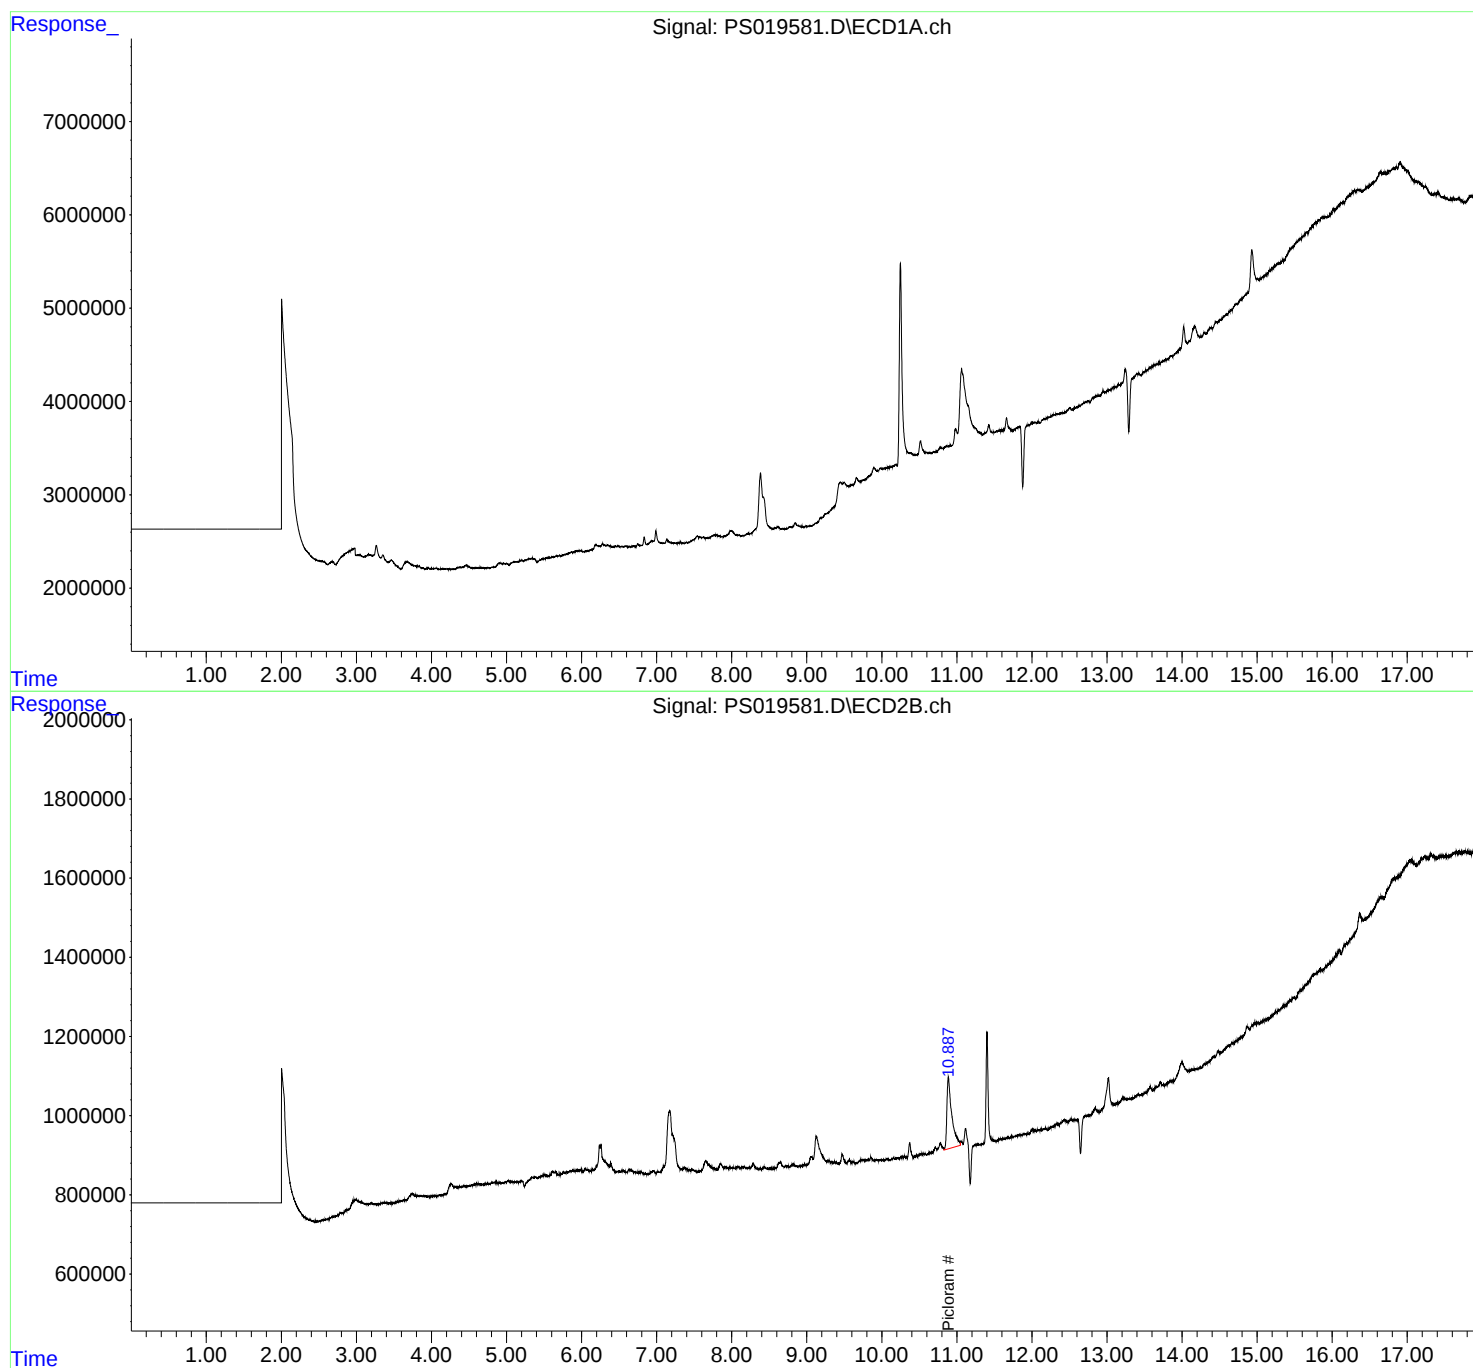


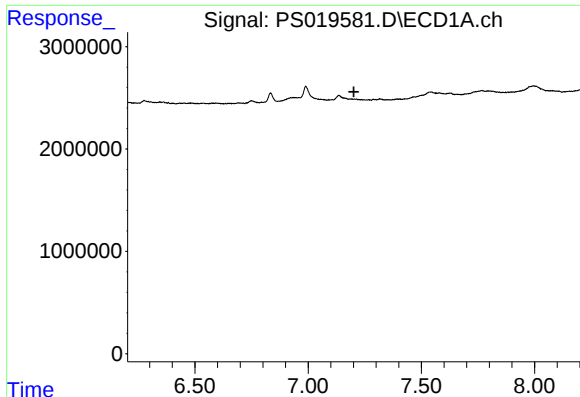

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.202 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

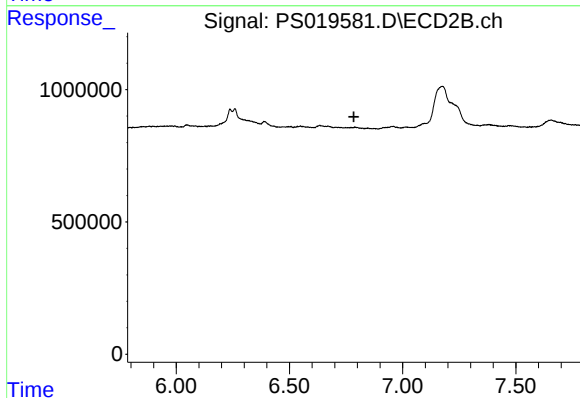


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

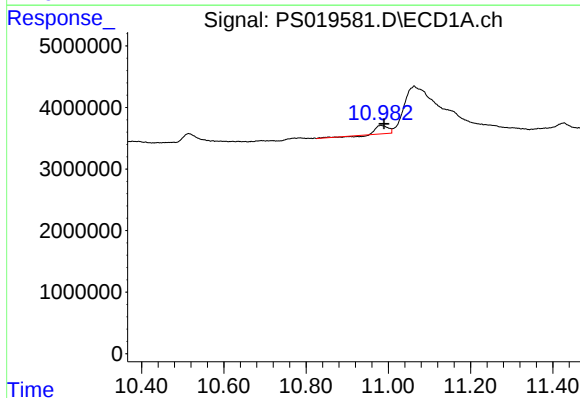

#15 Picloram

R.T.: 10.982 min
Delta R.T.: -0.007 min
Response: 2638451
Conc: N.D.

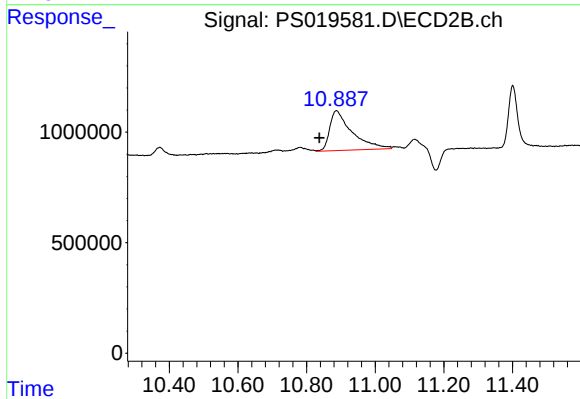

#15 Picloram

R.T.: 10.887 min
Delta R.T.: 0.050 min
Response: 8174832
Conc: 1.27 ng/ml