

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060122\
 Data File : PS019586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 12:54
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 03:55:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.783	1024.7E6	405.8E6	427.104	523.696
Target Compounds							
2) T	3,5-DICHL...	6.460f	0.000	407441	0	<MDL	N.D. #
5) T	DICAMBA	0.000	7.009f	0	1378391	N.D.	<MDL
6) T	MCP	0.000	7.009	0	1378391	N.D.	<MDL
7) T	MCPA	7.696	0.000	4036521	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.622f	0	1565159	N.D.	1.772
9) T	2,4-D	0.000	7.838	0	151247	N.D.	<MDL
10) T	Pentachlo...	8.619	8.287	948022	2466428	<MDL	<MDL #
11) T	2,4,5-TP ...	9.130	8.649	3146399	377549	<MDL	<MDL #
12) T	2,4,5-T	9.425	9.049	10409727	1168420	<MDL	<MDL #
13) T	2,4-DB	10.050	9.553	10265619	552256	2.537	<MDL #
14) T	DINOSEB	0.000	9.858	0	240597	N.D.	<MDL
15) T	Picloram	10.961	10.874	213.1E6	7347868	7.181	1.142 #
16) T	DCPA	11.426	10.782	4035654	2139310	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060122\
Data File : PS019586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2022 12:54
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 03:55:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

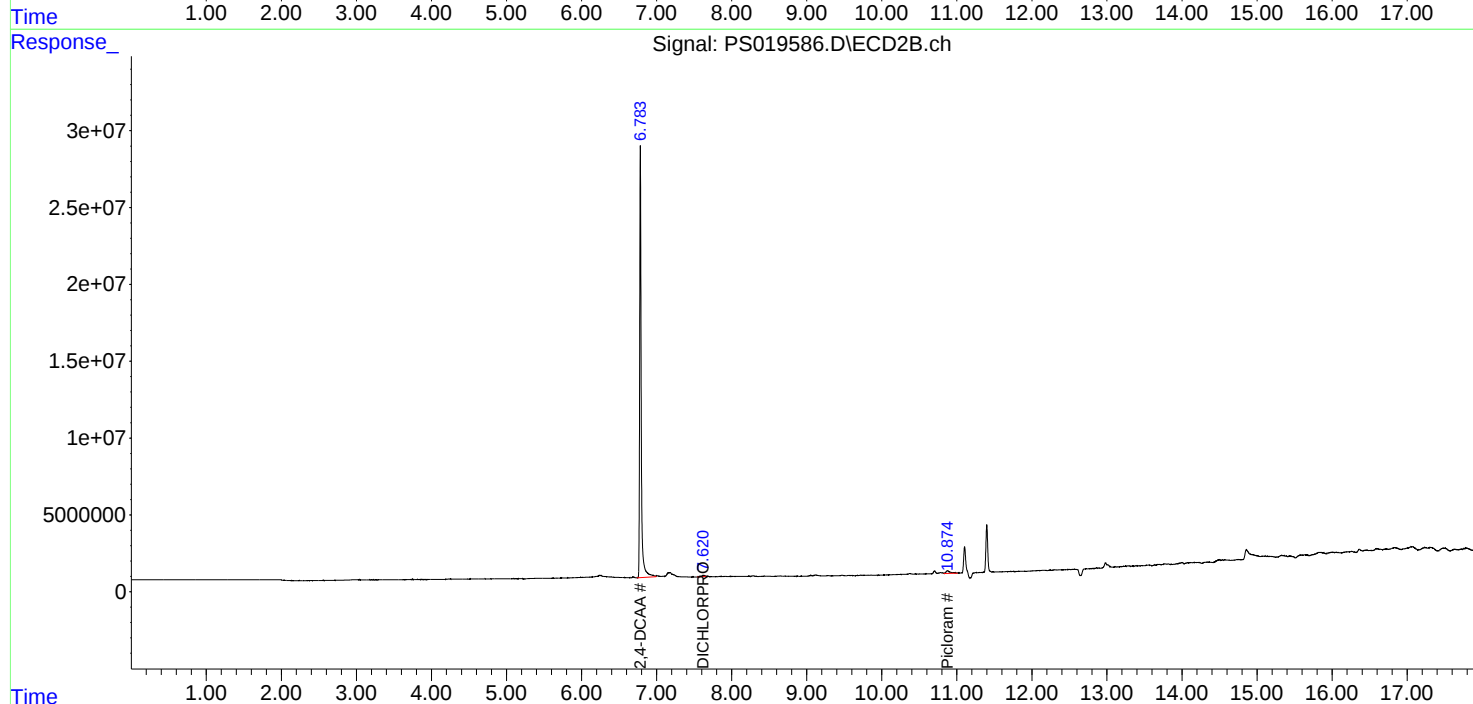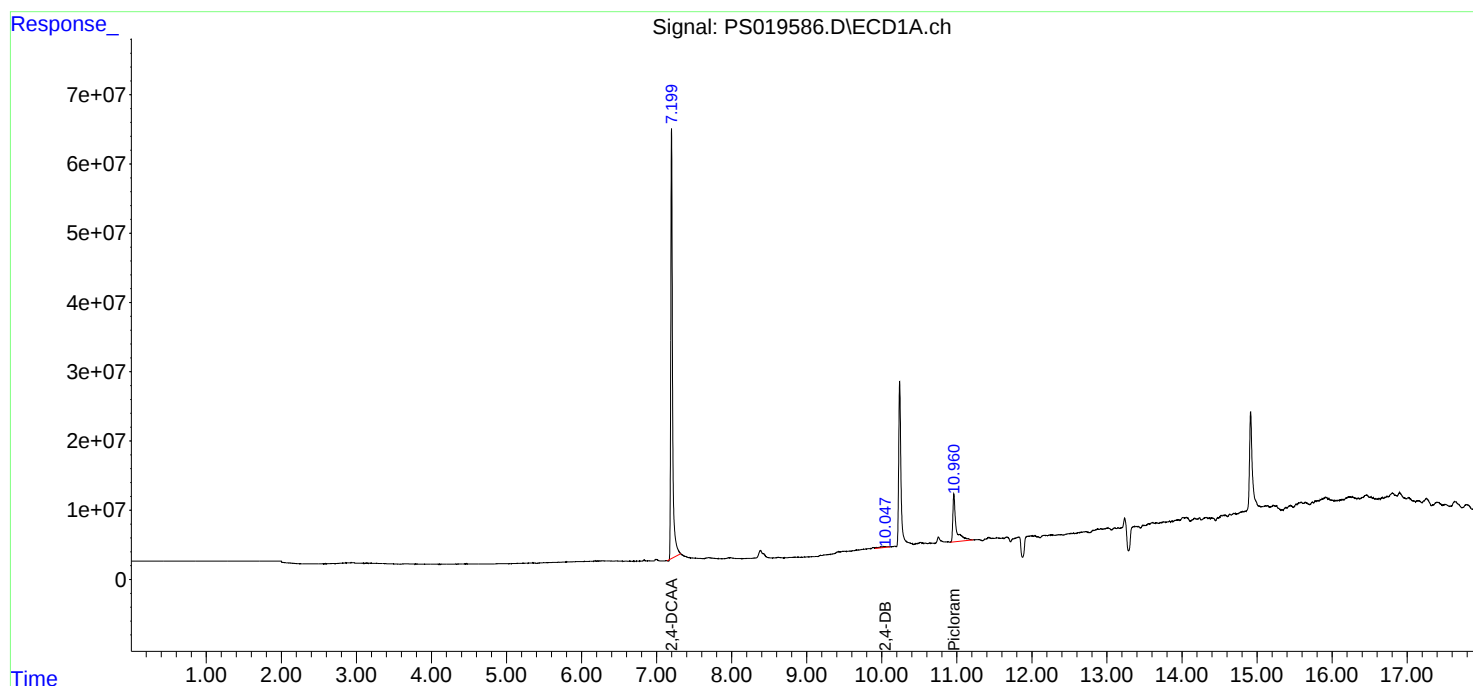


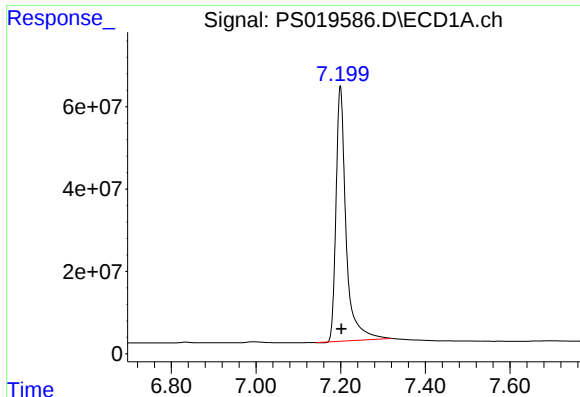

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1024694941
Conc: 427.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

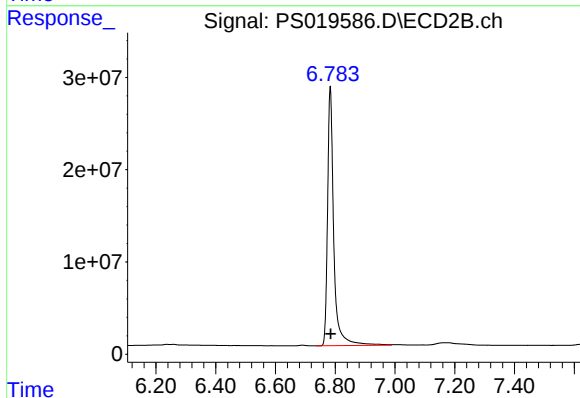


#4 2,4-DCAA

R.T.: 6.783 min
Delta R.T.: -0.001 min
Response: 405796832
Conc: 523.70 ng/ml

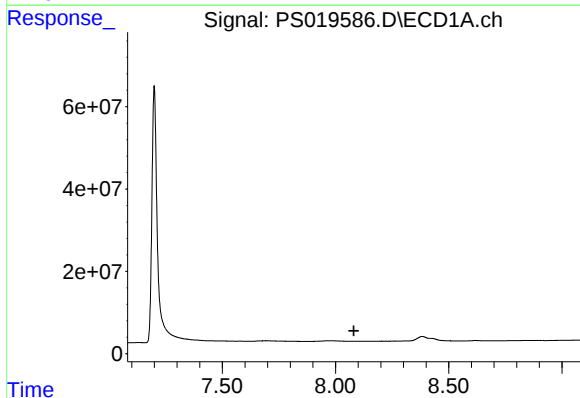


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.081 min
Response: 0
Conc: N.D.

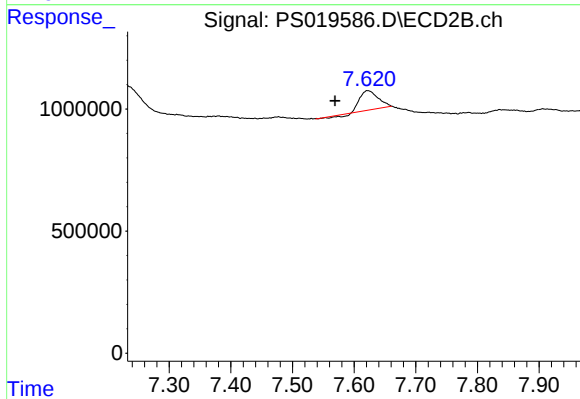

#8 DICHLORPROP


R.T.: 7.622 min
Delta R.T.: 0.053 min
Response: 1565159
Conc: 1.77 ng/ml

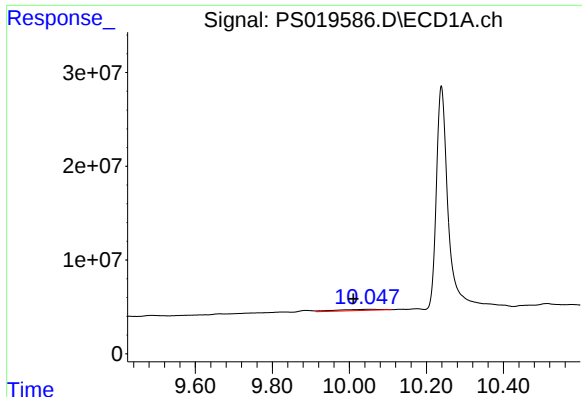

#13 2,4-DB


R.T.: 10.050 min
Delta R.T.: 0.039 min
Response: 10265619
Conc: 2.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

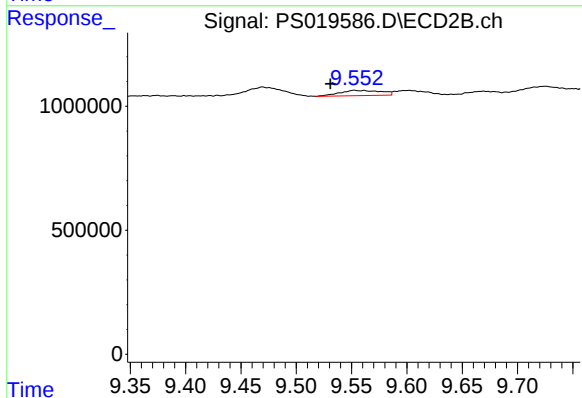


#13 2,4-DB

R.T.: 9.553 min
Delta R.T.: 0.022 min
Response: 552256
Conc: N.D.

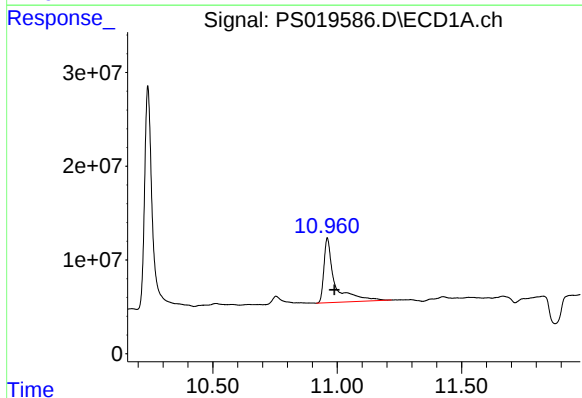

#15 Picloram

R.T.: 10.961 min
Delta R.T.: -0.029 min
Response: 213112263
Conc: 7.18 ng/ml

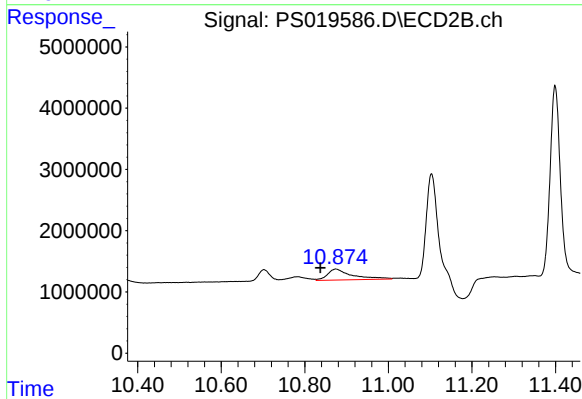

#15 Picloram

R.T.: 10.874 min
Delta R.T.: 0.037 min
Response: 7347868
Conc: 1.14 ng/ml