

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060123\
 Data File : PS023177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2023 12:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 03:49:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.486	6.857	779.3E6	292.8E6	512.385	521.748
Target Compounds							
3) T	4-Nitroph...	6.322	0.000	4299559	0	4.084	N.D. #
5) T	DICAMBA	6.633	7.077f	313274	1089441	<MDL	<MDL #
6) T	MCP	6.823	7.077f	-1373380	1089441	N.D.	<MDL
7) T	MCPA	6.861f	7.310	-5180840	7608672	N.D.	2.874
8) T	DICHLORPROP	7.242	7.664	1091176	1866185	<MDL	3.016 #
9) T	2,4-D	7.409	0.000	12085162	0	5.222	N.D. #
10) T	Pentachlo...	7.681	8.366	1175225	1018088	<MDL	<MDL #
11) T	2,4,5-TP ...	8.222	0.000	3310168	0	<MDL	N.D. #
12) T	2,4,5-T	8.491	9.099	4069983	989356	<MDL	<MDL #
13) T	2,4-DB	9.015	0.000	1192542	0	<MDL	N.D. #
14) T	DINOSEB	10.072	0.000	898463	0	<MDL	N.D. #
15) T	Picloram	9.910	10.904	21229941	3978313	1.238	<MDL #
16) T	DCPA	10.344	10.864	2916254	849405	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060123\
Data File : PS023177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2023 12:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 03:49:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

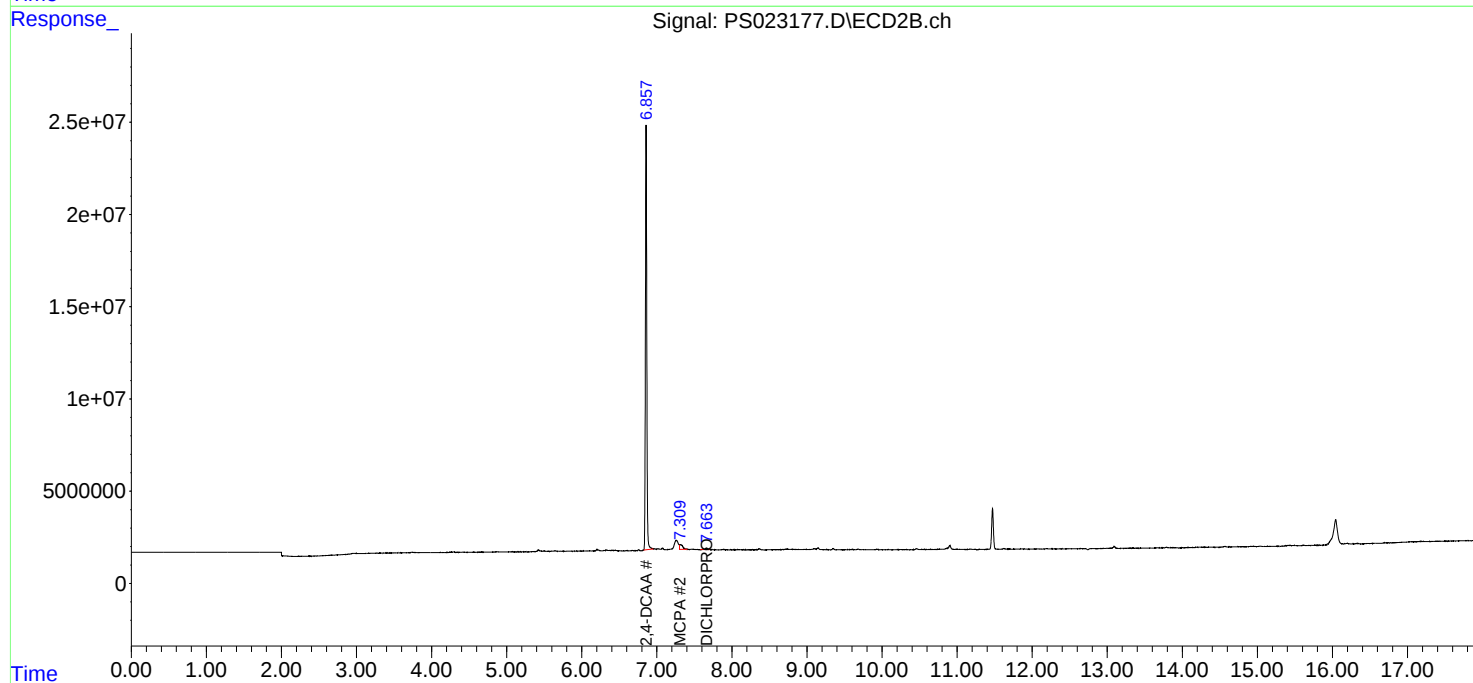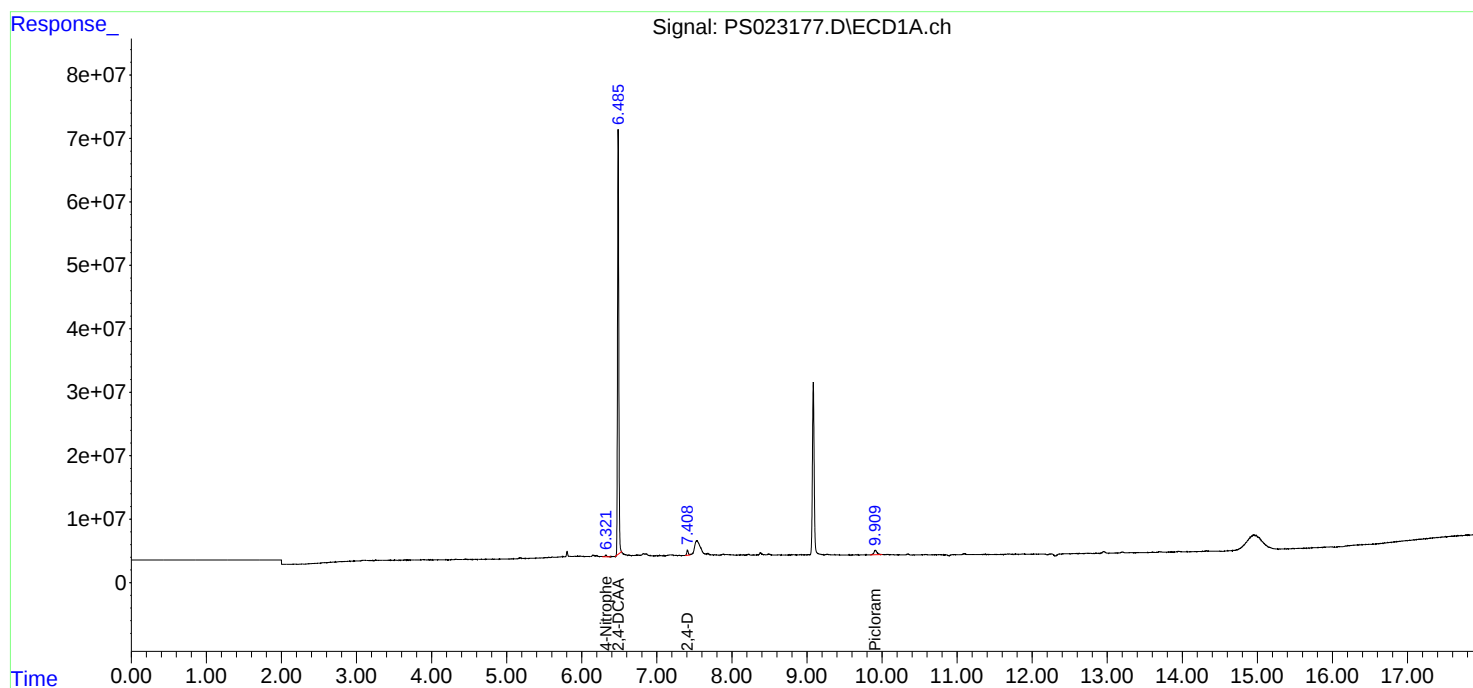


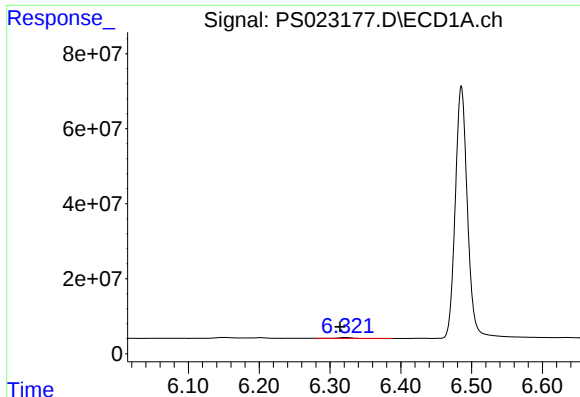

#3 4-Nitrophenol


R.T.: 6.322 min
Delta R.T.: 0.007 min
Response: 4299559
Conc: 4.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

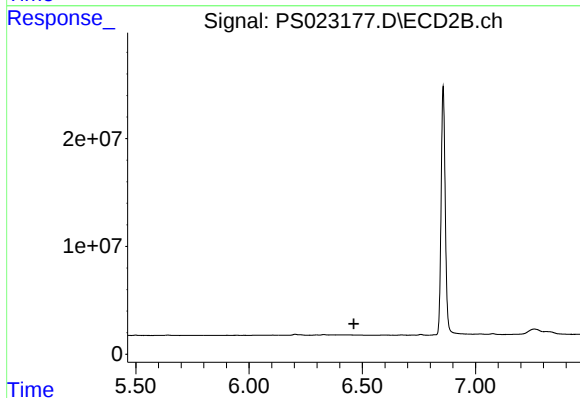


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

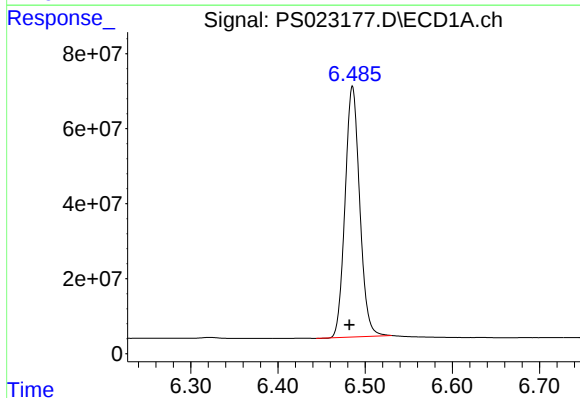


#4 2,4-DCAA

R.T.: 6.486 min
Delta R.T.: 0.003 min
Response: 779335497
Conc: 512.39 ng/ml

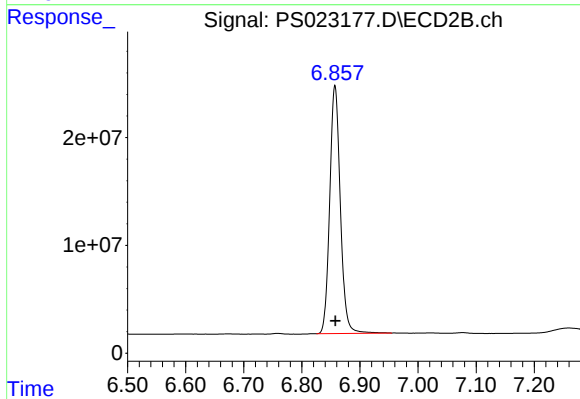

#4 2,4-DCAA


R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 292760937
Conc: 521.75 ng/ml

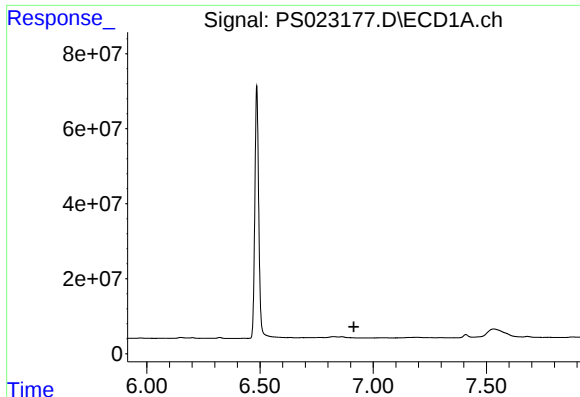

#7 MCPA


R.T.: 6.861 min
Delta R.T.: -0.054 min
Response: -5180840
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

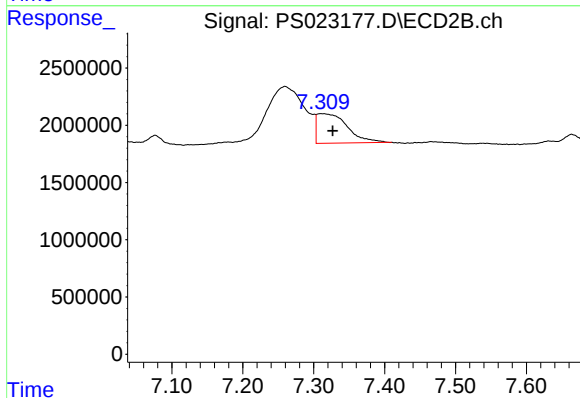


#7 MCPA

R.T.: 7.310 min
Delta R.T.: -0.017 min
Response: 7608672
Conc: 2.87 ug/ml

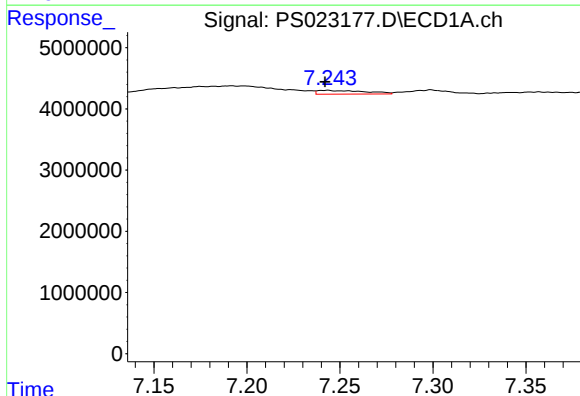


#8 DICHLORPROP

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 1091176
Conc: N.D.

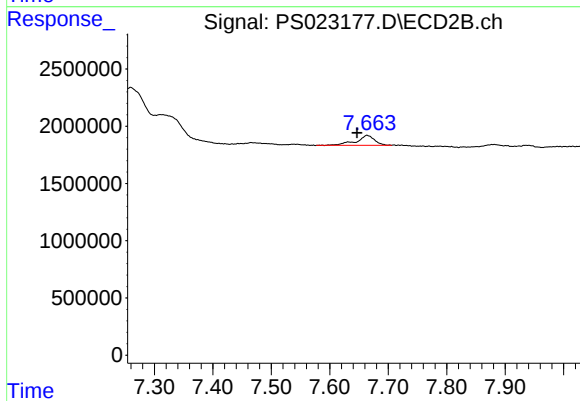

#8 DICHLORPROP


R.T.: 7.664 min
Delta R.T.: 0.017 min
Response: 1866185
Conc: 3.02 ng/ml

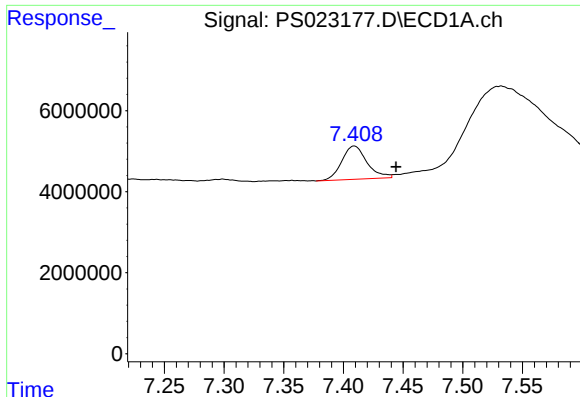

#9 2,4-D


R.T.: 7.409 min
Delta R.T.: -0.035 min
Response: 12085162
Conc: 5.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

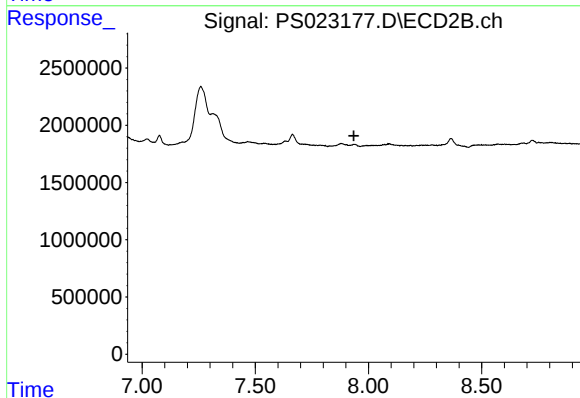


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.935 min
Response: 0
Conc: N.D.

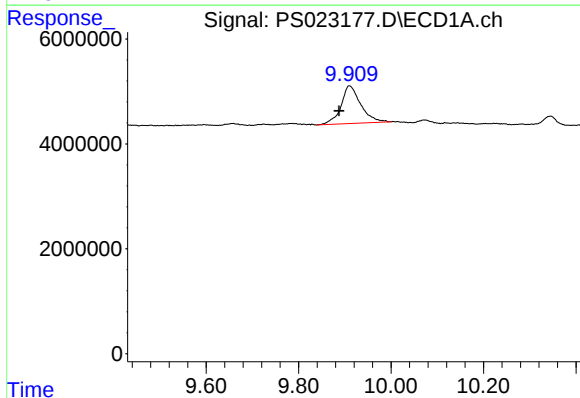

#15 Picloram

R.T.: 9.910 min
Delta R.T.: 0.022 min
Response: 21229941
Conc: 1.24 ng/ml

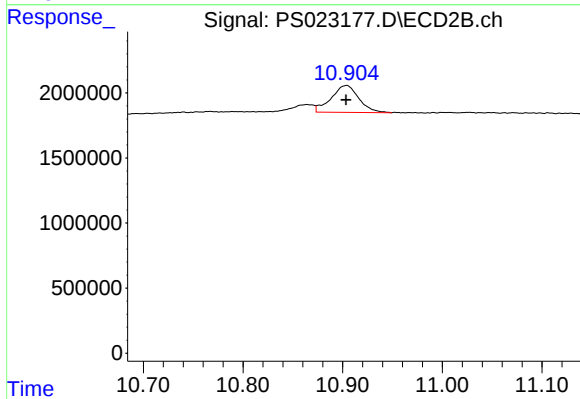

#15 Picloram

R.T.: 10.904 min
Delta R.T.: 0.000 min
Response: 3978313
Conc: N.D.