

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060220\
 Data File : PS010620.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 15:08
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 18:54:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.292	0.000	2508359	0	3.172	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.485	0.000	35551594	0	32.520	N.D. #
5) T	DICAMBA	7.423	7.090	8559740	7118686	2.722	3.163
6) T	MCP	0.000	7.154	0	23867456	N.D.	12.808
9) T	2,4-D	8.347	8.010	5003429	15916872	6.347	20.991 #
10) T	Pentachlo...	8.657	8.441	13389591	10828203	1.255	1.524
11) T	2,4,5-TP ...	9.208	8.802	15767844	11843844	3.687	3.944
12) T	2,4,5-T	9.493	9.182	27334039	20228002	6.721	6.741
14) T	DINOSEB	11.208	10.022	14961203	11005875	4.630	5.116
15) T	Picloram	11.026	11.004	176.4E6	143.3E6	34.552	34.739
16) T	DCPA	11.473	10.951	28591192	21828314	5.336	5.887



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060220\
Data File : PS010620.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 15:08
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 18:54:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

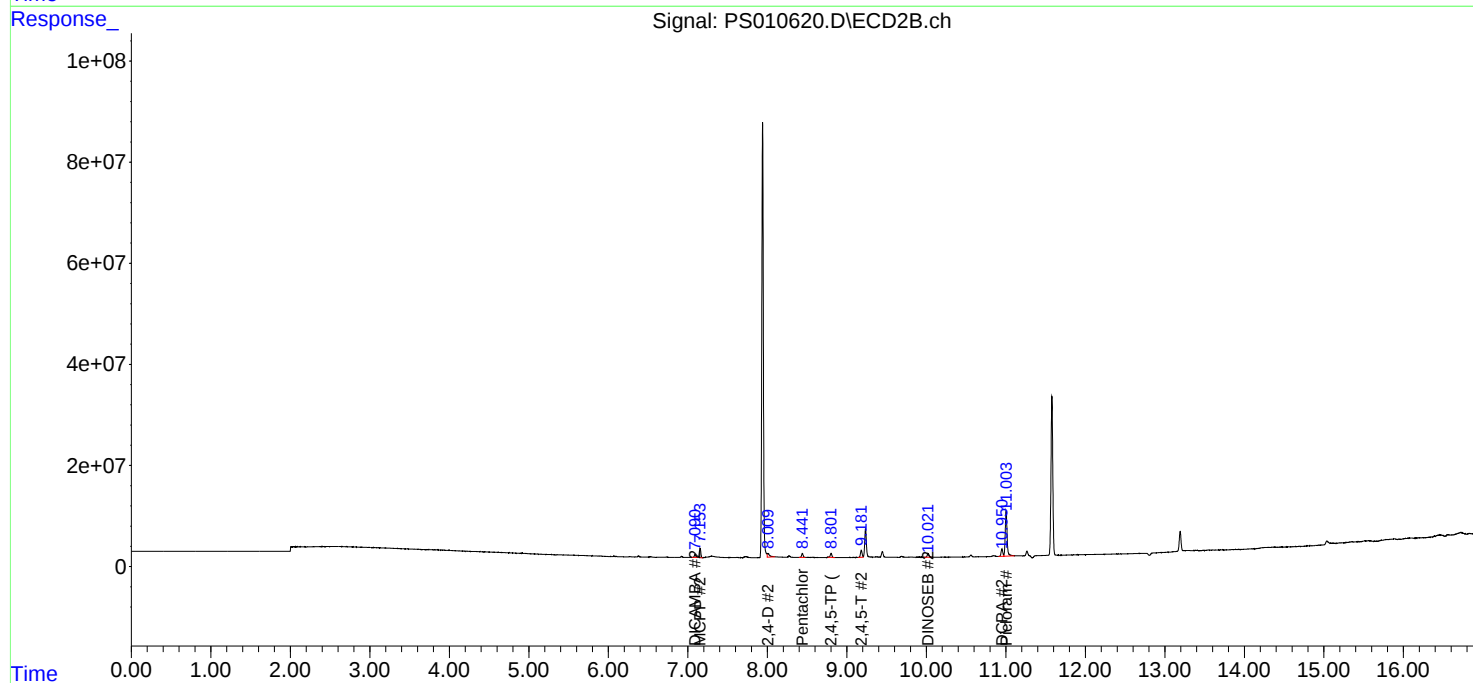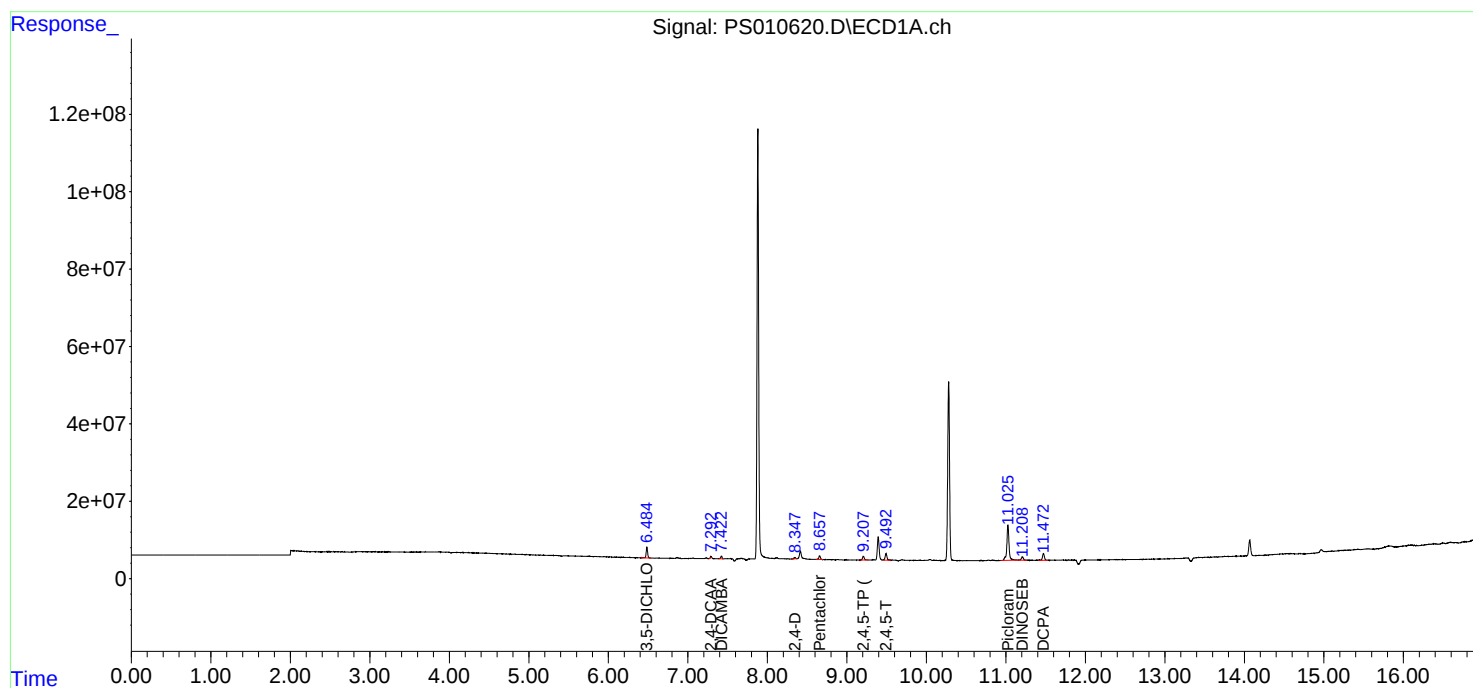


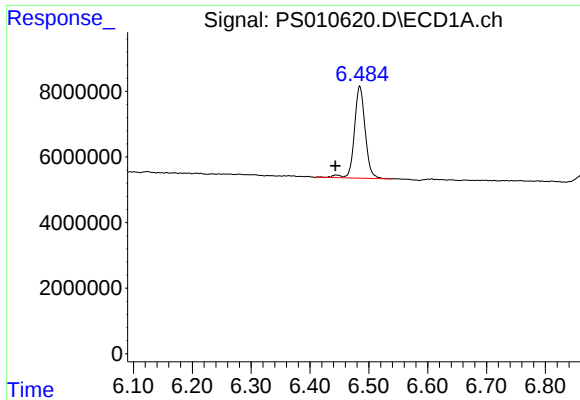

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.485 min
Delta R.T.: 0.042 min
Response: 35551594
Conc: 32.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

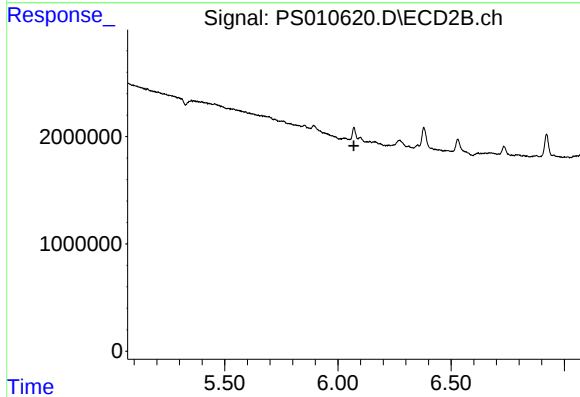


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.070 min
Response: 0
Conc: N.D.

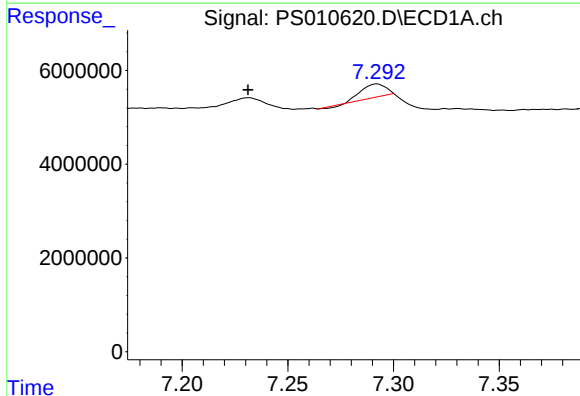


#4 2,4-DCAA

R.T.: 7.292 min
Delta R.T.: 0.061 min
Response: 2508359
Conc: 3.17 ng/ml

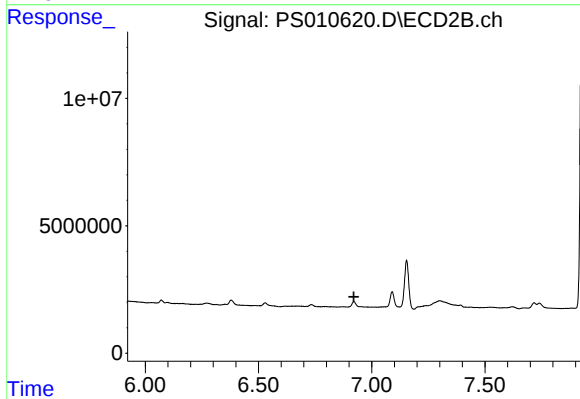

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

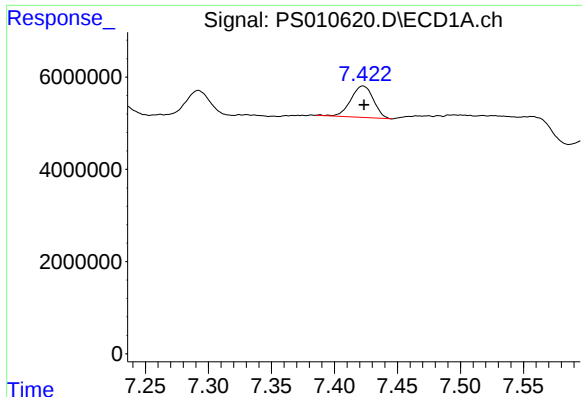

#5 DICAMBA


R.T.: 7.423 min
Delta R.T.: 0.000 min
Response: 8559740
Conc: 2.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

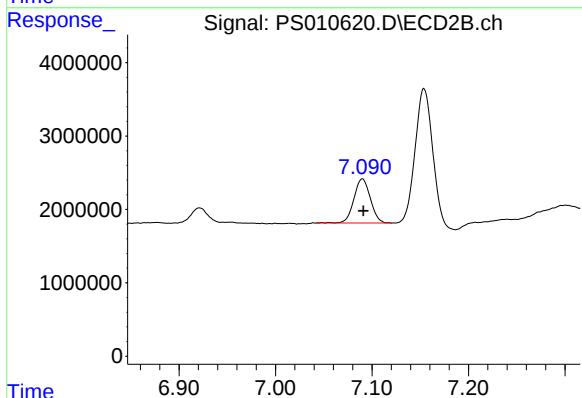


#5 DICAMBA

R.T.: 7.090 min
Delta R.T.: 0.000 min
Response: 7118686
Conc: 3.16 ng/ml

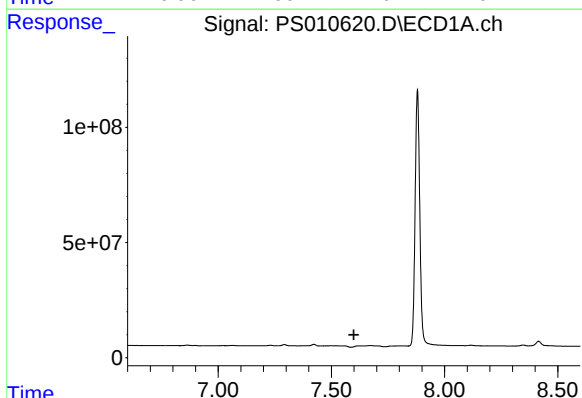


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.600 min
Response: 0
Conc: N.D.

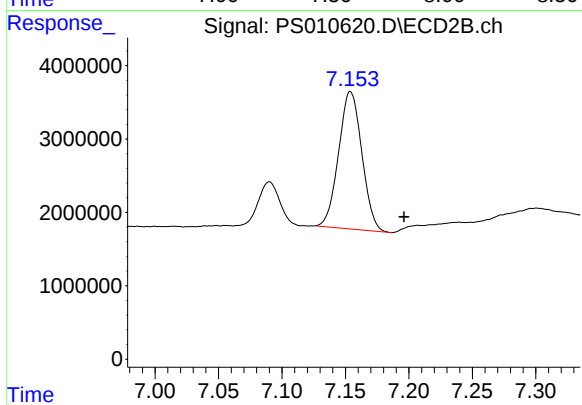

#6 MCP


R.T.: 7.154 min
Delta R.T.: -0.042 min
Response: 23867456
Conc: 12.81 ug/ml

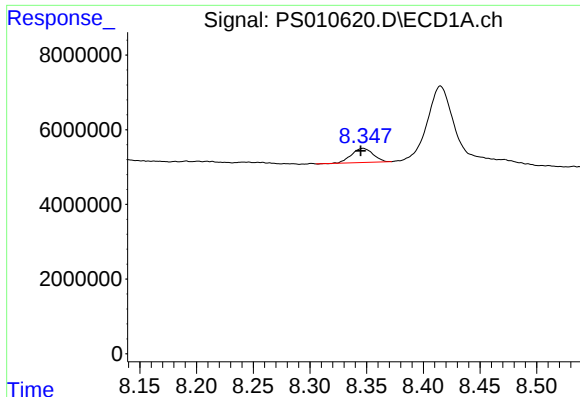

#9 2,4-D


R.T.: 8.347 min
Delta R.T.: 0.002 min
Response: 5003429
Conc: 6.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

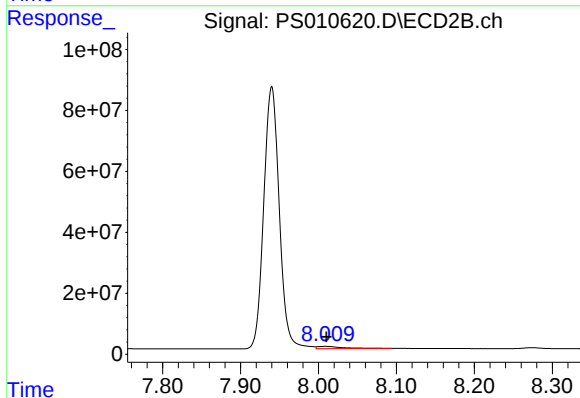


#9 2,4-D

R.T.: 8.010 min
Delta R.T.: 0.000 min
Response: 15916872
Conc: 20.99 ng/ml

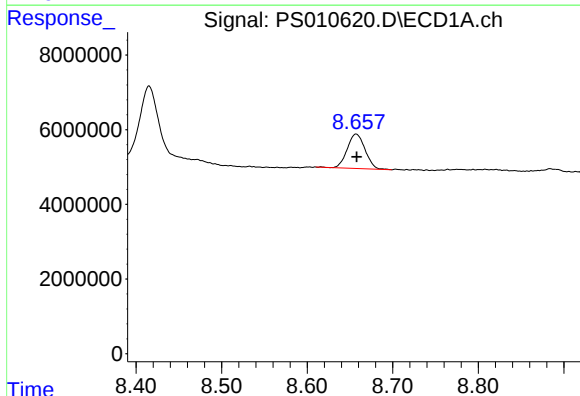


#10 Pentachlorophenol

R.T.: 8.657 min
Delta R.T.: 0.000 min
Response: 13389591
Conc: 1.26 ng/ml

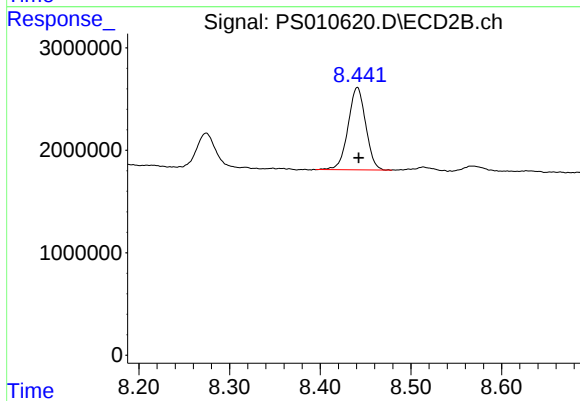

#10 Pentachlorophenol


R.T.: 8.441 min
Delta R.T.: -0.002 min
Response: 10828203
Conc: 1.52 ng/ml

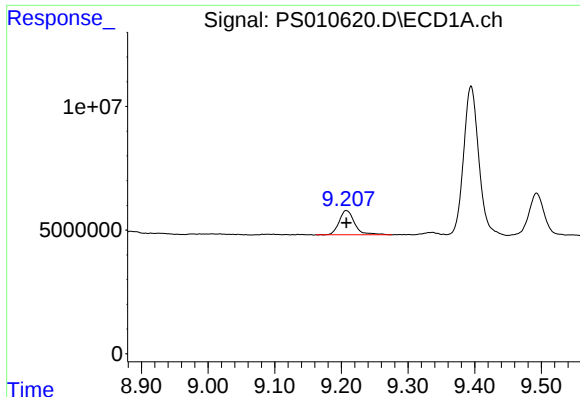

#11 2,4,5-TP (SILVEX)


R.T.: 9.208 min
Delta R.T.: 0.000 min
Response: 15767844
Conc: 3.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

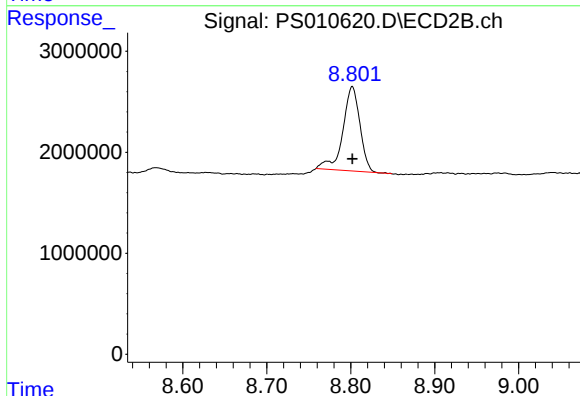


#11 2,4,5-TP (SILVEX)

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 11843844
Conc: 3.94 ng/ml

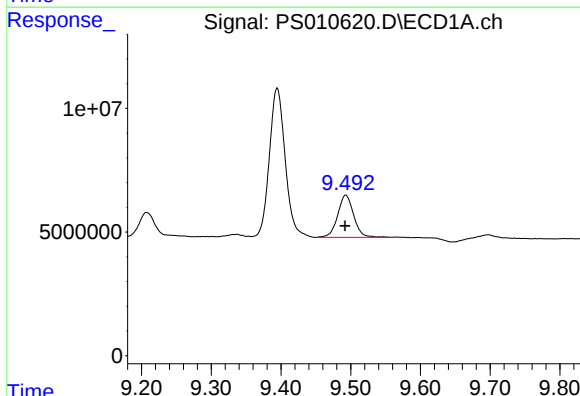


#12 2,4,5-T

R.T.: 9.493 min
Delta R.T.: 0.000 min
Response: 27334039
Conc: 6.72 ng/ml

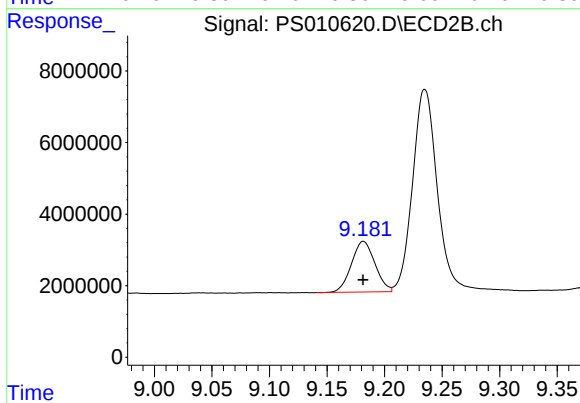

#12 2,4,5-T


R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 20228002
Conc: 6.74 ng/ml

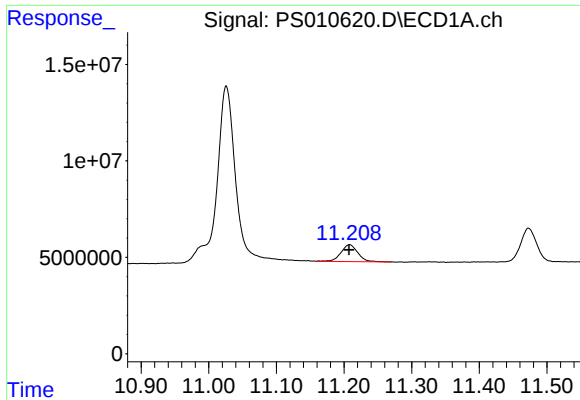

#14 DINOSEB


R.T.: 11.208 min
Delta R.T.: 0.000 min
Response: 14961203
Conc: 4.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

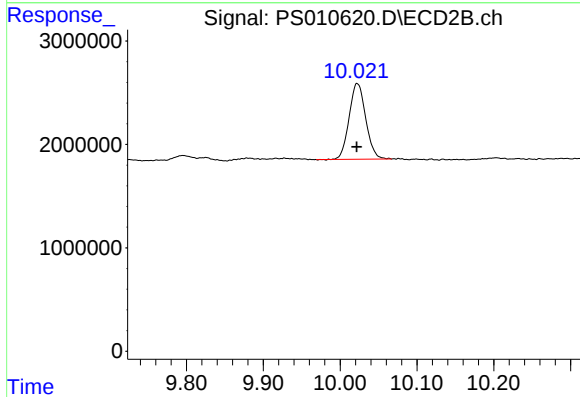


#14 DINOSEB

R.T.: 10.022 min
Delta R.T.: 0.000 min
Response: 11005875
Conc: 5.12 ng/ml

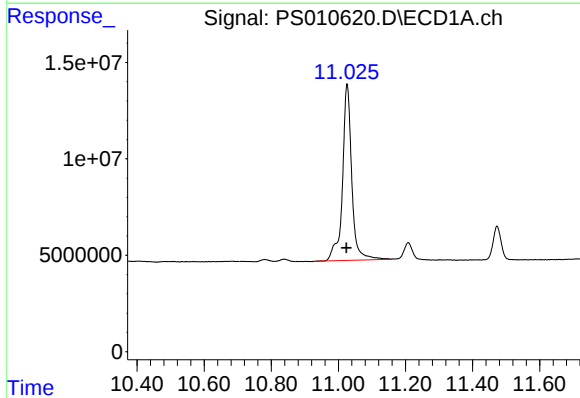


#15 Picloram

R.T.: 11.026 min
Delta R.T.: 0.002 min
Response: 176390552
Conc: 34.55 ng/ml

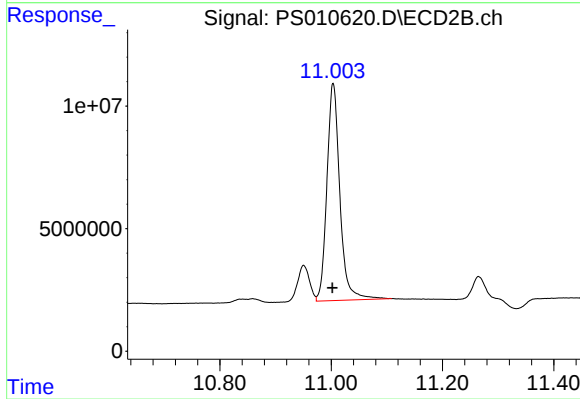

#15 Picloram


R.T.: 11.004 min
Delta R.T.: 0.001 min
Response: 143333559
Conc: 34.74 ng/ml

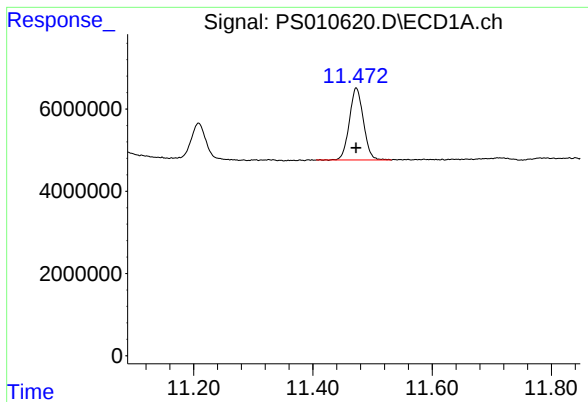

#16 DCPA

R.T.: 11.473 min
Delta R.T.: 0.000 min
Response: 28591192
Conc: 5.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

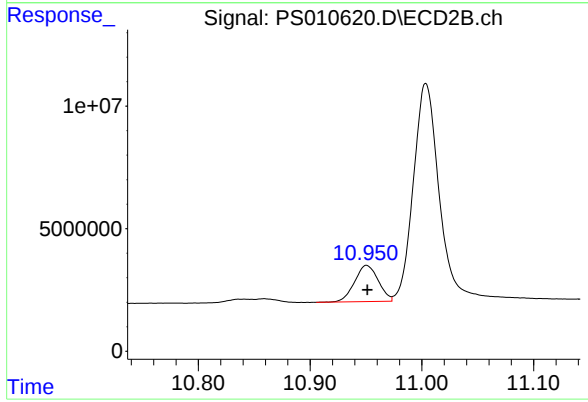

#16 DCPA

R.T.: 10.951 min
Delta R.T.: 0.000 min
Response: 21828314
Conc: 5.89 ng/ml