

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060220\
 Data File : PS010621.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 15:30
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 18:54:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.922	379.1E6	286.2E6	479.383	524.734
Target Compounds							
9) T	2,4-D	0.000	7.941	0	115.2E6	N.D.	151.923
12) T	2,4,5-T	9.492	9.182	13625814	9693983	3.350	3.230
15) T	Picloram	11.025	11.004	145.3E6	133.0E6	28.469	32.233
16) T	DCPA	11.472	10.950	13126964	10467364	2.450	2.823



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060220\
Data File : PS010621.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 15:30
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 18:54:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

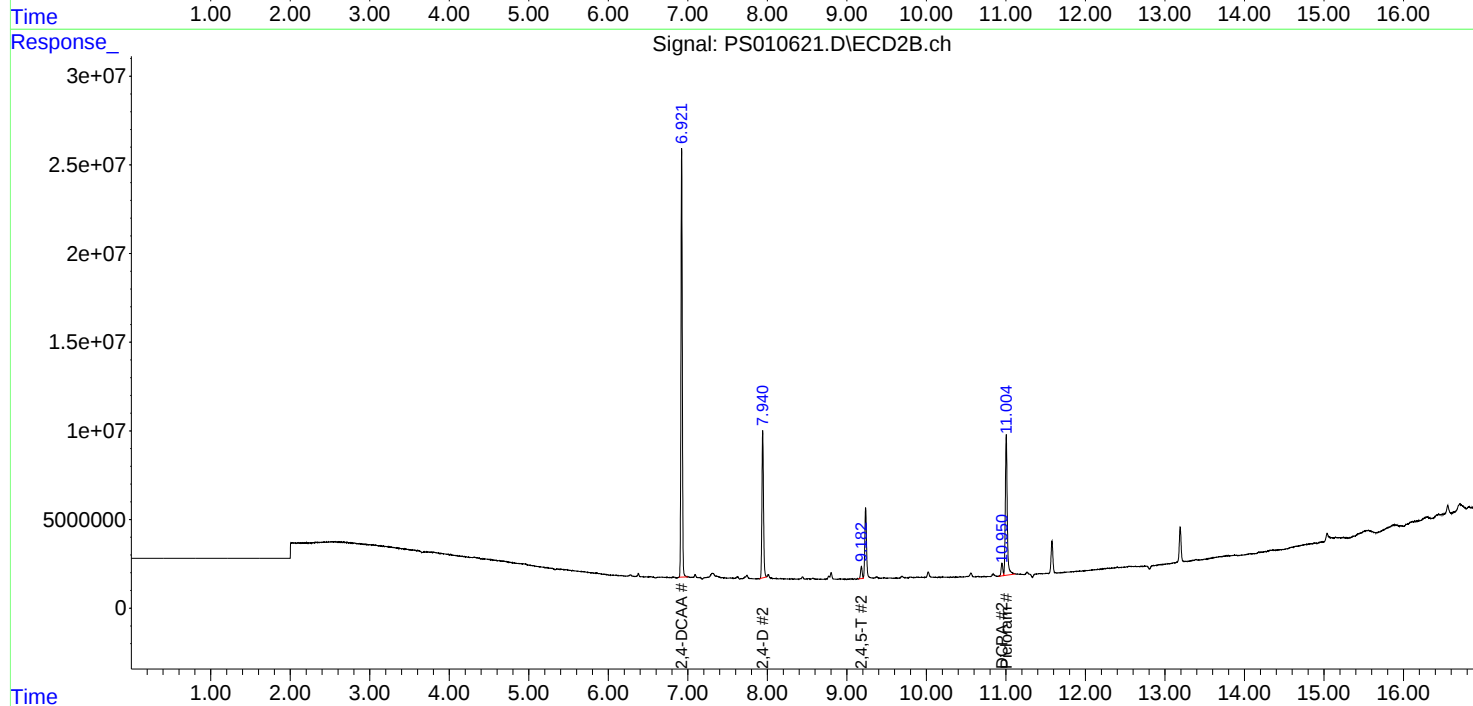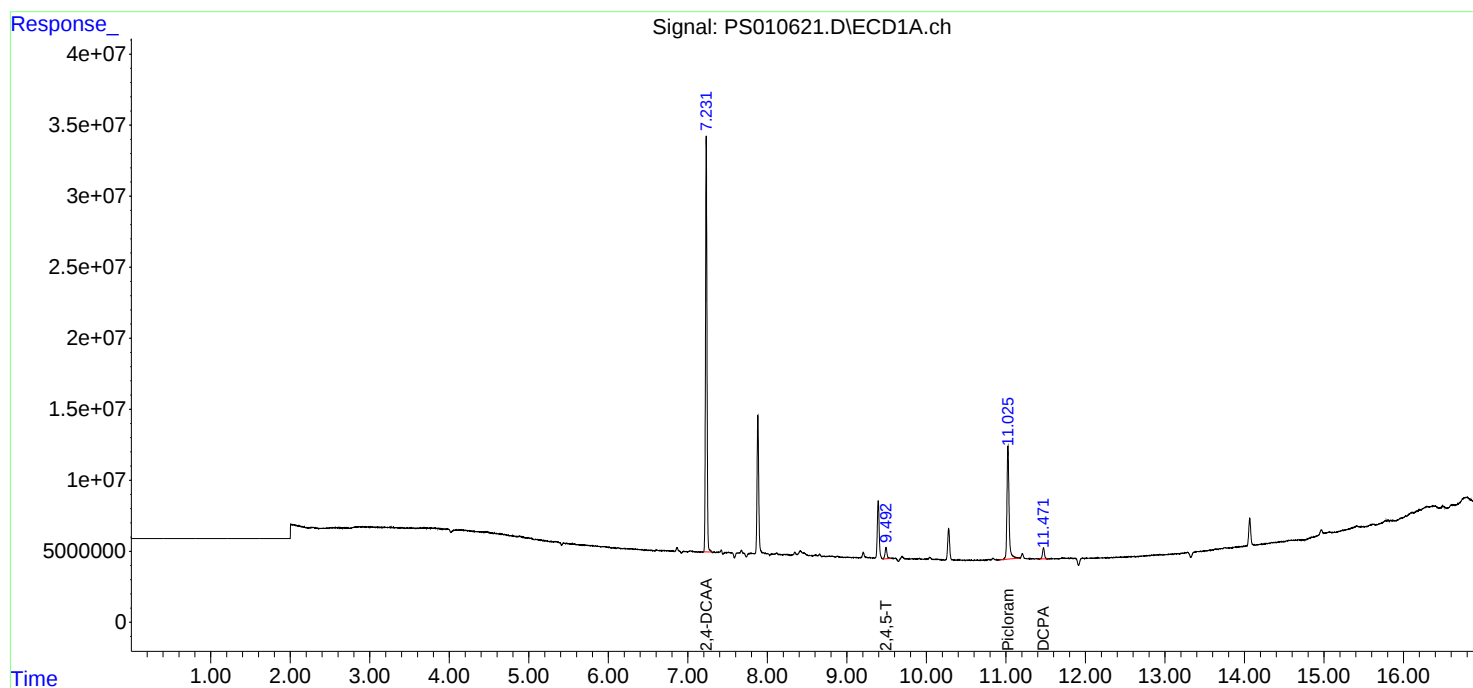


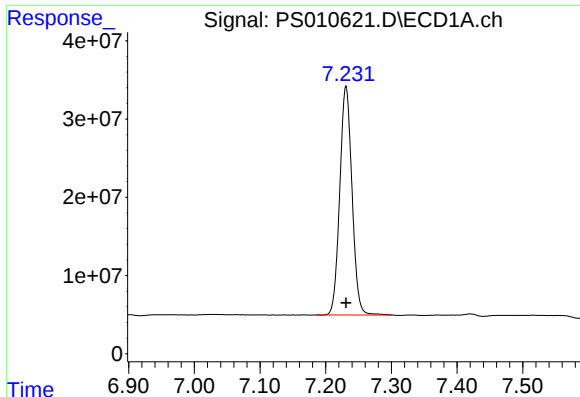

#4 2,4-DCAA


R.T.: 7.231 min
Delta R.T.: 0.000 min
Response: 379125877
Conc: 479.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

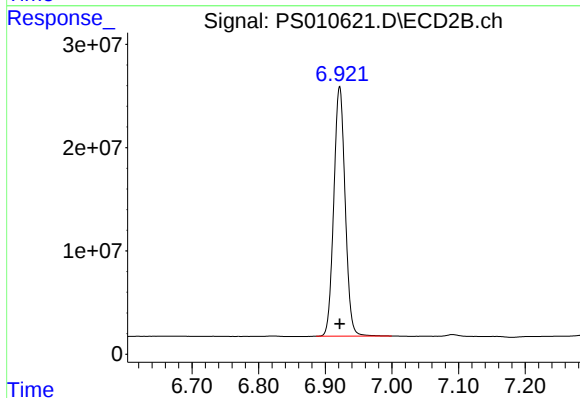


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: 0.000 min
Response: 286198347
Conc: 524.73 ng/ml

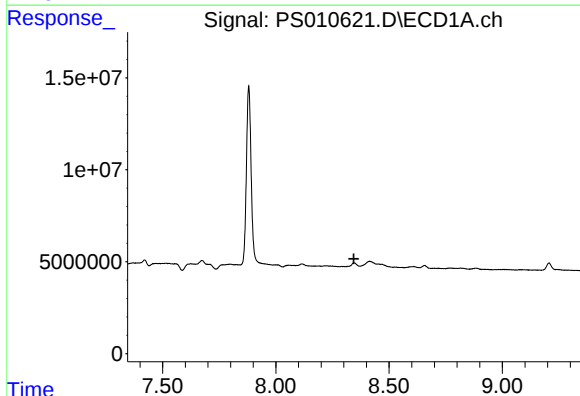


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

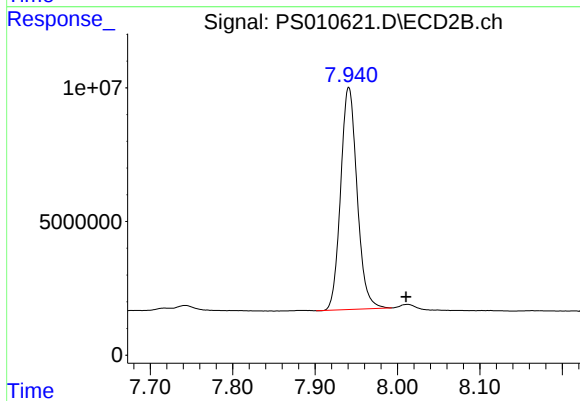

#9 2,4-D


R.T.: 7.941 min
Delta R.T.: -0.069 min
Response: 115196087
Conc: 151.92 ng/ml

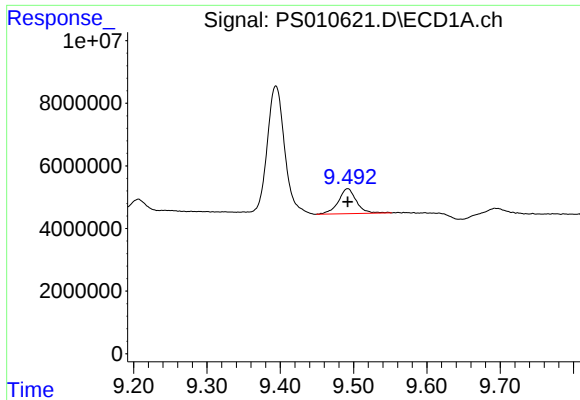

#12 2,4,5-T


R.T.: 9.492 min
Delta R.T.: 0.000 min
Response: 13625814
Conc: 3.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

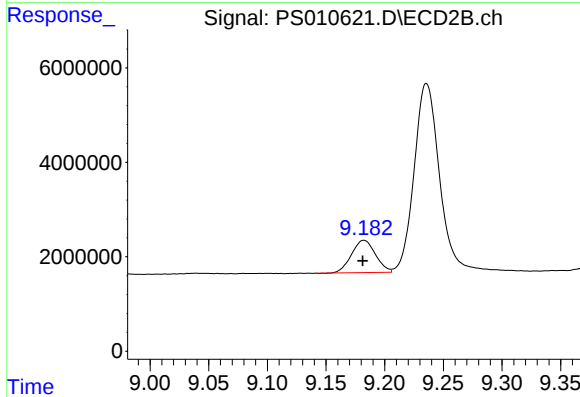


#12 2,4,5-T

R.T.: 9.182 min
Delta R.T.: 0.001 min
Response: 9693983
Conc: 3.23 ng/ml

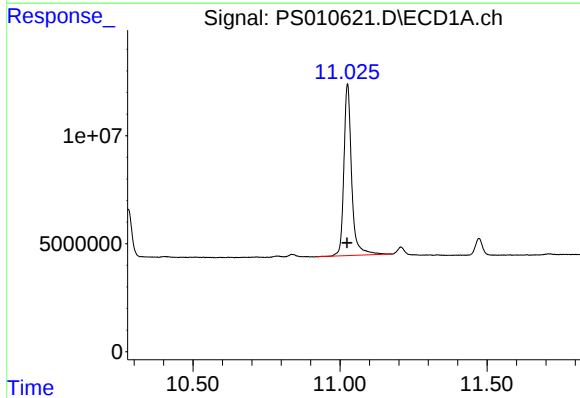


#15 Picloram

R.T.: 11.025 min
Delta R.T.: 0.001 min
Response: 145335529
Conc: 28.47 ng/ml

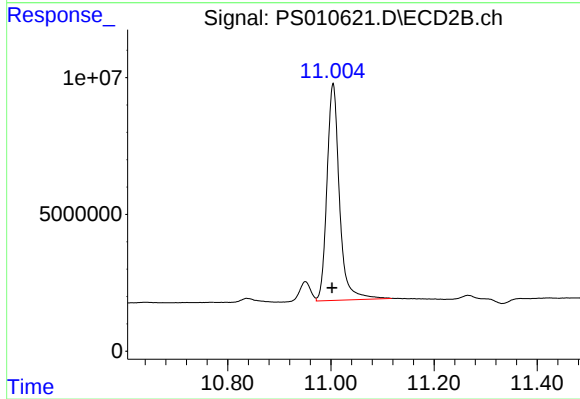

#15 Picloram


R.T.: 11.004 min
Delta R.T.: 0.002 min
Response: 132993642
Conc: 32.23 ng/ml

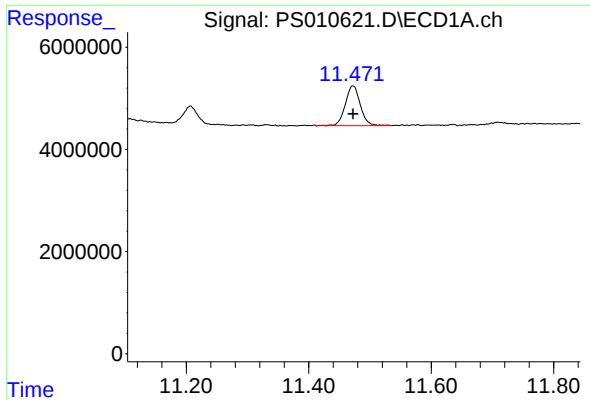

#16 DCPA

R.T.: 11.472 min
Delta R.T.: 0.000 min
Response: 13126964
Conc: 2.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

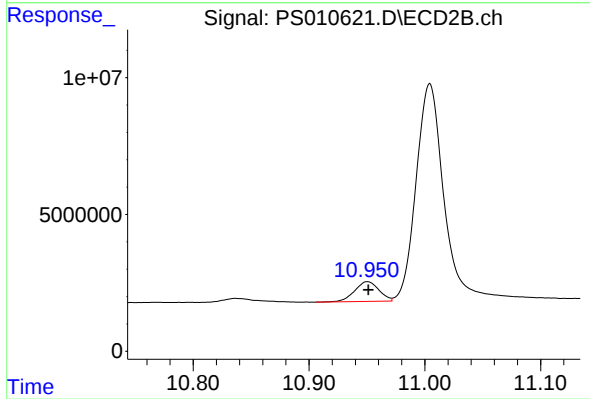

#16 DCPA

R.T.: 10.950 min
Delta R.T.: 0.000 min
Response: 10467364
Conc: 2.82 ng/ml