

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060221\
 Data File : PS015160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 11:35
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 17:47:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.782	1117.2E6	271.2E6	443.248	506.159
Target Compounds							
3) T	4-Nitroph...	7.024	0.000	4195396	0	2.976	N.D. #
7) T	MCPA	7.671f	0.000	5416366	0	<MDL	N.D. #
15) T	Picloram	11.017	10.845	53152995	13426250	3.208	3.233
16) T	DCPA	0.000	10.845	0	13426250	N.D.	3.114



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060221\
Data File : PS015160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 11:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 17:47:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

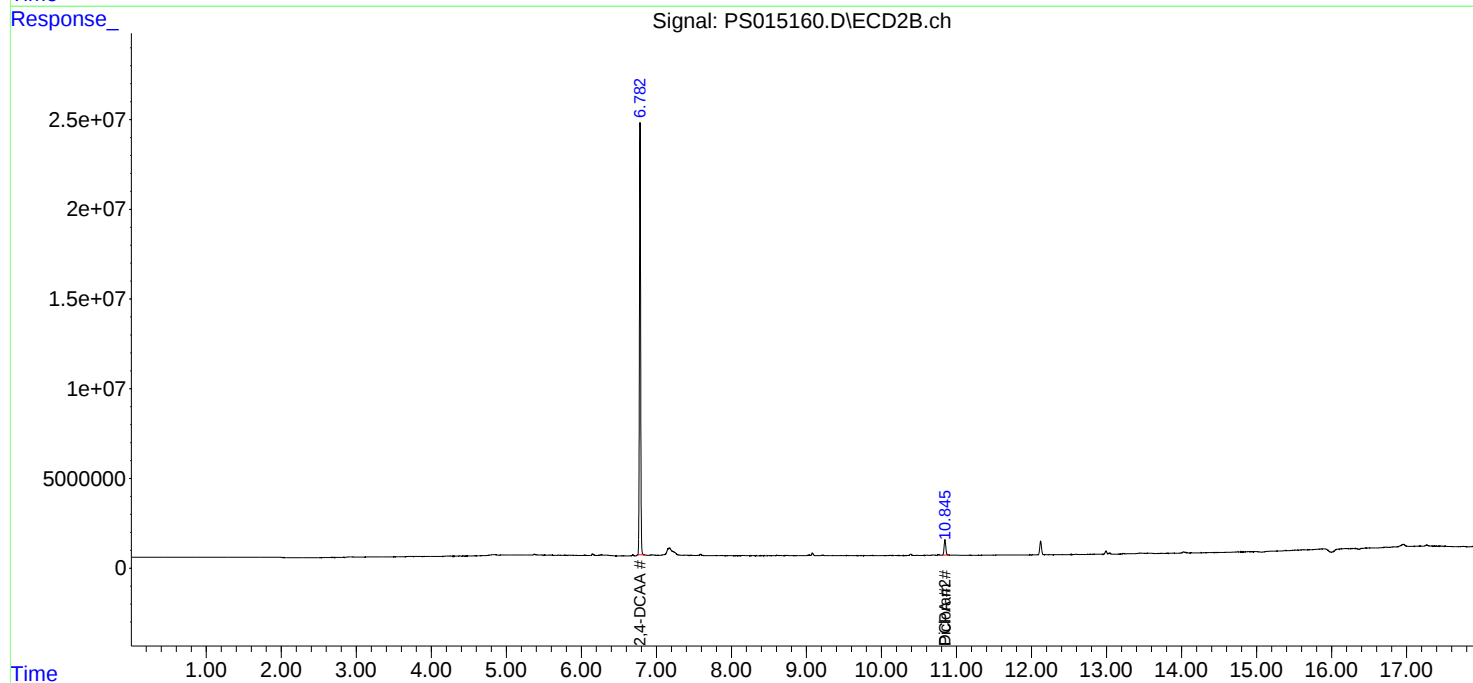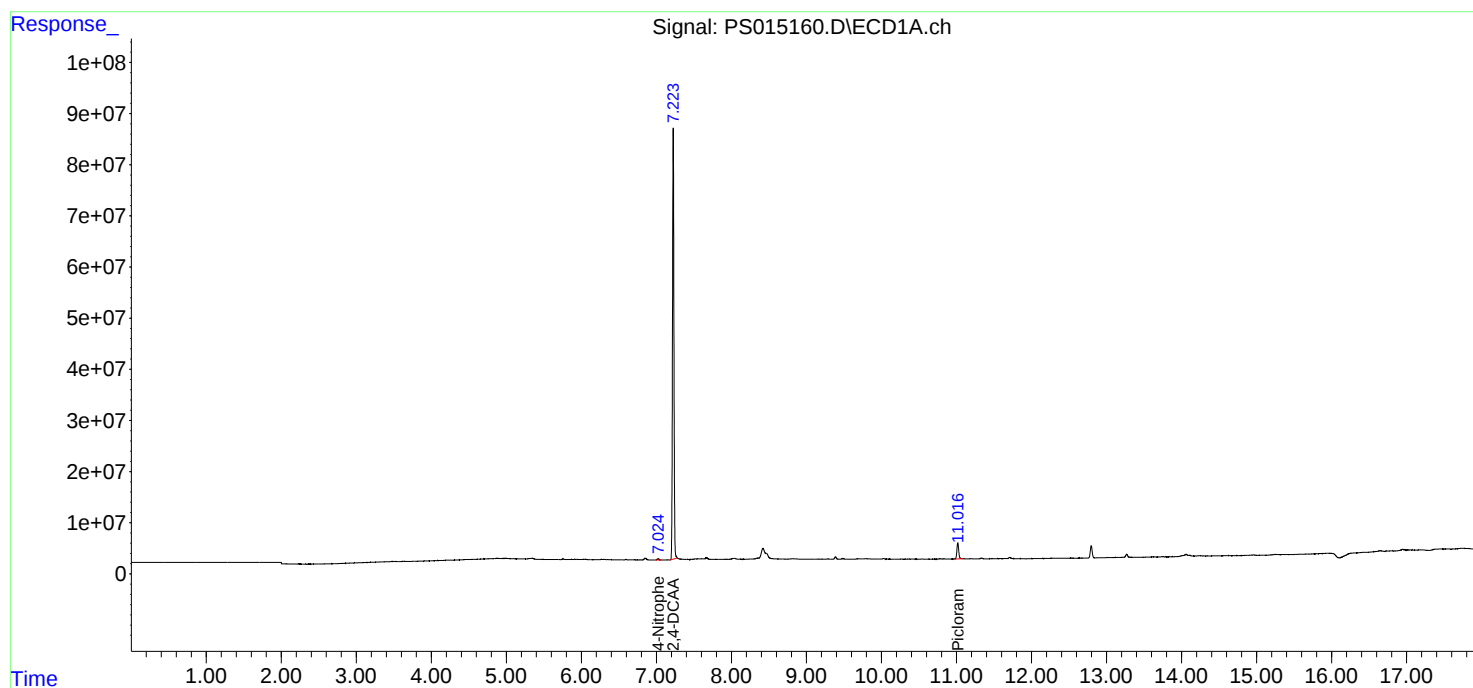


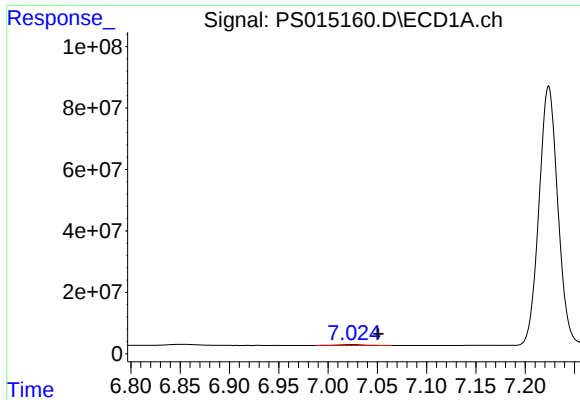

#3 4-Nitrophenol


R.T.: 7.024 min
Delta R.T.: -0.027 min
Response: 4195396
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

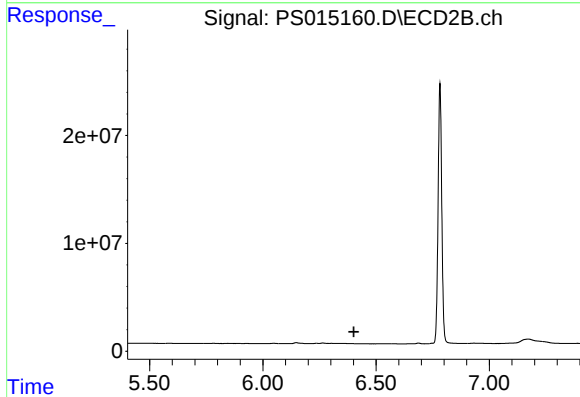


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

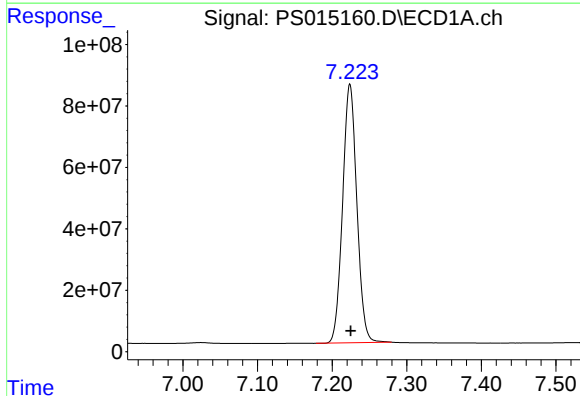


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: -0.001 min
Response: 1117151043
Conc: 443.25 ng/ml

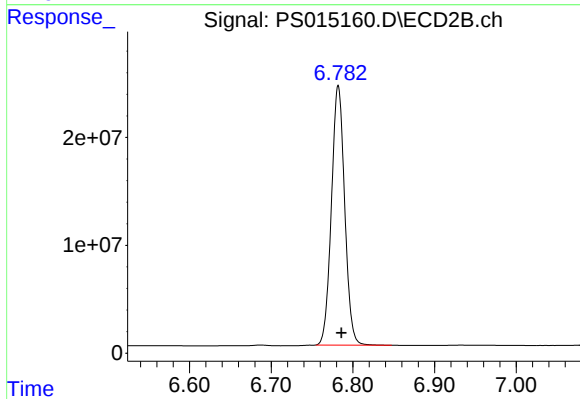

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.004 min
Response: 271185502
Conc: 506.16 ng/ml

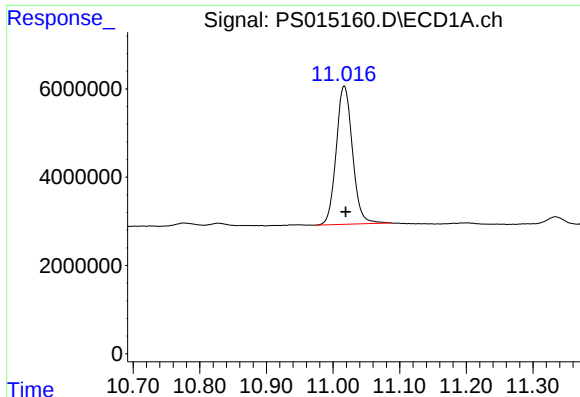

#15 Picloram


R.T.: 11.017 min
Delta R.T.: -0.002 min
Response: 53152995
Conc: 3.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

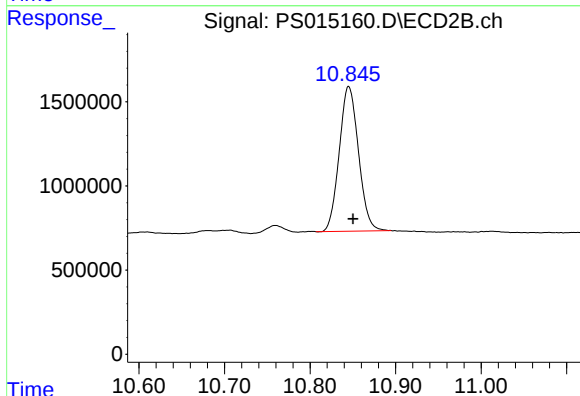


#15 Picloram

R.T.: 10.845 min
Delta R.T.: -0.005 min
Response: 13426250
Conc: 3.23 ng/ml

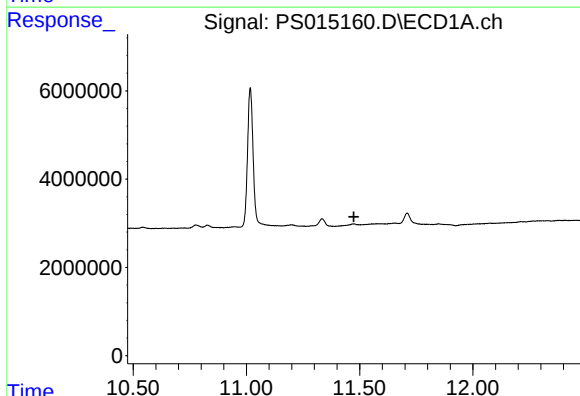

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.475 min
Response: 0
Conc: N.D.

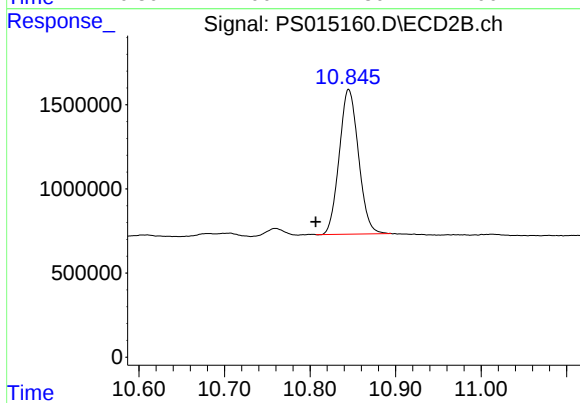

#16 DCPA

R.T.: 10.845 min
Delta R.T.: 0.039 min
Response: 13426250
Conc: 3.11 ng/ml