

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060221\
 Data File : PS015164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 14:59
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 17:48:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.785	1213.1E6	277.4E6	481.305	517.689
Target Compounds							
3) T	4-Nitroph...	7.027	0.000	4910173	0	3.483	N.D. #
5) T	DICAMBA	7.419	0.000	6318442	0	<MDL	N.D. #
7) T	MCPA	7.672f	0.000	14965201	0	1.491	N.D. #
9) T	2,4-D	8.344	0.000	6326200	0	2.483	N.D. #
10) T	Pentachlo...	8.655	8.295	14544799	3235707	<MDL	<MDL #
11) T	2,4,5-TP ...	9.206	0.000	9147033	0	<MDL	N.D. #
12) T	2,4,5-T	9.489	0.000	10253550	0	<MDL	N.D. #
15) T	Picloram	11.019	10.849	25283052	5961922	1.526	1.436
16) T	DCPA	11.472	10.849f	10464949	5961922	<MDL	1.383 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060221\
Data File : PS015164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 14:59
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 17:48:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

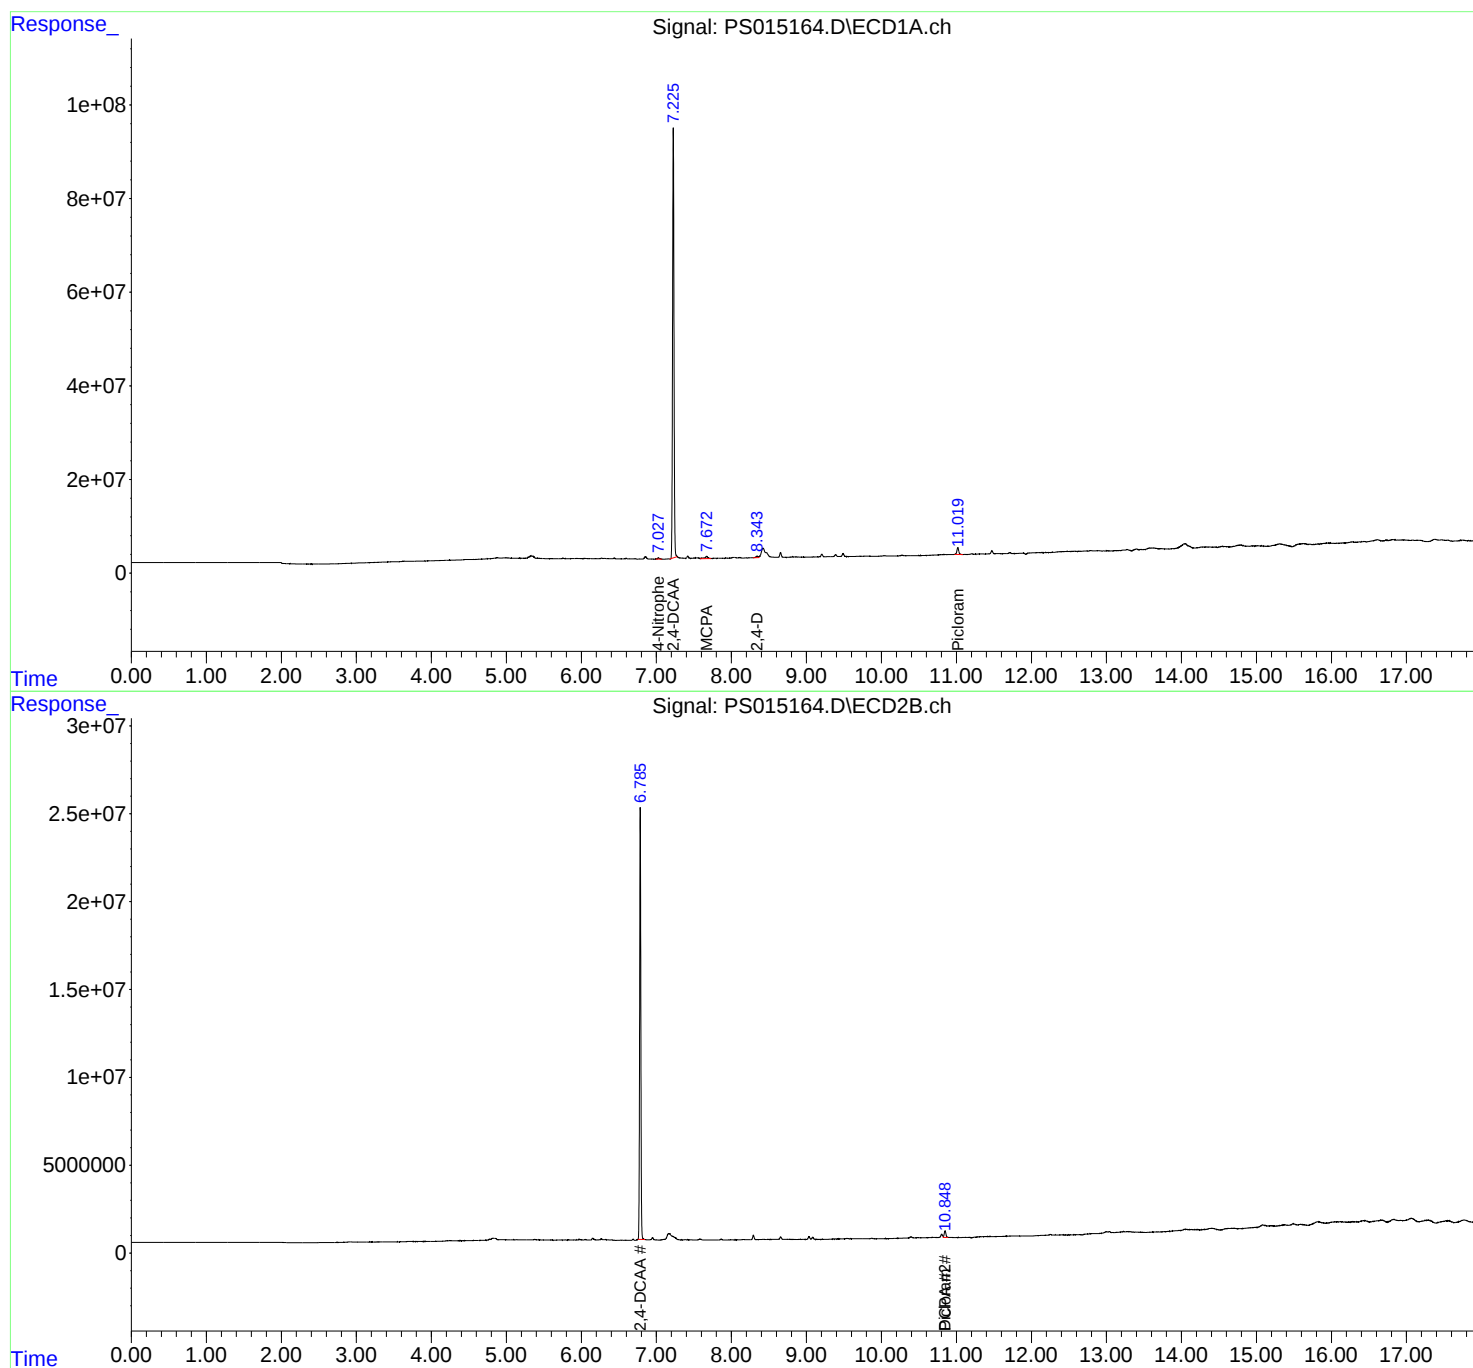


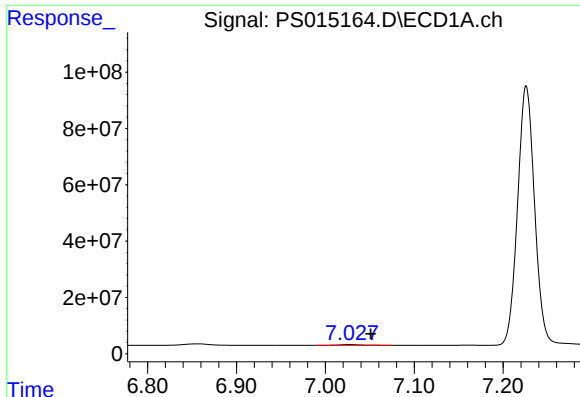

#3 4-Nitrophenol


R.T.: 7.027 min
Delta R.T.: -0.024 min
Response: 4910173
Conc: 3.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

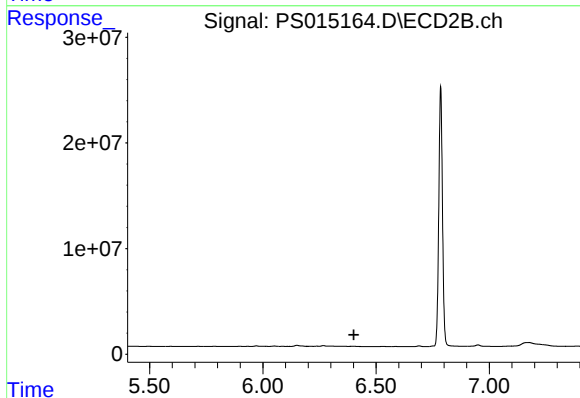


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

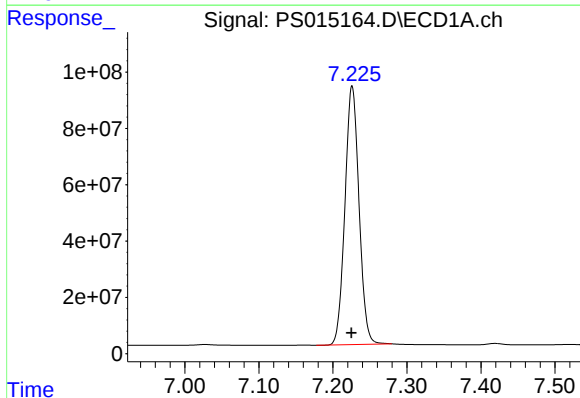


#4 2,4-DCAA

R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 1213068315
Conc: 481.30 ng/ml

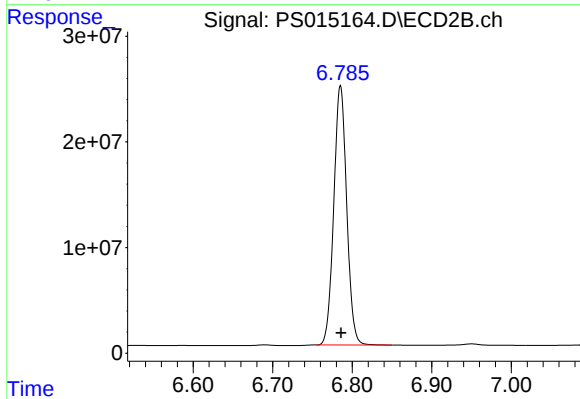

#4 2,4-DCAA


R.T.: 6.785 min
Delta R.T.: 0.000 min
Response: 277362676
Conc: 517.69 ng/ml

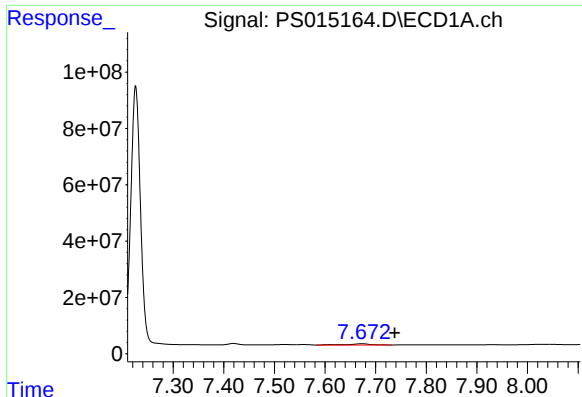

#7 MCPA


R.T.: 7.672 min
Delta R.T.: -0.066 min
Response: 14965201
Conc: 1.49 ug/ml

Instrument :
ECD_S
ClientSampleId :

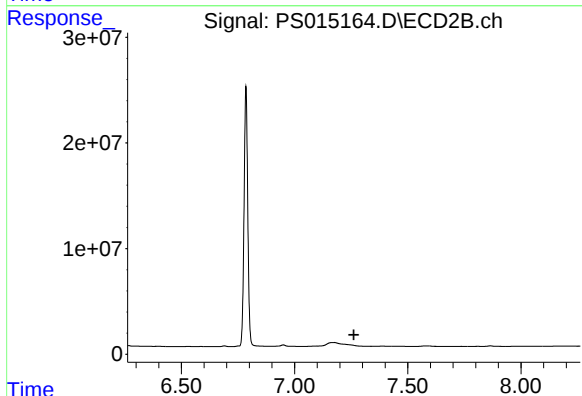


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

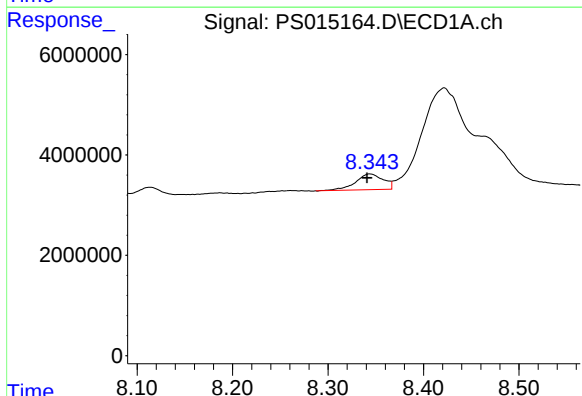


#9 2,4-D

R.T.: 8.344 min
Delta R.T.: 0.003 min
Response: 6326200
Conc: 2.48 ng/ml

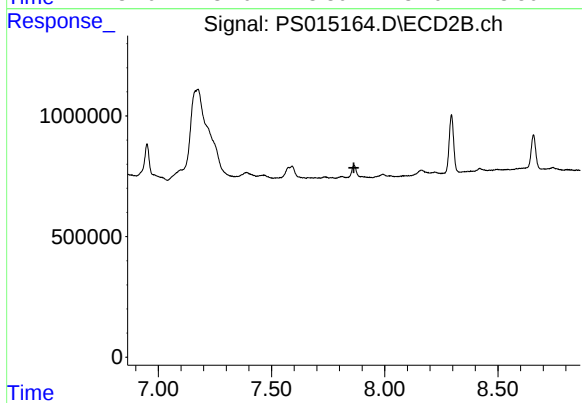

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

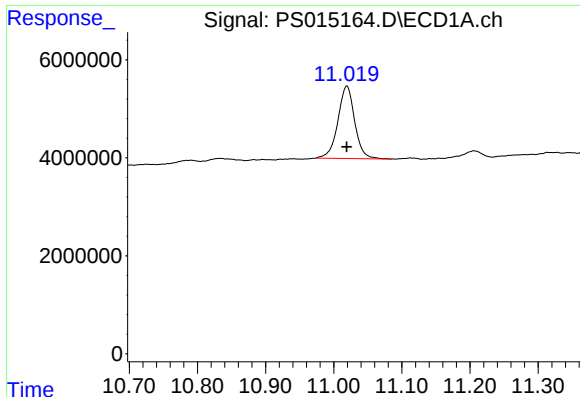

#15 Picloram


R.T.: 11.019 min
Delta R.T.: 0.000 min
Response: 25283052
Conc: 1.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

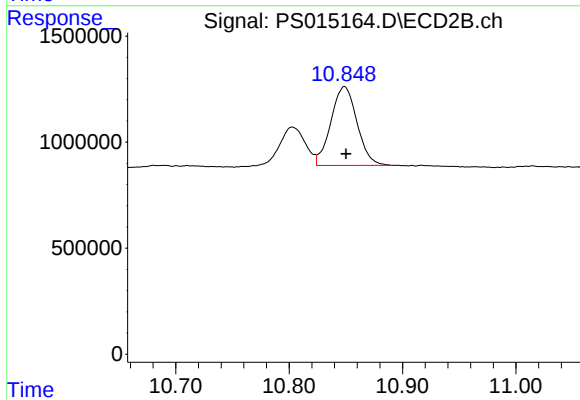


#15 Picloram

R.T.: 10.849 min
Delta R.T.: -0.001 min
Response: 5961922
Conc: 1.44 ng/ml

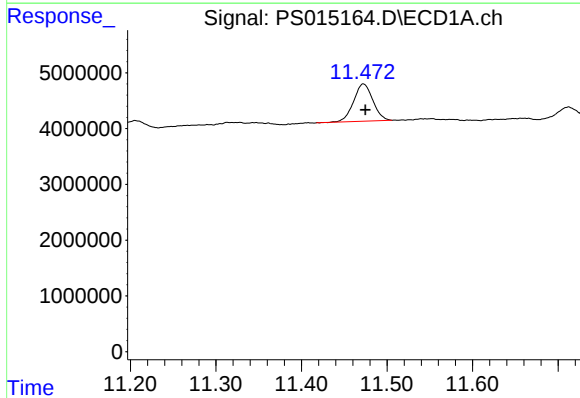

#16 DCPA

R.T.: 11.472 min
Delta R.T.: -0.002 min
Response: 10464949
Conc: N.D.

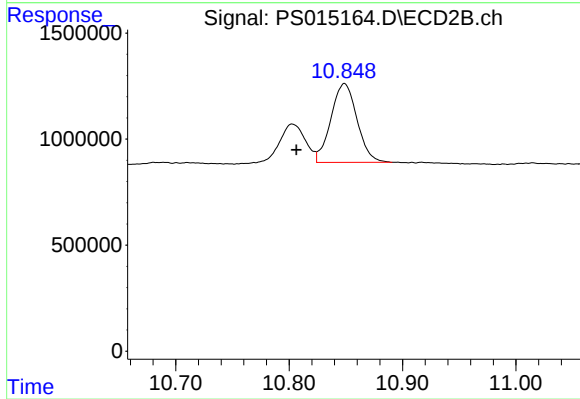

#16 DCPA

R.T.: 10.849 min
Delta R.T.: 0.042 min
Response: 5961922
Conc: 1.38 ng/ml