

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060223\
 Data File : PS023208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2023 10:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 12:25:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.483	6.855	799.1E6	299.5E6	525.404	533.752
Target Compounds							
1) T	Dalapon	2.584	0.000	820821	0	<MDL	N.D. #
3) T	4-Nitroph...	6.318	0.000	7448478	0	7.075	N.D. #
5) T	DICAMBA	0.000	7.021	0	760817	N.D.	<MDL
6) T	MCP	6.751	0.000	512378	0	<MDL	N.D. #
7) T	MCPA	0.000	7.309	0	7804847	N.D.	2.948
8) T	DICHLORPROP	7.262	7.663	590980	2887671	<MDL	4.666 #
9) T	2,4-D	7.407	7.879f	2509431	919254	1.084	1.285
10) T	Pentachlo...	7.676	0.000	1495546	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.215	0.000	3201400	0	<MDL	N.D. #
12) T	2,4,5-T	8.482	9.143f	2619892	2700697	<MDL	<MDL #
13) T	2,4-DB	8.980	0.000	4088854	0	1.743	N.D. #
14) T	DINOSEB	10.063	0.000	611417	0	<MDL	N.D. #
15) T	Picloram	9.894	10.899	52241534	8798761	3.046	2.066 #
16) T	DCPA	10.335	10.899	1795325	8798761	<MDL	2.355 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060223\
Data File : PS023208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2023 10:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 12:25:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

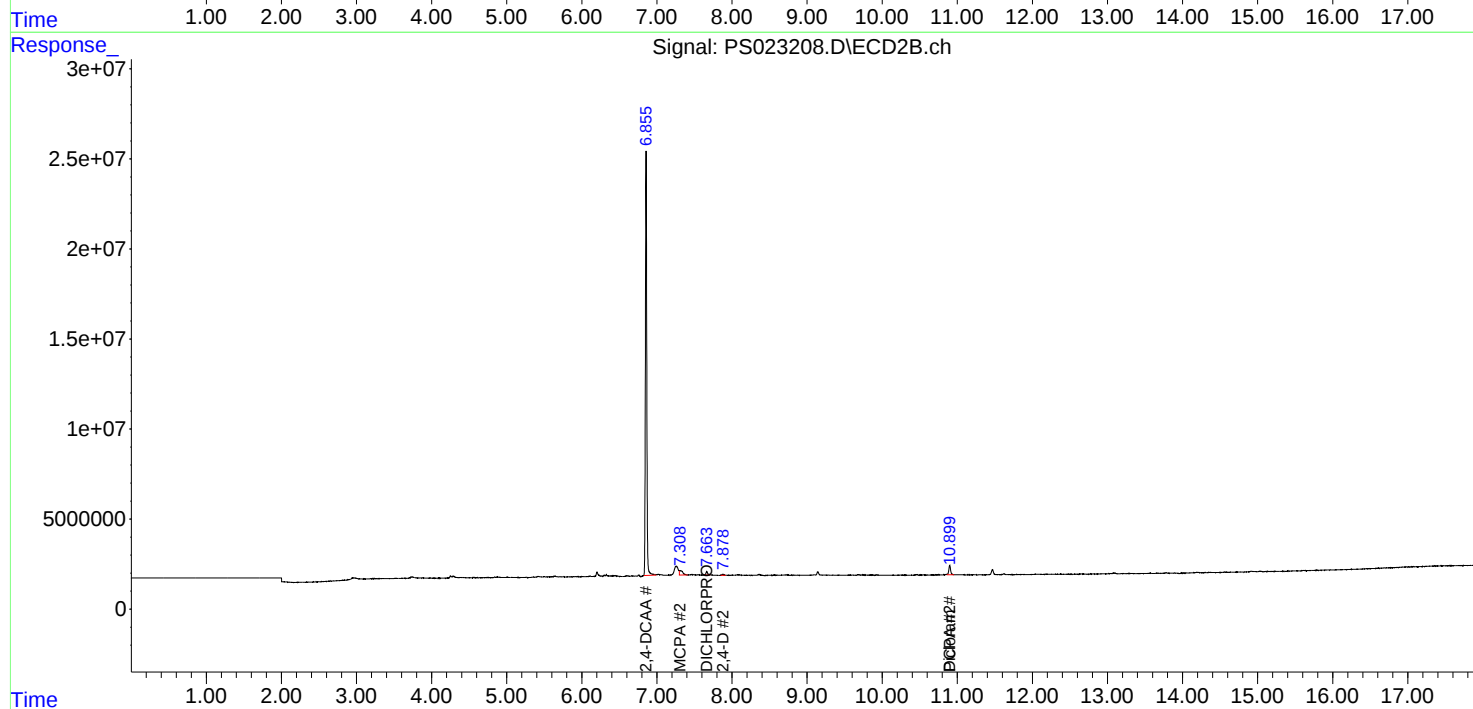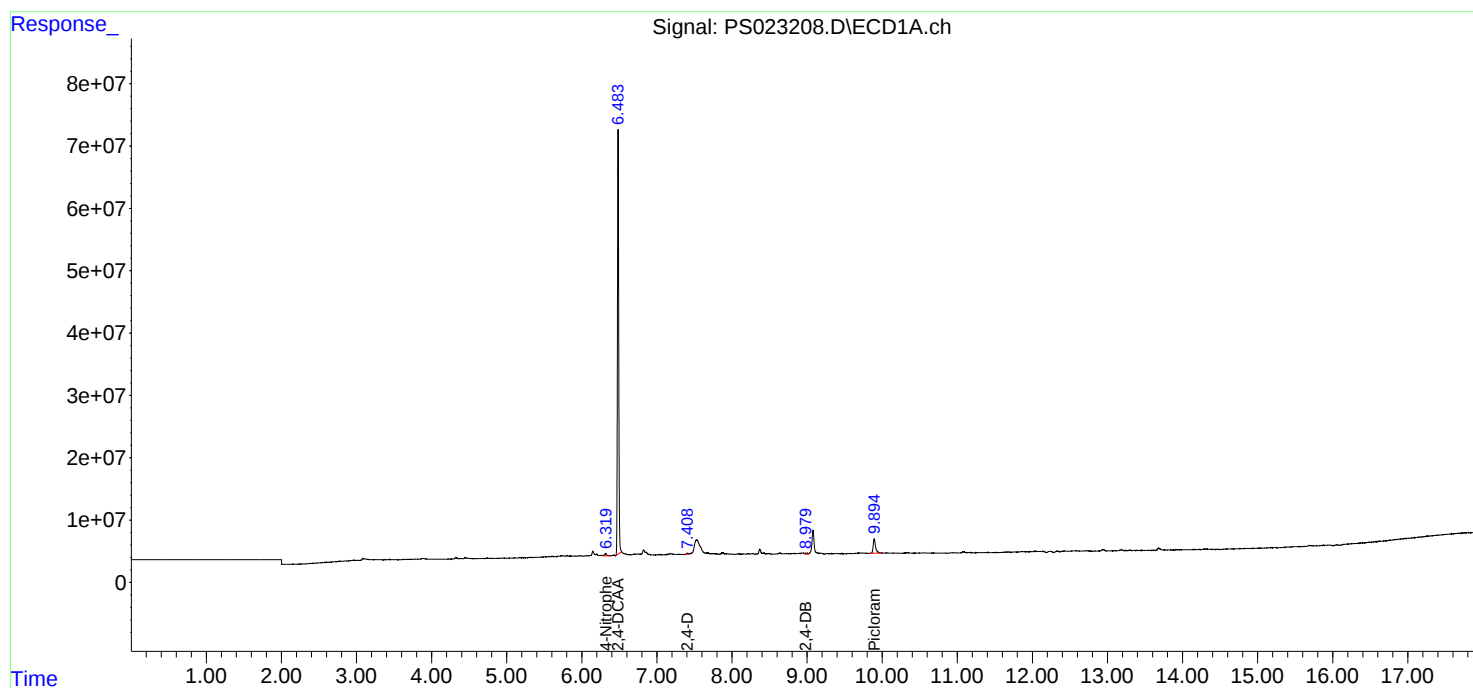


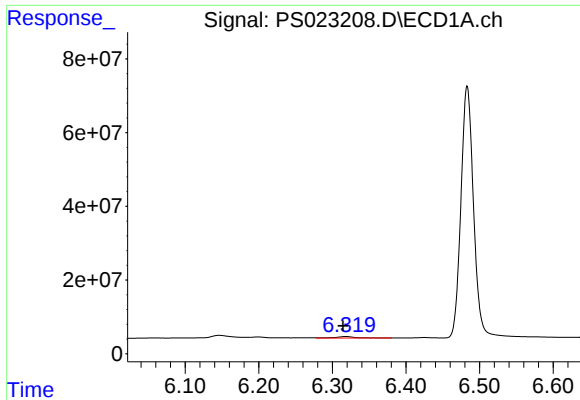

#3 4-Nitrophenol


R.T.: 6.318 min
Delta R.T.: 0.004 min
Response: 7448478
Conc: 7.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

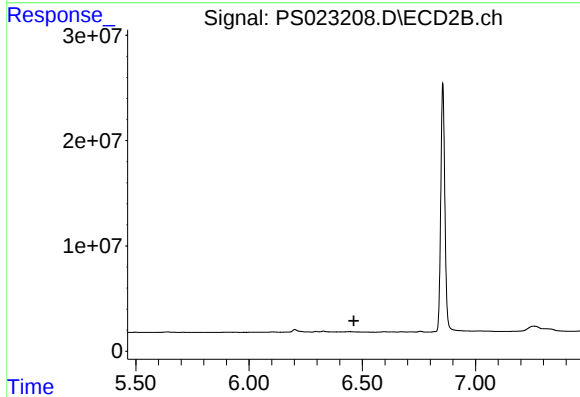


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

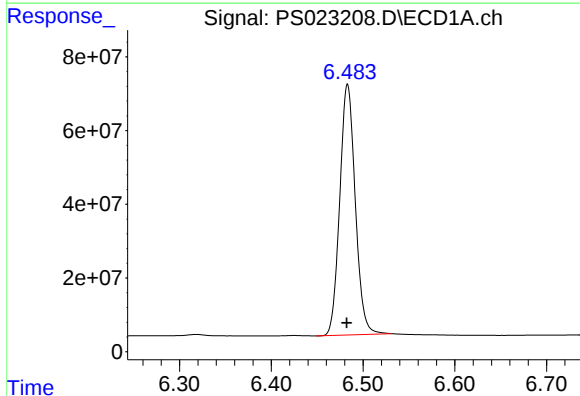


#4 2,4-DCAA

R.T.: 6.483 min
Delta R.T.: 0.001 min
Response: 799136749
Conc: 525.40 ng/ml

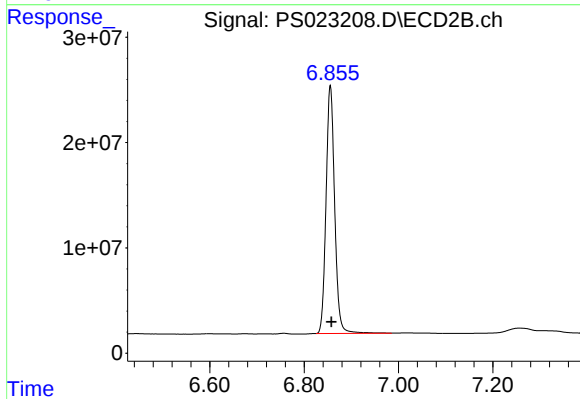

#4 2,4-DCAA


R.T.: 6.855 min
Delta R.T.: -0.003 min
Response: 299496437
Conc: 533.75 ng/ml

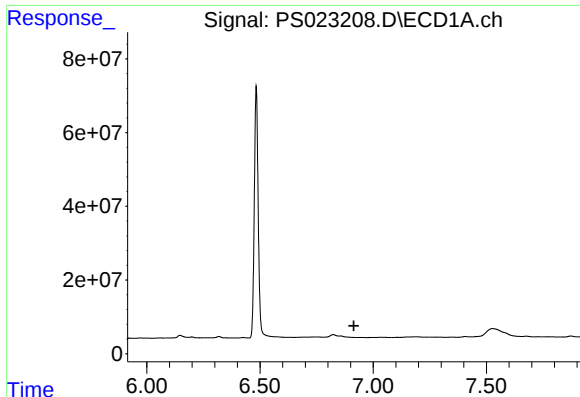

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.915 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

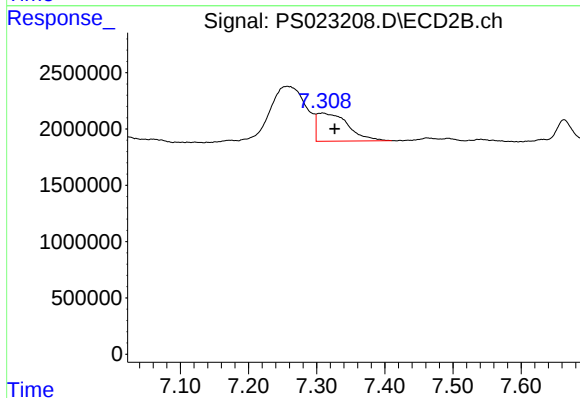


#7 MCPA

R.T.: 7.309 min
Delta R.T.: -0.018 min
Response: 7804847
Conc: 2.95 ug/ml

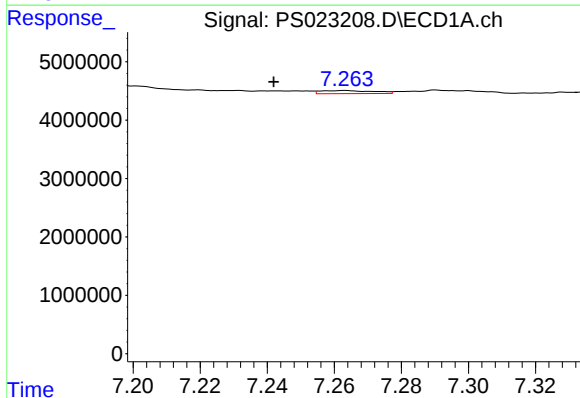


#8 DICHLORPROP

R.T.: 7.262 min
Delta R.T.: 0.020 min
Response: 590980
Conc: N.D.

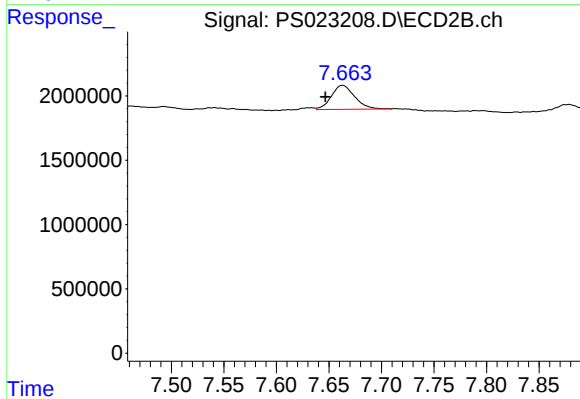

#8 DICHLORPROP


R.T.: 7.663 min
Delta R.T.: 0.016 min
Response: 2887671
Conc: 4.67 ng/ml

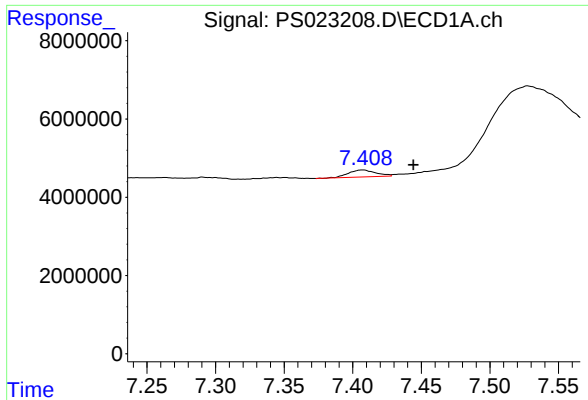

#9 2,4-D


R.T.: 7.407 min
Delta R.T.: -0.037 min
Response: 2509431
Conc: 1.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

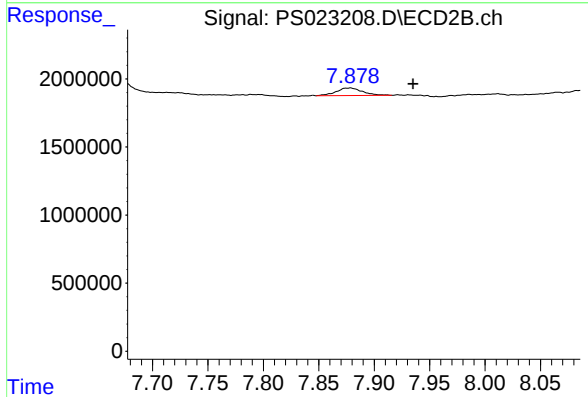


#9 2,4-D

R.T.: 7.879 min
Delta R.T.: -0.056 min
Response: 919254
Conc: 1.28 ng/ml

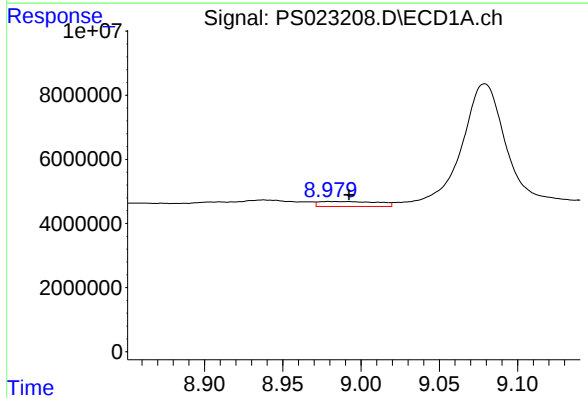


#13 2,4-DB

R.T.: 8.980 min
Delta R.T.: -0.012 min
Response: 4088854
Conc: 1.74 ng/ml

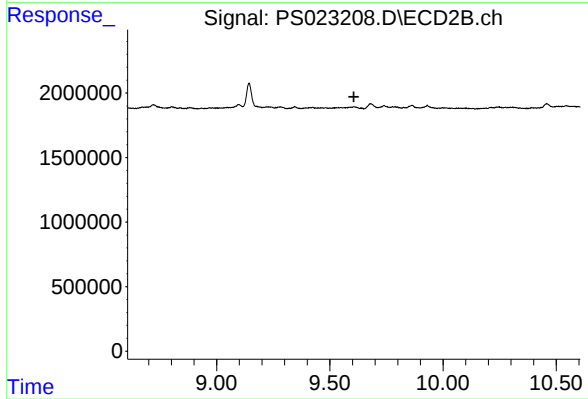

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.606 min
Response: 0
Conc: N.D.

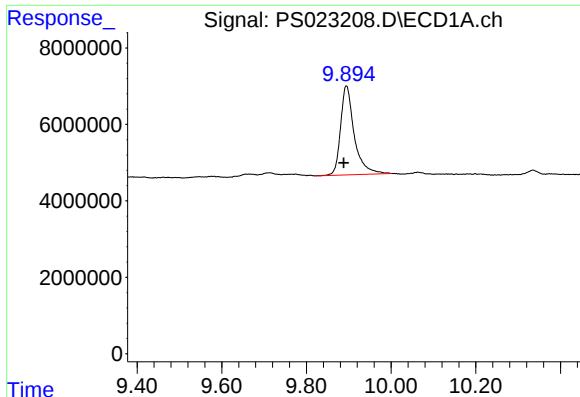

#15 Picloram


R.T.: 9.894 min
Delta R.T.: 0.007 min
Response: 52241534
Conc: 3.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

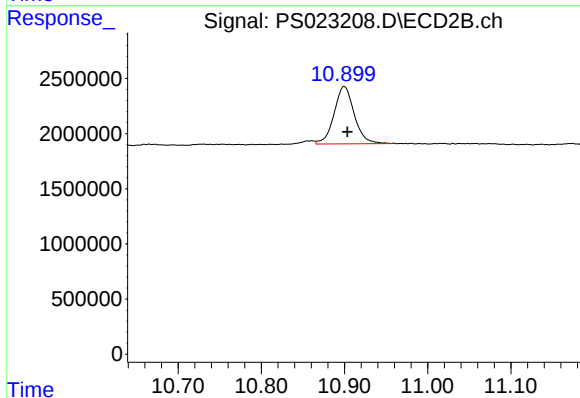


#15 Picloram

R.T.: 10.899 min
Delta R.T.: -0.004 min
Response: 8798761
Conc: 2.07 ng/ml

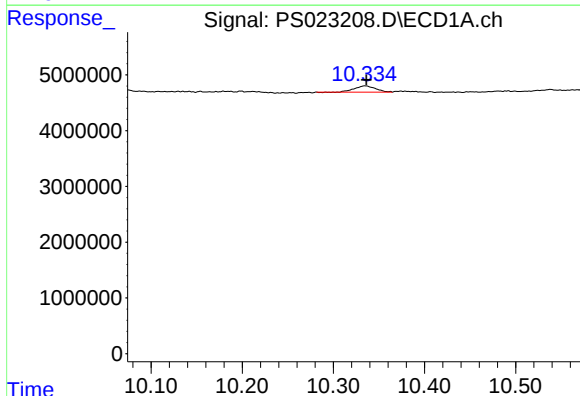

#16 DCPA

R.T.: 10.335 min
Delta R.T.: -0.001 min
Response: 1795325
Conc: N.D.

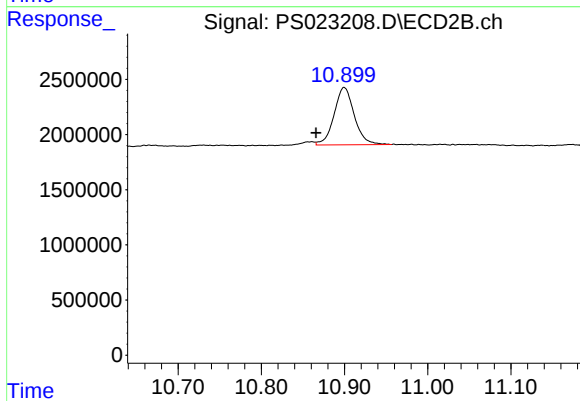

#16 DCPA

R.T.: 10.899 min
Delta R.T.: 0.034 min
Response: 8798761
Conc: 2.35 ng/ml