

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060223\
 Data File : PS023211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2023 12:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 16:01:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.484	6.855	783.2E6	294.9E6	514.947	525.609
Target Compounds							
1) T	Dalapon	2.578	0.000	2755491	0	1.704	N.D. #
2) T	3,5-DICHL...	5.842	6.069f	-577492	634143	N.D.	<MDL
3) T	4-Nitroph...	6.319	0.000	6819252	0	6.477	N.D. #
5) T	DICAMBA	6.636	0.000	210867	0	<MDL	N.D. #
6) T	MCP	6.754	0.000	284080	0	<MDL	N.D. #
7) T	MCPA	6.943	7.306	266362	6893130	<MDL	2.603 #
8) T	DICHLORPROP	7.237	7.662	519643	3174119	<MDL	5.129 #
9) T	2,4-D	7.407	0.000	3448254	0	1.490	N.D. #
10) T	Pentachlo...	7.677	0.000	1176194	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.215	0.000	2974687	0	<MDL	N.D. #
12) T	2,4,5-T	8.484	9.142f	2586012	763949	<MDL	<MDL #
13) T	2,4-DB	8.940f	0.000	5473478	0	2.333	N.D. #
14) T	DINOSEB	10.068	0.000	1089426	0	<MDL	N.D. #
15) T	Picloram	9.898	10.899	21222591	3719870	1.238	<MDL #
16) T	DCPA	10.340	10.899	1796310	3719870	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060223\
Data File : PS023211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2023 12:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 16:01:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

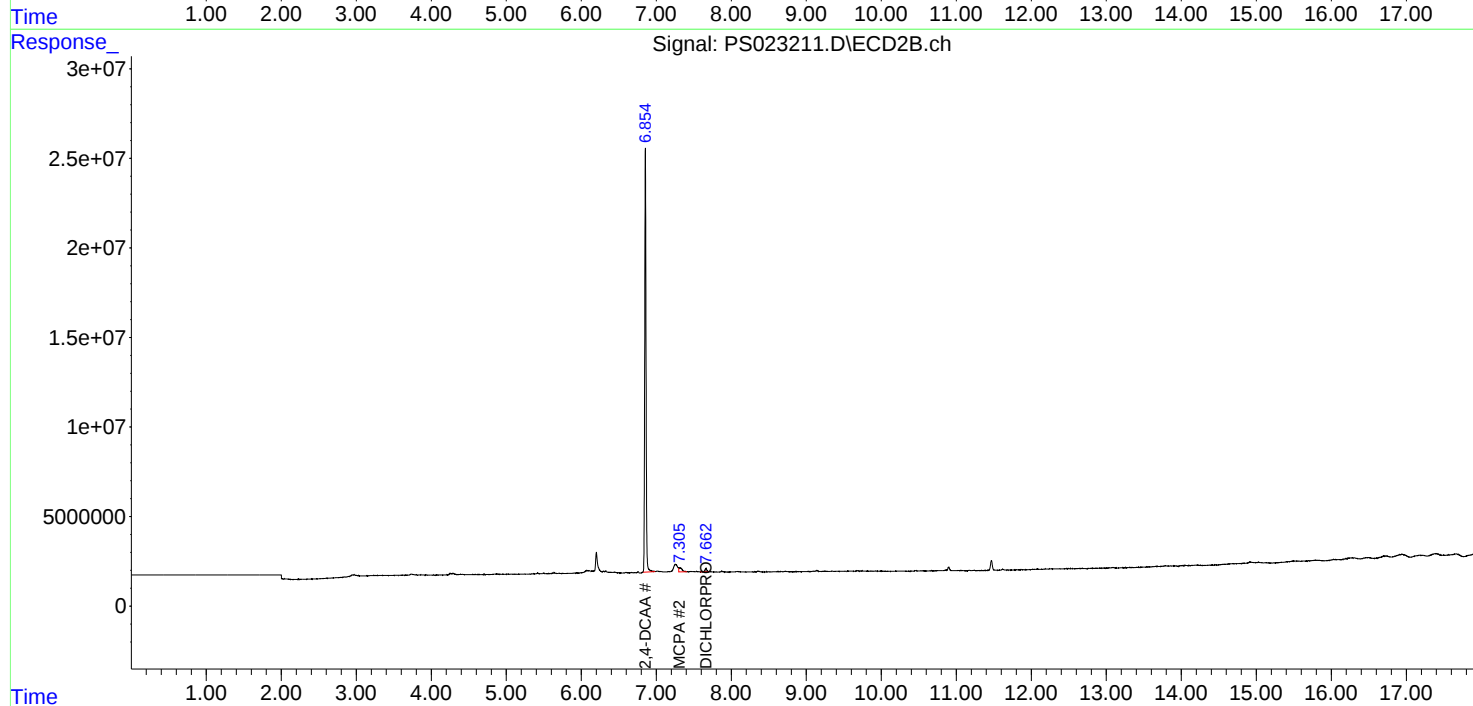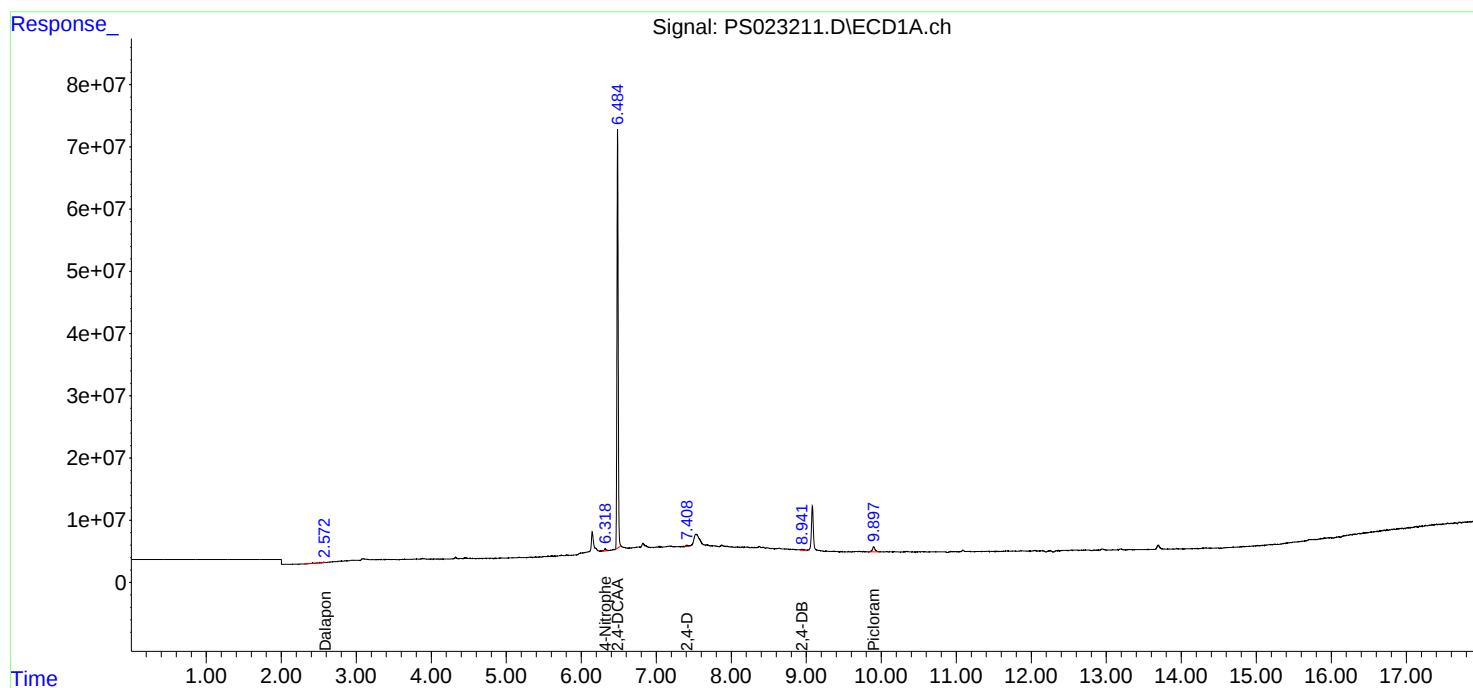


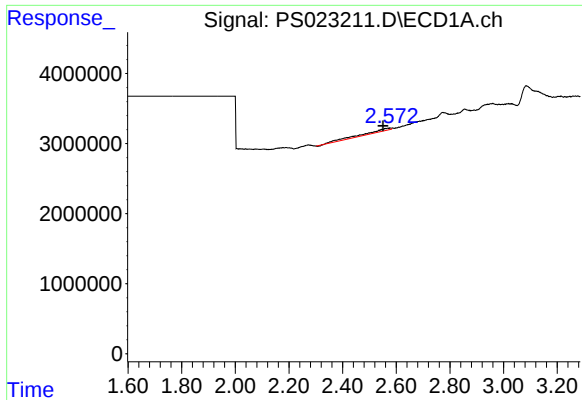

#1 Dalapon


R.T.: 2.578 min
Delta R.T.: 0.027 min
Response: 2755491
Conc: 1.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

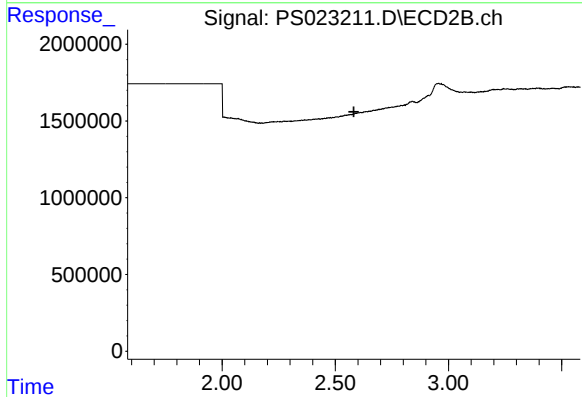


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.582 min
Response: 0
Conc: N.D.

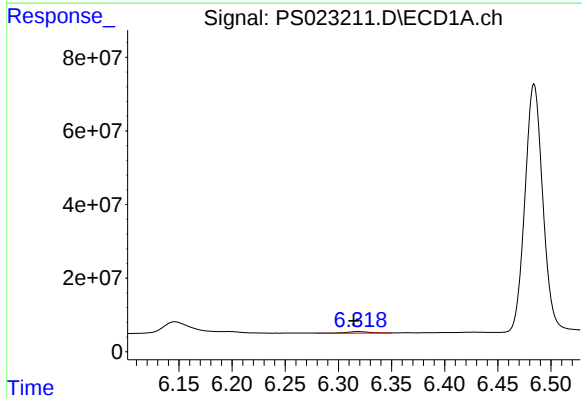


#3 4-Nitrophenol

R.T.: 6.319 min
Delta R.T.: 0.004 min
Response: 6819252
Conc: 6.48 ng/ml

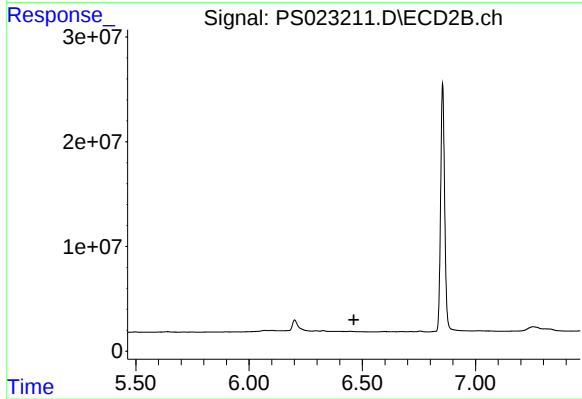

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

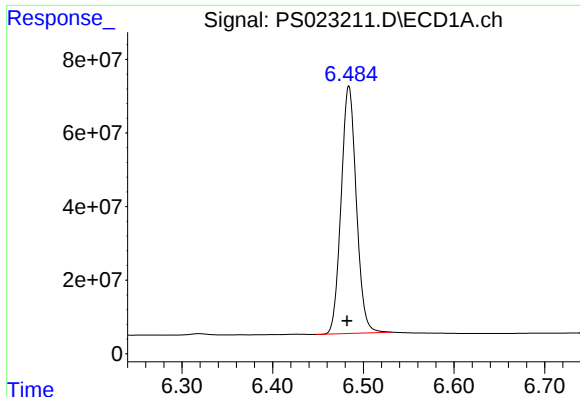

#4 2,4-DCAA


R.T.: 6.484 min
Delta R.T.: 0.002 min
Response: 783231625
Conc: 514.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

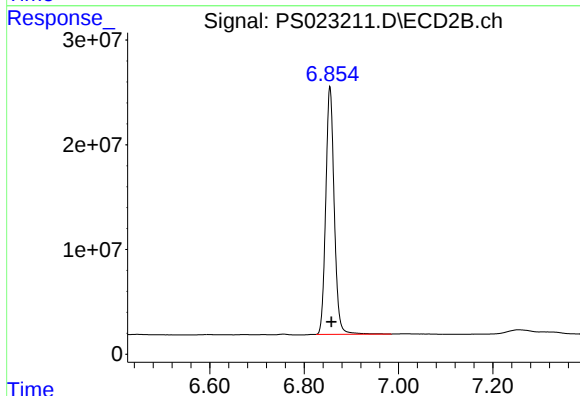


#4 2,4-DCAA

R.T.: 6.855 min
Delta R.T.: -0.003 min
Response: 294927480
Conc: 525.61 ng/ml

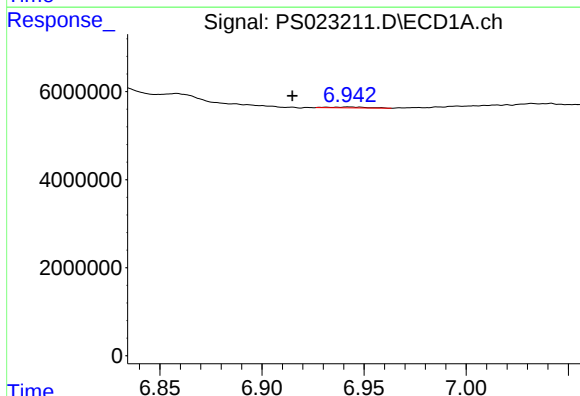


#7 MCPA

R.T.: 6.943 min
Delta R.T.: 0.028 min
Response: 266362
Conc: N.D.

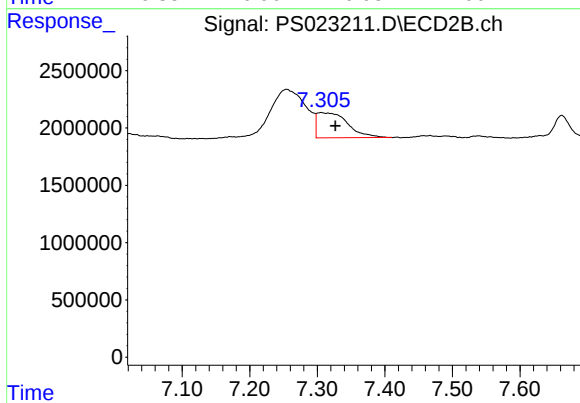

#7 MCPA


R.T.: 7.306 min
Delta R.T.: -0.021 min
Response: 6893130
Conc: 2.60 ug/ml

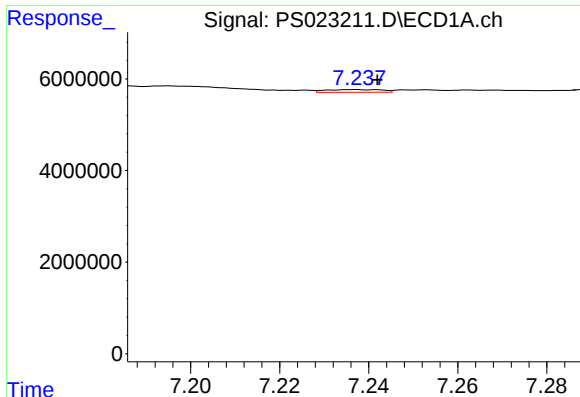

#8 DICHLORPROP


R.T.: 7.237 min
Delta R.T.: -0.005 min
Response: 519643
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

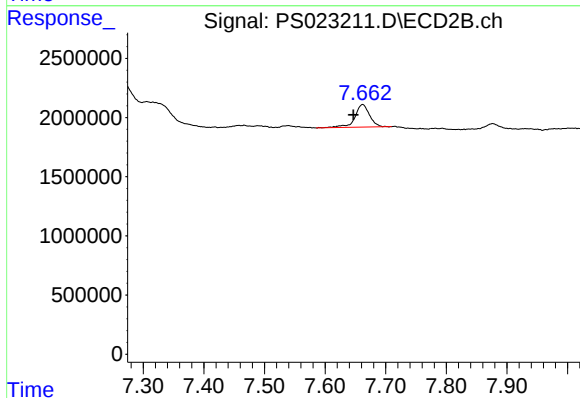


#8 DICHLORPROP

R.T.: 7.662 min
Delta R.T.: 0.015 min
Response: 3174119
Conc: 5.13 ng/ml

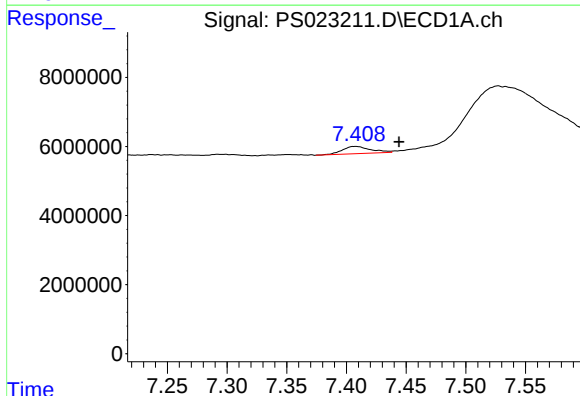


#9 2,4-D

R.T.: 7.407 min
Delta R.T.: -0.037 min
Response: 3448254
Conc: 1.49 ng/ml

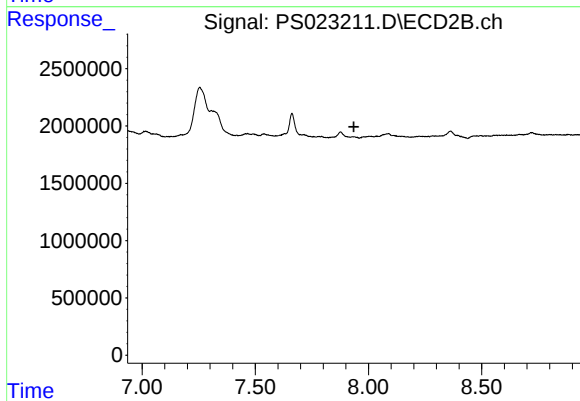

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.935 min
Response: 0
Conc: N.D.

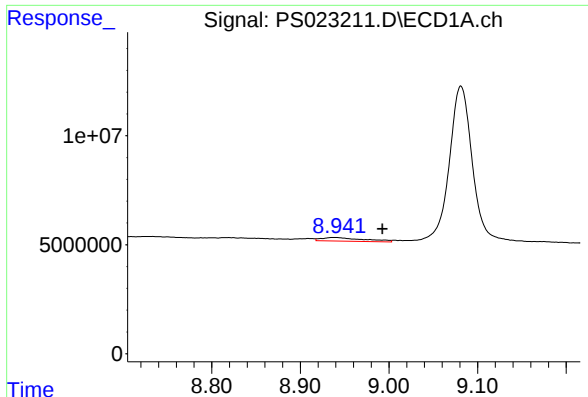

#13 2,4-DB


R.T.: 8.940 min
Delta R.T.: -0.052 min
Response: 5473478
Conc: 2.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

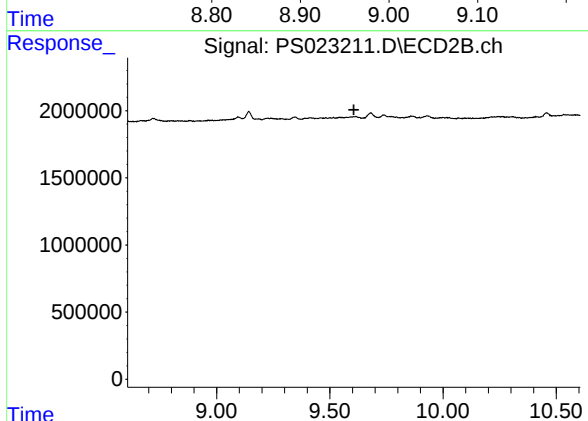


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.606 min
Response: 0
Conc: N.D.

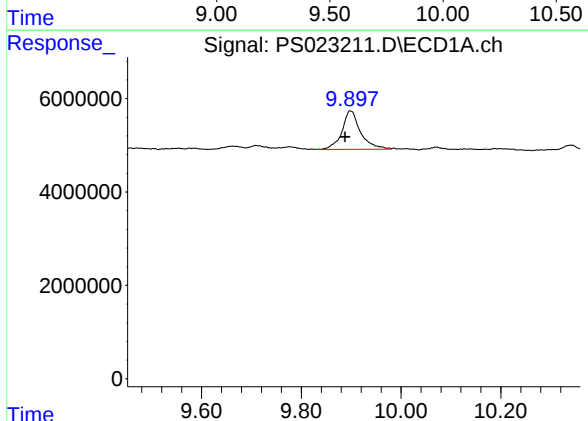

#15 Picloram

R.T.: 9.898 min
Delta R.T.: 0.010 min
Response: 21222591
Conc: 1.24 ng/ml

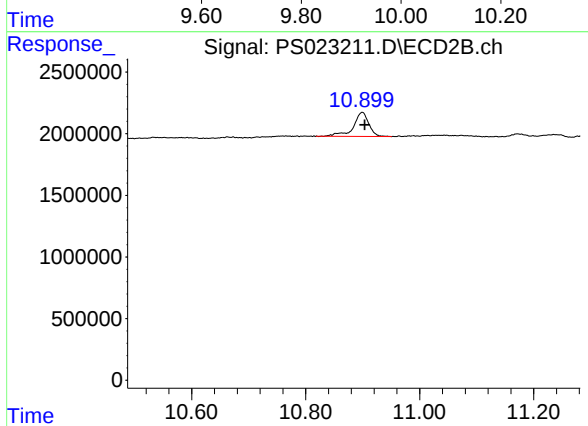

#15 Picloram

R.T.: 10.899 min
Delta R.T.: -0.004 min
Response: 3719870
Conc: N.D.