

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060225\
 Data File : PS030436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2025 08:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 12:52:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060225.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 02 12:26:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.732	7.301	1883.6E6	598.1E6	464.805	470.002
Target Compounds							
1) T	Dalapon	0.000	2.453f	0	7162979	N.D.	2.062
3) T	4-Nitroph...	6.538	0.000	11912864	0	5.118	N.D. #
5) T	DICAMBA	6.903	7.468	88464	2668195	<MDL	<MDL #
6) T	MCP	7.124f	0.000	2918844	0	<MDL	N.D. #
7) T	MCPA	7.228	7.785f	-516103	56947725	N.D.	14.055
8) T	DICHLORPROP	7.575	8.179	517555	4833416	<MDL	2.564 #
9) T	2,4-D	7.769	0.000	4490902	0	1.027	N.D. #
10) T	Pentachlo...	8.045	8.961	17364480	3618560	<MDL	<MDL #
11) T	2,4,5-TP ...	8.614	9.344	4142460	2431809	<MDL	<MDL #
12) T	2,4,5-T	8.896	9.745	998711	1514913	<MDL	<MDL #
13) T	2,4-DB	9.431	0.000	3934604	0	1.123	N.D. #
14) T	DINOSEB	10.570	0.000	3536497	0	<MDL	N.D. #
15) T	Picloram	10.399	11.692	44716189	14599471	1.627	<MDL #
16) T	DCPA	10.873	11.692	8155582	14599471	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060225\
Data File : PS030436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2025 08:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 12:52:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060225.M
Quant Title : 8080.M
QLast Update : Mon Jun 02 12:26:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

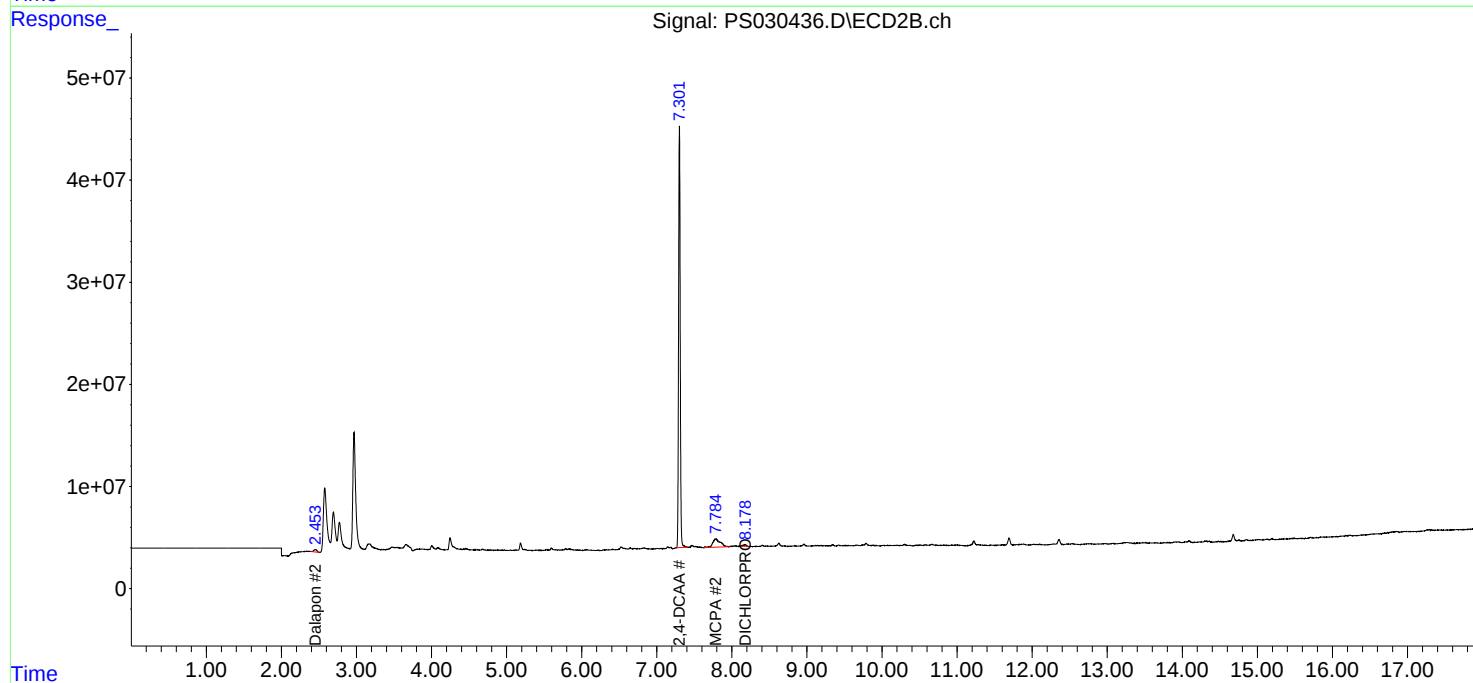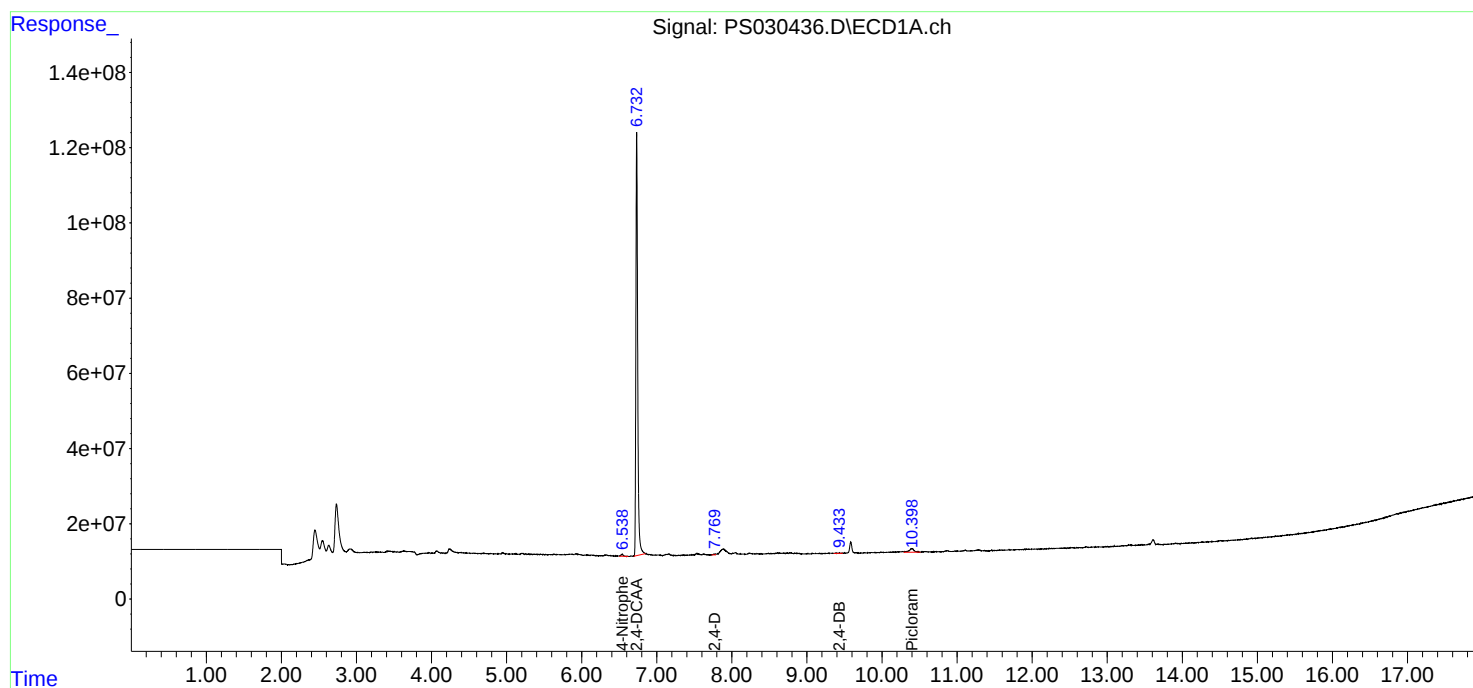


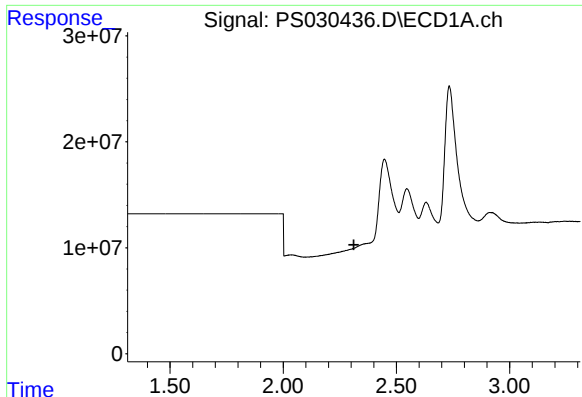

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.312 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

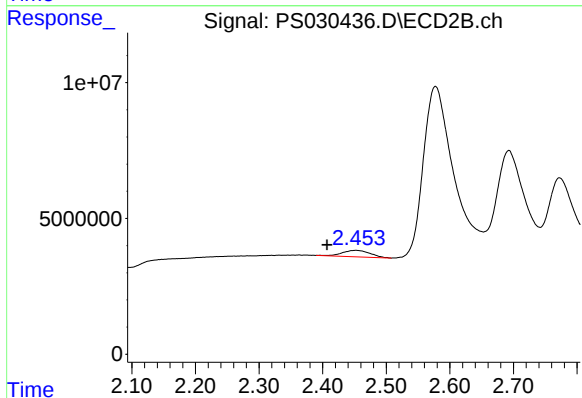


#1 Dalapon

R.T.: 2.453 min
Delta R.T.: 0.046 min
Response: 7162979
Conc: 2.06 ng/ml

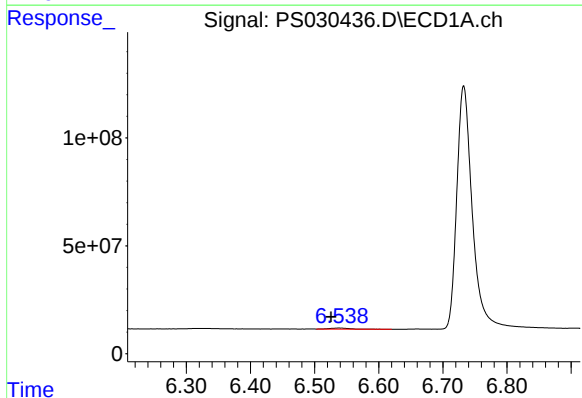


#3 4-Nitrophenol

R.T.: 6.538 min
Delta R.T.: 0.013 min
Response: 11912864
Conc: 5.12 ng/ml

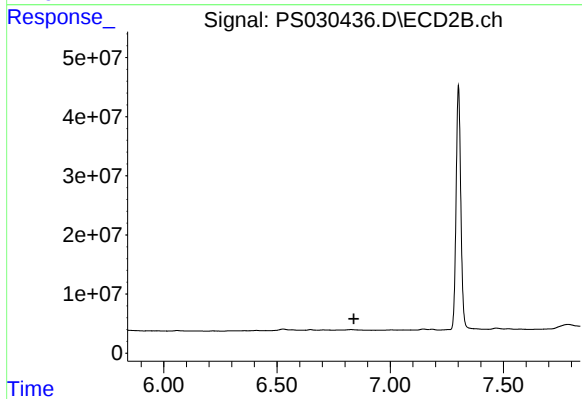

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.840 min
Response: 0
Conc: N.D.

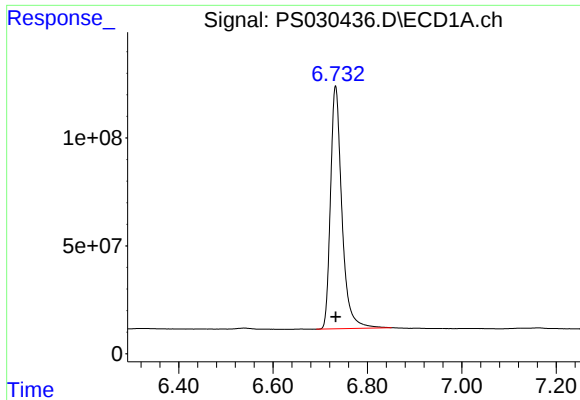

#4 2,4-DCAA


R.T.: 6.732 min
Delta R.T.: 0.000 min
Response: 1883587944
Conc: 464.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

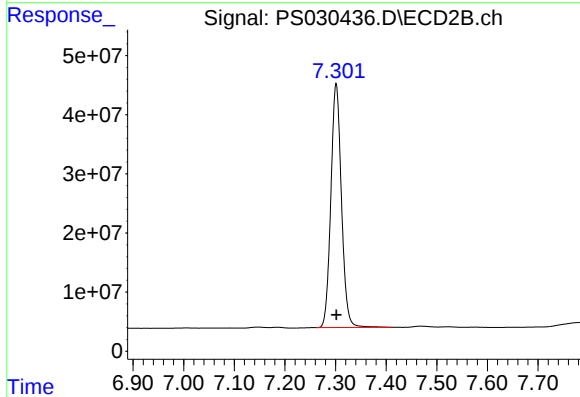


#4 2,4-DCAA

R.T.: 7.301 min
Delta R.T.: 0.000 min
Response: 598061434
Conc: 470.00 ng/ml

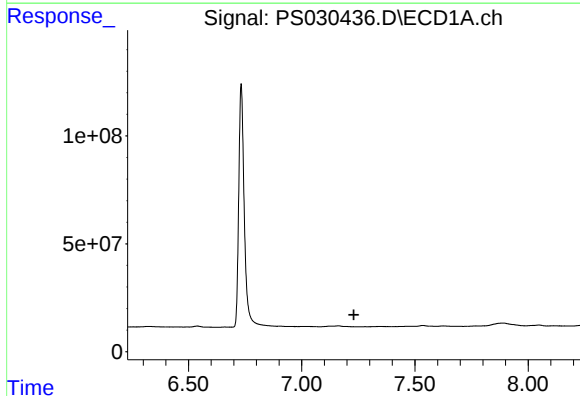


#7 MCPA

R.T.: 7.228 min
Delta R.T.: -0.002 min
Response: -516103
Conc: N.D.

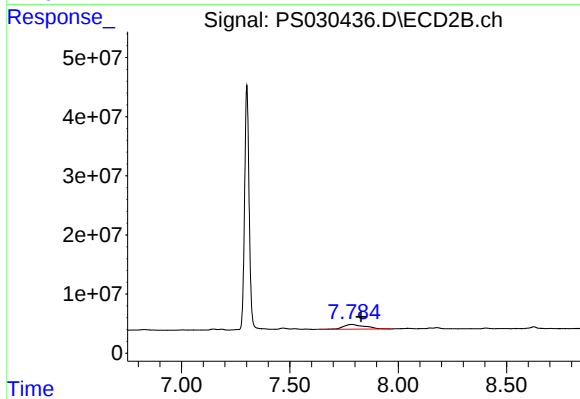

#7 MCPA


R.T.: 7.785 min
Delta R.T.: -0.043 min
Response: 56947725
Conc: 14.05 ug/ml

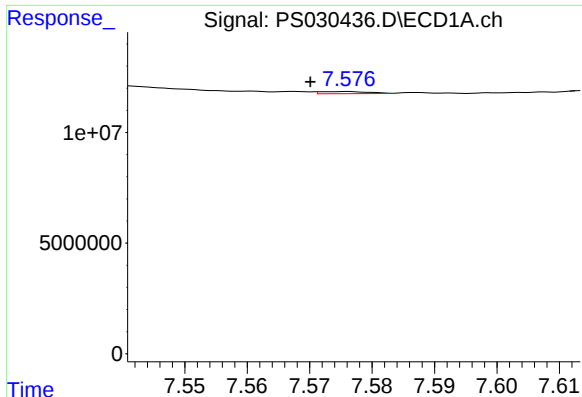

#8 DICHLORPROP


R.T.: 7.575 min
Delta R.T.: 0.005 min
Response: 517555
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

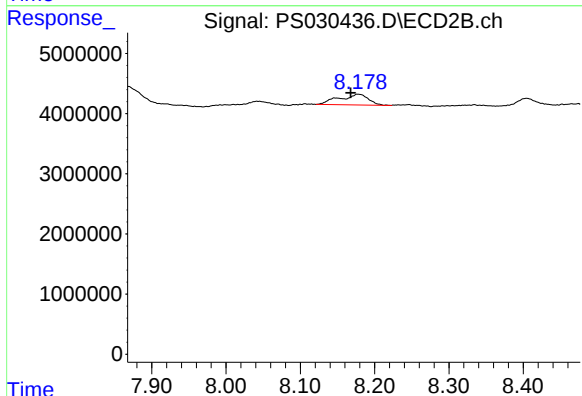


#8 DICHLORPROP

R.T.: 8.179 min
Delta R.T.: 0.011 min
Response: 4833416
Conc: 2.56 ng/ml

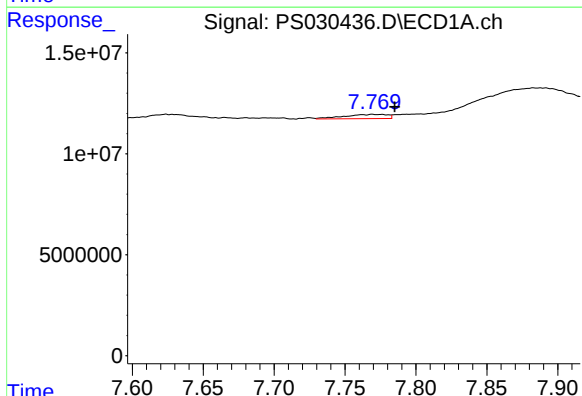


#9 2,4-D

R.T.: 7.769 min
Delta R.T.: -0.016 min
Response: 4490902
Conc: 1.03 ng/ml

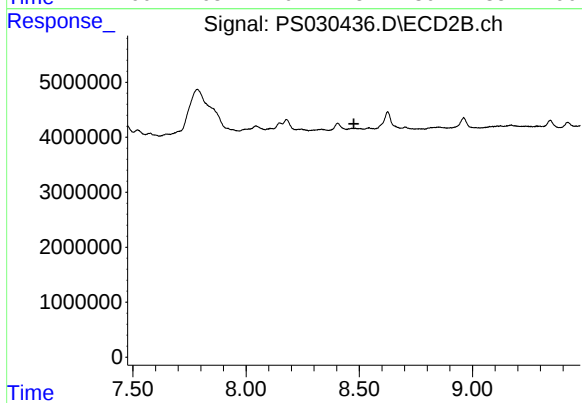

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

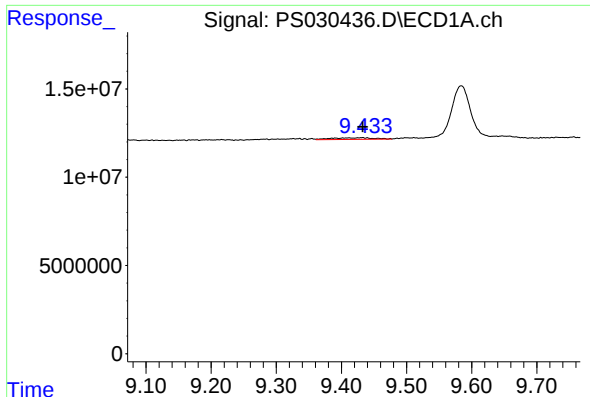

#13 2,4-DB


R.T.: 9.431 min
Delta R.T.: -0.002 min
Response: 3934604
Conc: 1.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

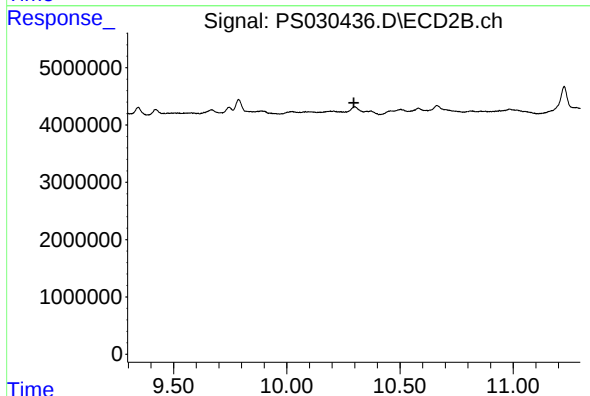


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.296 min
Response: 0
Conc: N.D.

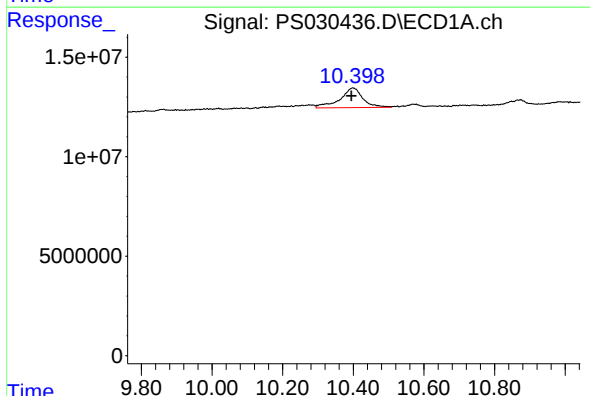

#15 Picloram

R.T.: 10.399 min
Delta R.T.: 0.004 min
Response: 44716189
Conc: 1.63 ng/ml

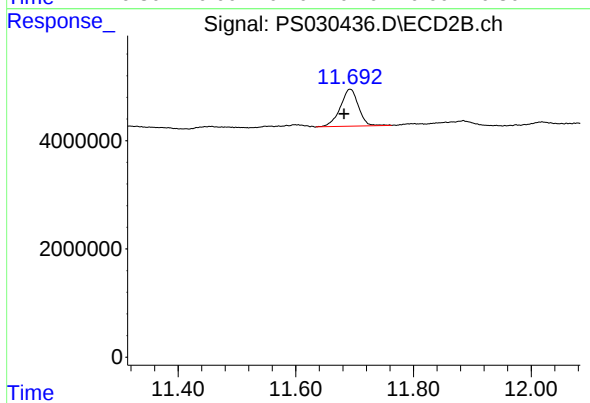

#15 Picloram

R.T.: 11.692 min
Delta R.T.: 0.011 min
Response: 14599471
Conc: N.D.