

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060321\
 Data File : PS015167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 10:40
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 15:42:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.785	1187.9E6	279.9E6	471.336	522.509
Target Compounds							
3) T	4-Nitroph...	7.026	0.000	6516292	0	4.622	N.D. #
7) T	MCPA	7.674f	0.000	11279940	0	1.124	N.D. #
9) T	2,4-D	8.345	0.000	4217677	0	1.655	N.D. #
10) T	Pentachlo...	8.655	0.000	3230848	0	<MDL	N.D. #
12) T	2,4,5-T	9.490	9.083f	5347900	9259453	<MDL	3.198 #
13) T	2,4-DB	10.032	0.000	6135904	0	2.410	N.D. #
15) T	Picloram	11.019	10.849	154.1E6	37360382	9.300	8.996
16) T	DCPA	11.473	10.849f	3830785	37360382	<MDL	8.666 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060321\
Data File : PS015167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 10:40
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 15:42:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

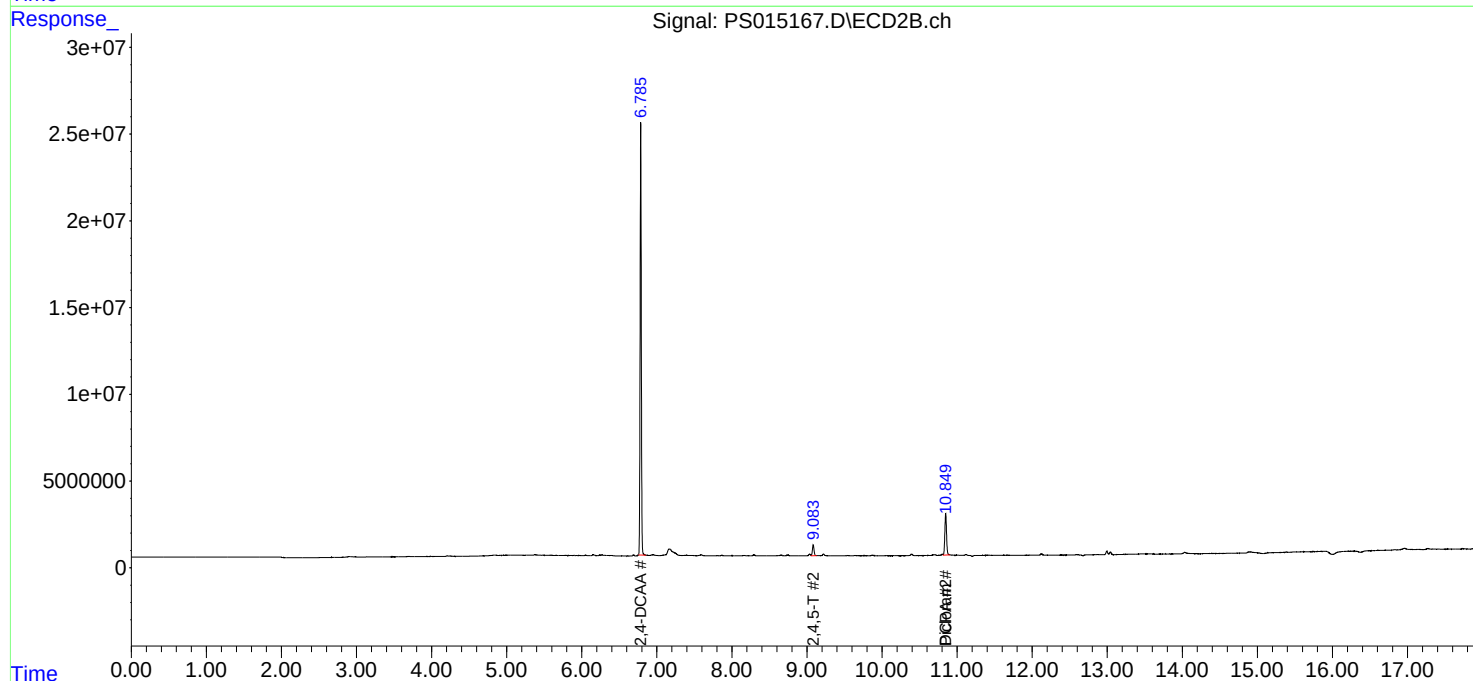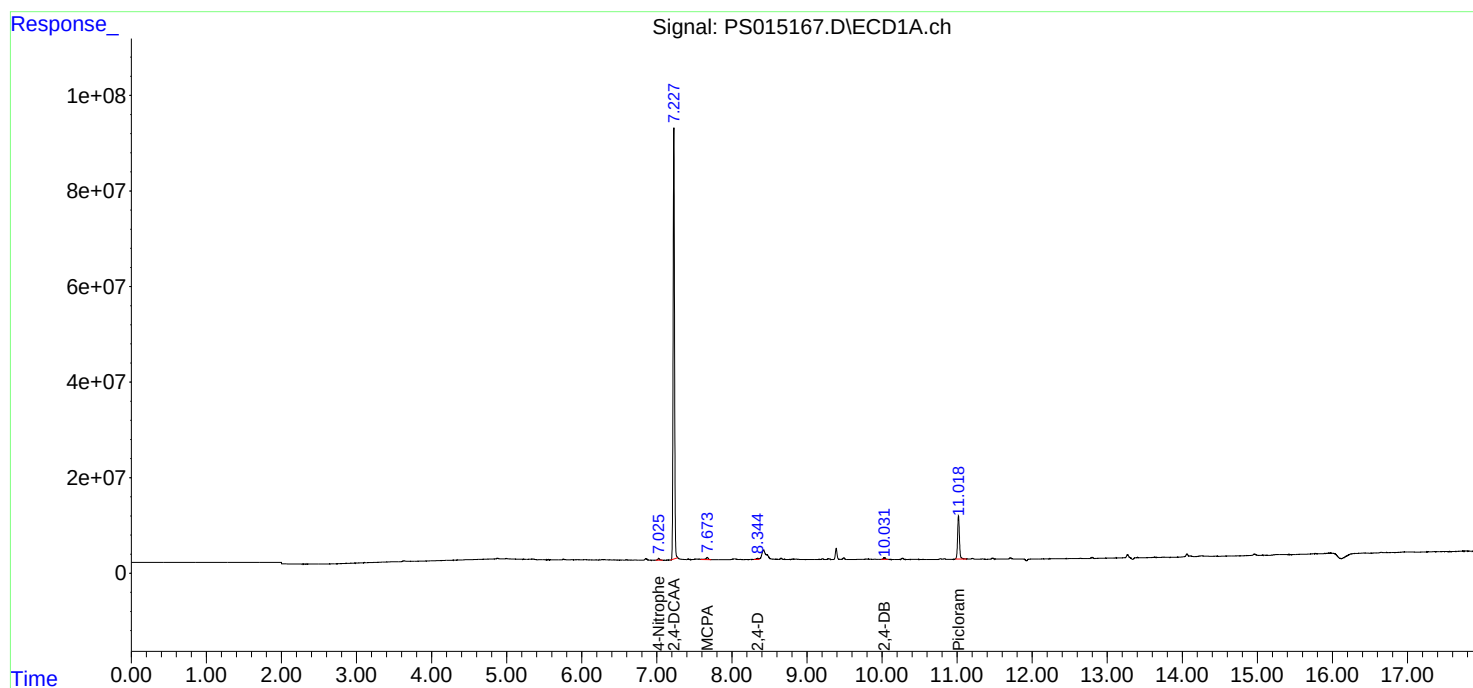


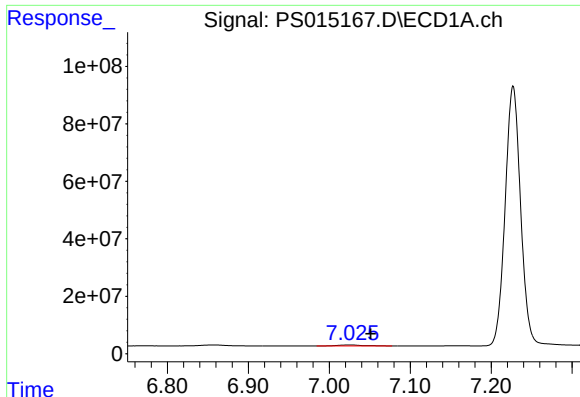

#3 4-Nitrophenol


R.T.: 7.026 min
Delta R.T.: -0.025 min
Response: 6516292
Conc: 4.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

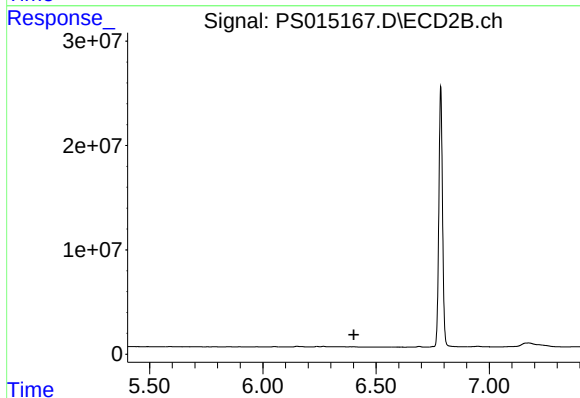


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.402 min
Response: 0
Conc: N.D.

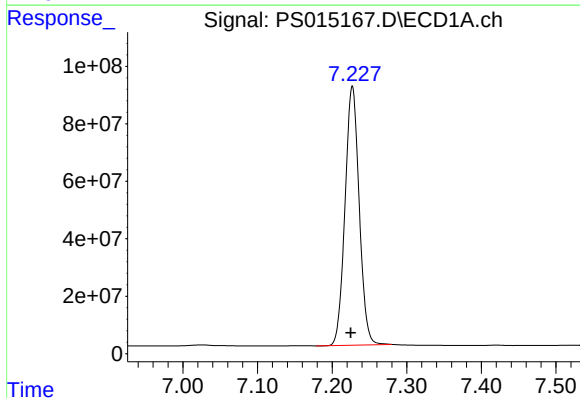


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.002 min
Response: 1187944331
Conc: 471.34 ng/ml

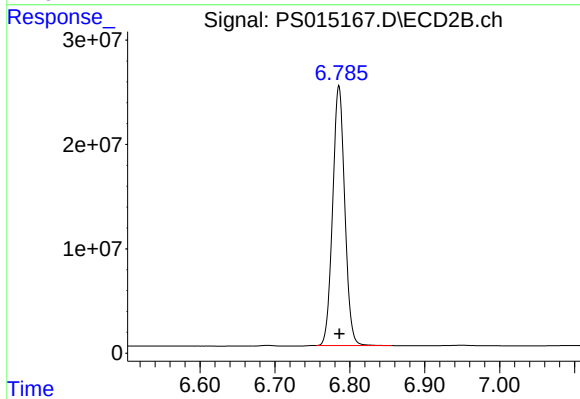

#4 2,4-DCAA


R.T.: 6.785 min
Delta R.T.: 0.000 min
Response: 279945225
Conc: 522.51 ng/ml

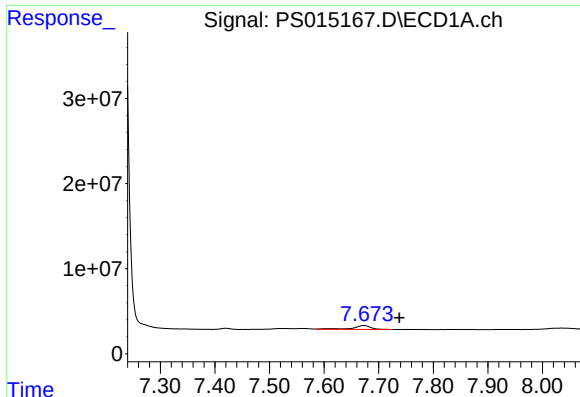

#7 MCPA


R.T.: 7.674 min
Delta R.T.: -0.065 min
Response: 11279940
Conc: 1.12 ug/ml

Instrument :
ECD_S
ClientSampleId :

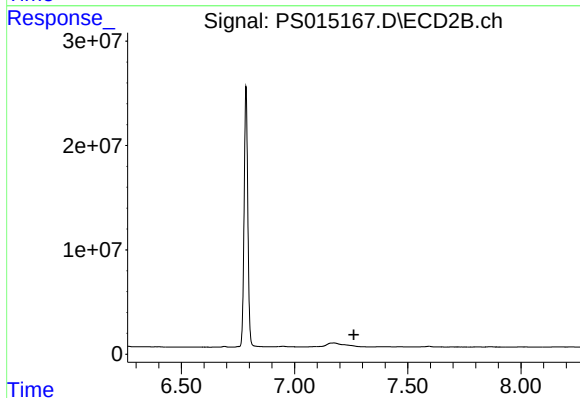


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

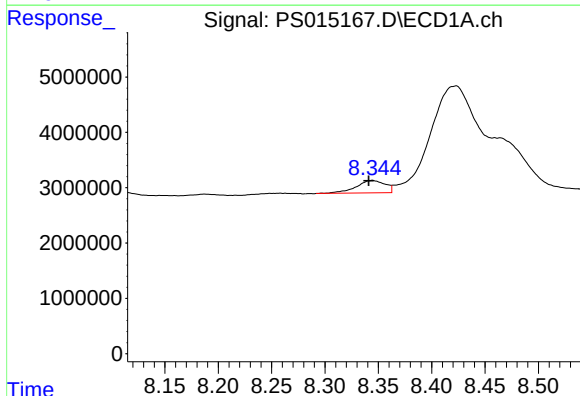


#9 2,4-D

R.T.: 8.345 min
Delta R.T.: 0.004 min
Response: 4217677
Conc: 1.66 ng/ml

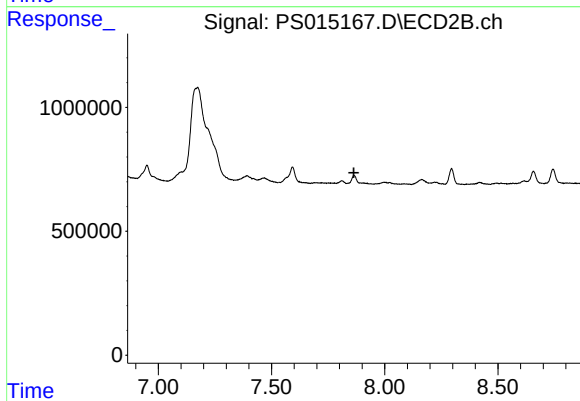

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

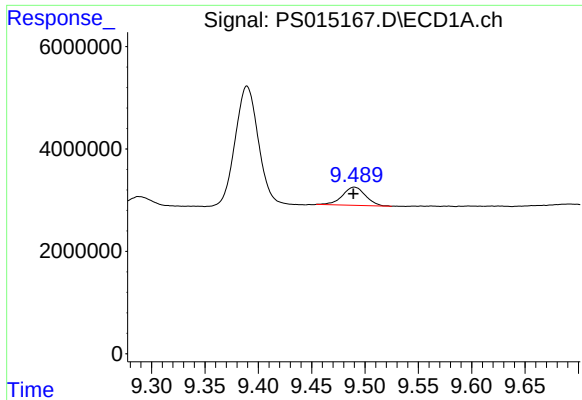

#12 2,4,5-T


R.T.: 9.490 min
Delta R.T.: 0.000 min
Response: 5347900
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

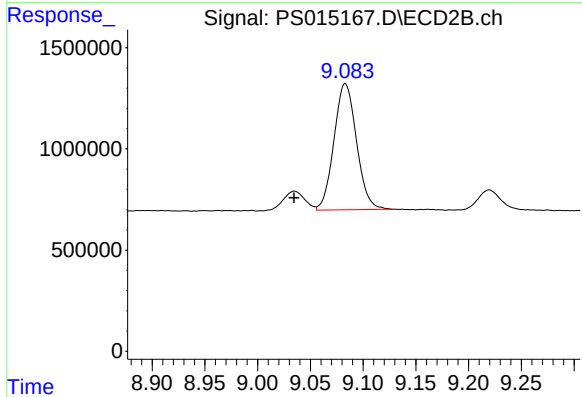


#12 2,4,5-T

R.T.: 9.083 min
Delta R.T.: 0.048 min
Response: 9259453
Conc: 3.20 ng/ml

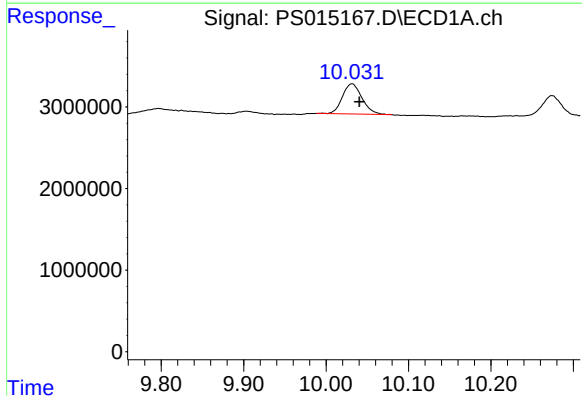


#13 2,4-DB

R.T.: 10.032 min
Delta R.T.: -0.009 min
Response: 6135904
Conc: 2.41 ng/ml

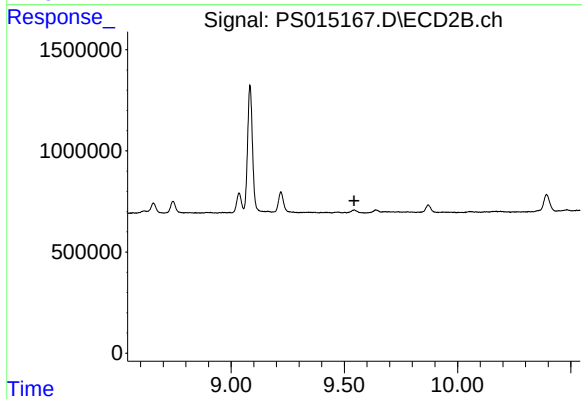

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.542 min
Response: 0
Conc: N.D.

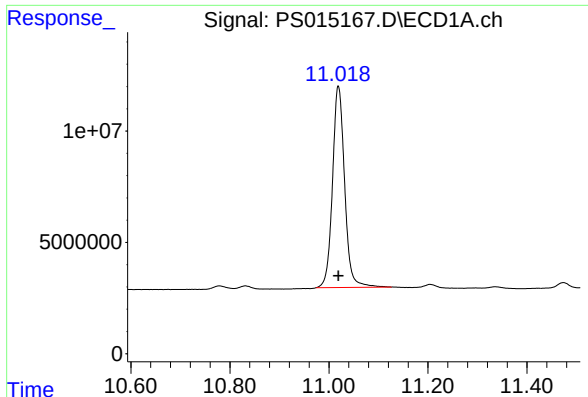

#15 Picloram


R.T.: 11.019 min
Delta R.T.: 0.000 min
Response: 154074394
Conc: 9.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

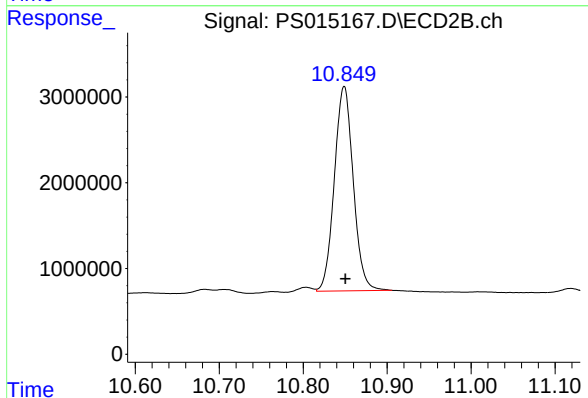


#15 Picloram

R.T.: 10.849 min
Delta R.T.: -0.001 min
Response: 37360382
Conc: 9.00 ng/ml

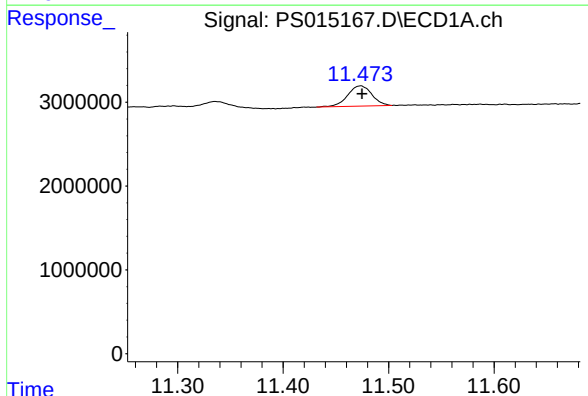

#16 DCPA

R.T.: 11.473 min
Delta R.T.: -0.001 min
Response: 3830785
Conc: N.D.

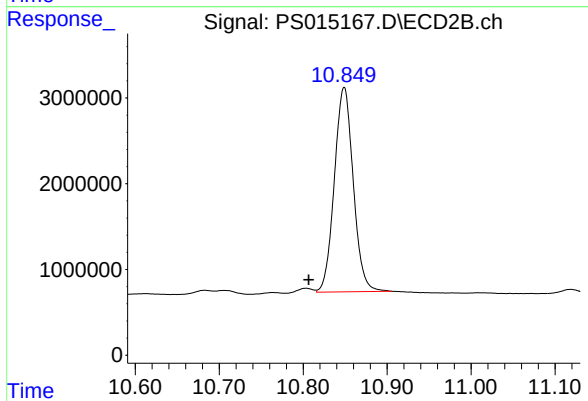

#16 DCPA

R.T.: 10.849 min
Delta R.T.: 0.043 min
Response: 37360382
Conc: 8.67 ng/ml