

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060321\
 Data File : PS015176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 14:30
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 15:44:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.784	1155.7E6	285.3E6	458.553	532.515
Target Compounds							
3) T	4-Nitroph...	7.027	0.000	5008257	0	3.553	N.D. #
5) T	DICAMBA	7.421	0.000	2309677	0	<MDL	N.D. #
7) T	MCPA	7.672f	0.000	11991021	0	1.195	N.D. #
9) T	2,4-D	8.410f	0.000	262.1E6	0	102.843	N.D. #
10) T	Pentachlo...	8.657	0.000	8542144	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.209	0.000	3896670	0	<MDL	N.D. #
12) T	2,4,5-T	9.492	0.000	5548764	0	<MDL	N.D. #
14) T	DINOSEB	11.207	0.000	3702195	0	<MDL	N.D. #
15) T	Picloram	11.022	0.000	11826615	0	<MDL	N.D. #
16) T	DCPA	11.475	0.000	5046911	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060321\
Data File : PS015176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 14:30
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 15:44:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

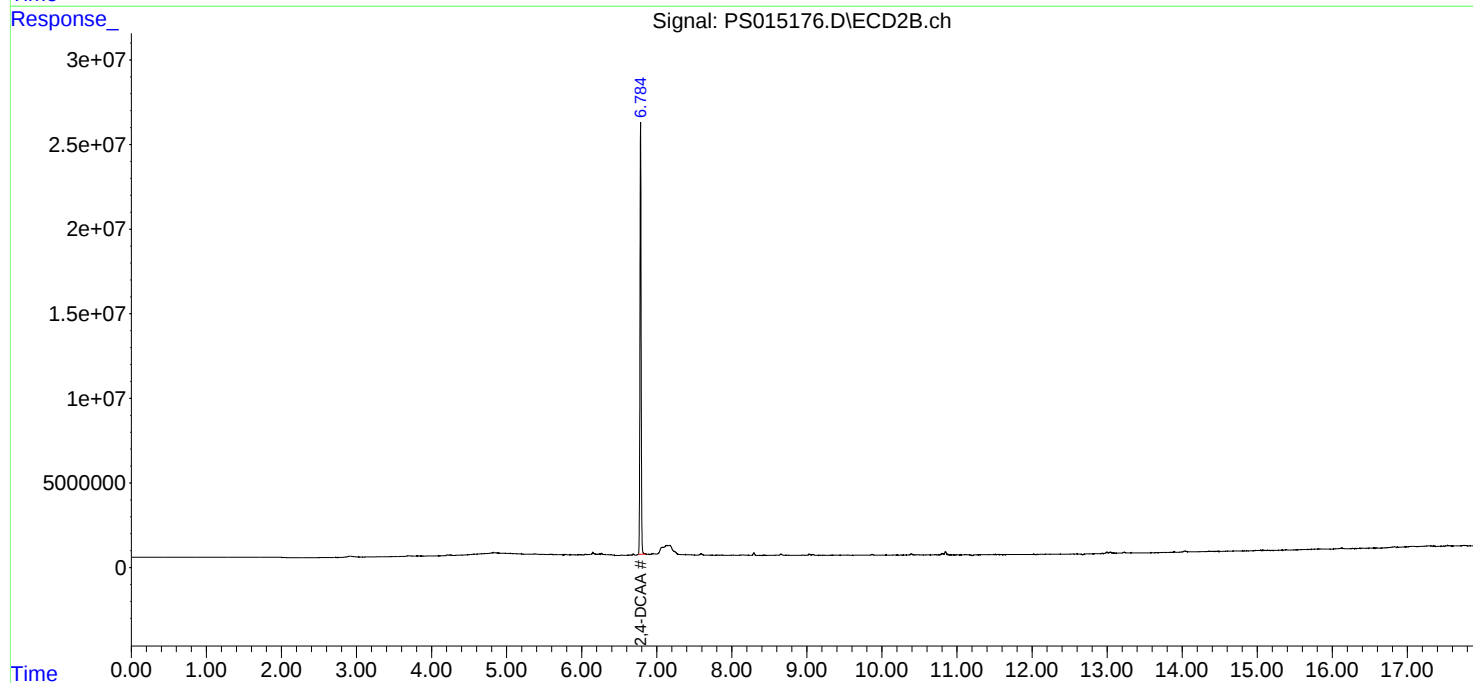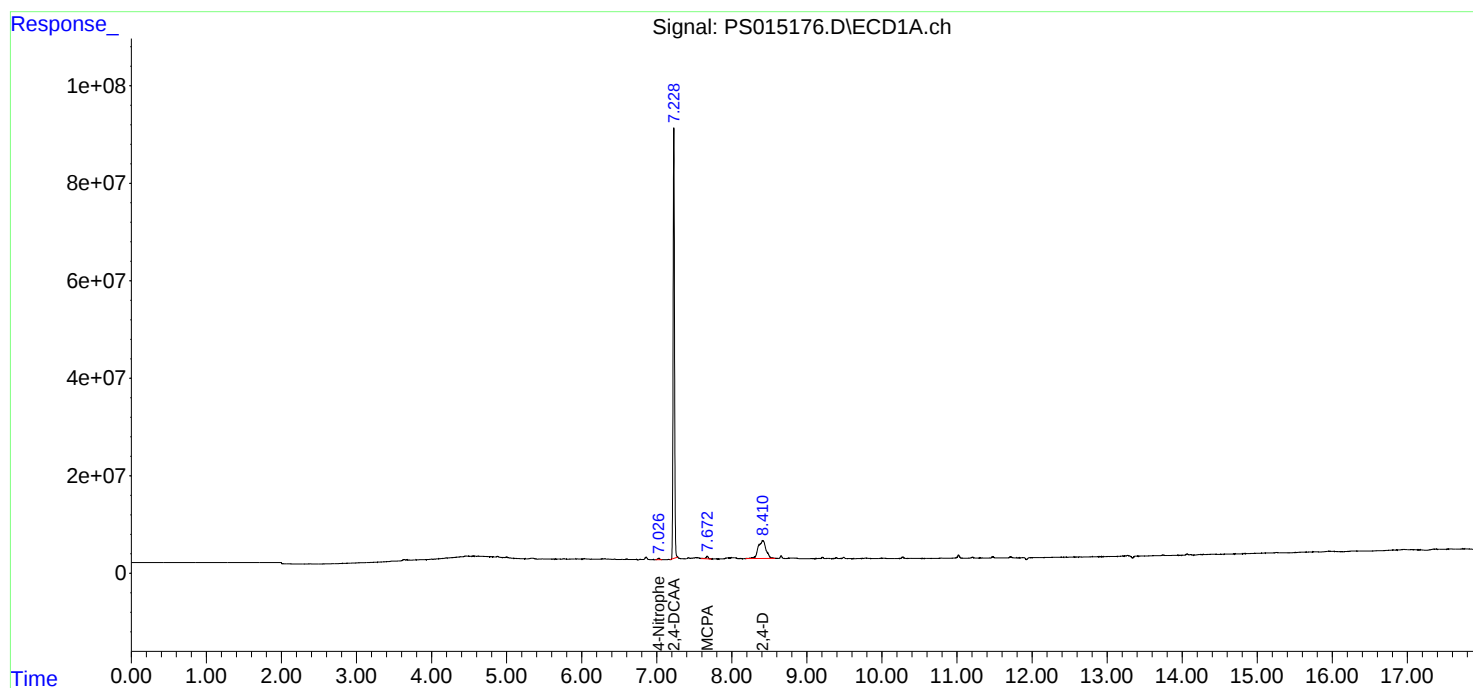


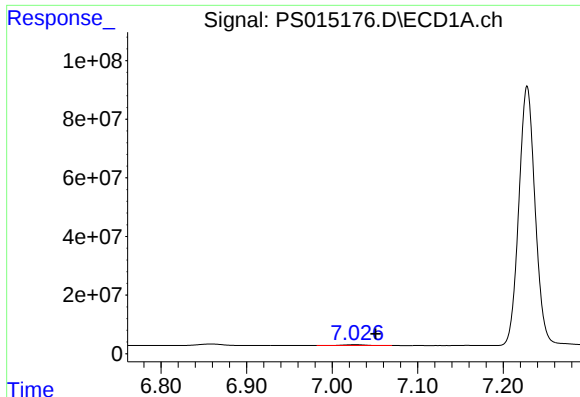

#3 4-Nitrophenol


R.T.: 7.027 min
Delta R.T.: -0.025 min
Response: 5008257
Conc: 3.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

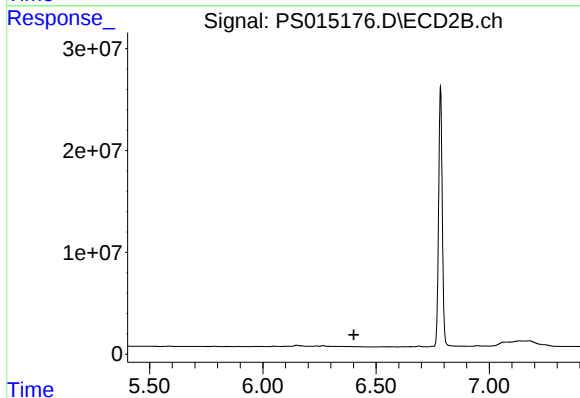


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.402 min
Response: 0
Conc: N.D.

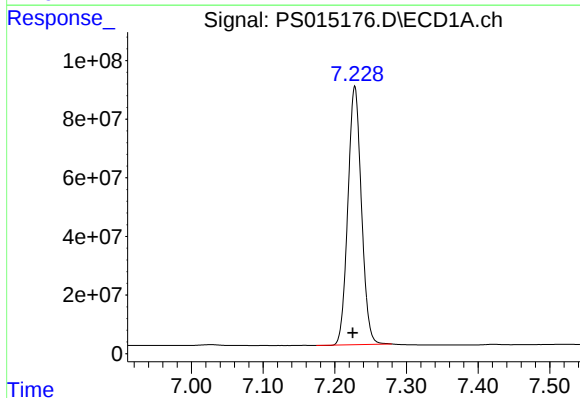


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.003 min
Response: 1155725838
Conc: 458.55 ng/ml

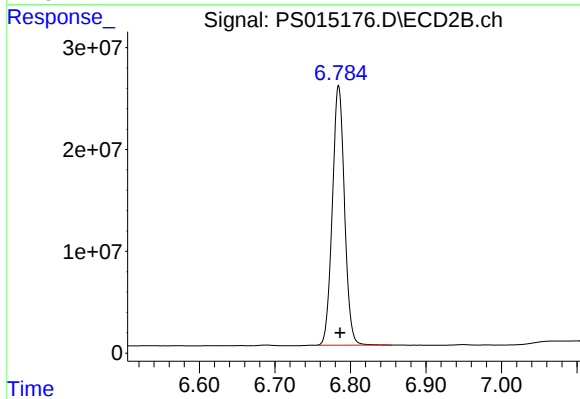

#4 2,4-DCAA


R.T.: 6.784 min
Delta R.T.: -0.002 min
Response: 285306014
Conc: 532.51 ng/ml

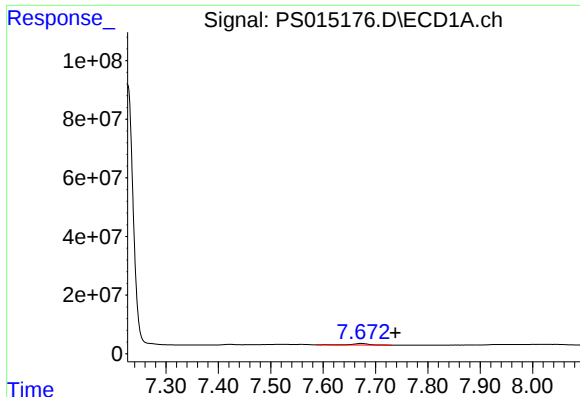

#7 MCPA


R.T.: 7.672 min
Delta R.T.: -0.066 min
Response: 11991021
Conc: 1.19 ug/ml

Instrument :
ECD_S
ClientSampleId :

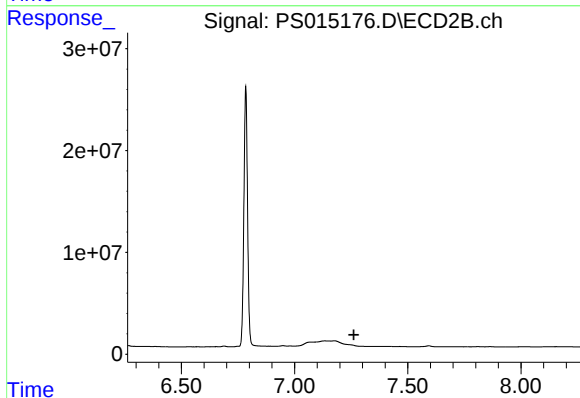


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

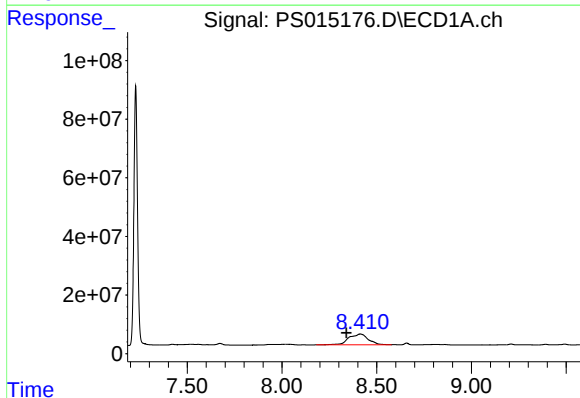

#9 2,4-D

R.T.: 8.410 min
Delta R.T.: 0.069 min
Response: 262054826
Conc: 102.84 ng/ml

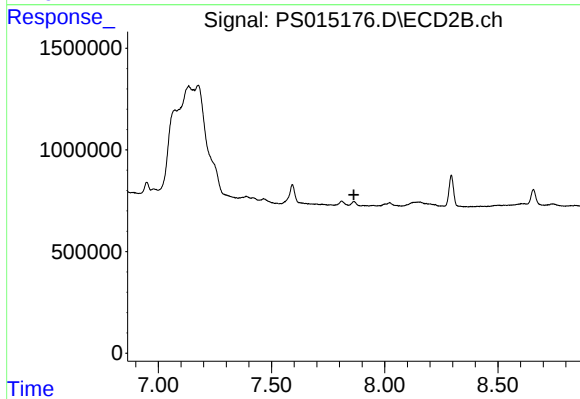

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.