

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060321\
 Data File : PS015188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 20:36
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 04:47:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.785	1149.3E6	284.1E6	456.000	530.230
Target Compounds							
3) T	4-Nitroph...	7.025	0.000	5293910	0	3.755	N.D. #
5) T	DICAMBA	7.420	0.000	2677625	0	<MDL	N.D. #
7) T	MCPA	7.671f	0.000	15171978	0	1.512	N.D. #
9) T	2,4-D	8.344	0.000	6791901	0	2.665	N.D. #
10) T	Pentachlo...	8.655	0.000	7236349	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.206	0.000	4885367	0	<MDL	N.D. #
12) T	2,4,5-T	9.489	0.000	6131787	0	<MDL	N.D. #
15) T	Picloram	11.017	10.848	18219412	3687379	1.100	<MDL #
16) T	DCPA	0.000	10.848f	0	3687379	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060321\
Data File : PS015188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 20:36
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 04:47:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

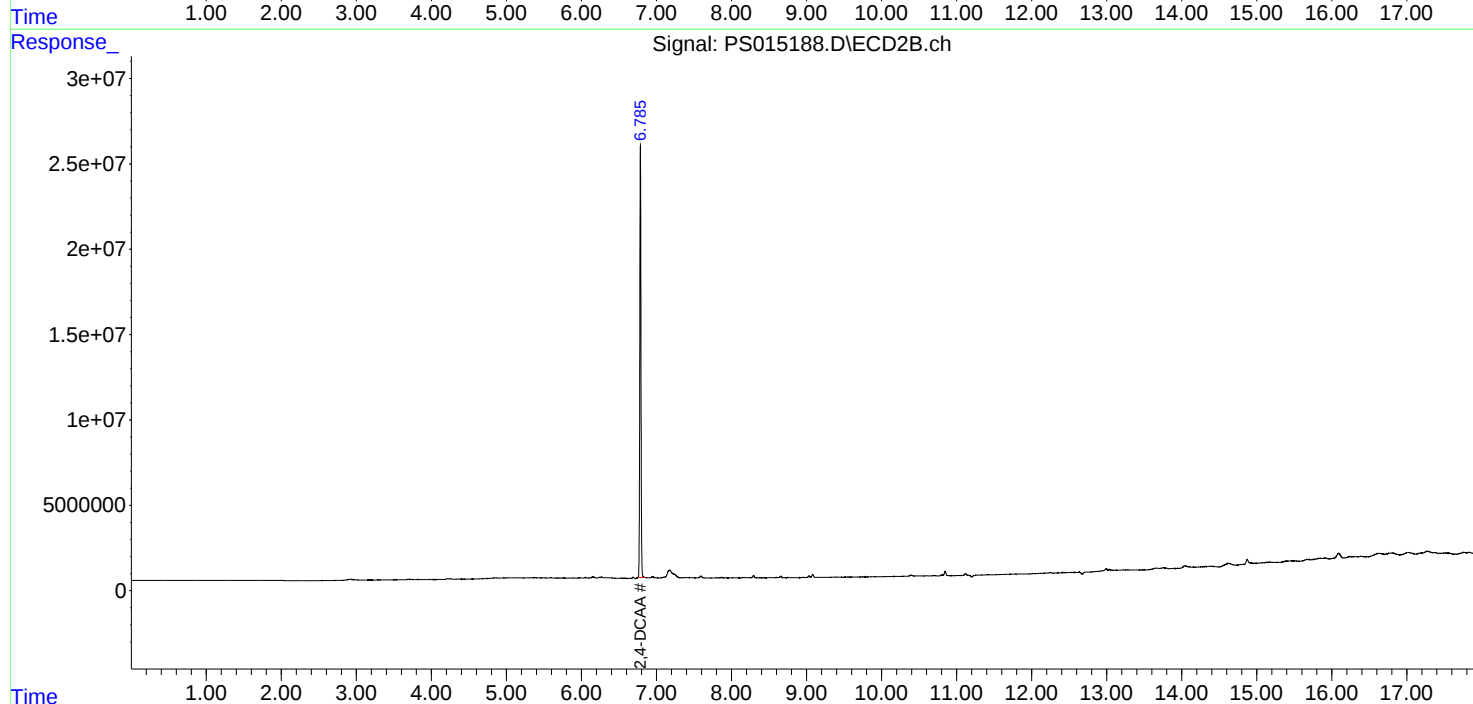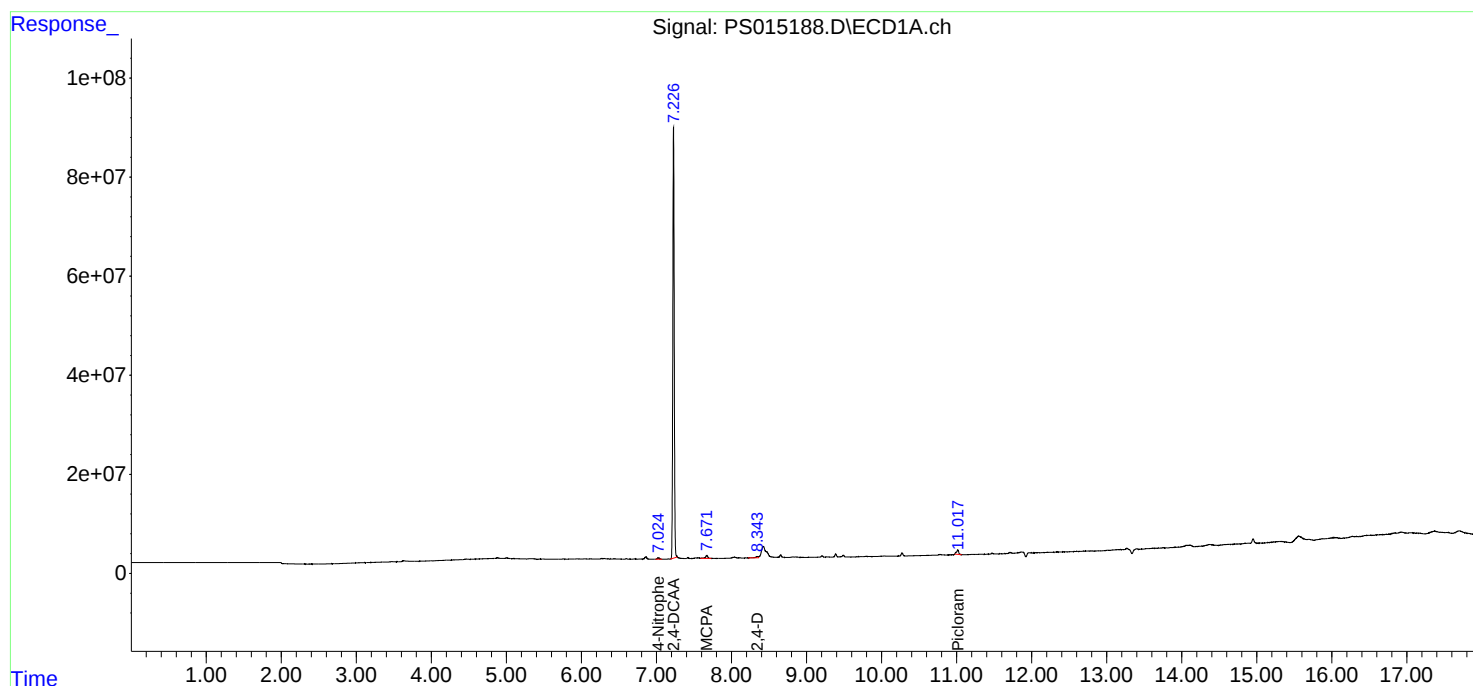


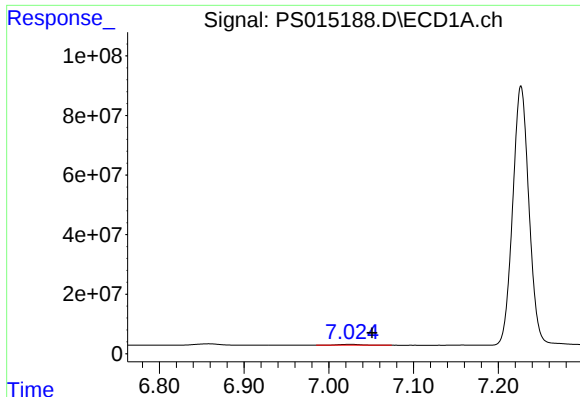

#3 4-Nitrophenol


R.T.: 7.025 min
Delta R.T.: -0.026 min
Response: 5293910
Conc: 3.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

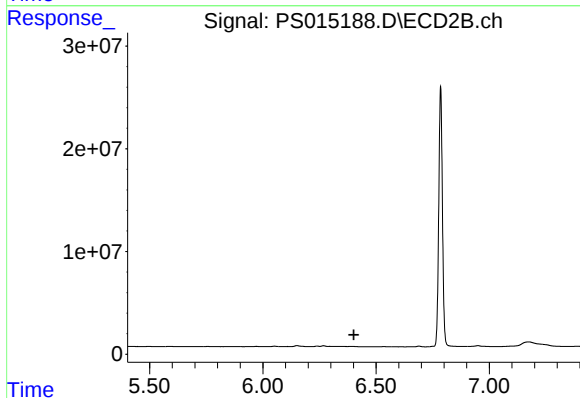


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

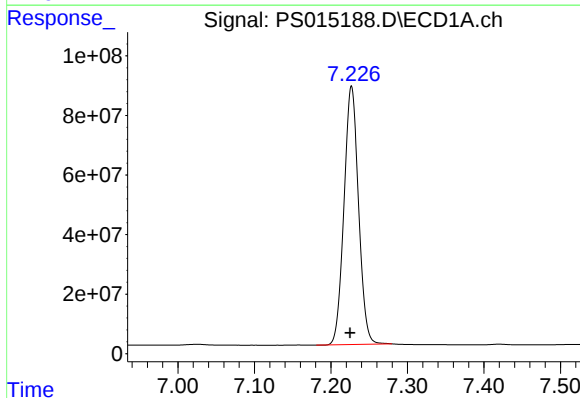


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.002 min
Response: 1149291525
Conc: 456.00 ng/ml

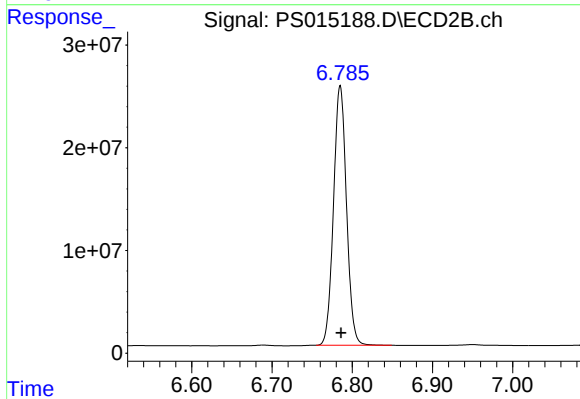

#4 2,4-DCAA


R.T.: 6.785 min
Delta R.T.: -0.001 min
Response: 284081768
Conc: 530.23 ng/ml

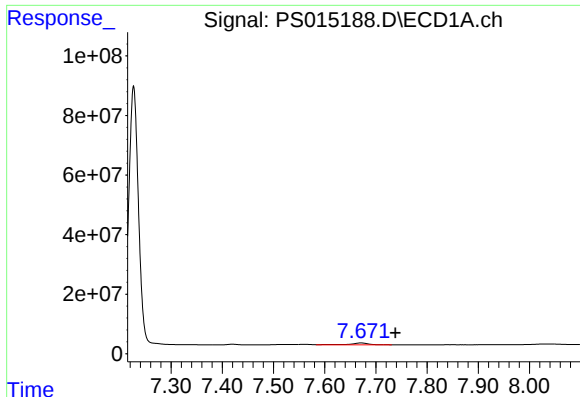

#7 MCPA


R.T.: 7.671 min
Delta R.T.: -0.067 min
Response: 15171978
Conc: 1.51 ug/ml

Instrument :
ECD_S
ClientSampleId :

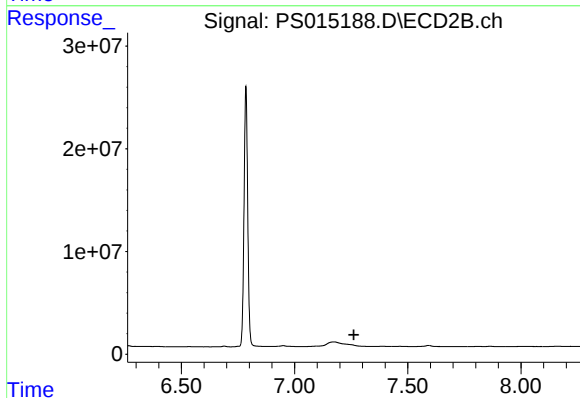


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

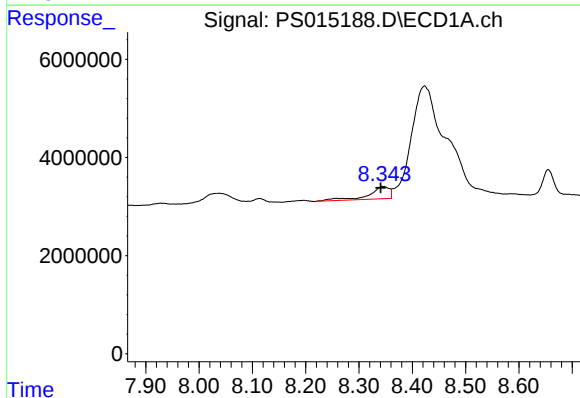


#9 2,4-D

R.T.: 8.344 min
Delta R.T.: 0.003 min
Response: 6791901
Conc: 2.67 ng/ml

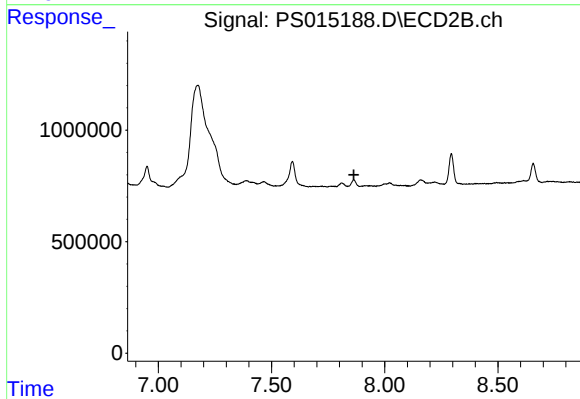

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

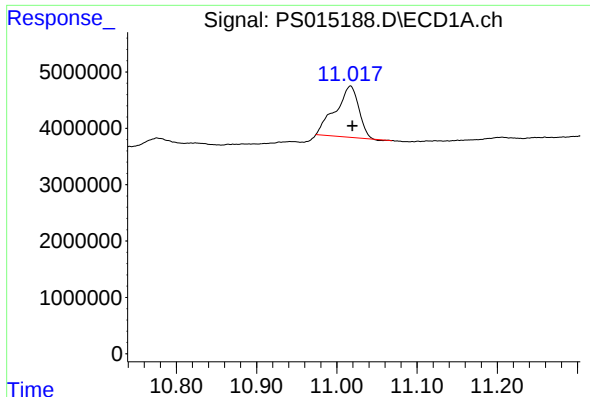

#15 Picloram

R.T.: 11.017 min
Delta R.T.: -0.002 min
Response: 18219412
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

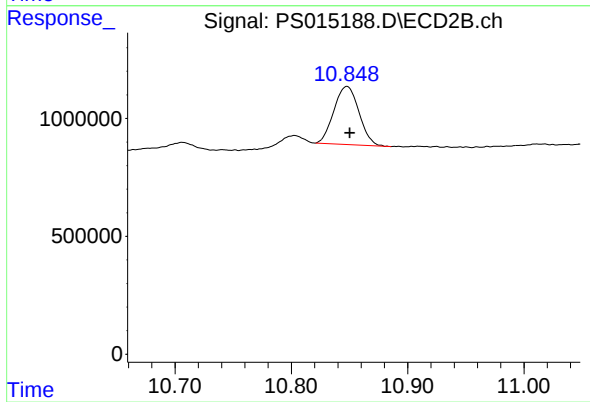

#15 Picloram

R.T.: 10.848 min
Delta R.T.: -0.002 min
Response: 3687379
Conc: N.D.