

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060322\
 Data File : PS019592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 10:25
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 16:17:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.201	6.784	1024.6E6	420.1E6	427.077	542.131 #
Target Compounds							
2) T	3,5-DICHL...	6.467f	0.000	1892406	0	<MDL	N.D. #
3) T	4-Nitroph...	6.992f	0.000	1026204	0	1.046	N.D. #
5) T	DICAMBA	0.000	7.010f	0	3143285	N.D.	<MDL
6) T	MCP	0.000	7.010	0	3143285	N.D.	1.161
7) T	MCPA	7.670	7.189f	261675	512442	<MDL	<MDL #
10) T	Pentachlo...	8.618	0.000	19960	0	<MDL	N.D. #
13) T	2,4-DB	10.073f	9.480f	7709112	393260	1.905	<MDL #
15) T	Picloram	10.968	10.779f	300.8E6	1193316	10.136	<MDL #
16) T	DCPA	11.429	10.779	2841317	1193316	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060322\
Data File : PS019592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 10:25
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 16:17:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

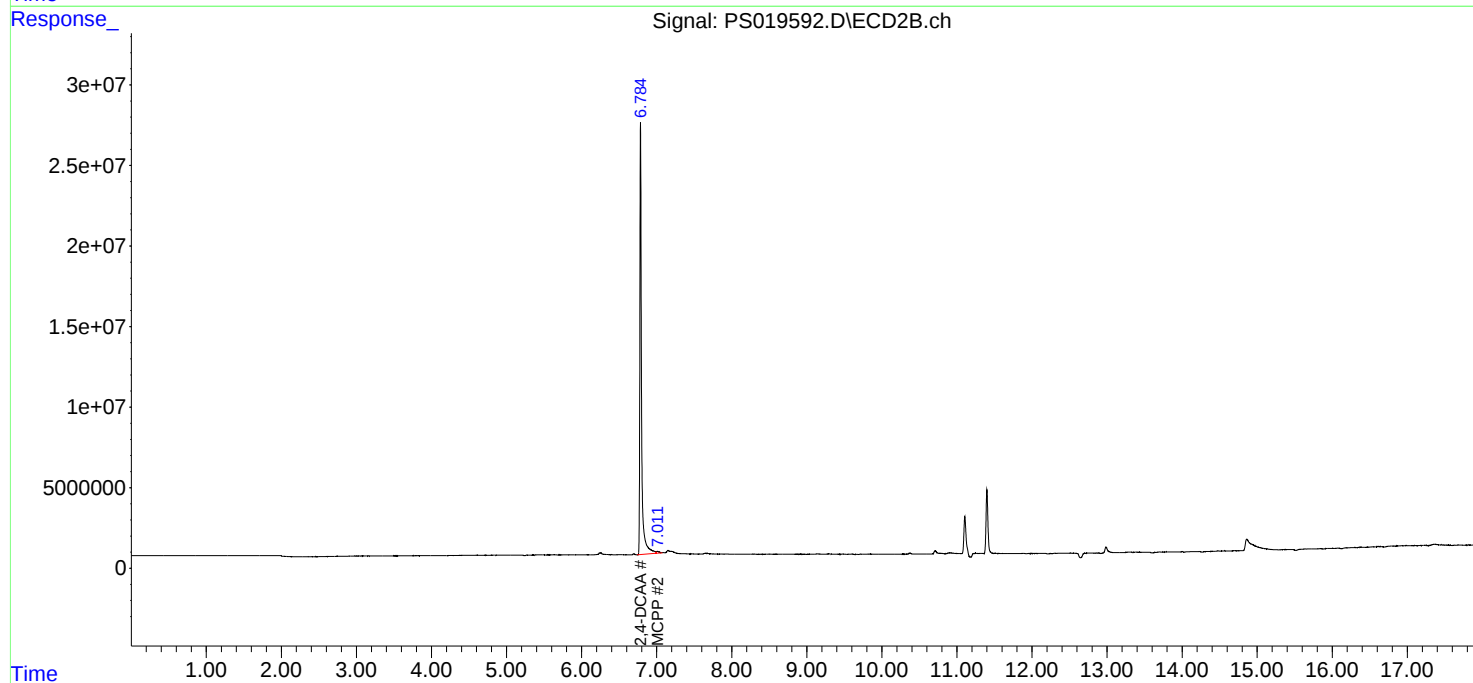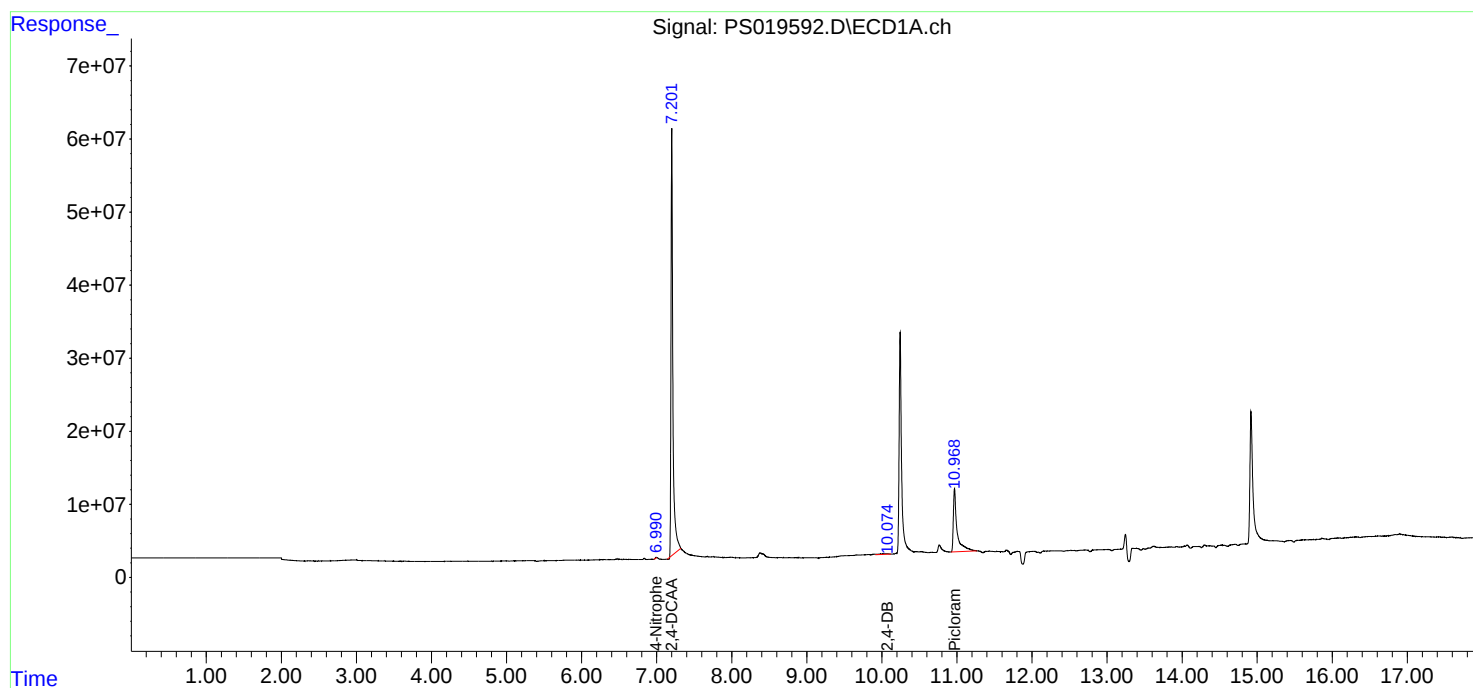


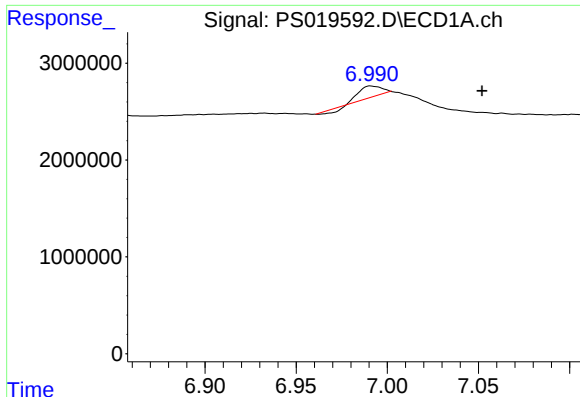

#3 4-Nitrophenol


R.T.: 6.992 min
Delta R.T.: -0.060 min
Response: 1026204
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

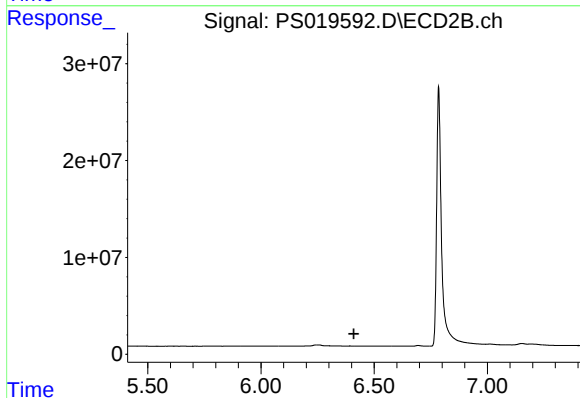


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

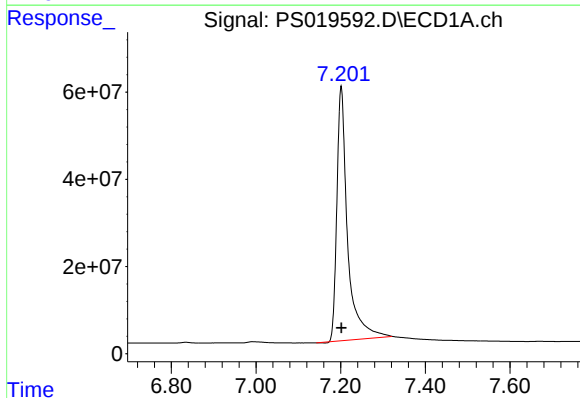


#4 2,4-DCAA

R.T.: 7.201 min
Delta R.T.: 0.000 min
Response: 1024628850
Conc: 427.08 ng/ml

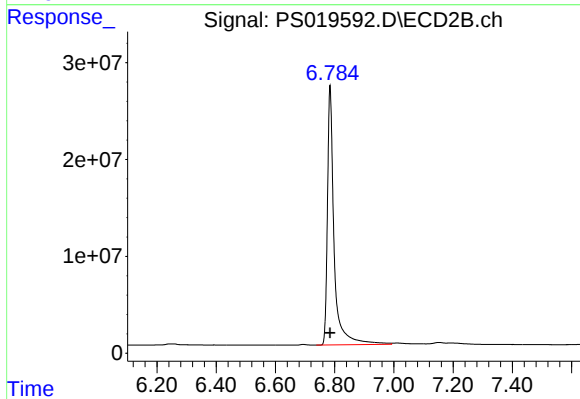

#4 2,4-DCAA


R.T.: 6.784 min
Delta R.T.: 0.000 min
Response: 420081234
Conc: 542.13 ng/ml

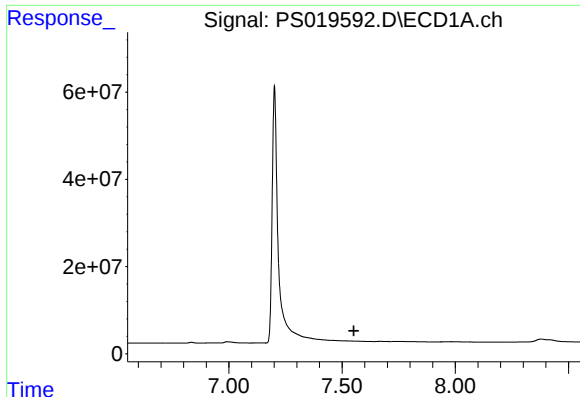

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

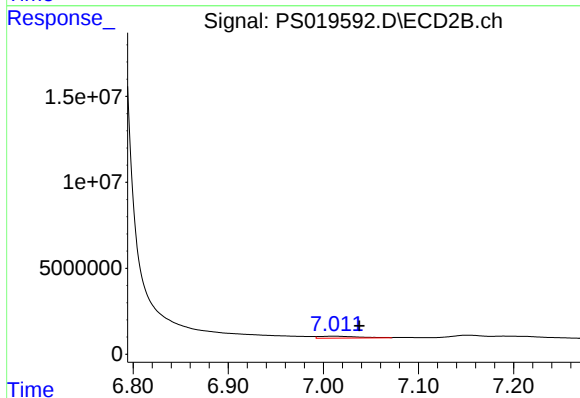


#6 MCPP

R.T.: 7.010 min
Delta R.T.: -0.028 min
Response: 3143285
Conc: 1.16 ug/ml

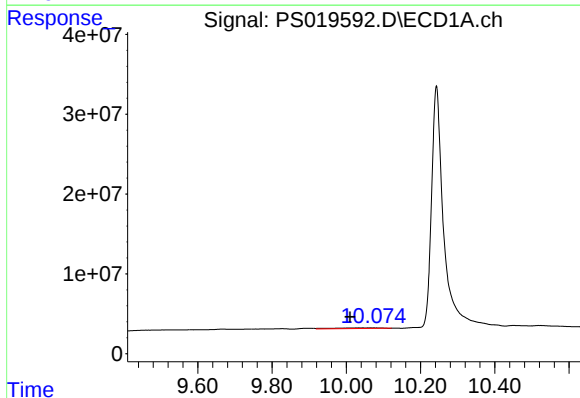


#13 2,4-DB

R.T.: 10.073 min
Delta R.T.: 0.062 min
Response: 7709112
Conc: 1.91 ng/ml

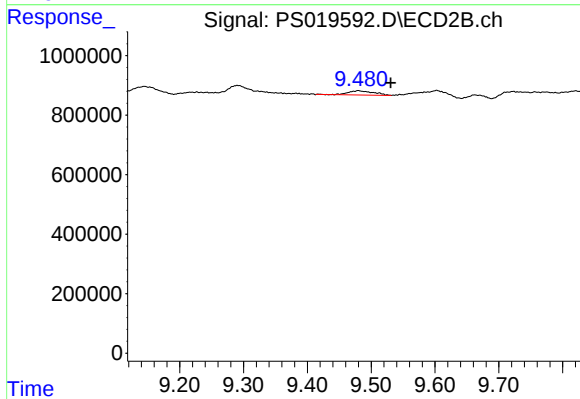

#13 2,4-DB


R.T.: 9.480 min
Delta R.T.: -0.051 min
Response: 393260
Conc: N.D.

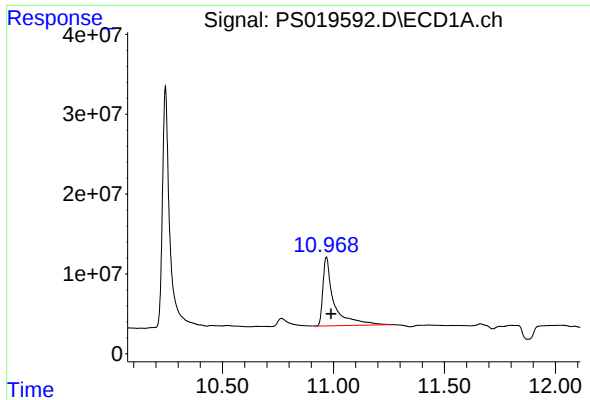

#15 Picloram

R.T.: 10.968 min
Delta R.T.: -0.021 min
Response: 300809511
Conc: 10.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

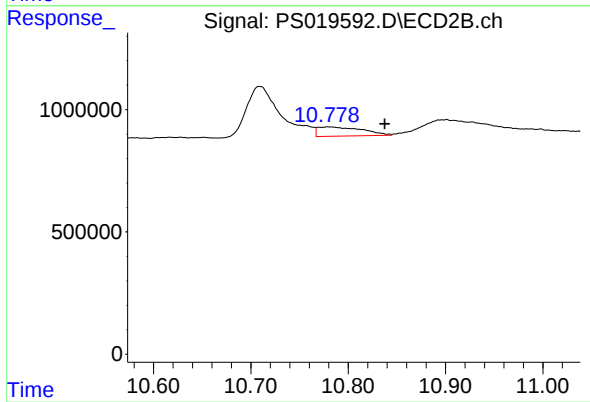

#15 Picloram

R.T.: 10.779 min
Delta R.T.: -0.058 min
Response: 1193316
Conc: N.D.