

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060322\
 Data File : PS019594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 13:44
 Operator : AJ\MA
 Sample : PB145272BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 16:18:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.202	6.781	1189.0E6	450.2E6	495.593	581.006
Target Compounds							
1) T	Dalapon	2.970f	2.519	256.9E6	88005408	50.676	87.704 #
2) T	3,5-DICHL...	6.440	5.986	50534	64464870	<MDL	53.780 #
3) T	4-Nitroph...	7.037	6.401	8477541	2911186	8.639	6.801
5) T	DICAMBA	7.382	6.937	245037	7475251	<MDL	2.187 #
6) T	MCPD	7.559	7.049	23423813	2416911	3.121	<MDL #
7) T	MCPA	7.699	7.240	17686472	18899954	1.637	4.919 #
8) T	DICHLORPROP	8.066	7.591	-1218478	47904635	N.D.	54.229
9) T	2,4-D	8.280	7.840	1630530	22748861	<MDL	21.328 #
10) T	Pentachlo...	8.639	8.284	10047109	2710215	<MDL	<MDL #
11) T	2,4,5-TP ...	9.174	8.684	2657134	21789974	<MDL	4.334 #
12) T	2,4,5-T	9.474	9.029	12777036	16834126	<MDL	3.579 #
13) T	2,4-DB	9.973	9.540	61513295	70125451	15.203	113.478 #
14) T	DINOSEB	11.132	9.857	1241.7E6	115.5E6	80.278	32.518 #
15) T	Picloram	10.967	10.853	105.7E6	35287783	3.561	5.486 #
16) T	DCPA	11.457	10.788	-42029808	17009453	N.D.	2.756



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060322\
Data File : PS019594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 13:44
Operator : AJ\MA
Sample : PB145272BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 16:18:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

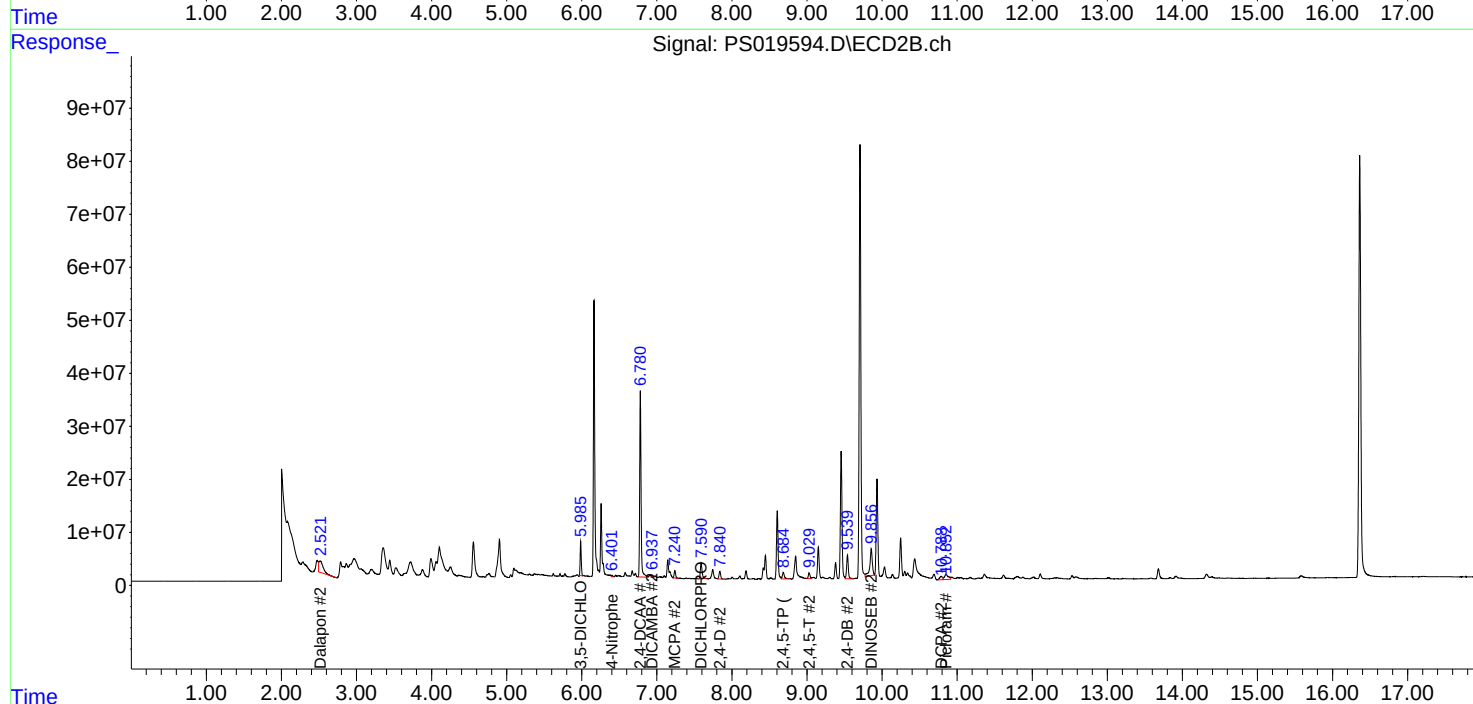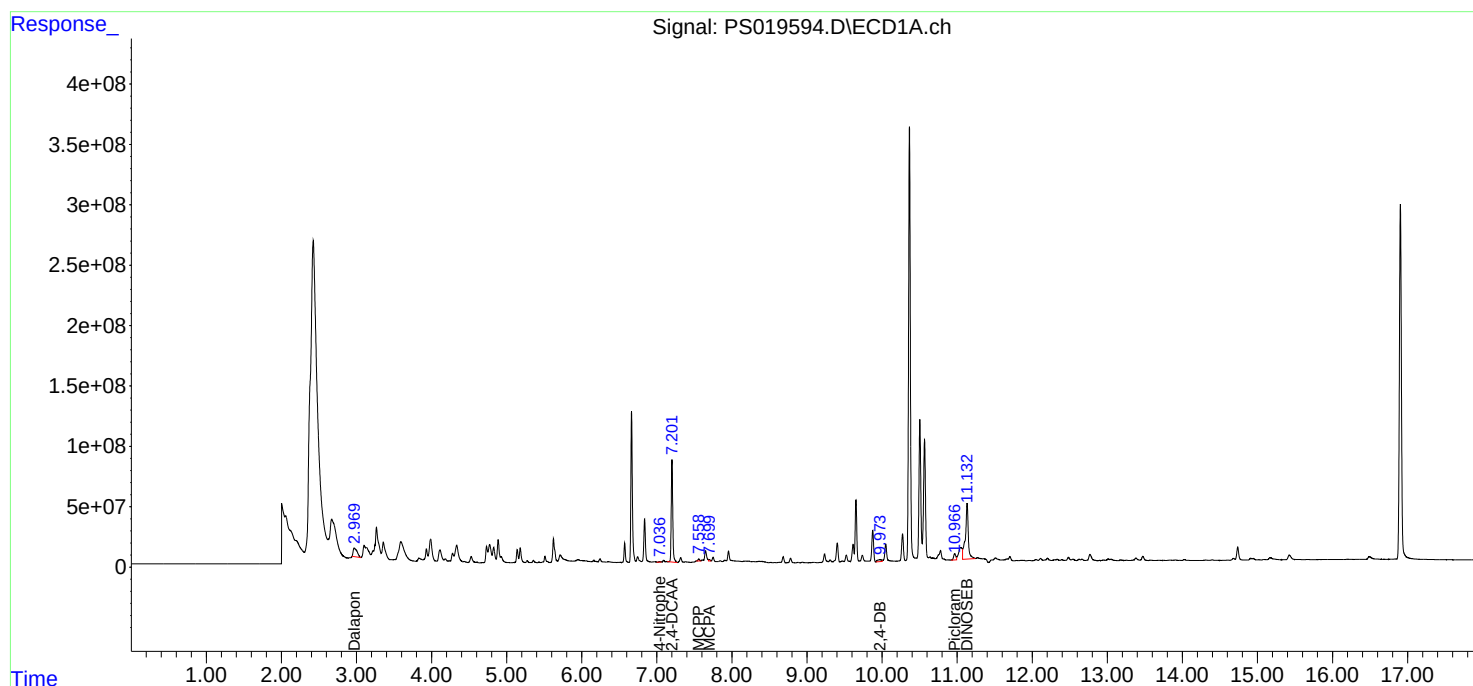


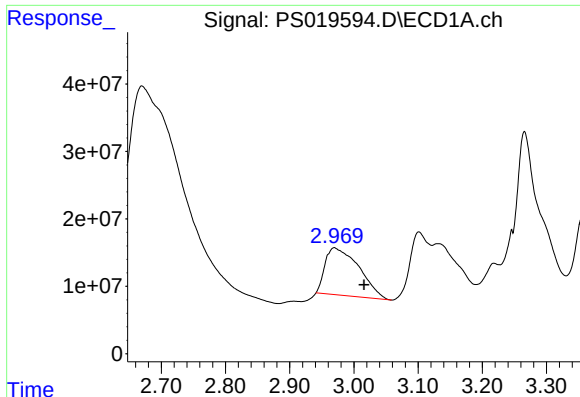

#1 Dalapon


R.T.: 2.970 min
Delta R.T.: -0.046 min
Response: 256863322
Conc: 50.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

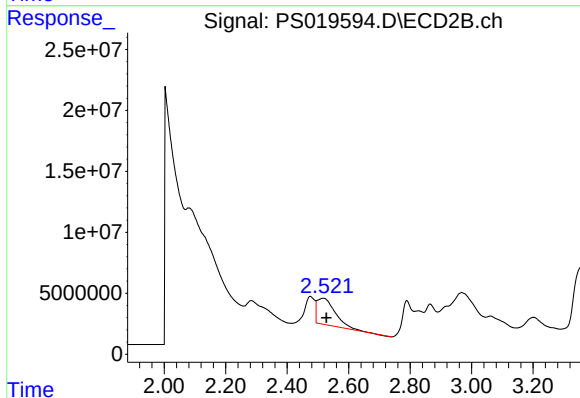


#1 Dalapon

R.T.: 2.519 min
Delta R.T.: -0.009 min
Response: 88005408
Conc: 87.70 ng/ml

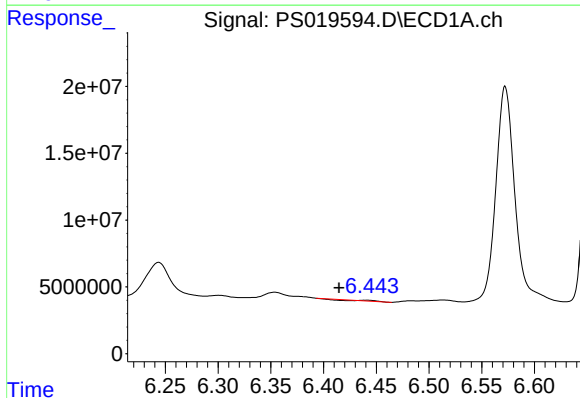


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.440 min
Delta R.T.: 0.026 min
Response: 50534
Conc: N.D.

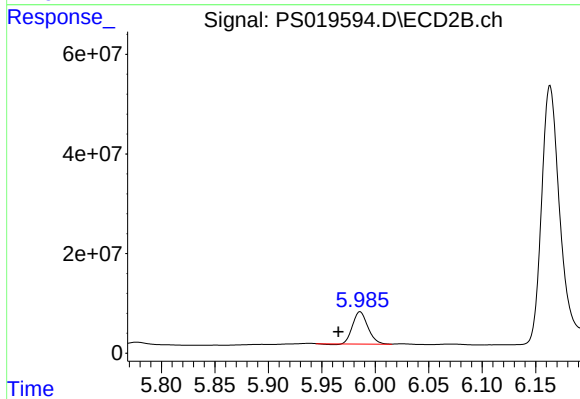

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.986 min
Delta R.T.: 0.020 min
Response: 64464870
Conc: 53.78 ng/ml

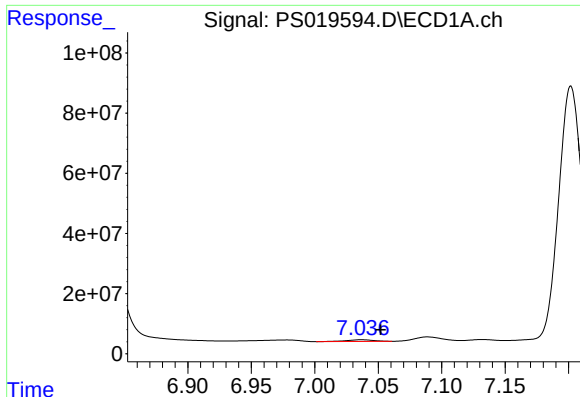

#3 4-Nitrophenol


R.T.: 7.037 min
Delta R.T.: -0.015 min
Response: 8477541
Conc: 8.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

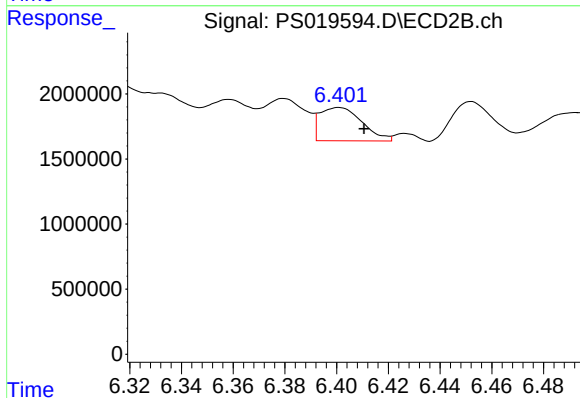


#3 4-Nitrophenol

R.T.: 6.401 min
Delta R.T.: -0.010 min
Response: 2911186
Conc: 6.80 ng/ml

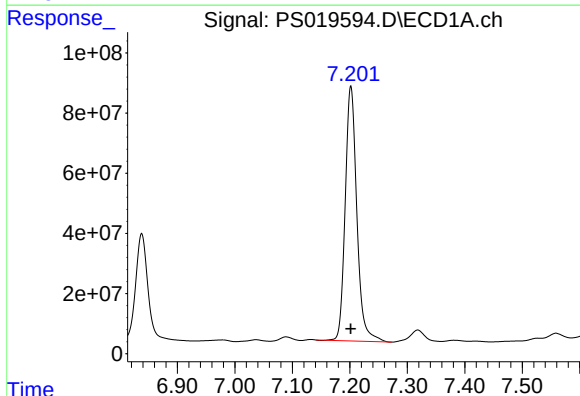


#4 2,4-DCAA

R.T.: 7.202 min
Delta R.T.: 0.000 min
Response: 1189010880
Conc: 495.59 ng/ml

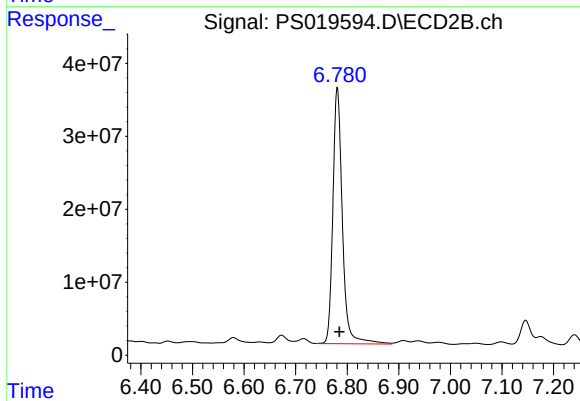

#4 2,4-DCAA


R.T.: 6.781 min
Delta R.T.: -0.004 min
Response: 450204360
Conc: 581.01 ng/ml

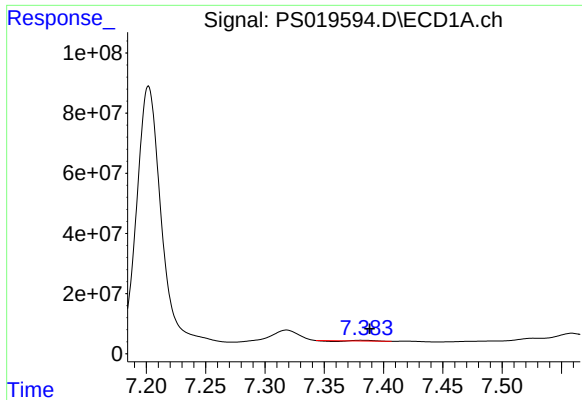

#5 DICAMBA


R.T.: 7.382 min
Delta R.T.: -0.007 min
Response: 245037
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

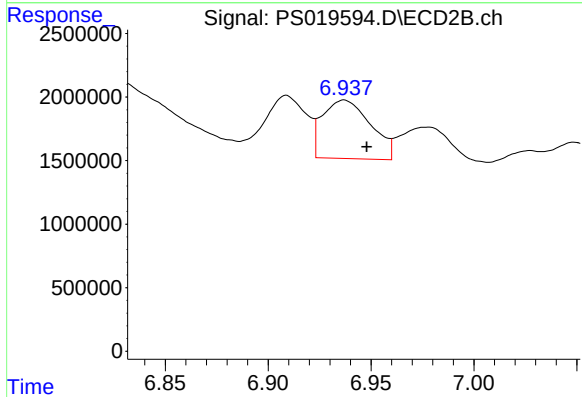


#5 DICAMBA

R.T.: 6.937 min
Delta R.T.: -0.011 min
Response: 7475251
Conc: 2.19 ng/ml

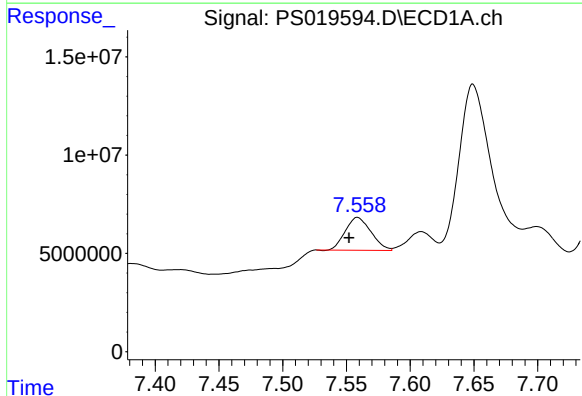


#6 MCP

R.T.: 7.559 min
Delta R.T.: 0.007 min
Response: 23423813
Conc: 3.12 ug/ml

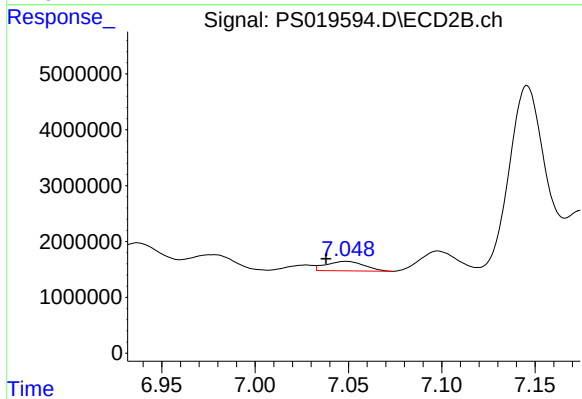

#6 MCP


R.T.: 7.049 min
Delta R.T.: 0.011 min
Response: 2416911
Conc: N.D.

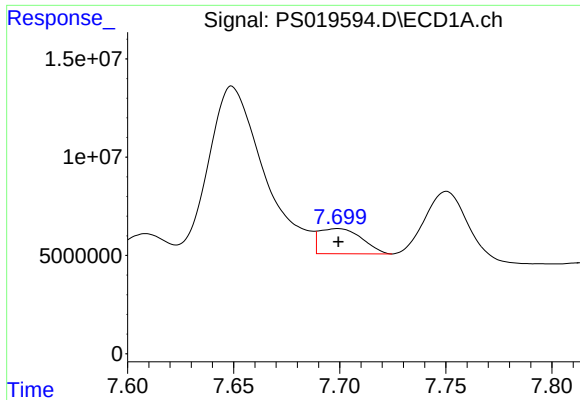

#7 MCPA


R.T.: 7.699 min
Delta R.T.: 0.000 min
Response: 17686472
Conc: 1.64 ug/ml

Instrument :
ECD_S
ClientSampleId :

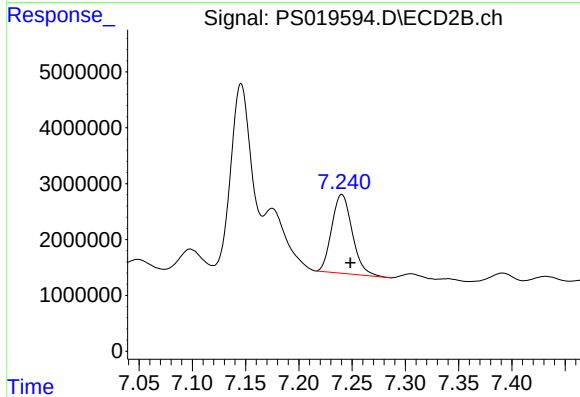


#7 MCPA

R.T.: 7.240 min
Delta R.T.: -0.008 min
Response: 18899954
Conc: 4.92 ug/ml

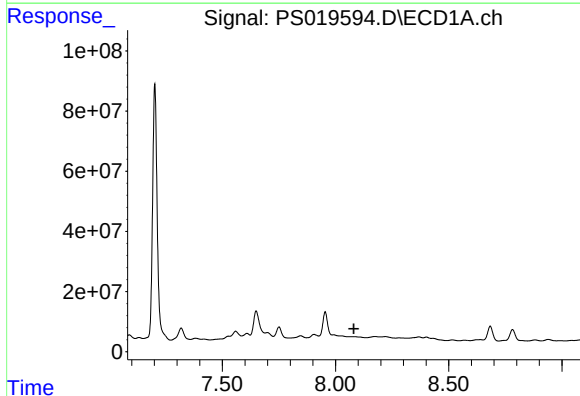


#8 DICHLORPROP

R.T.: 8.066 min
Delta R.T.: -0.015 min
Response: -1218478
Conc: N.D.

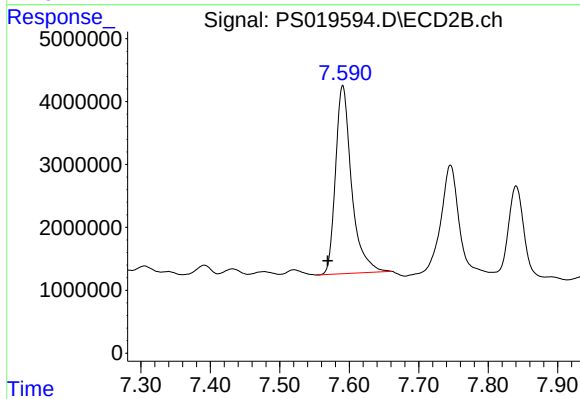

#8 DICHLORPROP


R.T.: 7.591 min
Delta R.T.: 0.022 min
Response: 47904635
Conc: 54.23 ng/ml

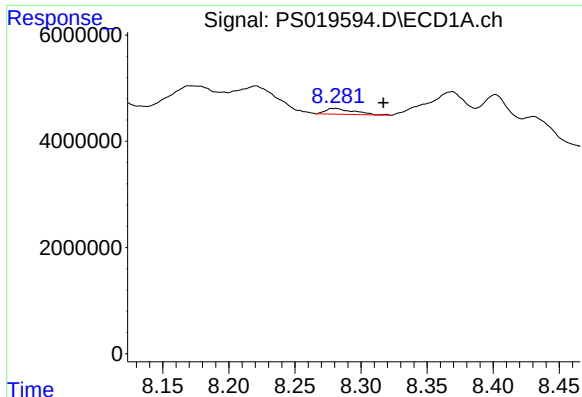

#9 2,4-D


R.T.: 8.280 min
Delta R.T.: -0.037 min
Response: 1630530
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

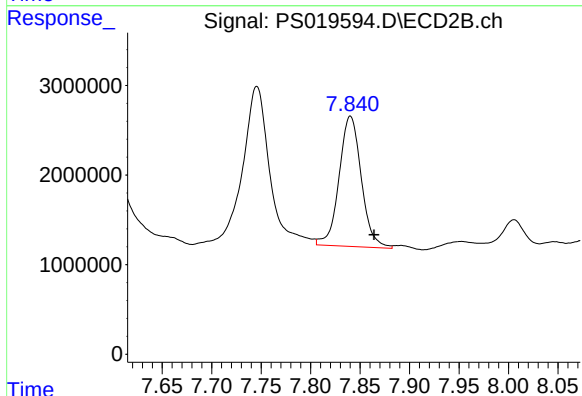


#9 2,4-D

R.T.: 7.840 min
Delta R.T.: -0.024 min
Response: 22748861
Conc: 21.33 ng/ml

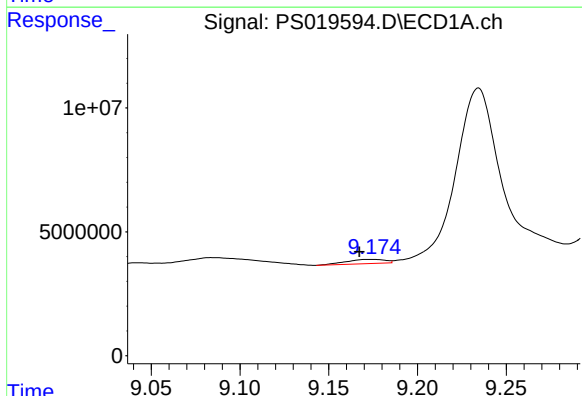


#11 2,4,5-TP (SILVEX)

R.T.: 9.174 min
Delta R.T.: 0.007 min
Response: 2657134
Conc: N.D.

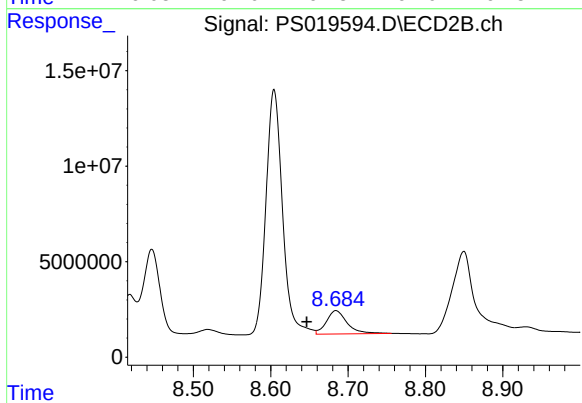

#11 2,4,5-TP (SILVEX)


R.T.: 8.684 min
Delta R.T.: 0.038 min
Response: 21789974
Conc: 4.33 ng/ml

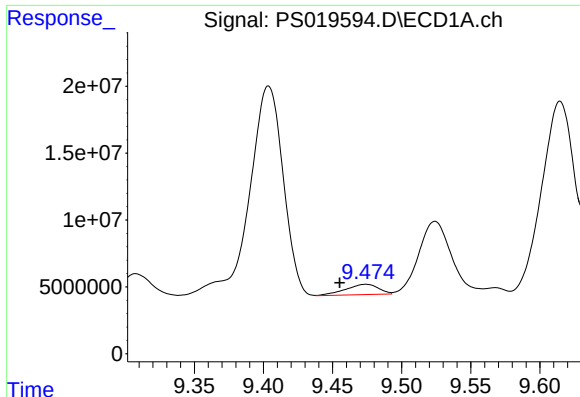

#12 2,4,5-T


R.T.: 9.474 min
Delta R.T.: 0.019 min
Response: 12777036
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

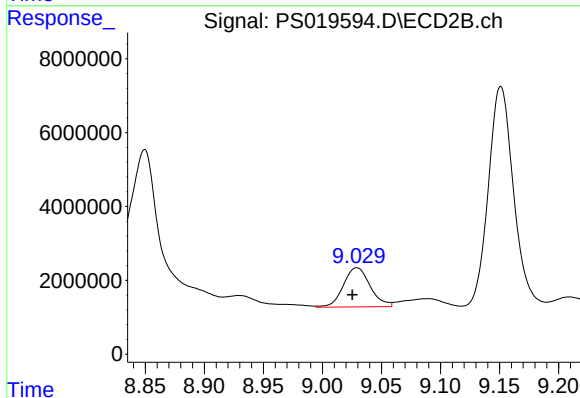


#12 2,4,5-T

R.T.: 9.029 min
Delta R.T.: 0.004 min
Response: 16834126
Conc: 3.58 ng/ml

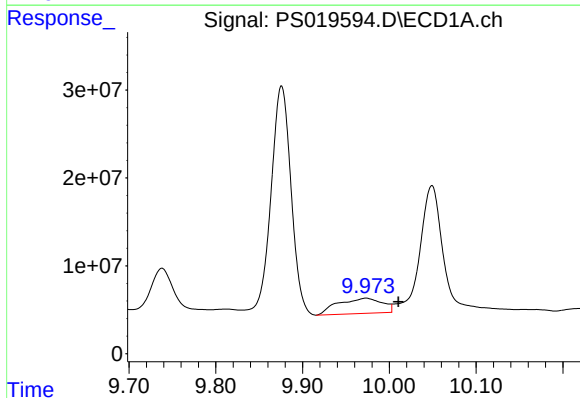


#13 2,4-DB

R.T.: 9.973 min
Delta R.T.: -0.037 min
Response: 61513295
Conc: 15.20 ng/ml

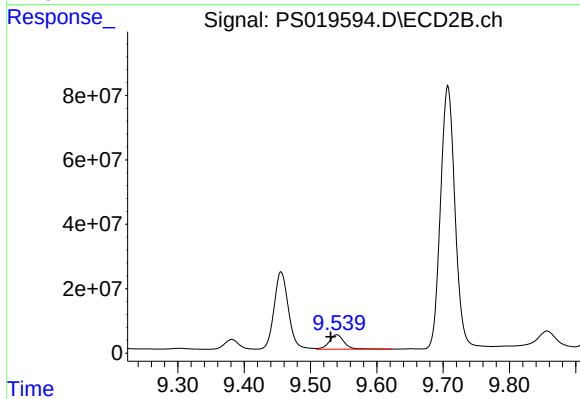

#13 2,4-DB


R.T.: 9.540 min
Delta R.T.: 0.009 min
Response: 70125451
Conc: 113.48 ng/ml

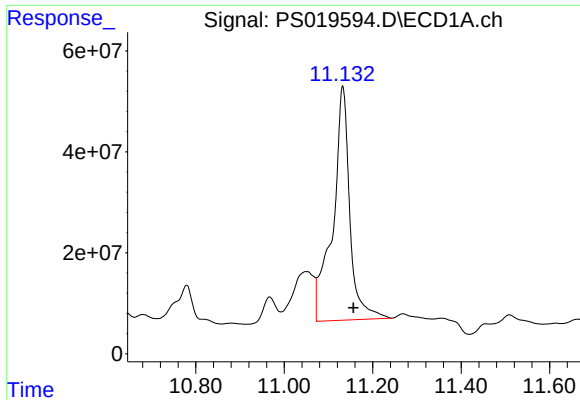

#14 DINOSEB


R.T.: 11.132 min
Delta R.T.: -0.024 min
Response: 1241672601
Conc: 80.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

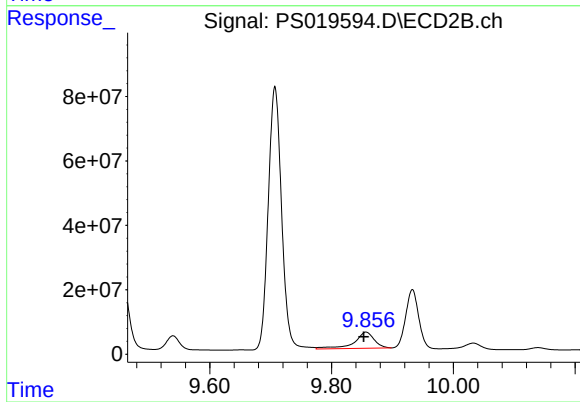


#14 DINOSEB

R.T.: 9.857 min
Delta R.T.: 0.004 min
Response: 115522506
Conc: 32.52 ng/ml

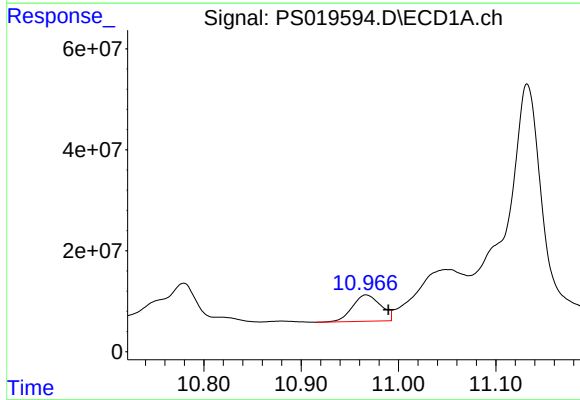


#15 Picloram

R.T.: 10.967 min
Delta R.T.: -0.023 min
Response: 105675615
Conc: 3.56 ng/ml

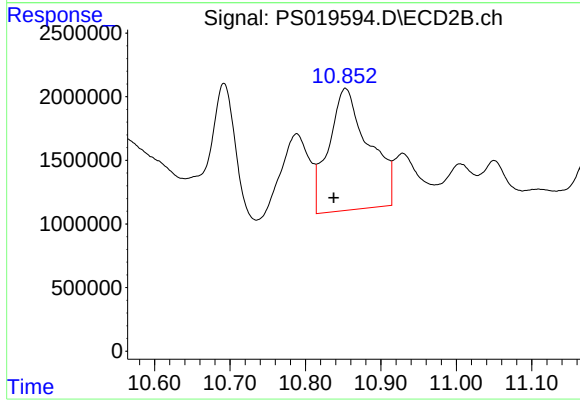

#15 Picloram


R.T.: 10.853 min
Delta R.T.: 0.016 min
Response: 35287783
Conc: 5.49 ng/ml

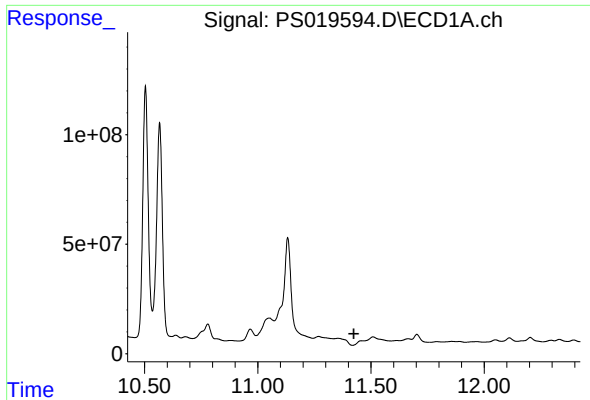

#16 DCPA

R.T.: 11.457 min
Delta R.T.: 0.032 min
Response: -42029808
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

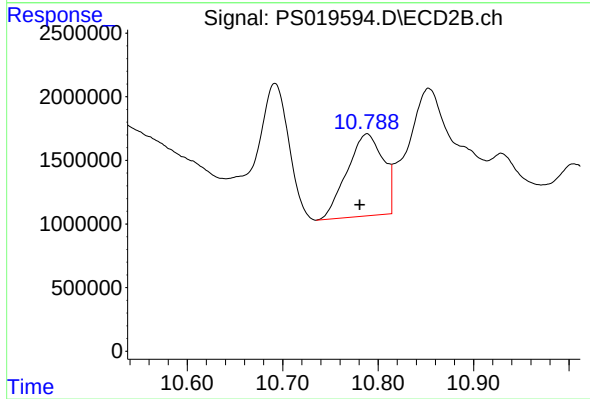

#16 DCPA

R.T.: 10.788 min
Delta R.T.: 0.008 min
Response: 17009453
Conc: 2.76 ng/ml