

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060322\
 Data File : PS019601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 16:31
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 17:06:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.784	1153.4E6	435.3E6	480.750	561.832
Target Compounds							
1) T	Dalapon	3.033	0.000	391787	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.468f	0.000	2496252	0	<MDL	N.D. #
3) T	4-Nitroph...	6.990f	0.000	1748968	0	1.782	N.D. #
5) T	DICAMBA	0.000	7.012f	0	2360169	N.D.	<MDL
6) T	MCP	0.000	7.012	0	2360169	N.D.	<MDL
7) T	MCPA	7.706	0.000	6217179	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.626f	0	3990988	N.D.	4.518
9) T	2,4-D	0.000	7.913f	0	424911	N.D.	<MDL
10) T	Pentachlo...	8.618	8.284	2680537	1443068	<MDL	<MDL #
11) T	2,4,5-TP ...	9.182	8.650	1660038	243463	<MDL	<MDL #
12) T	2,4,5-T	9.493	9.056	3055527	516481	<MDL	<MDL #
13) T	2,4-DB	10.006	9.560	7068167	409900	1.747	<MDL #
14) T	DINOSEB	11.151	9.859	11570242	612939	<MDL	<MDL #
15) T	Picloram	10.961	10.885f	307.7E6	2997884	10.367	<MDL #
16) T	DCPA	11.428	10.784	3390175	1354542	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060322\
Data File : PS019601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 16:31
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 17:06:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

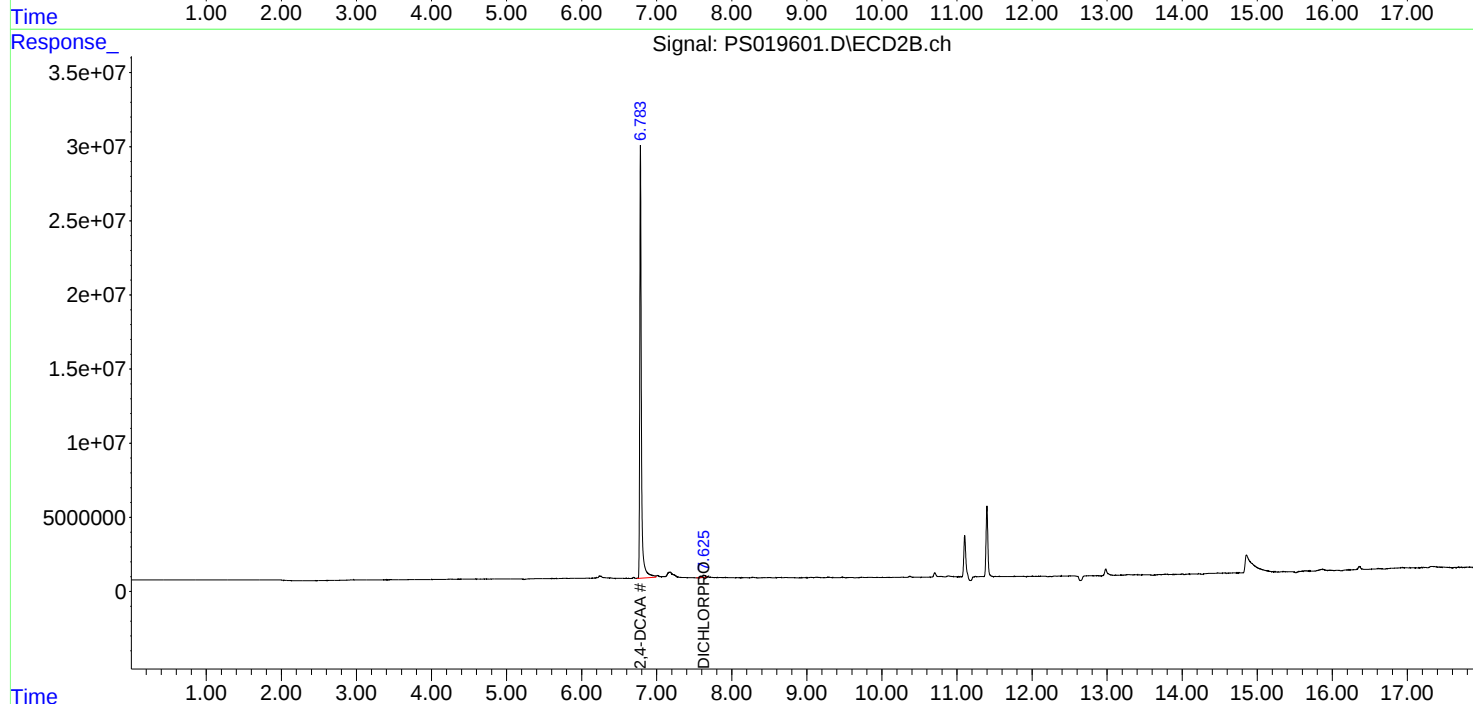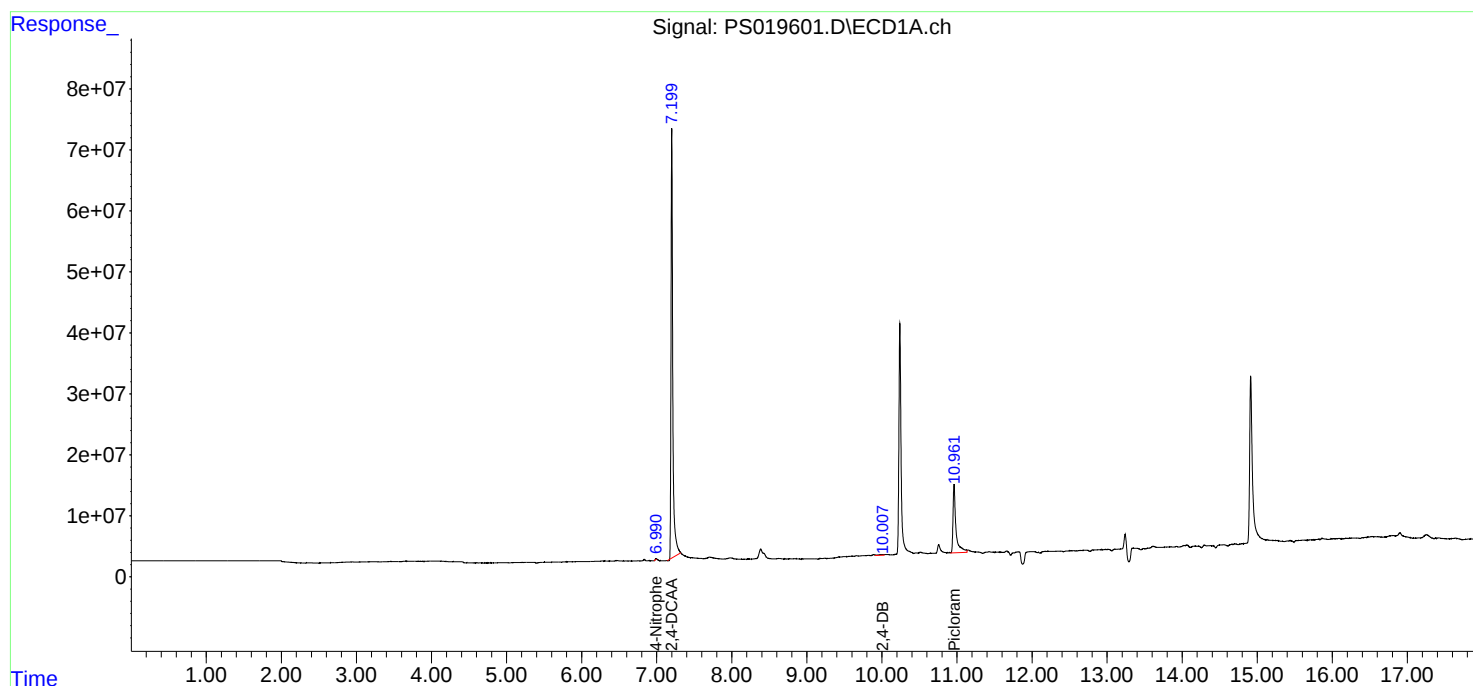


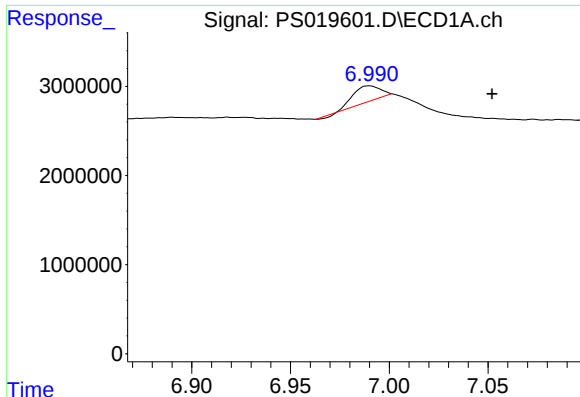

#3 4-Nitrophenol


R.T.: 6.990 min
Delta R.T.: -0.062 min
Response: 1748968
Conc: 1.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

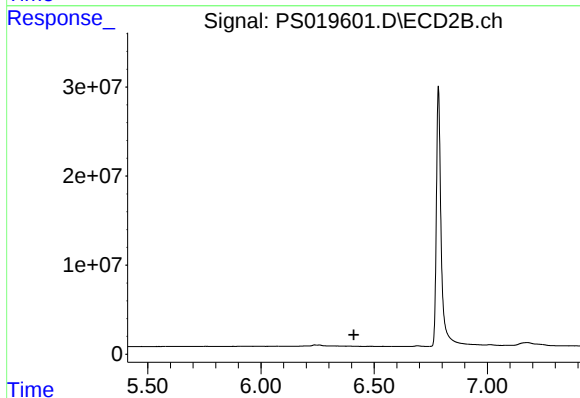


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

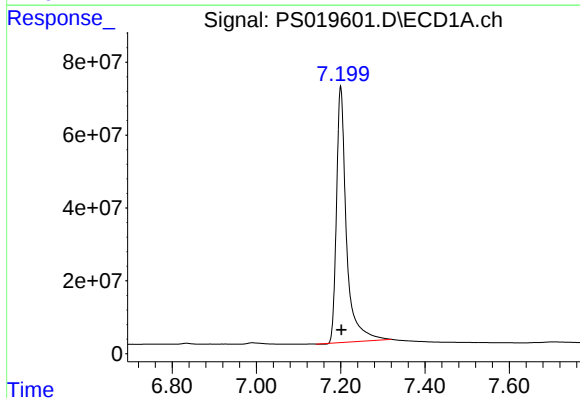


#4 2,4-DCAA

R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1153399405
Conc: 480.75 ng/ml

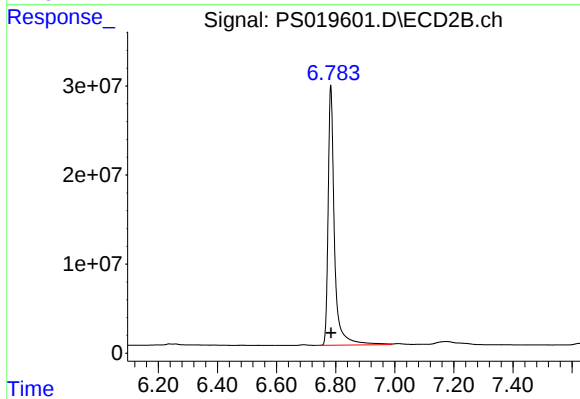

#4 2,4-DCAA


R.T.: 6.784 min
Delta R.T.: -0.001 min
Response: 435347243
Conc: 561.83 ng/ml

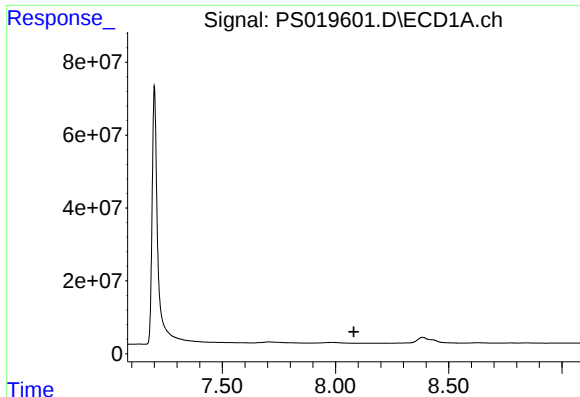

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.081 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

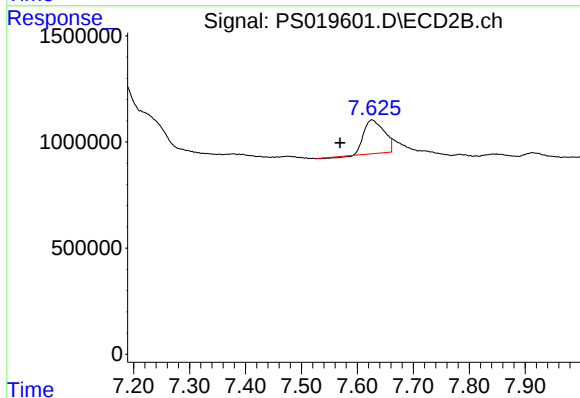


#8 DICHLORPROP

R.T.: 7.626 min
Delta R.T.: 0.057 min
Response: 3990988
Conc: 4.52 ng/ml

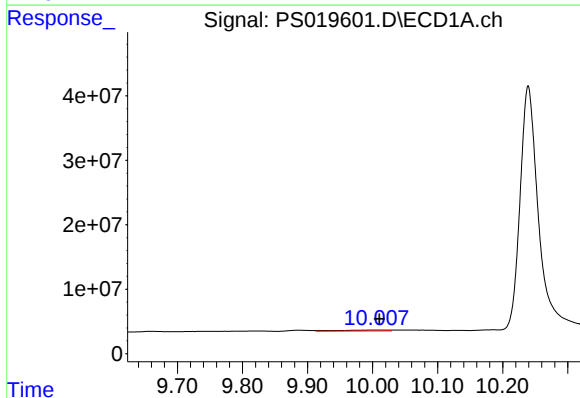


#13 2,4-DB

R.T.: 10.006 min
Delta R.T.: -0.005 min
Response: 7068167
Conc: 1.75 ng/ml

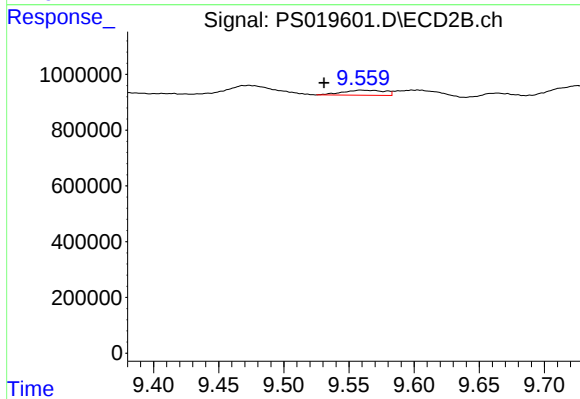

#13 2,4-DB


R.T.: 9.560 min
Delta R.T.: 0.029 min
Response: 409900
Conc: N.D.

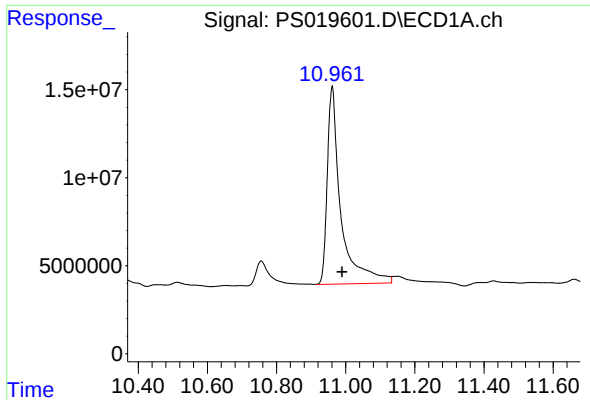

#15 Picloram

R.T.: 10.961 min
Delta R.T.: -0.029 min
Response: 307663400
Conc: 10.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

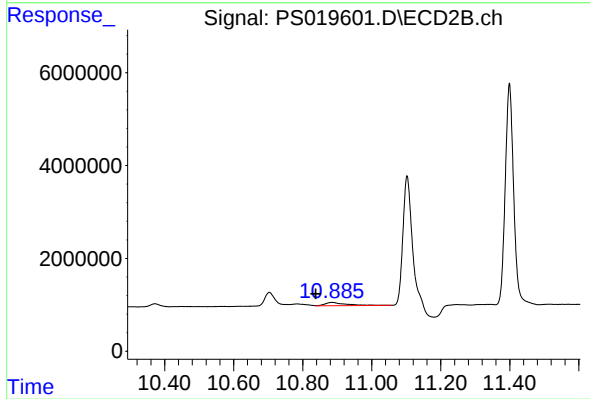

#15 Picloram

R.T.: 10.885 min
Delta R.T.: 0.048 min
Response: 2997884
Conc: N.D.