

Data Path : Y:\PESTPCBSRV\HPCHEM1\ECD_S\Data\PS060418\
 Data File : PS000199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2018 15:56
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 07:50:44 2018
 Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.861	11.229	-72786584	121.1E6	N.D.	385.488
Target Compounds							
10) T	Pentachlo...	14.130	0.000	2216154	0	0.443	N.D. #
15) T	Picloram	17.380	17.184	9634901	4841336	3.683	2.272 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Y:\PESTPCBSRV\HPCHEM1\ECD_S\Data\PS060418\
Data File : PS000199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2018 15:56
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 07:50:44 2018
Quant Method : Y:\PESTPCBSRV\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

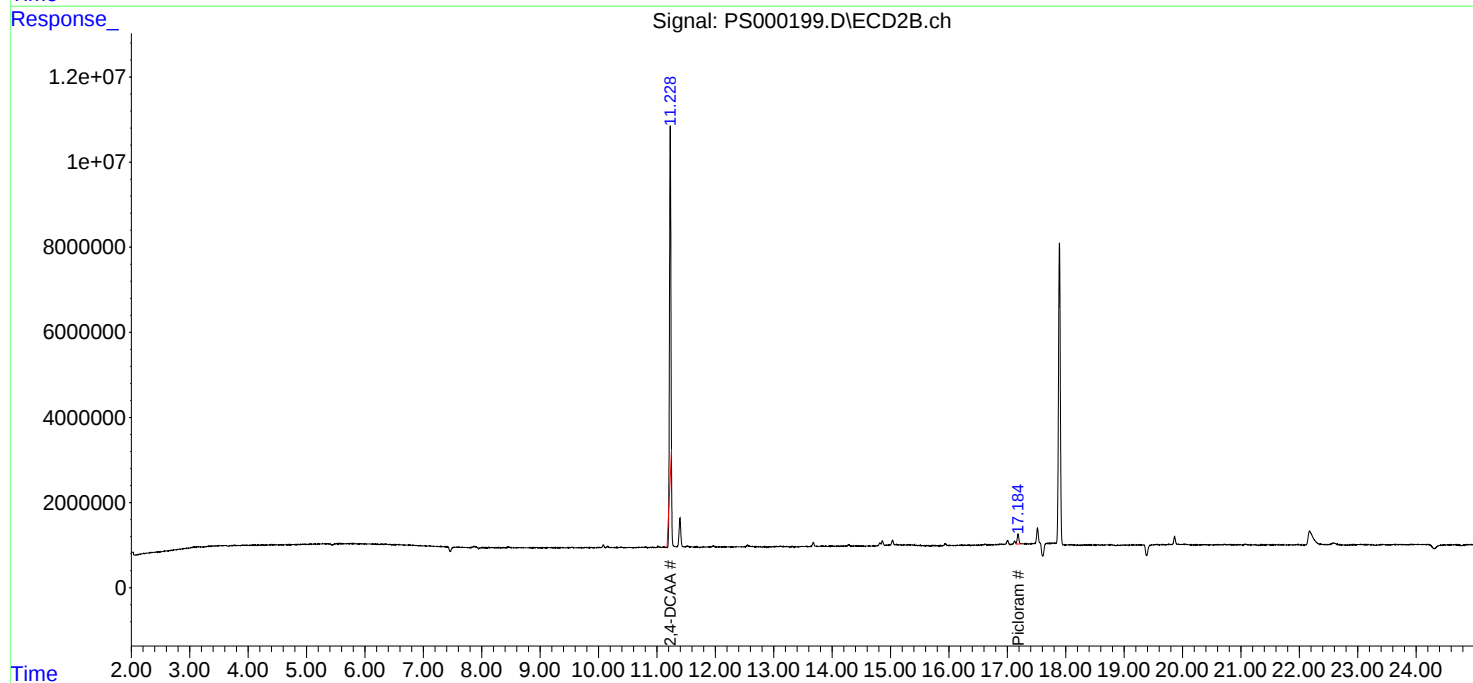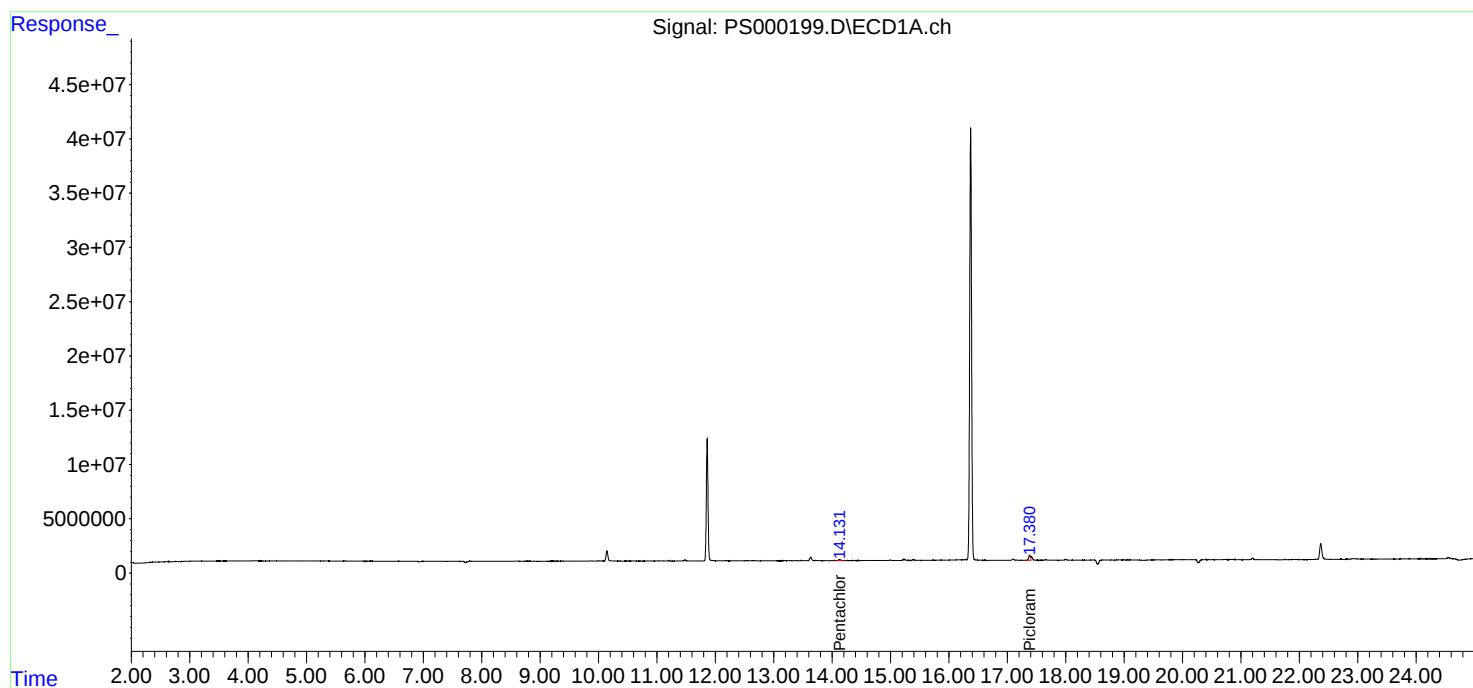


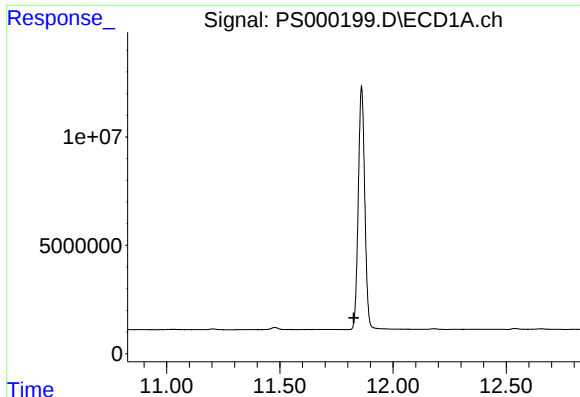

#4 2,4-DCAA


R.T.: 11.861 min
Delta R.T.: 0.034 min
Response: -72786584
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

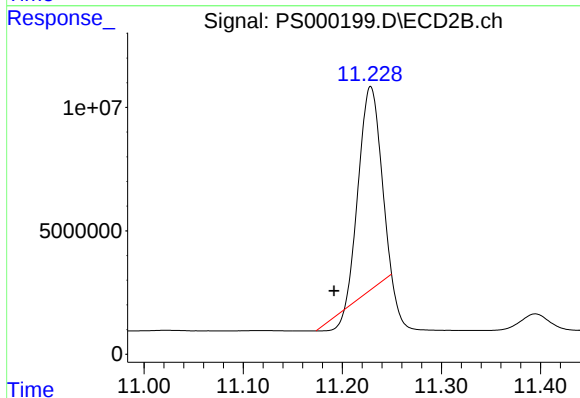


#4 2,4-DCAA

R.T.: 11.229 min
Delta R.T.: 0.037 min
Response: 121082597
Conc: 385.49 ng/ml

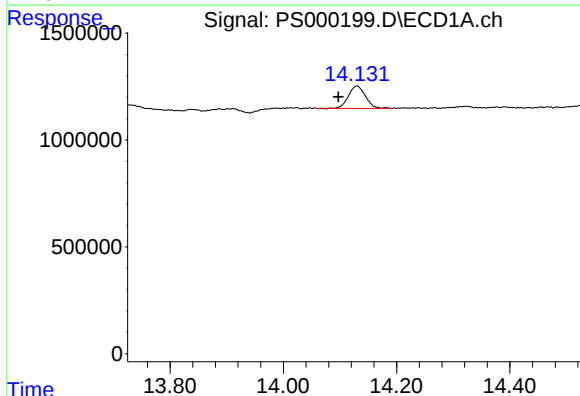


#10 Pentachlorophenol

R.T.: 14.130 min
Delta R.T.: 0.032 min
Response: 2216154
Conc: 0.44 ng/ml

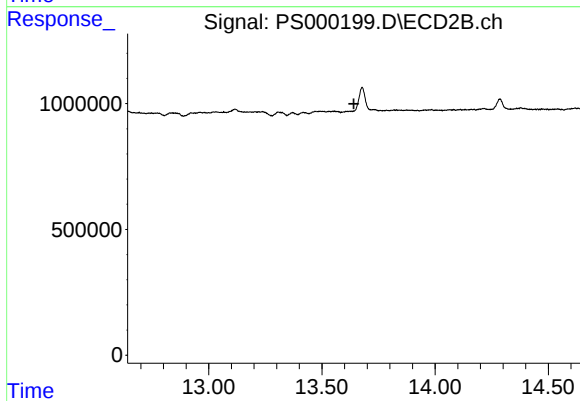

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.641 min
Response: 0
Conc: N.D.

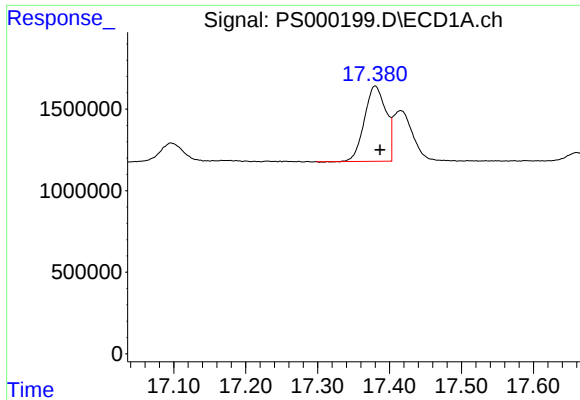

#15 Picloram

R.T.: 17.380 min
Delta R.T.: -0.007 min
Response: 9634901
Conc: 3.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

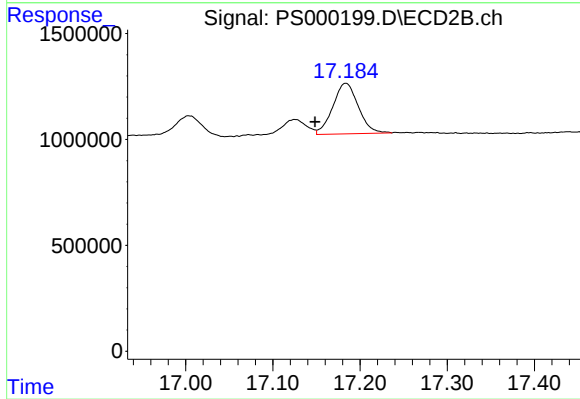

#15 Picloram

R.T.: 17.184 min
Delta R.T.: 0.036 min
Response: 4841336
Conc: 2.27 ng/ml