

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
 Data File : PS004893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 13:37
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:29:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.591	5.298	687.4E6	516.5E6	490.409	535.289
Target Compounds							
2) T	3,5-DICHL...	4.955	0.000	32117559	0	18.624	N.D. #
5) T	DICAMBA	0.000	5.453	0	32616004	N.D.	8.829
6) T	MCP	5.980	0.000	7731584	0	1.857	N.D. #
7) T	MCPA	5.980	0.000	7731584	0	1.335	N.D. #
8) T	DICHLORPROP	0.000	5.989	0	20351355	N.D.	21.585
9) T	2,4-D	6.632	0.000	96349185	0	70.435	N.D. #
10) T	Pentachlo...	6.892	0.000	14549534	0	<MDL	N.D. #
15) T	Picloram	9.127	9.113	728.0E6	36593146	69.870	4.905 #
16) T	DCPA	0.000	9.113	0	36593146	N.D.	5.649



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
Data File : PS004893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 13:37
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:29:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

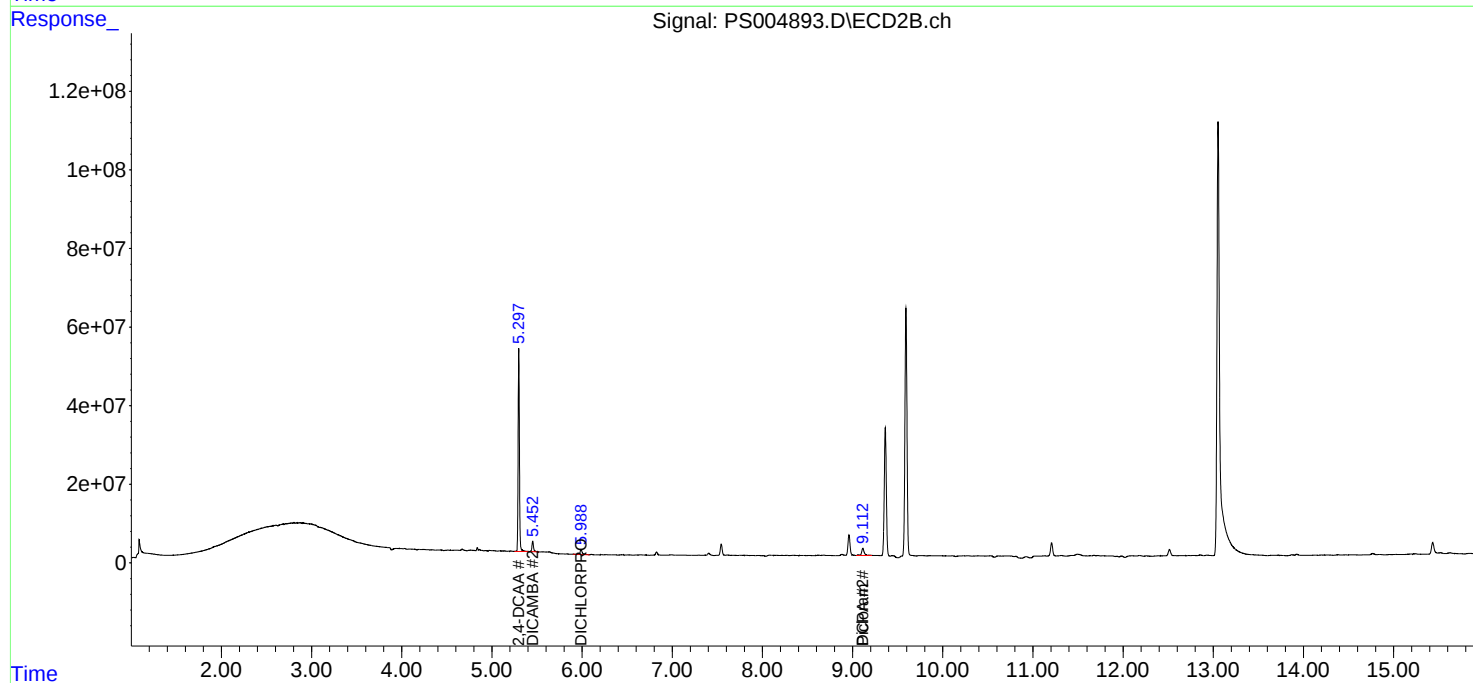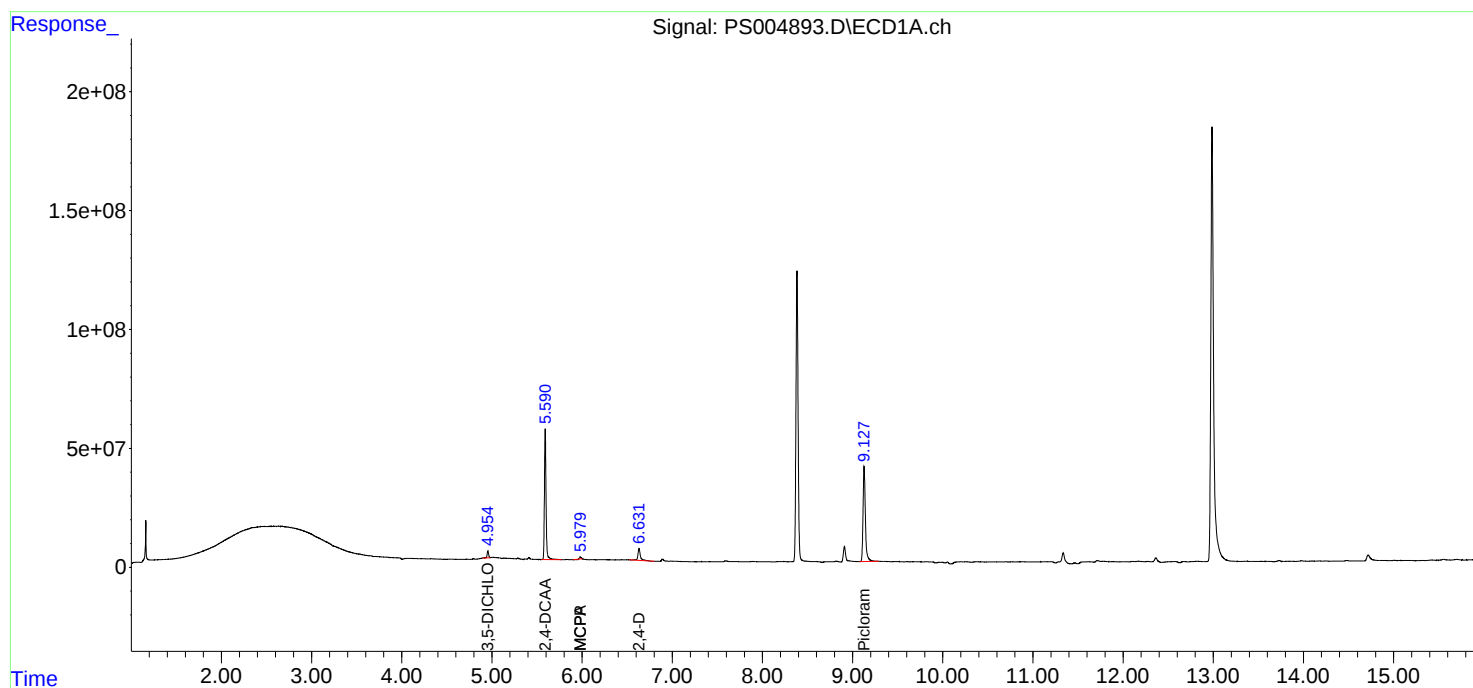


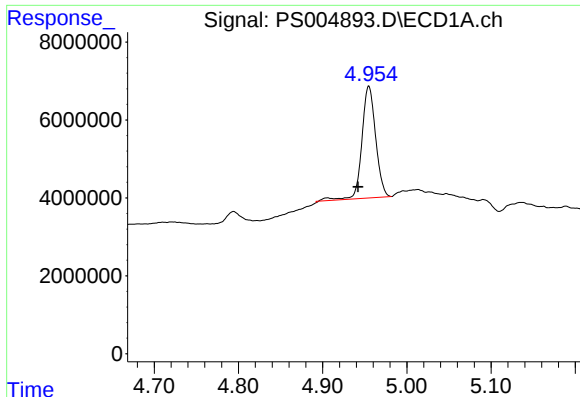

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.955 min
Delta R.T.: 0.013 min
Response: 32117559
Conc: 18.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

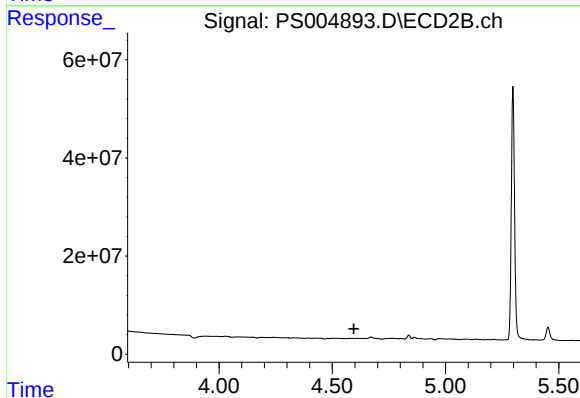


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

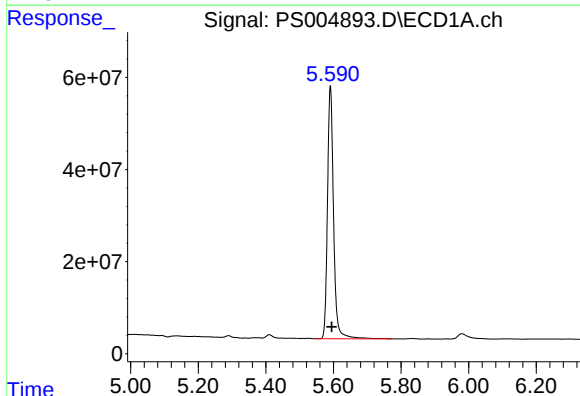


#4 2,4-DCAA

R.T.: 5.591 min
Delta R.T.: -0.004 min
Response: 687433116
Conc: 490.41 ng/ml

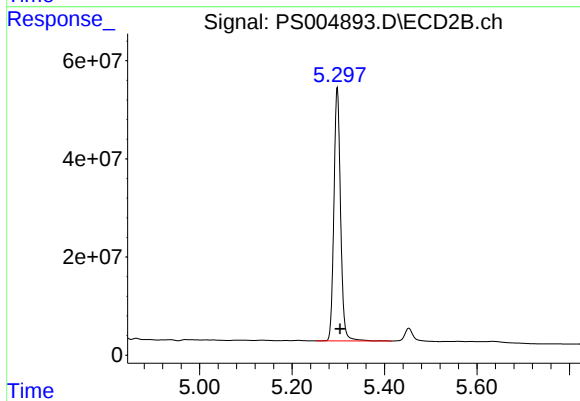

#4 2,4-DCAA


R.T.: 5.298 min
Delta R.T.: -0.006 min
Response: 516465894
Conc: 535.29 ng/ml

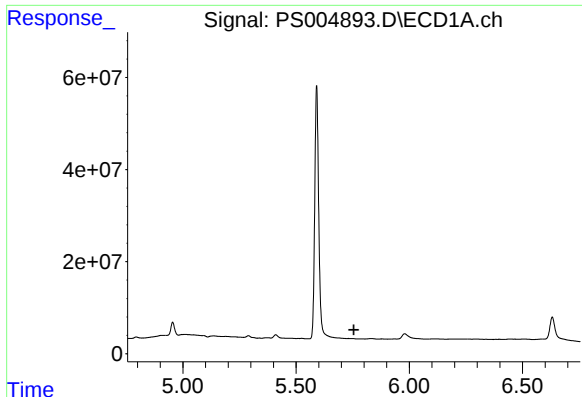

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

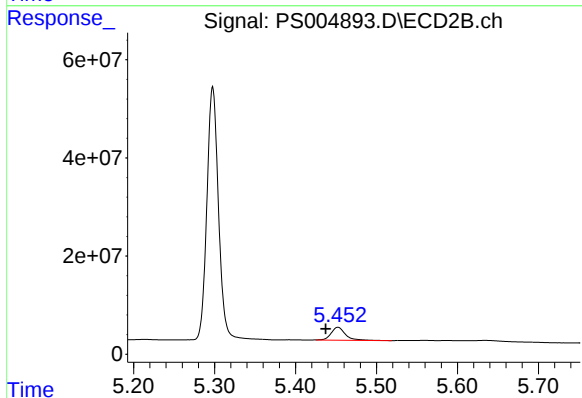


#5 DICAMBA

R.T.: 5.453 min
Delta R.T.: 0.015 min
Response: 32616004
Conc: 8.83 ng/ml

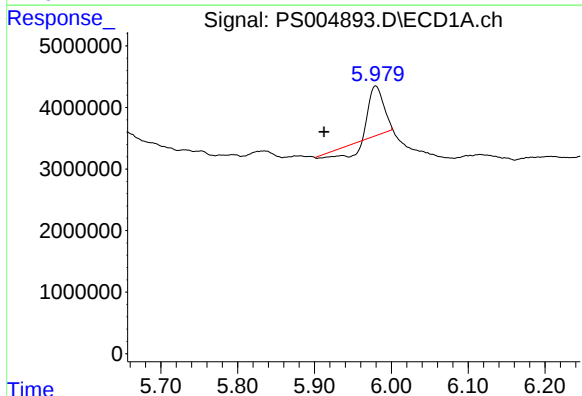


#6 MCP

R.T.: 5.980 min
Delta R.T.: 0.067 min
Response: 7731584
Conc: 1.86 ug/ml

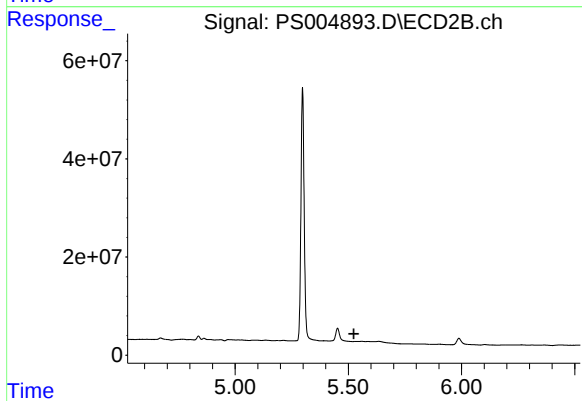

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

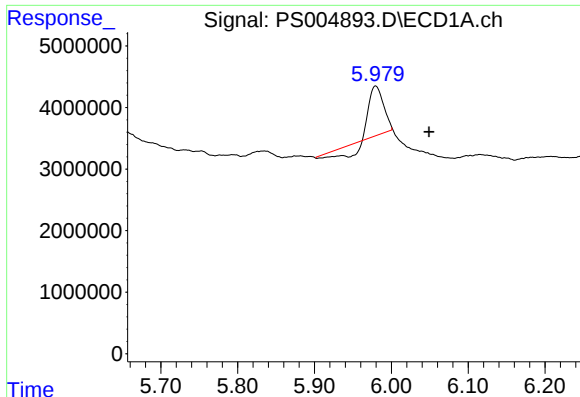

#7 MCPA


R.T.: 5.980 min
Delta R.T.: -0.069 min
Response: 7731584
Conc: 1.33 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

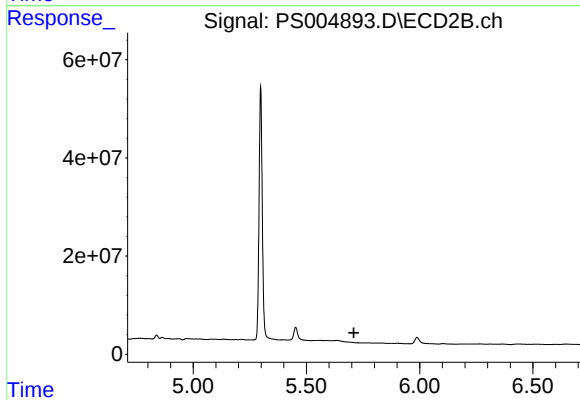


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.709 min
Response: 0
Conc: N.D.

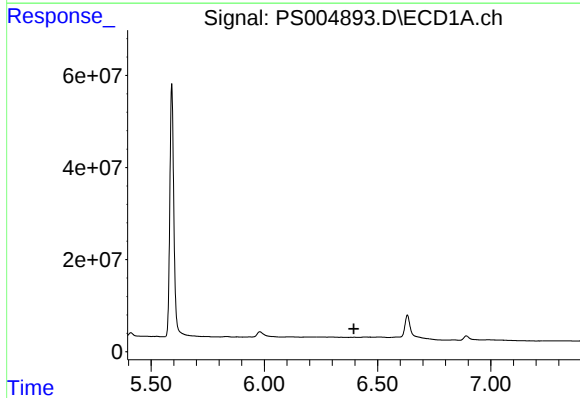


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

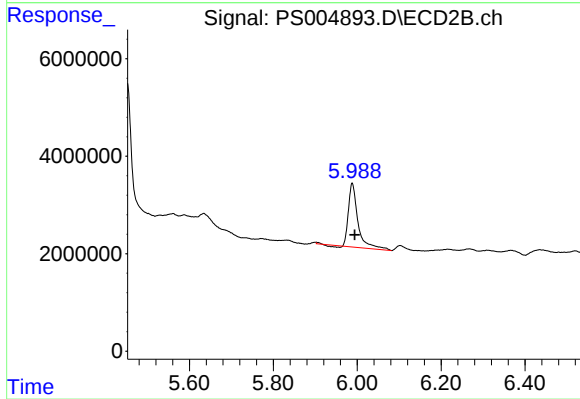

#8 DICHLORPROP


R.T.: 5.989 min
Delta R.T.: -0.005 min
Response: 20351355
Conc: 21.59 ng/ml

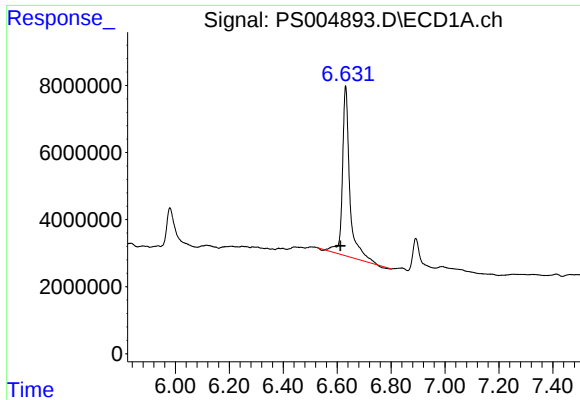

#9 2,4-D


R.T.: 6.632 min
Delta R.T.: 0.020 min
Response: 96349185
Conc: 70.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

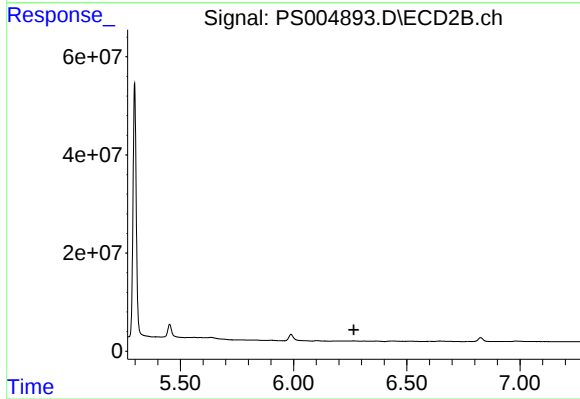


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

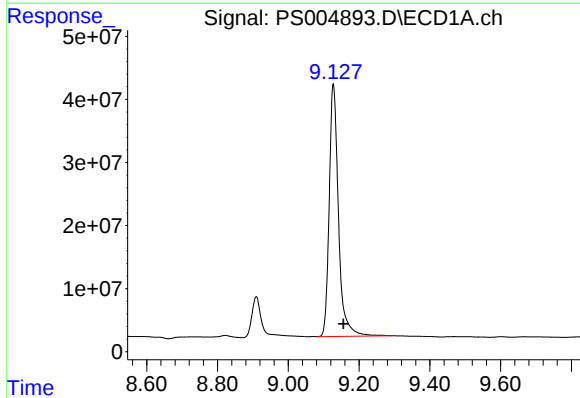


#15 Picloram

R.T.: 9.127 min
Delta R.T.: -0.028 min
Response: 728040821
Conc: 69.87 ng/ml

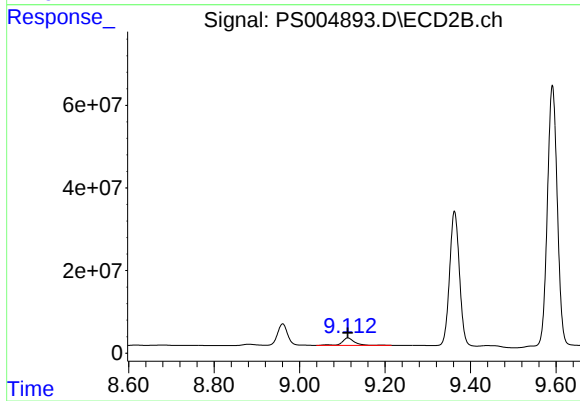

#15 Picloram


R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 36593146
Conc: 4.90 ng/ml

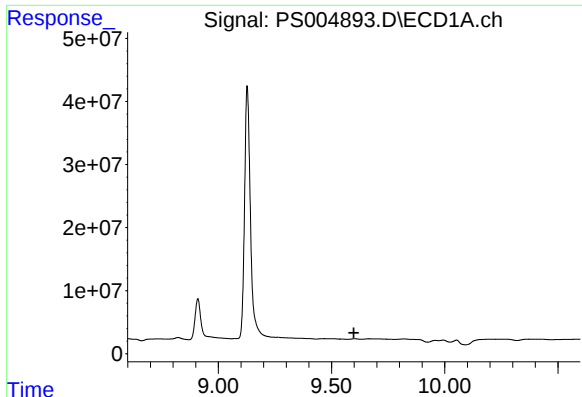

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

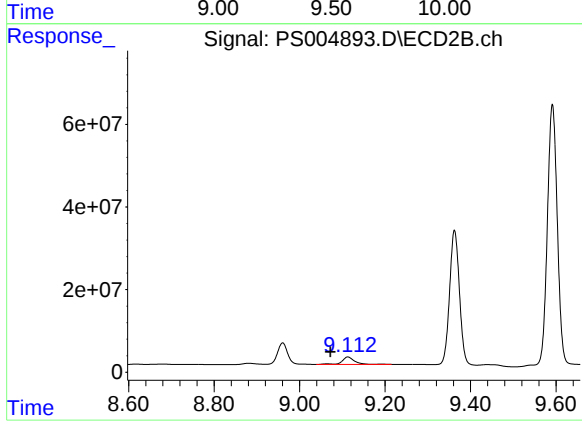

#16 DCPA

R.T.: 9.113 min
Delta R.T.: 0.041 min
Response: 36593146
Conc: 5.65 ng/ml