

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
 Data File : PS004898.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 15:43
 Operator : SM\AJ
 Sample : K2641-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-053119-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:31:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.573	5.285	474.2E6	345.8E6	338.306	358.424
Target Compounds							
1) T	Dalapon	2.154	1.765	15347590	-3088268	9.258	N.D. #
2) T	3,5-DICHL...	0.000	4.603	0	201.9E6	N.D.	163.829
5) T	DICAMBA	0.000	5.391	0	17484492	N.D.	4.733
6) T	MCP	5.961	0.000	4206385	0	1.010	N.D. #
7) T	MCPA	0.000	5.743	0	379.3E6	N.D.	92.708
8) T	DICHLORPROP	0.000	5.973	0	22985777	N.D.	24.380
9) T	2,4-D	6.659	0.000	26462079	0	19.345	N.D. #
11) T	2,4,5-TP ...	0.000	6.940	0	115.2E6	N.D.	22.386



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
Data File : PS004898.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 15:43
Operator : SM\AJ
Sample : K2641-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:31:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

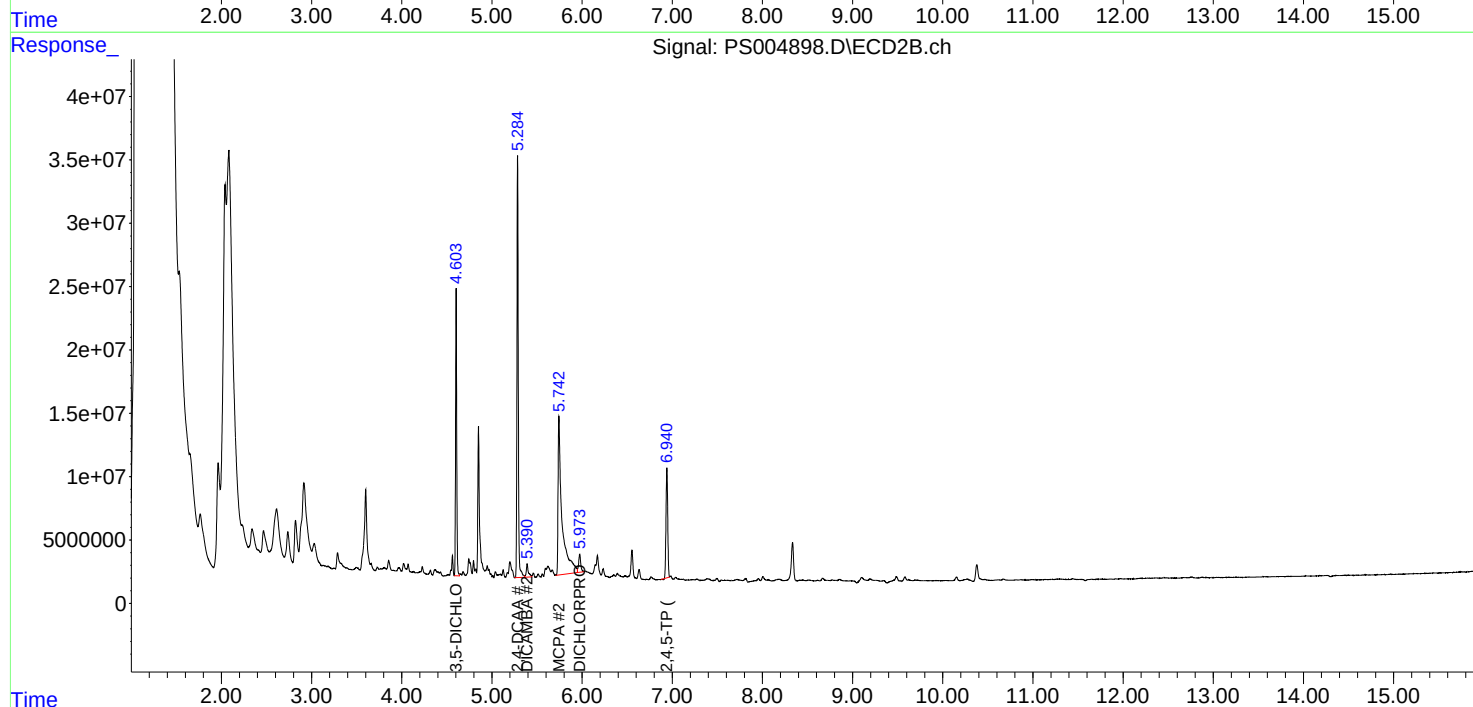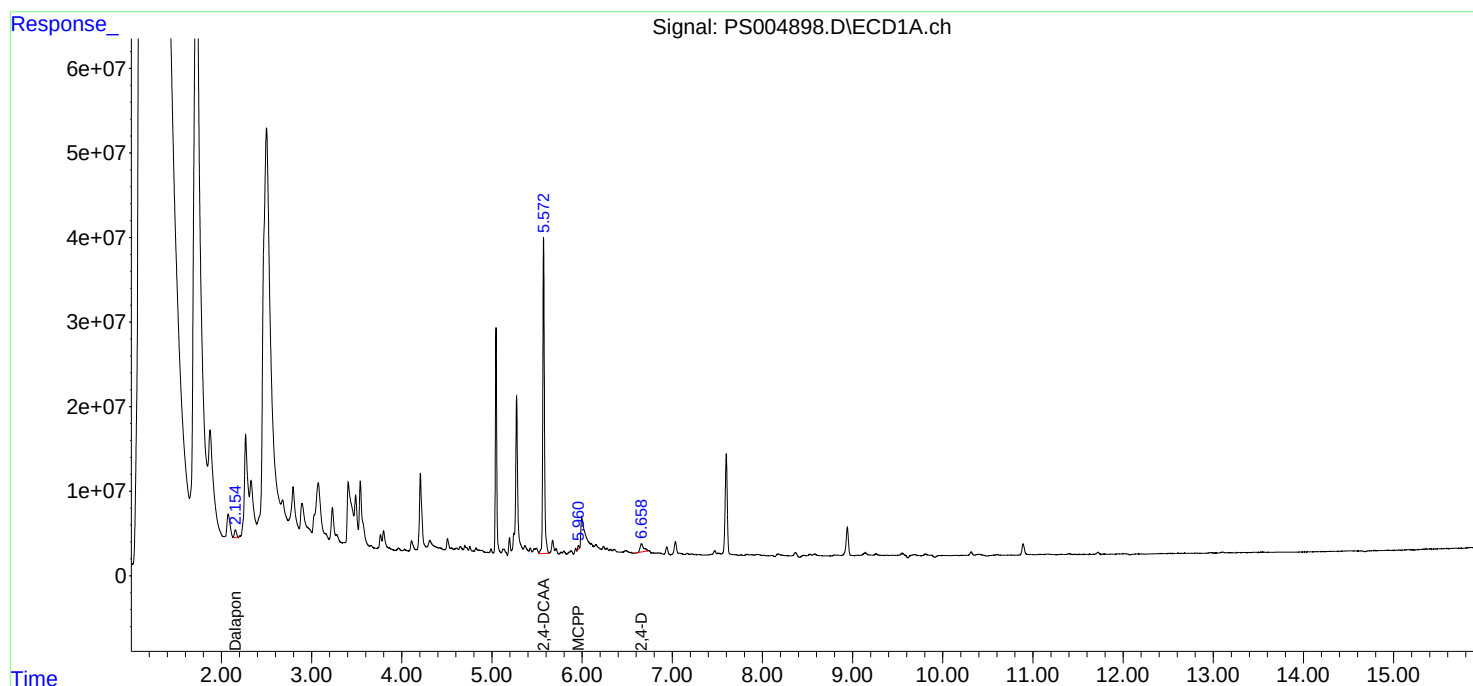


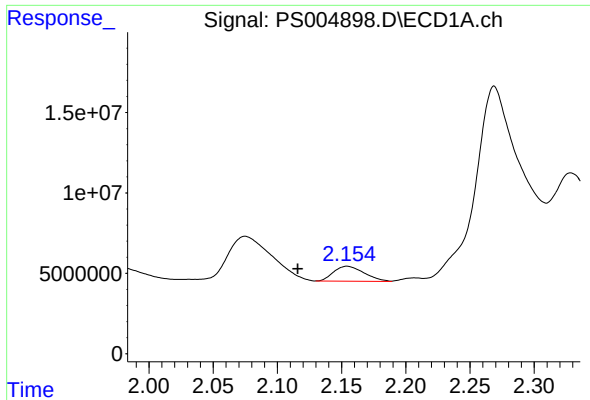

#1 Dalapon


R.T.: 2.154 min
Delta R.T.: 0.038 min
Response: 15347590
Conc: 9.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-A

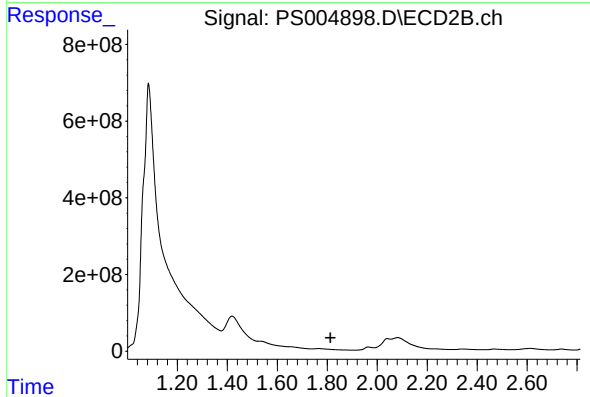


#1 Dalapon

R.T.: 1.765 min
Delta R.T.: -0.048 min
Response: -3088268
Conc: N.D.

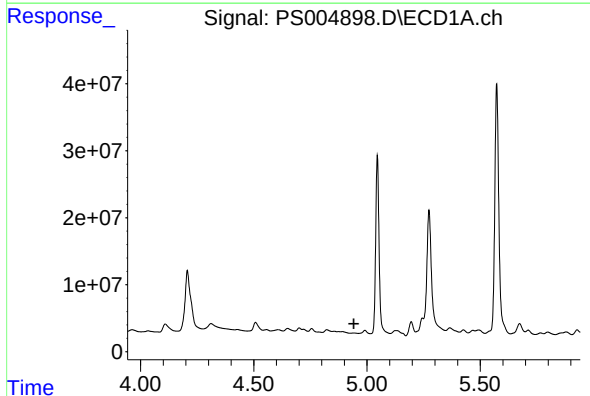


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

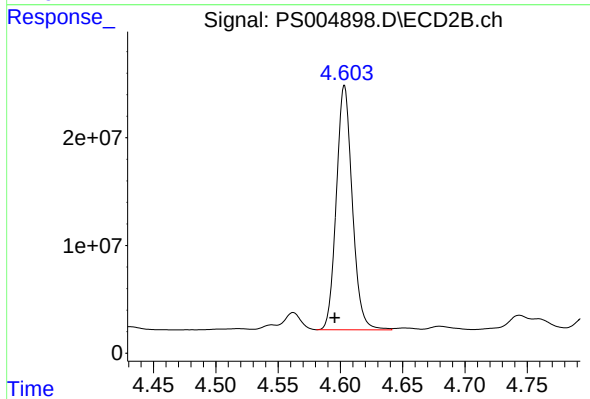

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.008 min
Response: 201858333
Conc: 163.83 ng/ml

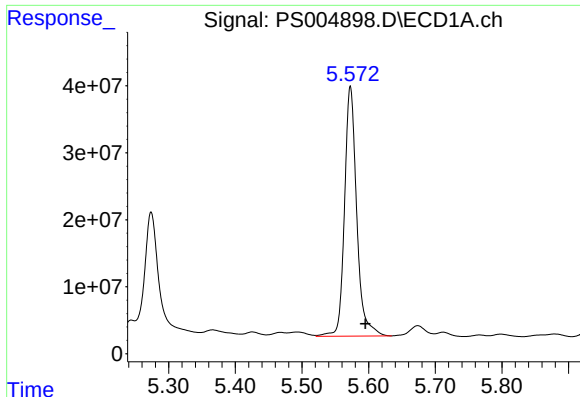

#4 2,4-DCAA


R.T.: 5.573 min
Delta R.T.: -0.022 min
Response: 474221857
Conc: 338.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-A

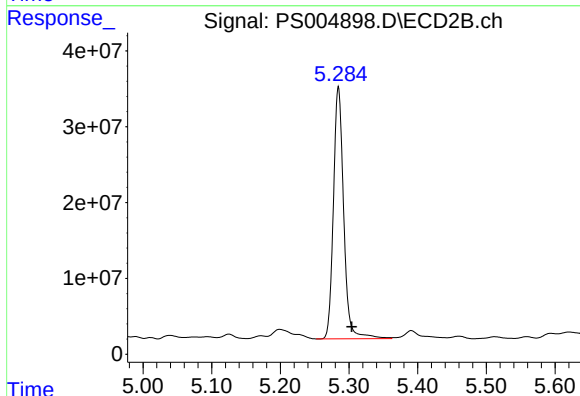


#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: -0.019 min
Response: 345820754
Conc: 358.42 ng/ml

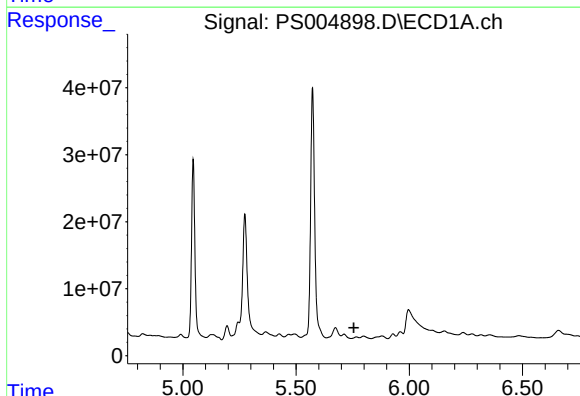


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

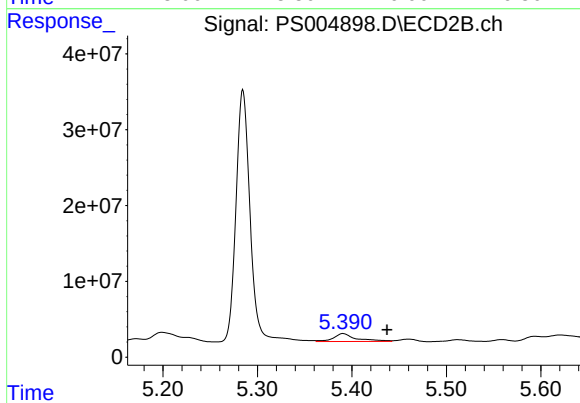

#5 DICAMBA


R.T.: 5.391 min
Delta R.T.: -0.047 min
Response: 17484492
Conc: 4.73 ng/ml

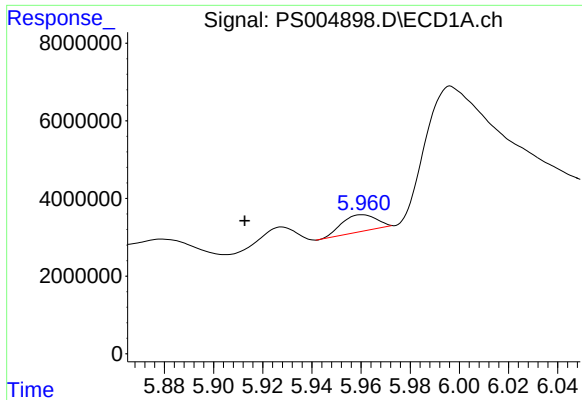

#6 MCPP


R.T.: 5.961 min
Delta R.T.: 0.048 min
Response: 4206385
Conc: 1.01 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-A

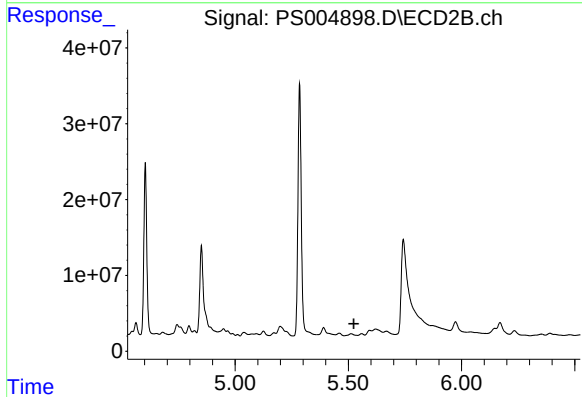


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

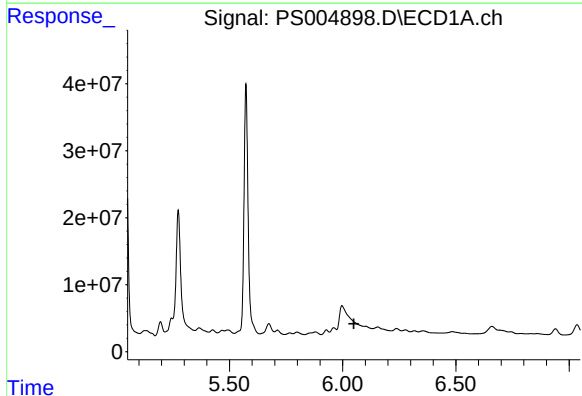


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

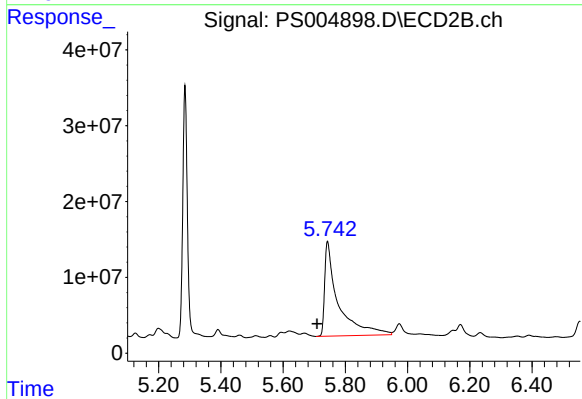

#7 MCPA


R.T.: 5.743 min
Delta R.T.: 0.034 min
Response: 379327861
Conc: 92.71 ug/ml

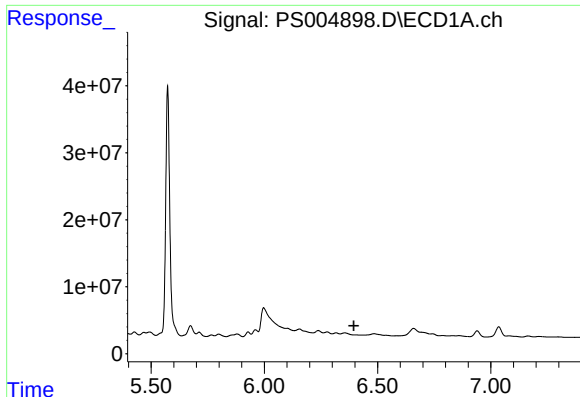

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-A

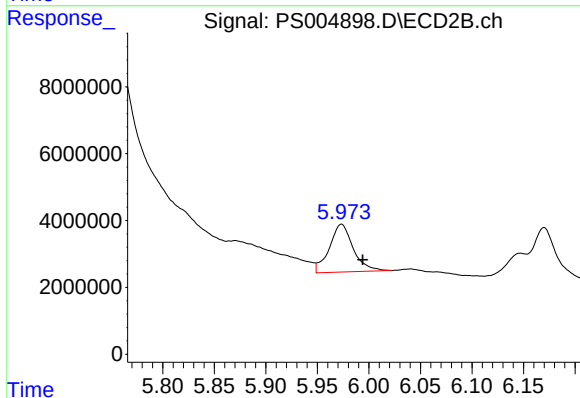


#8 DICHLORPROP

R.T.: 5.973 min
Delta R.T.: -0.021 min
Response: 22985777
Conc: 24.38 ng/ml

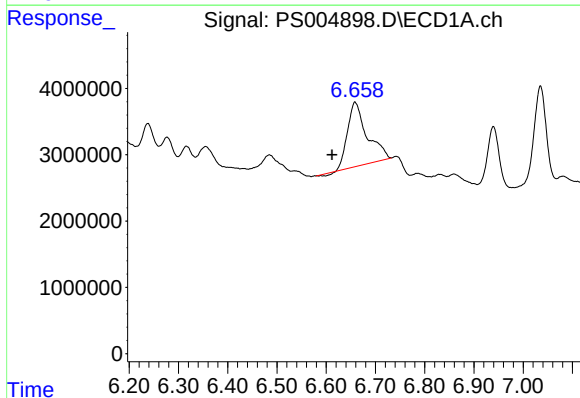


#9 2,4-D

R.T.: 6.659 min
Delta R.T.: 0.047 min
Response: 26462079
Conc: 19.34 ng/ml

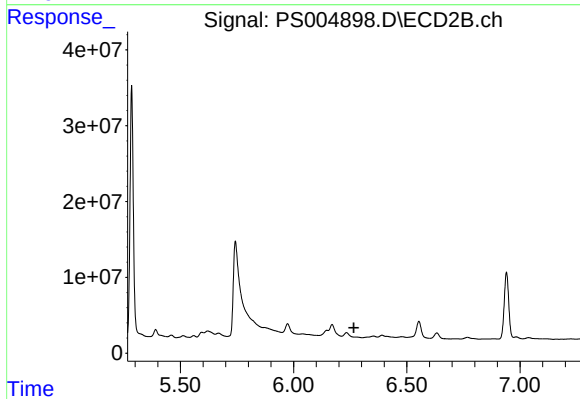

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

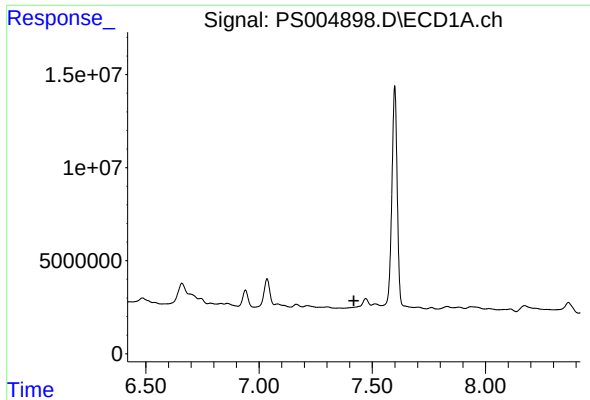

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-A

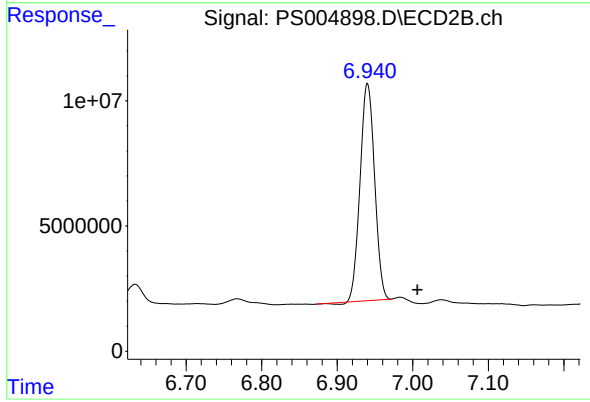

#11 2,4,5-TP (SILVEX)

R.T.: 6.940 min
Delta R.T.: -0.066 min
Response: 115185132
Conc: 22.39 ng/ml