

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
 Data File : PS004904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 17:56
 Operator : SM\AJ
 Sample : K2641-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-053119-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:33:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.594	5.306	481.7E6	337.6E6	343.635	349.877
Target Compounds							
1) T	Dalapon	2.098	0.000	37079909	0	22.368	N.D. #
2) T	3,5-DICHL...	0.000	4.584	0	12137295	N.D.	9.851
3) T	4-Nitroph...	5.387	0.000	26258608	0	42.114	N.D. #
5) T	DICAMBA	5.696	5.413	15267023	10639048	2.875	2.880
7) T	MCPA	6.019	5.765	120.4E6	414.0E6	20.786	101.189 #
8) T	DICHLORPROP	0.000	5.995	0	13154431	N.D.	13.952
9) T	2,4-D	6.681	0.000	44435047	0	32.484	N.D. #
10) T	Pentachlo...	0.000	6.574	0	30629283	N.D.	2.493
11) T	2,4,5-TP ...	0.000	6.962	0	155.0E6	N.D.	30.127



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
Data File : PS004904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 17:56
Operator : SM\AJ
Sample : K2641-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:33:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

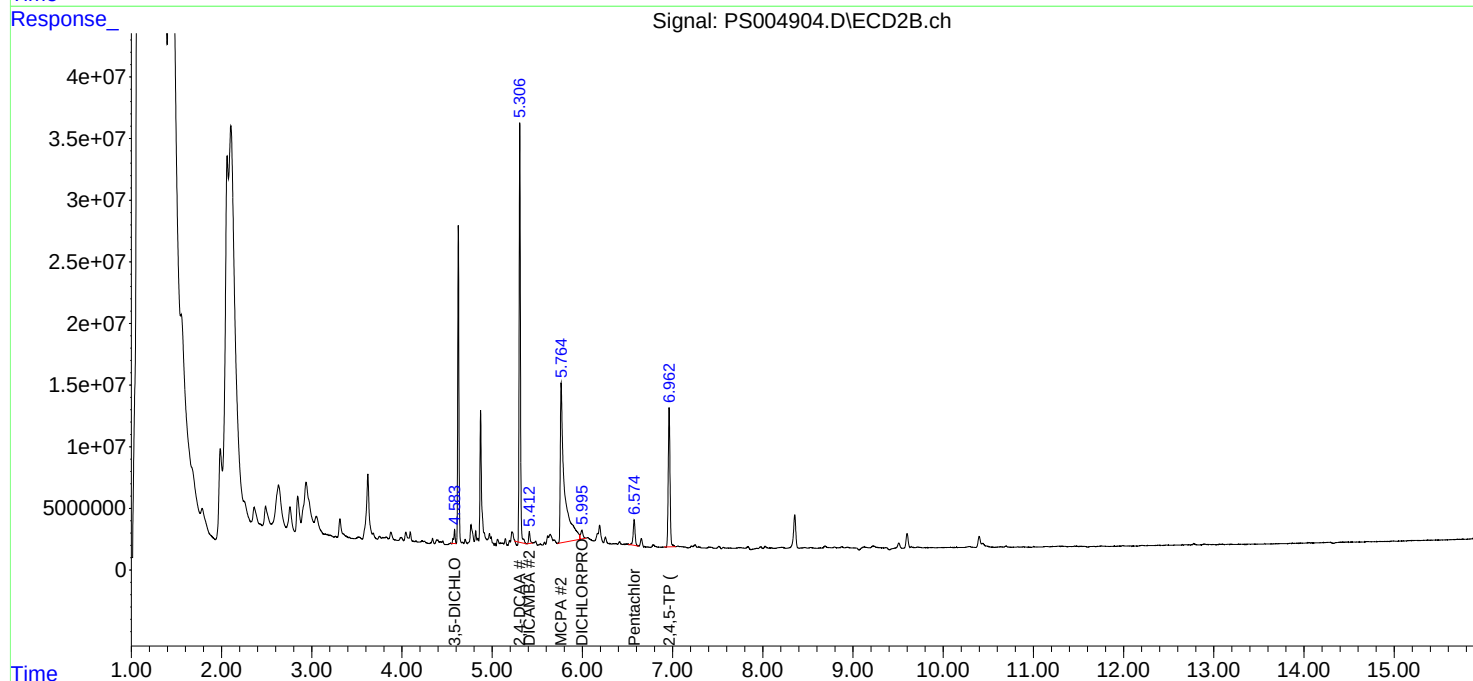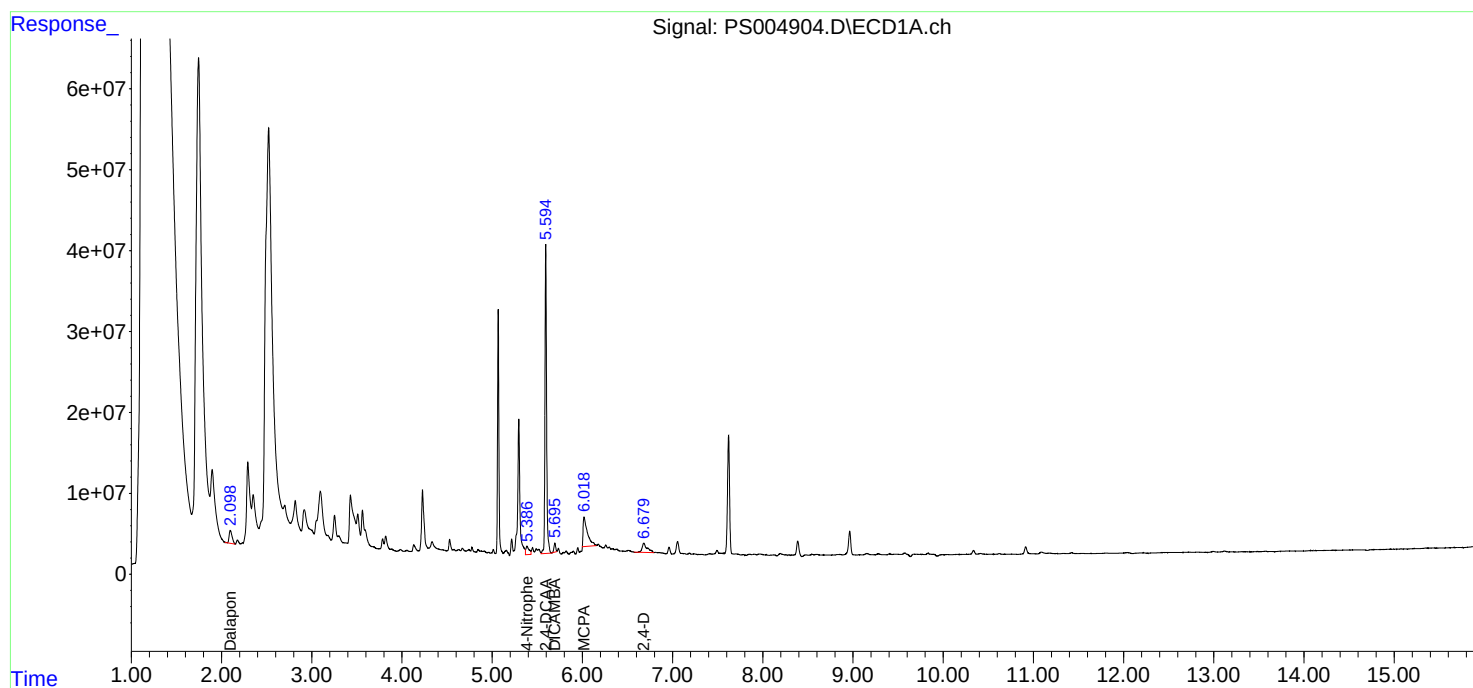


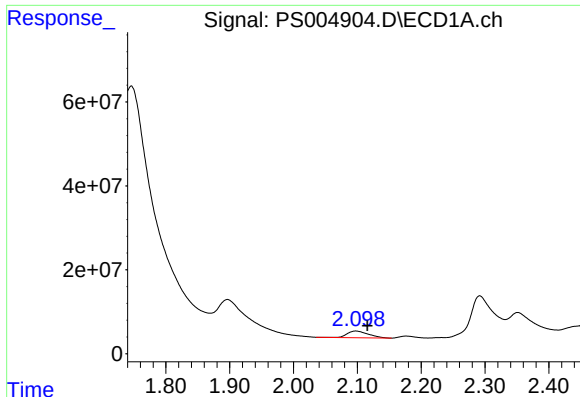

#1 Dalapon


R.T.: 2.098 min
Delta R.T.: -0.018 min
Response: 37079909
Conc: 22.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-E

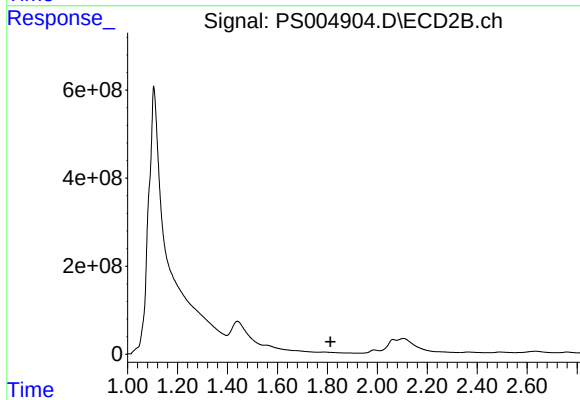


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

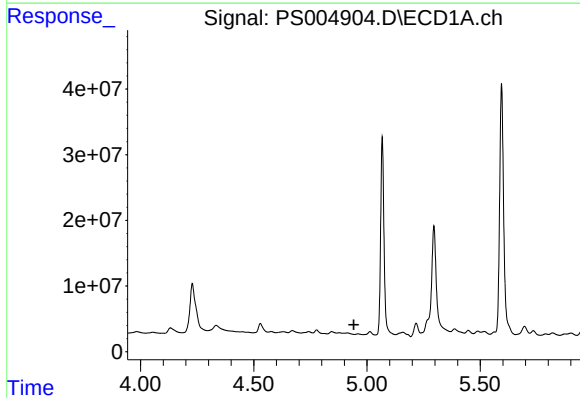


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

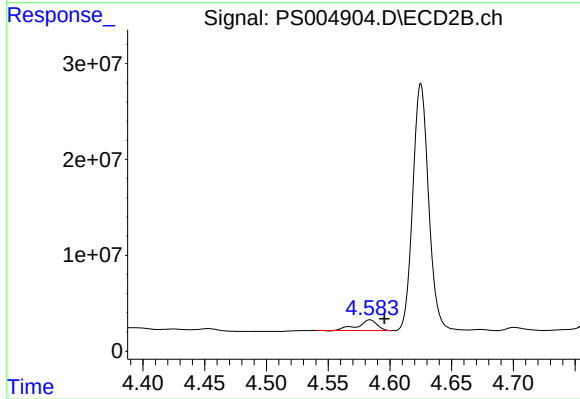

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.584 min
Delta R.T.: -0.012 min
Response: 12137295
Conc: 9.85 ng/ml

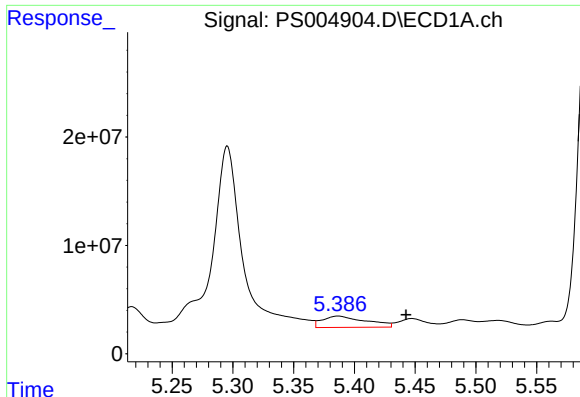

#3 4-Nitrophenol


R.T.: 5.387 min
Delta R.T.: -0.056 min
Response: 26258608
Conc: 42.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-E

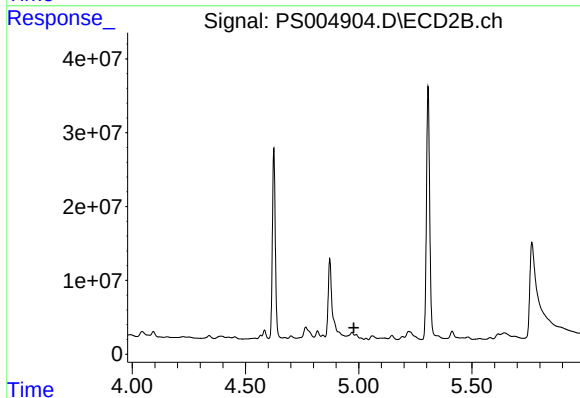


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

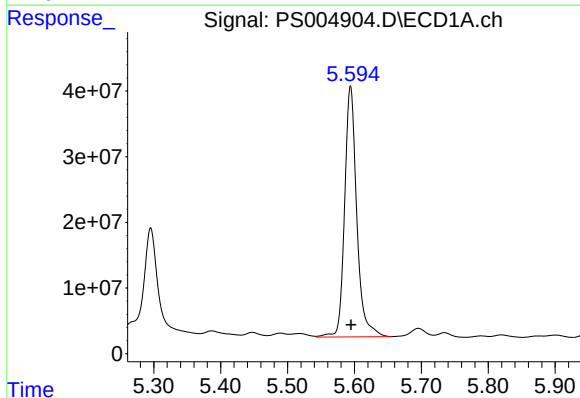


#4 2,4-DCAA

R.T.: 5.594 min
Delta R.T.: 0.000 min
Response: 481692989
Conc: 343.64 ng/ml

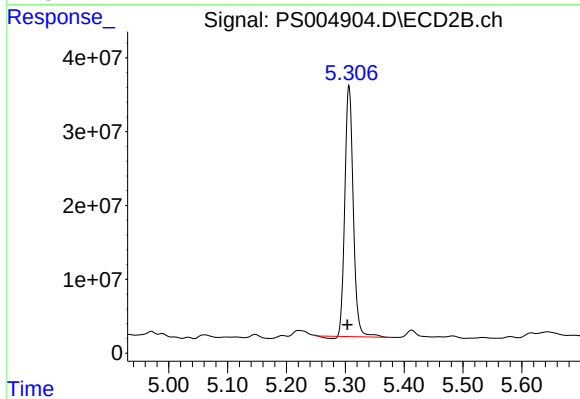

#4 2,4-DCAA


R.T.: 5.306 min
Delta R.T.: 0.003 min
Response: 337574047
Conc: 349.88 ng/ml

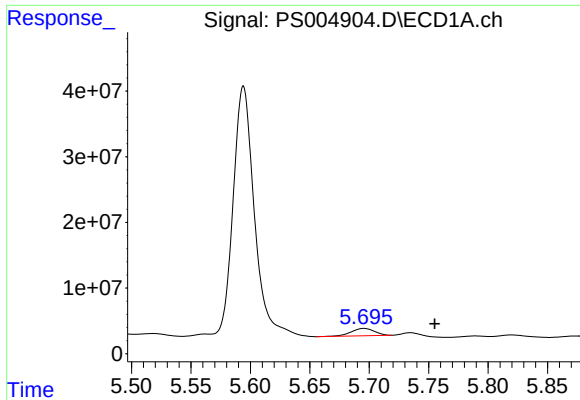

#5 DICAMBA


R.T.: 5.696 min
Delta R.T.: -0.059 min
Response: 15267023
Conc: 2.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-E

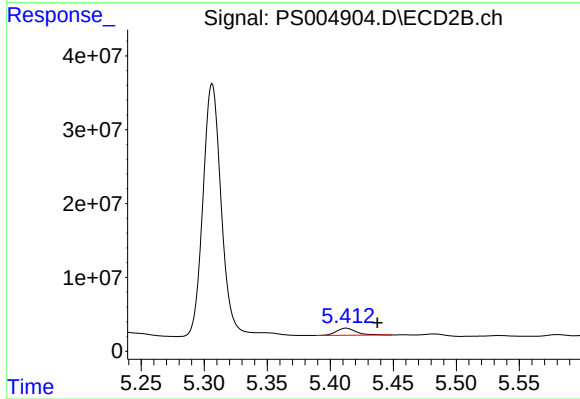


#5 DICAMBA

R.T.: 5.413 min
Delta R.T.: -0.025 min
Response: 10639048
Conc: 2.88 ng/ml

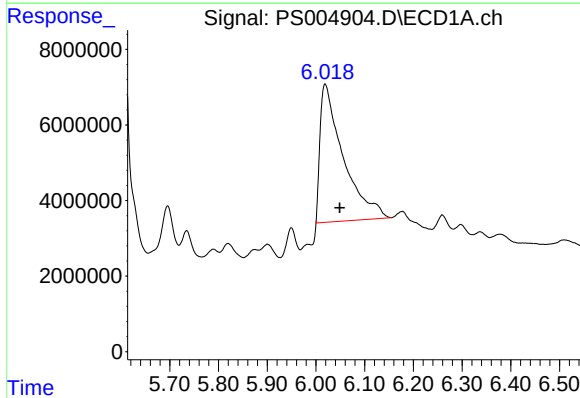


#7 MCPA

R.T.: 6.019 min
Delta R.T.: -0.030 min
Response: 120397628
Conc: 20.79 ug/ml

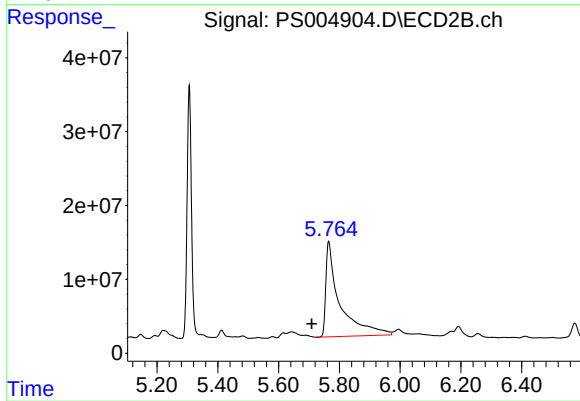

#7 MCPA


R.T.: 5.765 min
Delta R.T.: 0.056 min
Response: 414030230
Conc: 101.19 ug/ml

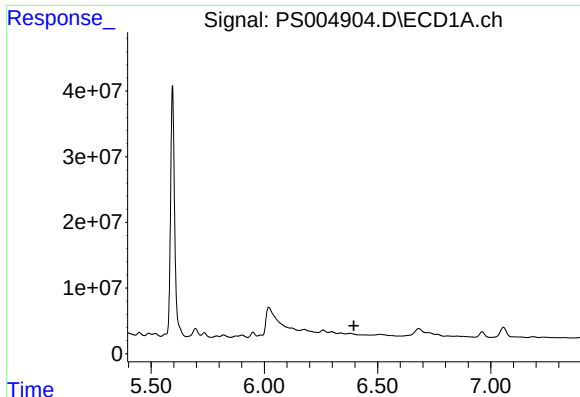

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-E

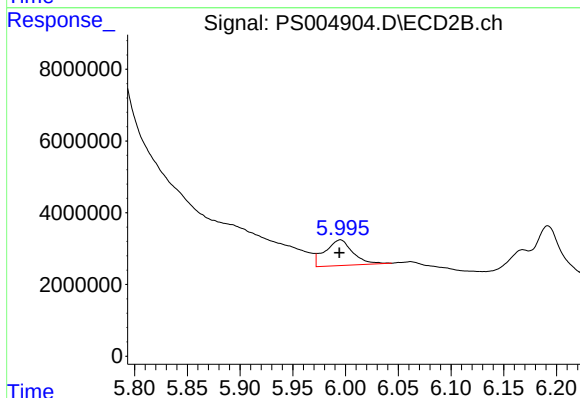


#8 DICHLORPROP

R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 13154431
Conc: 13.95 ng/ml

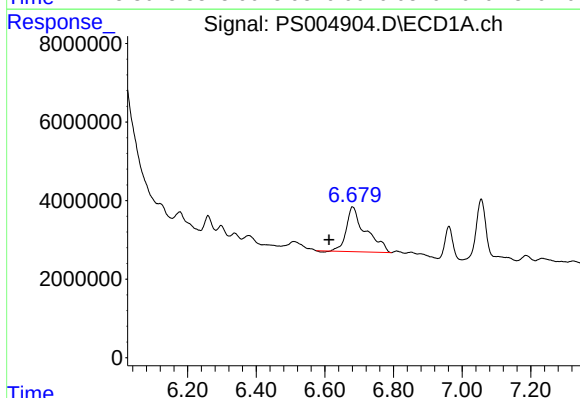


#9 2,4-D

R.T.: 6.681 min
Delta R.T.: 0.069 min
Response: 44435047
Conc: 32.48 ng/ml

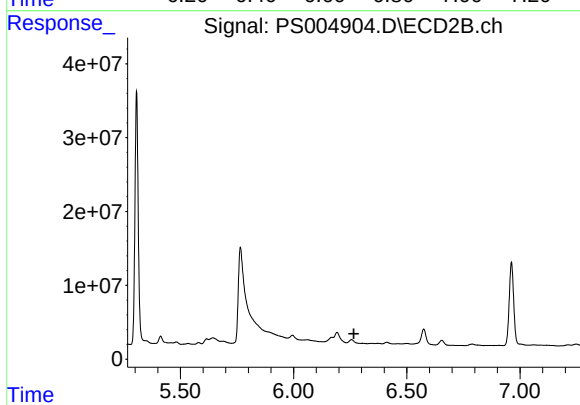

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

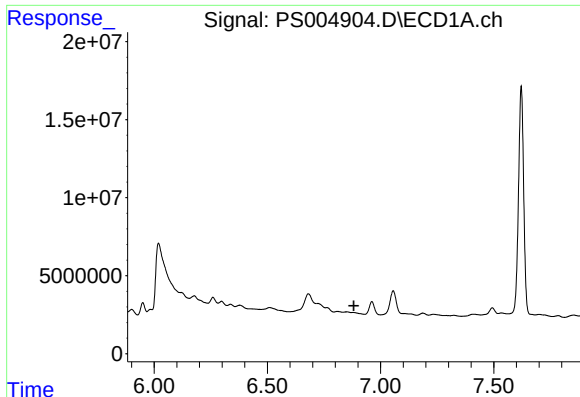

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-053119-E

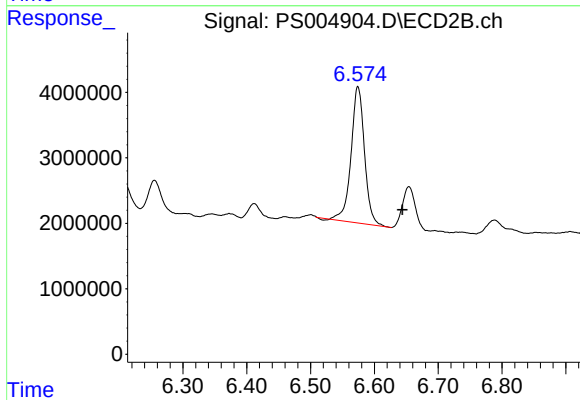


#10 Pentachlorophenol

R.T.: 6.574 min
Delta R.T.: -0.069 min
Response: 30629283
Conc: 2.49 ng/ml

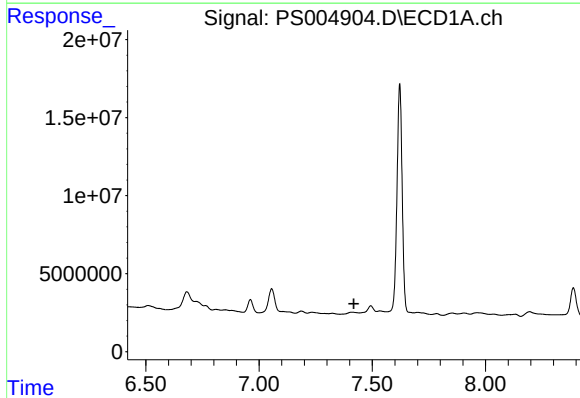

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

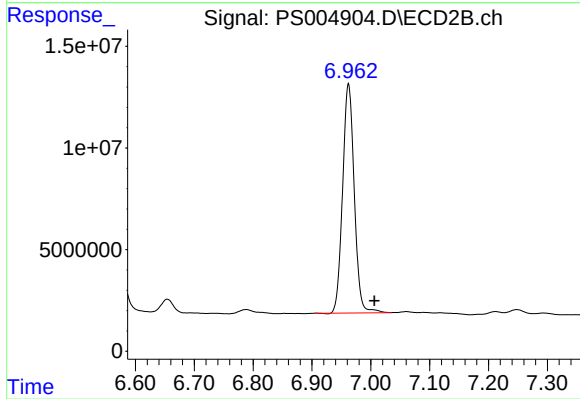

#11 2,4,5-TP (SILVEX)

R.T.: 6.962 min
Delta R.T.: -0.044 min
Response: 155012572
Conc: 30.13 ng/ml