

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
 Data File : PS004908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 19:24
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:35:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.588	5.300	699.1E6	517.7E6	498.744	536.531
Target Compounds							
2) T	3,5-DICHL...	4.954	0.000	36772197	0	21.323	N.D. #
5) T	DICAMBA	0.000	5.455	0	40501715	N.D.	10.964
6) T	MCP	5.981	5.455	6951389	40501715	1.670	14.782 #
7) T	MCPA	5.981	0.000	6951389	0	1.200	N.D. #
8) T	DICHLORPROP	0.000	5.993	0	25299136	N.D.	26.833
9) T	2,4-D	6.629	0.000	141.9E6	0	103.771	N.D. #
15) T	Picloram	9.124	9.118	771.5E6	16431486	74.044	2.202 #
16) T	DCPA	0.000	9.118	0	16431486	N.D.	2.536



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
Data File : PS004908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 19:24
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:35:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

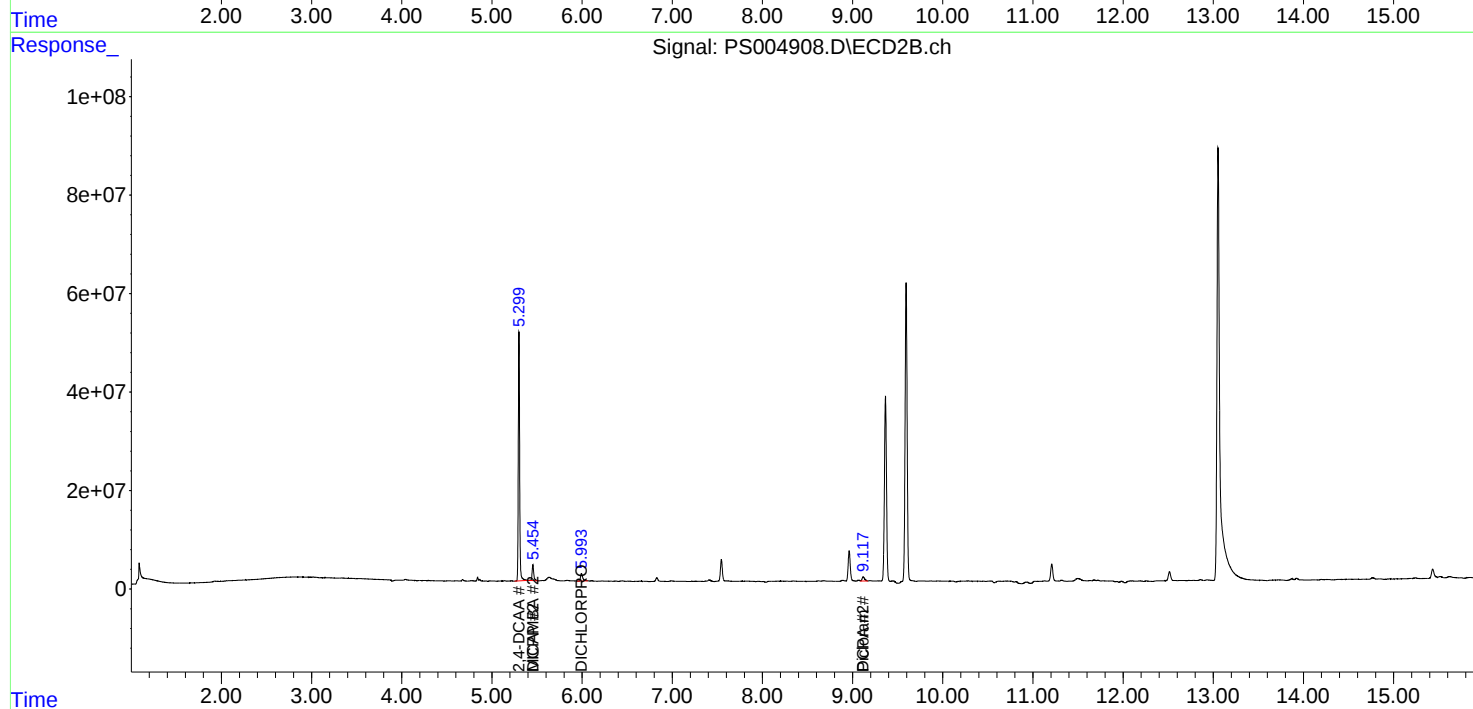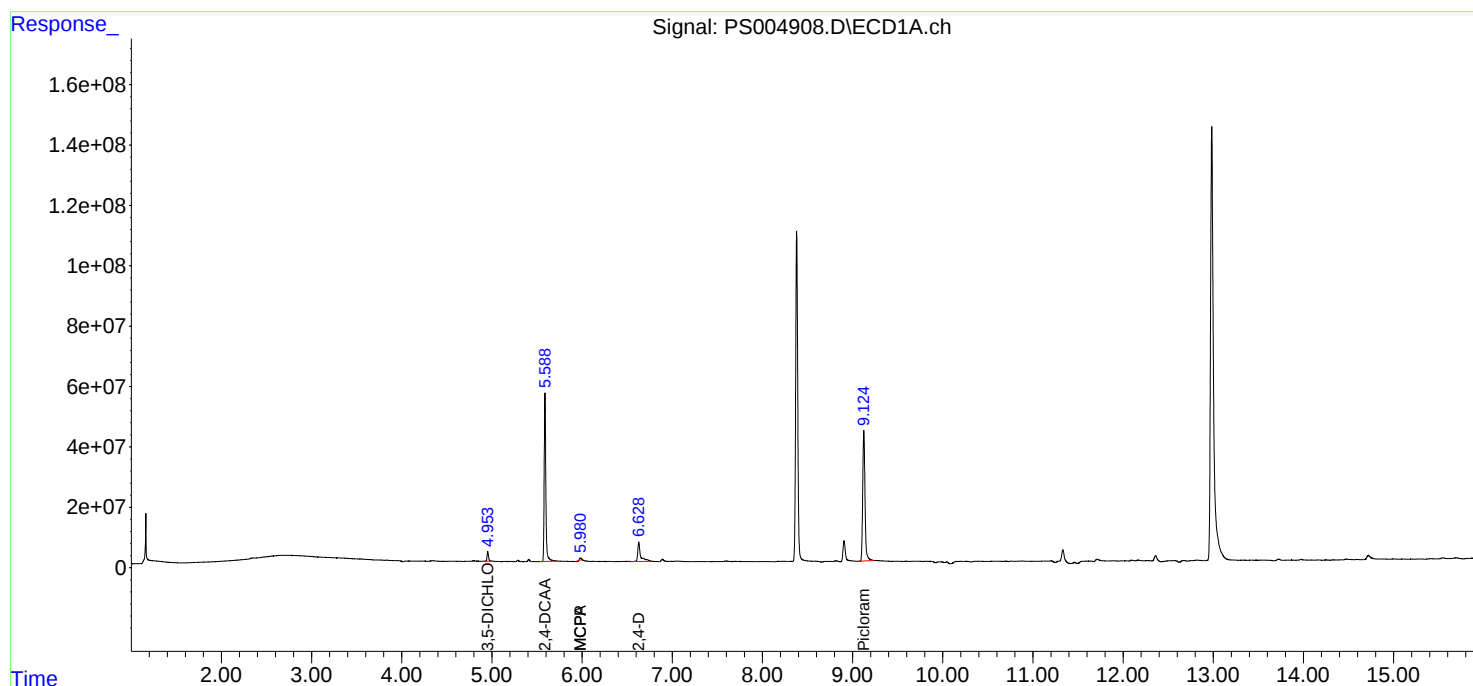


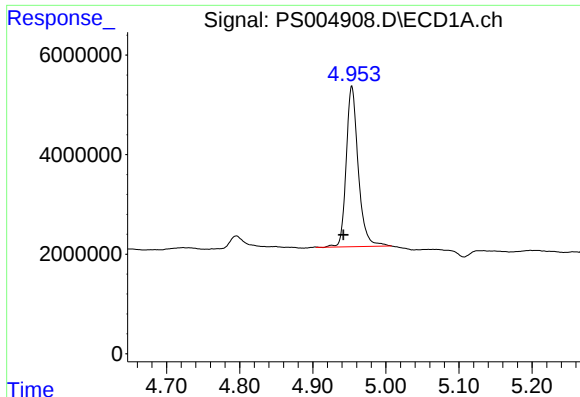

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.954 min
Delta R.T.: 0.011 min
Response: 36772197
Conc: 21.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

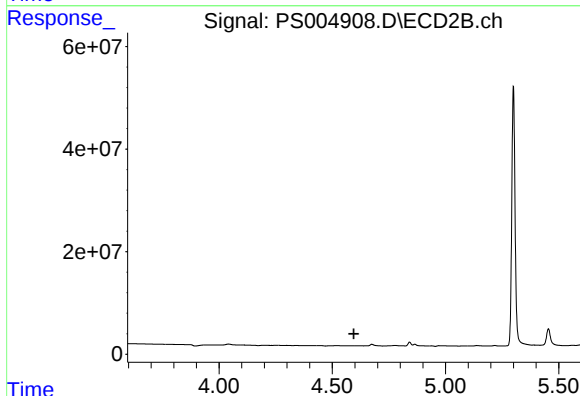


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

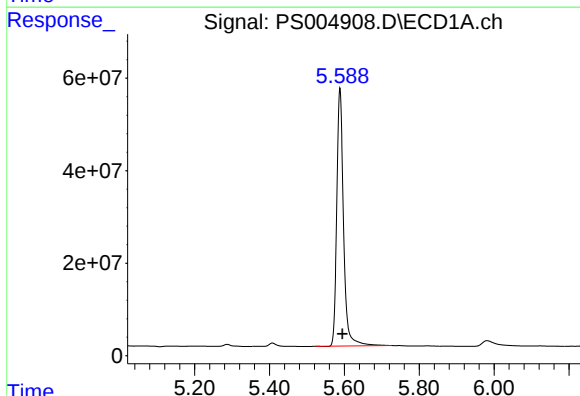


#4 2,4-DCAA

R.T.: 5.588 min
Delta R.T.: -0.007 min
Response: 699116971
Conc: 498.74 ng/ml

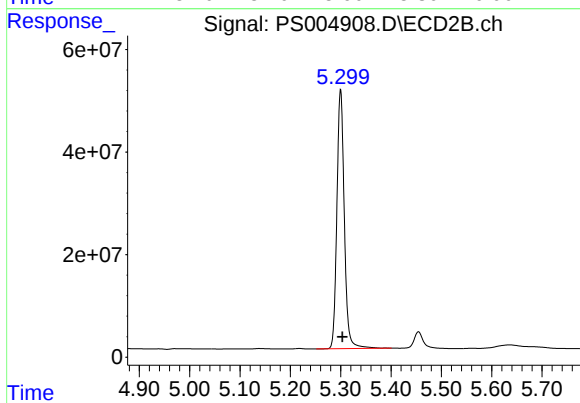

#4 2,4-DCAA


R.T.: 5.300 min
Delta R.T.: -0.004 min
Response: 517664439
Conc: 536.53 ng/ml

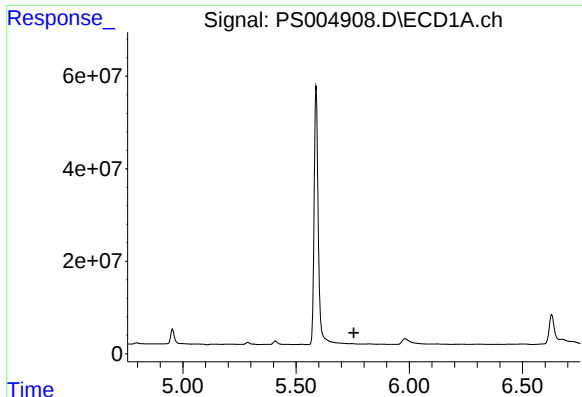

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

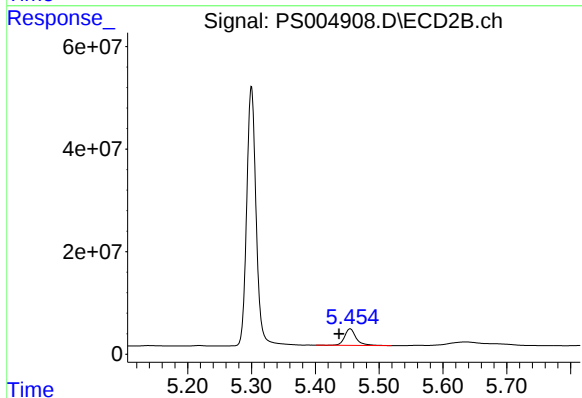


#5 DICAMBA

R.T.: 5.455 min
Delta R.T.: 0.017 min
Response: 40501715
Conc: 10.96 ng/ml

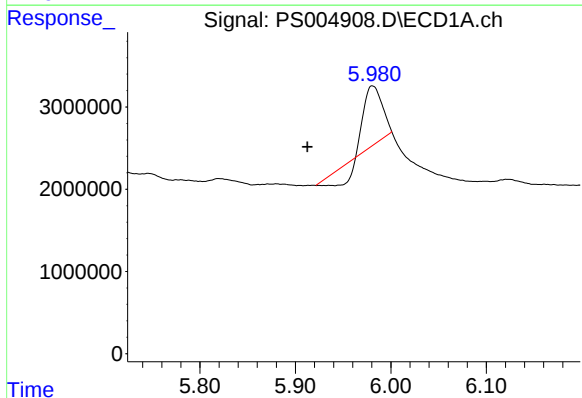


#6 MCP

R.T.: 5.981 min
Delta R.T.: 0.069 min
Response: 6951389
Conc: 1.67 ug/ml

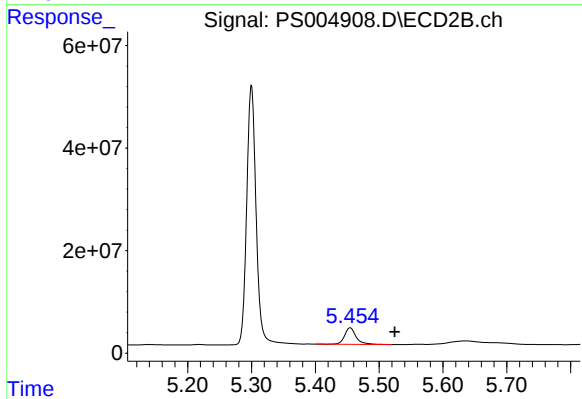

#6 MCP


R.T.: 5.455 min
Delta R.T.: -0.070 min
Response: 40501715
Conc: 14.78 ug/ml

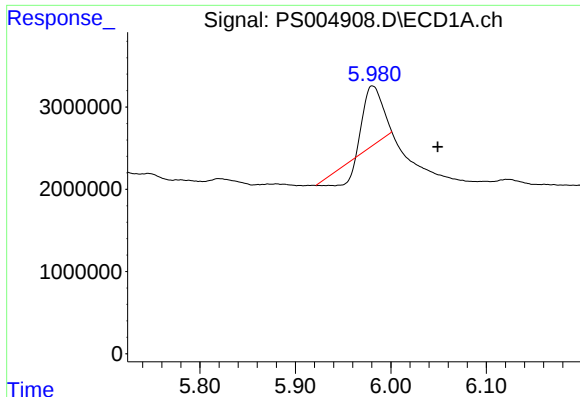

#7 MCPA


R.T.: 5.981 min
Delta R.T.: -0.068 min
Response: 6951389
Conc: 1.20 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

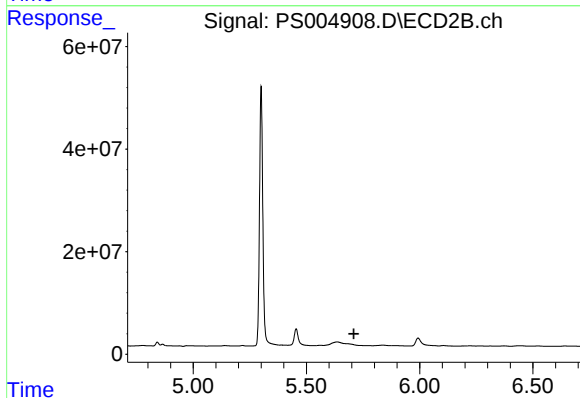


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.709 min
Response: 0
Conc: N.D.

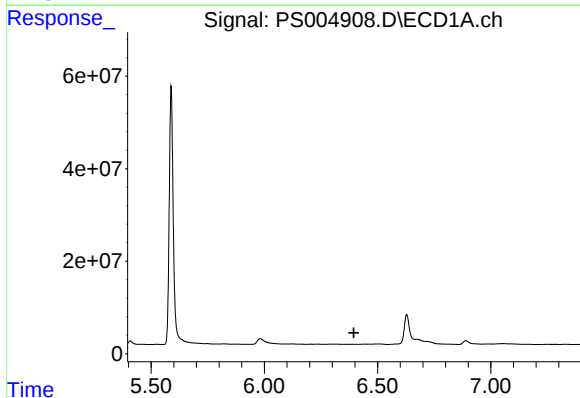


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

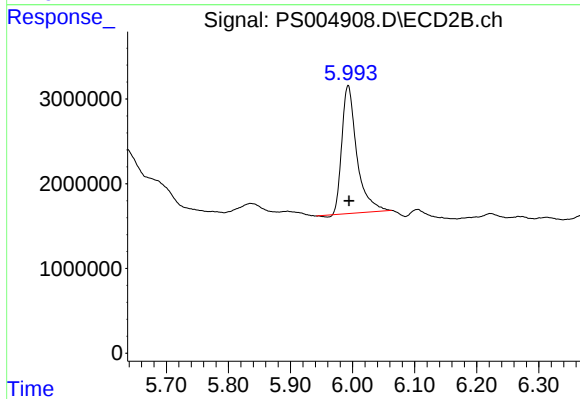

#8 DICHLORPROP


R.T.: 5.993 min
Delta R.T.: -0.001 min
Response: 25299136
Conc: 26.83 ng/ml

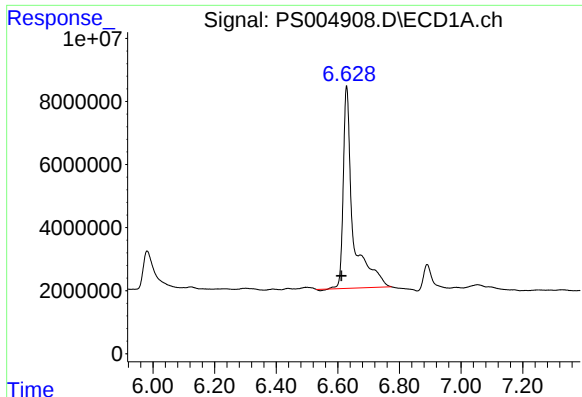

#9 2,4-D


R.T.: 6.629 min
Delta R.T.: 0.017 min
Response: 141948972
Conc: 103.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

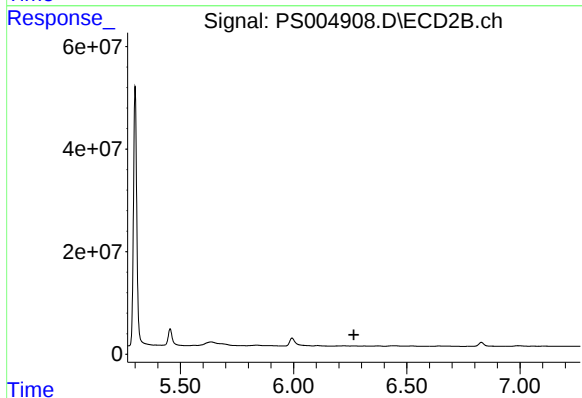


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

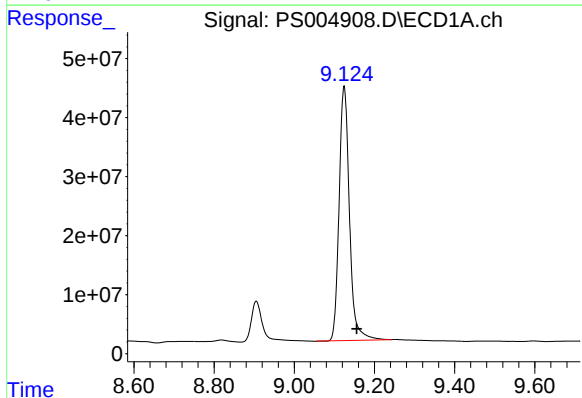


#15 Picloram

R.T.: 9.124 min
Delta R.T.: -0.031 min
Response: 771543484
Conc: 74.04 ng/ml

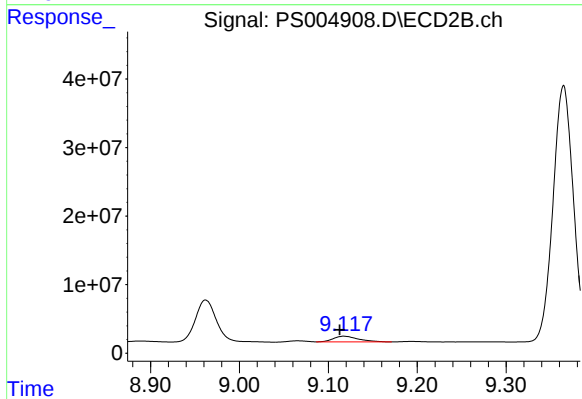

#15 Picloram


R.T.: 9.118 min
Delta R.T.: 0.005 min
Response: 16431486
Conc: 2.20 ng/ml

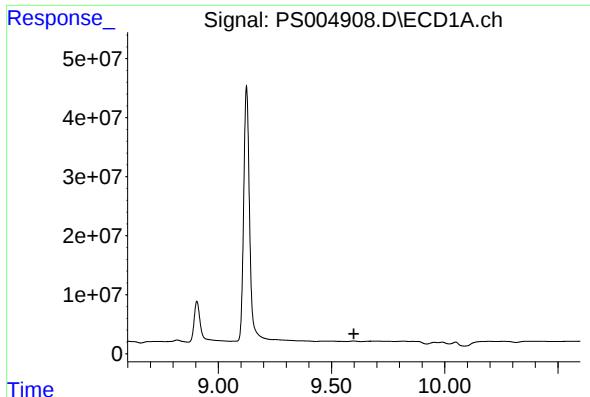

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

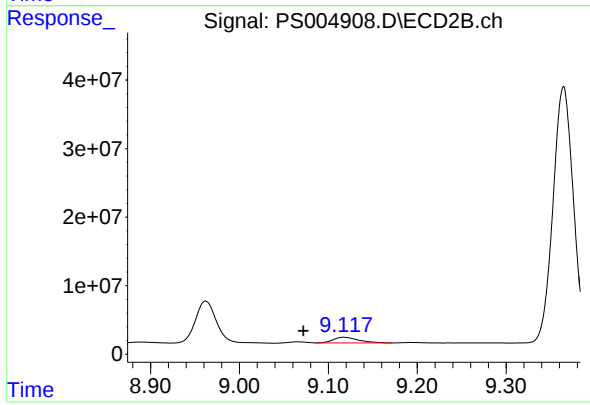

#16 DCPA

R.T.: 9.118 min
Delta R.T.: 0.046 min
Response: 16431486
Conc: 2.54 ng/ml