

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
 Data File : PS004914.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 21:36
 Operator : SM\AJ
 Sample : K3110-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-01-B1-C1-B1A-C1A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:37:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.593	5.304	387.1E6	243.8E6	276.145	252.638
Target Compounds							
1) T	Dalapon	2.094	0.000	40987930	0	24.726	N.D. #
2) T	3,5-DICHL...	0.000	4.623	0	204.8E6	N.D.	166.237
3) T	4-Nitroph...	5.396	0.000	39320346	0	63.063	N.D. #
5) T	DICAMBA	5.694	0.000	26718731	0	5.032	N.D. #
7) T	MCPA	6.086	5.696	19196420	28682139	3.314	7.010 #
9) T	2,4-D	6.681	0.000	15349162	0	11.221	N.D. #
11) T	2,4,5-TP ...	0.000	6.960	0	71382156	N.D.	13.873
13) T	2,4-DB	8.241	7.864	178.8E6	38422698	185.152	58.785 #
14) T	DINOSEB	0.000	8.169	0	35288182	N.D.	9.180



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
Data File : PS004914.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 21:36
Operator : SM\AJ
Sample : K3110-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B1-C1-B1A-C1A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:37:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

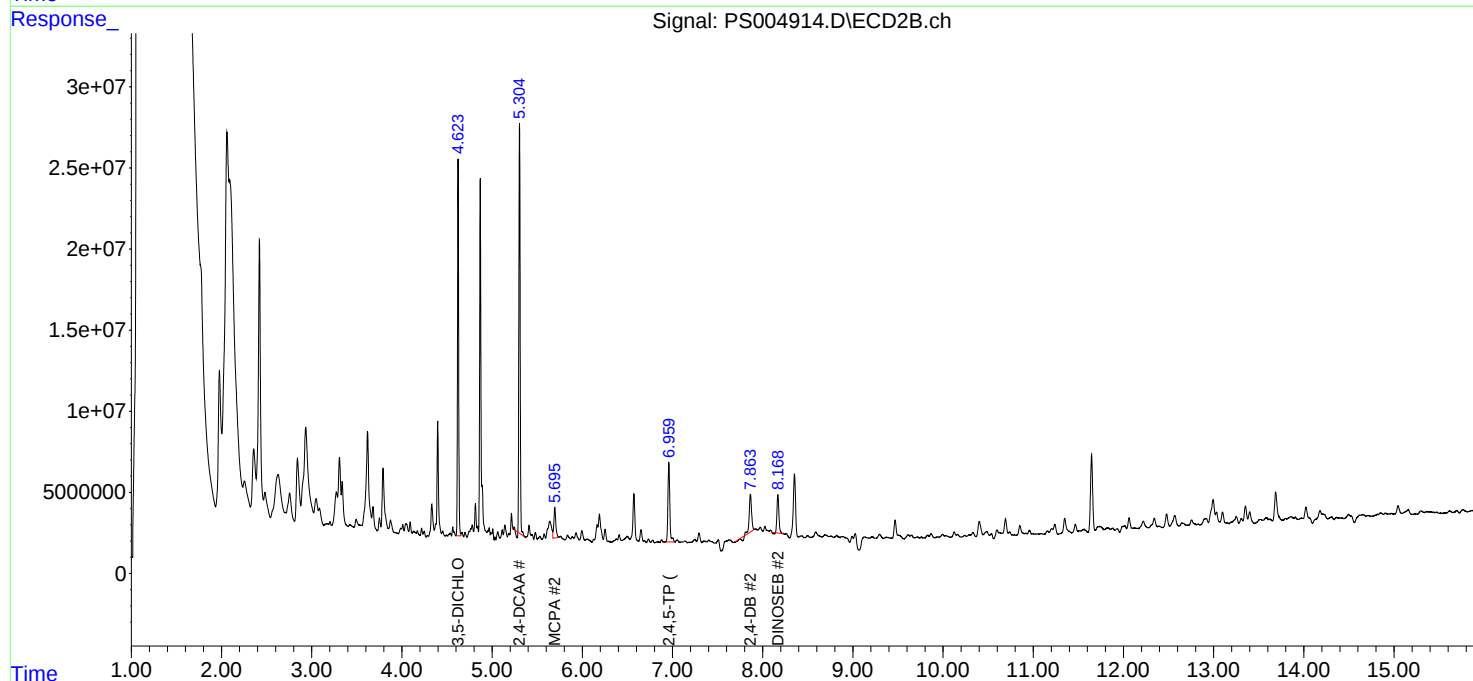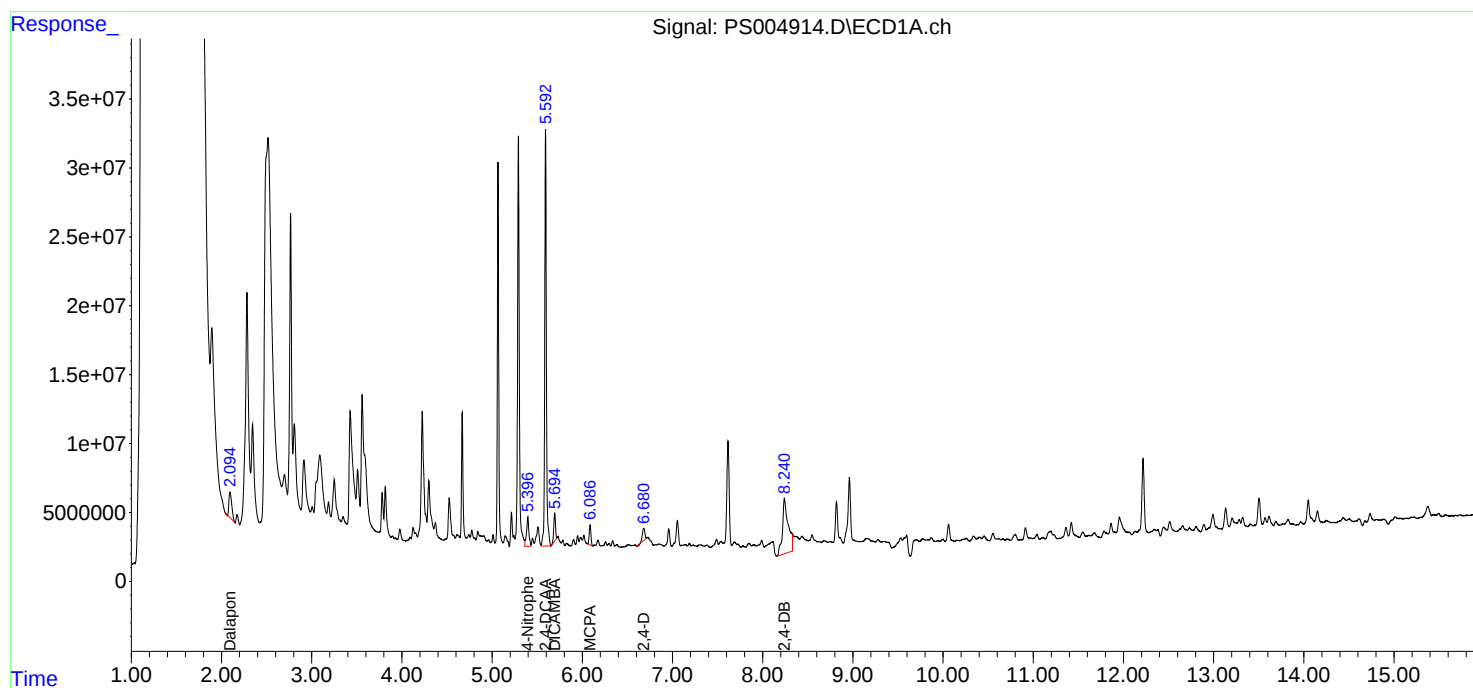


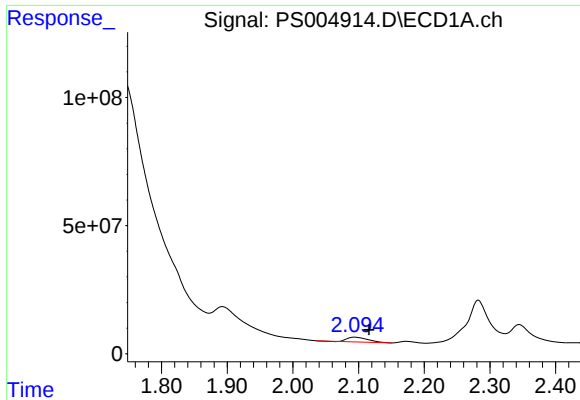

#1 Dalapon


R.T.: 2.094 min
Delta R.T.: -0.022 min
Response: 40987930
Conc: 24.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B1-C1-B1A-C1A

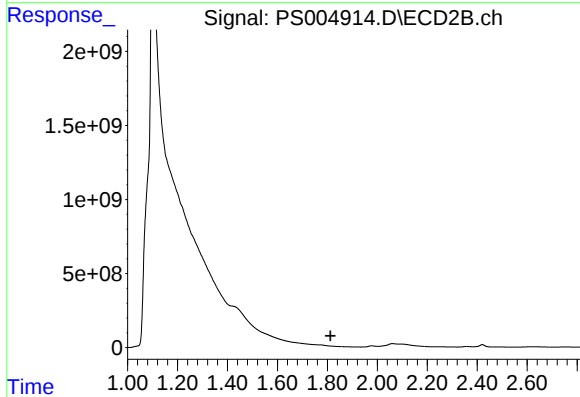


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

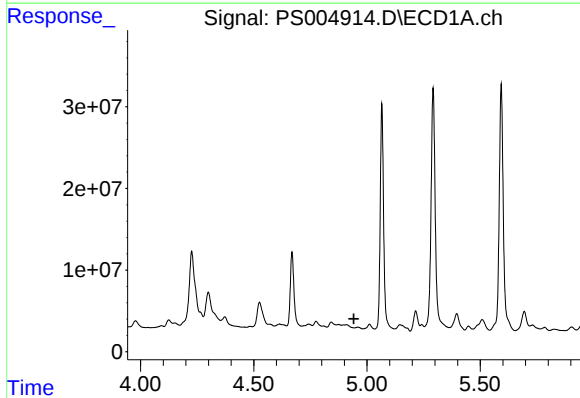


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

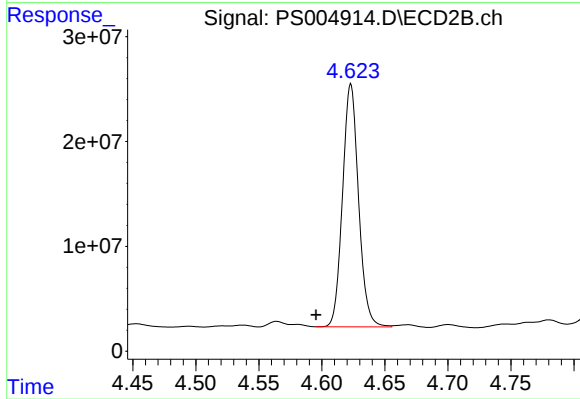

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.623 min
Delta R.T.: 0.027 min
Response: 204825569
Conc: 166.24 ng/ml

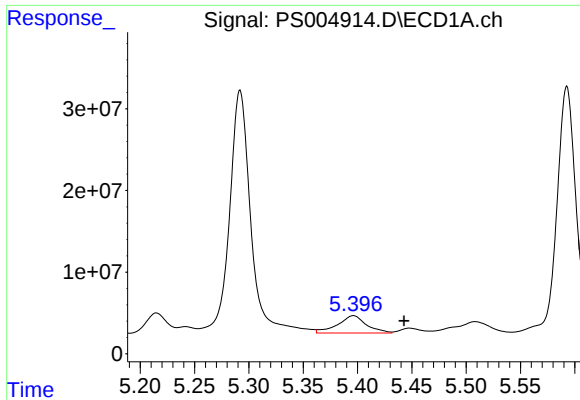

#3 4-Nitrophenol


R.T.: 5.396 min
Delta R.T.: -0.047 min
Response: 39320346
Conc: 63.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B1-C1-B1A-C1A

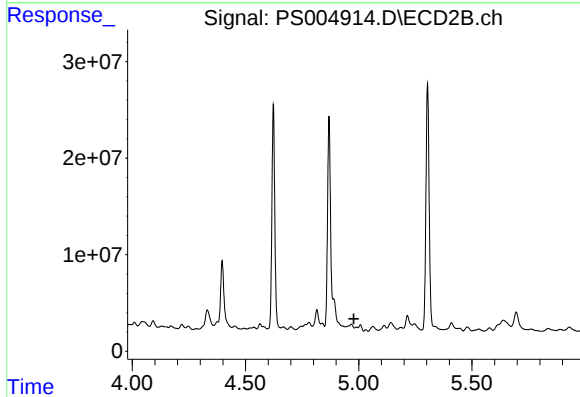


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

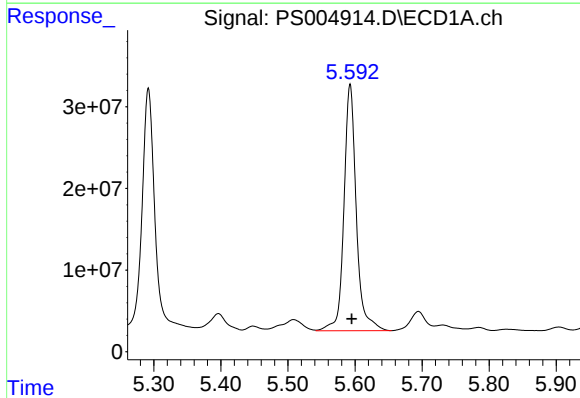


#4 2,4-DCAA

R.T.: 5.593 min
Delta R.T.: -0.002 min
Response: 387087279
Conc: 276.14 ng/ml

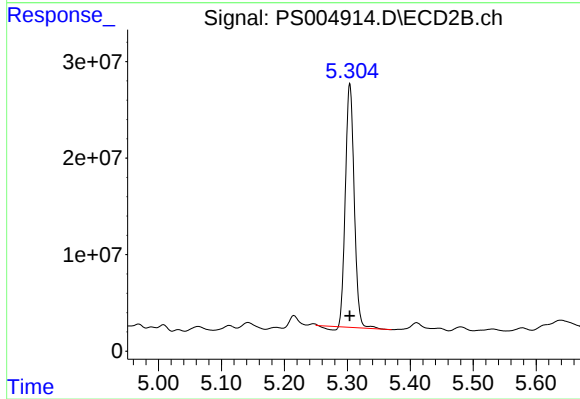

#4 2,4-DCAA


R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 243754219
Conc: 252.64 ng/ml

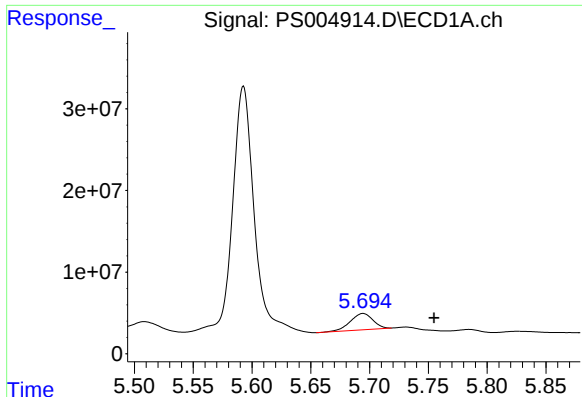

#5 DICAMBA


R.T.: 5.694 min
Delta R.T.: -0.061 min
Response: 26718731
Conc: 5.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B1-C1-B1A-C1A

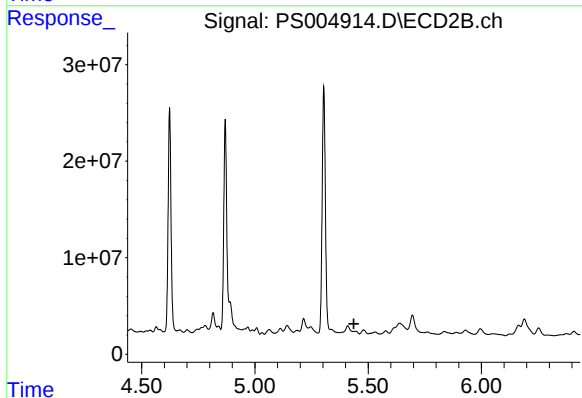


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.437 min
Response: 0
Conc: N.D.

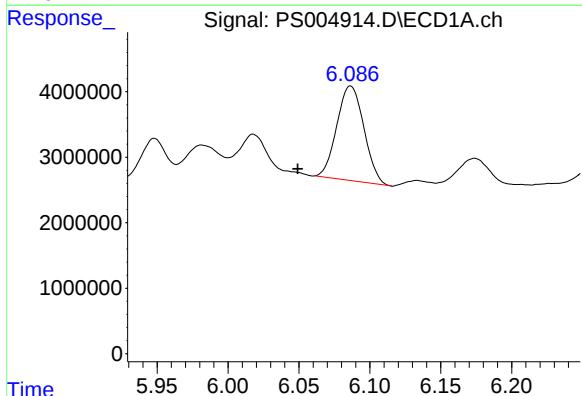


#7 MCPA

R.T.: 6.086 min
Delta R.T.: 0.037 min
Response: 19196420
Conc: 3.31 ug/ml

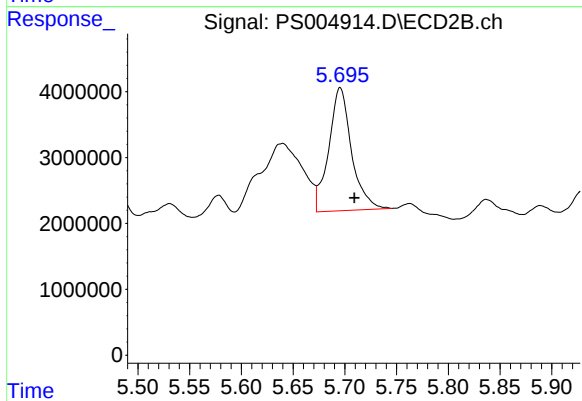

#7 MCPA


R.T.: 5.696 min
Delta R.T.: -0.014 min
Response: 28682139
Conc: 7.01 ug/ml

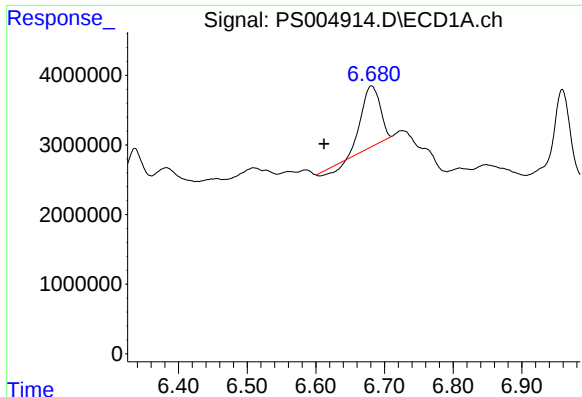

#9 2,4-D


R.T.: 6.681 min
Delta R.T.: 0.069 min
Response: 15349162
Conc: 11.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B1-C1-B1A-C1A

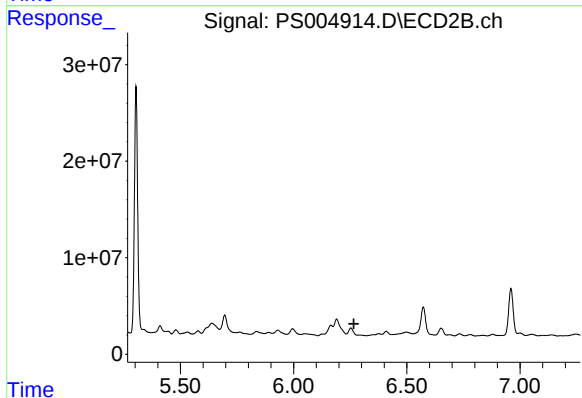


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

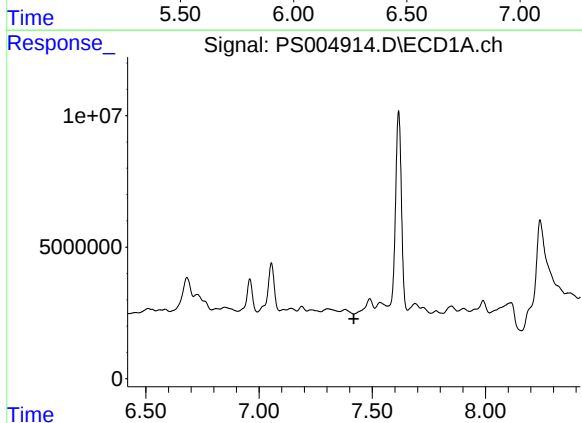


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

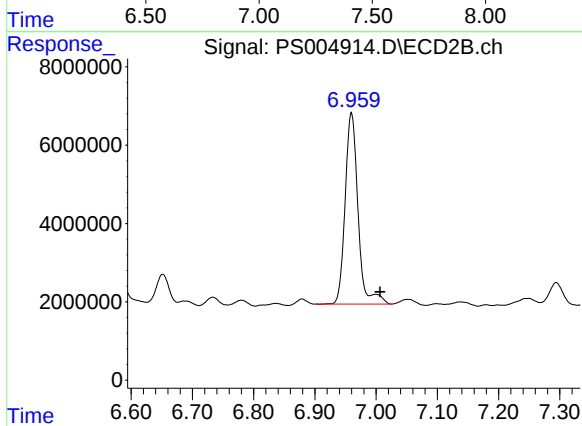

#11 2,4,5-TP (SILVEX)


R.T.: 6.960 min
Delta R.T.: -0.046 min
Response: 71382156
Conc: 13.87 ng/ml

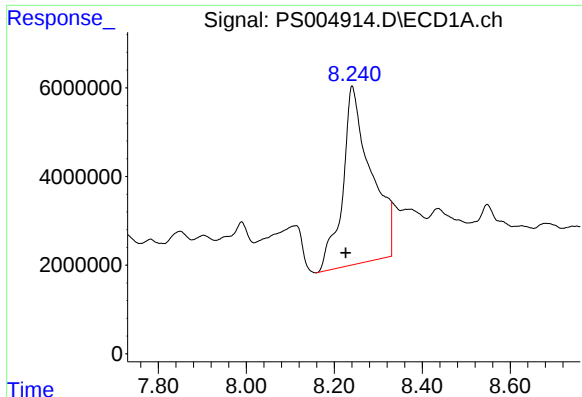

#13 2,4-DB


R.T.: 8.241 min
Delta R.T.: 0.014 min
Response: 178849566
Conc: 185.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-B1-C1-B1A-C1A

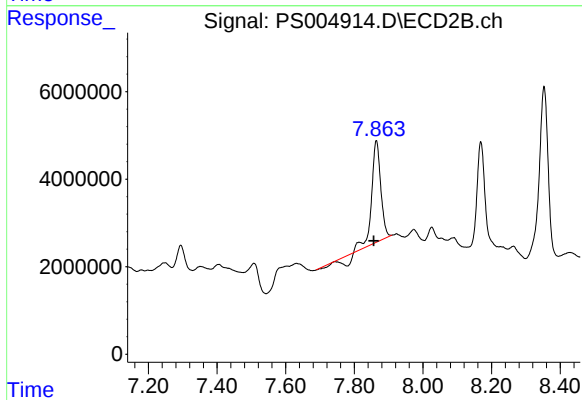


#13 2,4-DB

R.T.: 7.864 min
Delta R.T.: 0.008 min
Response: 38422698
Conc: 58.78 ng/ml

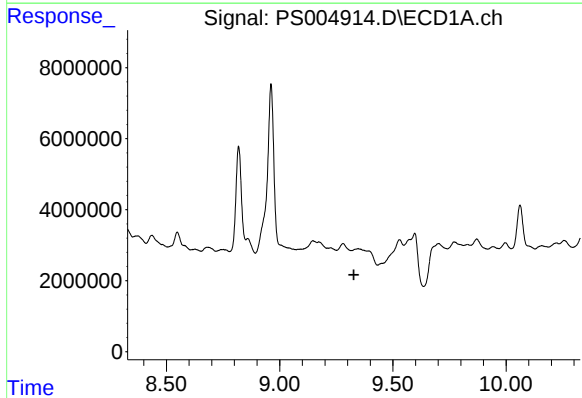

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.328 min
Response: 0
Conc: N.D.

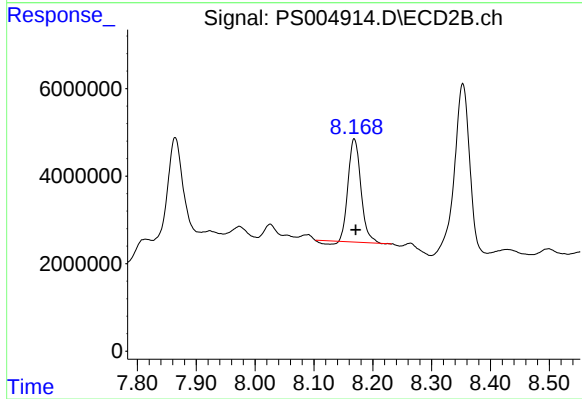

#14 DINOSEB

R.T.: 8.169 min
Delta R.T.: -0.002 min
Response: 35288182
Conc: 9.18 ng/ml