

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
 Data File : PS004915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 21:58
 Operator : SM\AJ
 Sample : K3111-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-01-D1-D2-D1A-D2A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:37:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.588	5.300	406.5E6	267.8E6	289.970	277.518
Target Compounds							
1) T	Dalapon	2.090	0.000	39078112	0	23.574	N.D. #
2) T	3,5-DICHL...	0.000	4.619	0	205.1E6	N.D.	166.480
3) T	4-Nitroph...	5.392	0.000	33563628	0	53.830	N.D. #
5) T	DICAMBA	5.690	0.000	25051127	0	4.718	N.D. #
7) T	MCPA	6.082	5.692	20793928	26552053	3.590	6.489 #
9) T	2,4-D	6.677	0.000	17156224	0	12.542	N.D. #
11) T	2,4,5-TP ...	0.000	6.956	0	69406035	N.D.	13.489
13) T	2,4-DB	8.237	7.861	185.3E6	68555419	191.790	104.886 #
14) T	DINOSEB	0.000	8.164	0	41036235	N.D.	10.675



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
Data File : PS004915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 21:58
Operator : SM\AJ
Sample : K3111-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-D1-D2-D1A-D2A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:37:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

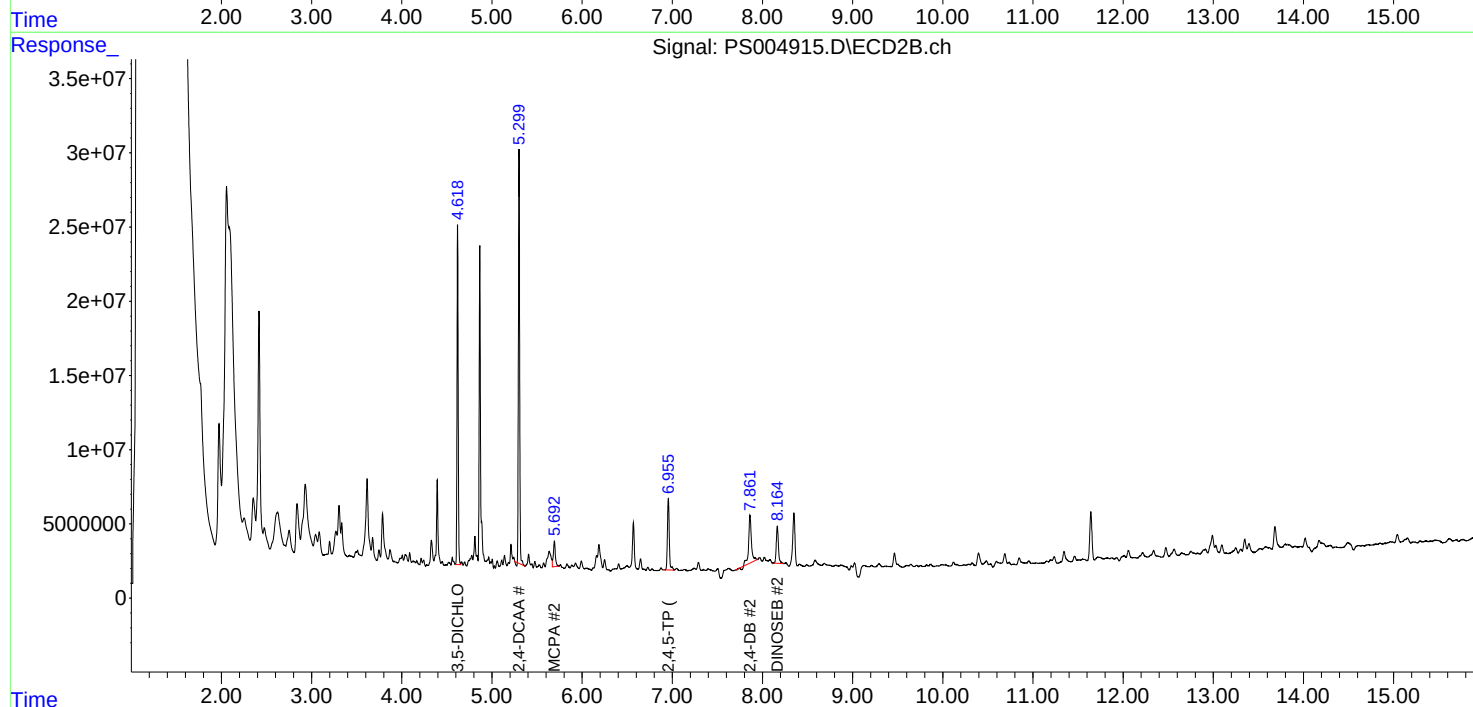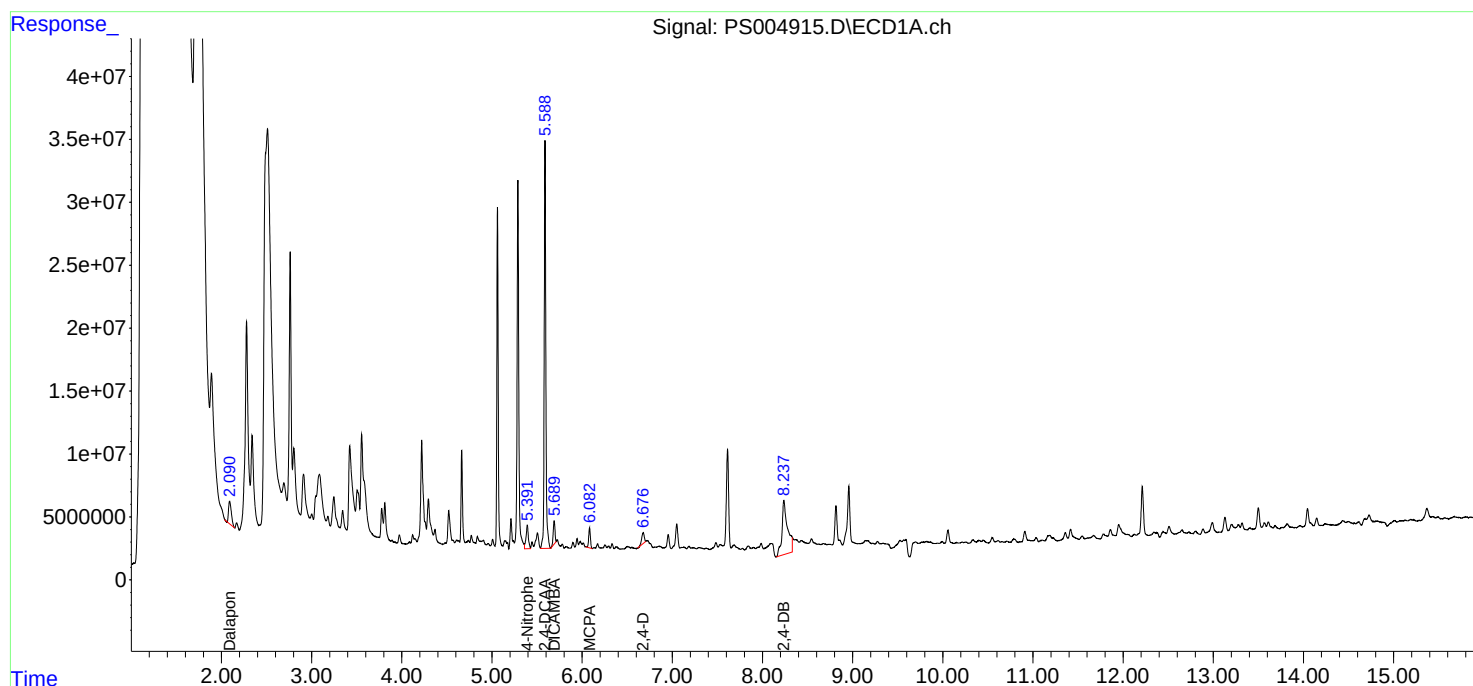


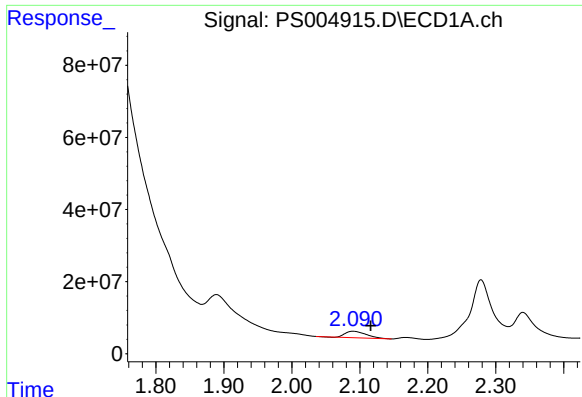

#1 Dalapon


R.T.: 2.090 min
Delta R.T.: -0.026 min
Response: 39078112
Conc: 23.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-D1-D2-D1A-D2A

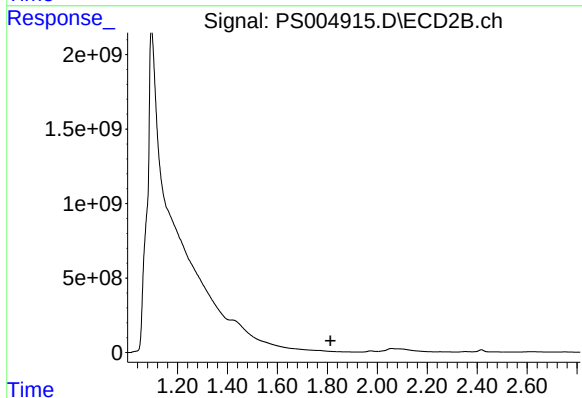


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

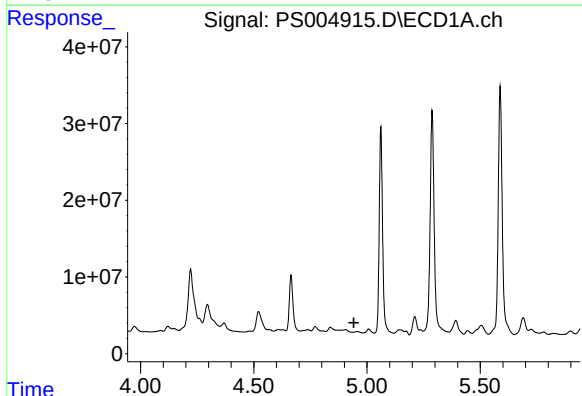


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

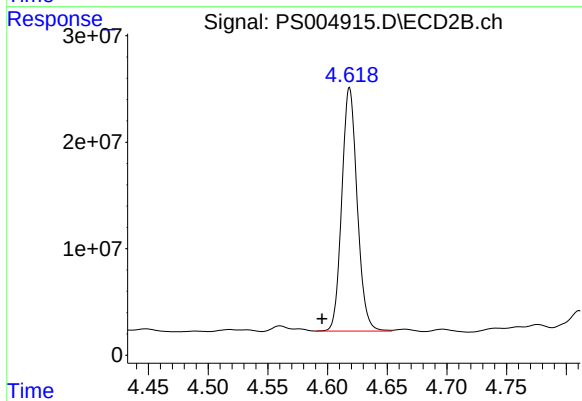

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.619 min
Delta R.T.: 0.023 min
Response: 205125210
Conc: 166.48 ng/ml

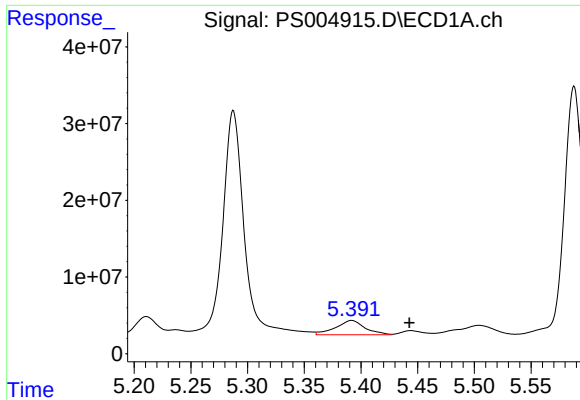

#3 4-Nitrophenol


R.T.: 5.392 min
Delta R.T.: -0.051 min
Response: 33563628
Conc: 53.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-D1-D2-D1A-D2A

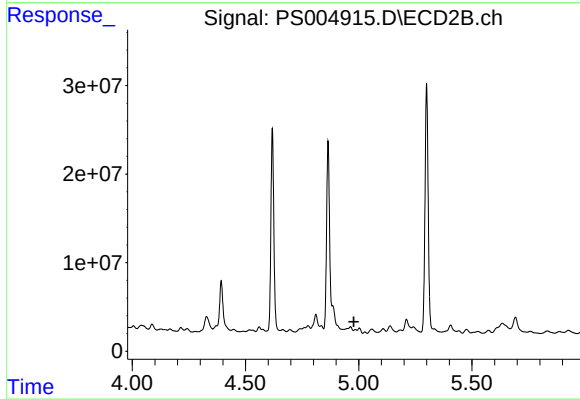


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

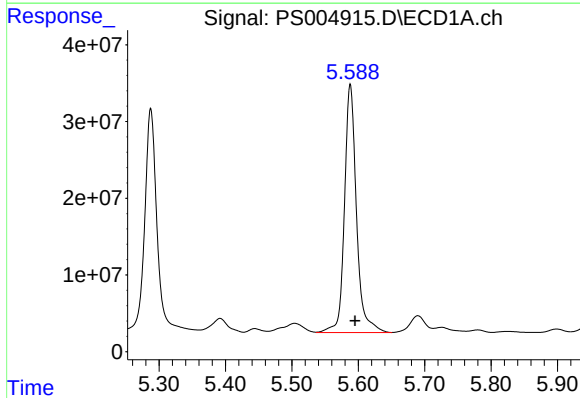


#4 2,4-DCAA

R.T.: 5.588 min
Delta R.T.: -0.007 min
Response: 406467187
Conc: 289.97 ng/ml

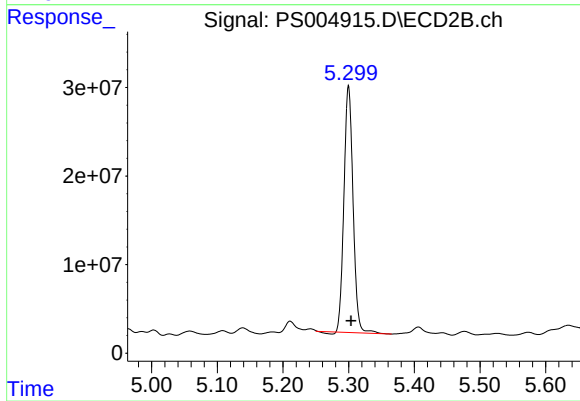

#4 2,4-DCAA


R.T.: 5.300 min
Delta R.T.: -0.004 min
Response: 267758910
Conc: 277.52 ng/ml

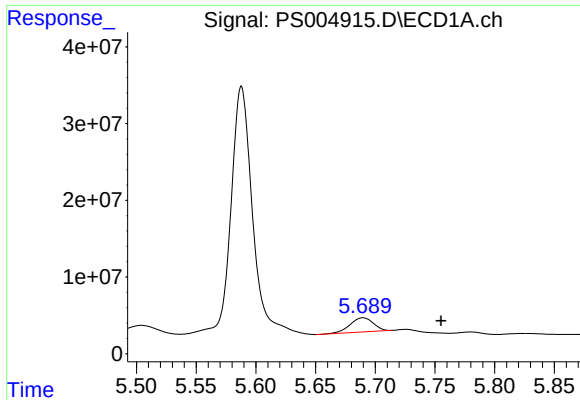

#5 DICAMBA


R.T.: 5.690 min
Delta R.T.: -0.065 min
Response: 25051127
Conc: 4.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-D1-D2-D1A-D2A

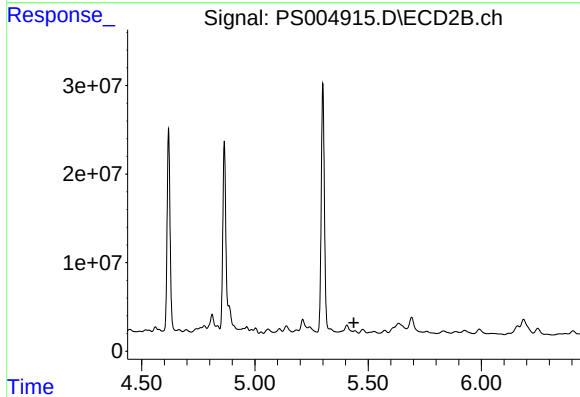


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.437 min
Response: 0
Conc: N.D.

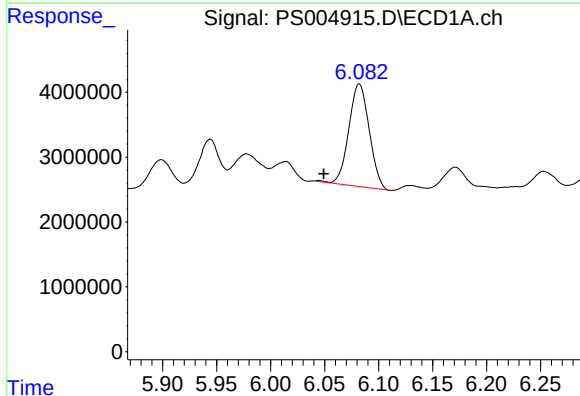


#7 MCPA

R.T.: 6.082 min
Delta R.T.: 0.033 min
Response: 20793928
Conc: 3.59 ug/ml

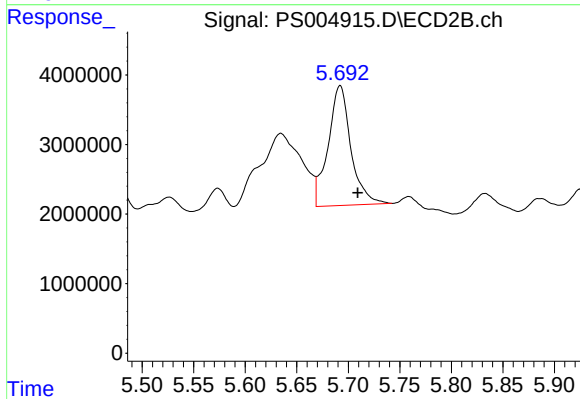

#7 MCPA


R.T.: 5.692 min
Delta R.T.: -0.017 min
Response: 26552053
Conc: 6.49 ug/ml

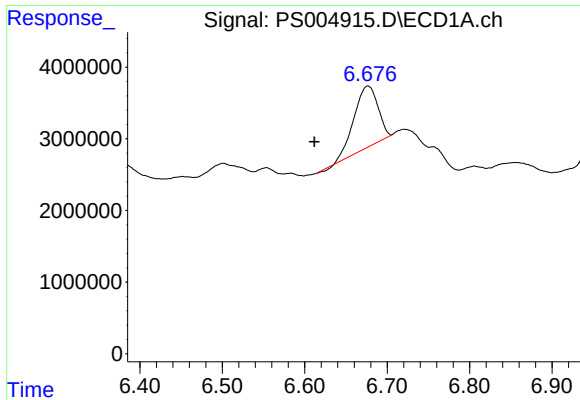

#9 2,4-D


R.T.: 6.677 min
Delta R.T.: 0.065 min
Response: 17156224
Conc: 12.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-D1-D2-D1A-D2A

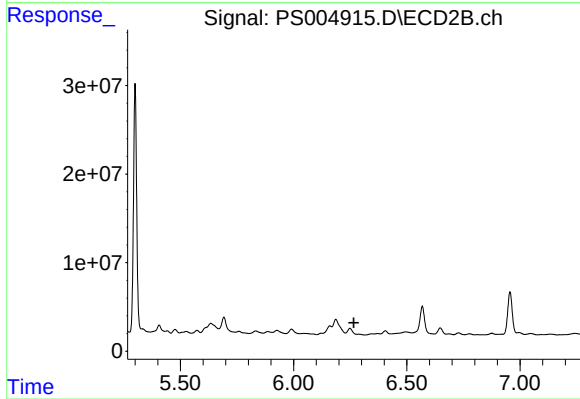


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

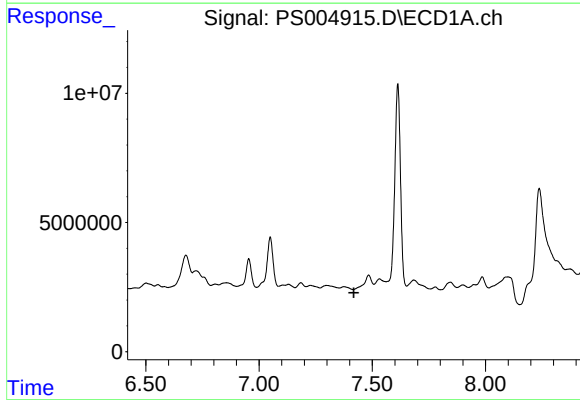


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

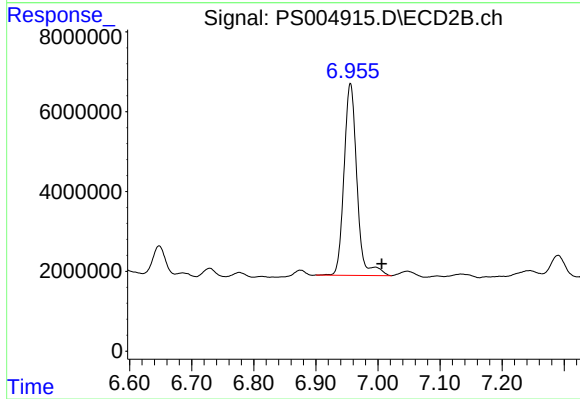

#11 2,4,5-TP (SILVEX)


R.T.: 6.956 min
Delta R.T.: -0.051 min
Response: 69406035
Conc: 13.49 ng/ml

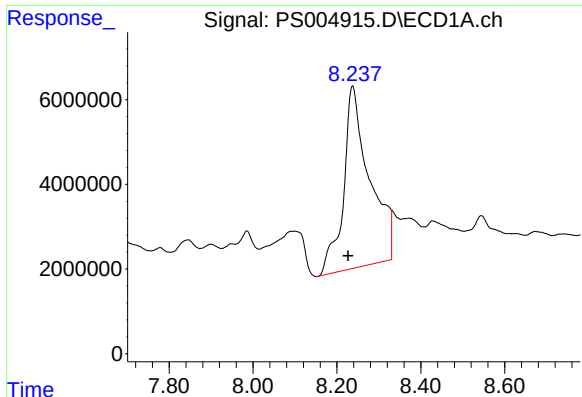

#13 2,4-DB


R.T.: 8.237 min
Delta R.T.: 0.011 min
Response: 185262014
Conc: 191.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-D1-D2-D1A-D2A

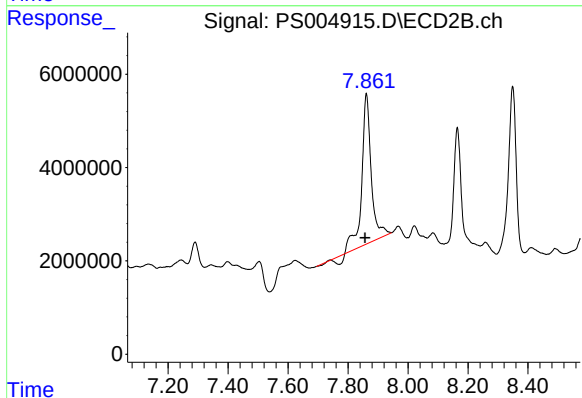


#13 2,4-DB

R.T.: 7.861 min
Delta R.T.: 0.005 min
Response: 68555419
Conc: 104.89 ng/ml

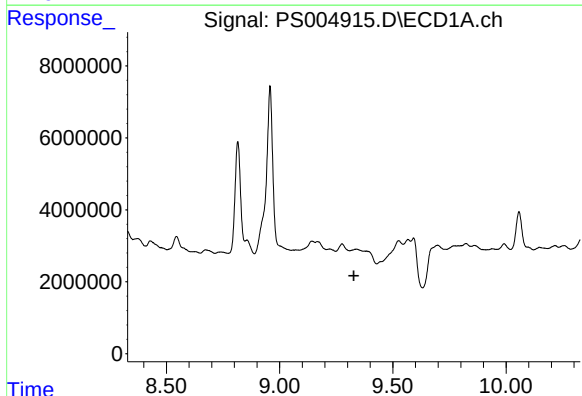

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.328 min
Response: 0
Conc: N.D.

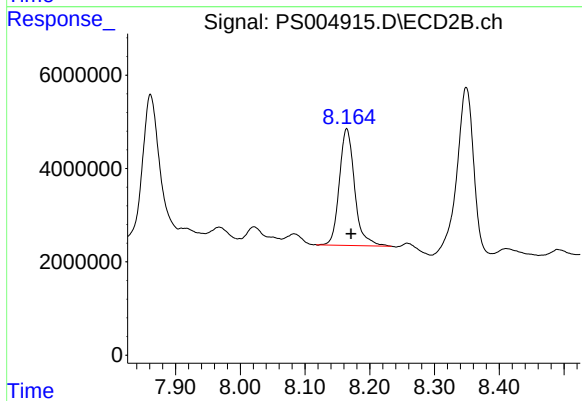

#14 DINOSEB

R.T.: 8.164 min
Delta R.T.: -0.007 min
Response: 41036235
Conc: 10.68 ng/ml