

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
 Data File : PS004922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2019 00:32
 Operator : SM\AJ
 Sample : K3175-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-03-007-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:40:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.590	5.303	339.0E6	227.8E6	241.844	236.134
Target Compounds							
2) T	3,5-DICHL...	0.000	4.622	0	221.3E6	N.D.	179.595
3) T	4-Nitroph...	5.394	0.000	31516324	0	50.547	N.D. #
5) T	DICAMBA	5.692	5.409	14698965	14989107	2.768	4.057 #
7) T	MCPA	6.017	5.696	15416316	24510738	2.662	5.990 #
8) T	DICHLORPROP	0.000	5.929	0	26848162	N.D.	28.476
9) T	2,4-D	6.677	0.000	5640222	0	4.123	N.D. #
10) T	Pentachlo...	6.868	0.000	15192775	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.959	0	86568287	N.D.	16.825
13) T	2,4-DB	8.240	7.864	100.9E6	42054506	104.488	64.341 #
14) T	DINOSEB	0.000	8.167	0	60532573	N.D.	15.747



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
Data File : PS004922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2019 00:32
Operator : SM\AJ
Sample : K3175-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-007-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:40:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

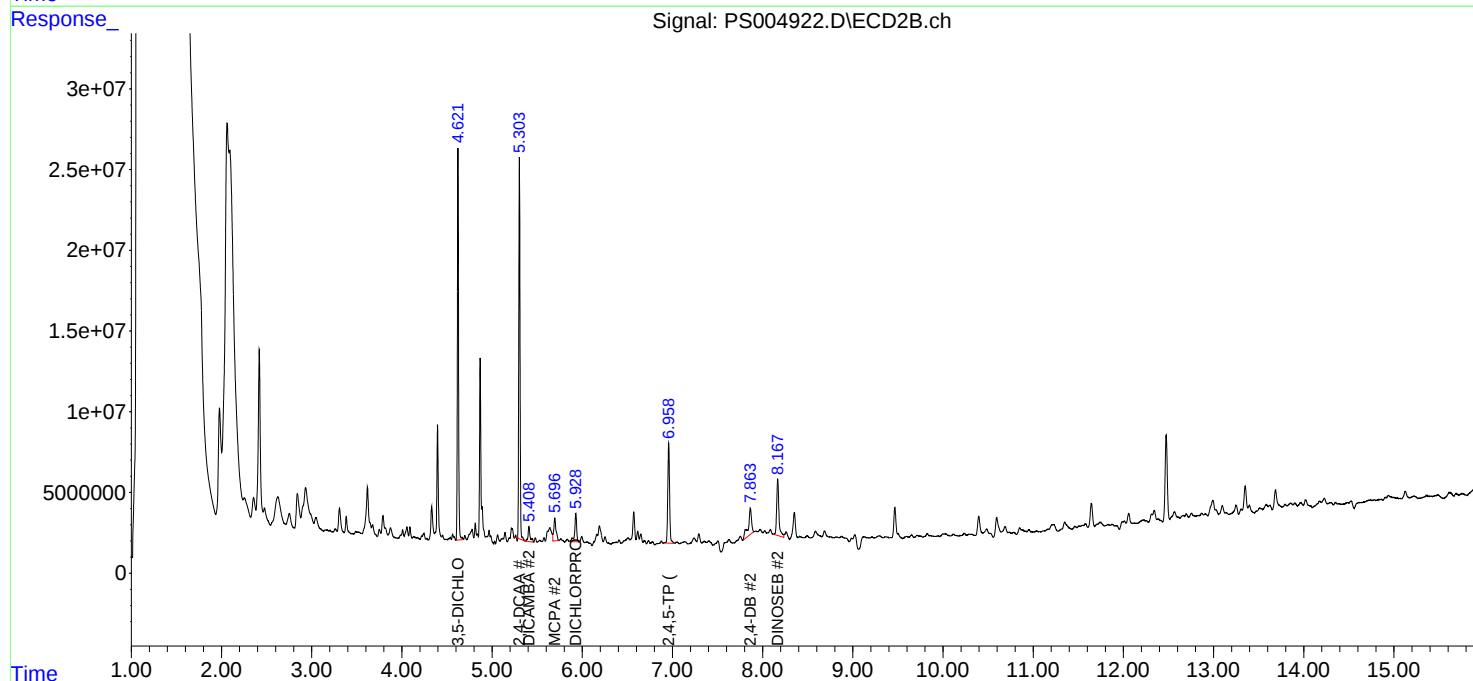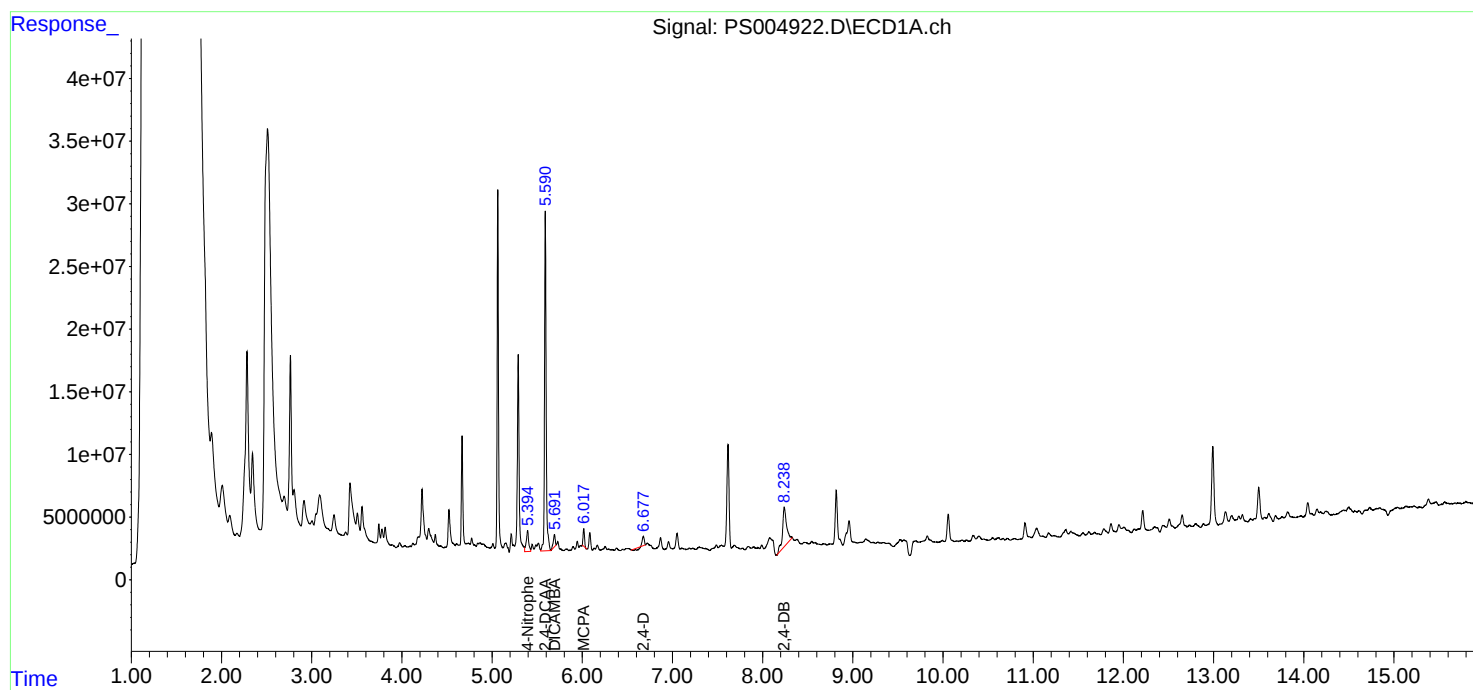


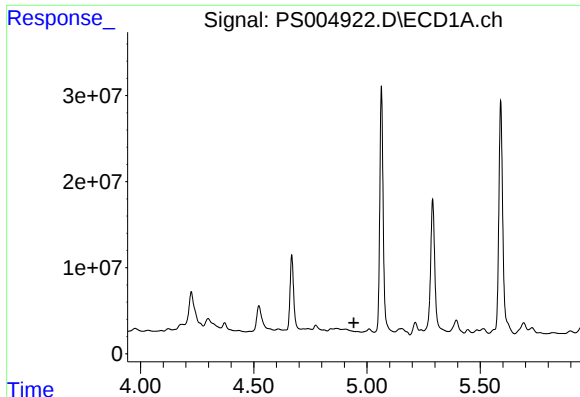

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-007-ABCD

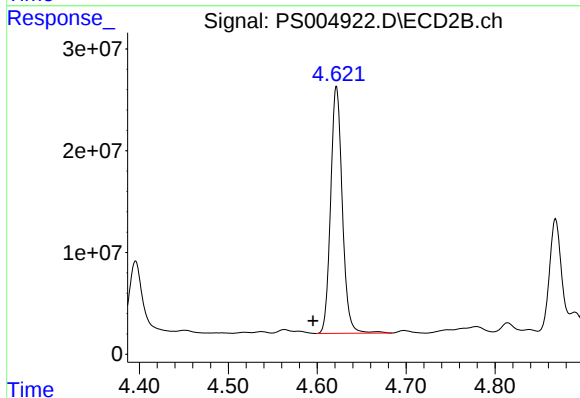


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.622 min
Delta R.T.: 0.026 min
Response: 221284361
Conc: 179.60 ng/ml

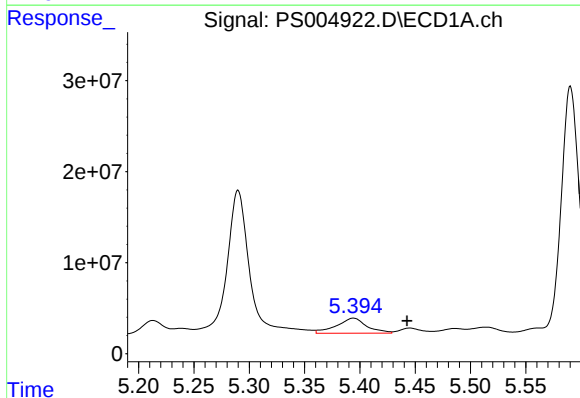


#3 4-Nitrophenol

R.T.: 5.394 min
Delta R.T.: -0.049 min
Response: 31516324
Conc: 50.55 ng/ml

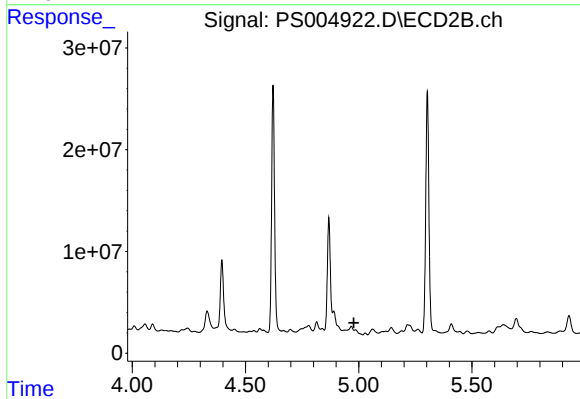

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

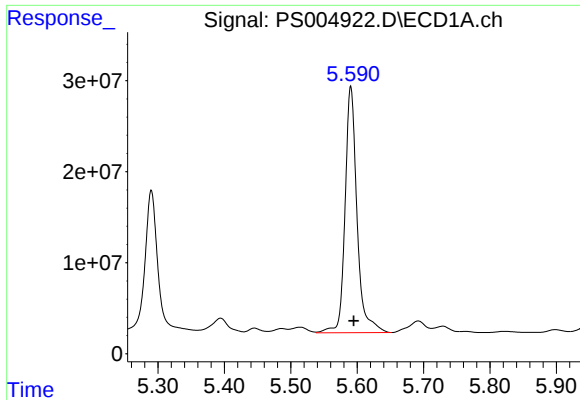

#4 2,4-DCAA


R.T.: 5.590 min
Delta R.T.: -0.005 min
Response: 339006647
Conc: 241.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-007-ABCD

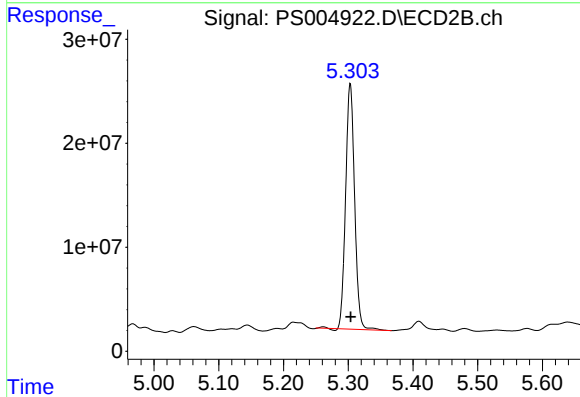


#4 2,4-DCAA

R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 227831046
Conc: 236.13 ng/ml

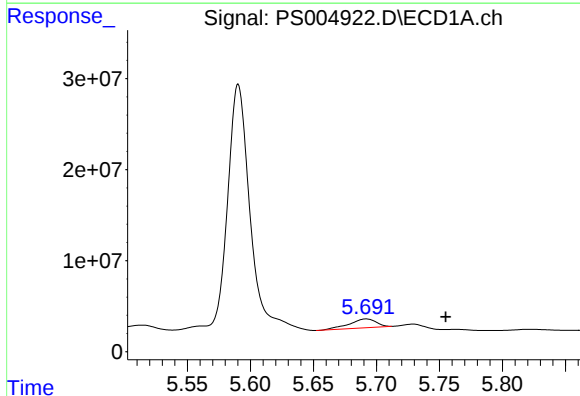


#5 DICAMBA

R.T.: 5.692 min
Delta R.T.: -0.063 min
Response: 14698965
Conc: 2.77 ng/ml

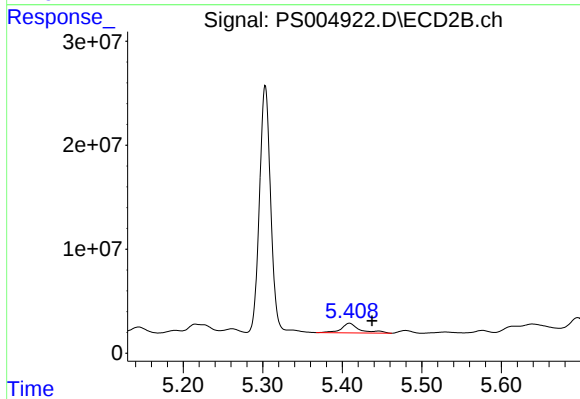

#5 DICAMBA


R.T.: 5.409 min
Delta R.T.: -0.028 min
Response: 14989107
Conc: 4.06 ng/ml

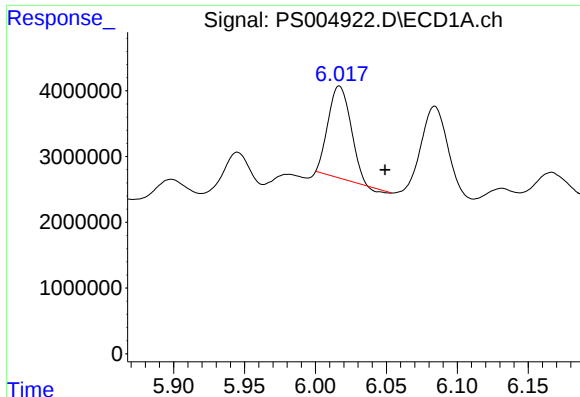

#7 MCPA


R.T.: 6.017 min
Delta R.T.: -0.032 min
Response: 15416316
Conc: 2.66 ug/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-007-ABCD

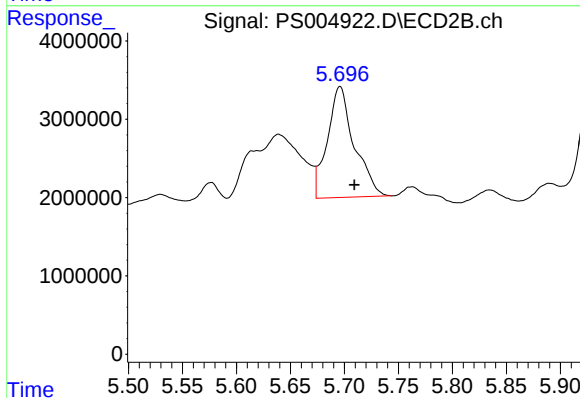


#7 MCPA

R.T.: 5.696 min
Delta R.T.: -0.013 min
Response: 24510738
Conc: 5.99 ug/ml

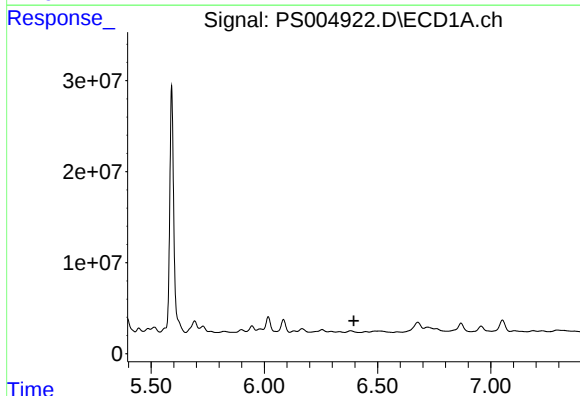


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

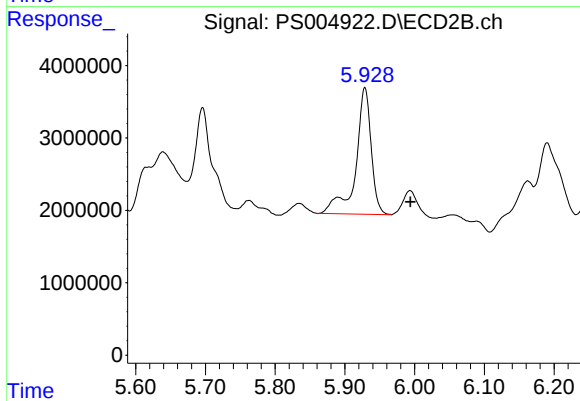

#8 DICHLORPROP


R.T.: 5.929 min
Delta R.T.: -0.065 min
Response: 26848162
Conc: 28.48 ng/ml

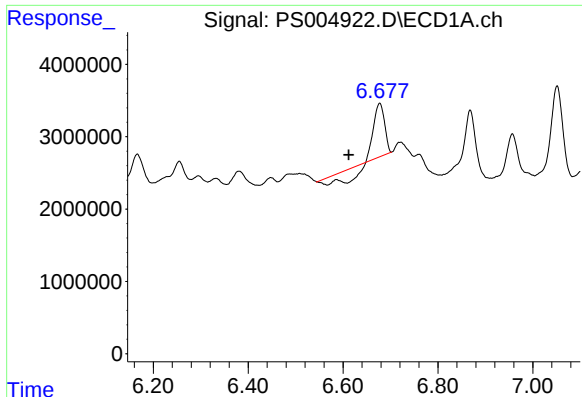

#9 2,4-D


R.T.: 6.677 min
Delta R.T.: 0.065 min
Response: 5640222
Conc: 4.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-007-ABCD

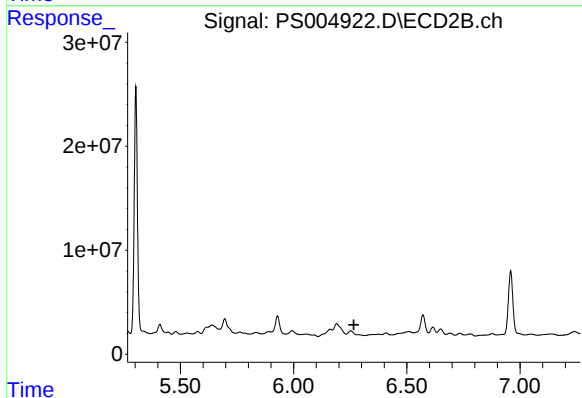


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

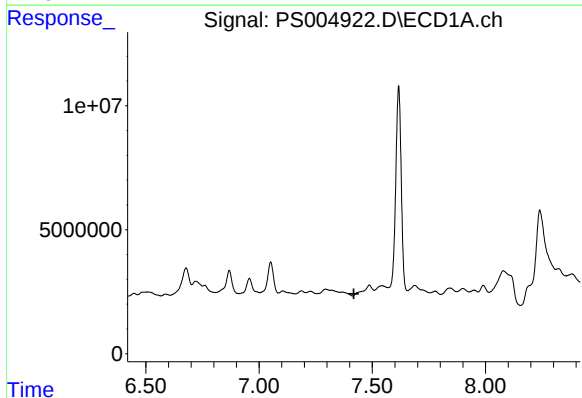


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

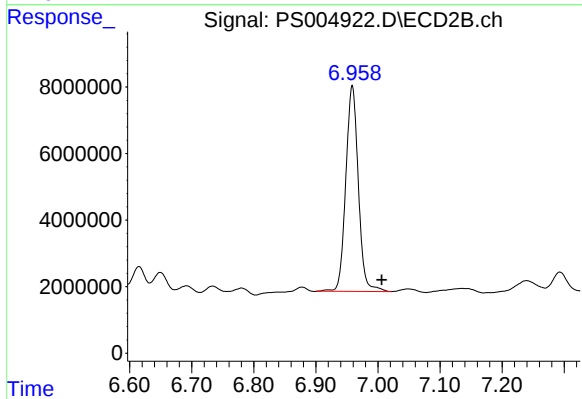

#11 2,4,5-TP (SILVEX)


R.T.: 6.959 min
Delta R.T.: -0.048 min
Response: 86568287
Conc: 16.82 ng/ml

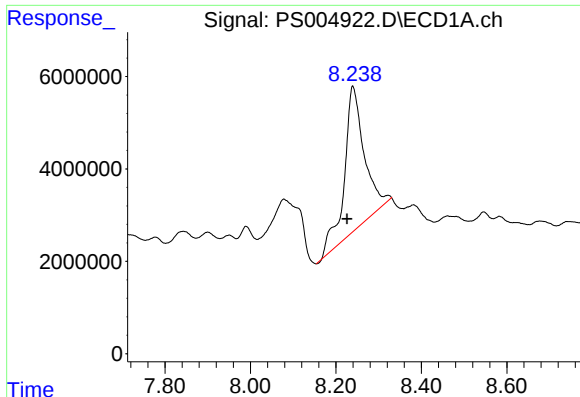

#13 2,4-DB


R.T.: 8.240 min
Delta R.T.: 0.013 min
Response: 100931543
Conc: 104.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-007-ABCD

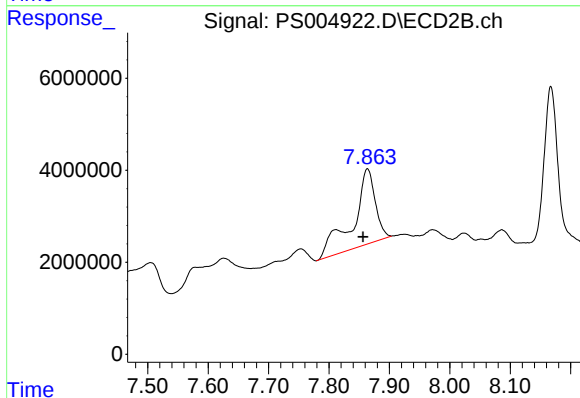


#13 2,4-DB

R.T.: 7.864 min
Delta R.T.: 0.007 min
Response: 42054506
Conc: 64.34 ng/ml

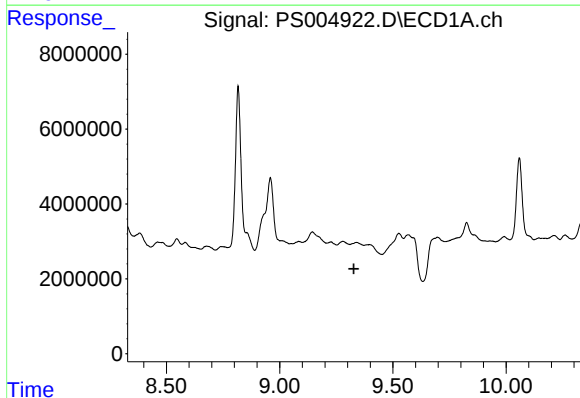

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.328 min
Response: 0
Conc: N.D.

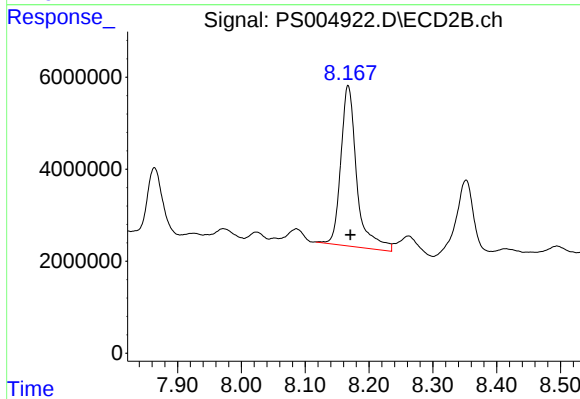

#14 DINOSEB

R.T.: 8.167 min
Delta R.T.: -0.004 min
Response: 60532573
Conc: 15.75 ng/ml