

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
 Data File : PS004923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2019 00:54
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:40:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.588	5.299	760.1E6	534.2E6	542.234	553.682
Target Compounds							
2) T	3,5-DICHL...	4.953	0.000	41769568	0	24.220	N.D. #
5) T	DICAMBA	0.000	5.454	0	42334553	N.D.	11.460
6) T	MCP	5.979	0.000	9043494	0	2.172	N.D. #
7) T	MCPA	5.979	0.000	9043494	0	1.561	N.D. #
8) T	DICHLORPROP	0.000	5.992	0	38287443	N.D.	40.609
9) T	2,4-D	6.629	0.000	156.6E6	0	114.449	N.D. #
10) T	Pentachlo...	6.889	0.000	19883056	0	1.132	N.D. #
15) T	Picloram	9.125	0.000	876.7E6	0	84.139	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
Data File : PS004923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2019 00:54
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:40:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

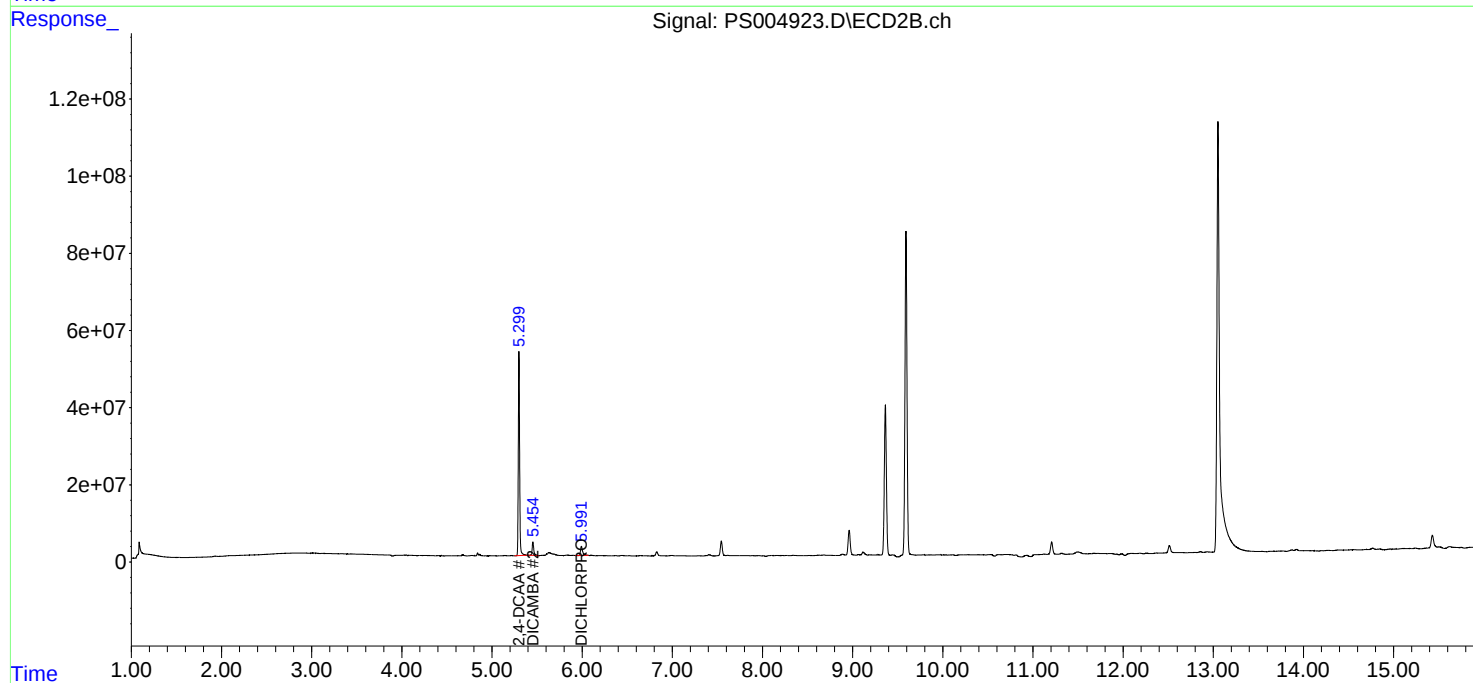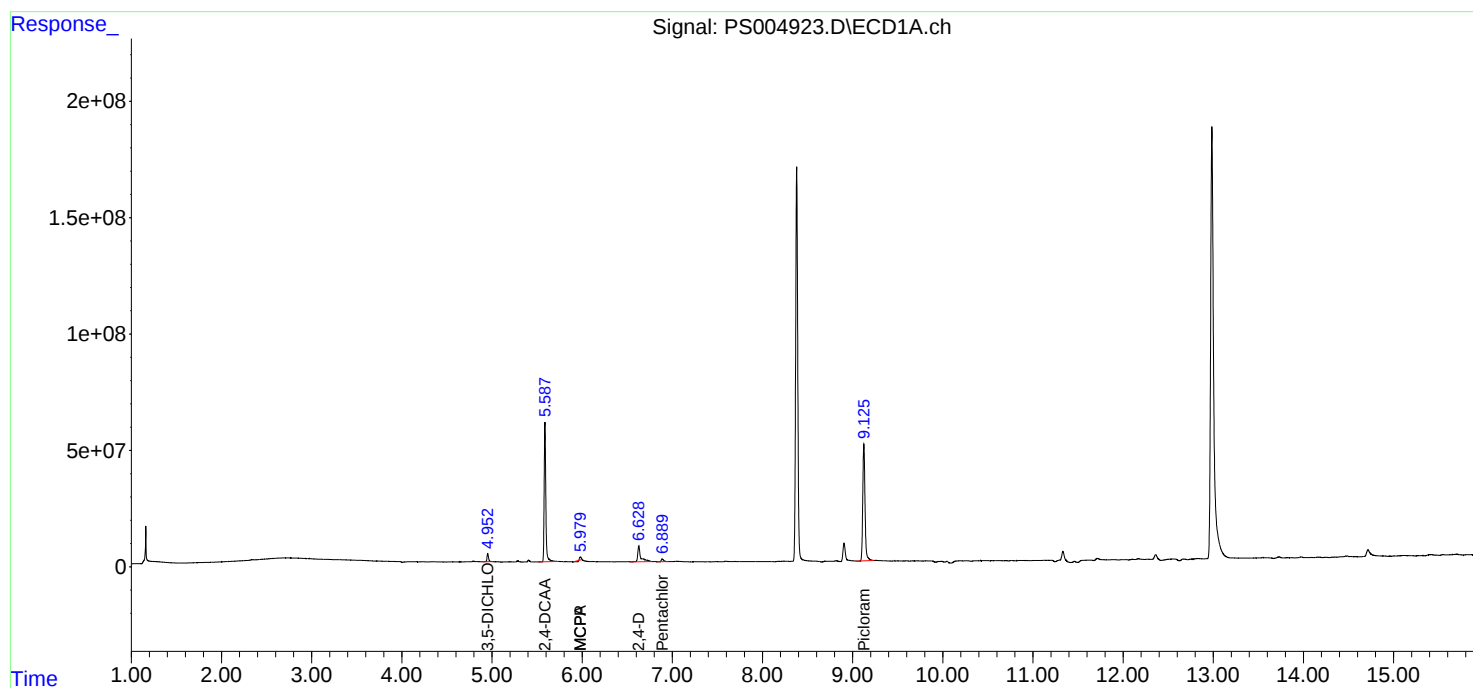


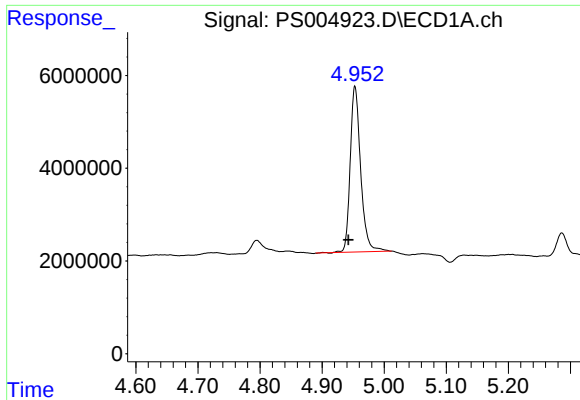

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.953 min
Delta R.T.: 0.011 min
Response: 41769568
Conc: 24.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

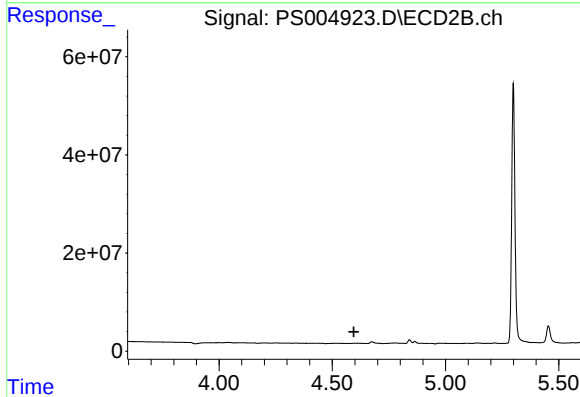


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

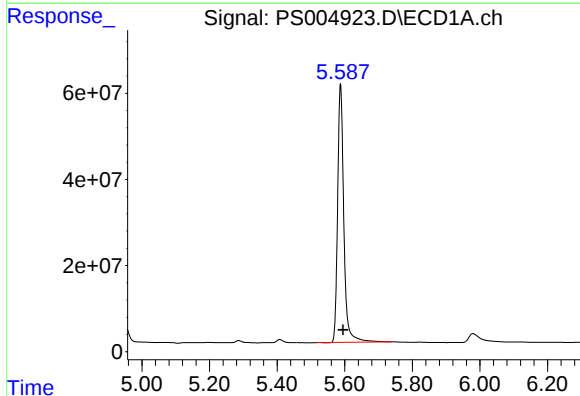


#4 2,4-DCAA

R.T.: 5.588 min
Delta R.T.: -0.008 min
Response: 760080054
Conc: 542.23 ng/ml

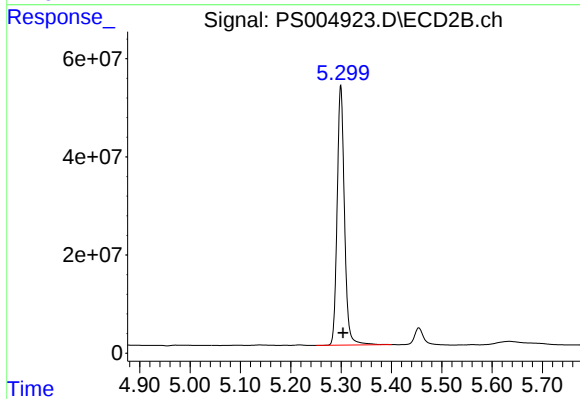

#4 2,4-DCAA


R.T.: 5.299 min
Delta R.T.: -0.004 min
Response: 534212242
Conc: 553.68 ng/ml

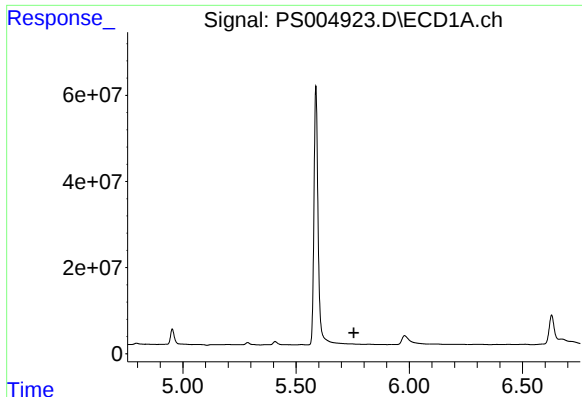

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

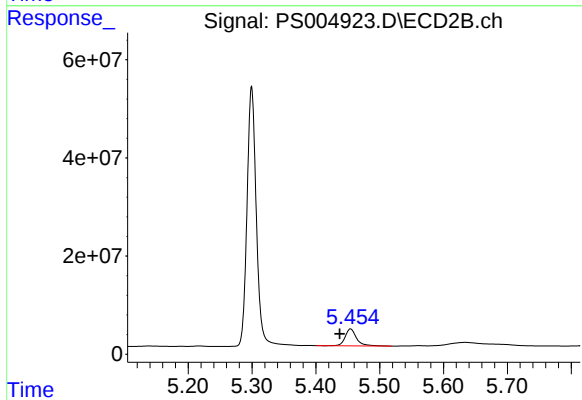


#5 DICAMBA

R.T.: 5.454 min
Delta R.T.: 0.017 min
Response: 42334553
Conc: 11.46 ng/ml

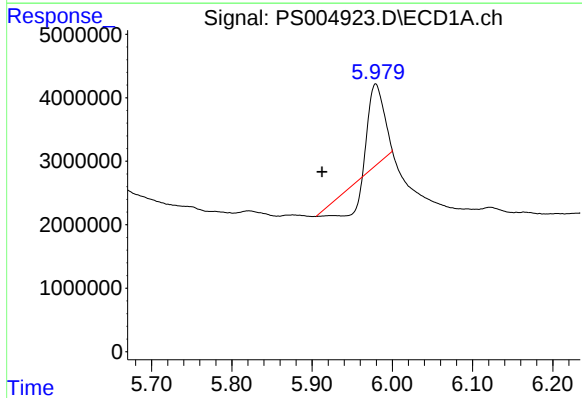


#6 MCP

R.T.: 5.979 min
Delta R.T.: 0.067 min
Response: 9043494
Conc: 2.17 ug/ml

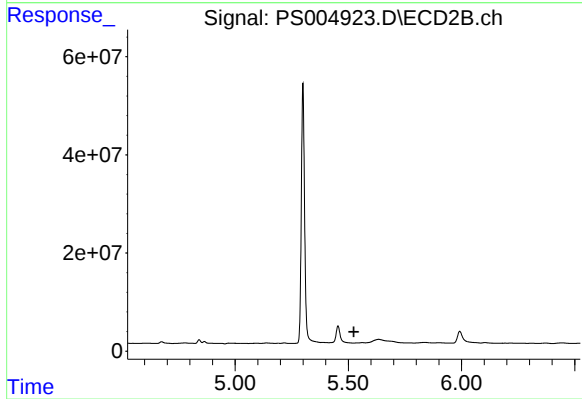

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

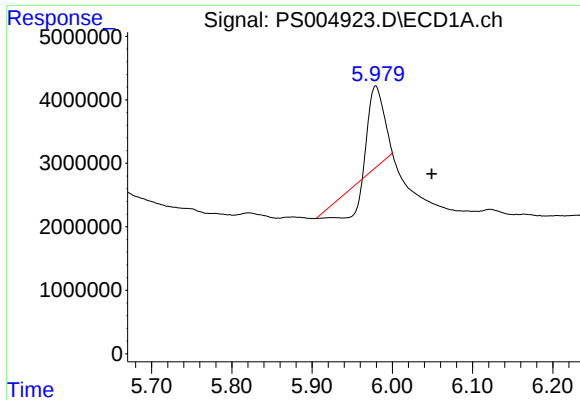

#7 MCPA


R.T.: 5.979 min
Delta R.T.: -0.070 min
Response: 9043494
Conc: 1.56 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

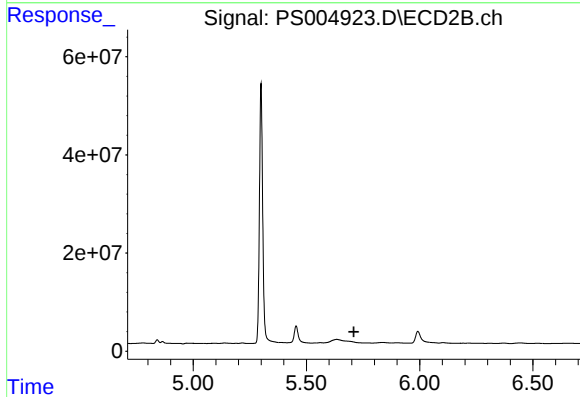


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.709 min
Response: 0
Conc: N.D.

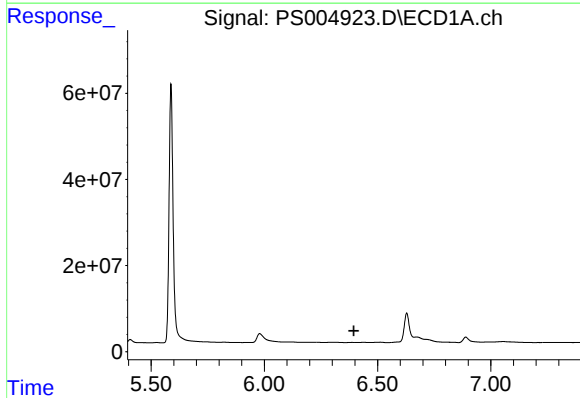


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

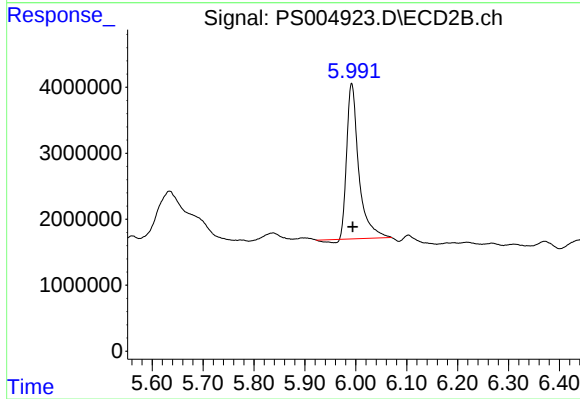

#8 DICHLORPROP


R.T.: 5.992 min
Delta R.T.: -0.002 min
Response: 38287443
Conc: 40.61 ng/ml

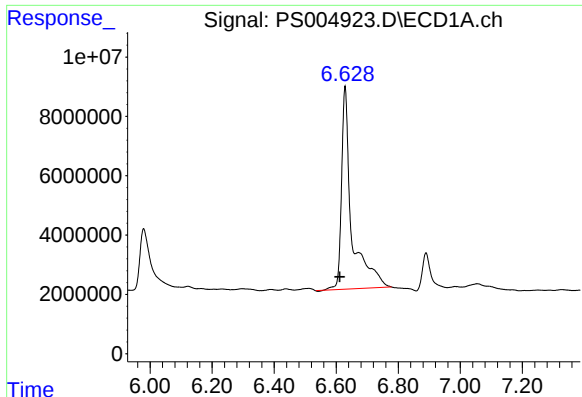

#9 2,4-D


R.T.: 6.629 min
Delta R.T.: 0.017 min
Response: 156555212
Conc: 114.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

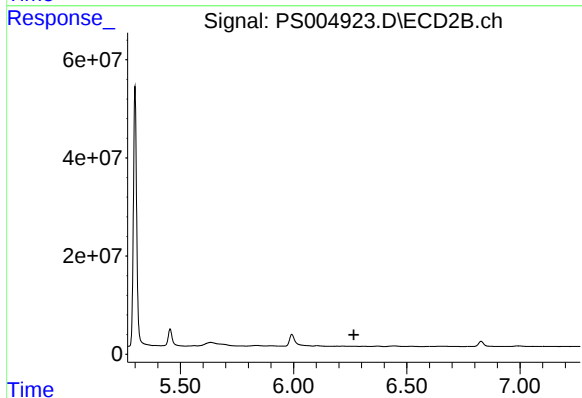


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

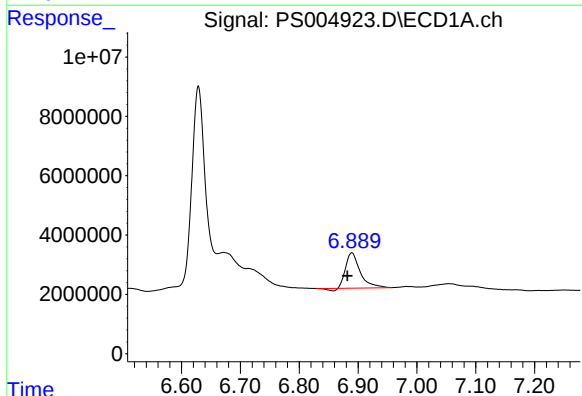


#10 Pentachlorophenol

R.T.: 6.889 min
Delta R.T.: 0.007 min
Response: 19883056
Conc: 1.13 ng/ml

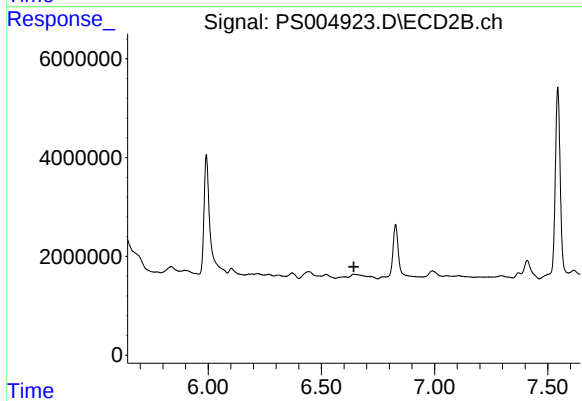

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.644 min
Response: 0
Conc: N.D.

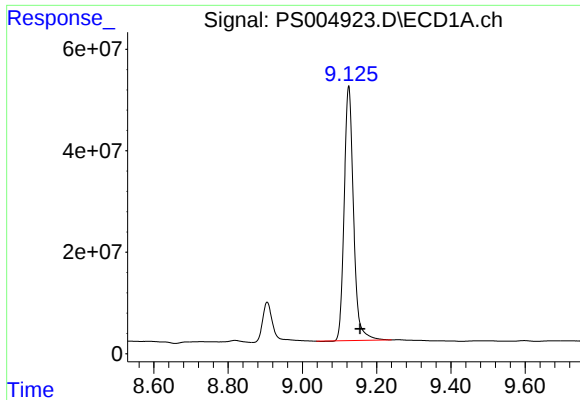

#15 Picloram

R.T.: 9.125 min
Delta R.T.: -0.031 min
Response: 876728177
Conc: 84.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

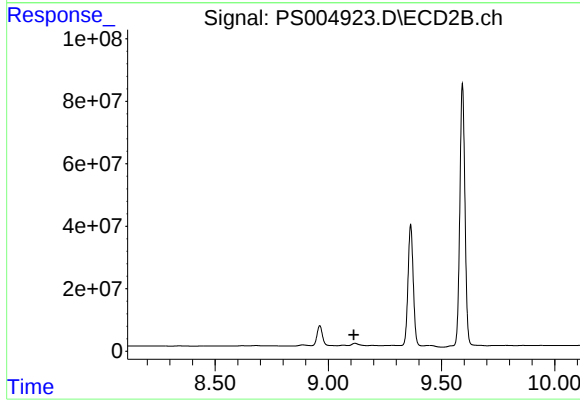

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.113 min
Response: 0
Conc: N.D.