

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
 Data File : PS004927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2019 03:06
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 07:01:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.288	757.1E6	541.8E6	540.076	561.539
Target Compounds							
2) T	3,5-DICHL...	4.941	0.000	80723003	0	46.808	N.D. #
3) T	4-Nitroph...	5.395	0.000	11491565	0	18.431	N.D. #
5) T	DICAMBA	0.000	5.443	0 63715283		N.D.	17.247
6) T	MCP	5.965	0.000	26846695	0	6.449	N.D. #
8) T	DICHLORPROP	0.000	5.979	0 34352436		N.D.	36.436
9) T	2,4-D	6.617	0.000	43099529	0	31.508	N.D. #
10) T	Pentachlo...	6.876	0.000	21269558	0	1.211	N.D. #
15) T	Picloram	9.113	9.104	877.5E6	28977815	84.210	3.884 #
16) T	DCPA	0.000	9.104	0 28977815		N.D.	4.473



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060419\
Data File : PS004927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2019 03:06
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 07:01:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

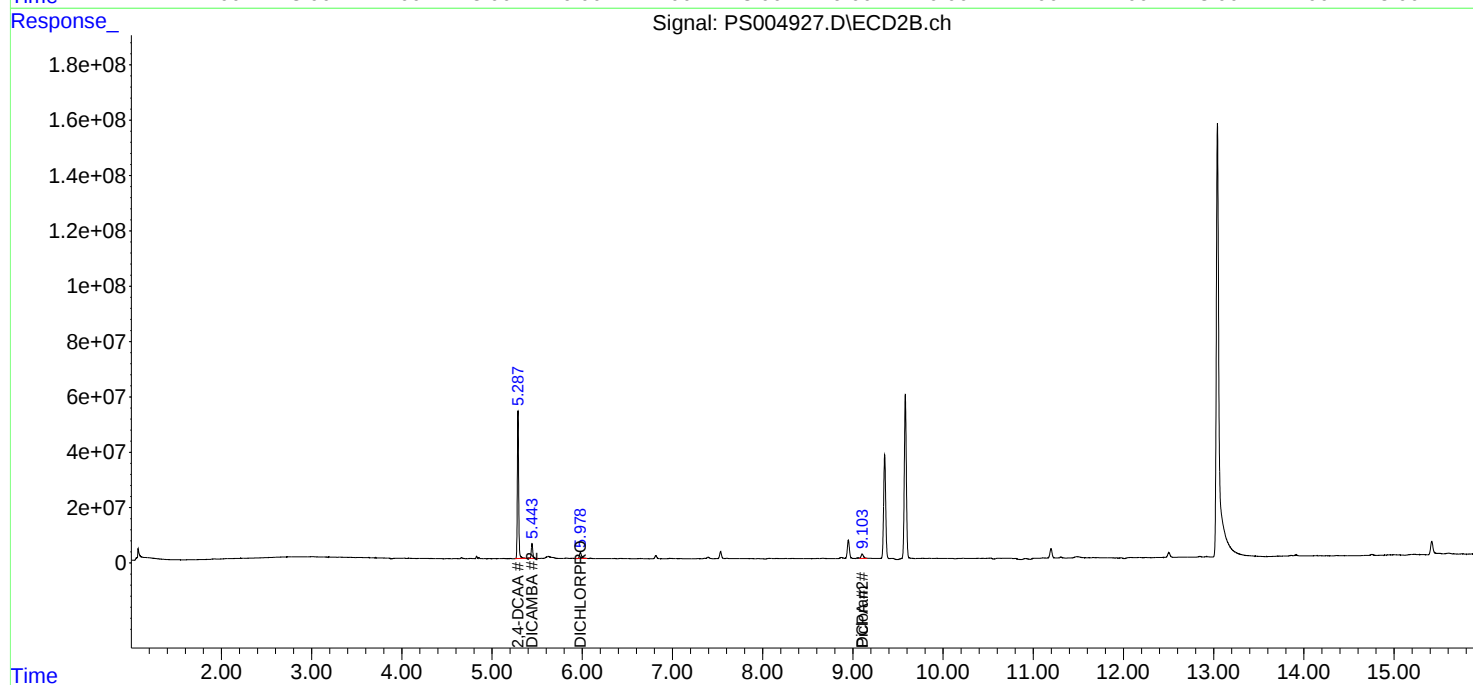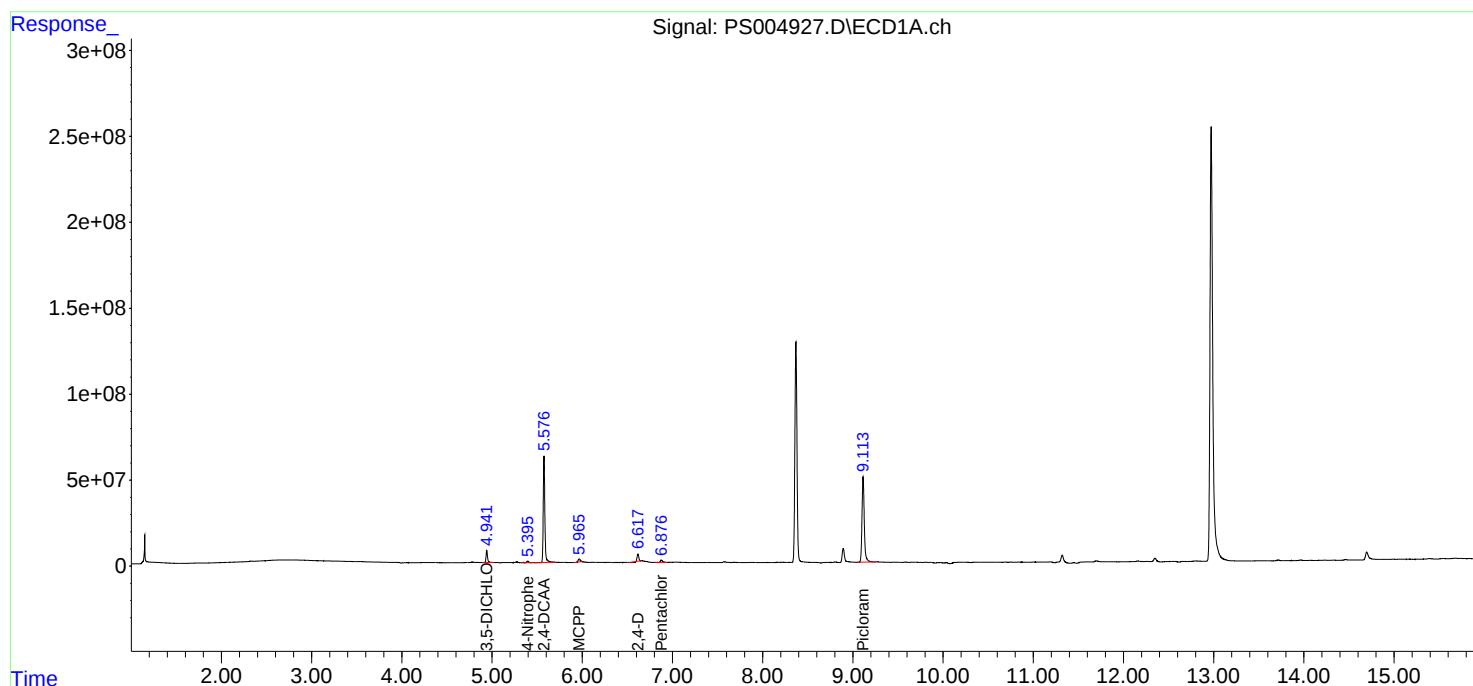


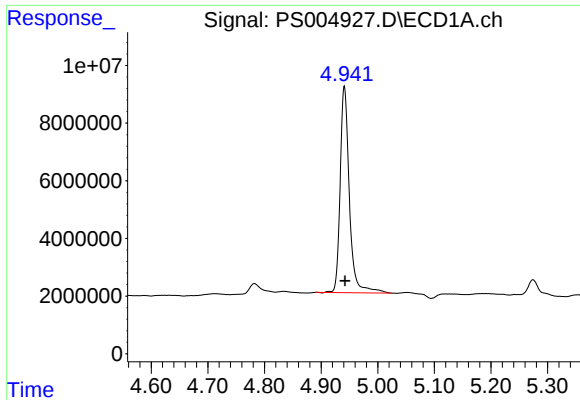

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 80723003
Conc: 46.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

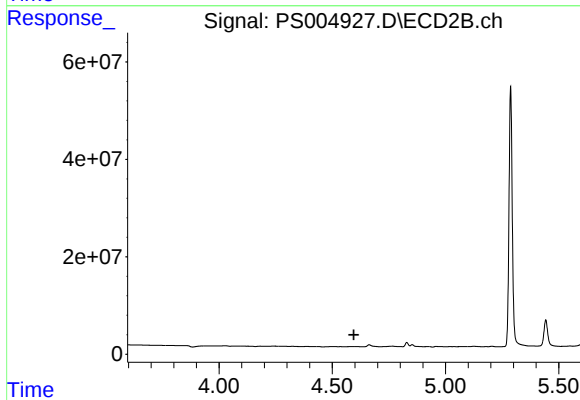


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

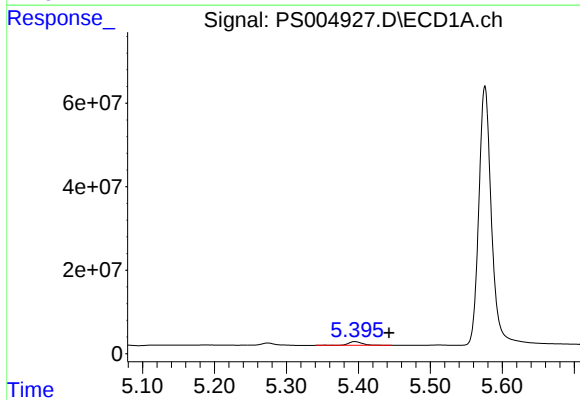


#3 4-Nitrophenol

R.T.: 5.395 min
Delta R.T.: -0.048 min
Response: 11491565
Conc: 18.43 ng/ml

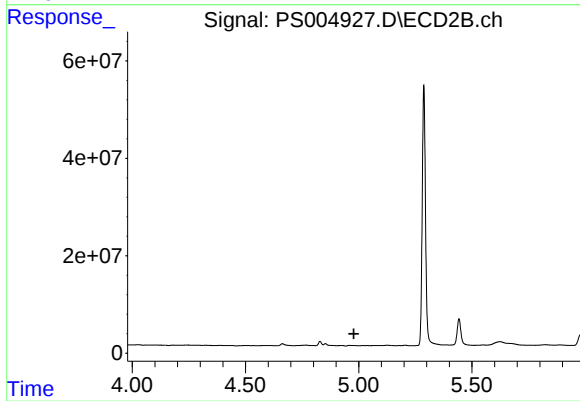

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

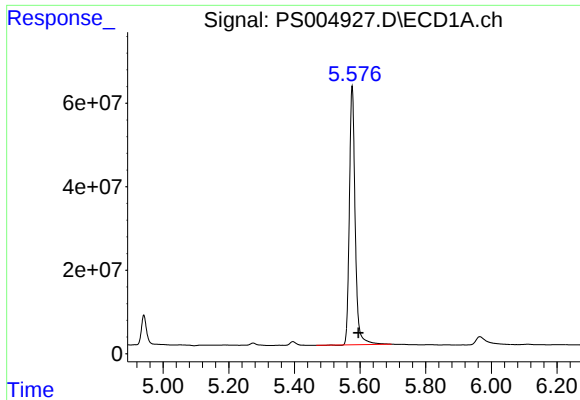

#4 2,4-DCAA


R.T.: 5.576 min
Delta R.T.: -0.019 min
Response: 757054717
Conc: 540.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

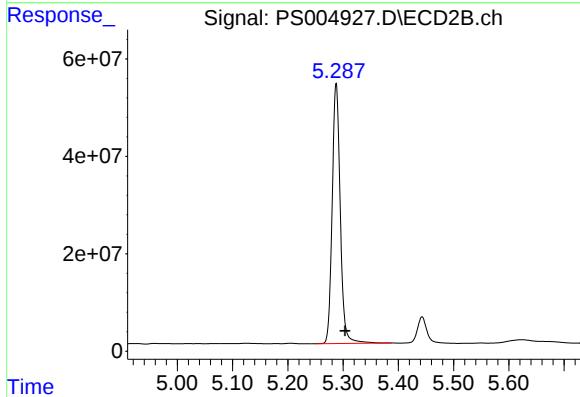


#4 2,4-DCAA

R.T.: 5.288 min
Delta R.T.: -0.016 min
Response: 541793057
Conc: 561.54 ng/ml

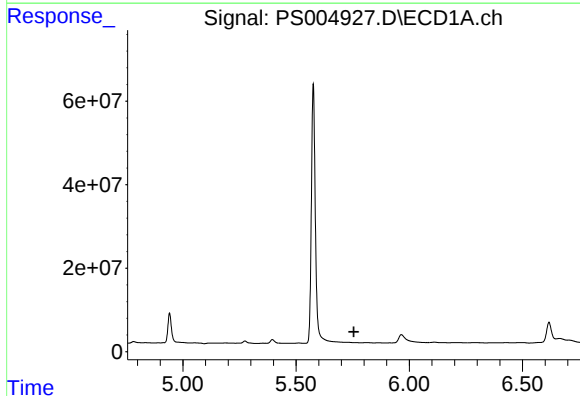


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

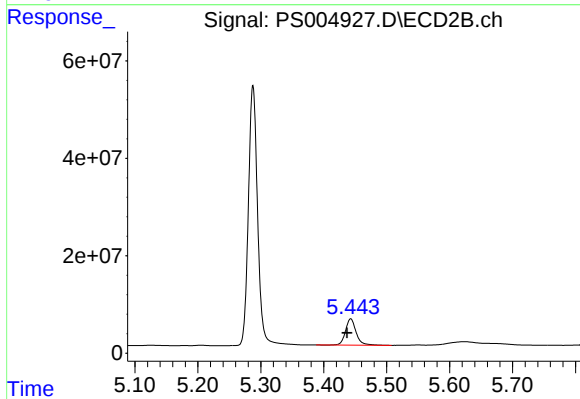

#5 DICAMBA


R.T.: 5.443 min
Delta R.T.: 0.006 min
Response: 63715283
Conc: 17.25 ng/ml

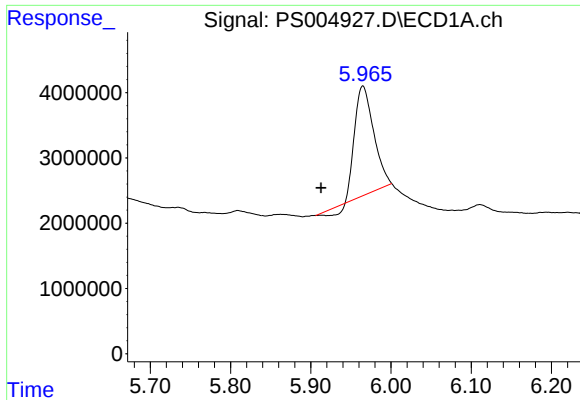

#6 MCP


R.T.: 5.965 min
Delta R.T.: 0.053 min
Response: 26846695
Conc: 6.45 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

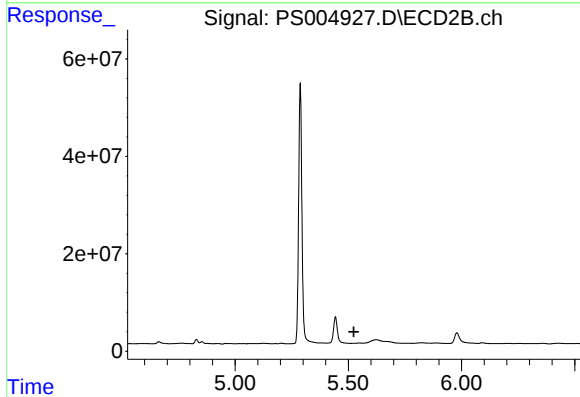


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

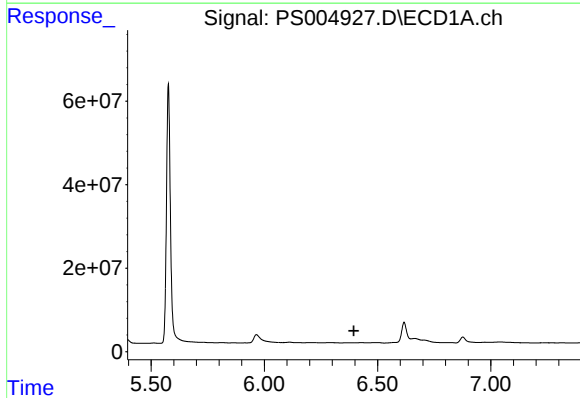


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

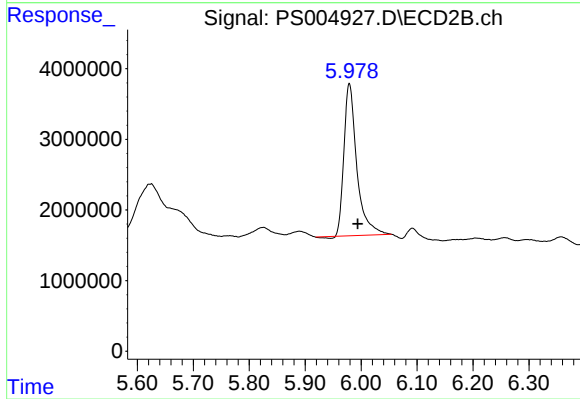

#8 DICHLORPROP


R.T.: 5.979 min
Delta R.T.: -0.015 min
Response: 34352436
Conc: 36.44 ng/ml

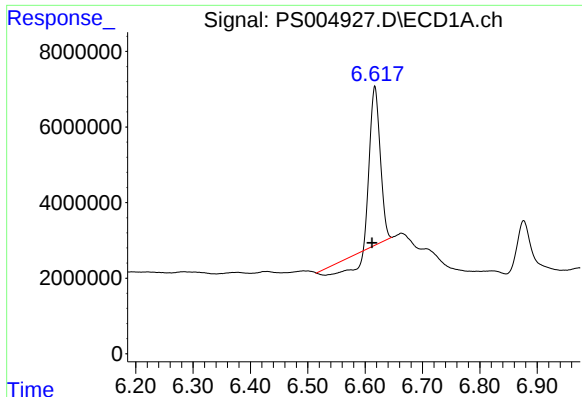

#9 2,4-D


R.T.: 6.617 min
Delta R.T.: 0.005 min
Response: 43099529
Conc: 31.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

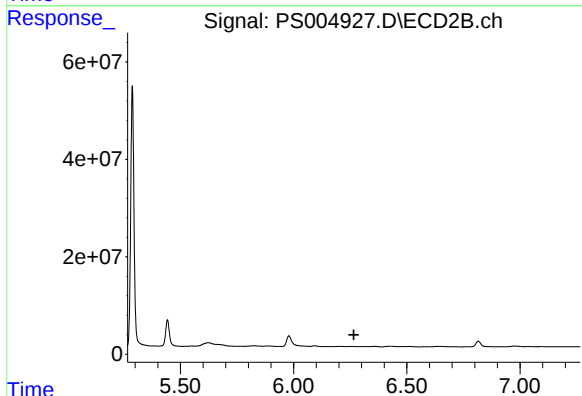


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

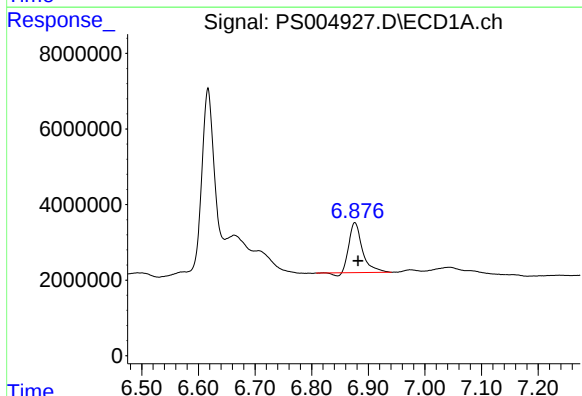


#10 Pentachlorophenol

R.T.: 6.876 min
Delta R.T.: -0.006 min
Response: 21269558
Conc: 1.21 ng/ml

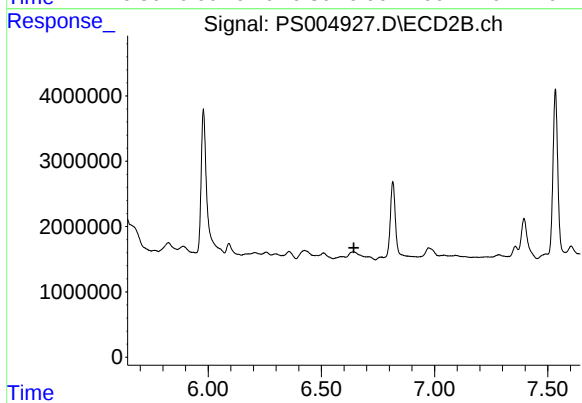

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.644 min
Response: 0
Conc: N.D.

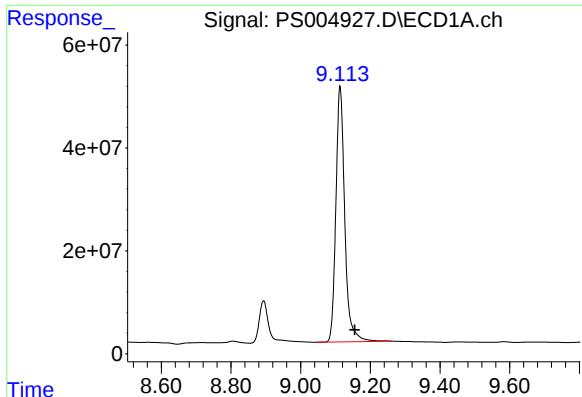

#15 Picloram


R.T.: 9.113 min
Delta R.T.: -0.042 min
Response: 877464314
Conc: 84.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

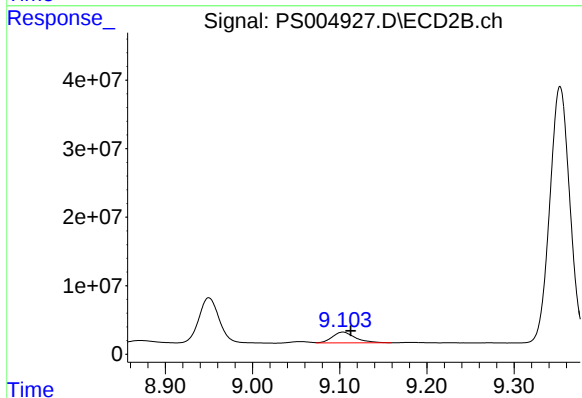


#15 Picloram

R.T.: 9.104 min
Delta R.T.: -0.009 min
Response: 28977815
Conc: 3.88 ng/ml

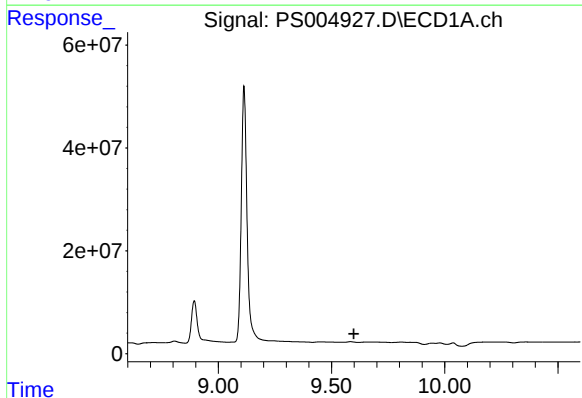

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

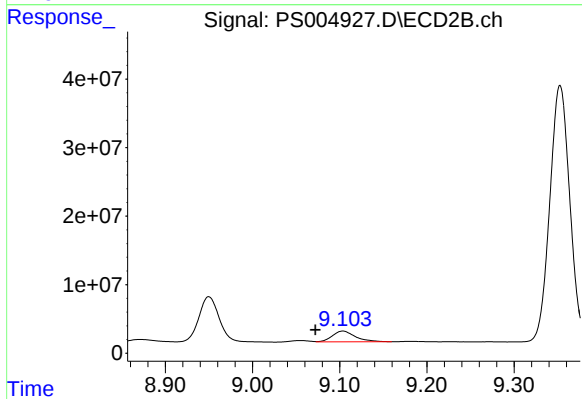

#16 DCPA

R.T.: 9.104 min
Delta R.T.: 0.031 min
Response: 28977815
Conc: 4.47 ng/ml