

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
 Data File : PS010643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2020 08:12
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 13:21:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.484	0.000	40661296	0	37.194	N.D. #
5) T	DICAMBA	0.000	7.154	0	33741098	N.D.	14.991
6) T	MCP	0.000	7.154	0	33741098	N.D.	18.106
12) T	2,4,5-T	0.000	9.237	0	9640264	N.D.	3.212
15) T	Picloram	11.027	11.005	35170257	35331912	6.889	8.563
16) T	DCPA	0.000	11.005	0	35331912	N.D.	9.528



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
Data File : PS010643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2020 08:12
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 13:21:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

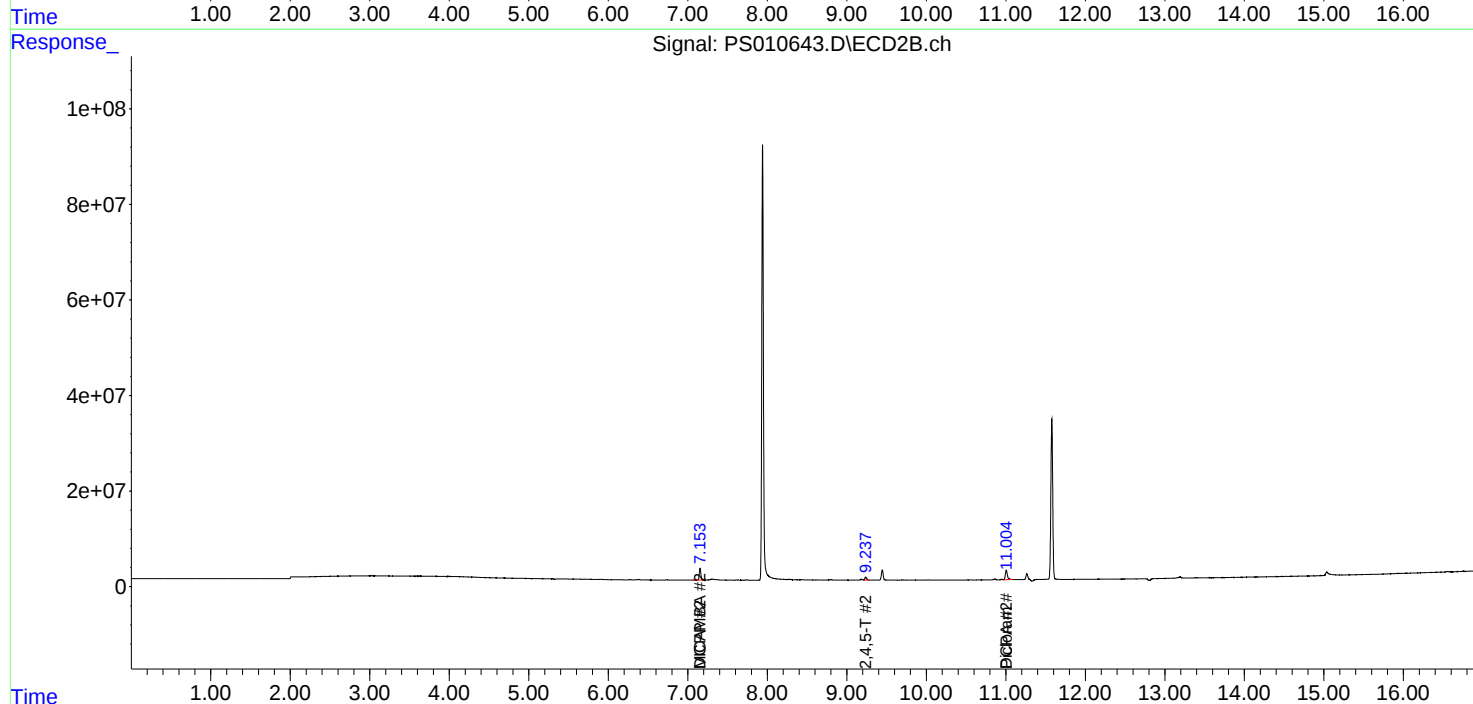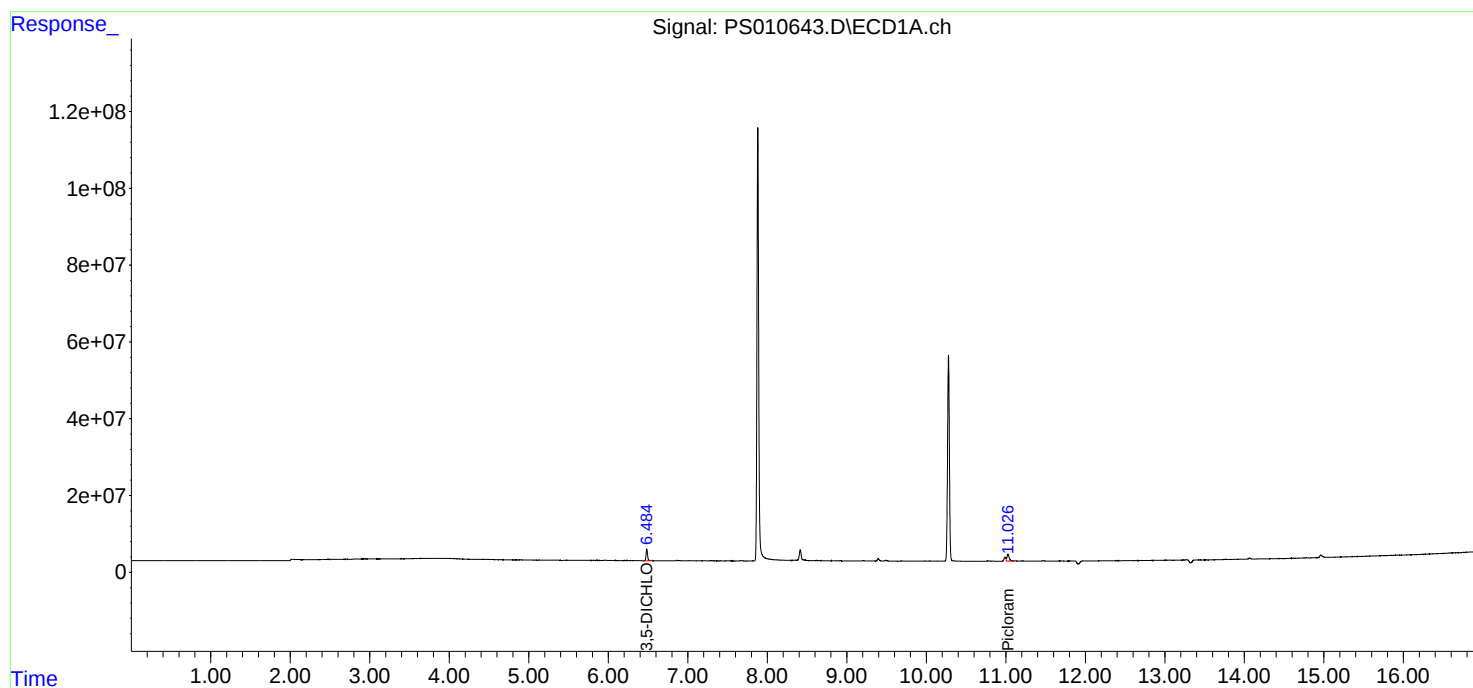


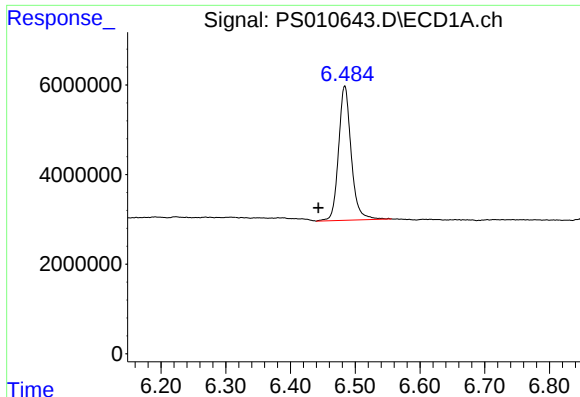

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.484 min
Delta R.T.: 0.041 min
Response: 40661296
Conc: 37.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

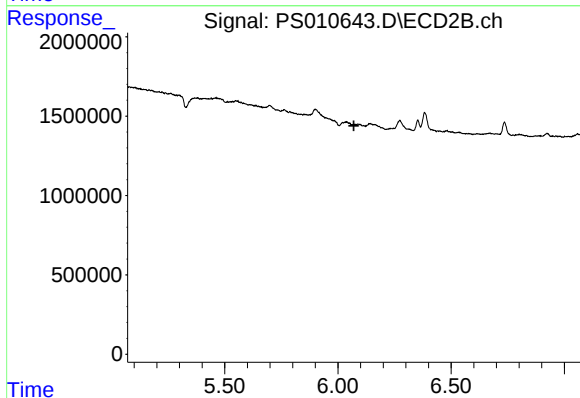


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.070 min
Response: 0
Conc: N.D.

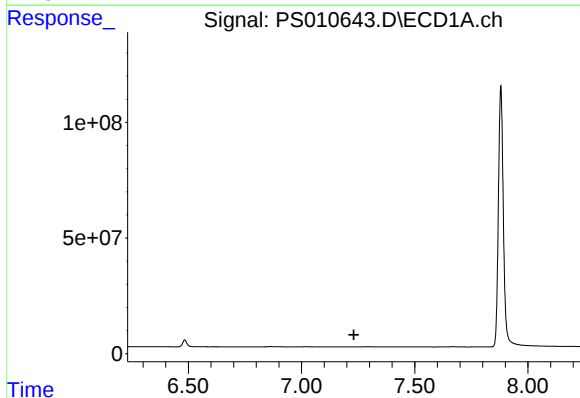


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.231 min
Response: 0
Conc: N.D.

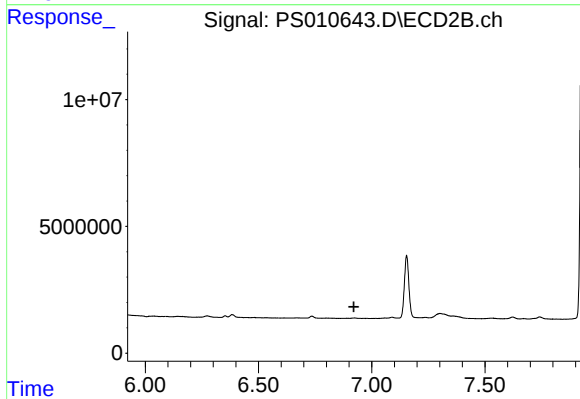

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

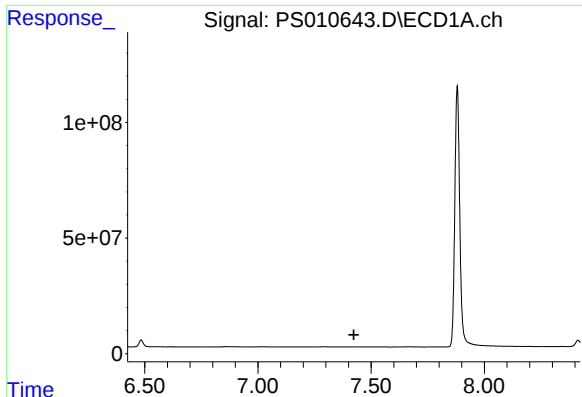

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

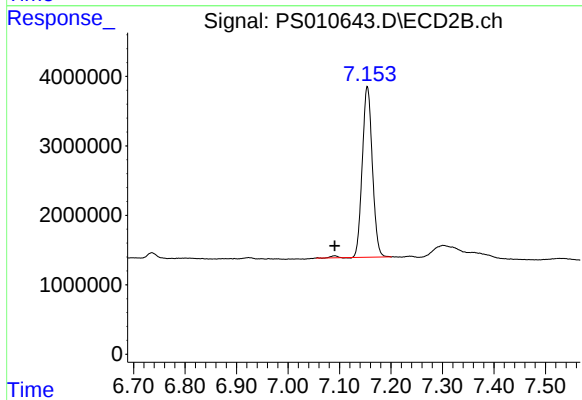


#5 DICAMBA

R.T.: 7.154 min
Delta R.T.: 0.063 min
Response: 33741098
Conc: 14.99 ng/ml

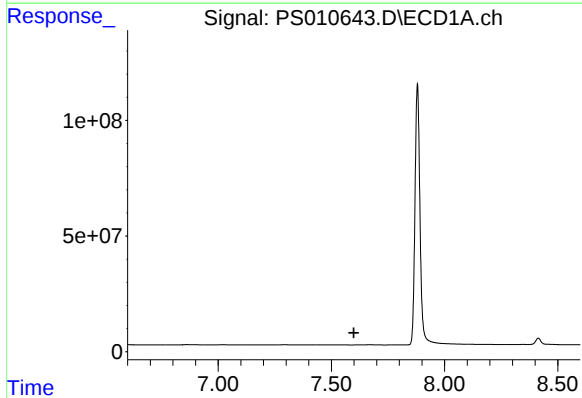


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.600 min
Response: 0
Conc: N.D.

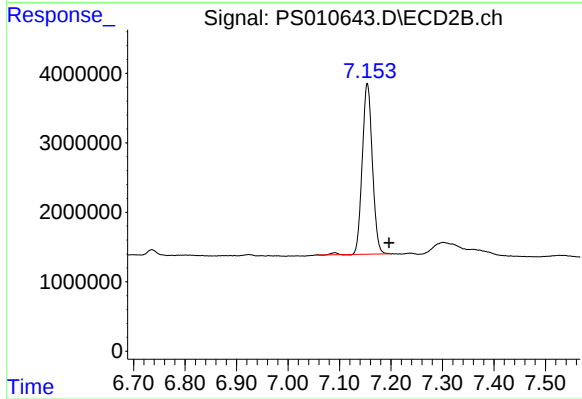

#6 MCP


R.T.: 7.154 min
Delta R.T.: -0.042 min
Response: 33741098
Conc: 18.11 ug/ml

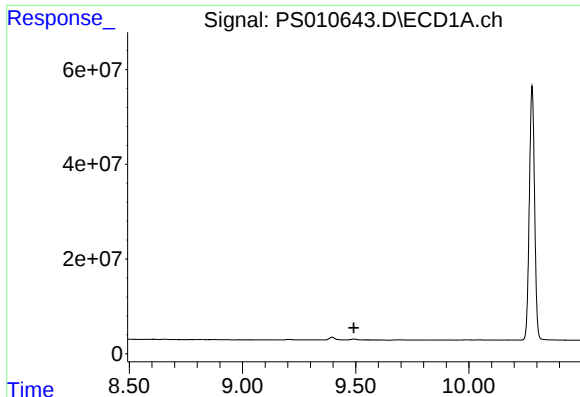

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

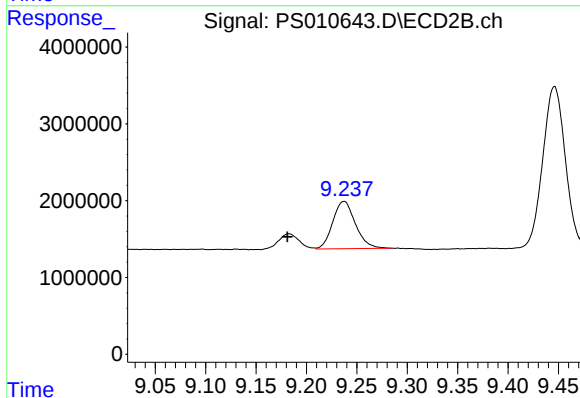


#12 2,4,5-T

R.T.: 9.237 min
Delta R.T.: 0.056 min
Response: 9640264
Conc: 3.21 ng/ml

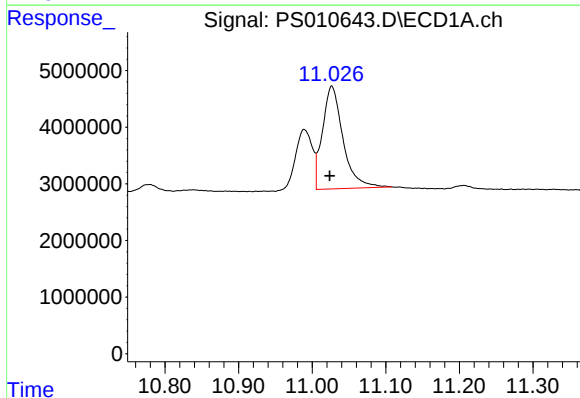


#15 Picloram

R.T.: 11.027 min
Delta R.T.: 0.003 min
Response: 35170257
Conc: 6.89 ng/ml

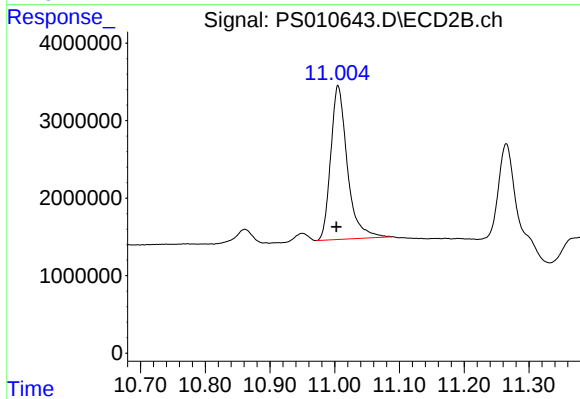

#15 Picloram


R.T.: 11.005 min
Delta R.T.: 0.003 min
Response: 35331912
Conc: 8.56 ng/ml

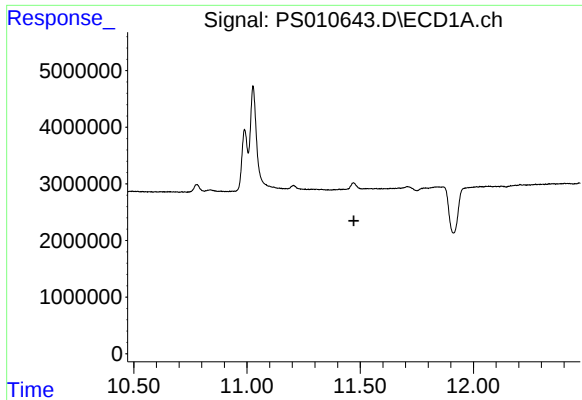

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

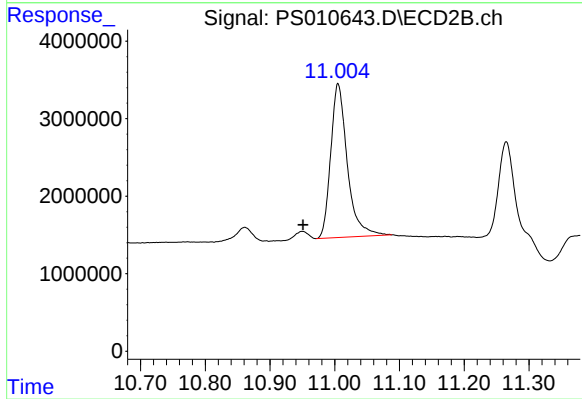

#16 DCPA

R.T.: 11.005 min
Delta R.T.: 0.054 min
Response: 35331912
Conc: 9.53 ng/ml