

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
 Data File : PS010676.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2020 21:41
 Operator : DD\AJ
 Sample : PB129273BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:03:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.920	405.7E6	292.9E6	512.930	537.011
Target Compounds							
1) T	Dalapon	2.997	2.583	39245198	103.4E6	39.916	141.277 #
2) T	3,5-DICHL...	0.000	6.100	0	61123580	N.D.	74.573
5) T	DICAMBA	0.000	7.055	0	6127415	N.D.	2.722
7) T	MCPA	7.778	7.385	39621023	35251250	11.333	12.971
8) T	DICHLORPROP	0.000	7.738	0	8018912	N.D.	13.907
10) T	Pentachlo...	8.712	0.000	10111177	0	<MDL	N.D. #
12) T	2,4,5-T	9.512	0.000	7308727	0	1.797	N.D. #
14) T	DINOSEB	11.170	10.036	32733721	7344101	10.131	3.414 #
15) T	Picloram	10.995	11.002	102.8E6	10572661	20.144	2.562 #
16) T	DCPA	11.541	11.002	-7183426	10572661	N.D.	2.851



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
Data File : PS010676.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2020 21:41
Operator : DD\AJ
Sample : PB129273BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:03:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

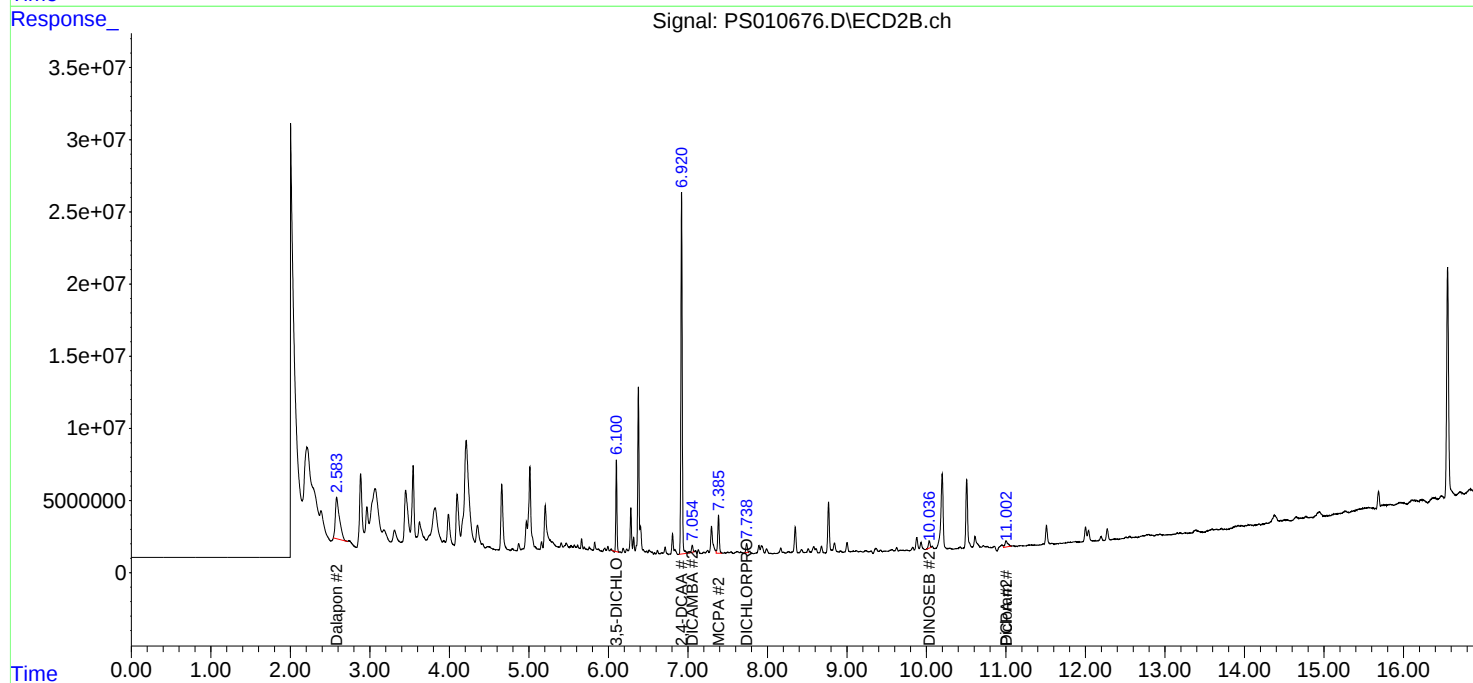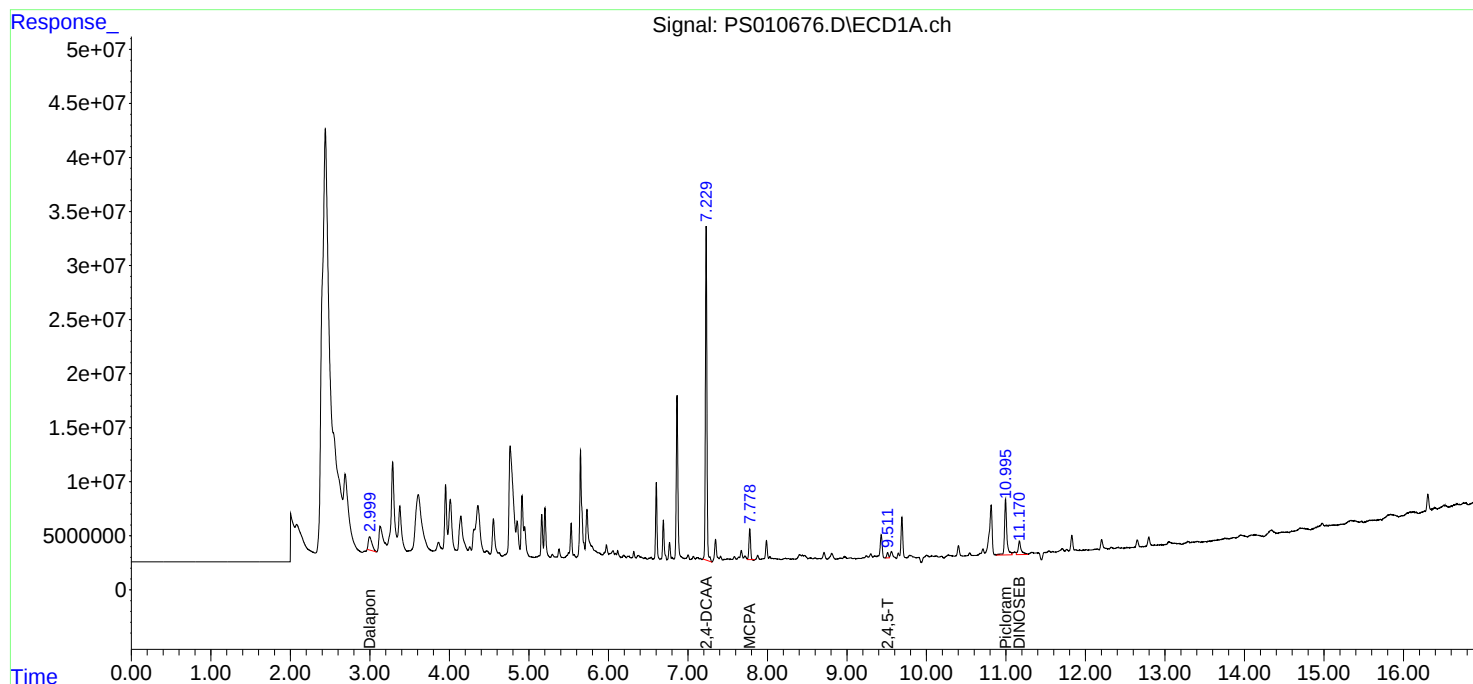


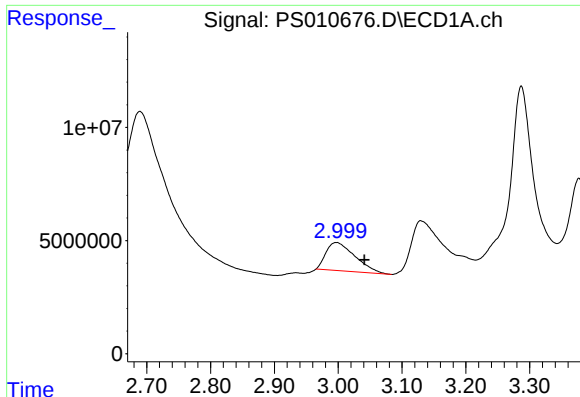

#1 Dalapon


R.T.: 2.997 min
Delta R.T.: -0.044 min
Response: 39245198
Conc: 39.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

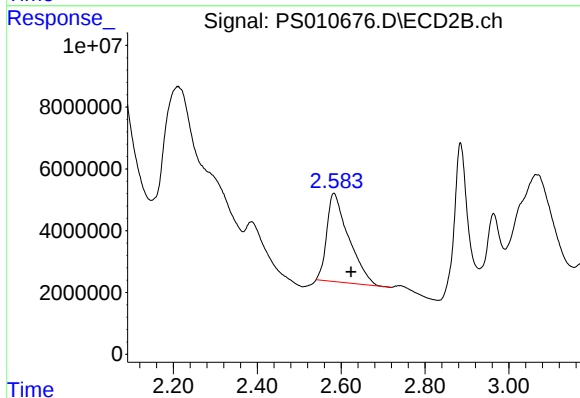


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.041 min
Response: 103434910
Conc: 141.28 ng/ml

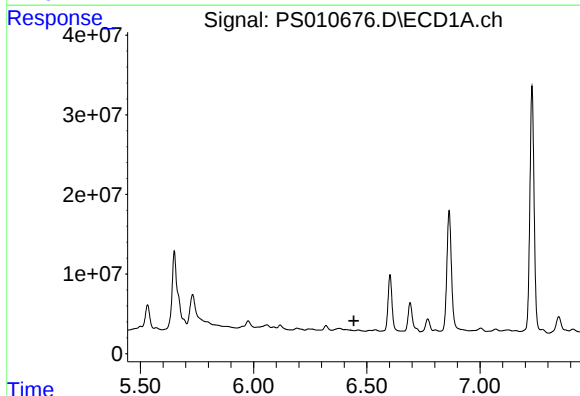


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

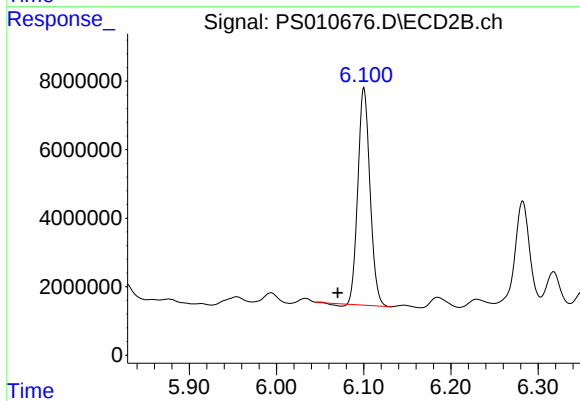

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 61123580
Conc: 74.57 ng/ml

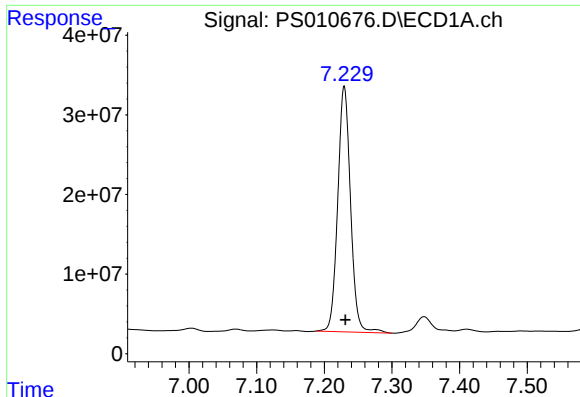

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: -0.002 min
Response: 405656567
Conc: 512.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

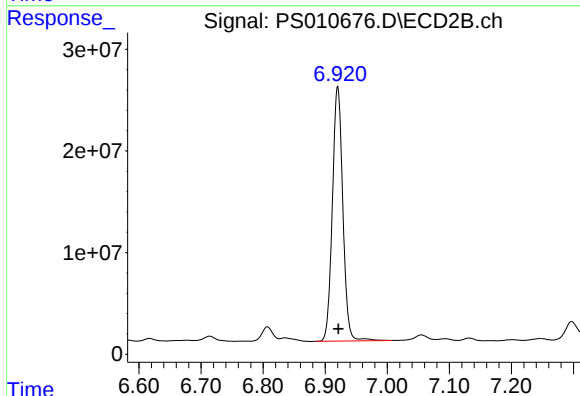


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 292894127
Conc: 537.01 ng/ml

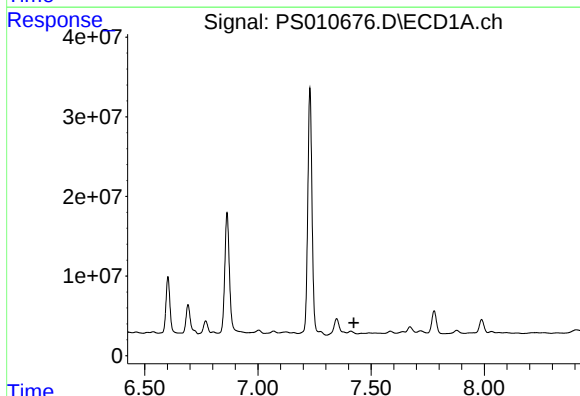


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.423 min
Response: 0
Conc: N.D.

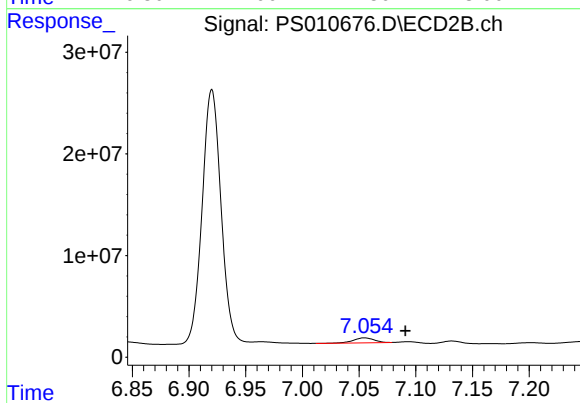

#5 DICAMBA


R.T.: 7.055 min
Delta R.T.: -0.036 min
Response: 6127415
Conc: 2.72 ng/ml

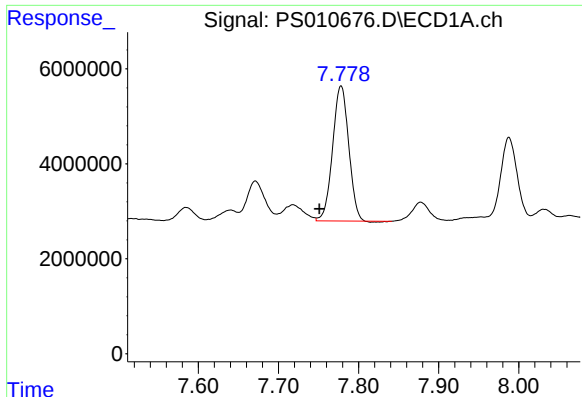

#7 MCPA


R.T.: 7.778 min
Delta R.T.: 0.027 min
Response: 39621023
Conc: 11.33 ug/ml

Instrument :
ECD_S
ClientSampleId :

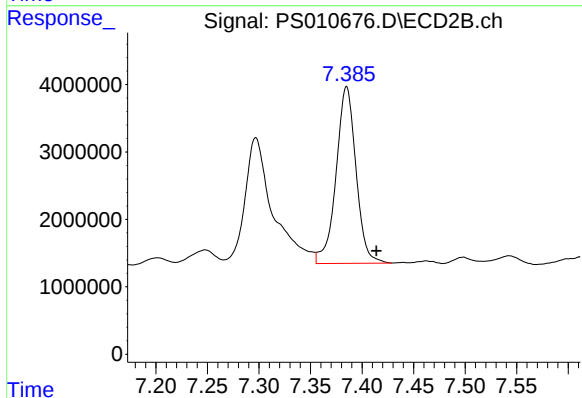


#7 MCPA

R.T.: 7.385 min
Delta R.T.: -0.029 min
Response: 35251250
Conc: 12.97 ug/ml

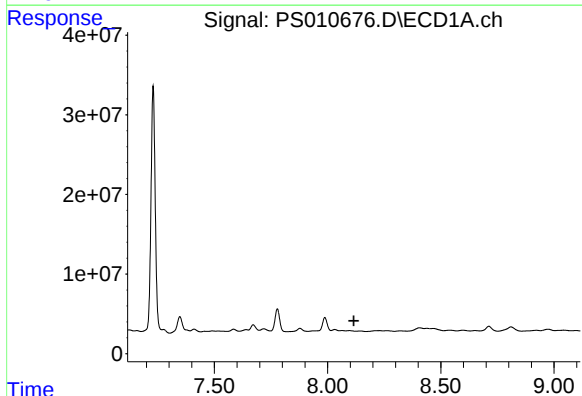


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

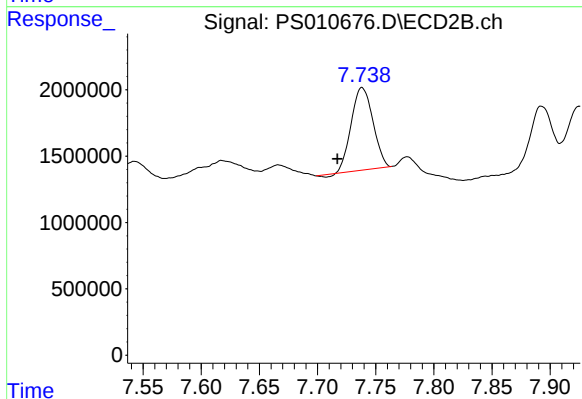

#8 DICHLORPROP


R.T.: 7.738 min
Delta R.T.: 0.021 min
Response: 8018912
Conc: 13.91 ng/ml

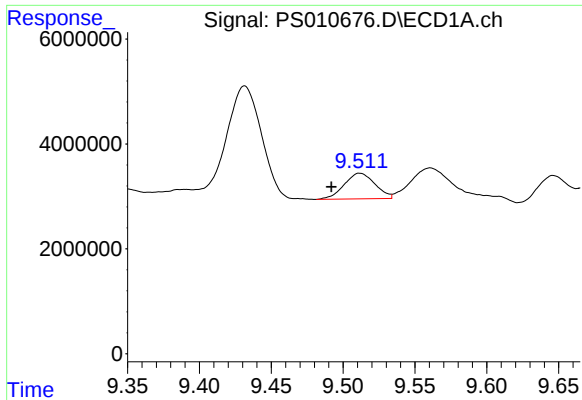

#12 2,4,5-T


R.T.: 9.512 min
Delta R.T.: 0.020 min
Response: 7308727
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

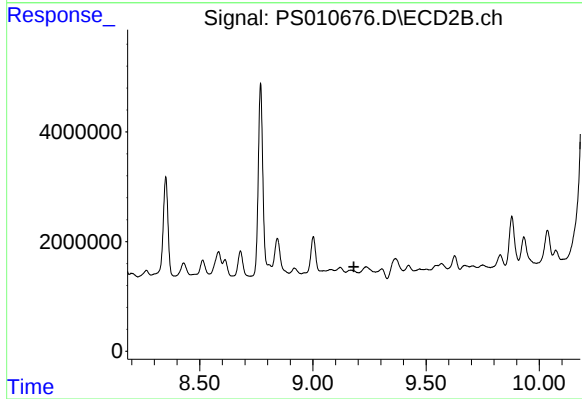


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.181 min
Response: 0
Conc: N.D.

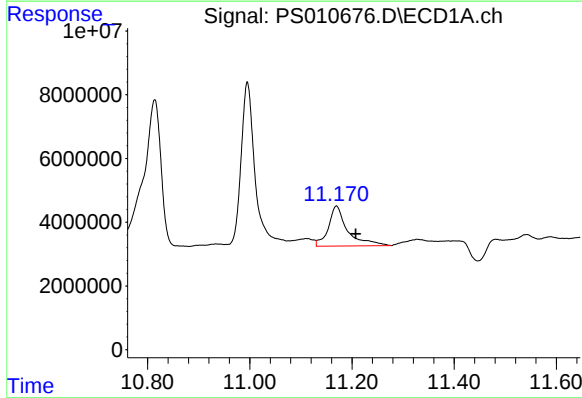


#14 DINOSEB

R.T.: 11.170 min
Delta R.T.: -0.038 min
Response: 32733721
Conc: 10.13 ng/ml

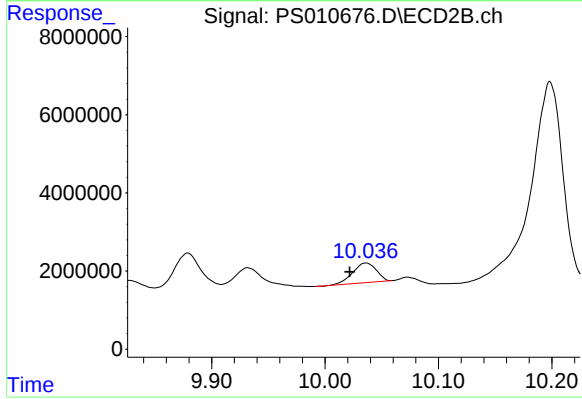

#14 DINOSEB


R.T.: 10.036 min
Delta R.T.: 0.014 min
Response: 7344101
Conc: 3.41 ng/ml

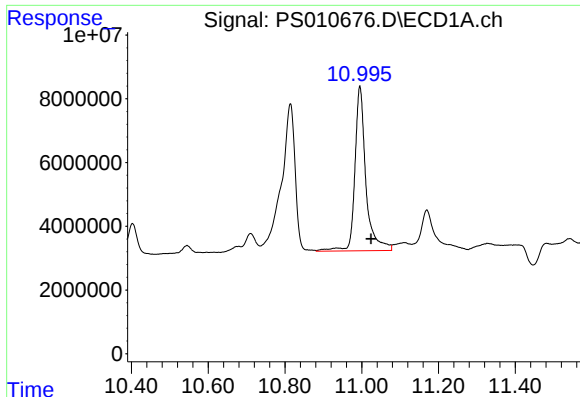

#15 Picloram


R.T.: 10.995 min
Delta R.T.: -0.029 min
Response: 102836196
Conc: 20.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

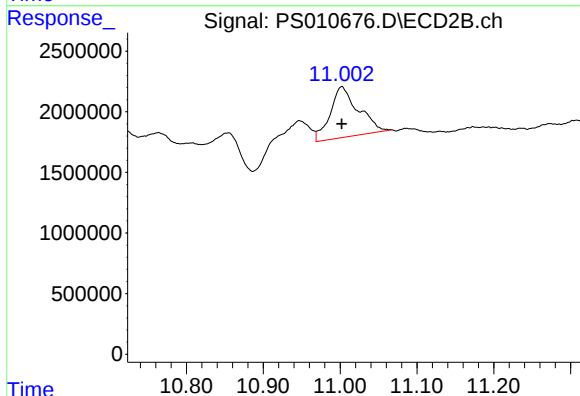


#15 Picloram

R.T.: 11.002 min
Delta R.T.: 0.000 min
Response: 10572661
Conc: 2.56 ng/ml

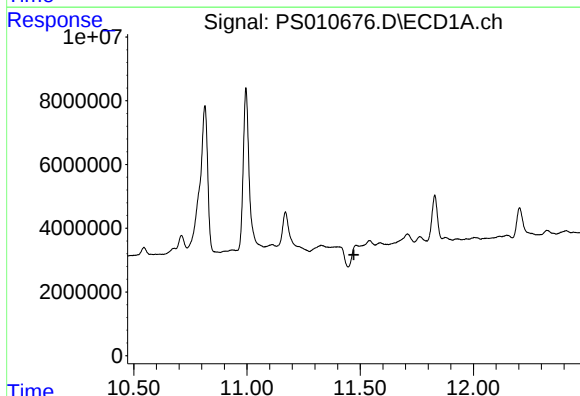

#16 DCPA

R.T.: 11.541 min
Delta R.T.: 0.069 min
Response: -7183426
Conc: N.D.

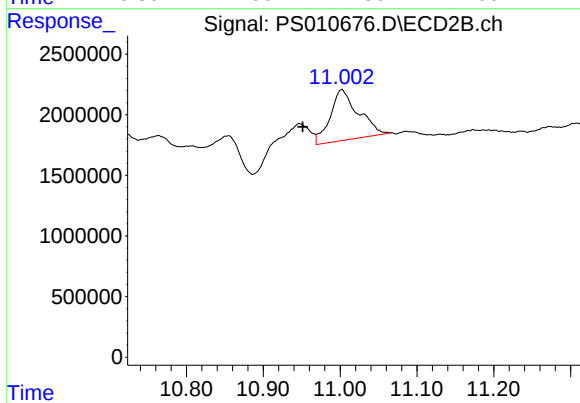

#16 DCPA

R.T.: 11.002 min
Delta R.T.: 0.051 min
Response: 10572661
Conc: 2.85 ng/ml