

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
 Data File : PS010685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2020 01:08
 Operator : DD\AJ
 Sample : PB129307TB
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 04:33:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	282.7E6	218.0E6	357.429	399.768
Target Compounds							
1) T	Dalapon	2.995	2.585	36291492	138.1E6	36.912	188.600 #
2) T	3,5-DICHL...	0.000	6.101	0	60981359	N.D.	74.400
5) T	DICAMBA	0.000	7.054	0	11286511	N.D.	5.014
7) T	MCPA	0.000	7.454	0	69217891	N.D.	25.469
8) T	DICHLORPROP	0.000	7.739	0	14549212	N.D.	25.232
12) T	2,4,5-T	9.431	0.000	28181986	0	6.929	N.D. #
14) T	DINOSEB	11.170	10.067	22418608	28141391	6.938	13.080 #
15) T	Picloram	10.996	11.004	111.2E6	9431363	21.783	2.286 #
16) T	DCPA	0.000	11.004	0	9431363	N.D.	2.543



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
Data File : PS010685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2020 01:08
Operator : DD\AJ
Sample : PB129307TB
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 04:33:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

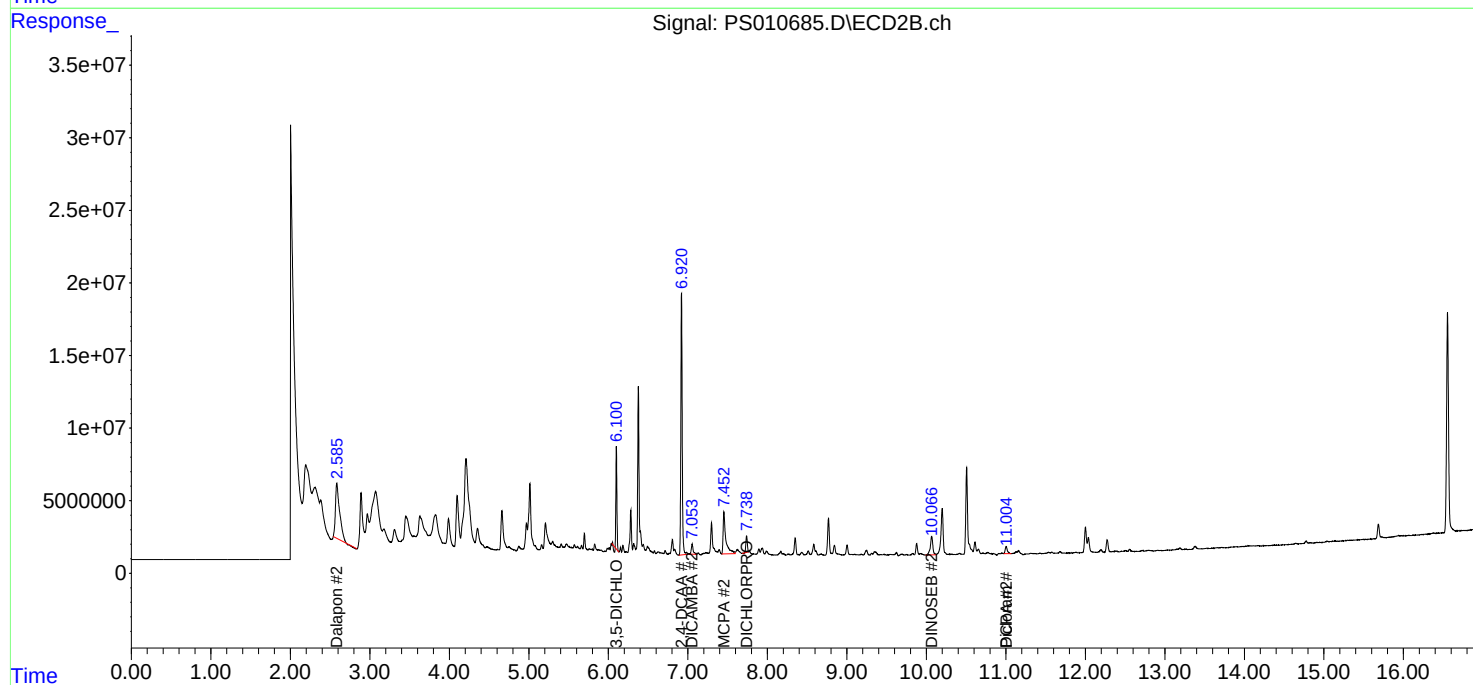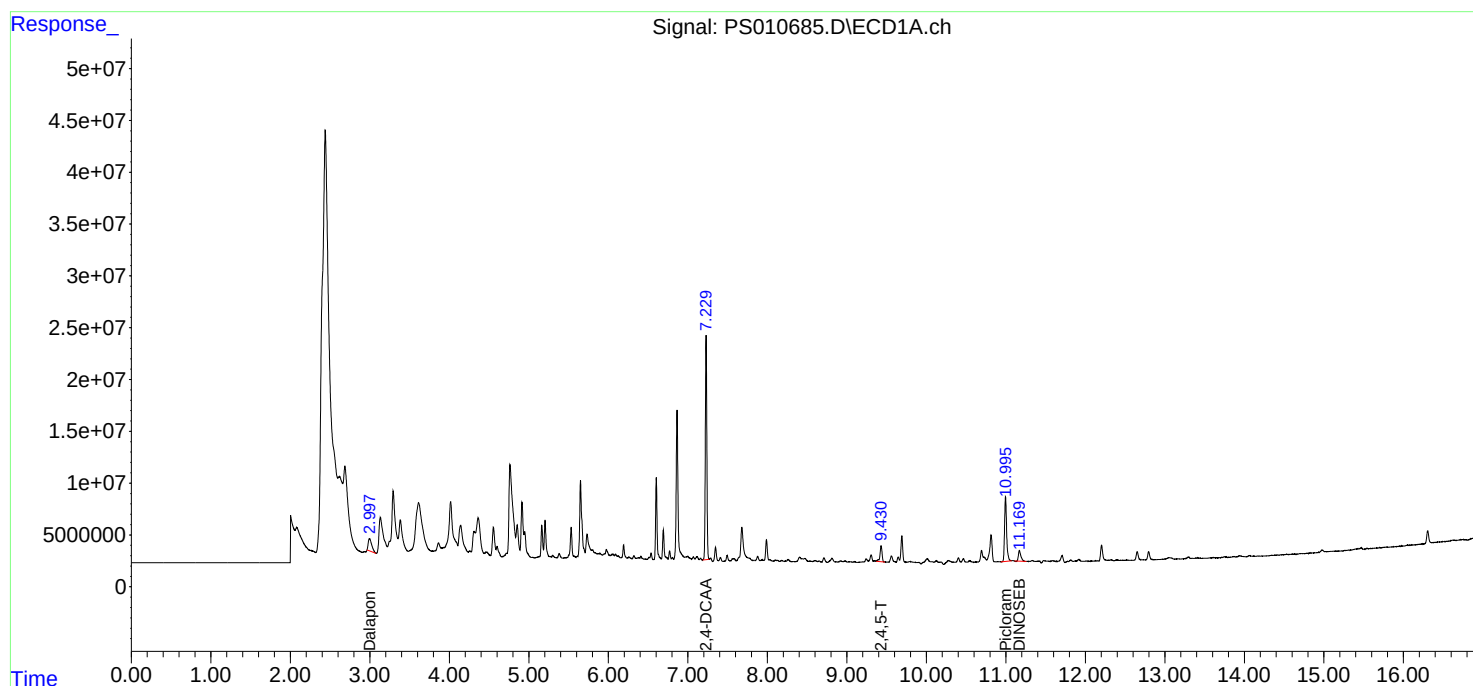


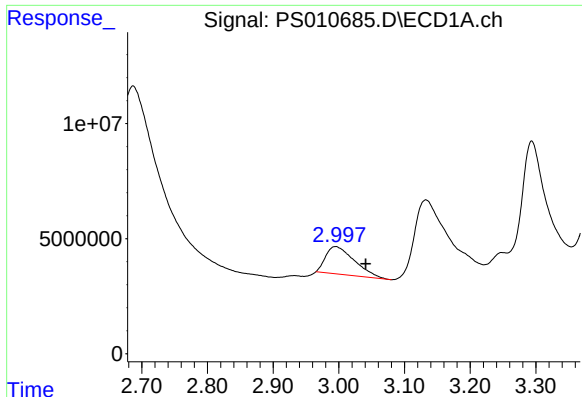

#1 Dalapon


R.T.: 2.995 min
Delta R.T.: -0.046 min
Response: 36291492
Conc: 36.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

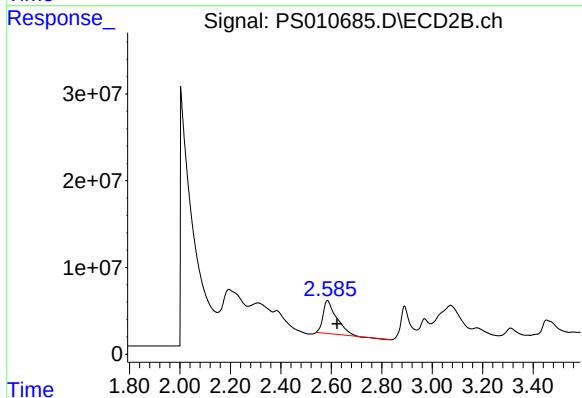


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.039 min
Response: 138082108
Conc: 188.60 ng/ml

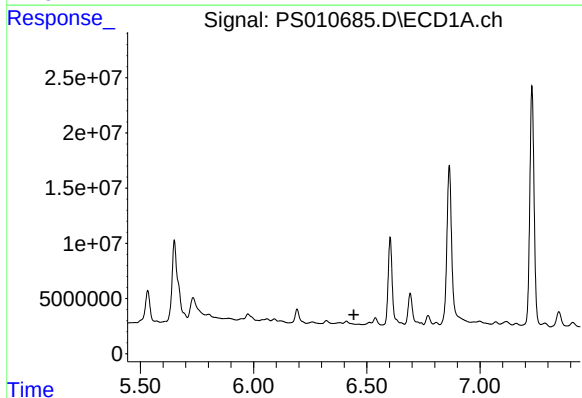


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

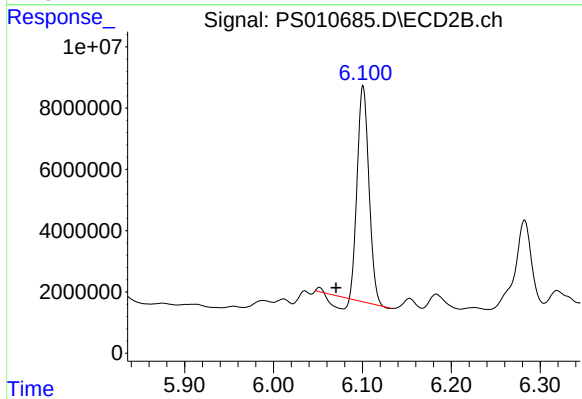

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.031 min
Response: 60981359
Conc: 74.40 ng/ml

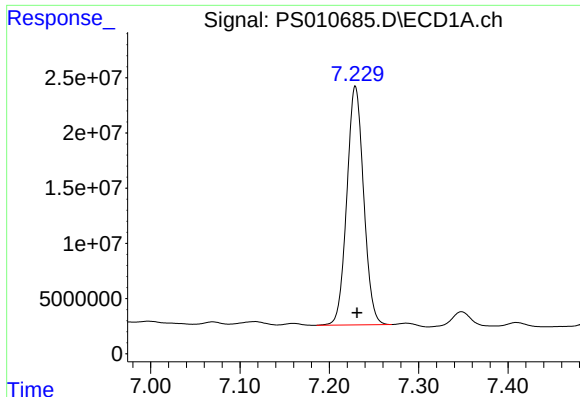

#4 2,4-DCAA


R.T.: 7.229 min
Delta R.T.: -0.002 min
Response: 282677225
Conc: 357.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

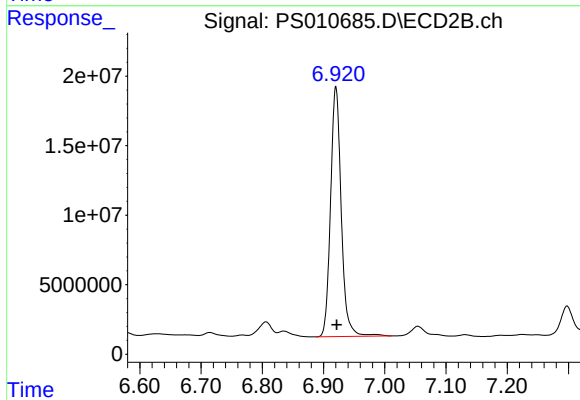


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 218039673
Conc: 399.77 ng/ml

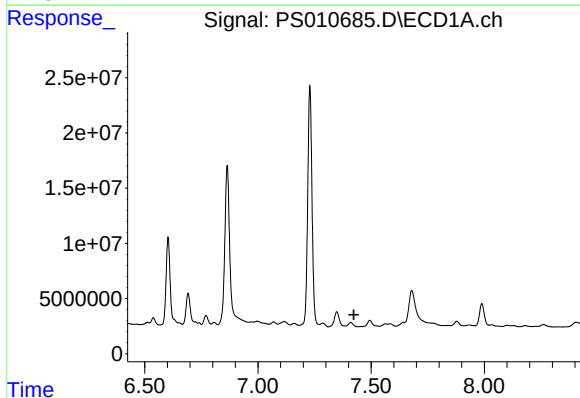


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.423 min
Response: 0
Conc: N.D.

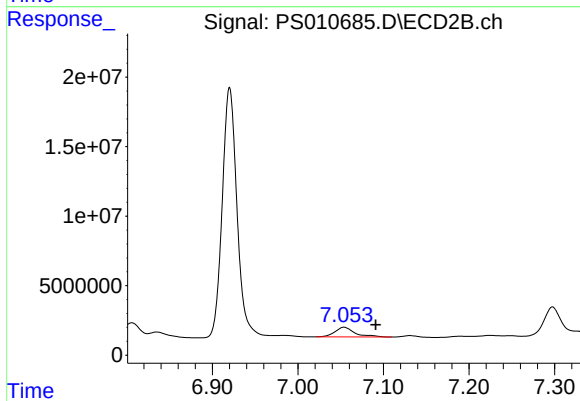

#5 DICAMBA


R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 11286511
Conc: 5.01 ng/ml

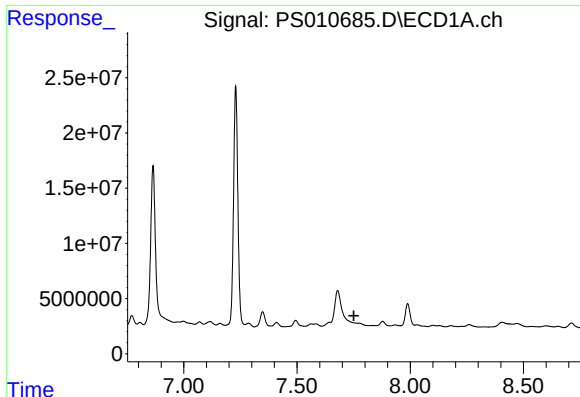

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.751 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

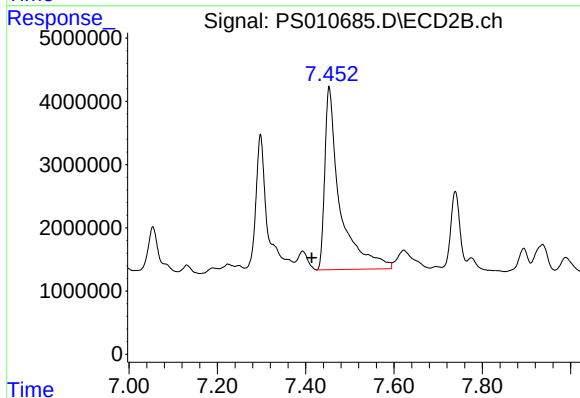


#7 MCPA

R.T.: 7.454 min
Delta R.T.: 0.040 min
Response: 69217891
Conc: 25.47 ug/ml

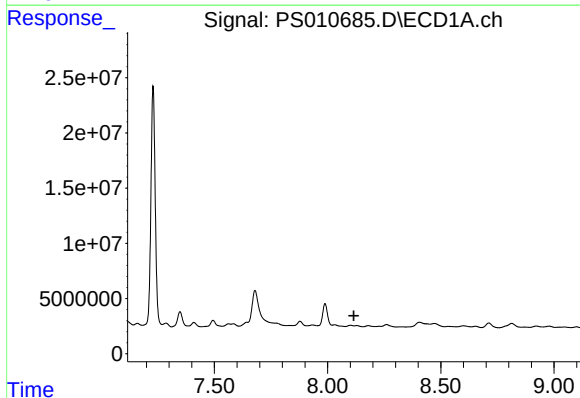


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

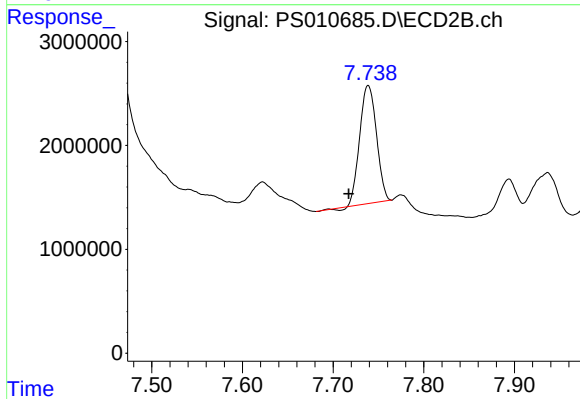

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.022 min
Response: 14549212
Conc: 25.23 ng/ml

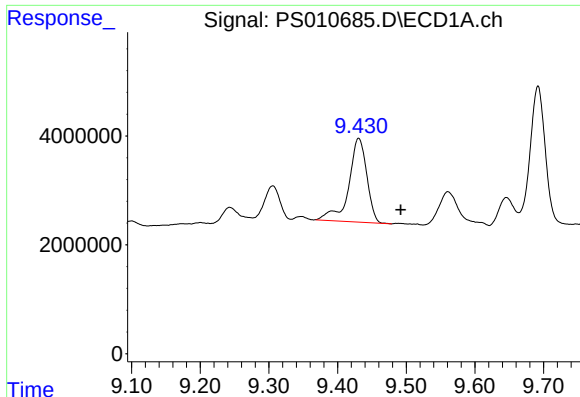

#12 2,4,5-T


R.T.: 9.431 min
Delta R.T.: -0.061 min
Response: 28181986
Conc: 6.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

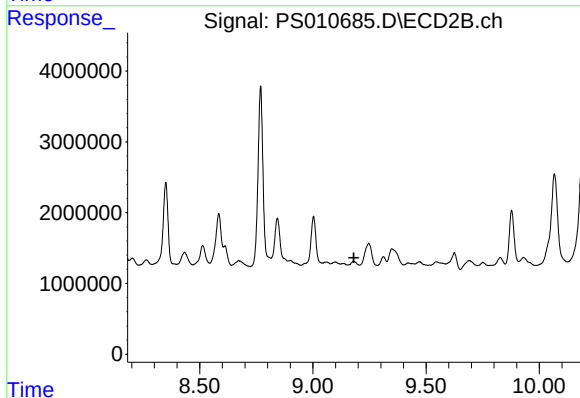


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.181 min
Response: 0
Conc: N.D.

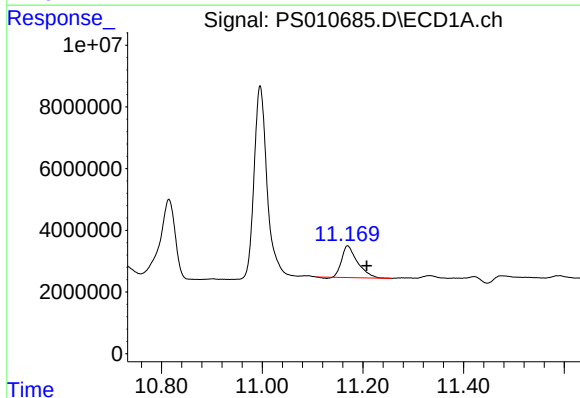


#14 DINOSEB

R.T.: 11.170 min
Delta R.T.: -0.038 min
Response: 22418608
Conc: 6.94 ng/ml

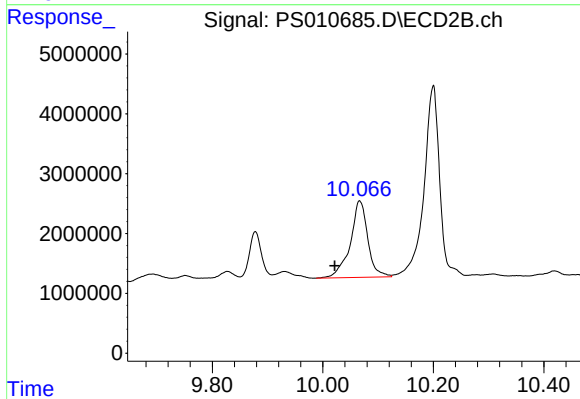

#14 DINOSEB


R.T.: 10.067 min
Delta R.T.: 0.045 min
Response: 28141391
Conc: 13.08 ng/ml

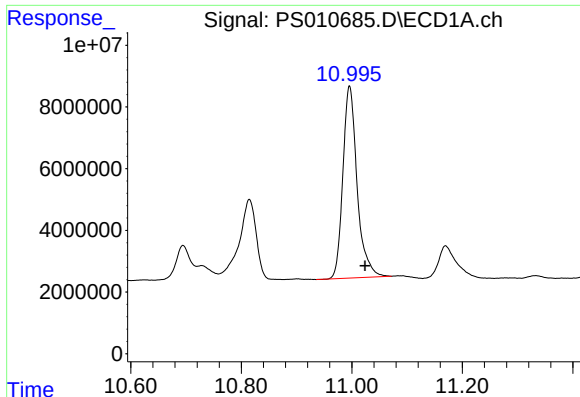

#15 Picloram


R.T.: 10.996 min
Delta R.T.: -0.028 min
Response: 111207557
Conc: 21.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

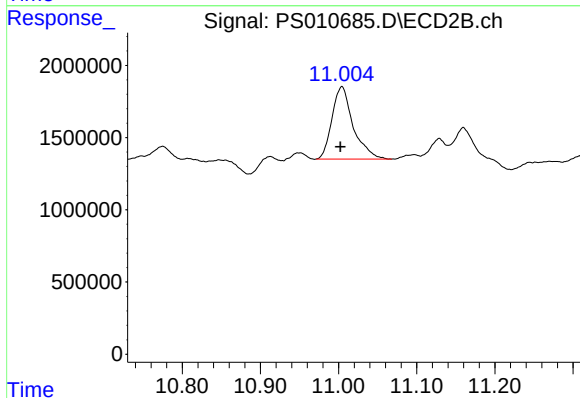


#15 Picloram

R.T.: 11.004 min
Delta R.T.: 0.002 min
Response: 9431363
Conc: 2.29 ng/ml

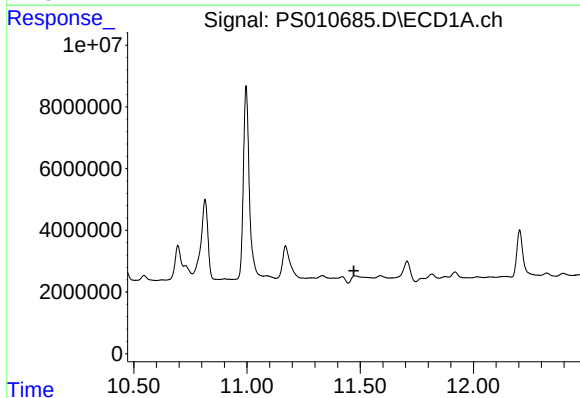

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.472 min
Response: 0
Conc: N.D.

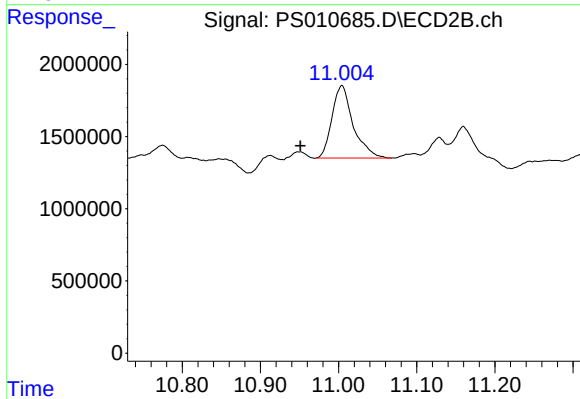

#16 DCPA

R.T.: 11.004 min
Delta R.T.: 0.053 min
Response: 9431363
Conc: 2.54 ng/ml