

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
 Data File : PS010690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2020 03:03
 Operator : DD\AJ
 Sample : L2837-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 04:35:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	263.7E6	203.8E6	333.470	373.707
Target Compounds							
1) T	Dalapon	2.993	2.584	36940614	160.6E6	37.572	219.320 #
2) T	3,5-DICHL...	0.000	6.101	0	78253935	N.D.	95.473
5) T	DICAMBA	0.000	7.054	0	14469025	N.D.	6.428
7) T	MCPA	0.000	7.452	0	82434679	N.D.	30.332
8) T	DICHLORPROP	0.000	7.739	0	12602160	N.D.	21.855
9) T	2,4-D	8.343	8.010	13063178	17546109	16.572	23.140 #
10) T	Pentachlo...	8.712	0.000	7519267	0	<MDL	N.D. #
12) T	2,4,5-T	9.431	0.000	26504162	0	6.517	N.D. #
14) T	DINOSEB	11.169	10.067	24620820	33648616	7.620	15.640 #
15) T	Picloram	10.996	11.003	161.1E6	37336752	31.556	9.049 #
16) T	DCPA	0.000	11.003	0	37336752	N.D.	10.069


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
Data File : PS010690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2020 03:03
Operator : DD\AJ
Sample : L2837-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 04:35:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

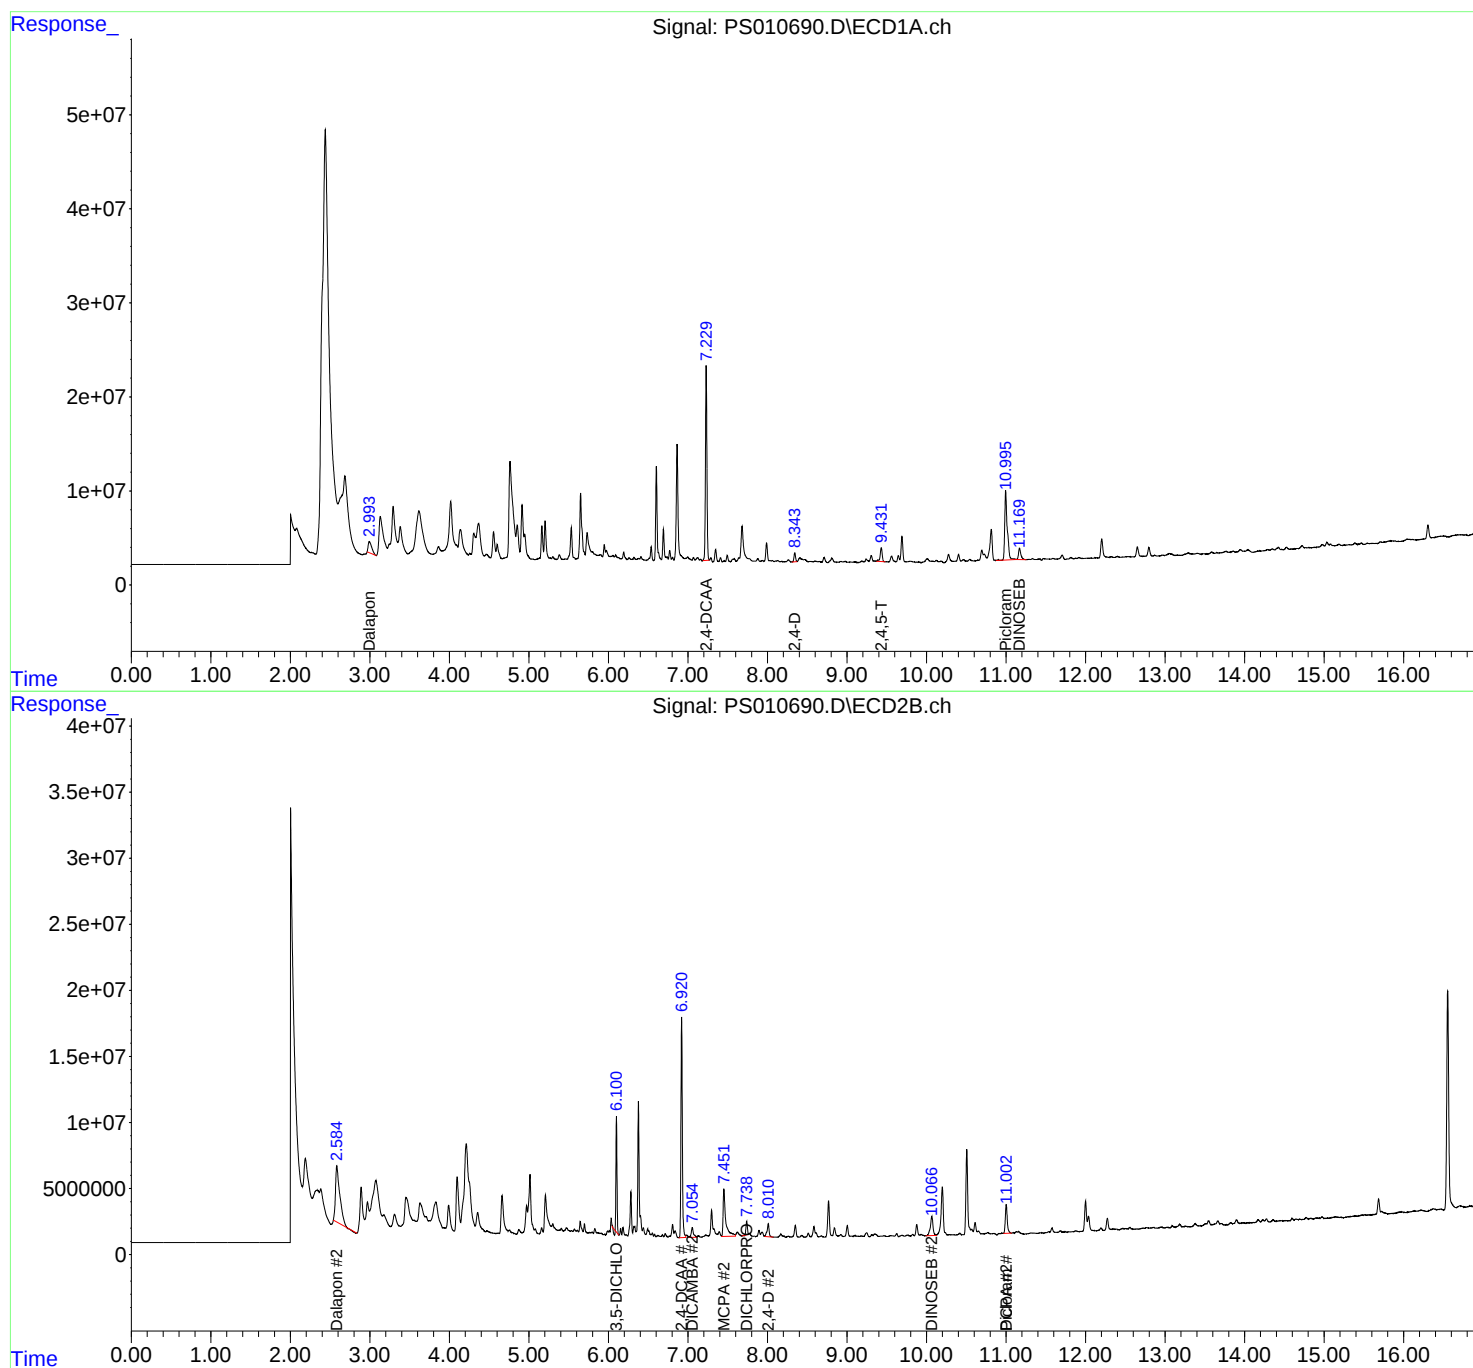


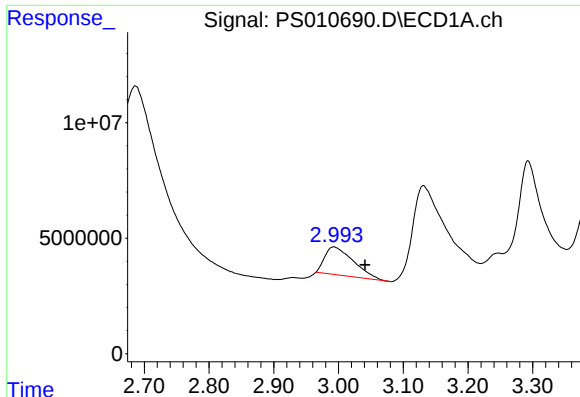

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.048 min
Response: 36940614
Conc: 37.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

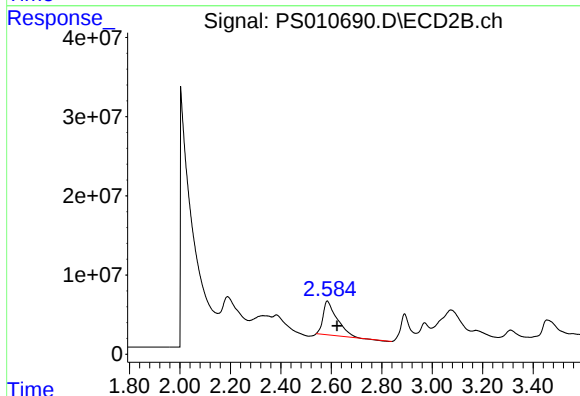


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.039 min
Response: 160573918
Conc: 219.32 ng/ml

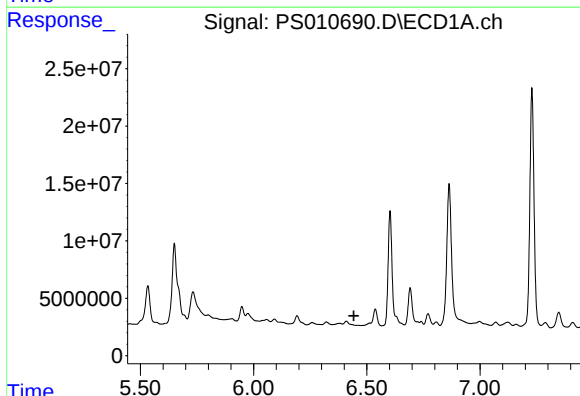


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

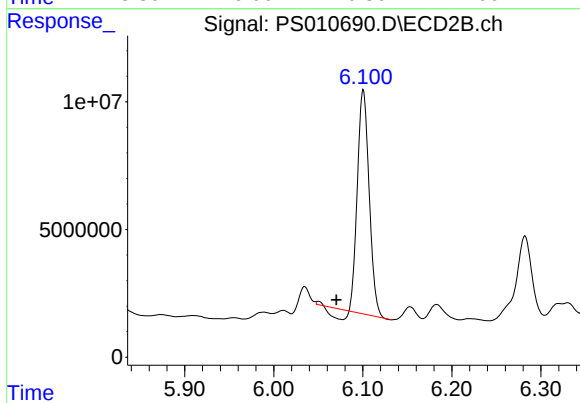

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 78253935
Conc: 95.47 ng/ml

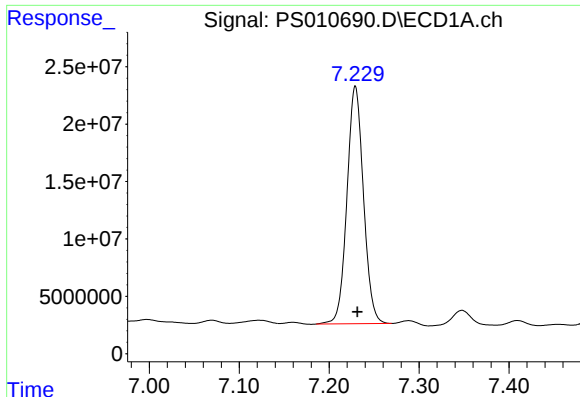

#4 2,4-DCAA


R.T.: 7.229 min
Delta R.T.: -0.002 min
Response: 263728454
Conc: 333.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

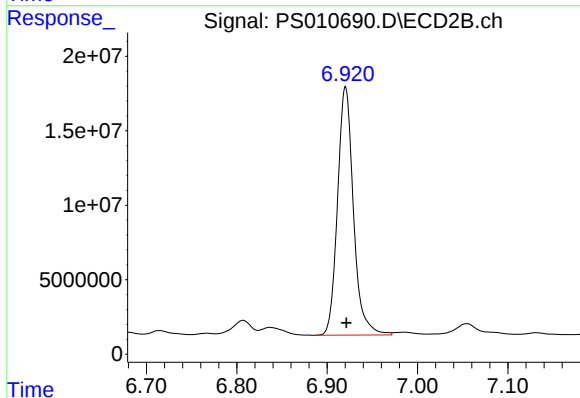


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 203825960
Conc: 373.71 ng/ml

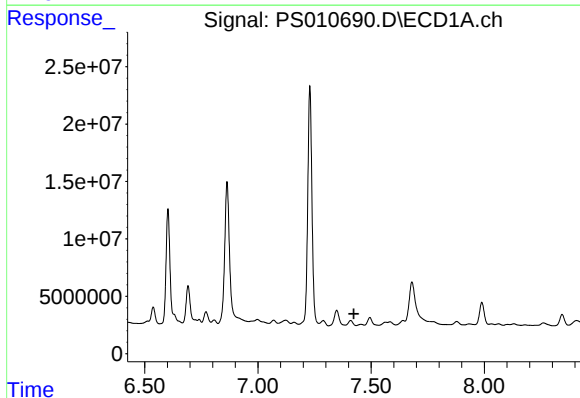


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.423 min
Response: 0
Conc: N.D.

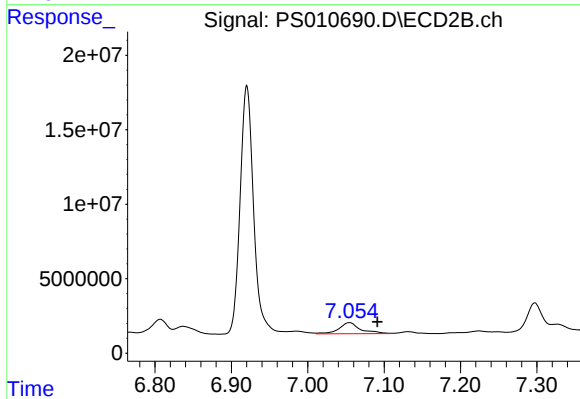

#5 DICAMBA


R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 14469025
Conc: 6.43 ng/ml

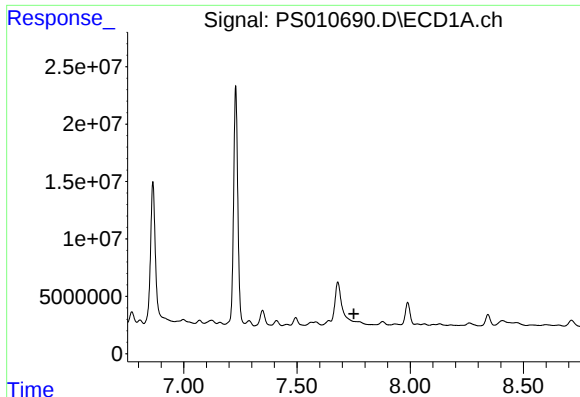

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.751 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

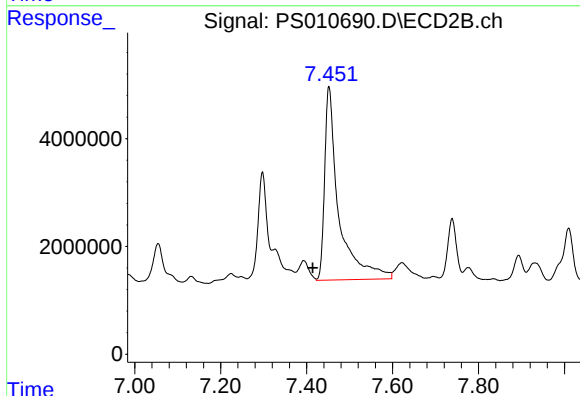


#7 MCPA

R.T.: 7.452 min
Delta R.T.: 0.038 min
Response: 82434679
Conc: 30.33 ug/ml

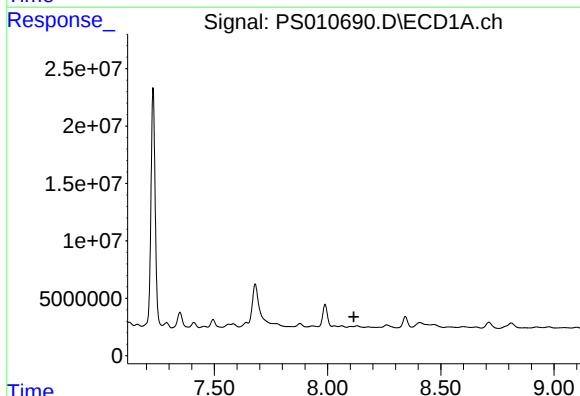


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

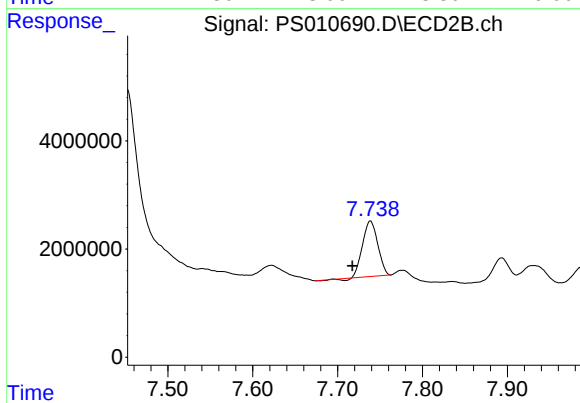

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.021 min
Response: 12602160
Conc: 21.85 ng/ml

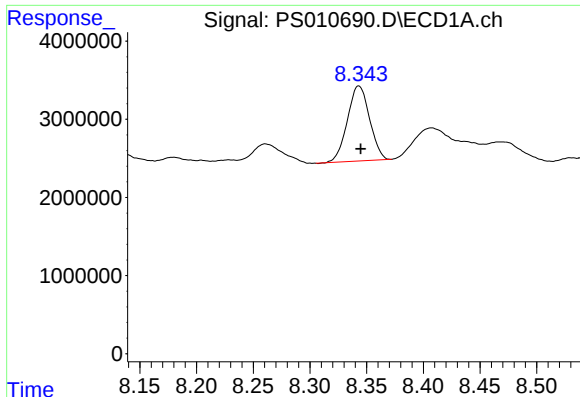

#9 2,4-D


R.T.: 8.343 min
Delta R.T.: -0.002 min
Response: 13063178
Conc: 16.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

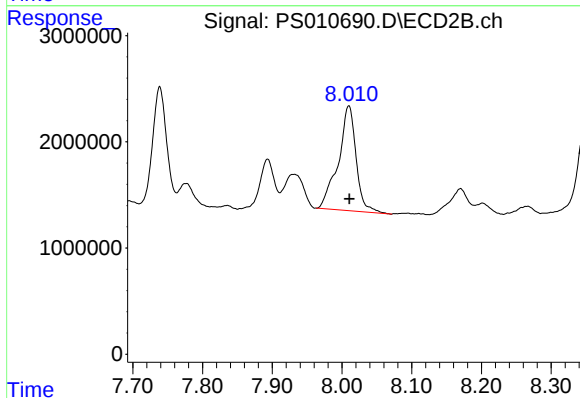


#9 2,4-D

R.T.: 8.010 min
Delta R.T.: 0.000 min
Response: 17546109
Conc: 23.14 ng/ml

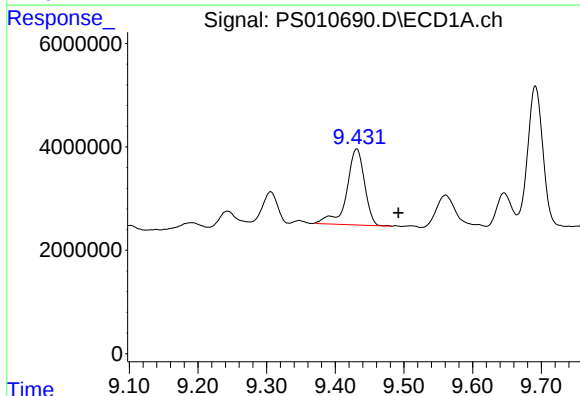


#12 2,4,5-T

R.T.: 9.431 min
Delta R.T.: -0.061 min
Response: 26504162
Conc: 6.52 ng/ml

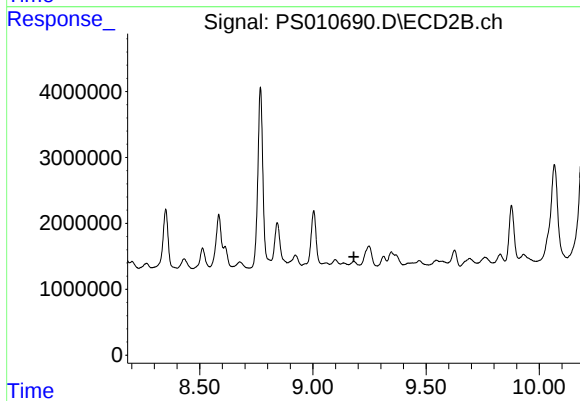

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.181 min
Response: 0
Conc: N.D.

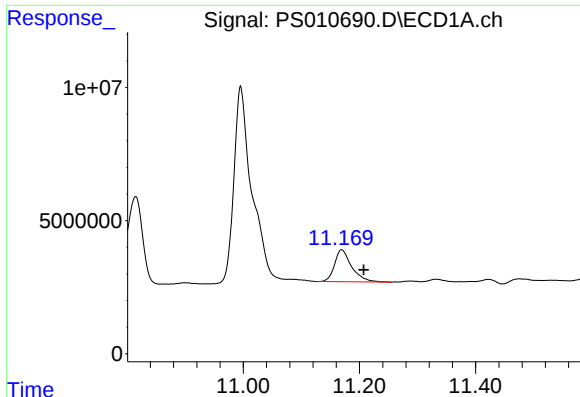

#14 DINOSEB


R.T.: 11.169 min
Delta R.T.: -0.038 min
Response: 24620820
Conc: 7.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

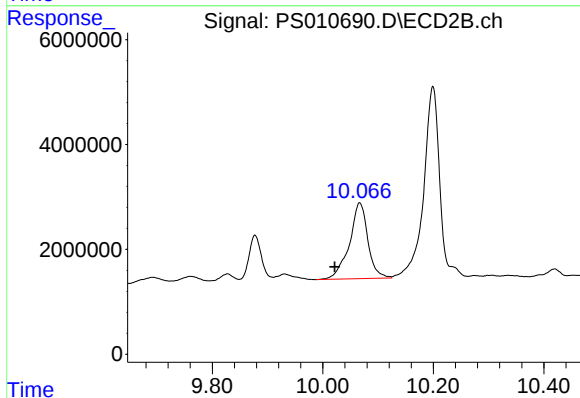


#14 DINOSEB

R.T.: 10.067 min
Delta R.T.: 0.045 min
Response: 33648616
Conc: 15.64 ng/ml

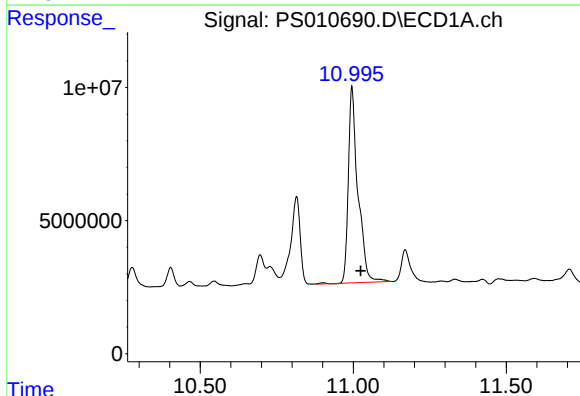


#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.028 min
Response: 161099405
Conc: 31.56 ng/ml

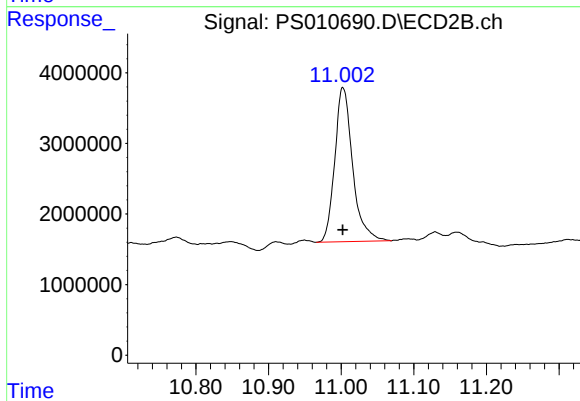

#15 Picloram


R.T.: 11.003 min
Delta R.T.: 0.000 min
Response: 37336752
Conc: 9.05 ng/ml

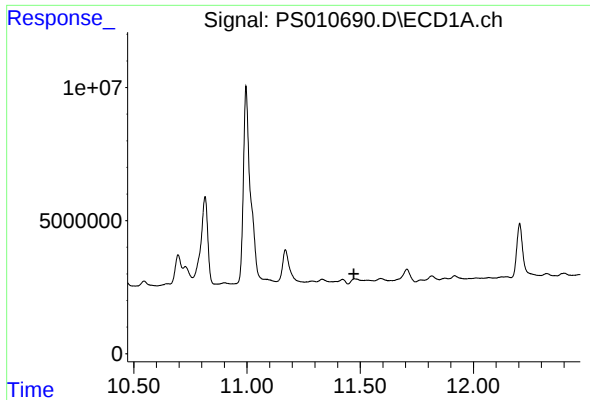

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

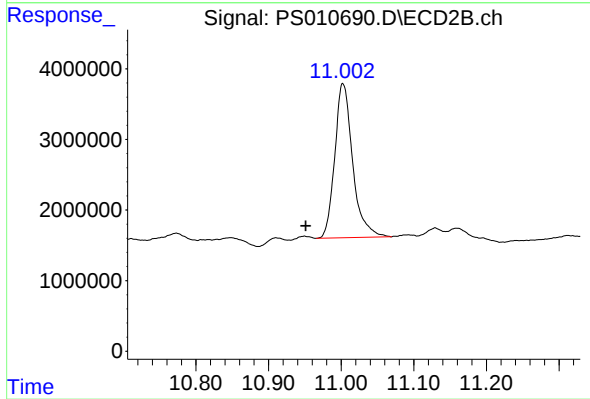

#16 DCPA

R.T.: 11.003 min
Delta R.T.: 0.051 min
Response: 37336752
Conc: 10.07 ng/ml