

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
 Data File : PS010691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2020 03:26
 Operator : DD\AJ
 Sample : L2871-04
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 04:35:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.921	322.4E6	232.1E6	407.651	425.535
Target Compounds							
1) T	Dalapon	2.993	2.584	32980998	91484330	33.545	124.954 #
2) T	3,5-DICHL...	0.000	6.101	0	79801960	N.D.	97.362
3) T	4-Nitroph...	7.106	0.000	8514406	0	22.967	N.D. #
5) T	DICAMBA	7.410	7.054	6123903	10994729	1.948	4.885 #
7) T	MCPA	0.000	7.452	0	112.4E6	N.D.	41.349
8) T	DICHLORPROP	0.000	7.739	0	14575439	N.D.	25.277
10) T	Pentachlo...	8.713	0.000	8363434	0	<MDL	N.D. #
12) T	2,4,5-T	9.431	0.000	22212181	0	5.462	N.D. #
14) T	DINOSEB	0.000	10.067	0	32796597	N.D.	15.244
15) T	Picloram	10.996	0.000	41385794	0	8.107	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060420\
Data File : PS010691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2020 03:26
Operator : DD\AJ
Sample : L2871-04
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 04:35:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

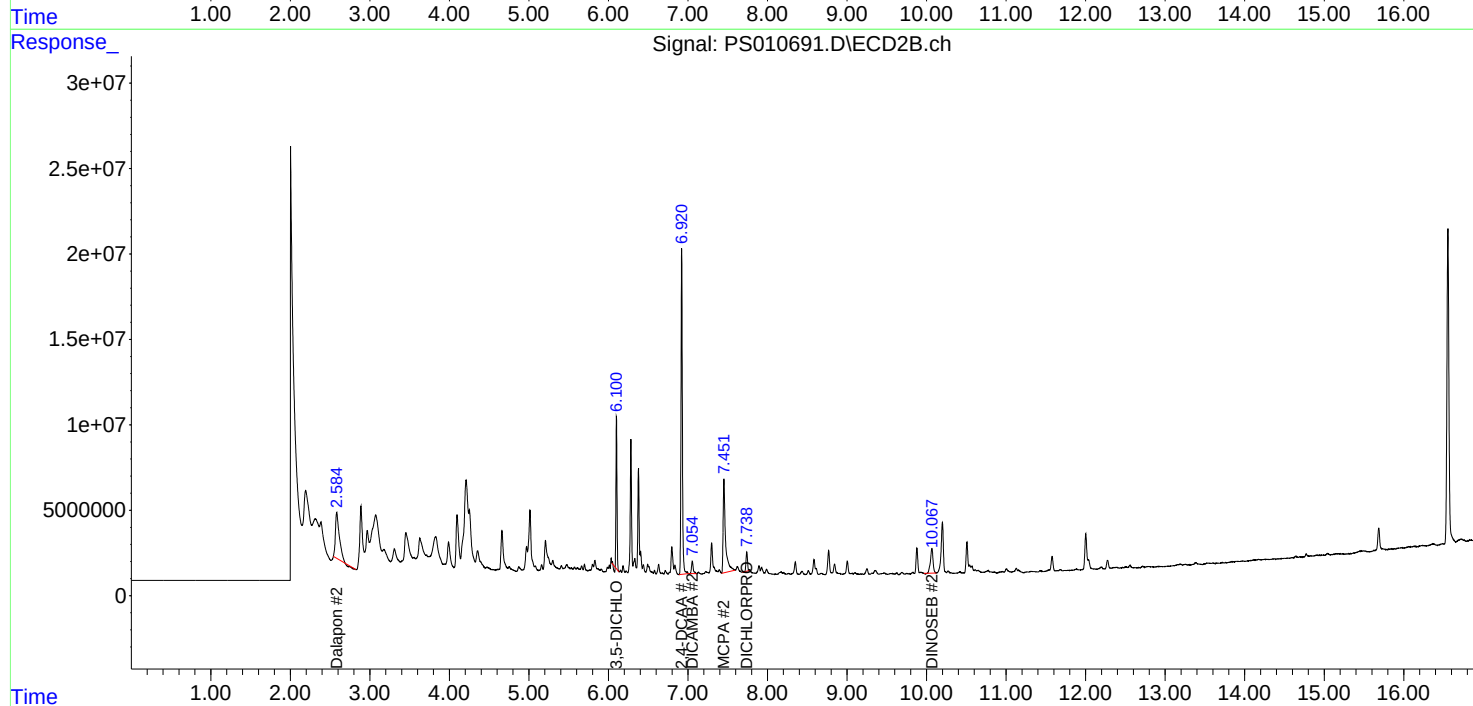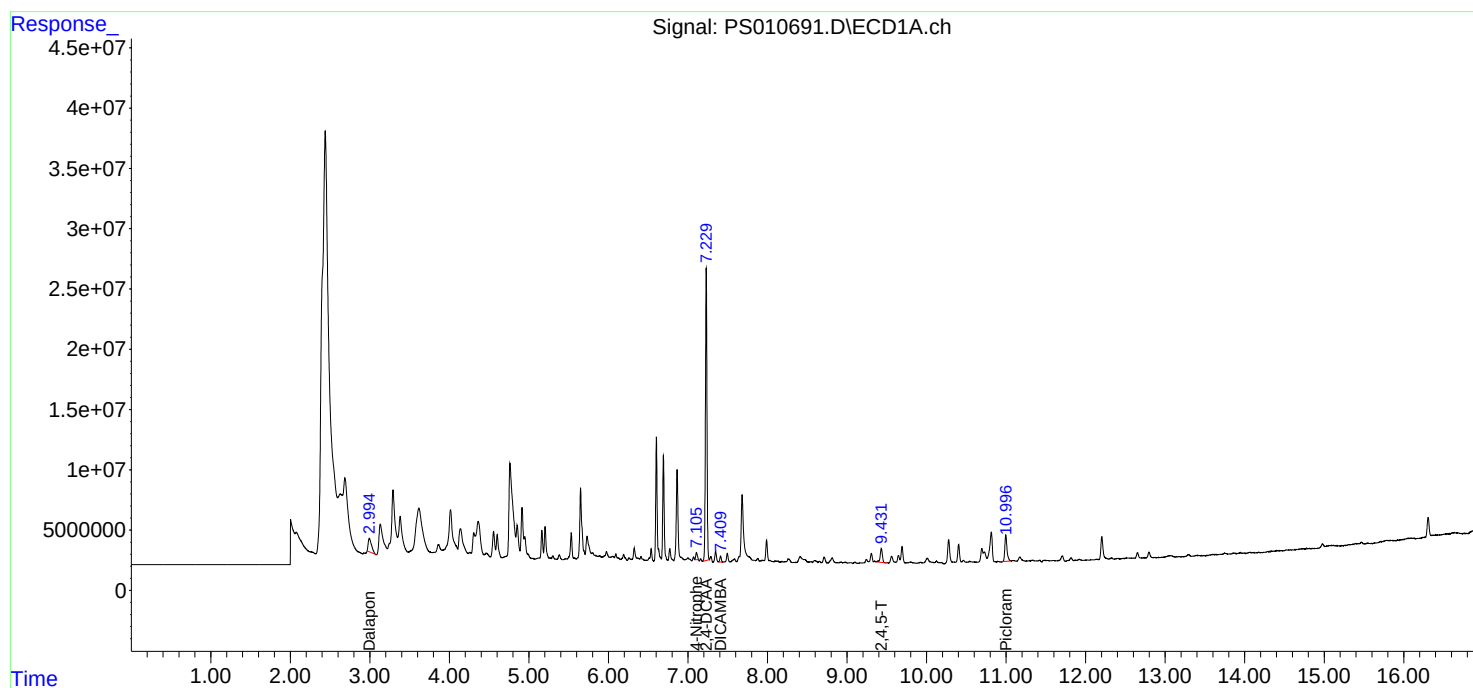


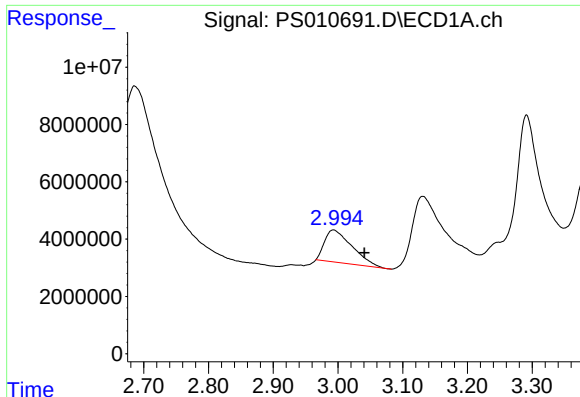

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.048 min
Response: 32980998
Conc: 33.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

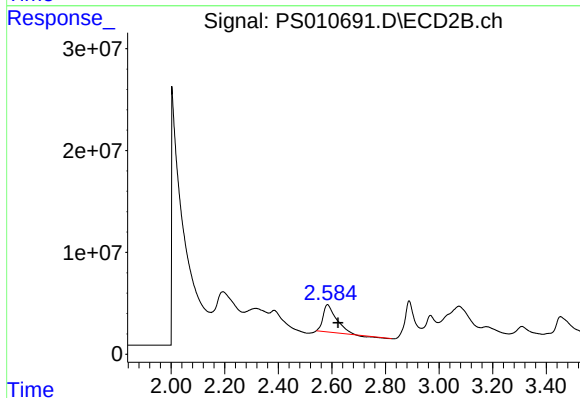


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.040 min
Response: 91484330
Conc: 124.95 ng/ml

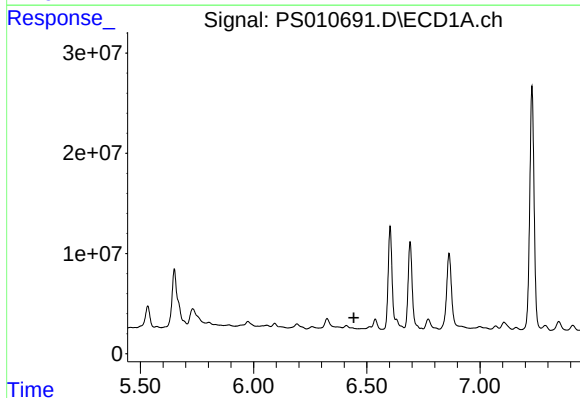


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

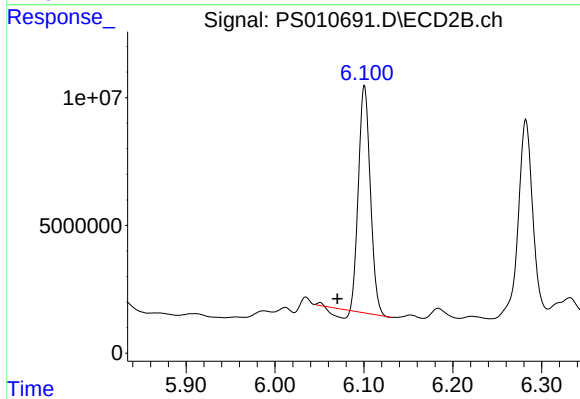

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 79801960
Conc: 97.36 ng/ml

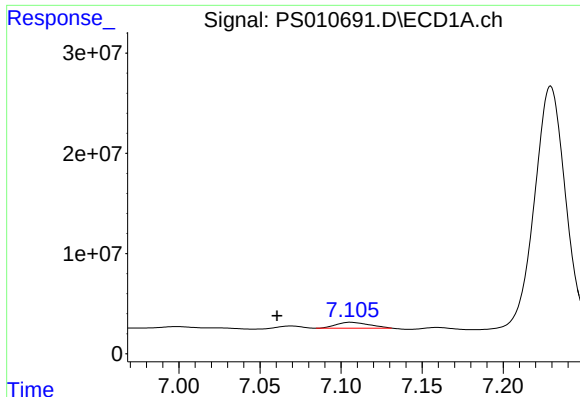

#3 4-Nitrophenol


R.T.: 7.106 min
Delta R.T.: 0.046 min
Response: 8514406
Conc: 22.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

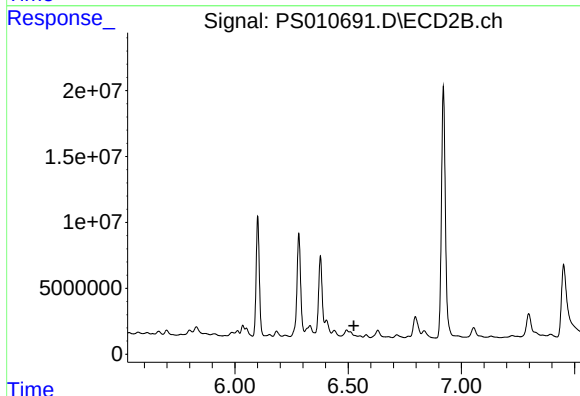


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

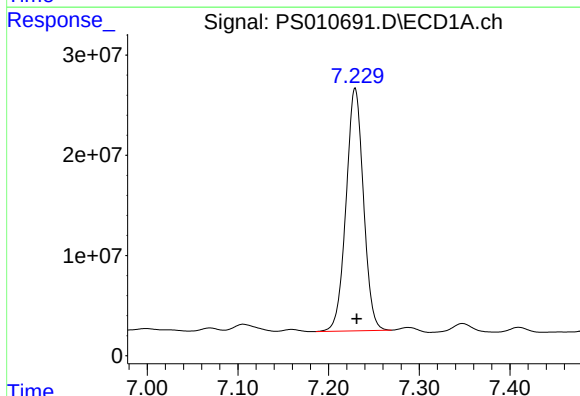


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: -0.002 min
Response: 322395948
Conc: 407.65 ng/ml

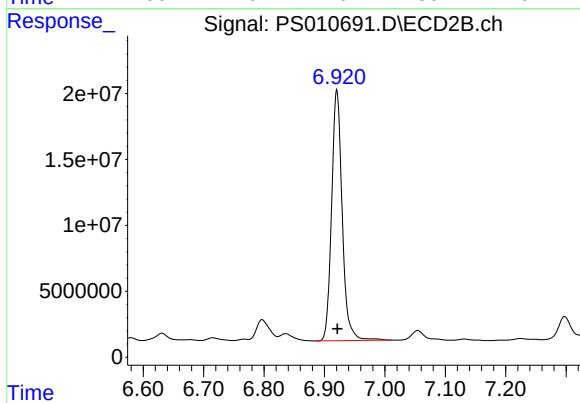

#4 2,4-DCAA


R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 232093298
Conc: 425.53 ng/ml

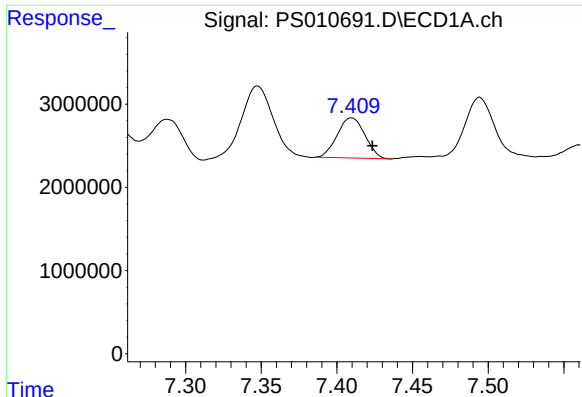

#5 DICAMBA


R.T.: 7.410 min
Delta R.T.: -0.014 min
Response: 6123903
Conc: 1.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

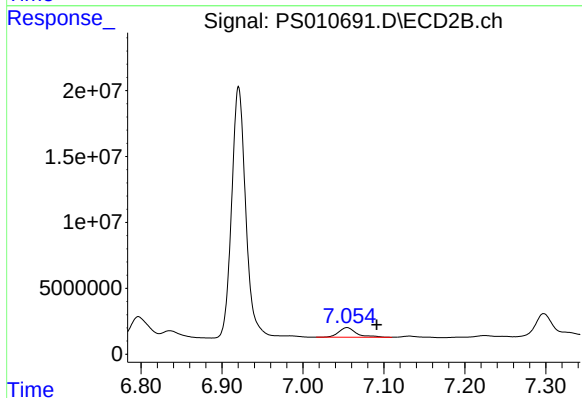


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 10994729
Conc: 4.88 ng/ml

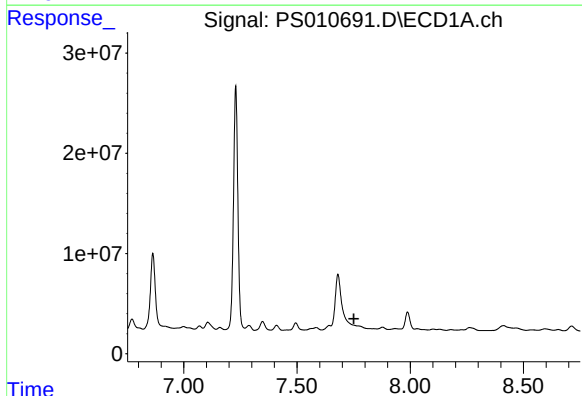


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.751 min
Response: 0
Conc: N.D.

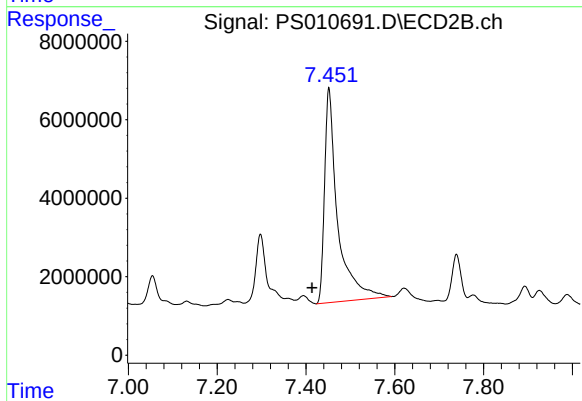

#7 MCPA


R.T.: 7.452 min
Delta R.T.: 0.038 min
Response: 112375140
Conc: 41.35 ug/ml

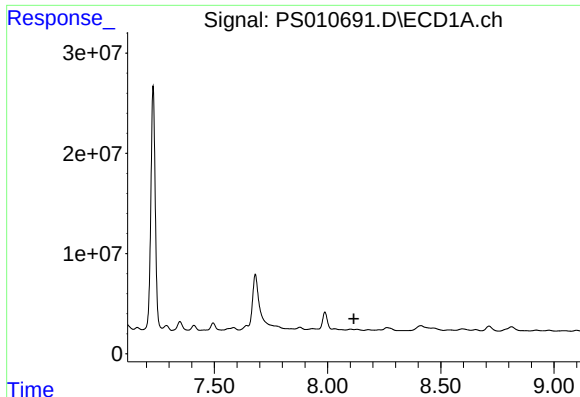

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

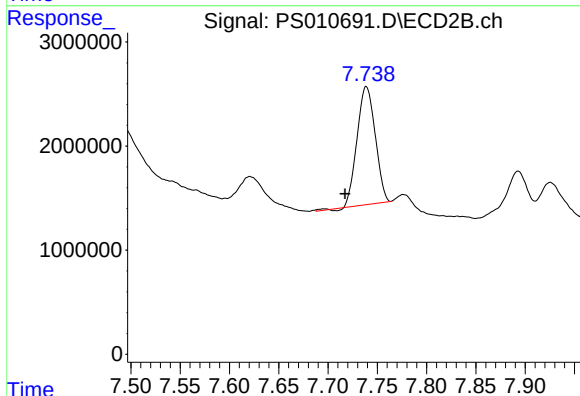


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.022 min
Response: 14575439
Conc: 25.28 ng/ml

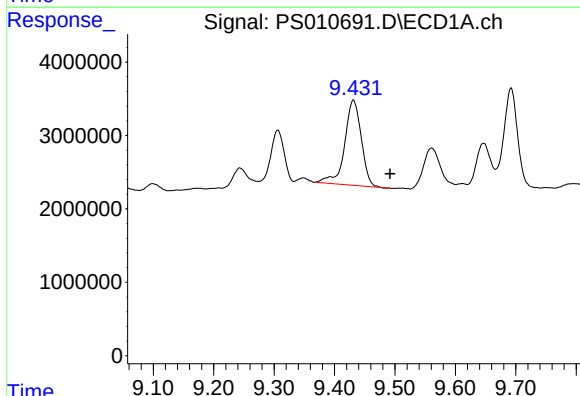


#12 2,4,5-T

R.T.: 9.431 min
Delta R.T.: -0.061 min
Response: 22212181
Conc: 5.46 ng/ml

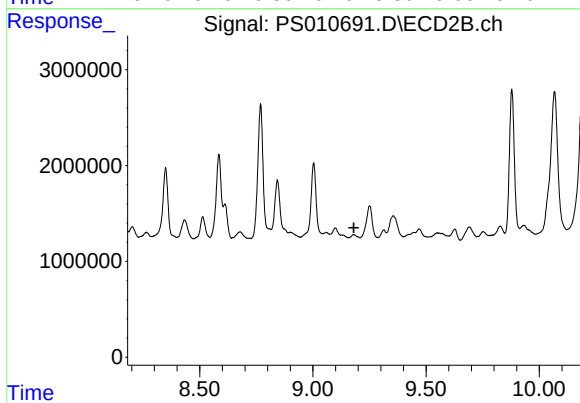

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

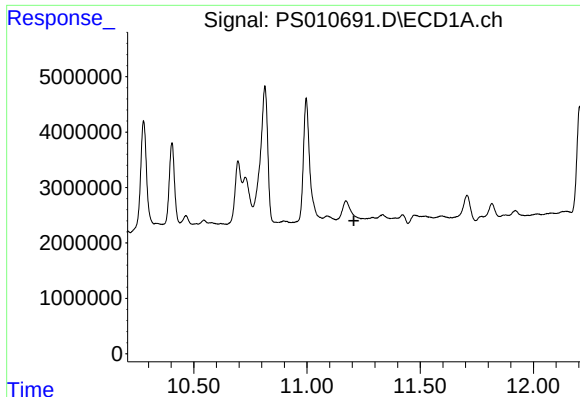

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

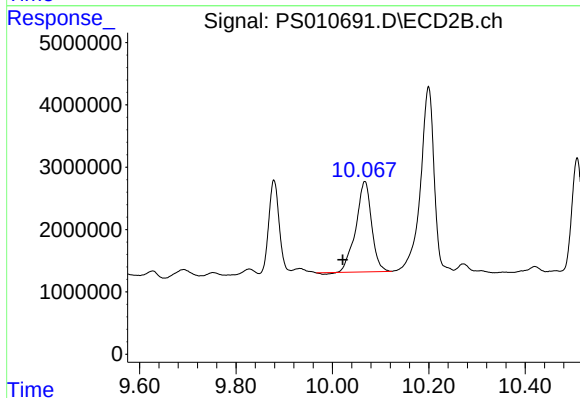


#14 DINOSEB

R.T.: 10.067 min
Delta R.T.: 0.045 min
Response: 32796597
Conc: 15.24 ng/ml

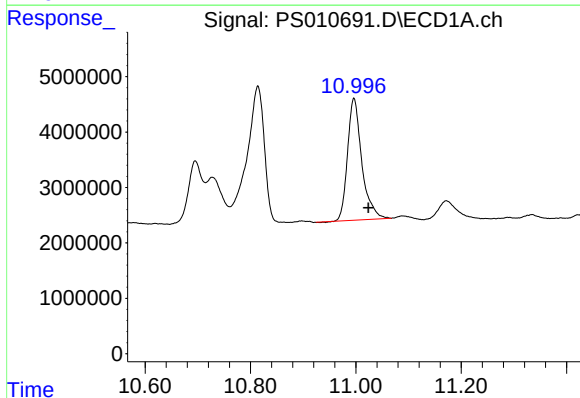

#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.028 min
Response: 41385794
Conc: 8.11 ng/ml

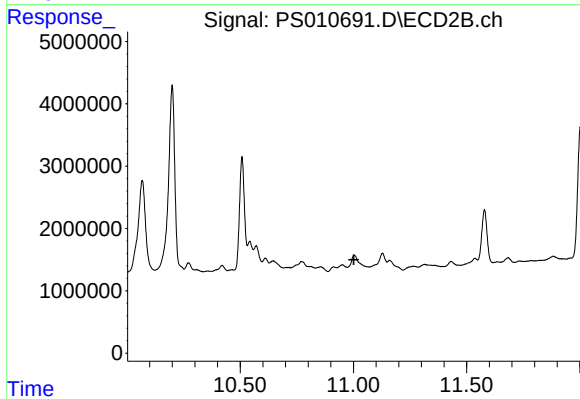

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.002 min
Response: 0
Conc: N.D.