

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060421\
 Data File : PS015203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2021 14:00
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 05:48:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.784	1140.9E6	279.6E6	452.668	521.905
Target Compounds							
2) T	3,5-DICHL...	0.000	5.966	0	4869718	N.D.	6.028
3) T	4-Nitroph...	7.027	0.000	8638805	0	6.128	N.D. #
5) T	DICAMBA	7.460f	0.000	13960590	0	1.465	N.D. #
6) T	MCP	7.589	0.000	10529677	0	1.463	N.D. #
7) T	MCPA	7.720	0.000	67312783	0	6.707	N.D. #
15) T	Picloram	11.017	0.000	4736420	0	<MDL	N.D. #
16) T	DCPA	11.542f	0.000	9717877	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060421\
Data File : PS015203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2021 14:00
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 05:48:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

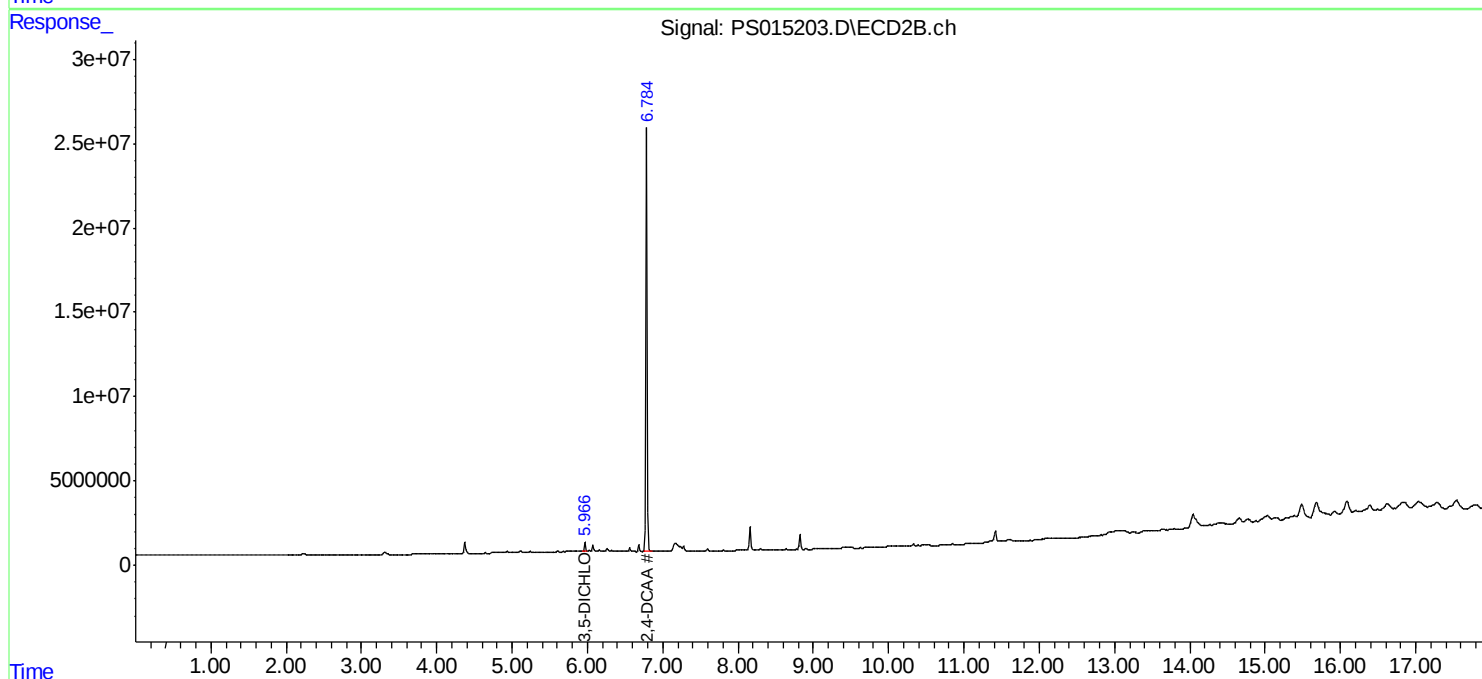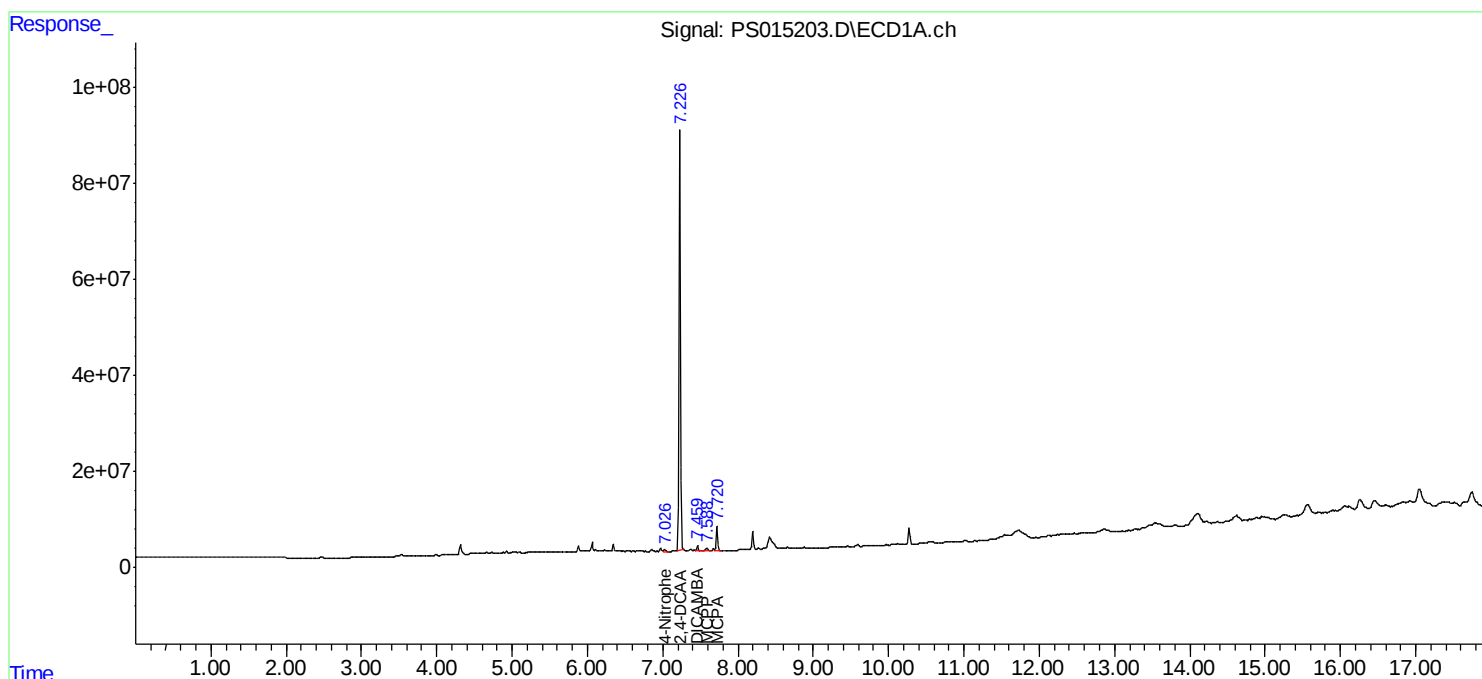


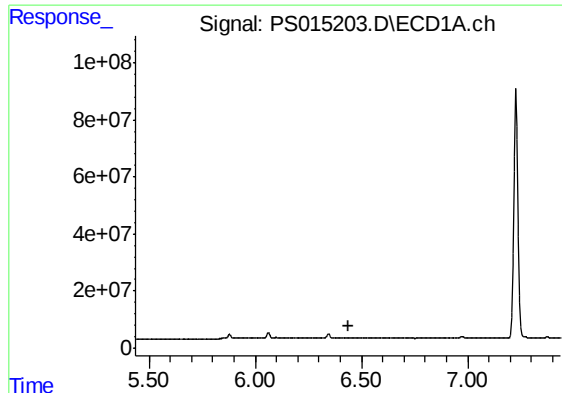

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

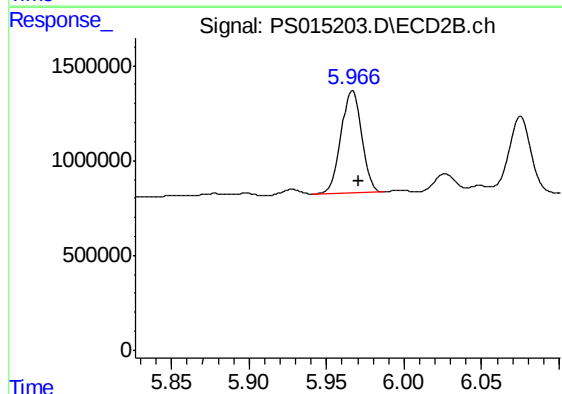


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.966 min
Delta R.T.: -0.005 min
Response: 4869718
Conc: 6.03 ng/ml

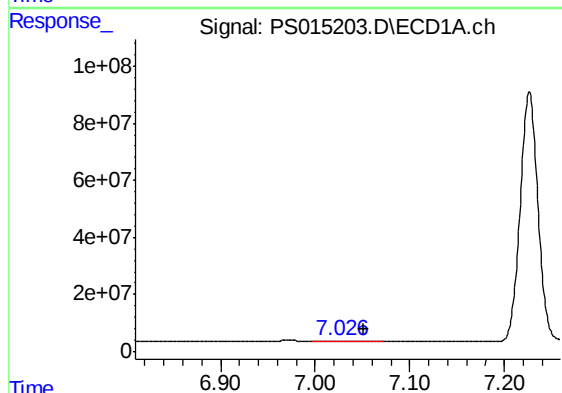


#3 4-Nitrophenol

R.T.: 7.027 min
Delta R.T.: -0.025 min
Response: 8638805
Conc: 6.13 ng/ml

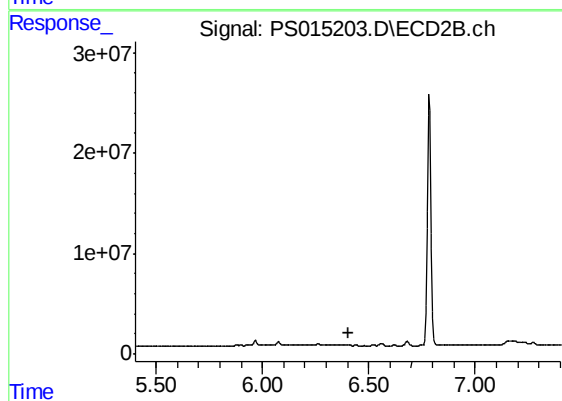

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

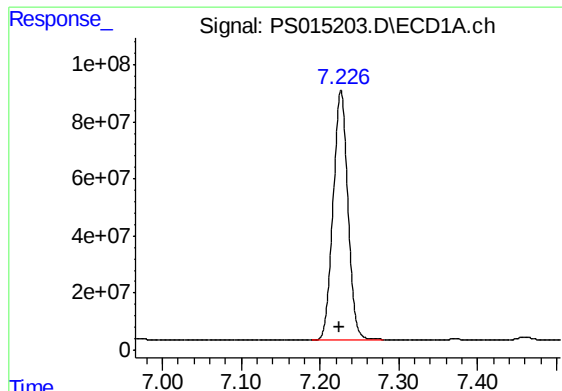

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.001 min
Response: 1140894281
Conc: 452.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

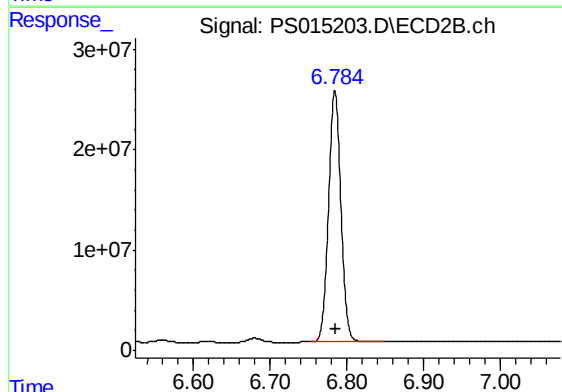


#4 2,4-DCAA

R.T.: 6.784 min
Delta R.T.: -0.002 min
Response: 279621336
Conc: 521.90 ng/ml

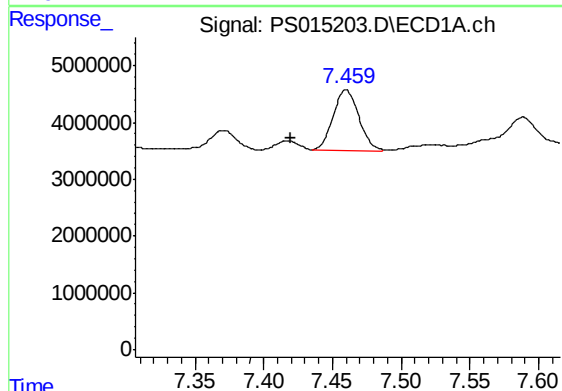


#5 DICAMBA

R.T.: 7.460 min
Delta R.T.: 0.041 min
Response: 13960590
Conc: 1.46 ng/ml

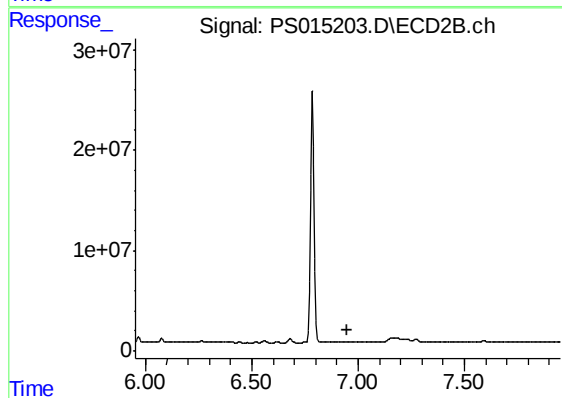

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

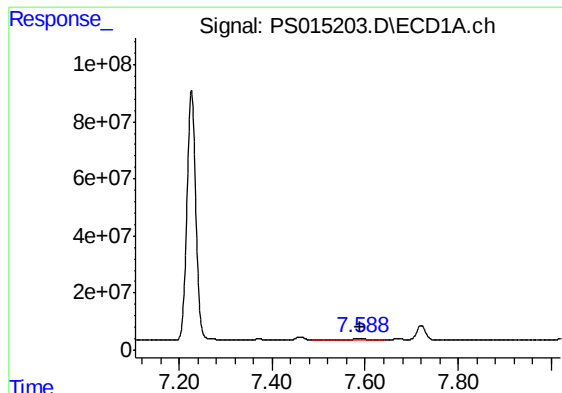

#6 MCPP


R.T.: 7.589 min
Delta R.T.: -0.001 min
Response: 10529677
Conc: 1.46 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

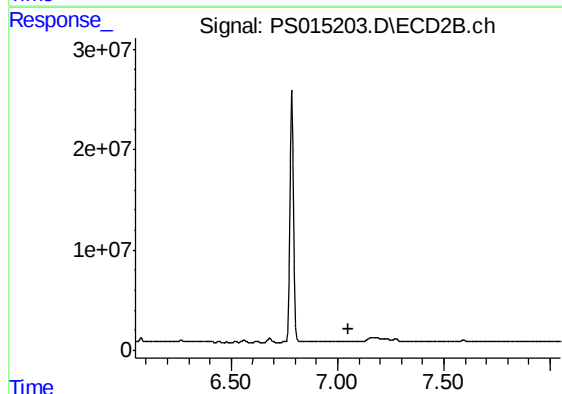


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.049 min
Response: 0
Conc: N.D.

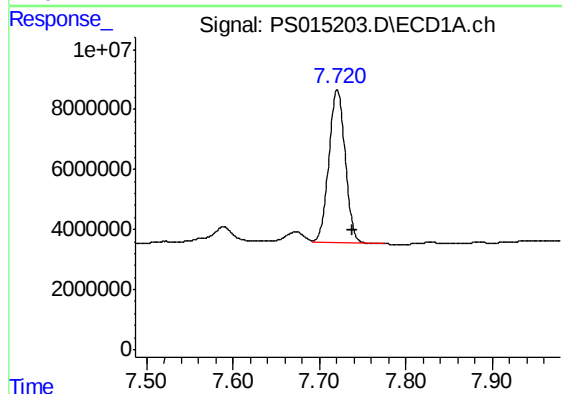

#7 MCPA

R.T.: 7.720 min
Delta R.T.: -0.018 min
Response: 67312783
Conc: 6.71 ug/ml

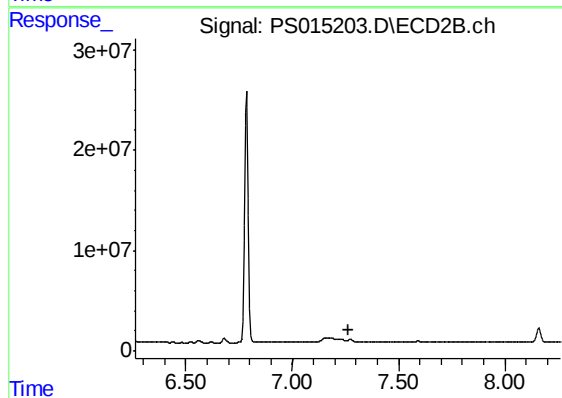

#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.