

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060421\
 Data File : PS015202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2021 13:36
 Operator : DD\AJ
 Sample : M2580-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 18-B5(0-2)

Manual Integrations
 APPROVED

Ankita
 6/8/2021 1:15:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 05:47:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.786	936.7E6	205.3E6	371.633m	383.116
Target Compounds							
10) T	Pentachlo...	8.656	8.295	4324.3E6	1358.8E6	133.586	184.584 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060421\
Data File : PS015202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2021 13:36
Operator : DD\AJ
Sample : M2580-13
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
18-B5(0-2)


Manual Integrations
APPROVED

Ankita
6/8/2021 1:15:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 05:47:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

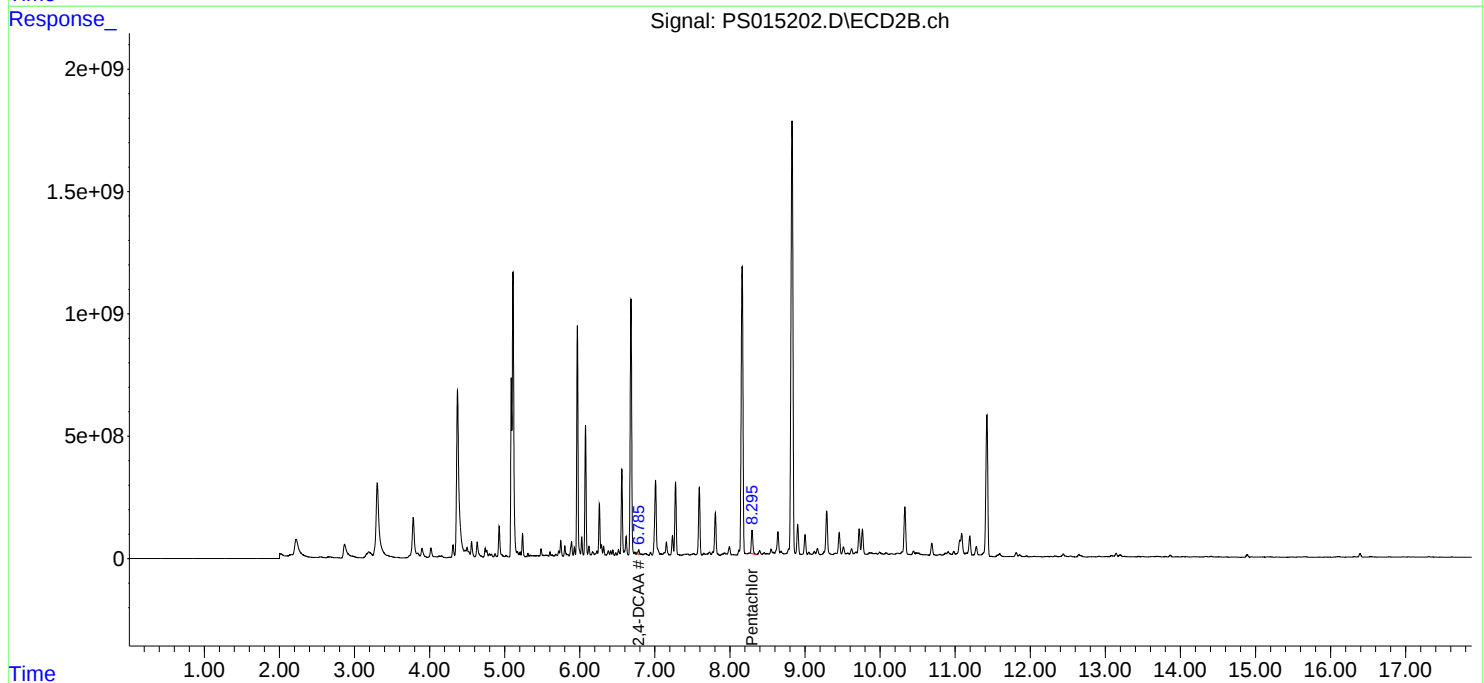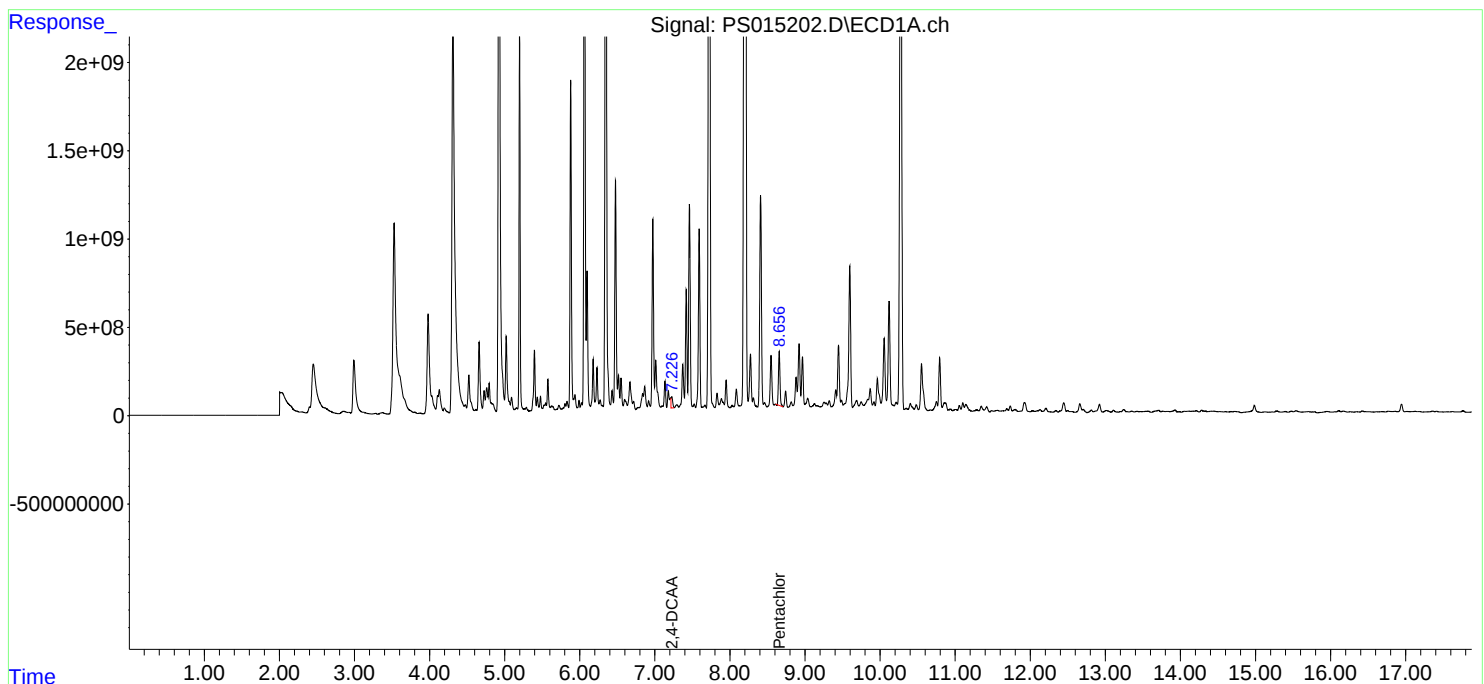

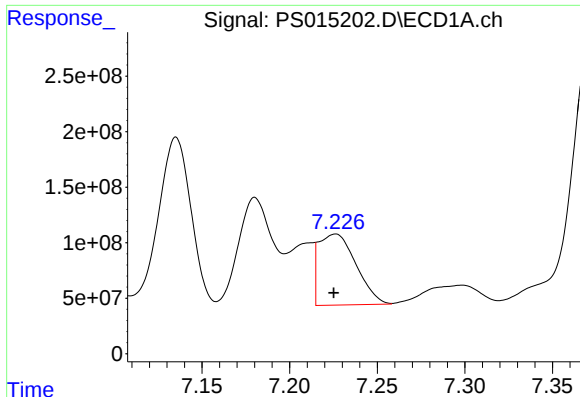


#4 2,4-DCAA

R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 936653522
Conc: 371.63 ng/ml m

Instrument :
ECD_S
ClientSampleId :
18-B5(0-2)


Manual Integrations
APPROVED

Ankita
6/8/2021 1:15:05 PM

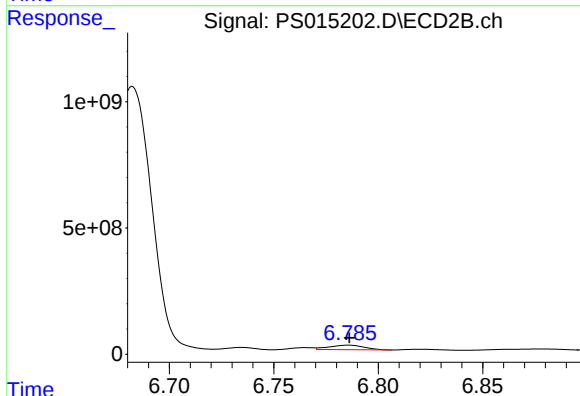


#4 2,4-DCAA

R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 205262322
Conc: 383.12 ng/ml

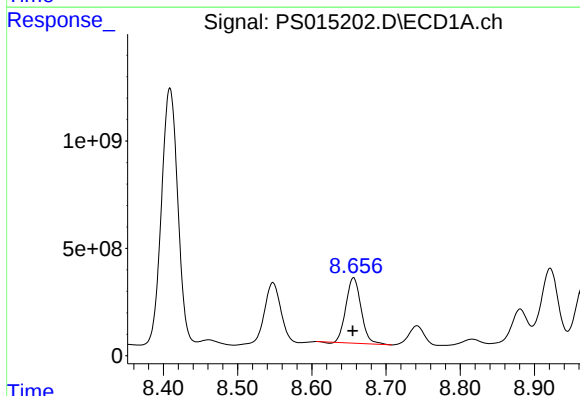

#10 Pentachlorophenol

R.T.: 8.656 min
Delta R.T.: 0.001 min
Response: 4324275085
Conc: 133.59 ng/ml

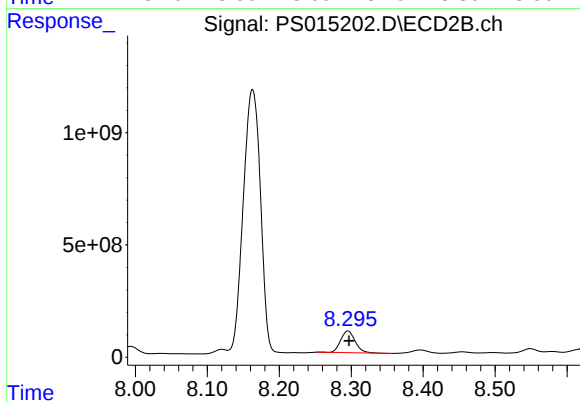

#10 Pentachlorophenol

R.T.: 8.295 min
Delta R.T.: -0.001 min
Response: 1358759378
Conc: 184.58 ng/ml