

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060525\
 Data File : PS030530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2025 13:03
 Operator : AR\AJ
 Sample : Q2176-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-26

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 01:20:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060425.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 04 13:21:22 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.364	7.767	268.0E6	77274836	70.995	71.843
Target Compounds							
1) T	Dalapon	0.000	2.681f	0	77380359	N.D.	28.241
2) T	3,5-DICHL...	6.512	0.000	612077	0	<MDL	N.D. #
3) T	4-Nitroph...	7.121f	7.322	796584	3324146	<MDL	2.121 #
5) T	DICAMBA	0.000	7.972	0	9883818	N.D.	1.534
6) T	MCPD	7.795f	0.000	29231905	0	2.951	N.D. #
7) T	MCPA	7.905	0.000	4940450	0	<MDL	N.D. #
8) T	DICHLORPROP	8.250f	8.744f	4396556	18841319	1.208	12.695 #
9) T	2,4-D	8.495	0.000	52054885	0	14.287	N.D. #
10) T	Pentachlo...	8.812	9.555	4951130	9135624	<MDL	<MDL #
11) T	2,4,5-TP ...	9.395	9.925	8905588	18392158	<MDL	1.341 #
12) T	2,4,5-T	9.692	10.359	4764171	11634215	<MDL	<MDL #
13) T	2,4-DB	10.268	10.913	3633448	12758048	1.197	11.098 #
14) T	DINOSEB	11.496	11.322	2833767	8977939	<MDL	<MDL #
15) T	Picloram	11.299	12.424	8986359	14074865	<MDL	<MDL #
16) T	DCPA	11.776	12.359	5963185	4188658	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060525\
Data File : PS030530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2025 13:03
Operator : AR\AJ
Sample : Q2176-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-26

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 01:20:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060425.M
Quant Title : 8080.M
QLast Update : Wed Jun 04 13:21:22 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

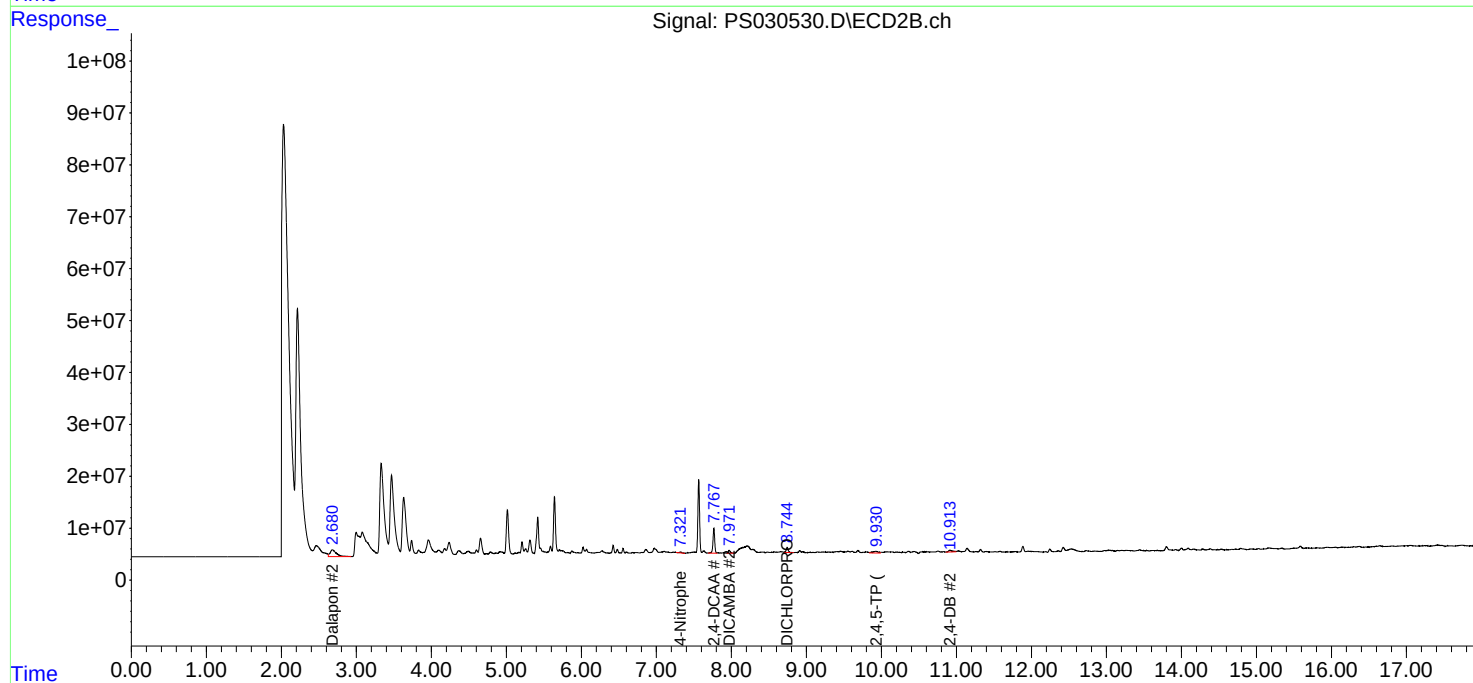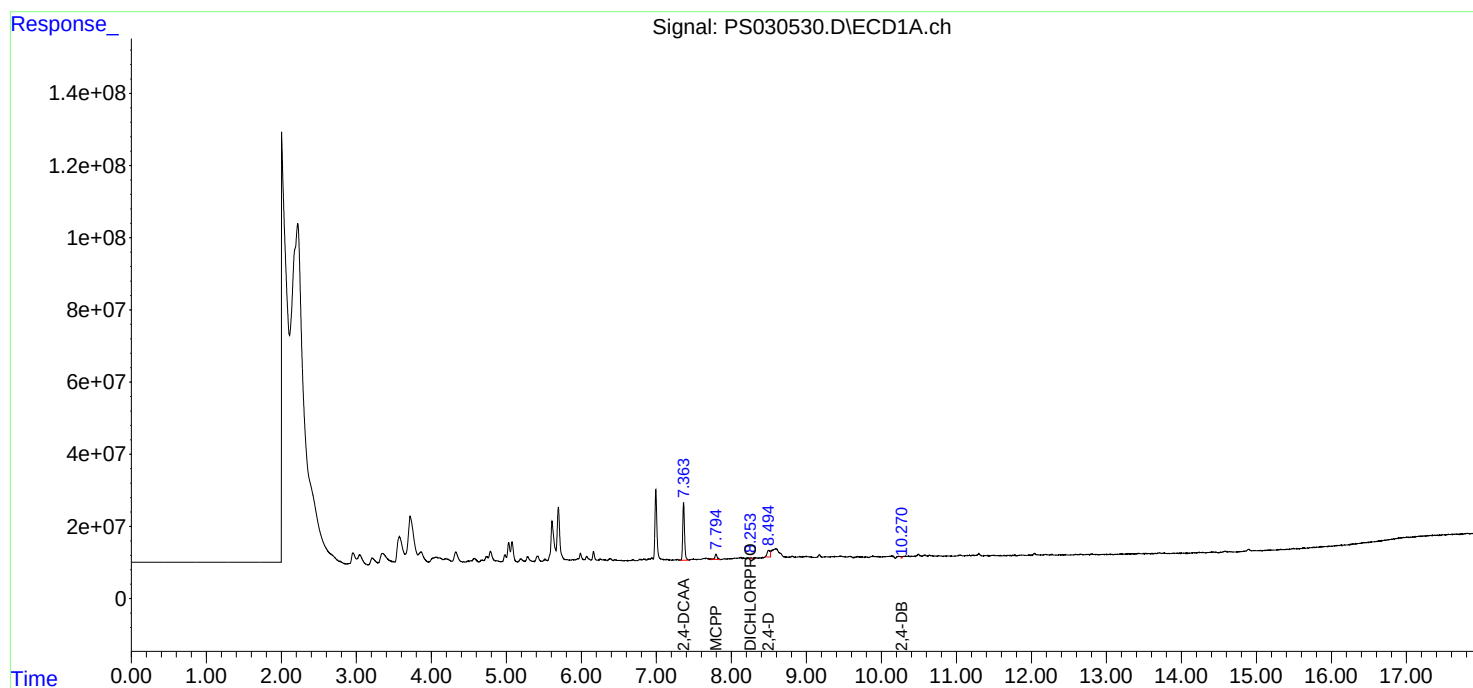


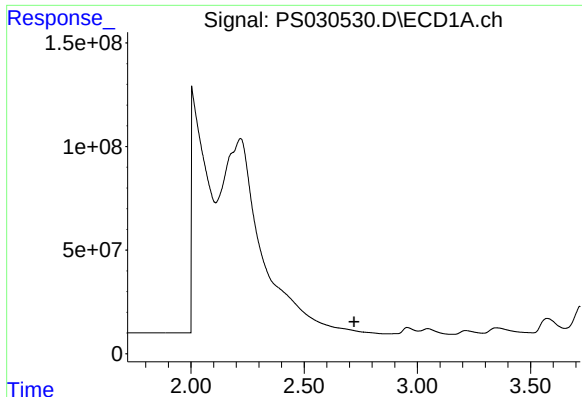

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.720 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-26

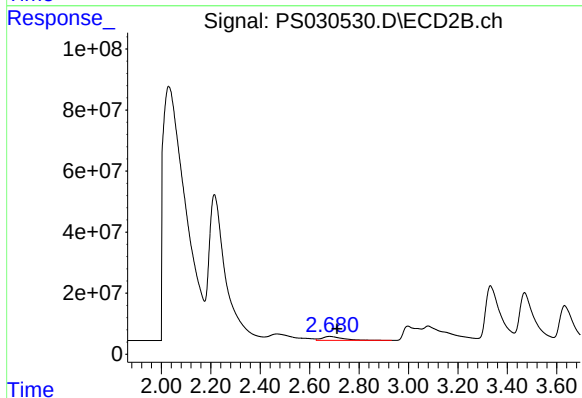


#1 Dalapon

R.T.: 2.681 min
Delta R.T.: -0.030 min
Response: 77380359
Conc: 28.24 ng/ml

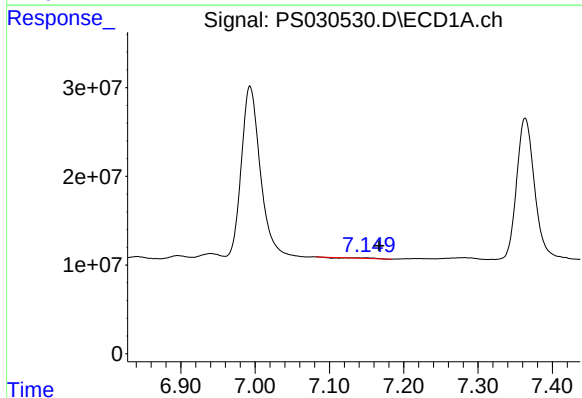


#3 4-Nitrophenol

R.T.: 7.121 min
Delta R.T.: -0.046 min
Response: 796584
Conc: N.D.

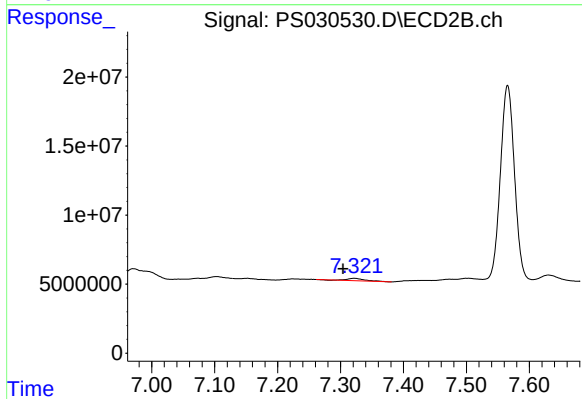

#3 4-Nitrophenol


R.T.: 7.322 min
Delta R.T.: 0.018 min
Response: 3324146
Conc: 2.12 ng/ml

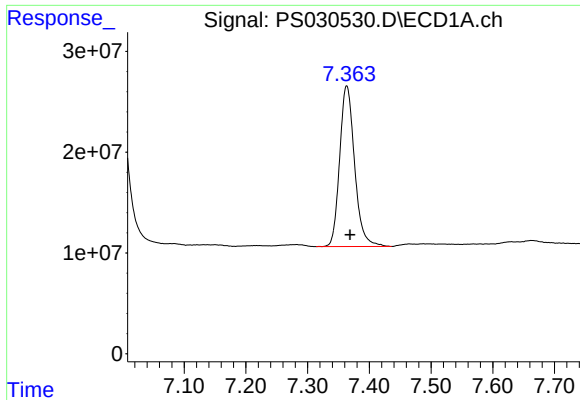

#4 2,4-DCAA


R.T.: 7.364 min
Delta R.T.: -0.006 min
Response: 268017107
Conc: 71.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-26

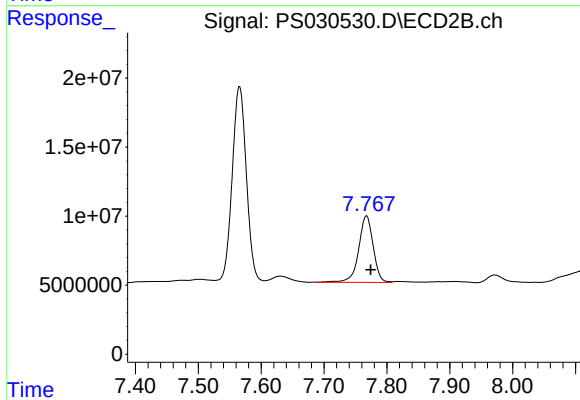


#4 2,4-DCAA

R.T.: 7.767 min
Delta R.T.: -0.007 min
Response: 77274836
Conc: 71.84 ng/ml

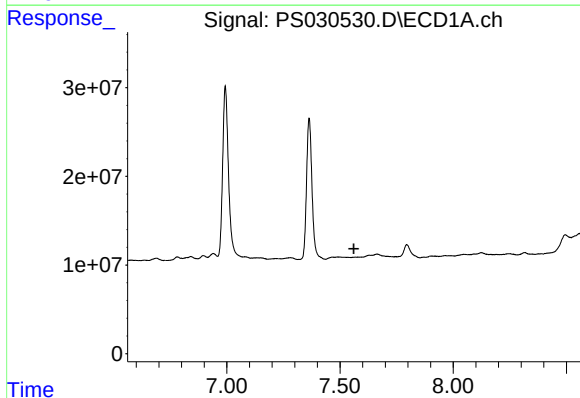


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.561 min
Response: 0
Conc: N.D.

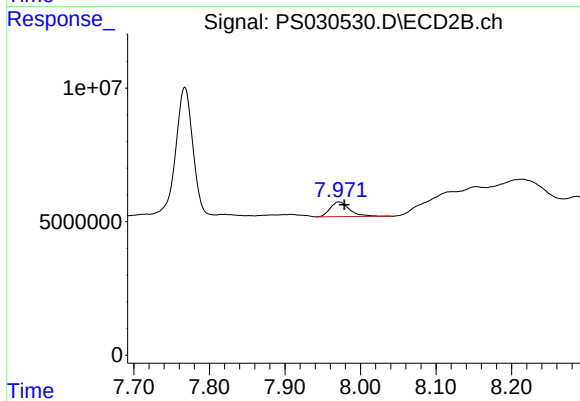

#5 DICAMBA


R.T.: 7.972 min
Delta R.T.: -0.007 min
Response: 9883818
Conc: 1.53 ng/ml

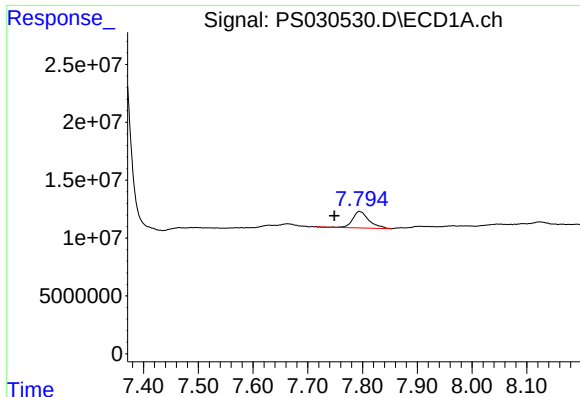

#6 MCPP


R.T.: 7.795 min
Delta R.T.: 0.046 min
Response: 29231905
Conc: 2.95 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-26

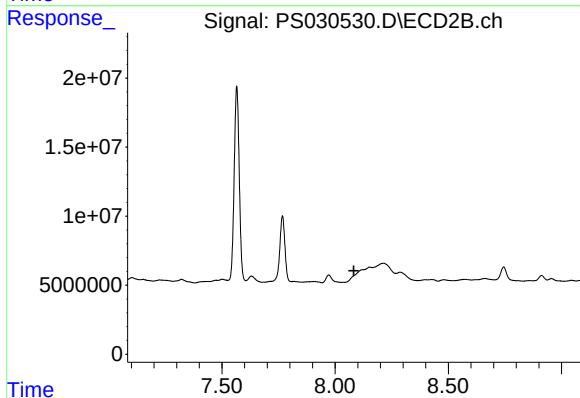


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.083 min
Response: 0
Conc: N.D.

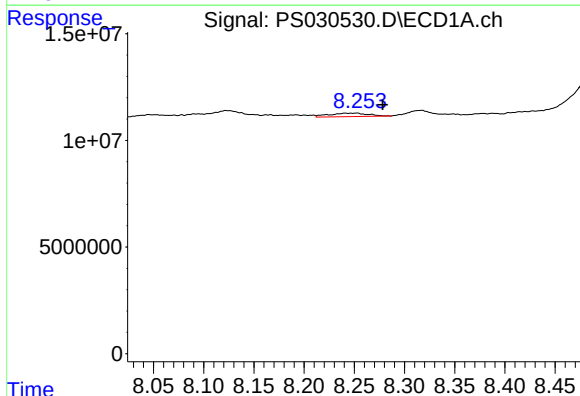


#8 DICHLORPROP

R.T.: 8.250 min
Delta R.T.: -0.028 min
Response: 4396556
Conc: 1.21 ng/ml

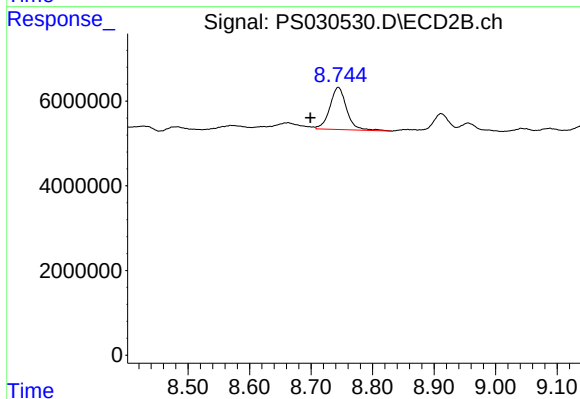

#8 DICHLORPROP


R.T.: 8.744 min
Delta R.T.: 0.045 min
Response: 18841319
Conc: 12.69 ng/ml

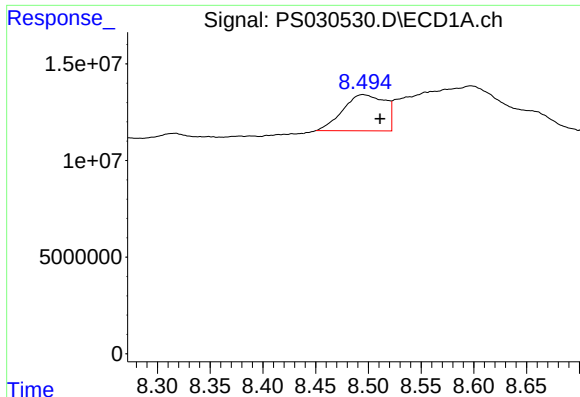

#9 2,4-D


R.T.: 8.495 min
Delta R.T.: -0.016 min
Response: 52054885
Conc: 14.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-26

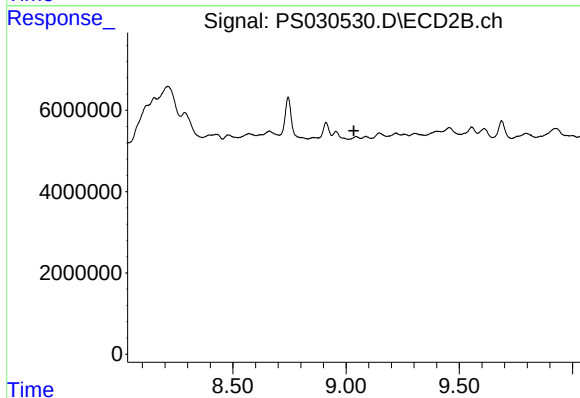


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 9.035 min
Response: 0
Conc: N.D.

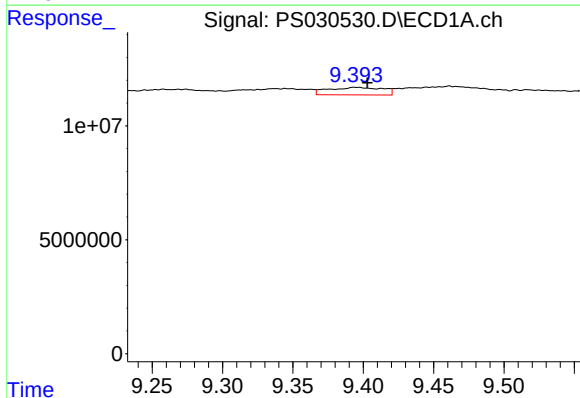


#11 2,4,5-TP (SILVEX)

R.T.: 9.395 min
Delta R.T.: -0.008 min
Response: 8905588
Conc: N.D.

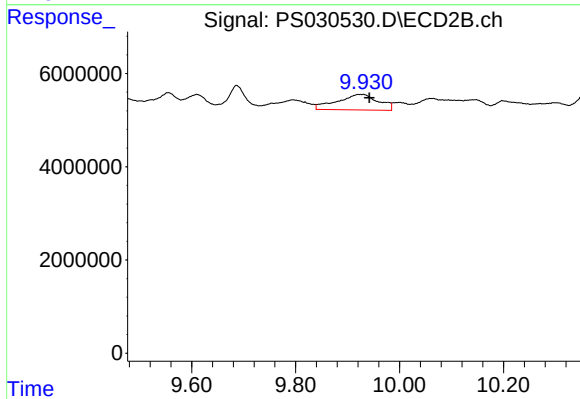

#11 2,4,5-TP (SILVEX)


R.T.: 9.925 min
Delta R.T.: -0.017 min
Response: 18392158
Conc: 1.34 ng/ml

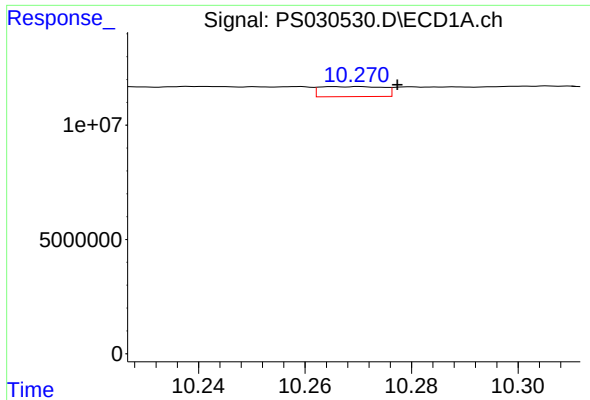

#13 2,4-DB

R.T.: 10.268 min
Delta R.T.: -0.009 min
Response: 3633448
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-26

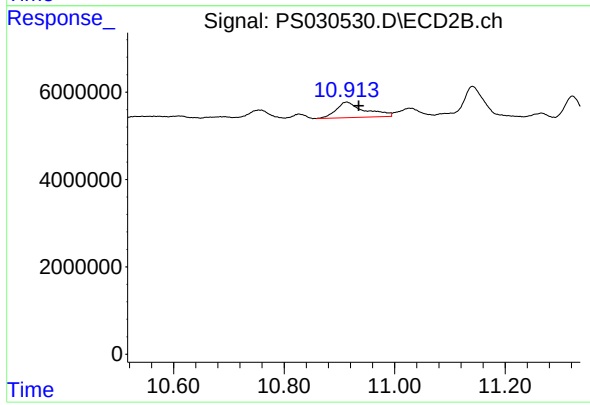

#13 2,4-DB

R.T.: 10.913 min
Delta R.T.: -0.022 min
Response: 12758048
Conc: 11.10 ng/ml