

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060623\
 Data File : PS023214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2023 10:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 17:28:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.483	6.857	909.9E6	291.3E6	514.274	513.188
Target Compounds							
1) T	Dalapon	2.562	0.000	3529459	0	1.930	N.D. #
2) T	3,5-DICHL...	5.799	0.000	136252	0	<MDL	N.D. #
3) T	4-Nitroph...	6.318	0.000	7140673	0	5.540	N.D. #
5) T	DICAMBA	6.631	7.054	99358	2236092	<MDL	<MDL #
6) T	MCPD	6.821	7.054f	819271	2236092	<MDL	1.251 #
7) T	MCPA	6.859f	7.340	3377818	29909289	<MDL	11.129 #
8) T	DICHLORPROP	7.260	0.000	5876856	0	2.848	N.D. #
9) T	2,4-D	7.400f	0.000	1514575	0	<MDL	N.D. #
10) T	Pentachlo...	7.675	8.358	-287600	5039685	N.D.	<MDL
11) T	2,4,5-TP ...	8.212	0.000	7617168	0	<MDL	N.D. #
12) T	2,4,5-T	8.482	9.143f	3636225	1240626	<MDL	<MDL #
13) T	2,4-DB	9.027	0.000	5300458	0	2.252	N.D. #
14) T	DINOSEB	10.066	0.000	802685	0	<MDL	N.D. #
15) T	Picloram	9.892	10.900	32294418	5438778	1.861	1.192 #
16) T	DCPA	10.333	10.900	4427793	5438778	<MDL	1.356 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060623\
Data File : PS023214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2023 10:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 17:28:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

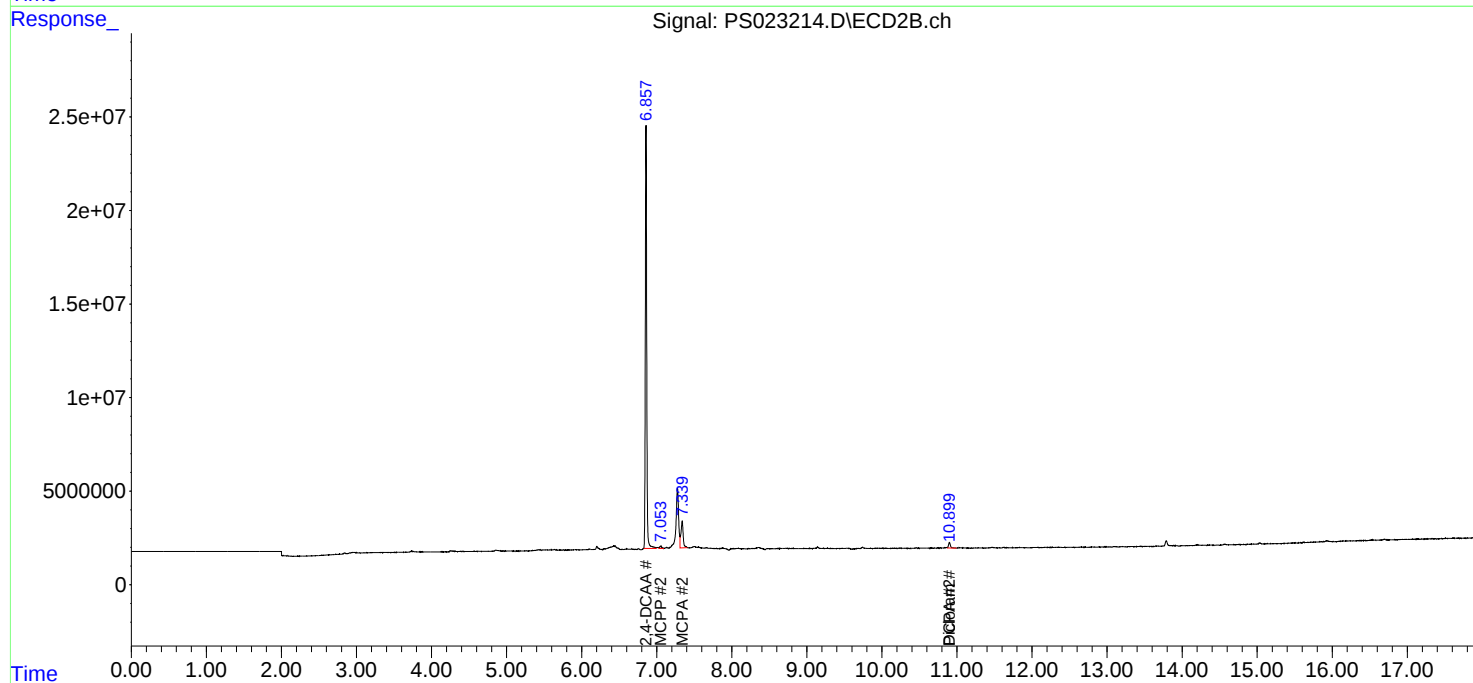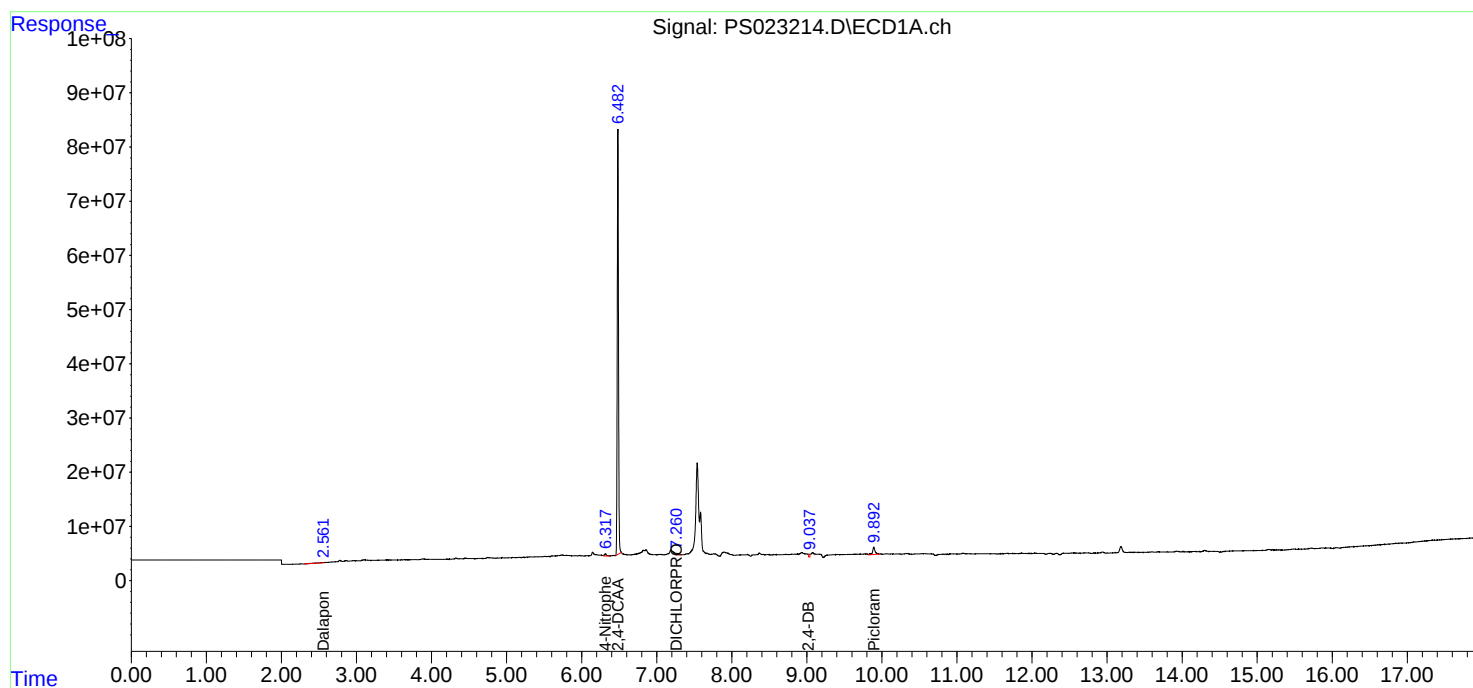


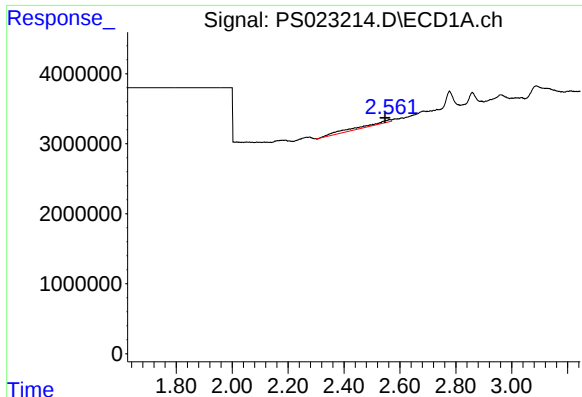

#1 Dalapon


R.T.: 2.562 min
Delta R.T.: 0.015 min
Response: 3529459
Conc: 1.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

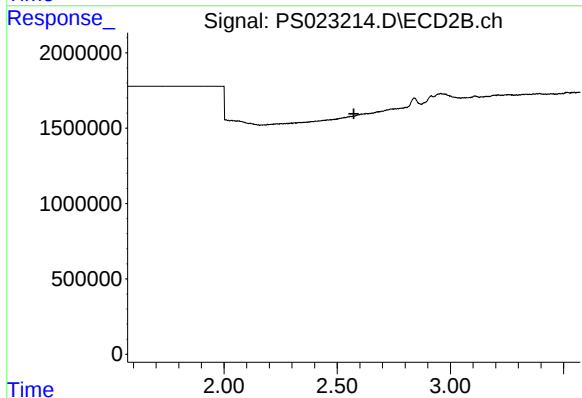


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

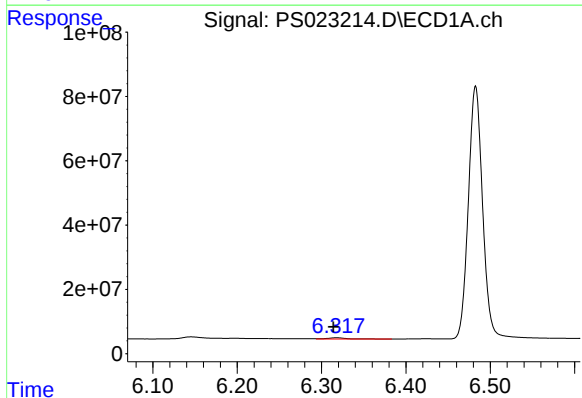


#3 4-Nitrophenol

R.T.: 6.318 min
Delta R.T.: 0.004 min
Response: 7140673
Conc: 5.54 ng/ml

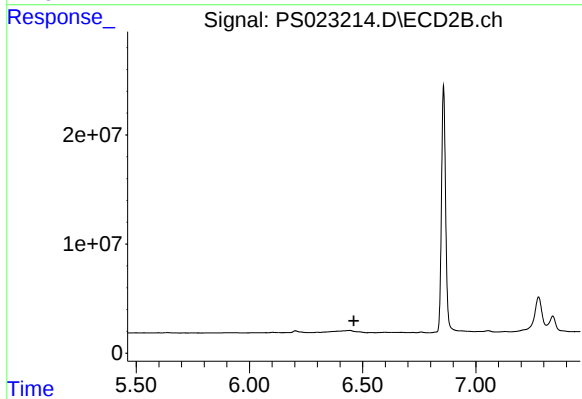

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

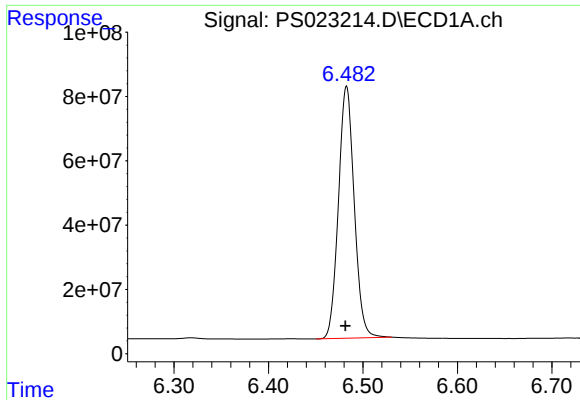

#4 2,4-DCAA


R.T.: 6.483 min
Delta R.T.: 0.001 min
Response: 909882035
Conc: 514.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

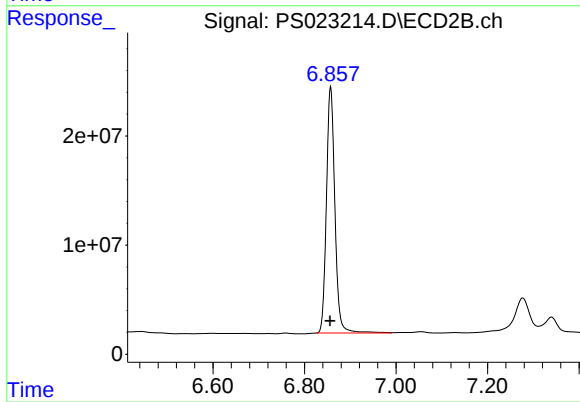


#4 2,4-DCAA

R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 291334660
Conc: 513.19 ng/ml

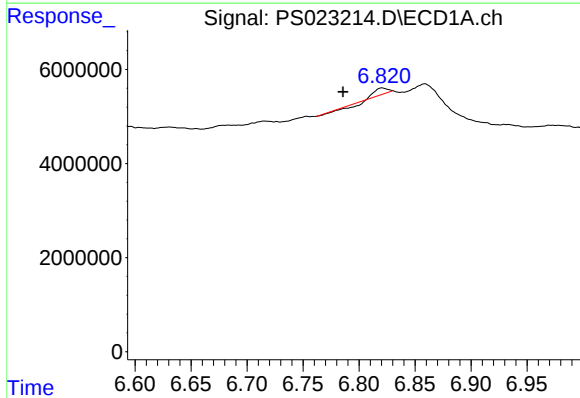


#6 MCP

R.T.: 6.821 min
Delta R.T.: 0.035 min
Response: 819271
Conc: N.D.

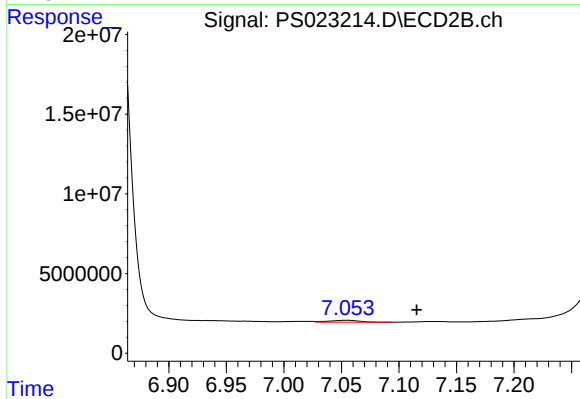

#6 MCP


R.T.: 7.054 min
Delta R.T.: -0.061 min
Response: 2236092
Conc: 1.25 ug/ml

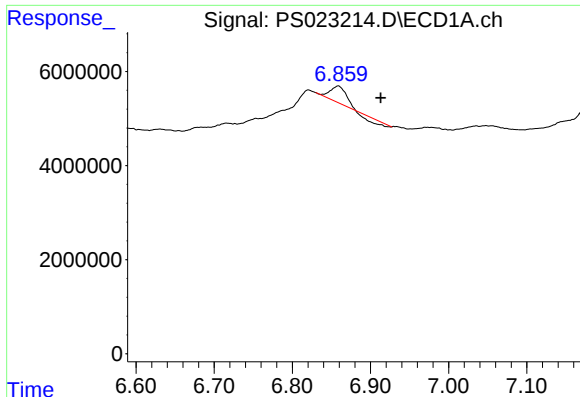

#7 MCPA


R.T.: 6.859 min
Delta R.T.: -0.054 min
Response: 3377818
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

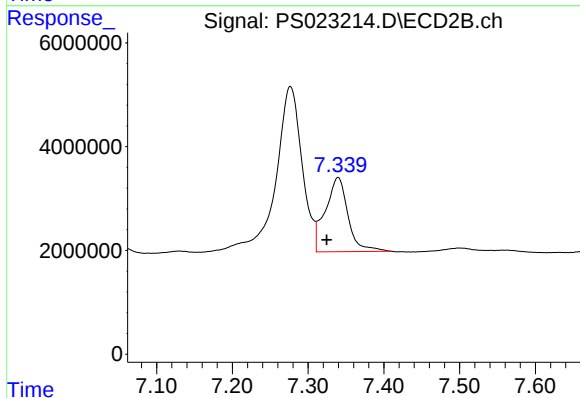


#7 MCPA

R.T.: 7.340 min
Delta R.T.: 0.015 min
Response: 29909289
Conc: 11.13 ug/ml

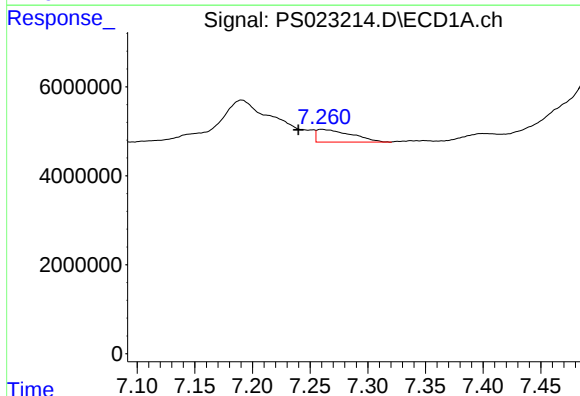


#8 DICHLORPROP

R.T.: 7.260 min
Delta R.T.: 0.020 min
Response: 5876856
Conc: 2.85 ng/ml

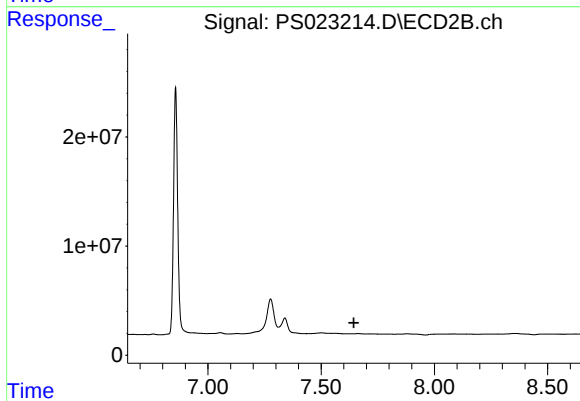

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

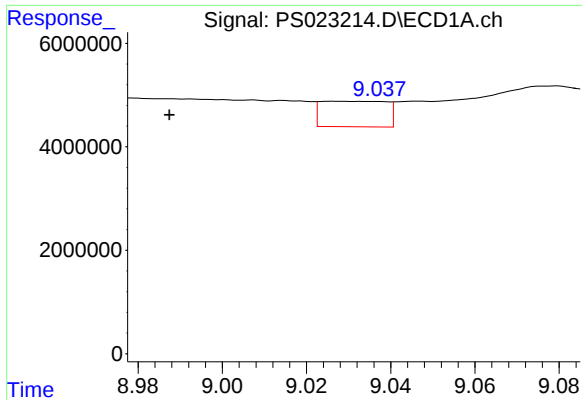

#13 2,4-DB


R.T.: 9.027 min
Delta R.T.: 0.040 min
Response: 5300458
Conc: 2.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

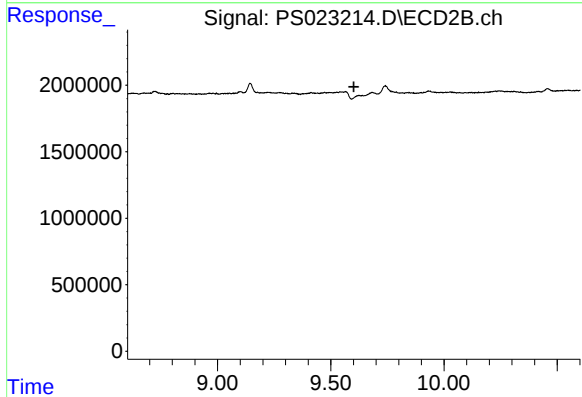


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.

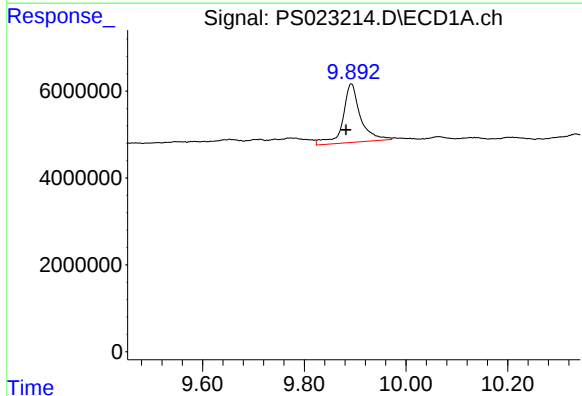


#15 Picloram

R.T.: 9.892 min
Delta R.T.: 0.010 min
Response: 32294418
Conc: 1.86 ng/ml

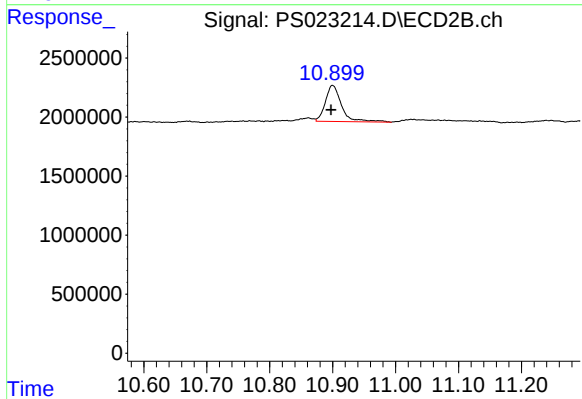

#15 Picloram


R.T.: 10.900 min
Delta R.T.: 0.002 min
Response: 5438778
Conc: 1.19 ng/ml

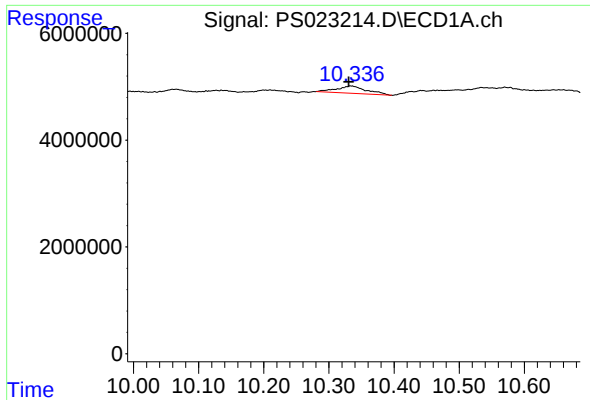

#16 DCPA

R.T.: 10.333 min
Delta R.T.: 0.002 min
Response: 4427793
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

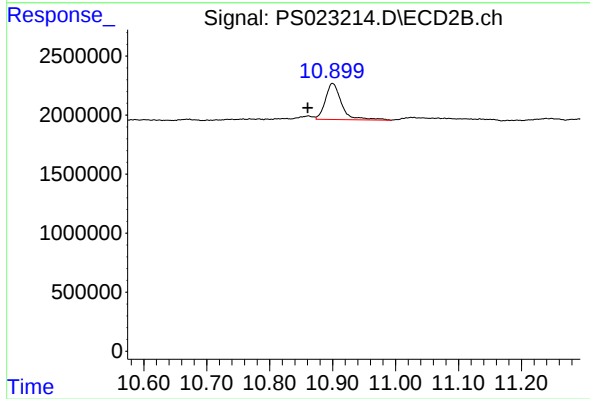

#16 DCPA

R.T.: 10.900 min
Delta R.T.: 0.039 min
Response: 5438778
Conc: 1.36 ng/ml