

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060721\
 Data File : PS015262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2021 00:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:56:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.784	1118.7E6	288.8E6	443.847	539.054
Target Compounds							
3) T	4-Nitroph...	7.026	0.000	3539602	0	2.511	N.D. #
7) T	MCPA	7.672f	0.000	19058048	0	1.899	N.D. #
15) T	Picloram	11.017	10.846	20463189	5227438	1.235	1.259
16) T	DCPA	0.000	10.846	0	5227438	N.D.	1.213



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060721\
Data File : PS015262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2021 00:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:56:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

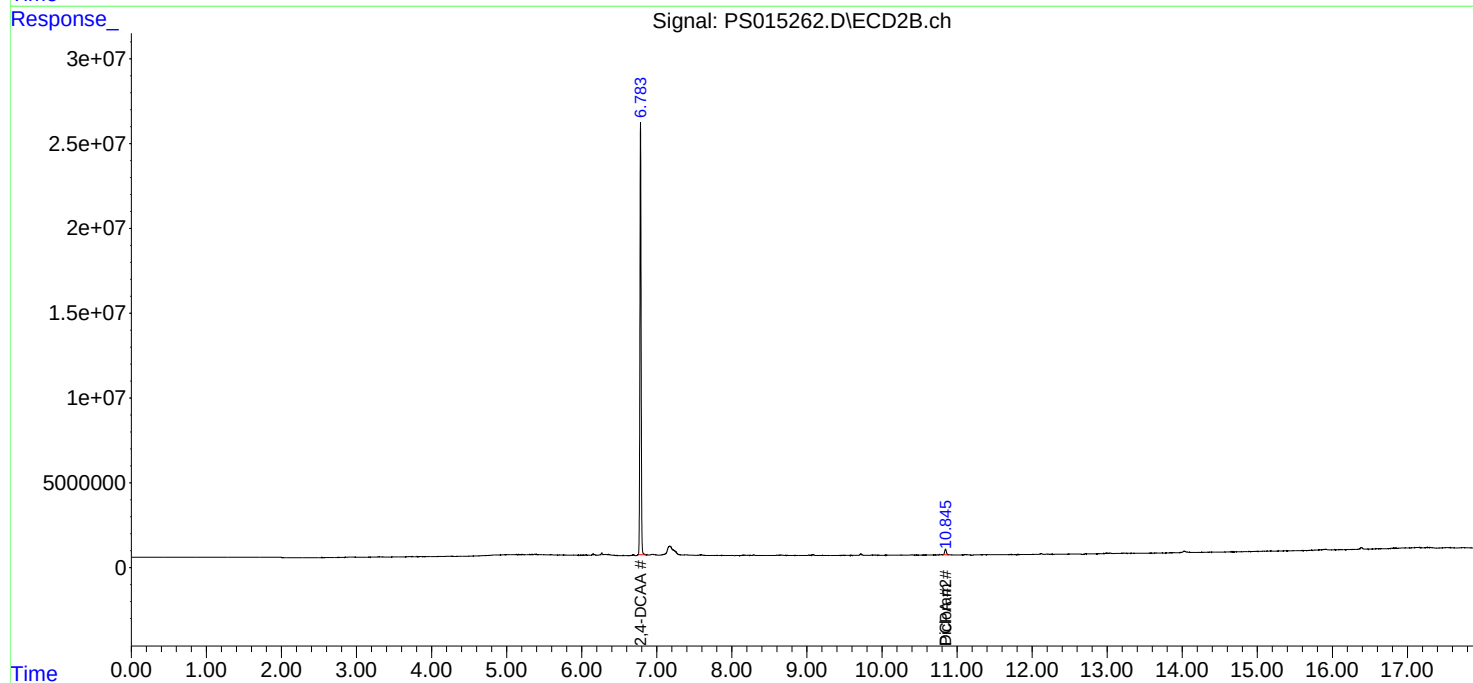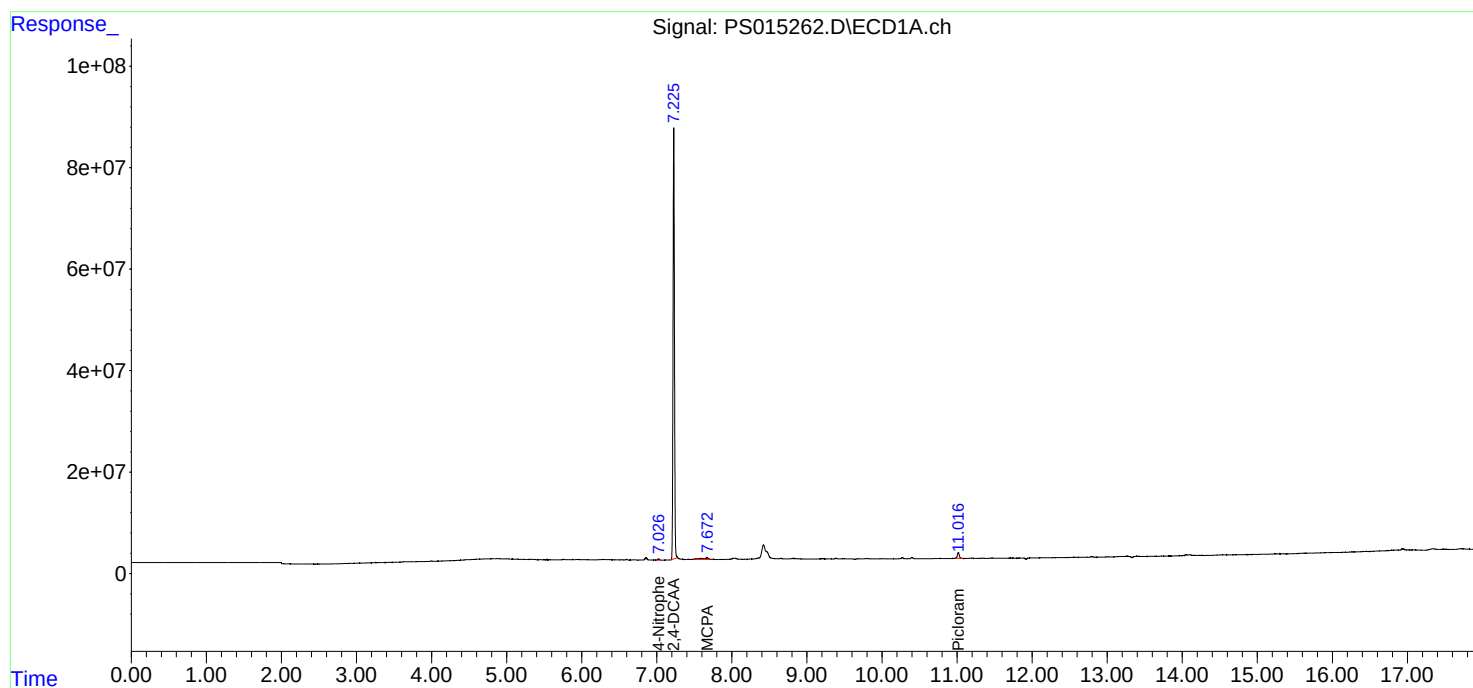


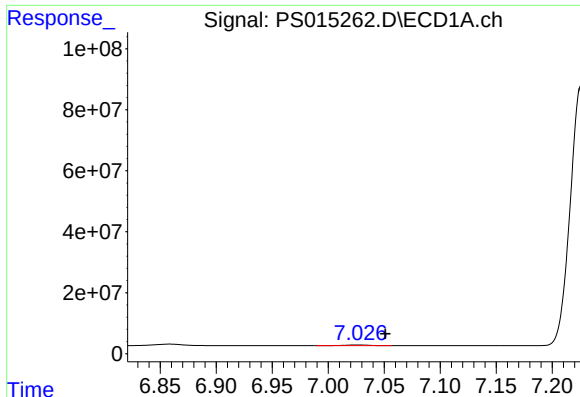

#3 4-Nitrophenol


R.T.: 7.026 min
Delta R.T.: -0.025 min
Response: 3539602
Conc: 2.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

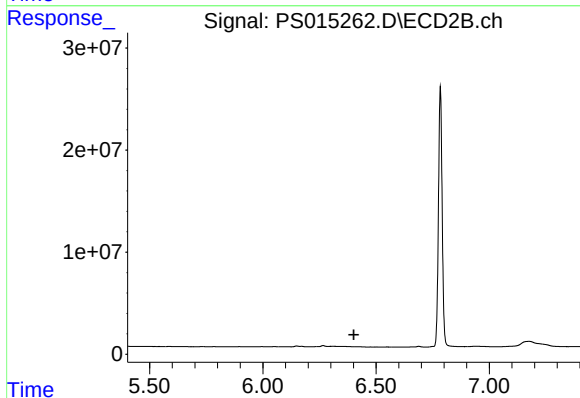


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

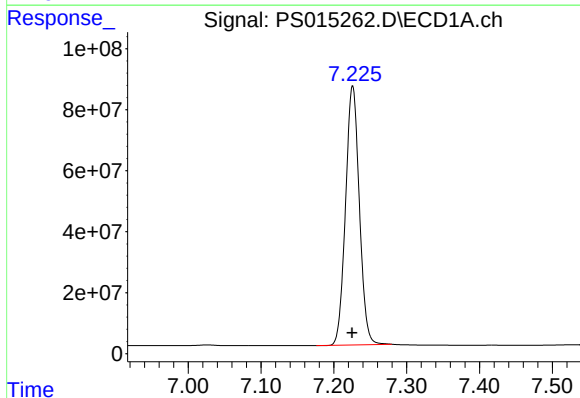


#4 2,4-DCAA

R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 1118661703
Conc: 443.85 ng/ml

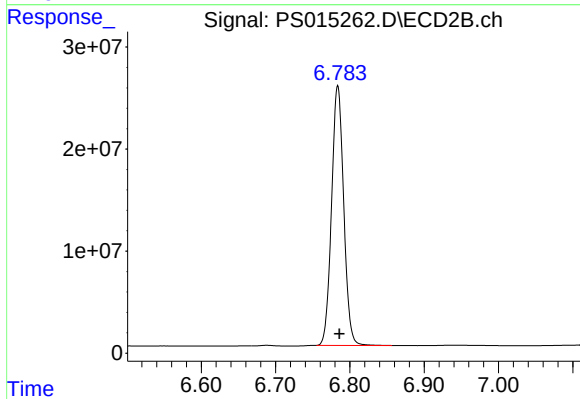

#4 2,4-DCAA


R.T.: 6.784 min
Delta R.T.: -0.002 min
Response: 288809449
Conc: 539.05 ng/ml

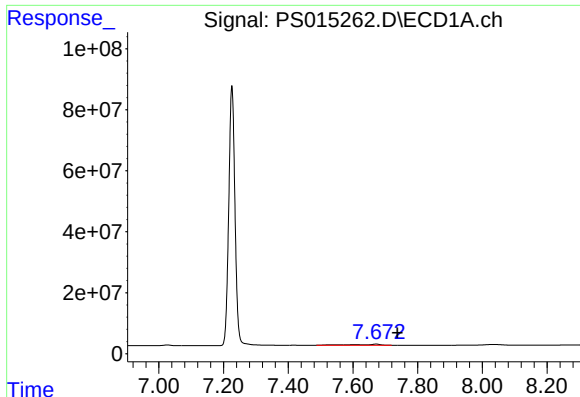

#7 MCPA


R.T.: 7.672 min
Delta R.T.: -0.066 min
Response: 19058048
Conc: 1.90 ug/ml

Instrument :
ECD_S
ClientSampleId :

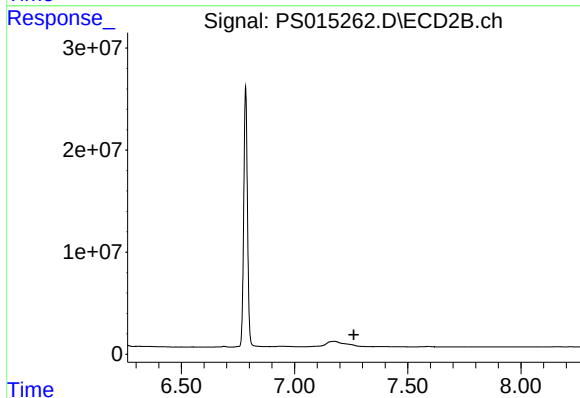


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

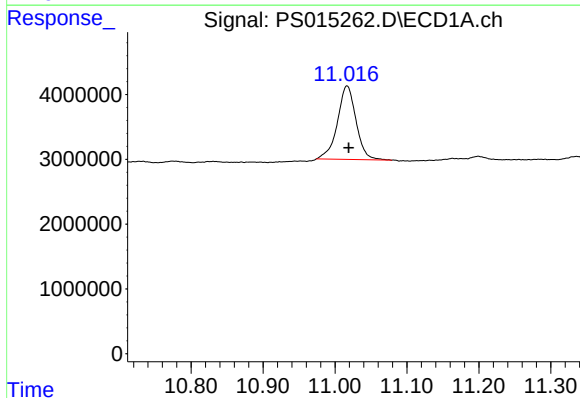


#15 Picloram

R.T.: 11.017 min
Delta R.T.: -0.002 min
Response: 20463189
Conc: 1.24 ng/ml

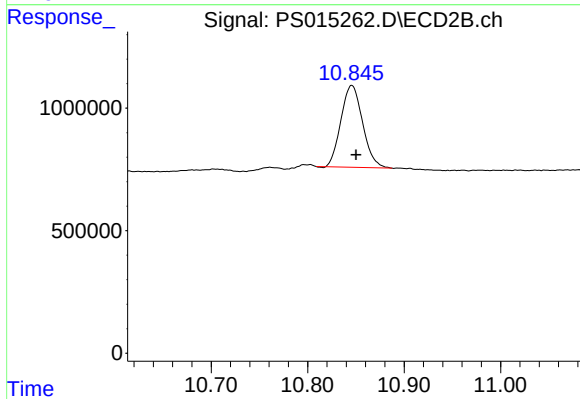

#15 Picloram


R.T.: 10.846 min
Delta R.T.: -0.004 min
Response: 5227438
Conc: 1.26 ng/ml

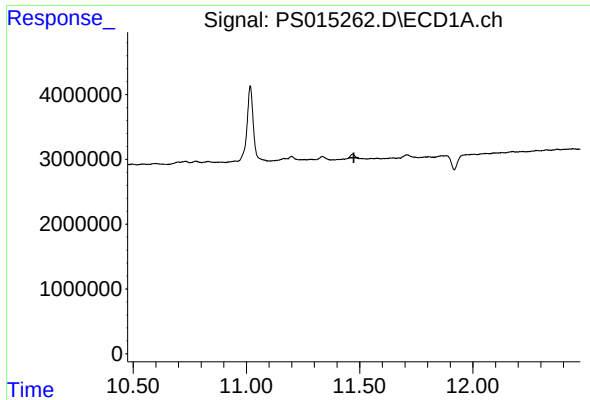

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

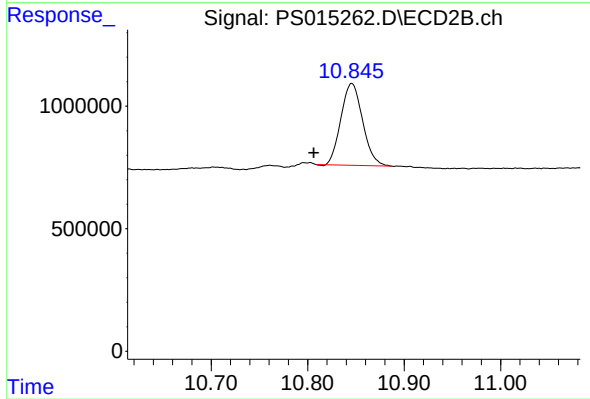

#16 DCPA

R.T.: 10.846 min
Delta R.T.: 0.039 min
Response: 5227438
Conc: 1.21 ng/ml