

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060721\
 Data File : PS015274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2021 05:14
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 06:54:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.784	1125.4E6	286.1E6	446.522	534.002
Target Compounds							
3) T	4-Nitroph...	7.025	0.000	3956527	0	2.807	N.D. #
7) T	MCPA	7.671f	0.000	5485086	0	<MDL	N.D. #
15) T	Picloram	11.016	10.845	23389315	6151944	1.412	1.481
16) T	DCPA	0.000	10.845	0	6151944	N.D.	1.427



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060721\
Data File : PS015274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2021 05:14
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 06:54:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

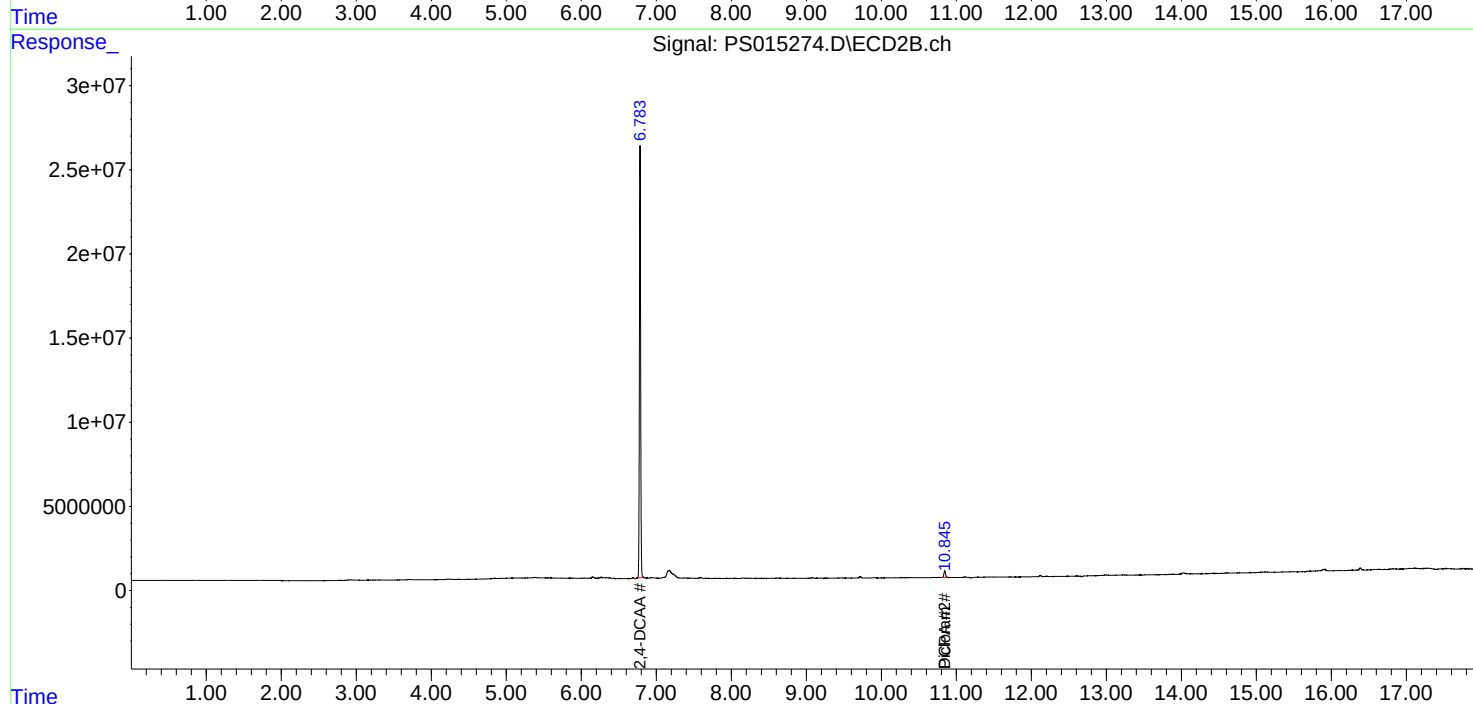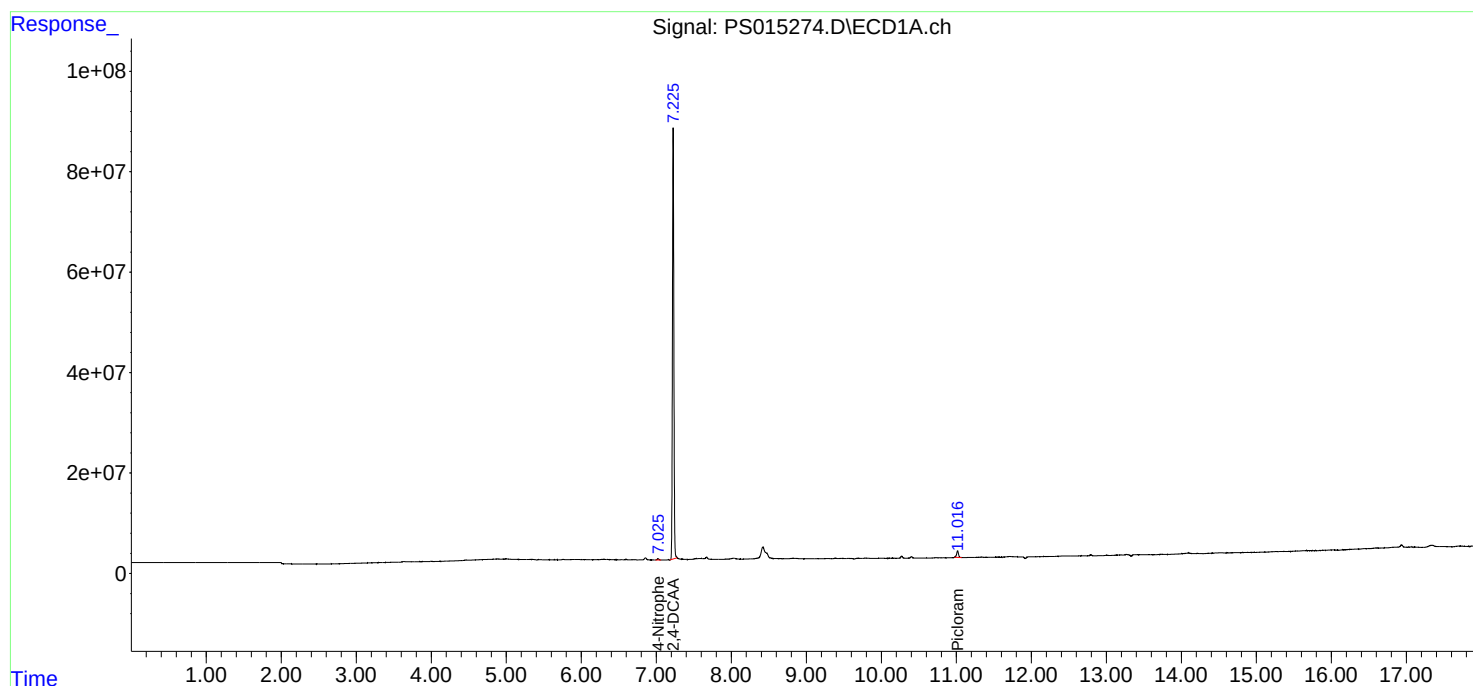


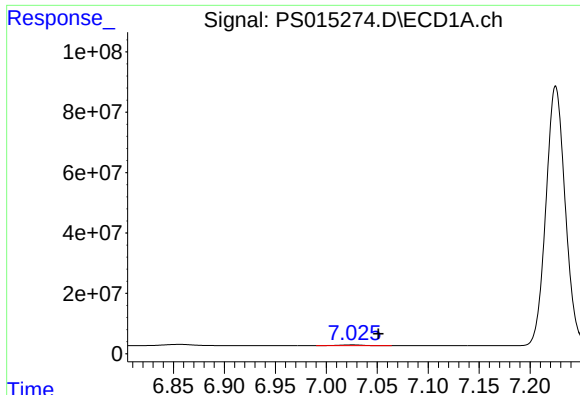

#3 4-Nitrophenol


R.T.: 7.025 min
Delta R.T.: -0.026 min
Response: 3956527
Conc: 2.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

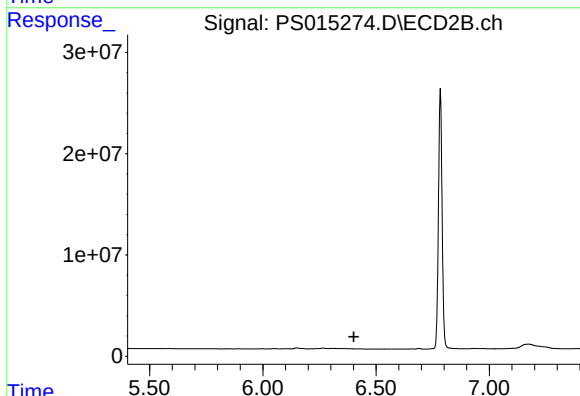


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

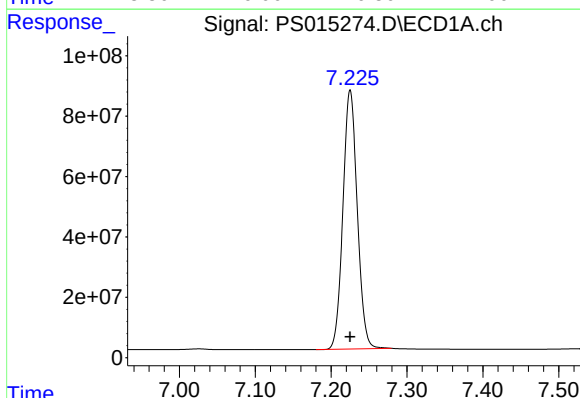


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 1125403718
Conc: 446.52 ng/ml

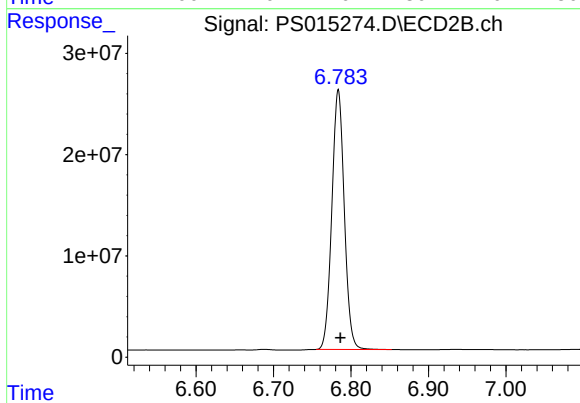

#4 2,4-DCAA


R.T.: 6.784 min
Delta R.T.: -0.003 min
Response: 286102618
Conc: 534.00 ng/ml

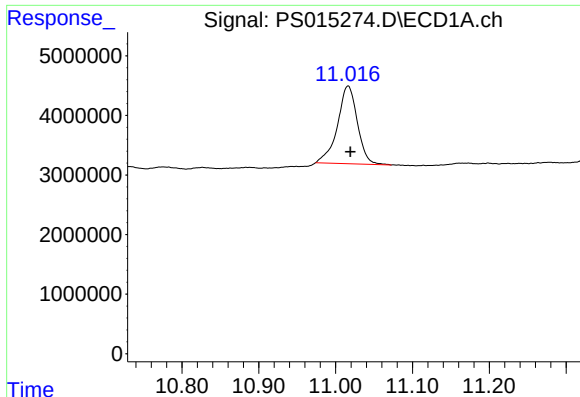

#15 Picloram


R.T.: 11.016 min
Delta R.T.: -0.003 min
Response: 23389315
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

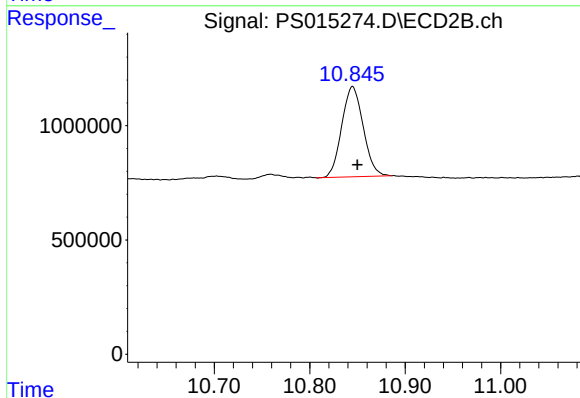


#15 Picloram

R.T.: 10.845 min
Delta R.T.: -0.005 min
Response: 6151944
Conc: 1.48 ng/ml

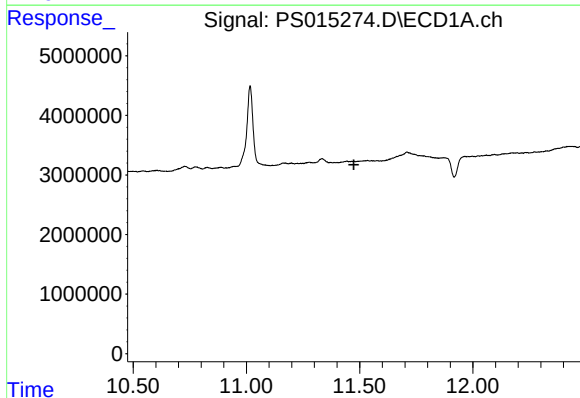

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.475 min
Response: 0
Conc: N.D.

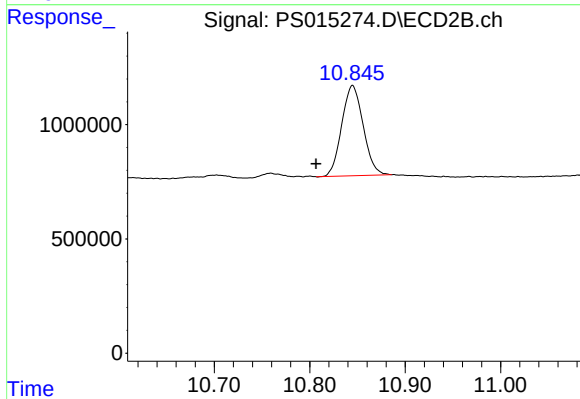

#16 DCPA

R.T.: 10.845 min
Delta R.T.: 0.038 min
Response: 6151944
Conc: 1.43 ng/ml