

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060721\
 Data File : PS015258.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 22:47
 Operator : DD\AJ
 Sample : M2589-21MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 18-B7(0-2)MS

Manual Integrations
 APPROVED

Ankita
 6/9/2021 1:49:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:55:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.784	1325.7E6	267.6E6	525.981	499.507
Target Compounds							
1) T	Dalapon	3.038	2.521	979.2E6	312.5E6	372.550	477.512m#
2) T	3,5-DICHL...	6.437	5.970	1766.1E6	415.9E6	512.152	514.867
5) T	DICAMBA	7.418	6.949	4655.1E6	1155.1E6	488.378	521.968
6) T	MCP	7.588	7.045	378.4E6	102.9E6	52.579	58.256
7) T	MCPA	7.736	7.258	510.5E6	155.5E6	50.864	59.819
8) T	DICHLORPROP	8.113	7.570	1208.4E6	308.7E6	524.679	568.173
9) T	2,4-D	8.341	7.861	1568.7E6	394.1E6	615.636	611.922m
10) T	Pentachlo...	8.654	8.293	15373.2E6	3731.1E6	474.910	506.856
11) T	2,4,5-TP ...	9.204	8.653	7354.9E6	2034.9E6	592.607	701.214m
12) T	2,4,5-T	9.487	9.031	6475.6E6	1713.5E6	539.143	591.870
13) T	2,4-DB	10.041	9.537	905.7E6	221.9E6	355.653	575.301 #
14) T	DINOSEB	11.202	9.867	3641.9E6	902.3E6	455.832	494.094m
15) T	Picloram	11.014	10.844	7184.6E6	1877.8E6	433.675m	452.166
16) T	DCPA	11.469	10.800	6986.2E6	1902.3E6	414.315	441.256

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060721\
Data File : PS015258.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 22:47
Operator : DD\AJ
Sample : M2589-21MS
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampled :
18-B7(0-2)MS


Manual Integrations
APPROVED

Ankita
6/9/2021 1:49:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:55:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

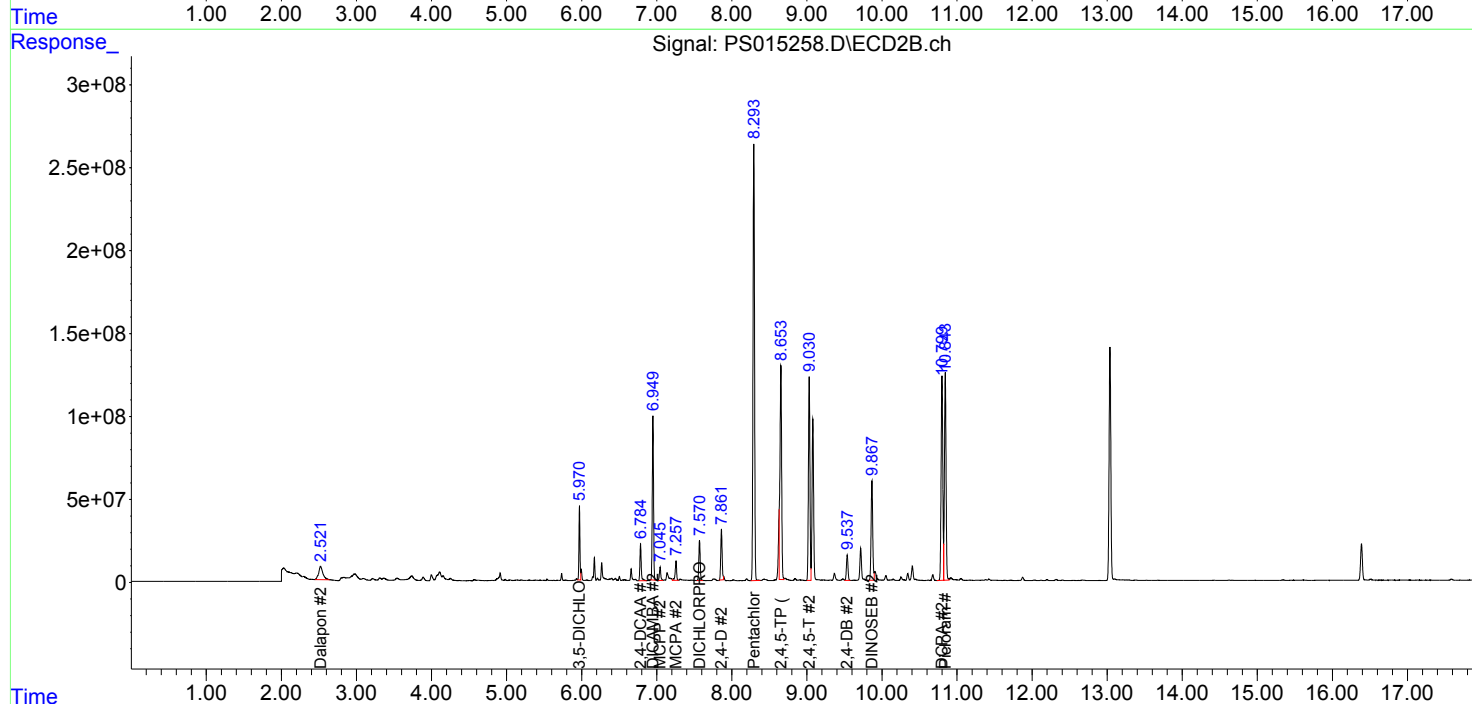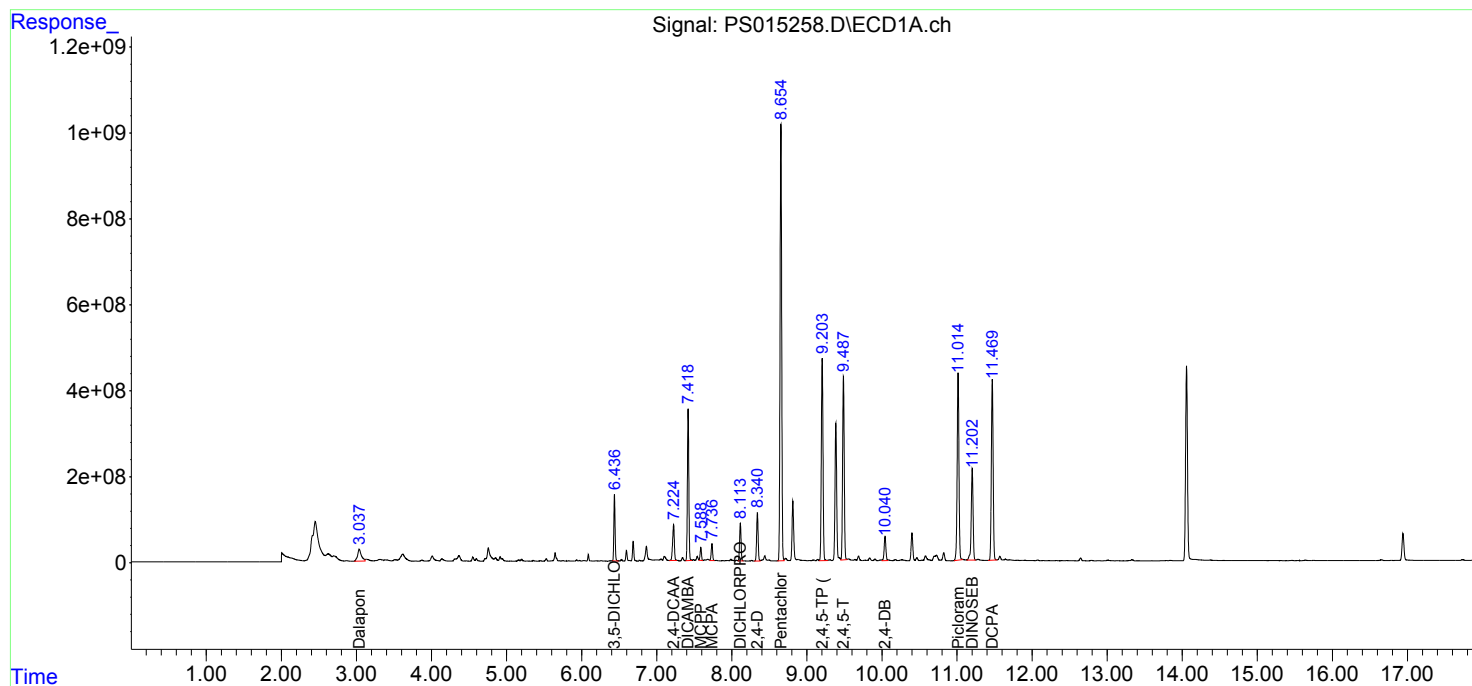

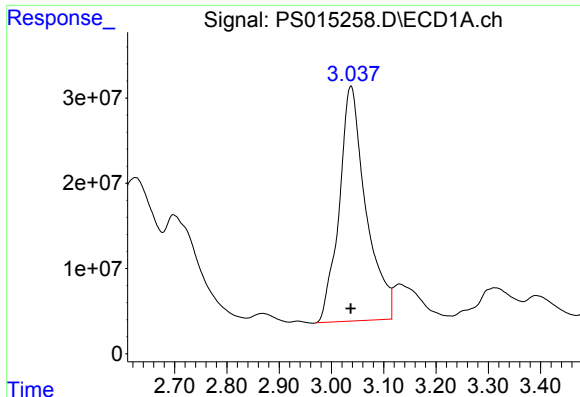


#1 Dalapon

R.T.: 3.038 min
Delta R.T.: 0.000 min
Response: 979200976
Conc: 372.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
18-B7(0-2)MS


Manual Integrations
APPROVED

Ankita
6/9/2021 1:49:55 PM

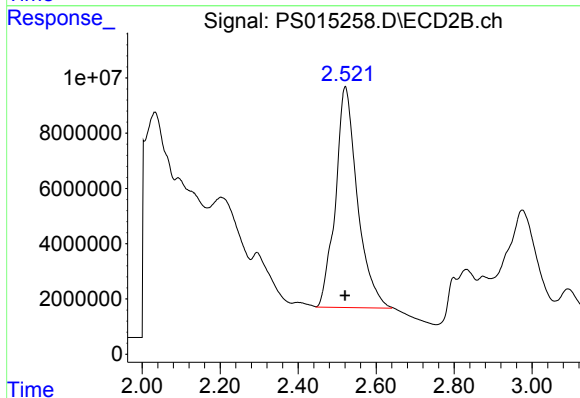


#1 Dalapon

R.T.: 2.521 min
Delta R.T.: 0.000 min
Response: 312508861
Conc: 477.51 ng/ml m

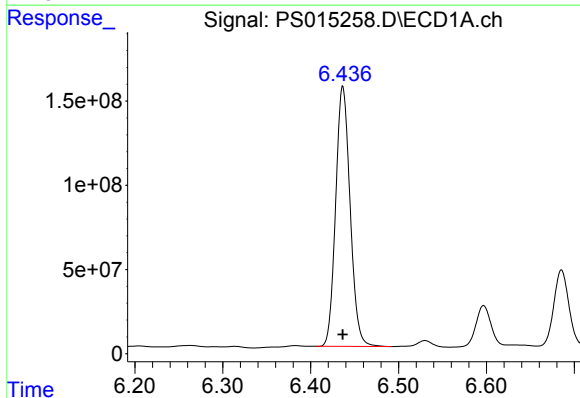


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.437 min
Delta R.T.: 0.000 min
Response: 1766112043
Conc: 512.15 ng/ml

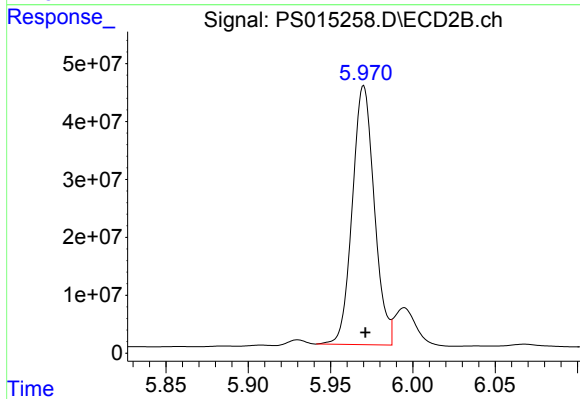

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 415932280
Conc: 514.87 ng/ml

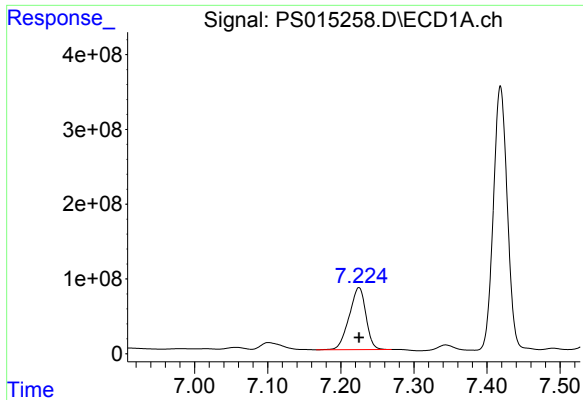


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 1325669013
Conc: 525.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
18-B7(0-2)MS


Manual Integrations
APPROVED

Ankita
6/9/2021 1:49:55 PM

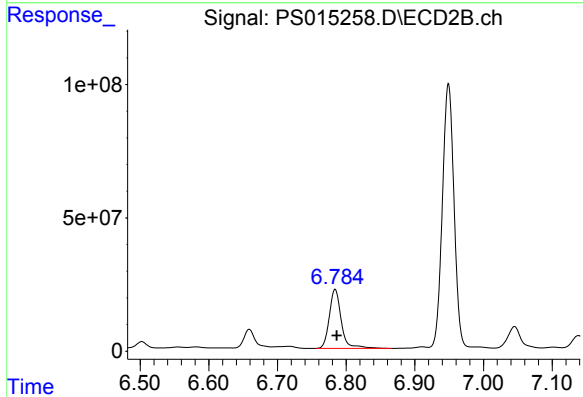


#4 2,4-DCAA

R.T.: 6.784 min
Delta R.T.: -0.002 min
Response: 267621431
Conc: 499.51 ng/ml

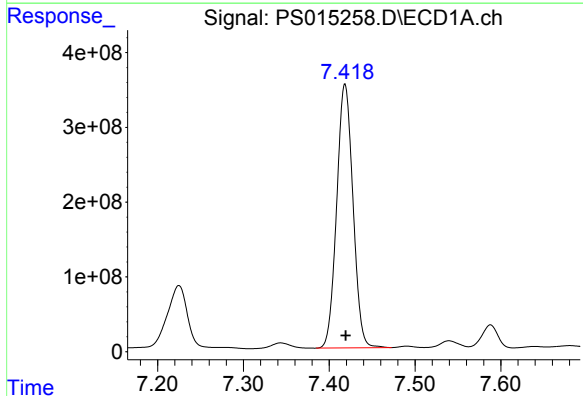


#5 DICAMBA

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 4655097731
Conc: 488.38 ng/ml

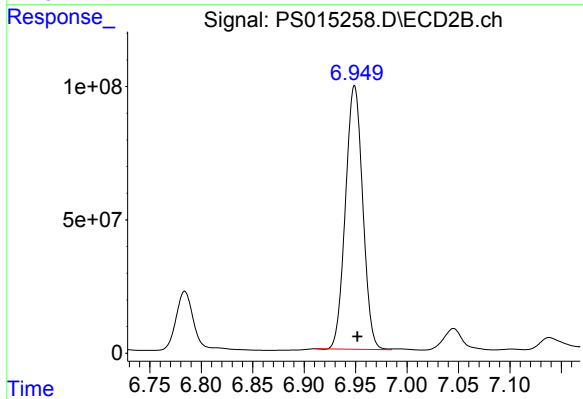

#5 DICAMBA

R.T.: 6.949 min
Delta R.T.: -0.003 min
Response: 1155082524
Conc: 521.97 ng/ml

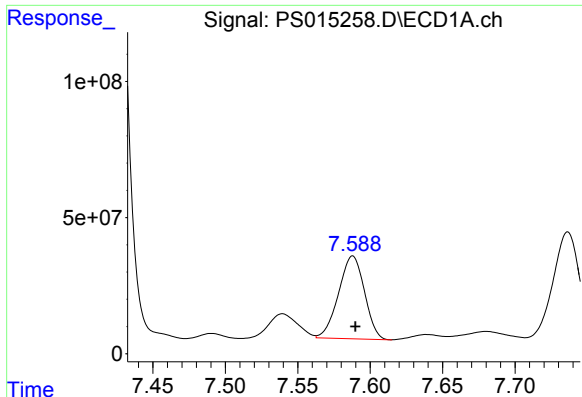


#6 MCP

R.T.: 7.588 min
Delta R.T.: -0.002 min
Response: 378373229
Conc: 52.58 ug/ml

Instrument :
ECD_S
ClientSampleId :
18-B7(0-2)MS


Manual Integrations
APPROVED

Ankita
6/9/2021 1:49:55 PM

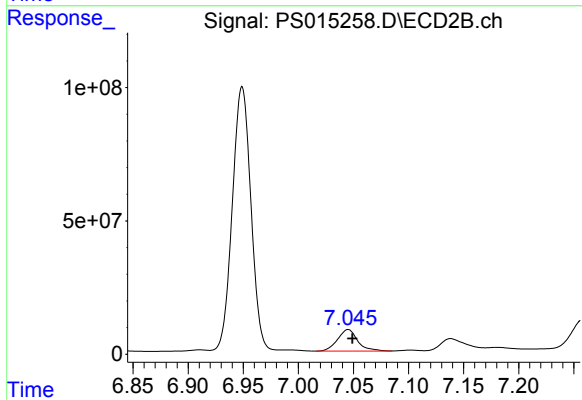


#6 MCP

R.T.: 7.045 min
Delta R.T.: -0.004 min
Response: 102945268
Conc: 58.26 ug/ml

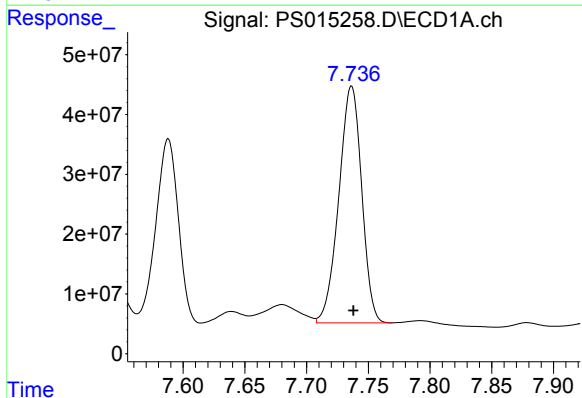


#7 MCP

R.T.: 7.736 min
Delta R.T.: -0.002 min
Response: 510494912
Conc: 50.86 ug/ml

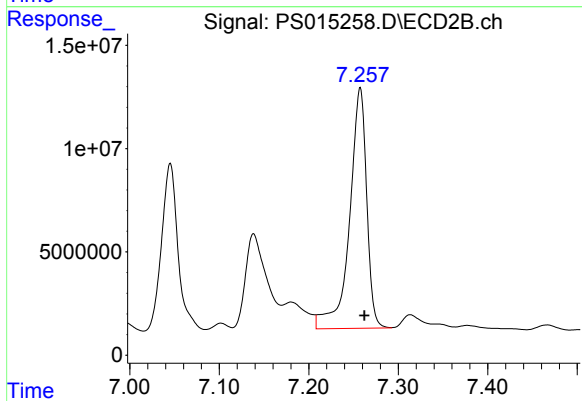

#7 MCP

R.T.: 7.258 min
Delta R.T.: -0.005 min
Response: 155454676
Conc: 59.82 ug/ml

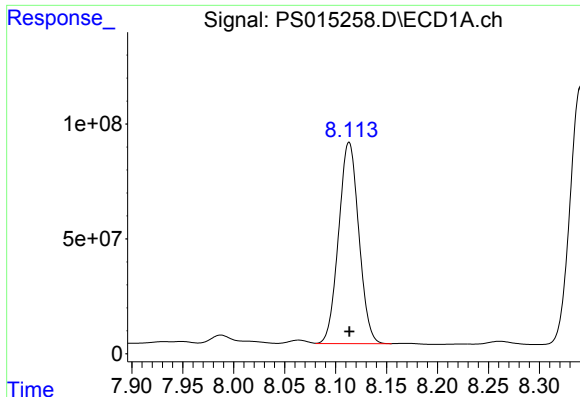


#8 DICHLORPROP

R.T.: 8.113 min
Delta R.T.: 0.000 min
Response: 1208389403
Conc: 524.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
18-B7(0-2)MS


Manual Integrations
APPROVED

Ankita
6/9/2021 1:49:55 PM

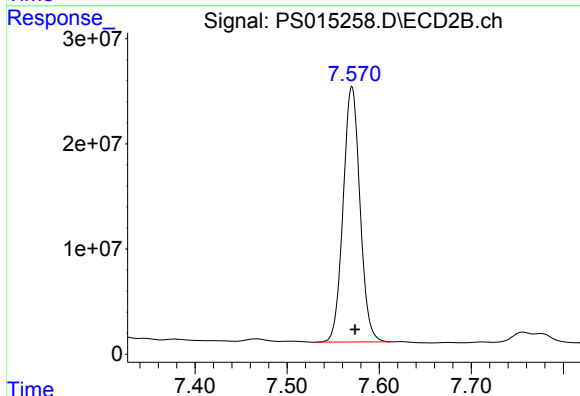


#8 DICHLORPROP

R.T.: 7.570 min
Delta R.T.: -0.003 min
Response: 308667925
Conc: 568.17 ng/ml

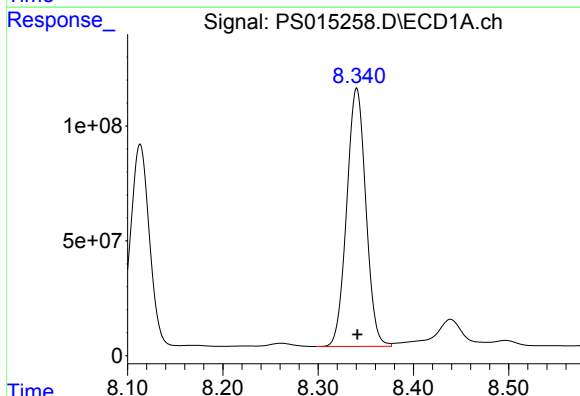


#9 2,4-D

R.T.: 8.341 min
Delta R.T.: 0.000 min
Response: 1568711026
Conc: 615.64 ng/ml

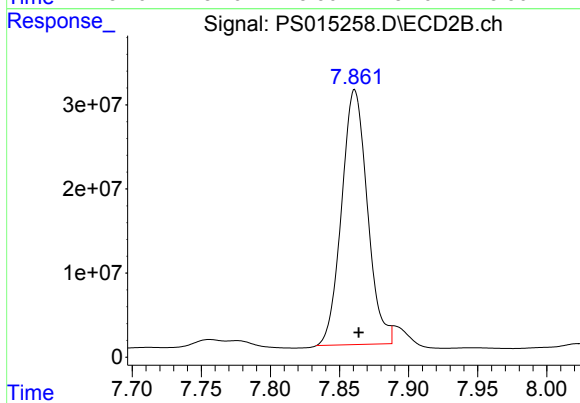

#9 2,4-D

R.T.: 7.861 min
Delta R.T.: -0.003 min
Response: 394092958
Conc: 611.92 ng/ml m

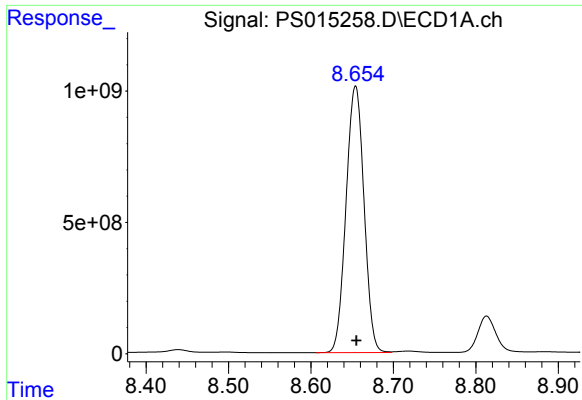


#10 Pentachlorophenol

R.T.: 8.654 min
Delta R.T.: -0.001 min
Response: 15373218201
Conc: 474.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
18-B7(0-2)MS


Manual Integrations
APPROVED

Ankita
6/9/2021 1:49:55 PM

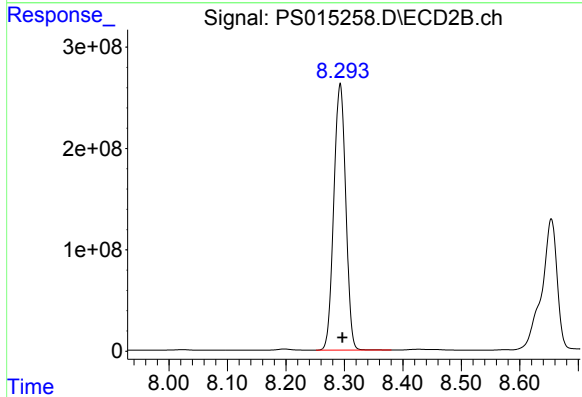


#10 Pentachlorophenol

R.T.: 8.293 min
Delta R.T.: -0.004 min
Response: 3731069120
Conc: 506.86 ng/ml

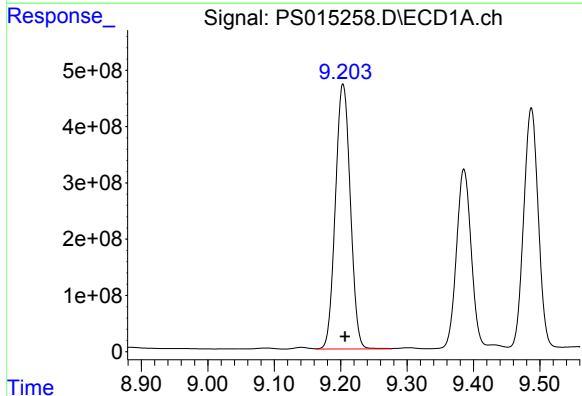


#11 2,4,5-TP (SILVEX)

R.T.: 9.204 min
Delta R.T.: -0.003 min
Response: 7354851124
Conc: 592.61 ng/ml

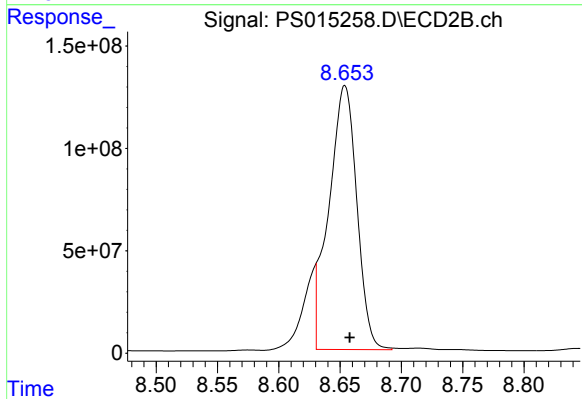

#11 2,4,5-TP (SILVEX)

R.T.: 8.653 min
Delta R.T.: -0.005 min
Response: 2034879245
Conc: 701.21 ng/ml m

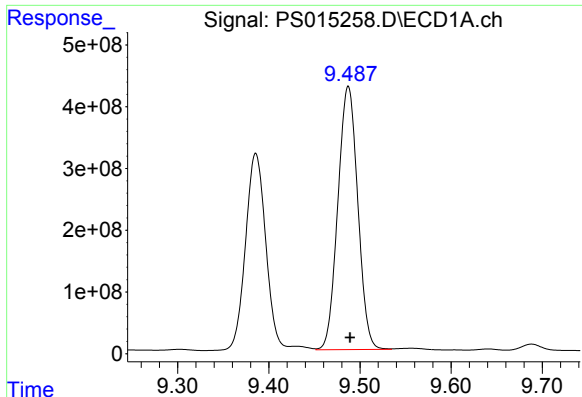


#12 2,4,5-T

R.T.: 9.487 min
Delta R.T.: -0.002 min
Response: 6475596309
Conc: 539.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
18-B7(0-2)MS


Manual Integrations
APPROVED

Ankita
6/9/2021 1:49:55 PM

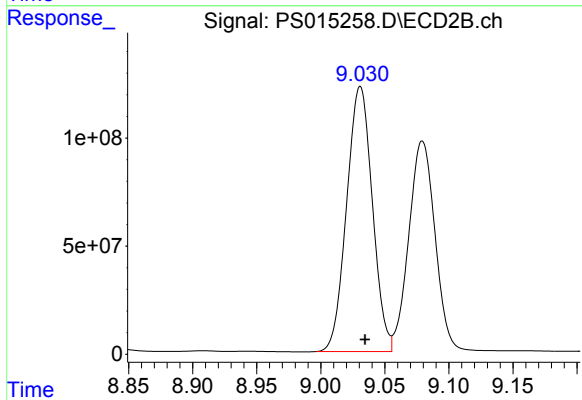


#12 2,4,5-T

R.T.: 9.031 min
Delta R.T.: -0.004 min
Response: 1713465617
Conc: 591.87 ng/ml

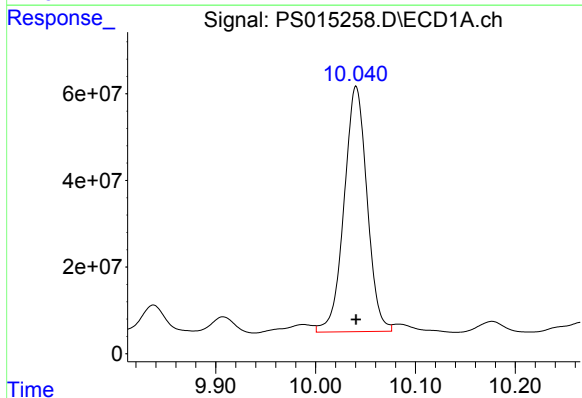


#13 2,4-DB

R.T.: 10.041 min
Delta R.T.: 0.000 min
Response: 905680913
Conc: 355.65 ng/ml

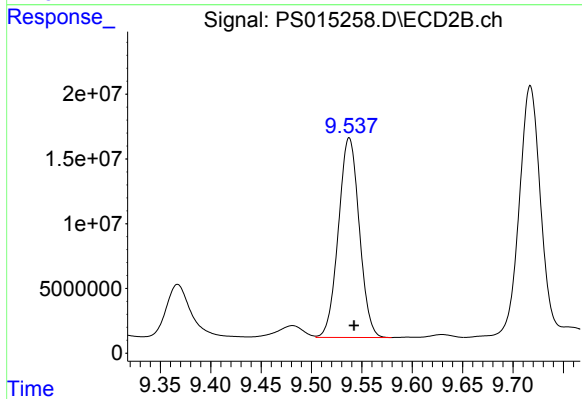

#13 2,4-DB

R.T.: 9.537 min
Delta R.T.: -0.005 min
Response: 221921908
Conc: 575.30 ng/ml

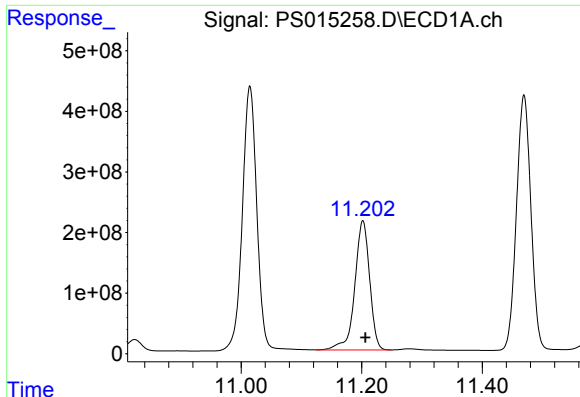


#14 DINOSEB

R.T.: 11.202 min
Delta R.T.: -0.004 min
Response: 3641905078
Conc: 455.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
18-B7(0-2)MS


Manual Integrations
APPROVED

Ankita
6/9/2021 1:49:55 PM

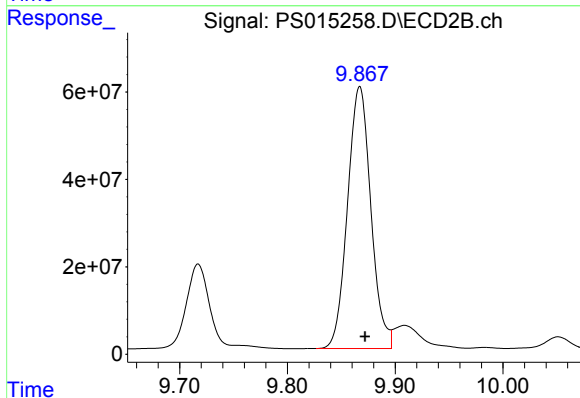


#14 DINOSEB

R.T.: 9.867 min
Delta R.T.: -0.005 min
Response: 902284955
Conc: 494.09 ng/ml m

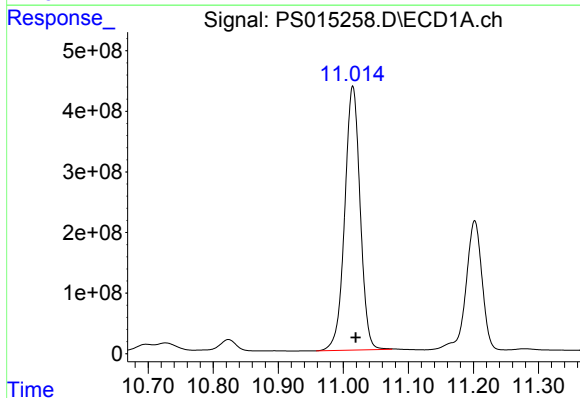


#15 Picloram

R.T.: 11.014 min
Delta R.T.: -0.005 min
Response: 7184590799
Conc: 433.67 ng/ml m

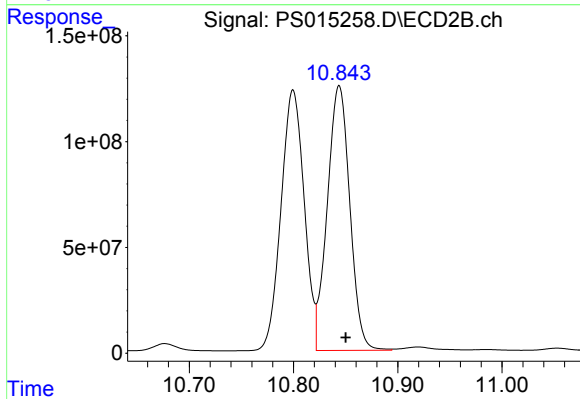

#15 Picloram

R.T.: 10.844 min
Delta R.T.: -0.006 min
Response: 1877798591
Conc: 452.17 ng/ml

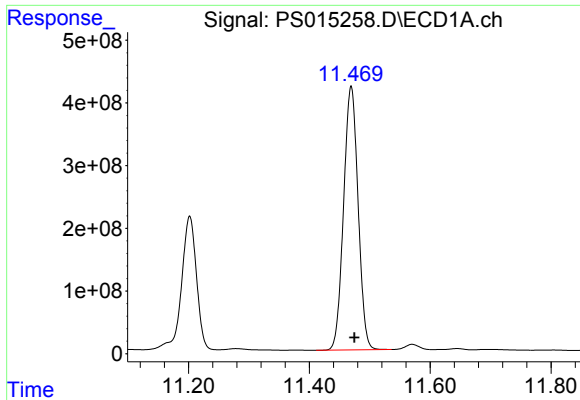


#16 DCPA

R.T.: 11.469 min
Delta R.T.: -0.006 min
Response: 6986217474
Conc: 414.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
18-B7(0-2)MS

Manual Integrations
APPROVED

Ankita
6/9/2021 1:49:55 PM

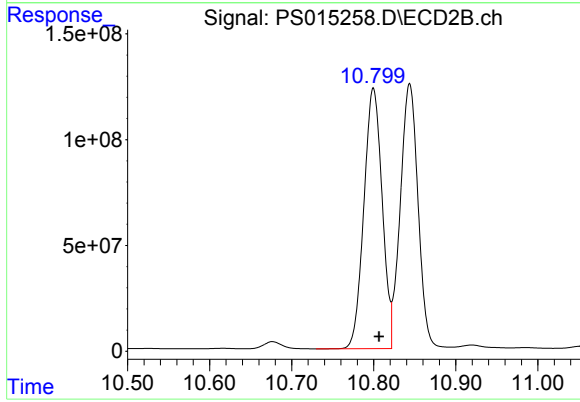

#16 DCPA

R.T.: 10.800 min
Delta R.T.: -0.007 min
Response: 1902250830
Conc: 441.26 ng/ml