

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060724\
 Data File : PS026932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2024 15:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 00:40:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051424.M
 Quant Title : 8080.M
 QLast Update : Wed May 15 02:07:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	7.770	1144.0E6	930.5E6	423.940	509.848
Target Compounds							
1) T	Dalapon	2.684f	2.745f	5465667	6070583	1.396	1.797 #
2) T	3,5-DICHL...	6.395f	0.000	9351947	0	2.511	N.D. #
3) T	4-Nitroph...	7.035f	7.267f	8770768	1295749	4.875	<MDL #
5) T	DICAMBA	7.421f	0.000	327790	0	<MDL	N.D. #
6) T	MCPD	7.665f	8.080	11670207	13371982	1.455	2.468 #
7) T	MCPA	7.773	0.000	532417	0	<MDL	N.D. #
8) T	DICHLORPROP	8.162	8.740f	398920	8689700	<MDL	4.159 #
9) T	2,4-D	8.378	0.000	92604786	0	25.990	N.D. #
10) T	Pentachlo...	8.686	9.543	470715	893553	<MDL	<MDL #
11) T	2,4,5-TP ...	9.221f	9.924	1747966	1713796	<MDL	<MDL #
12) T	2,4,5-T	9.533	10.340	426923	1199102	<MDL	<MDL #
13) T	2,4-DB	10.092	0.000	77653	0	<MDL	N.D. #
14) T	DINOSEB	11.352f	11.281	-148779	758017	N.D.	<MDL
15) T	Picloram	11.119	12.388	6599942	9103054	<MDL	<MDL #
16) T	DCPA	11.580f	0.000	2537364	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060724\
Data File : PS026932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2024 15:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 00:40:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051424.M
Quant Title : 8080.M
QLast Update : Wed May 15 02:07:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

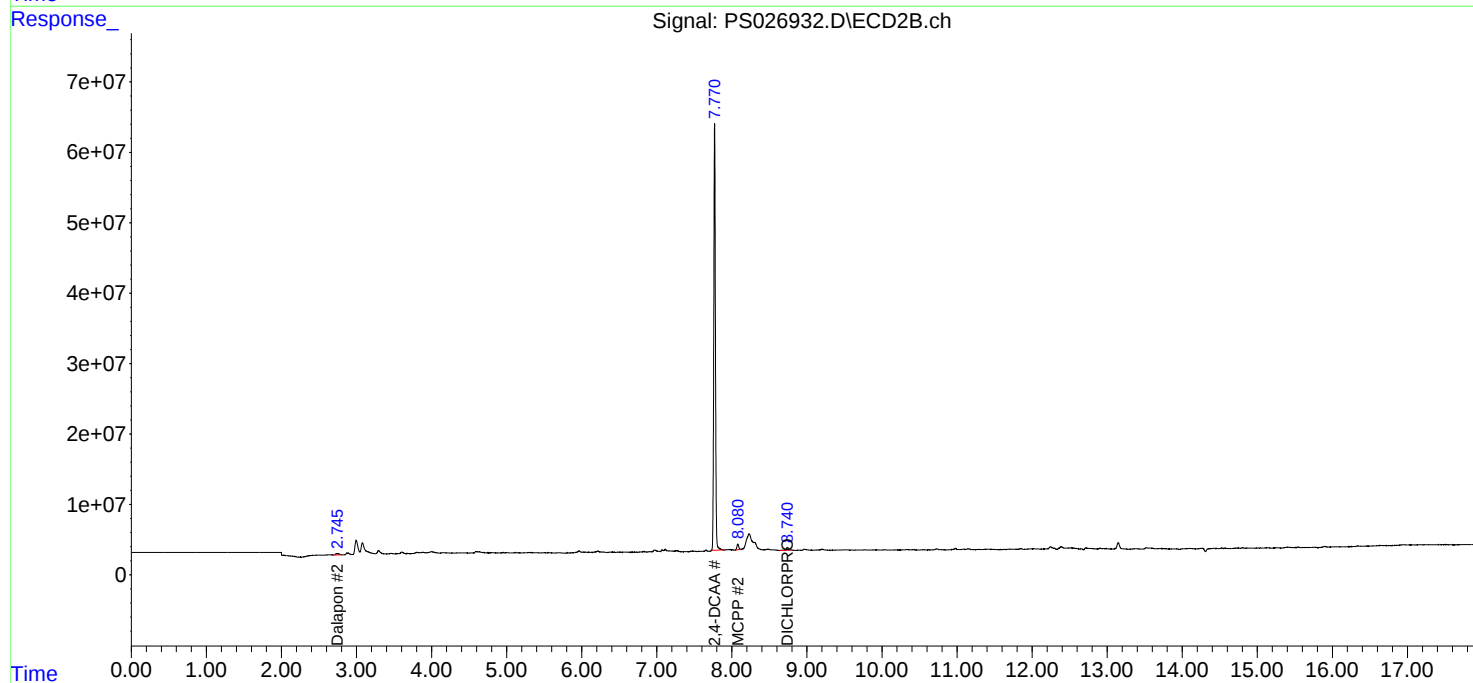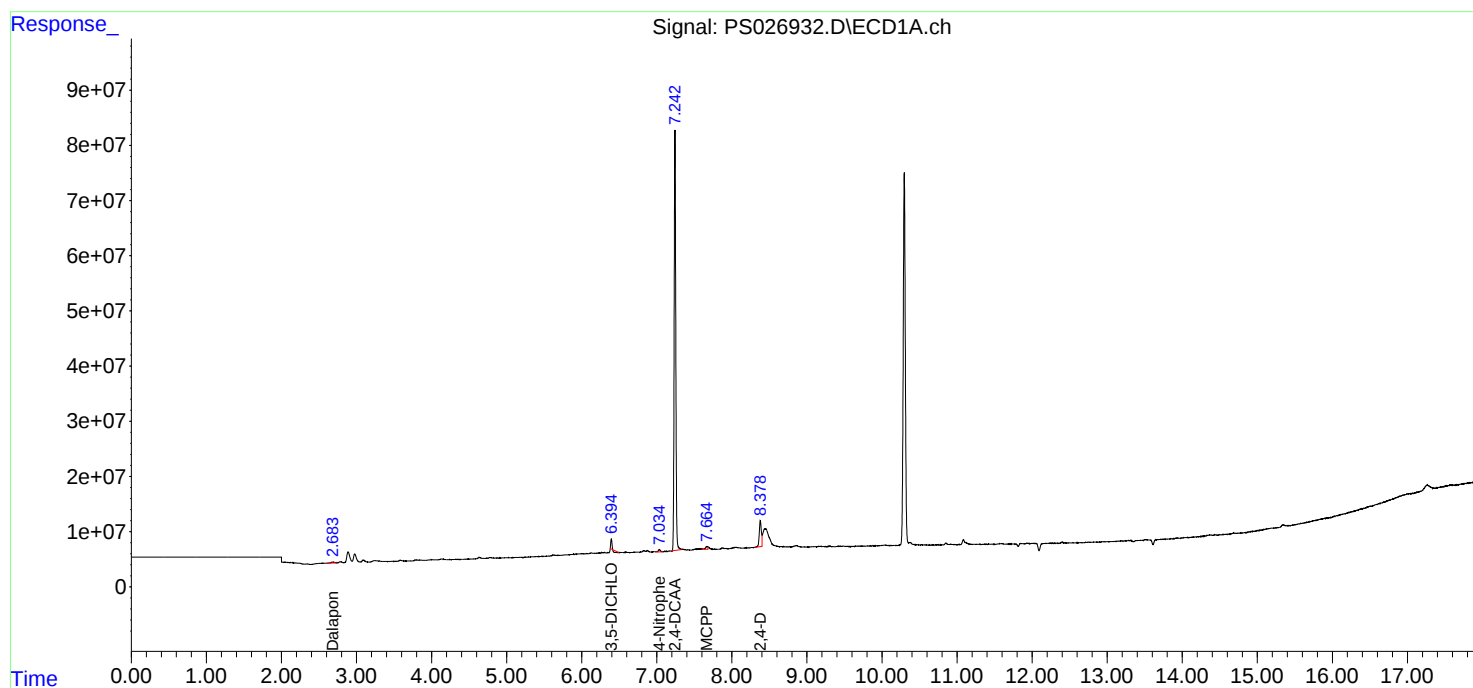


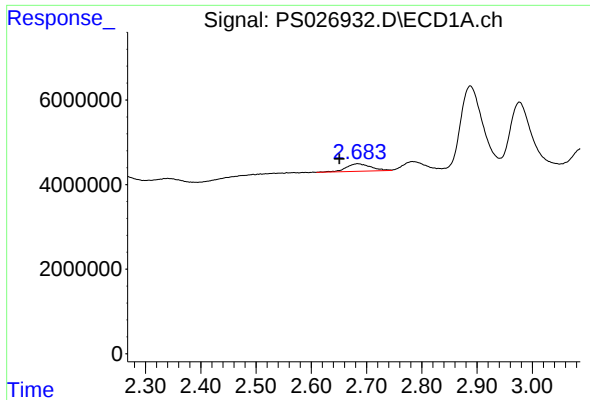

#1 Dalapon


R.T.: 2.684 min
Delta R.T.: 0.033 min
Response: 5465667
Conc: 1.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

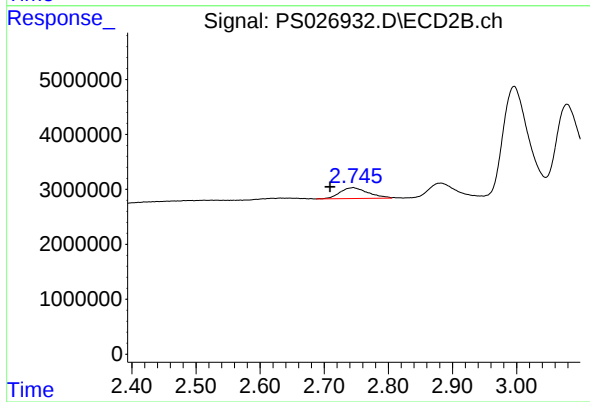


#1 Dalapon

R.T.: 2.745 min
Delta R.T.: 0.036 min
Response: 6070583
Conc: 1.80 ng/ml

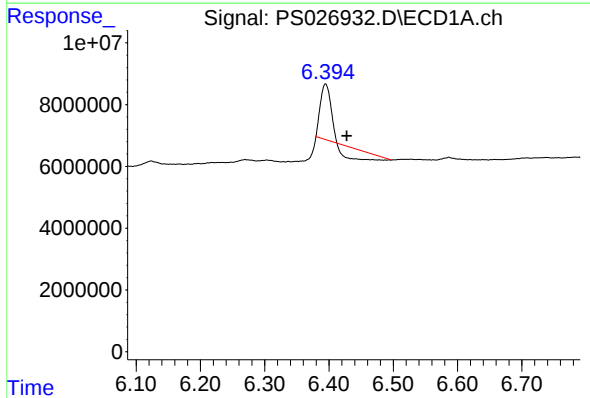


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.395 min
Delta R.T.: -0.033 min
Response: 9351947
Conc: 2.51 ng/ml

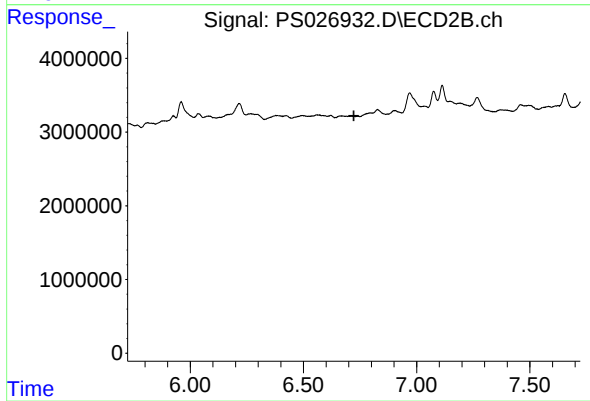

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.723 min
Response: 0
Conc: N.D.

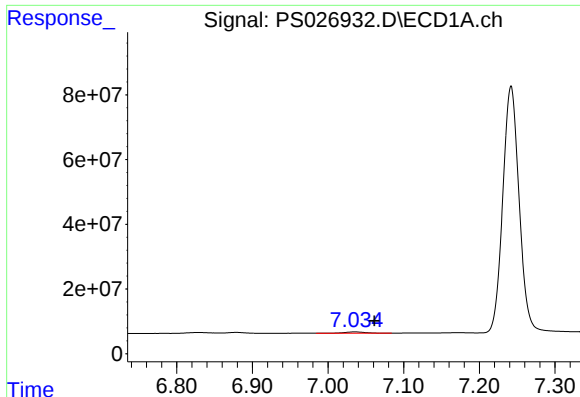

#3 4-Nitrophenol


R.T.: 7.035 min
Delta R.T.: -0.026 min
Response: 8770768
Conc: 4.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

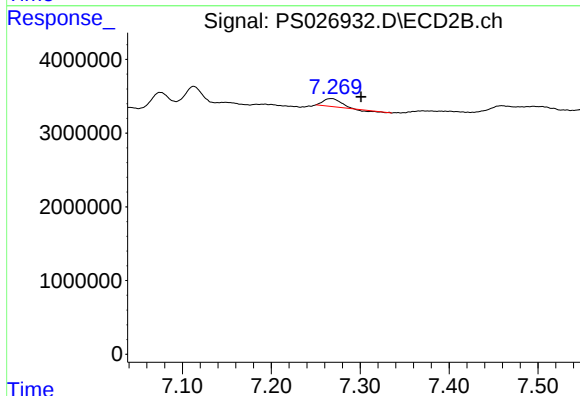


#3 4-Nitrophenol

R.T.: 7.267 min
Delta R.T.: -0.034 min
Response: 1295749
Conc: N.D.

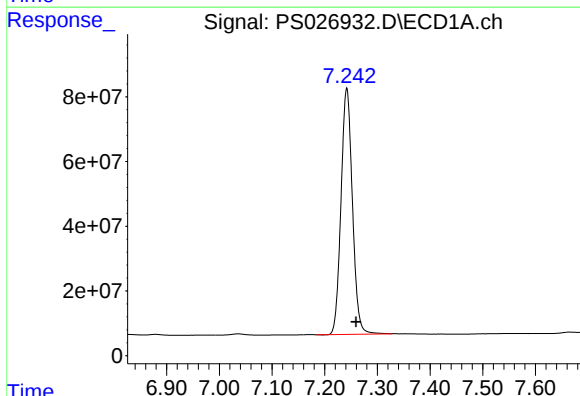


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: -0.018 min
Response: 1143955994
Conc: 423.94 ng/ml

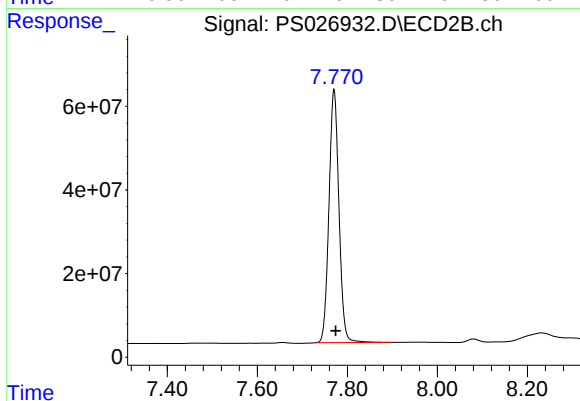

#4 2,4-DCAA


R.T.: 7.770 min
Delta R.T.: -0.004 min
Response: 930490672
Conc: 509.85 ng/ml

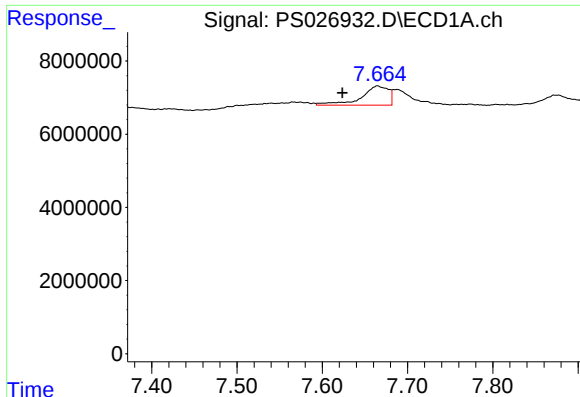

#6 MCP


R.T.: 7.665 min
Delta R.T.: 0.041 min
Response: 11670207
Conc: 1.46 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

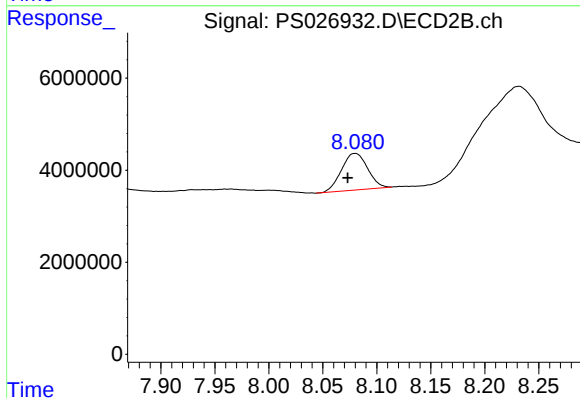


#6 MCP

R.T.: 8.080 min
Delta R.T.: 0.007 min
Response: 13371982
Conc: 2.47 ug/ml

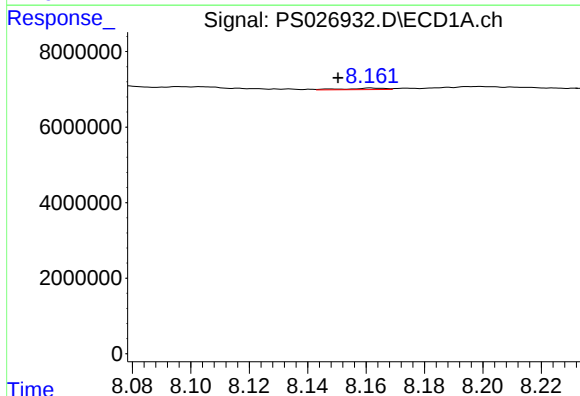


#8 DICHLORPROP

R.T.: 8.162 min
Delta R.T.: 0.011 min
Response: 398920
Conc: N.D.

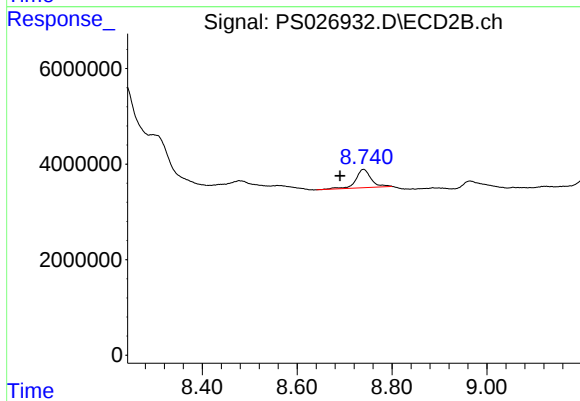

#8 DICHLORPROP


R.T.: 8.740 min
Delta R.T.: 0.049 min
Response: 8689700
Conc: 4.16 ng/ml

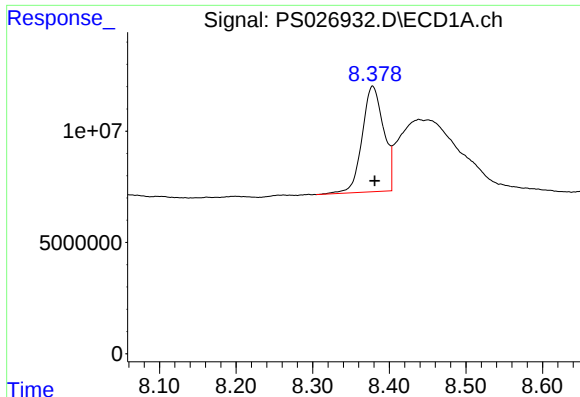

#9 2,4-D

R.T.: 8.378 min
Delta R.T.: -0.003 min
Response: 92604786
Conc: 25.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

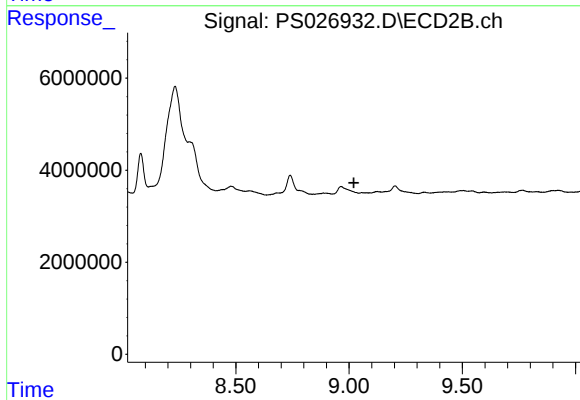

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 9.021 min
Response: 0
Conc: N.D.