

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060821\
 Data File : PS015286.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2021 10:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 04:09:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.783	1115.7E6	286.0E6	442.673	533.729
Target Compounds							
3) T	4-Nitroph...	7.022	0.000	5659299	0	4.015	N.D. #
7) T	MCPA	7.670f	0.000	24448546	0	2.436	N.D. #
9) T	2,4-D	8.344	0.000	4370820	0	1.715	N.D. #
12) T	2,4,5-T	9.487	9.080f	5925598	8032085	<MDL	2.774 #
13) T	2,4-DB	10.030	0.000	6209800	0	2.439	N.D. #
15) T	Picloram	11.015	10.843	216.2E6	55551448	13.047	13.377
16) T	DCPA	0.000	10.843	0	55551448	N.D.	12.886



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060821\
Data File : PS015286.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2021 10:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 04:09:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

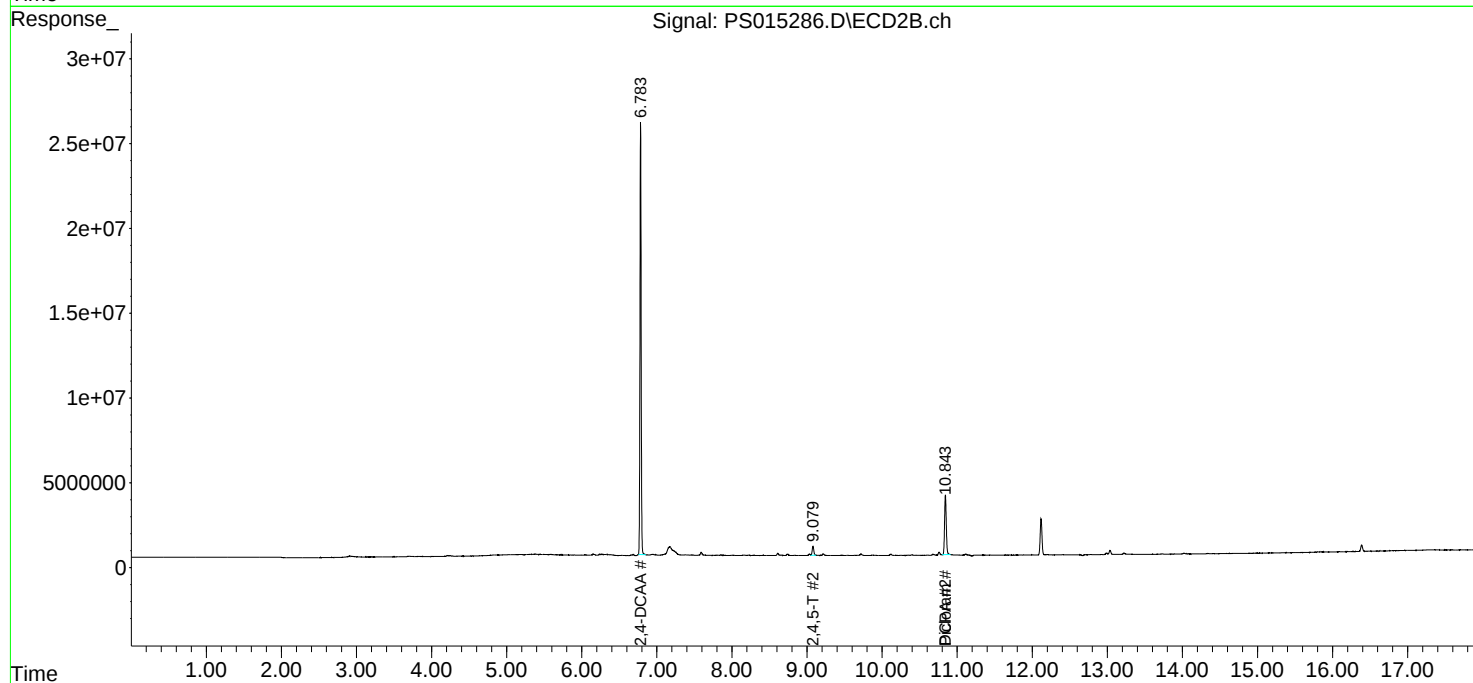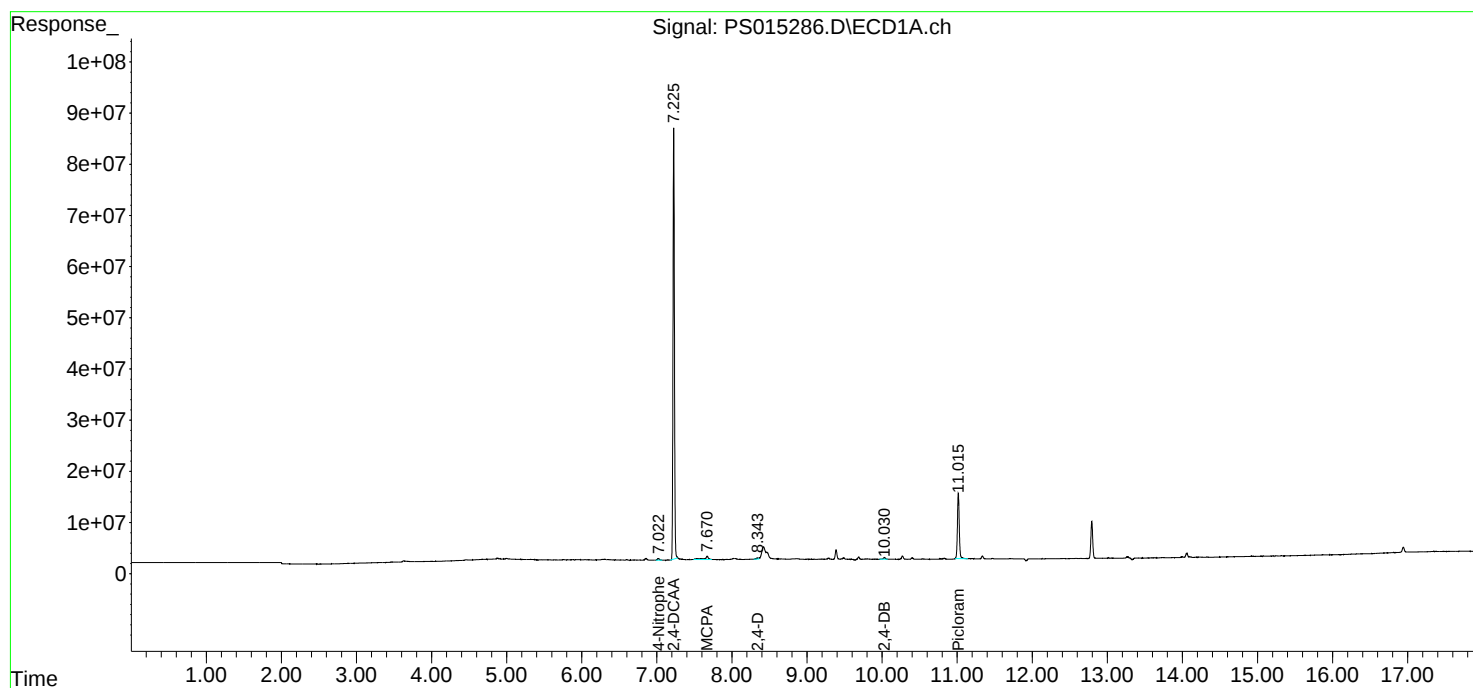


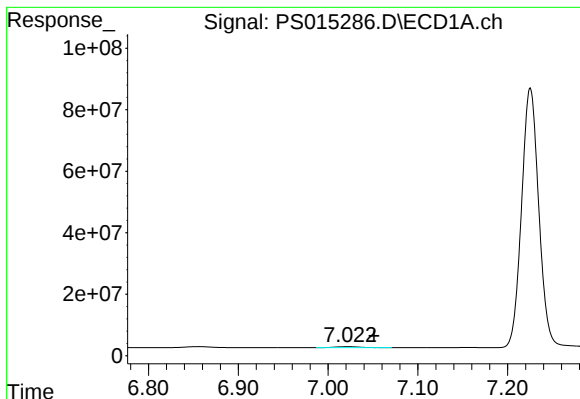

#3 4-Nitrophenol


R.T.: 7.022 min
Delta R.T.: -0.029 min
Response: 5659299
Conc: 4.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

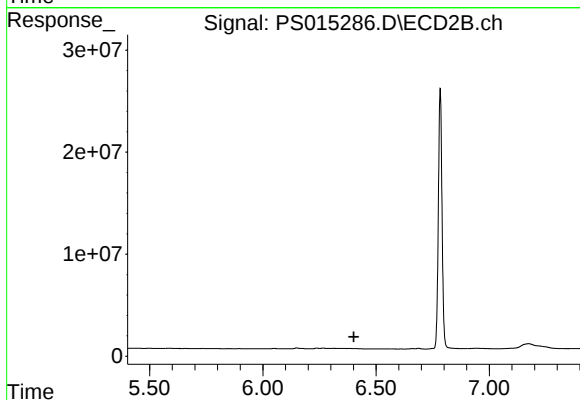


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

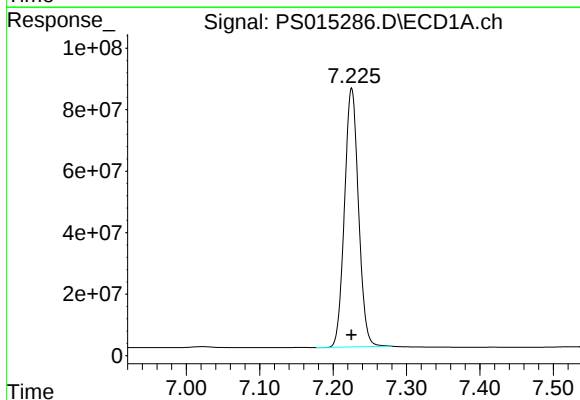


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 1115701628
Conc: 442.67 ng/ml

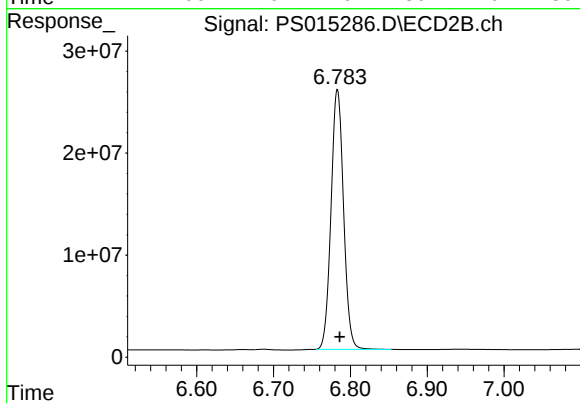

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: -0.003 min
Response: 285956497
Conc: 533.73 ng/ml

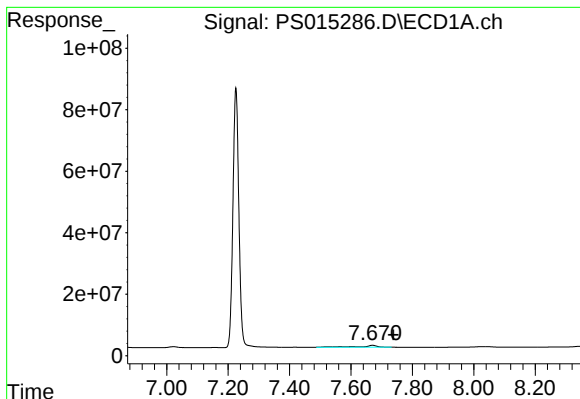

#7 MCPA


R.T.: 7.670 min
Delta R.T.: -0.068 min
Response: 24448546
Conc: 2.44 ug/ml

Instrument :
ECD_S
ClientSampleId :

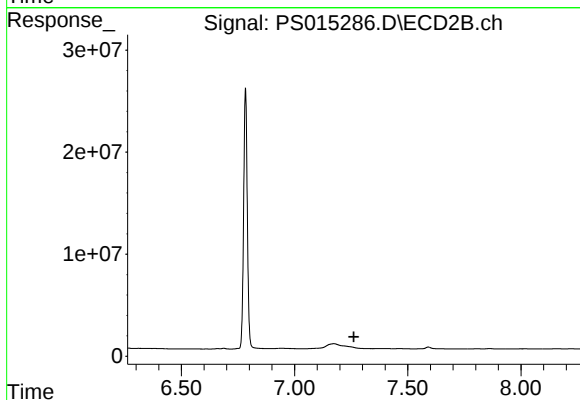


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

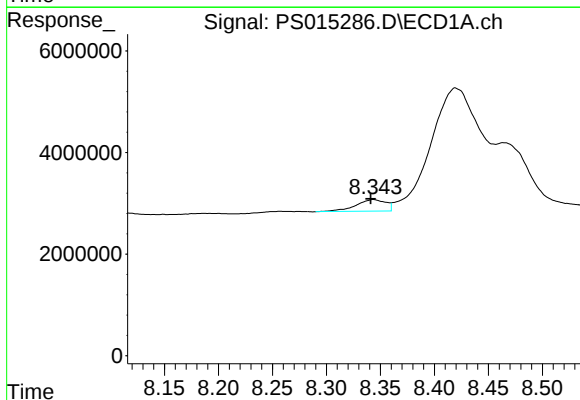


#9 2,4-D

R.T.: 8.344 min
Delta R.T.: 0.003 min
Response: 4370820
Conc: 1.72 ng/ml

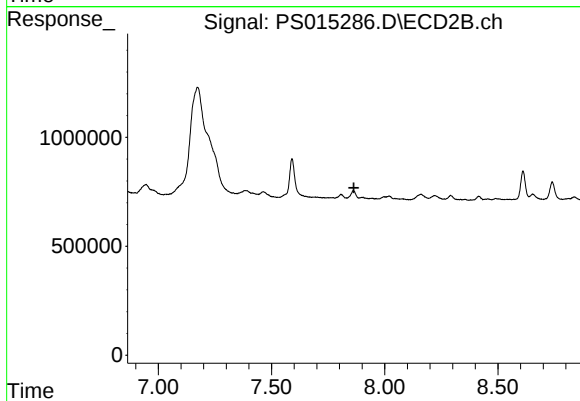

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

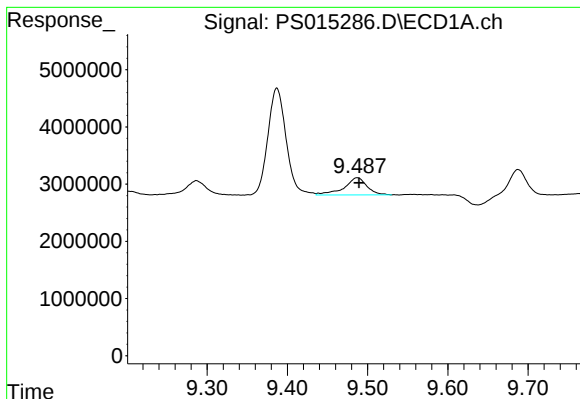

#12 2,4,5-T


R.T.: 9.487 min
Delta R.T.: -0.002 min
Response: 5925598
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

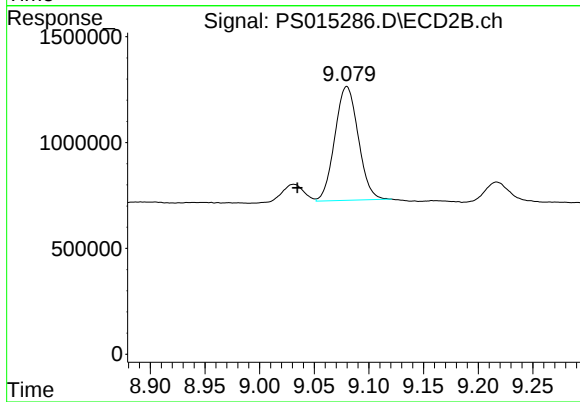


#12 2,4,5-T

R.T.: 9.080 min
Delta R.T.: 0.045 min
Response: 8032085
Conc: 2.77 ng/ml

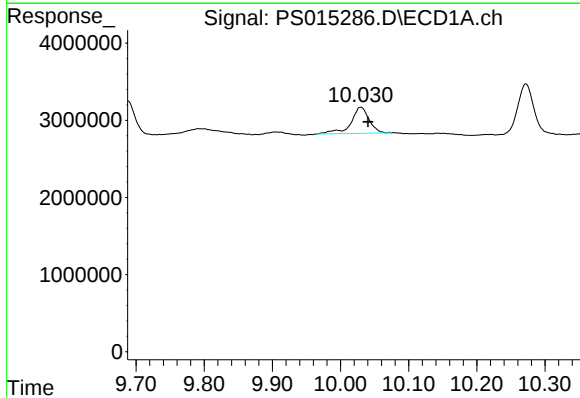


#13 2,4-DB

R.T.: 10.030 min
Delta R.T.: -0.011 min
Response: 6209800
Conc: 2.44 ng/ml

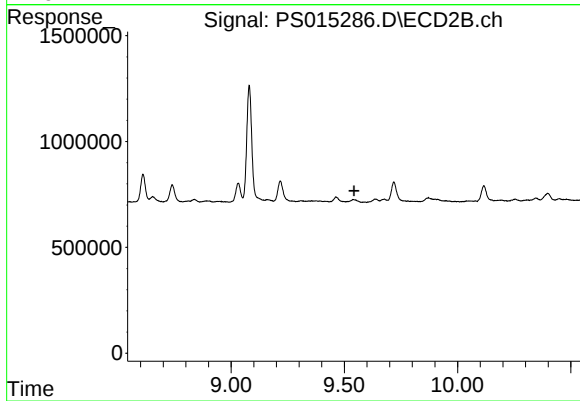

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.542 min
Response: 0
Conc: N.D.

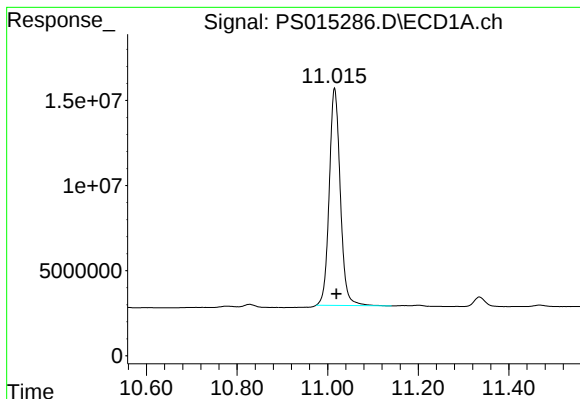

#15 Picloram


R.T.: 11.015 min
Delta R.T.: -0.004 min
Response: 216153109
Conc: 13.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

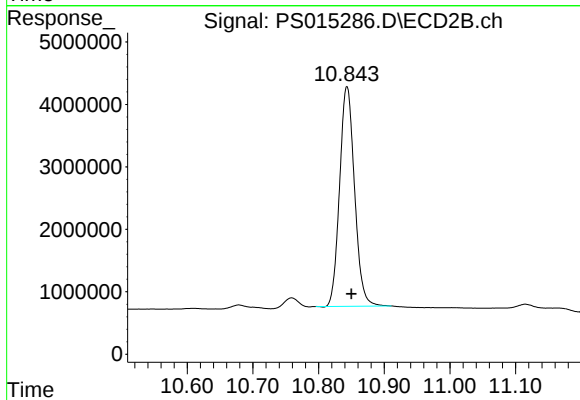


#15 Picloram

R.T.: 10.843 min
Delta R.T.: -0.007 min
Response: 55551448
Conc: 13.38 ng/ml

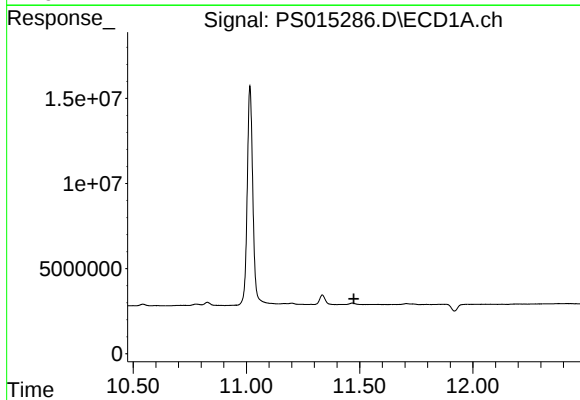

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.475 min
Response: 0
Conc: N.D.

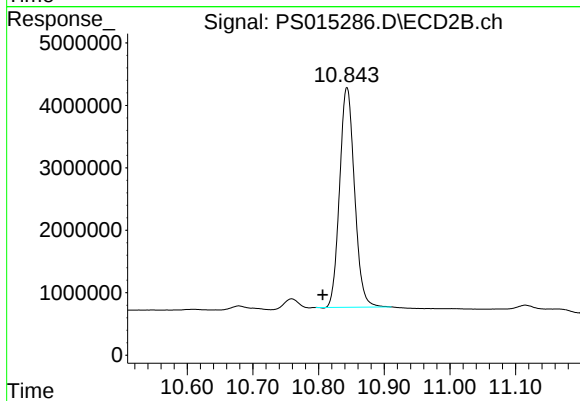

#16 DCPA

R.T.: 10.843 min
Delta R.T.: 0.037 min
Response: 55551448
Conc: 12.89 ng/ml