

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060920\
 Data File : PS010731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2020 19:38
 Operator : DD\AJ
 Sample : L2815-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 03:16:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.239	6.921	280.1E6	208.6E6	354.131	382.541
Target Compounds							
1) T	Dalapon	3.006	2.585	40471149	127.9E6	41.163	174.709 #
2) T	3,5-DICHL...	0.000	6.101	0	86769689	N.D.	105.863
3) T	4-Nitroph...	7.007	0.000	3080708	0	8.310	N.D. #
5) T	DICAMBA	7.419	7.055	5349143	13763350	1.701	6.115 #
7) T	MCPA	7.693	7.455	133.8E6	119.5E6	38.261	43.985
8) T	DICHLORPROP	0.000	7.740	0	10430589	N.D.	18.089
10) T	Pentachlo...	8.721	0.000	7757905	0	<MDL	N.D. #
12) T	2,4,5-T	9.441	0.000	39282057	0	9.659	N.D. #
14) T	DINOSEB	11.180	10.069	13332979	16796341	4.126	7.807 #
15) T	Picloram	11.004	0.000	42088665	0	8.244	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060920\
Data File : PS010731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2020 19:38
Operator : DD\AJ
Sample : L2815-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 03:16:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

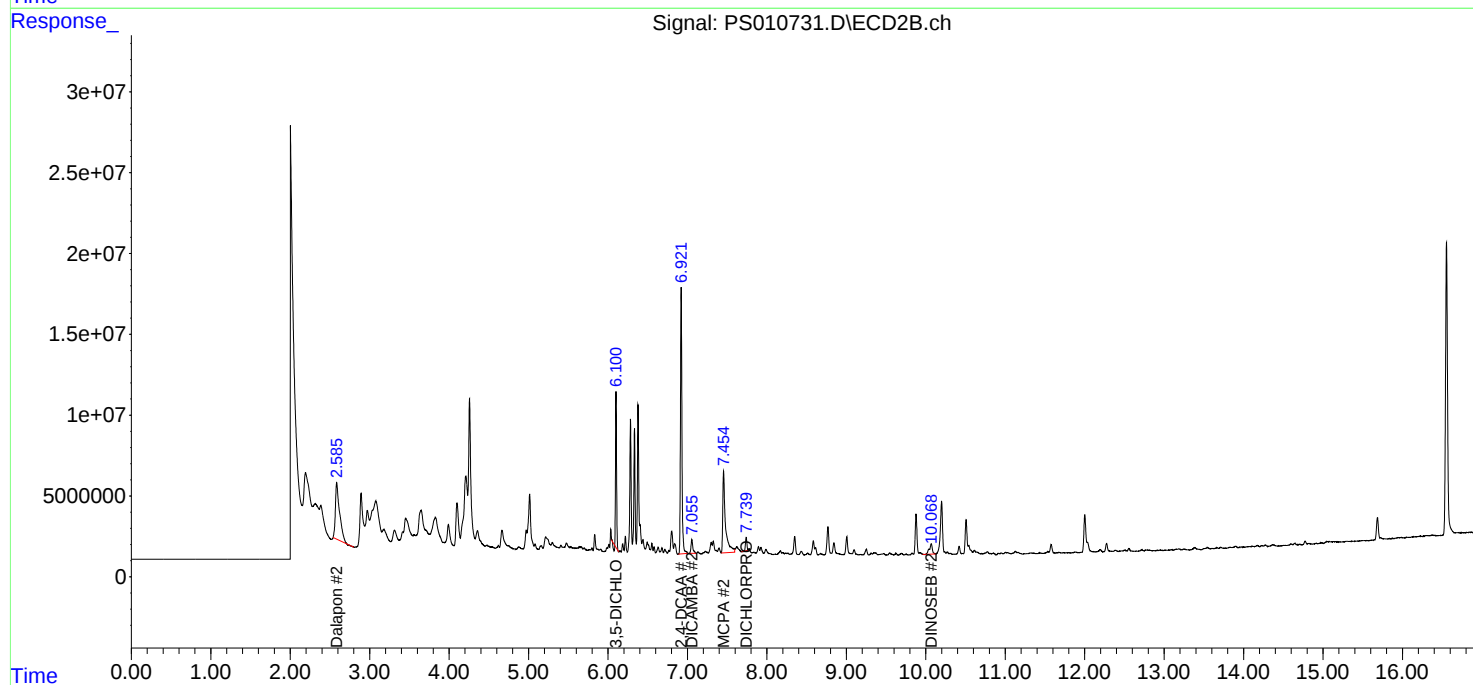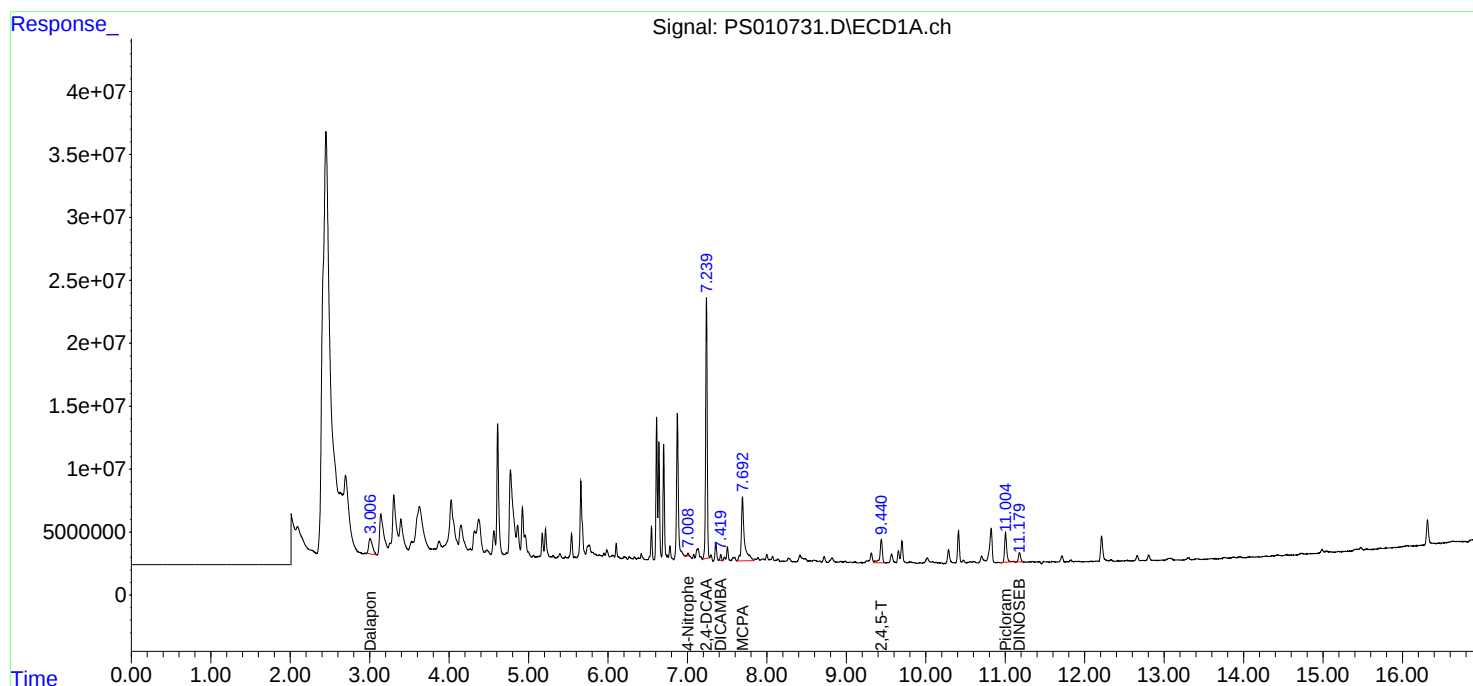


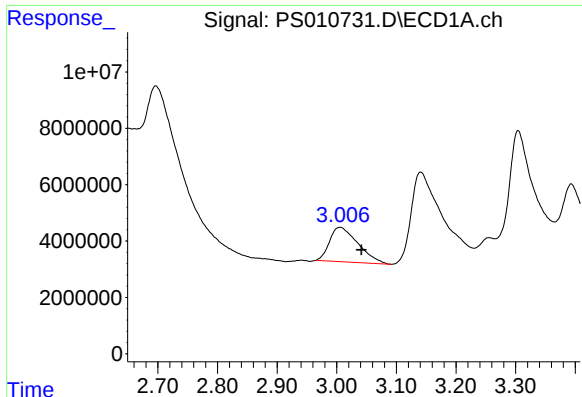

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.035 min
Response: 40471149
Conc: 41.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

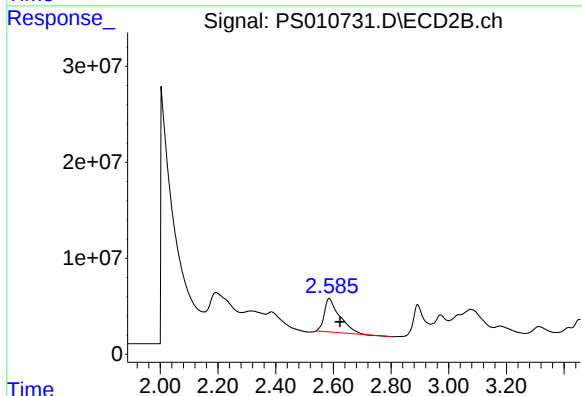


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.038 min
Response: 127912510
Conc: 174.71 ng/ml

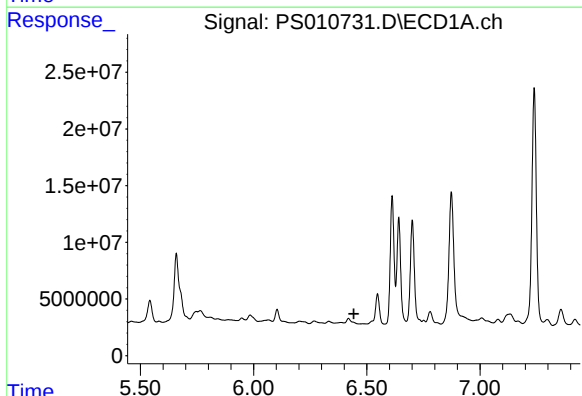


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

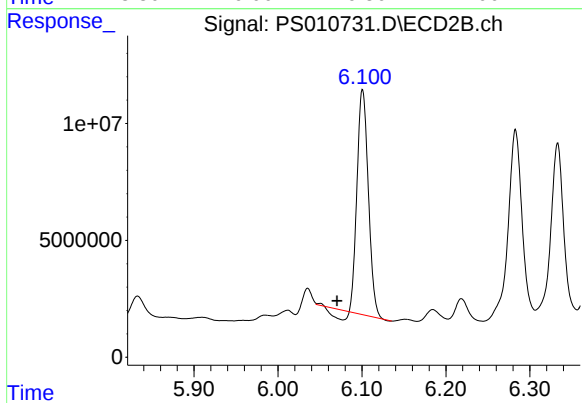

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.031 min
Response: 86769689
Conc: 105.86 ng/ml

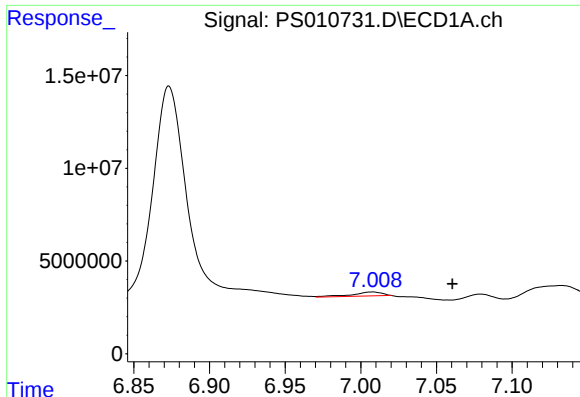

#3 4-Nitrophenol


R.T.: 7.007 min
Delta R.T.: -0.053 min
Response: 3080708
Conc: 8.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

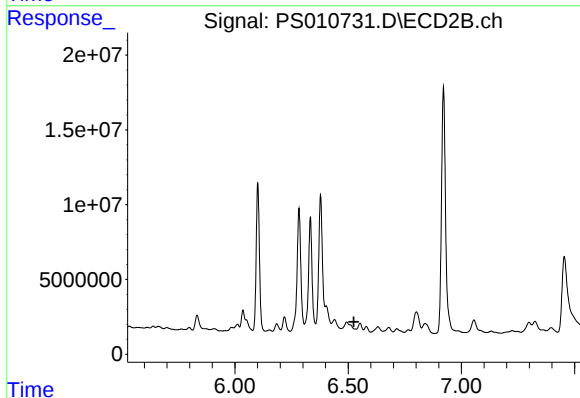


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

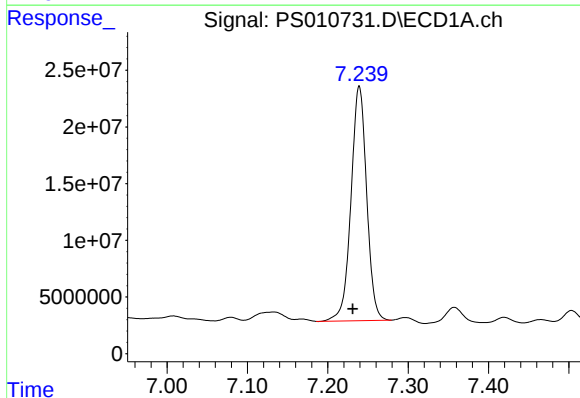


#4 2,4-DCAA

R.T.: 7.239 min
Delta R.T.: 0.008 min
Response: 280068942
Conc: 354.13 ng/ml

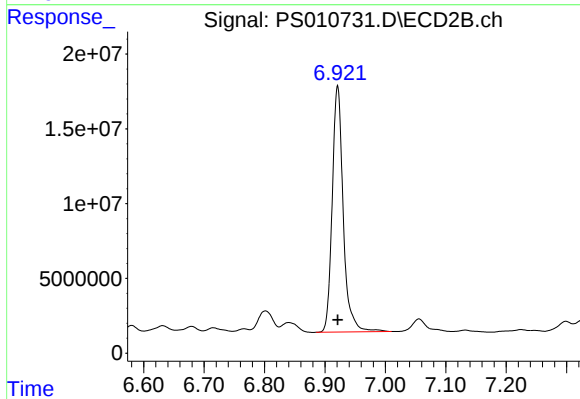

#4 2,4-DCAA


R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 208643938
Conc: 382.54 ng/ml

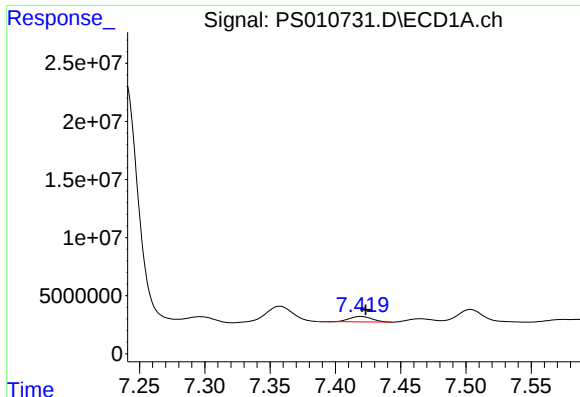

#5 DICAMBA


R.T.: 7.419 min
Delta R.T.: -0.004 min
Response: 5349143
Conc: 1.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

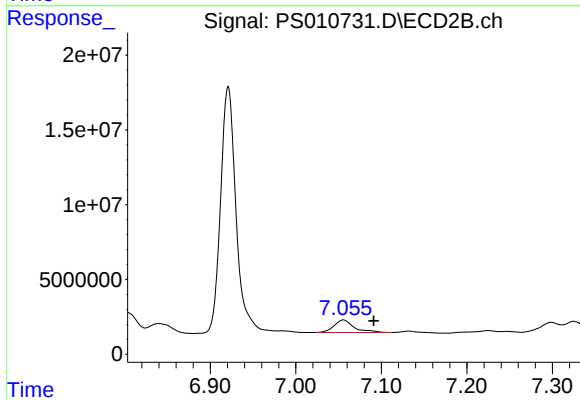


#5 DICAMBA

R.T.: 7.055 min
Delta R.T.: -0.036 min
Response: 13763350
Conc: 6.11 ng/ml

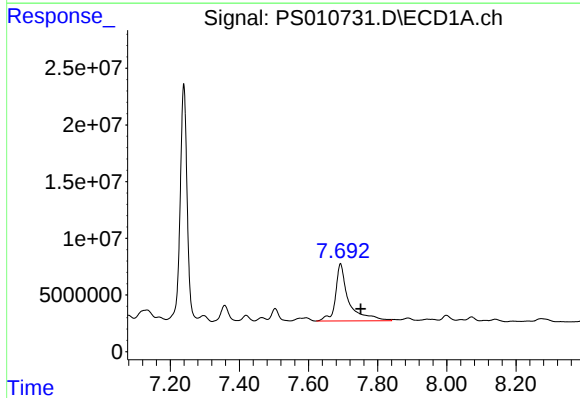


#7 MCPA

R.T.: 7.693 min
Delta R.T.: -0.058 min
Response: 133760896
Conc: 38.26 ug/ml

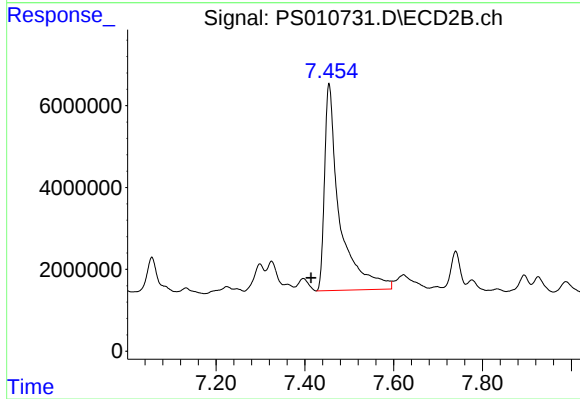

#7 MCPA


R.T.: 7.455 min
Delta R.T.: 0.041 min
Response: 119541404
Conc: 43.99 ug/ml

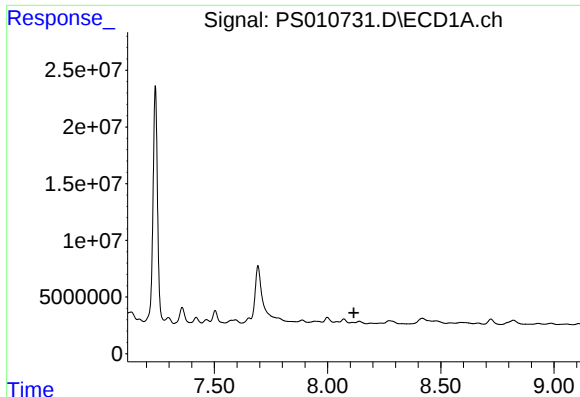

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

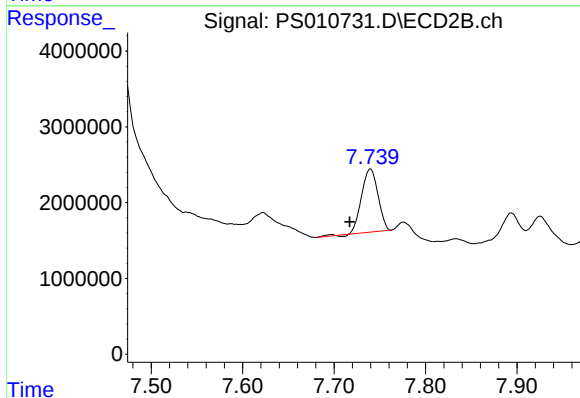


#8 DICHLORPROP

R.T.: 7.740 min
Delta R.T.: 0.022 min
Response: 10430589
Conc: 18.09 ng/ml

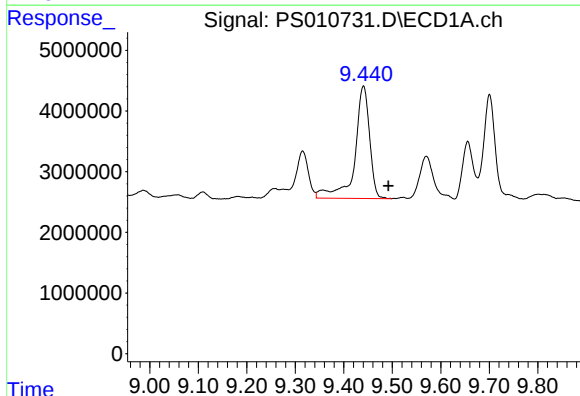


#12 2,4,5-T

R.T.: 9.441 min
Delta R.T.: -0.051 min
Response: 39282057
Conc: 9.66 ng/ml

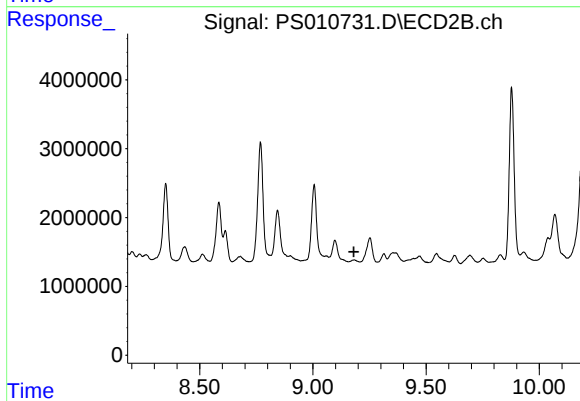

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

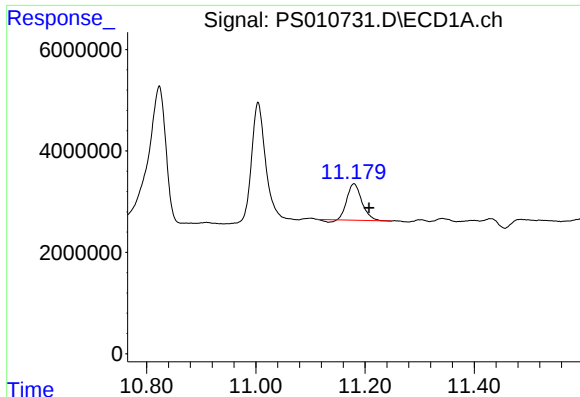

#14 DINOSEB


R.T.: 11.180 min
Delta R.T.: -0.028 min
Response: 13332979
Conc: 4.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

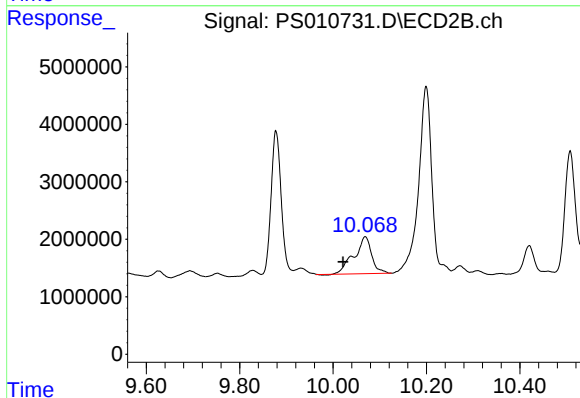


#14 DINOSEB

R.T.: 10.069 min
Delta R.T.: 0.047 min
Response: 16796341
Conc: 7.81 ng/ml

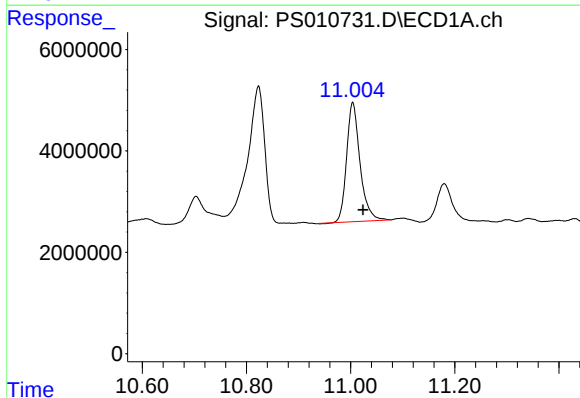

#15 Picloram

R.T.: 11.004 min
Delta R.T.: -0.020 min
Response: 42088665
Conc: 8.24 ng/ml

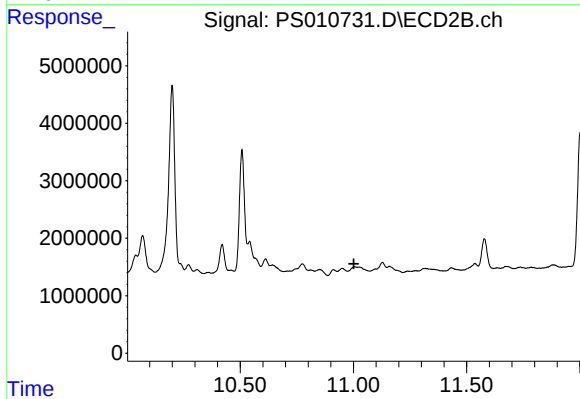

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.