

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060920\
 Data File : PS010738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2020 22:20
 Operator : DD\AJ
 Sample : L2939-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PHC-326FB-010

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 03:18:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.921	58036562	47732528	73.384	87.516
Target Compounds							
2) T	3,5-DICHL...	0.000	6.101	0	26114409	N.D.	31.861
3) T	4-Nitroph...	6.999	0.000	3061897	0	8.259	N.D. #
7) T	MCPA	7.682	7.450	260.2E6	285.6E6	74.427	105.069 #
8) T	DICHLORPROP	0.000	7.739	0	8949426	N.D.	15.520
11) T	2,4,5-TP ...	0.000	8.784	0	8612071	N.D.	2.868
12) T	2,4,5-T	9.430	0.000	28684790	0	7.053	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060920\
Data File : PS010738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2020 22:20
Operator : DD\AJ
Sample : L2939-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PHC-326FB-010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 03:18:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

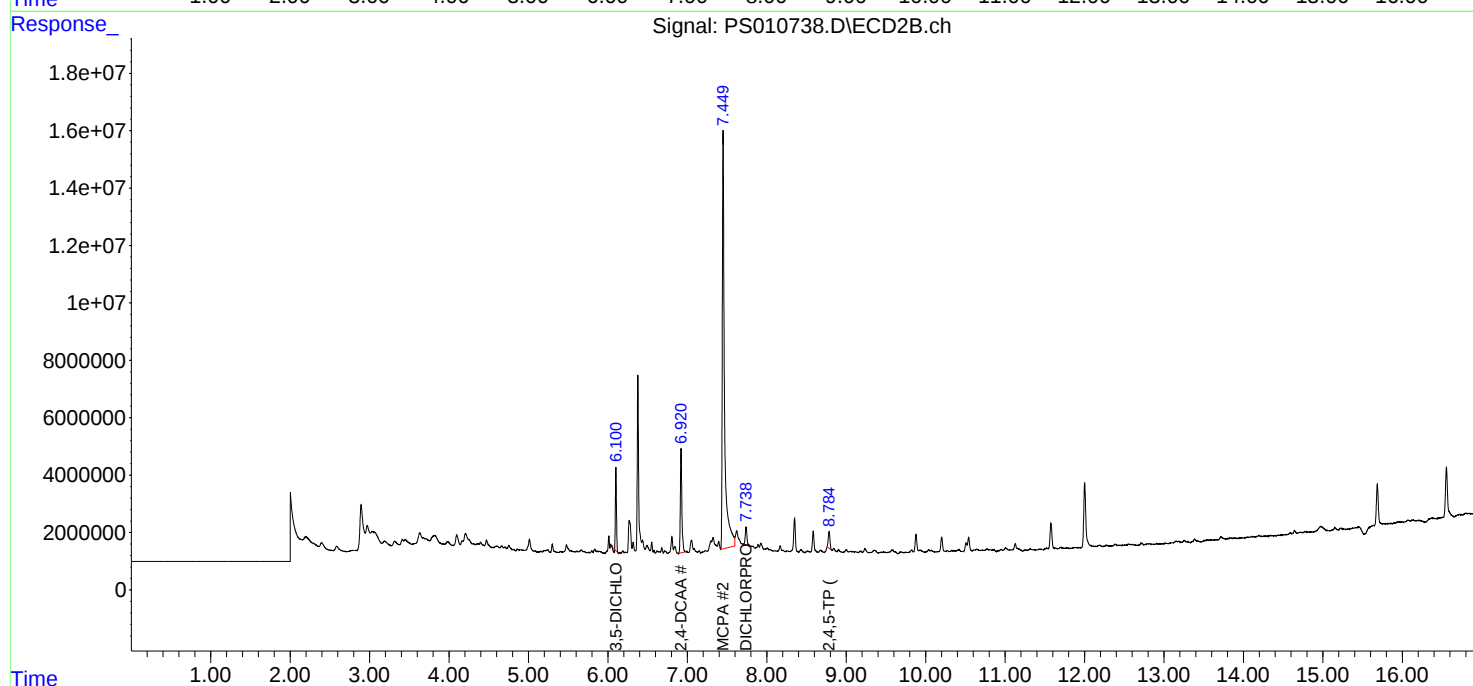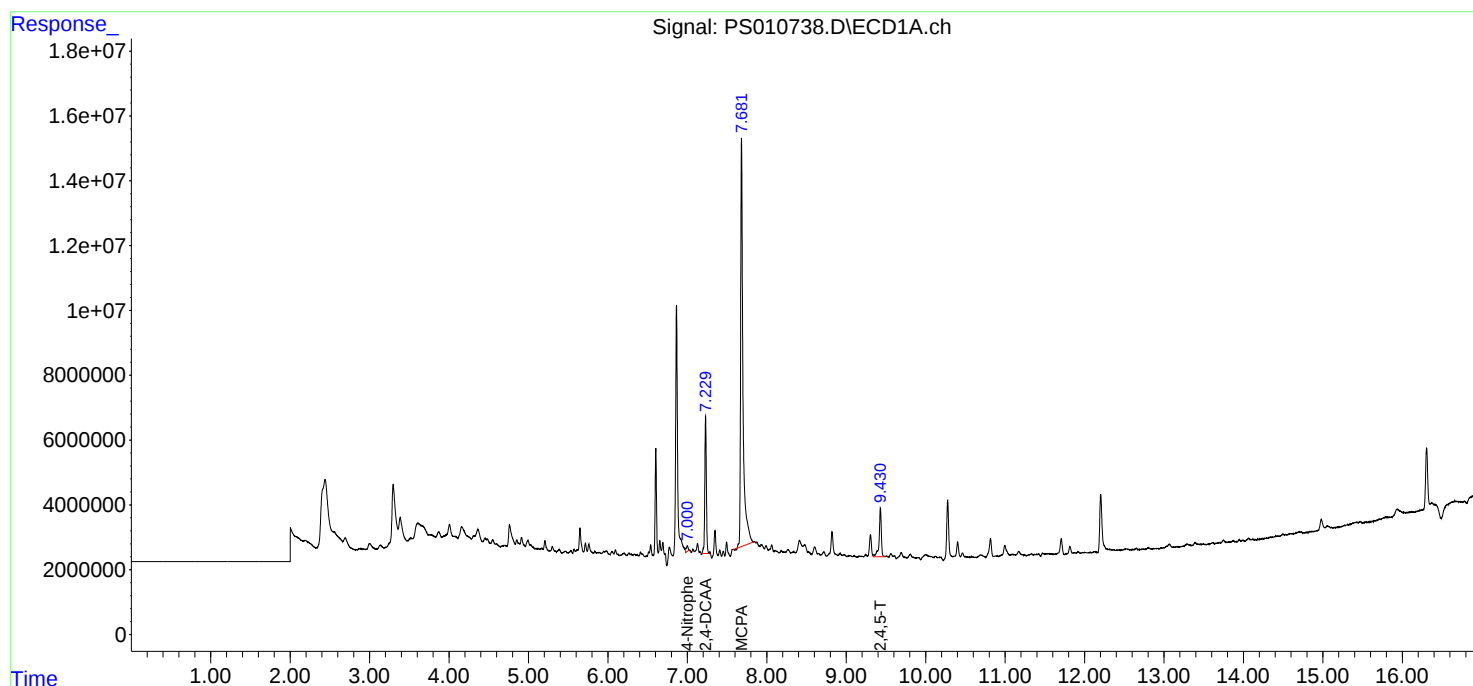


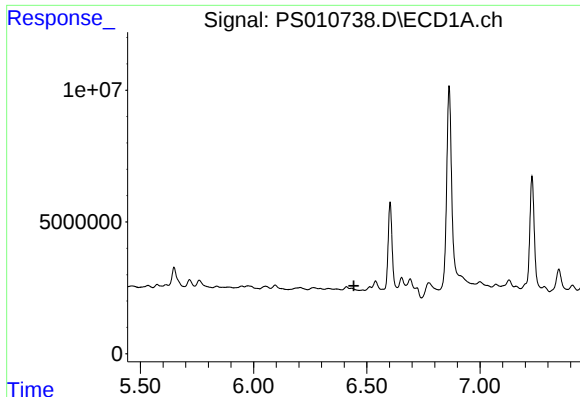

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.443 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PHC-326FB-010

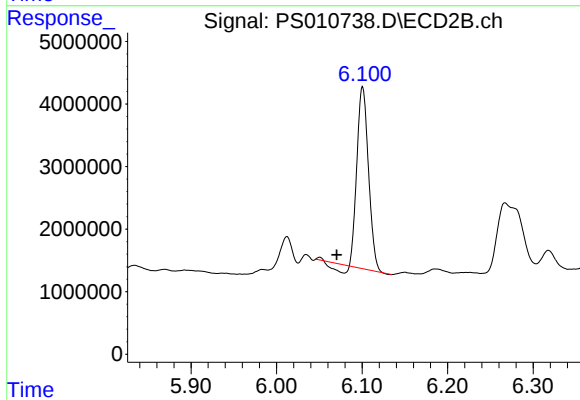


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 26114409
Conc: 31.86 ng/ml

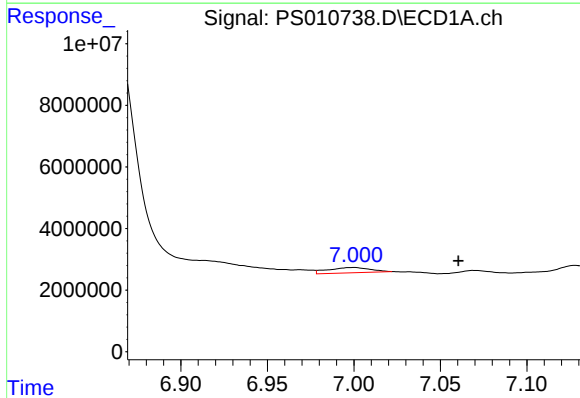


#3 4-Nitrophenol

R.T.: 6.999 min
Delta R.T.: -0.061 min
Response: 3061897
Conc: 8.26 ng/ml

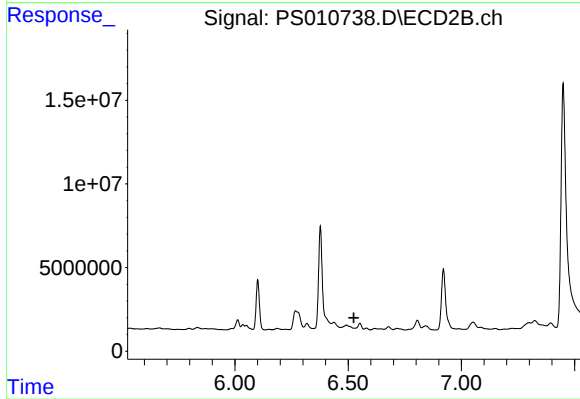

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

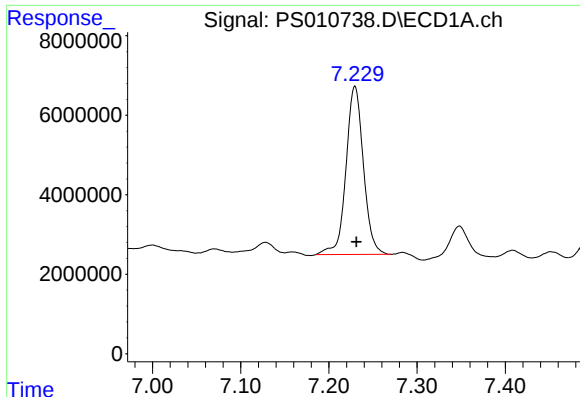

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: -0.002 min
Response: 58036562
Conc: 73.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
PHC-326FB-010

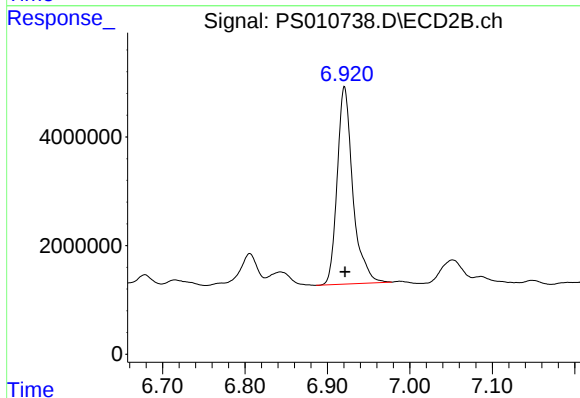


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 47732528
Conc: 87.52 ng/ml

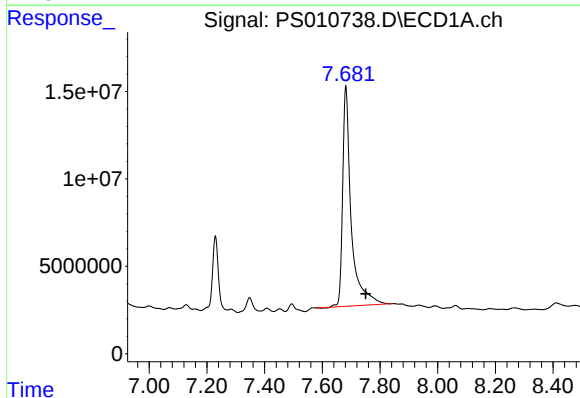


#7 MCPA

R.T.: 7.682 min
Delta R.T.: -0.069 min
Response: 260196541
Conc: 74.43 ug/ml

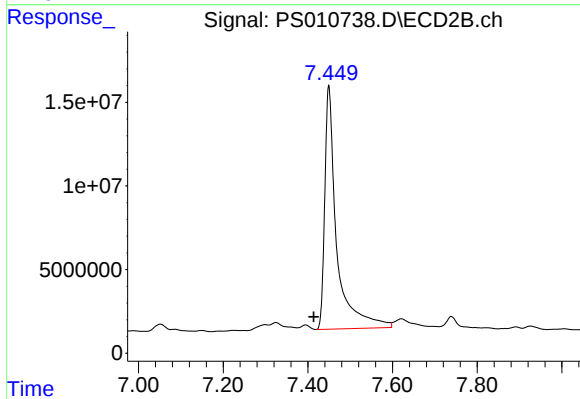

#7 MCPA


R.T.: 7.450 min
Delta R.T.: 0.036 min
Response: 285552028
Conc: 105.07 ug/ml

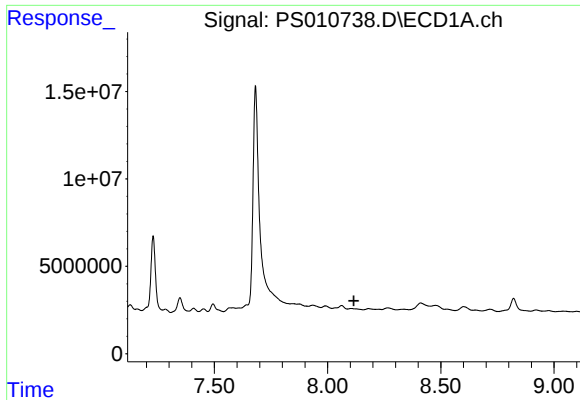

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PHC-326FB-010

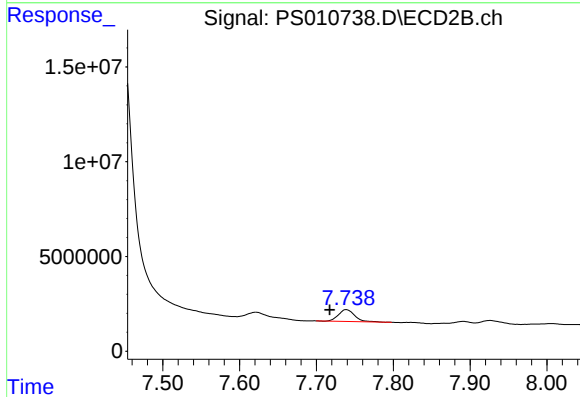


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.022 min
Response: 8949426
Conc: 15.52 ng/ml

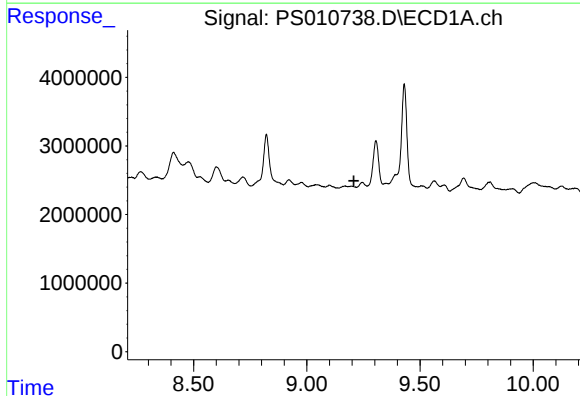


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

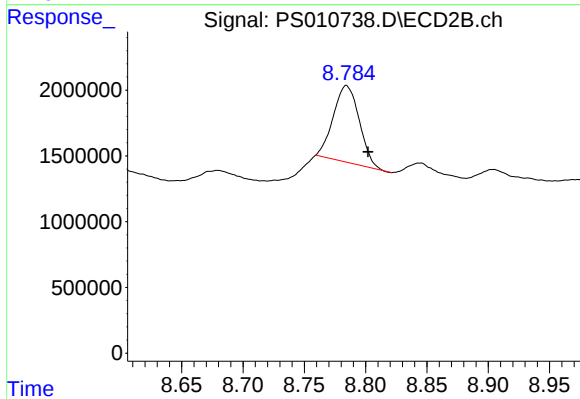

#11 2,4,5-TP (SILVEX)


R.T.: 8.784 min
Delta R.T.: -0.018 min
Response: 8612071
Conc: 2.87 ng/ml

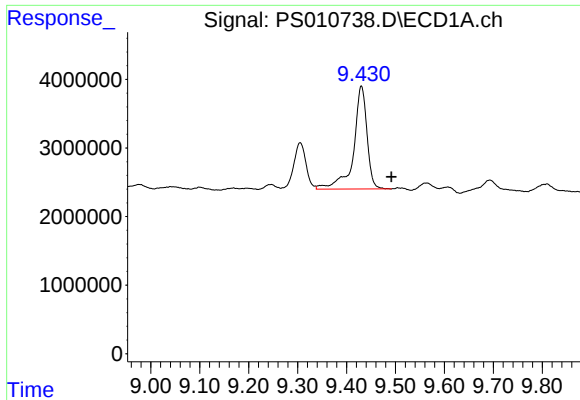

#12 2,4,5-T

R.T.: 9.430 min
Delta R.T.: -0.062 min
Response: 28684790
Conc: 7.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
PHC-326FB-010

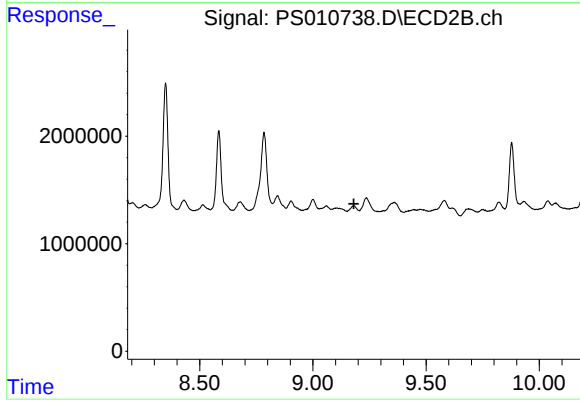

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.181 min
Response: 0
Conc: N.D.